

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062620\
 Data File : PS010977.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jun 2020 22:24
 Operator : DD\AJ
 Sample : PB129810TB
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB129810TB

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 27 04:03:27 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062420.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 25 02:45:12 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.228	6.919	329.6E6	230.4E6	363.485	415.873
Target Compounds							
1) T	Dalapon	2.998	2.586	38383184	74924577	34.279	99.322 #
2) T	3,5-DICHL...	0.000	6.100	0	75277886	N.D.	90.389
3) T	4-Nitroph...	6.997	0.000	3469723	0	8.692	N.D. #
5) T	DICAMBA	7.410	0.000	8402995	0	2.305	N.D. #
6) T	MCPD	7.641	0.000	1772804	0	<MDL	N.D. #
7) T	MCPA	7.686	7.458	74025101	60310393	18.588	21.852
8) T	DICHLORPROP	0.000	7.739	0	15861636	N.D.	27.015
10) T	Pentachlo...	0.000	8.436	0	7268707	N.D.	1.045
12) T	2,4,5-T	9.427	9.247	35613602	9093190	7.646	3.054 #
15) T	Picloram	10.993	0.000	59495169	0	10.613	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062620\
Data File : PS010977.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jun 2020 22:24
Operator : DD\AJ
Sample : PB129810TB
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PB129810TB

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 27 04:03:27 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062420.M
Quant Title : 8080.M
QLast Update : Thu Jun 25 02:45:12 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

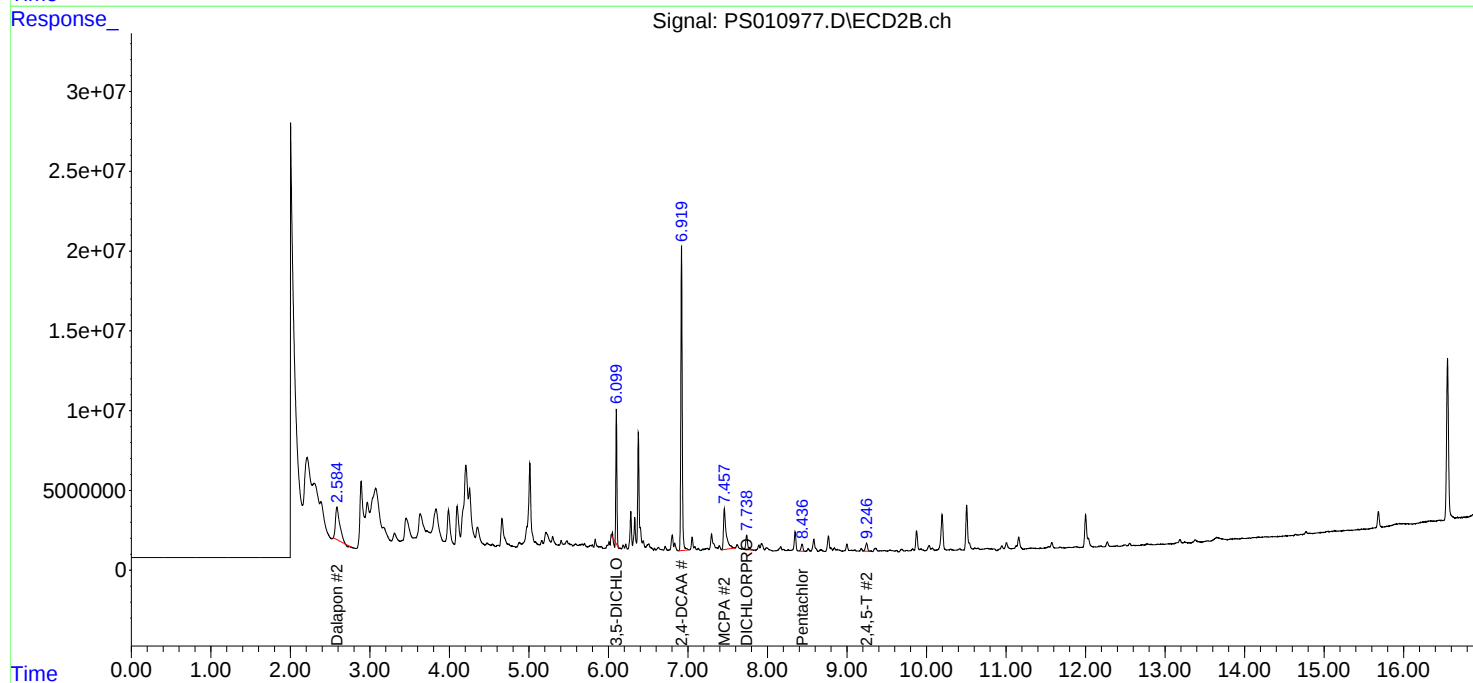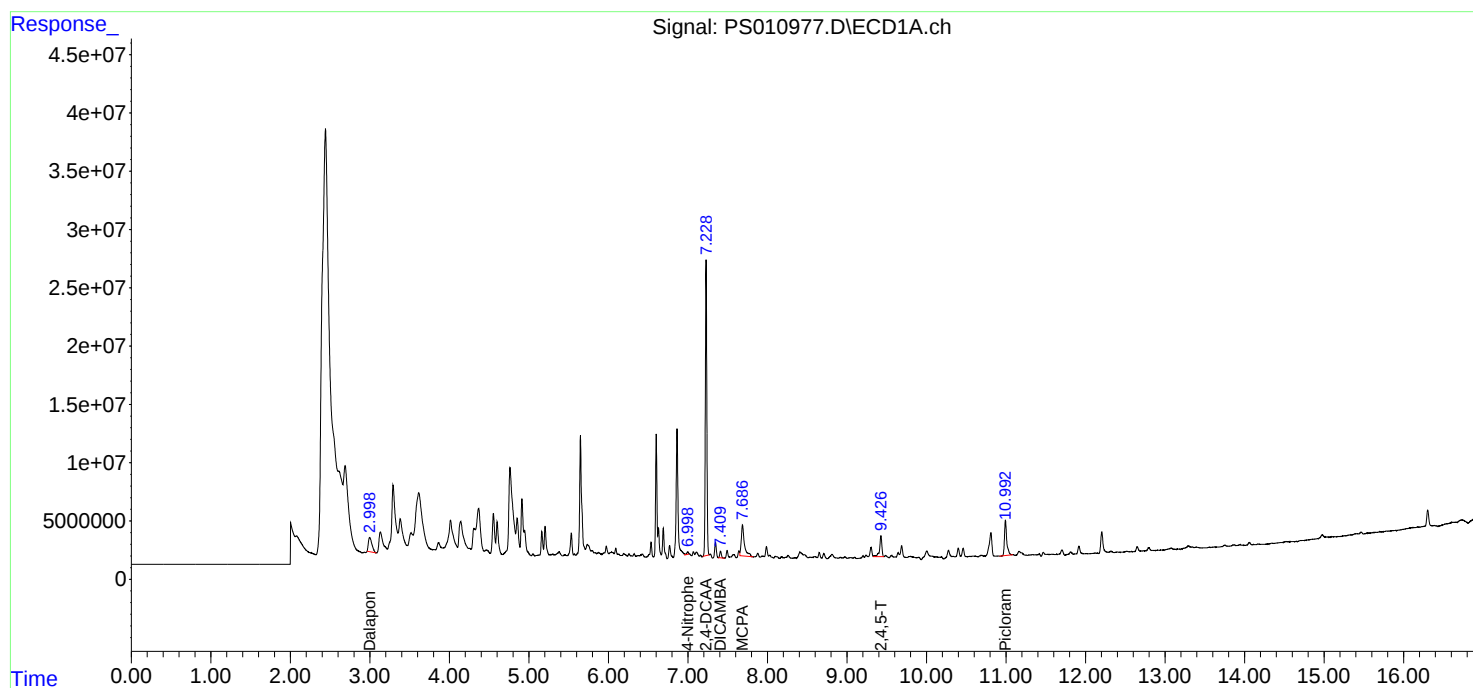


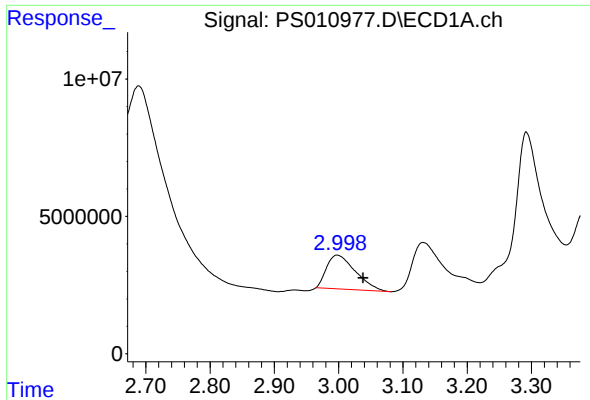

#1 Dalapon


R.T.: 2.998 min
Delta R.T.: -0.040 min
Response: 38383184
Conc: 34.28 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB129810TB

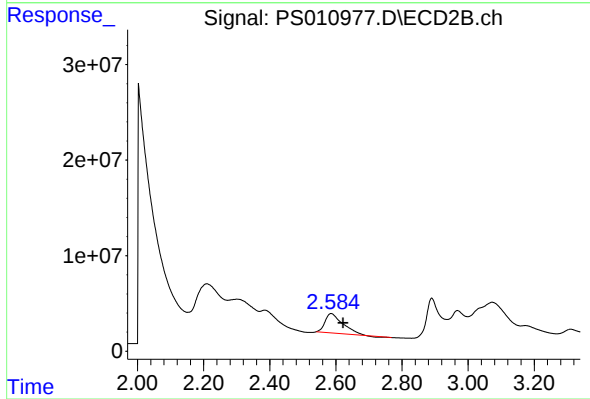


#1 Dalapon

R.T.: 2.586 min
Delta R.T.: -0.036 min
Response: 74924577
Conc: 99.32 ng/ml

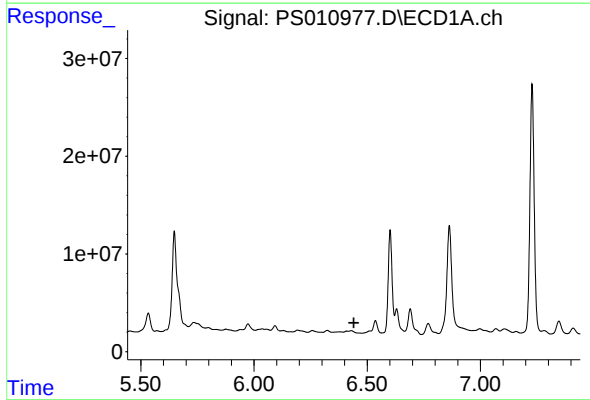


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.441 min
Response: 0
Conc: N.D.

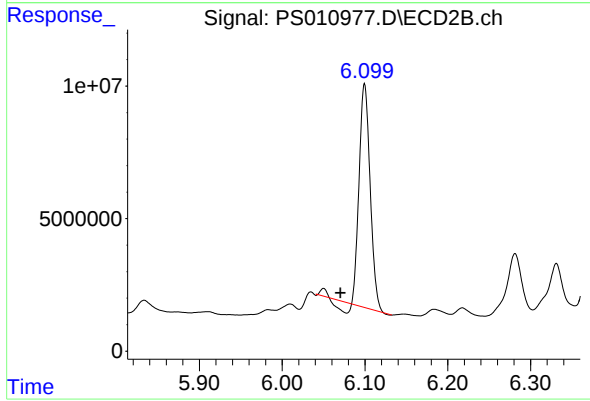

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.100 min
Delta R.T.: 0.029 min
Response: 75277886
Conc: 90.39 ng/ml

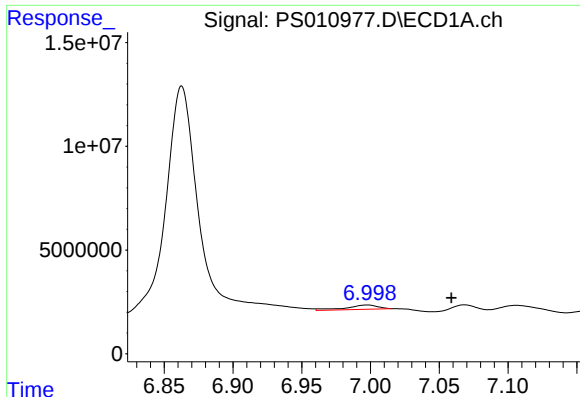

#3 4-Nitrophenol


R.T.: 6.997 min
Delta R.T.: -0.062 min
Response: 3469723
Conc: 8.69 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB129810TB

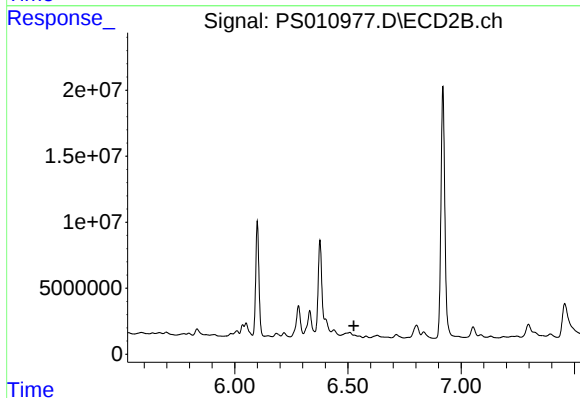


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 6.526 min
Response: 0
Conc: N.D.

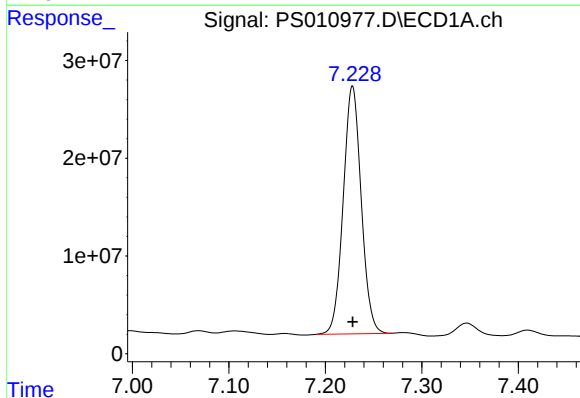


#4 2,4-DCAA

R.T.: 7.228 min
Delta R.T.: 0.000 min
Response: 329615343
Conc: 363.49 ng/ml

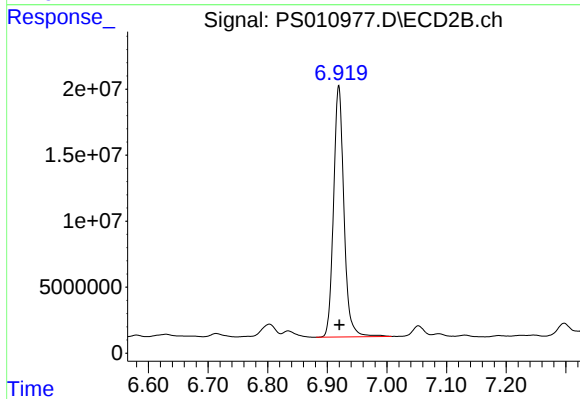

#4 2,4-DCAA


R.T.: 6.919 min
Delta R.T.: -0.001 min
Response: 230425594
Conc: 415.87 ng/ml

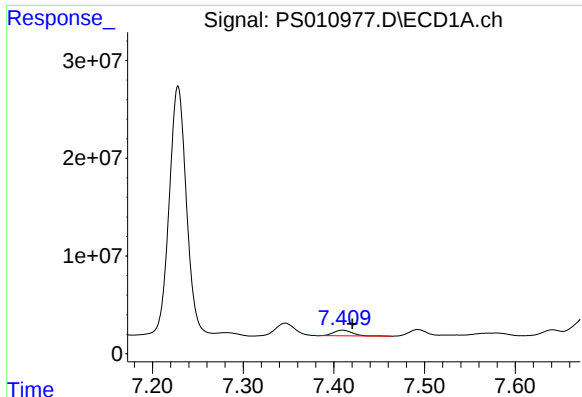

#5 DICAMBA


R.T.: 7.410 min
Delta R.T.: -0.011 min
Response: 8402995
Conc: 2.30 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB129810TB

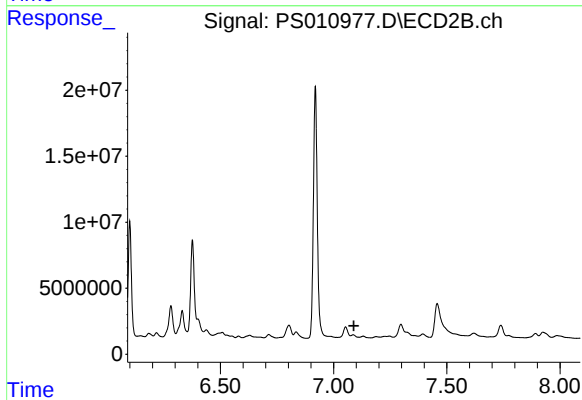


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.089 min
Response: 0
Conc: N.D.

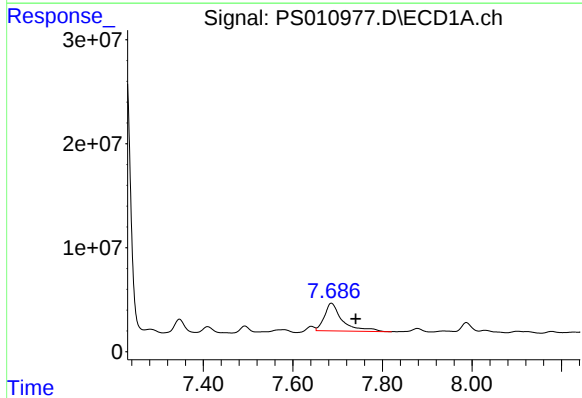


#7 MCPA

R.T.: 7.686 min
Delta R.T.: -0.054 min
Response: 74025101
Conc: 18.59 ug/ml

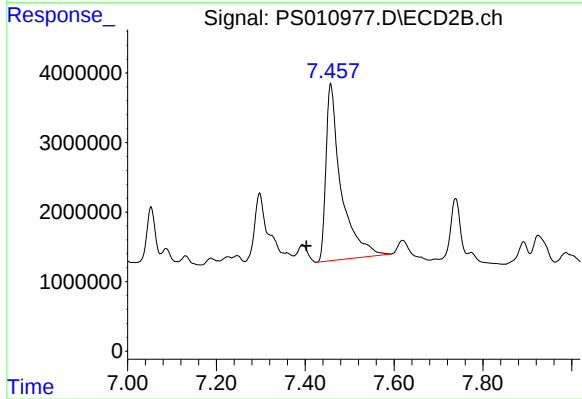

#7 MCPA


R.T.: 7.458 min
Delta R.T.: 0.055 min
Response: 60310393
Conc: 21.85 ug/ml

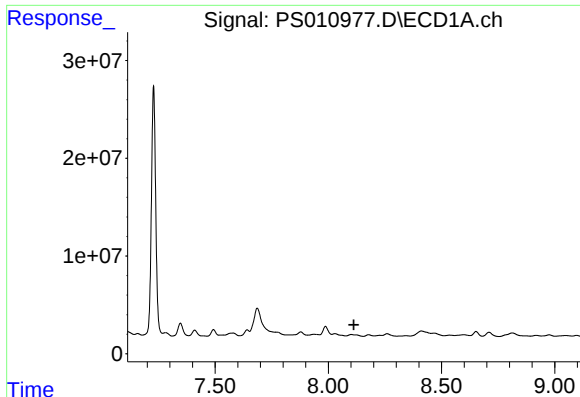

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.113 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB129810TB

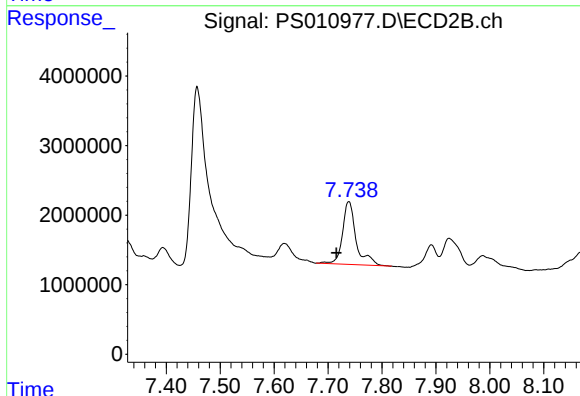


#8 DICHLORPROP

R.T.: 7.739 min
Delta R.T.: 0.023 min
Response: 15861636
Conc: 27.02 ng/ml

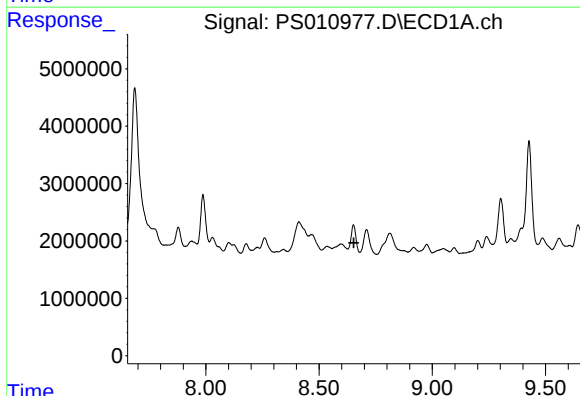


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 8.654 min
Response: 0
Conc: N.D.

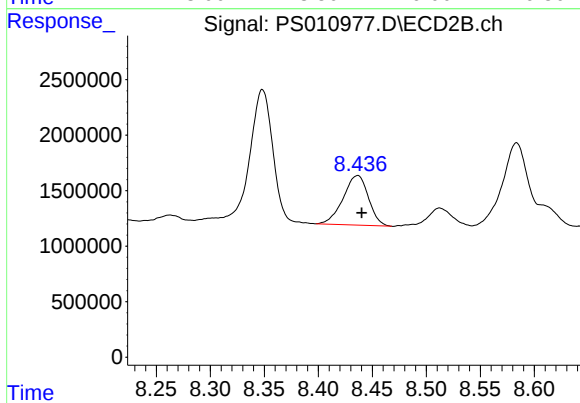

#10 Pentachlorophenol


R.T.: 8.436 min
Delta R.T.: -0.004 min
Response: 7268707
Conc: 1.05 ng/ml

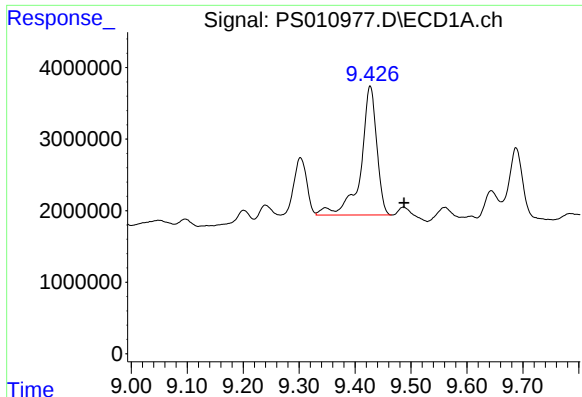

#12 2,4,5-T


R.T.: 9.427 min
Delta R.T.: -0.061 min
Response: 35613602
Conc: 7.65 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB129810TB

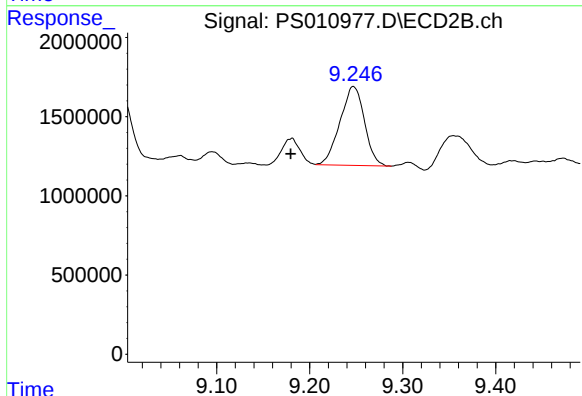


#12 2,4,5-T

R.T.: 9.247 min
Delta R.T.: 0.068 min
Response: 9093190
Conc: 3.05 ng/ml

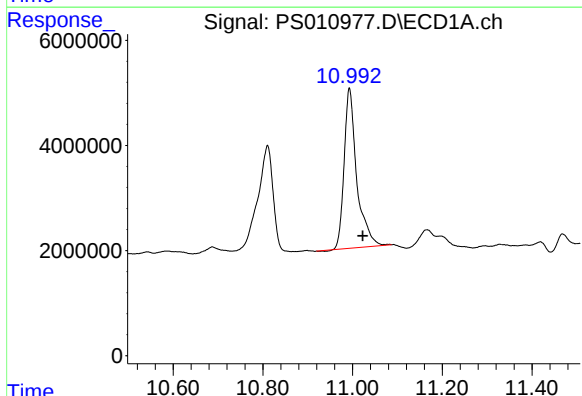

#15 Picloram

R.T.: 10.993 min
Delta R.T.: -0.029 min
Response: 59495169
Conc: 10.61 ng/ml

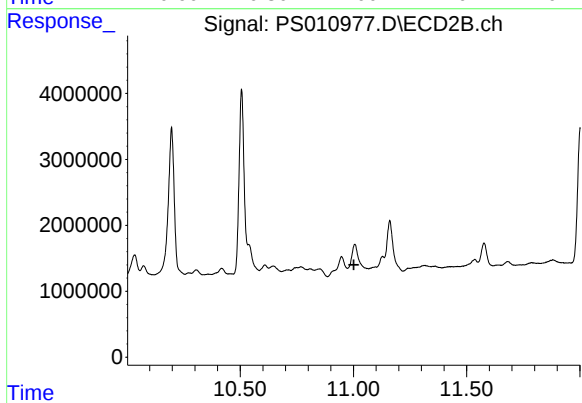

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 11.002 min
Response: 0
Conc: N.D.