

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062620\
 Data File : PS010957.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jun 2020 11:49
 Operator : DD\AJ
 Sample : PB129715BSD
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB129715BSD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 26 12:43:01 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062420.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 25 02:45:12 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.229	6.920	445.2E6	273.5E6	490.972	493.562
Target Compounds							
1) T	Dalapon	3.040	2.624	492.2E6	327.1E6	439.604	433.629
2) T	3,5-DICHL...	6.442	6.069	583.4E6	386.7E6	463.707	464.345
3) T	4-Nitroph...	7.060	6.526	186.0E6	147.3E6	466.000	458.442
5) T	DICAMBA	7.421	7.089	1722.8E6	1090.7E6	472.464	480.229
6) T	MCPD	7.588	7.184	130.4E6	87102746	45.745	46.018
7) T	MCPA	7.737	7.399	183.0E6	125.8E6	45.956	45.590
8) T	DICHLORPROP	8.113	7.714	406.7E6	273.8E6	463.758	466.381
9) T	2,4-D	8.343	8.009	413.3E6	337.8E6	467.387	467.379
10) T	Pentachlo...	8.654	8.440	6164.9E6	3532.7E6	495.804	508.039
11) T	2,4,5-TP ...	9.202	8.799	2389.0E6	1473.5E6	481.133	489.723
12) T	2,4,5-T	9.488	9.179	2243.5E6	1462.9E6	481.650	491.259
13) T	2,4-DB	10.041	9.686	274.7E6	194.6E6	462.132	473.423
14) T	DINOSEB	11.203	10.019	1701.2E6	1019.7E6	475.000	489.759
15) T	Picloram	11.023	11.002	2575.3E6	1973.8E6	459.366	471.112
16) T	DCPA	11.468	10.947	2966.9E6	1863.6E6	485.309	500.374



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062620\
Data File : PS010957.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jun 2020 11:49
Operator : DD\AJ
Sample : PB129715BSD
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PB129715BSD

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 26 12:43:01 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062420.M
Quant Title : 8080.M
QLast Update : Thu Jun 25 02:45:12 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

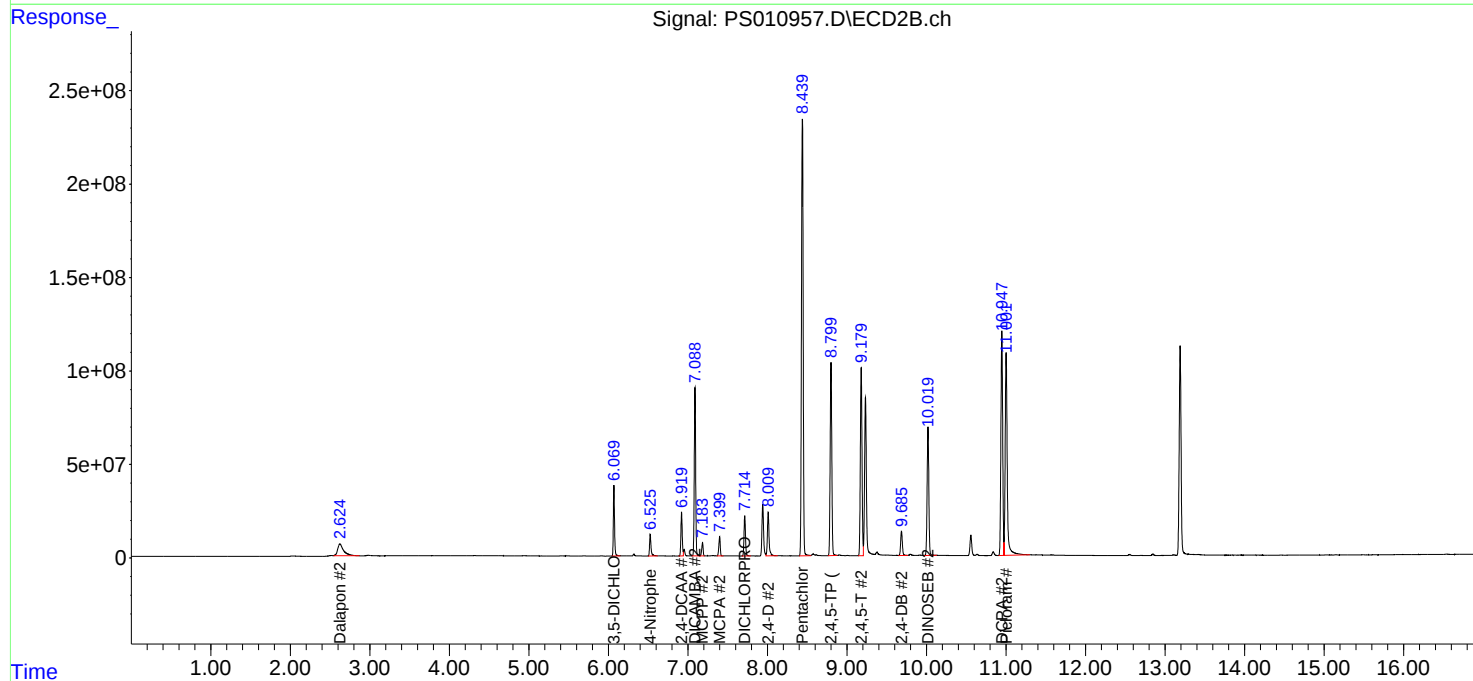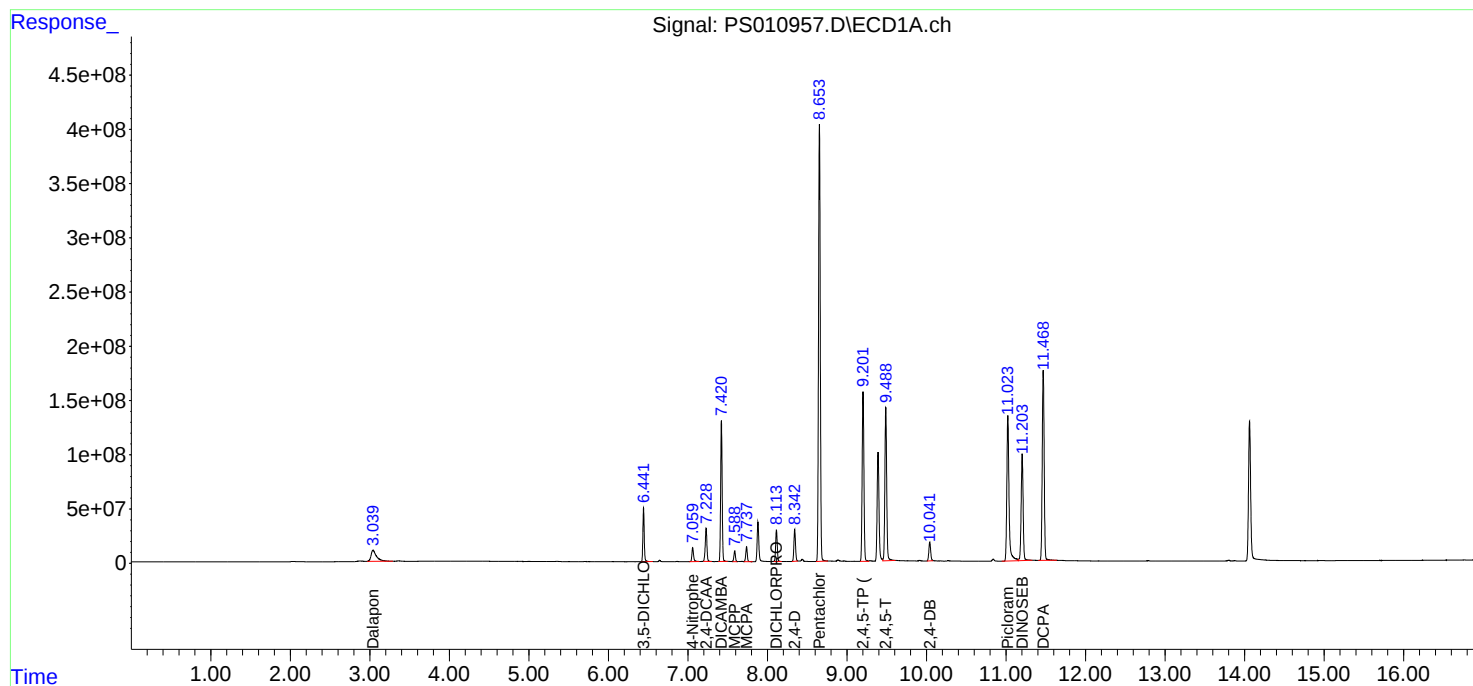


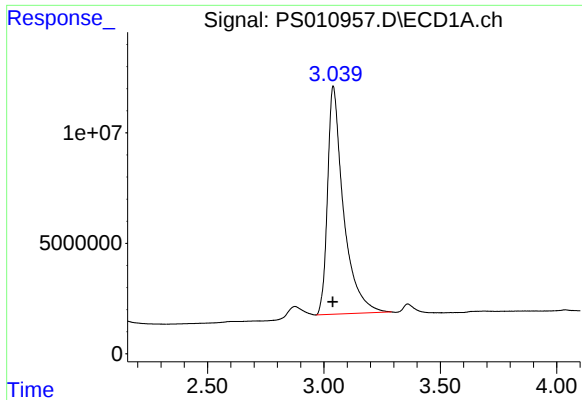

#1 Dalapon


R.T.: 3.040 min
Delta R.T.: 0.002 min
Response: 492234103
Conc: 439.60 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB129715BSD

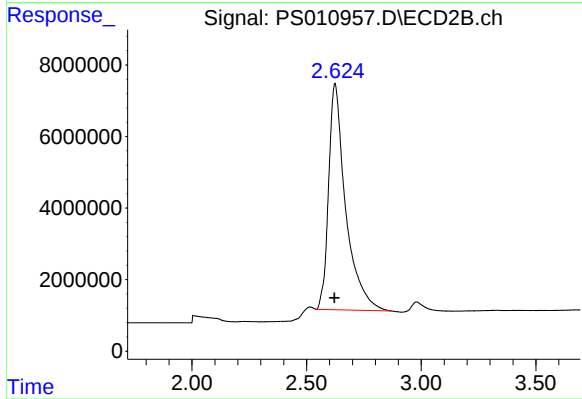


#1 Dalapon

R.T.: 2.624 min
Delta R.T.: 0.002 min
Response: 327112825
Conc: 433.63 ng/ml

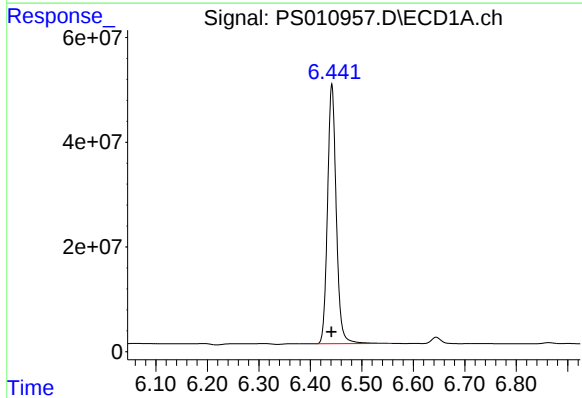


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.442 min
Delta R.T.: 0.000 min
Response: 583366663
Conc: 463.71 ng/ml

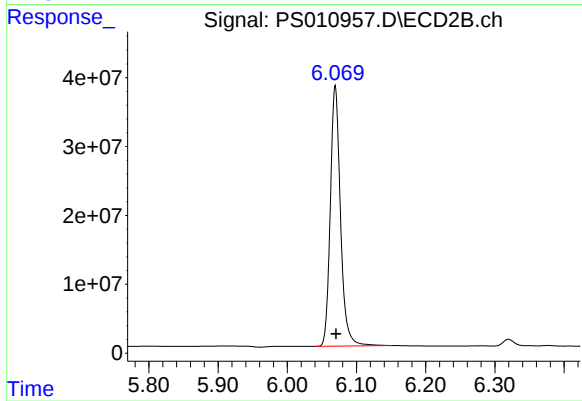

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.069 min
Delta R.T.: -0.001 min
Response: 386718192
Conc: 464.35 ng/ml

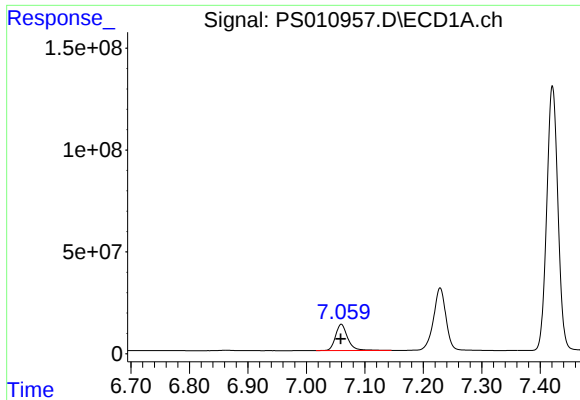

#3 4-Nitrophenol


R.T.: 7.060 min
Delta R.T.: 0.000 min
Response: 186016725
Conc: 466.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB129715BSD

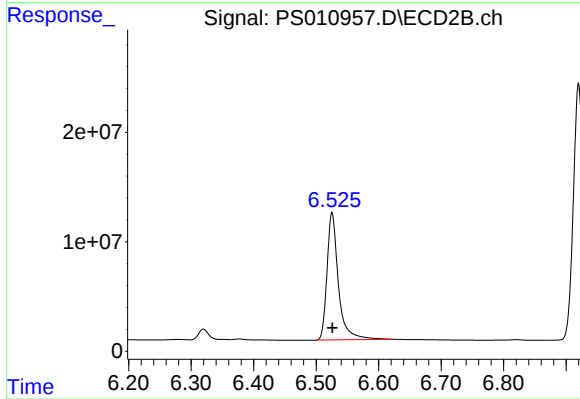


#3 4-Nitrophenol

R.T.: 6.526 min
Delta R.T.: 0.000 min
Response: 147313115
Conc: 458.44 ng/ml

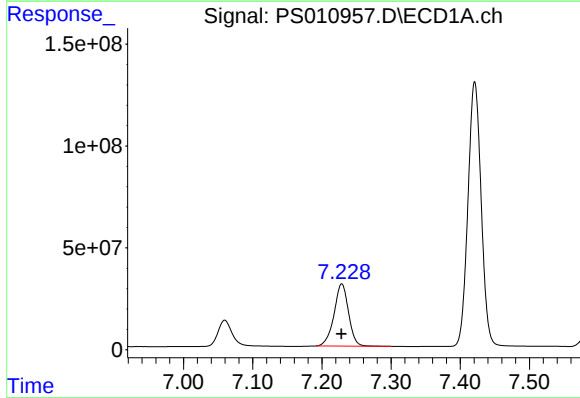


#4 2,4-DCAA

R.T.: 7.229 min
Delta R.T.: 0.000 min
Response: 445222674
Conc: 490.97 ng/ml

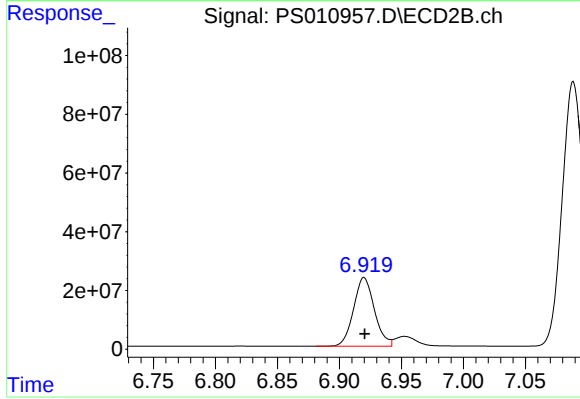

#4 2,4-DCAA


R.T.: 6.920 min
Delta R.T.: 0.000 min
Response: 273471040
Conc: 493.56 ng/ml

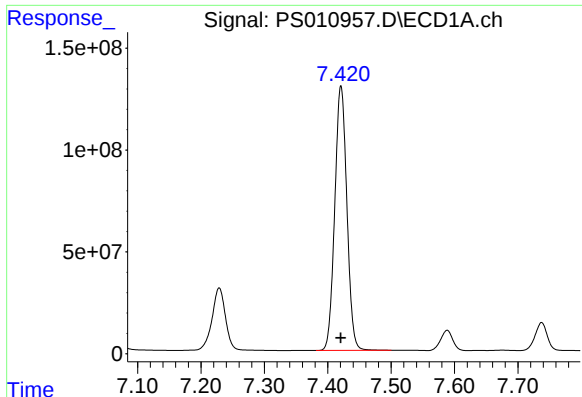

#5 DICAMBA


R.T.: 7.421 min
Delta R.T.: 0.000 min
Response: 1722758212
Conc: 472.46 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB129715BSD

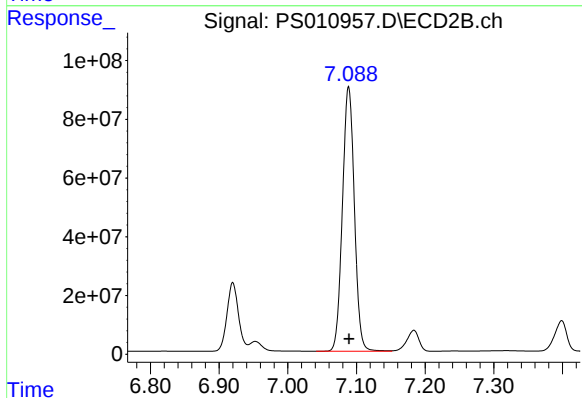


#5 DICAMBA

R.T.: 7.089 min
Delta R.T.: 0.000 min
Response: 1090736527
Conc: 480.23 ng/ml

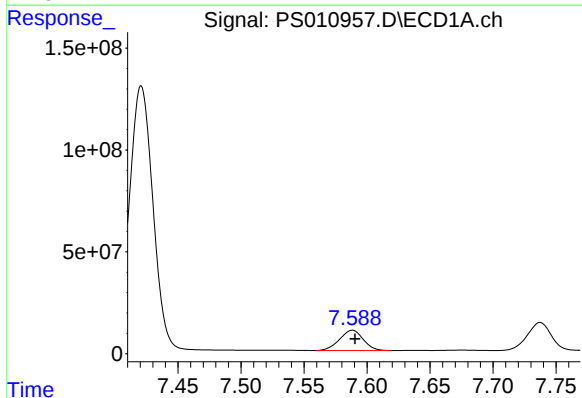


#6 MCP

R.T.: 7.588 min
Delta R.T.: -0.002 min
Response: 130441570
Conc: 45.74 ug/ml

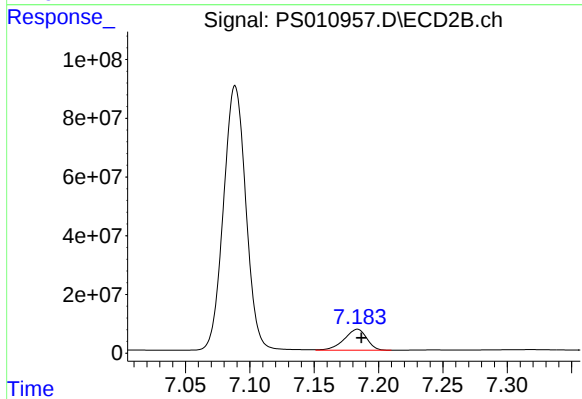

#6 MCP


R.T.: 7.184 min
Delta R.T.: -0.003 min
Response: 87102746
Conc: 46.02 ug/ml

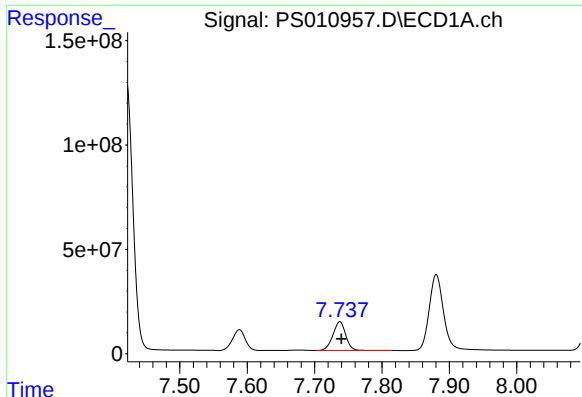

#7 MCPA


R.T.: 7.737 min
Delta R.T.: -0.003 min
Response: 183018060
Conc: 45.96 ug/ml

Instrument :
ECD_S
ClientSampleId :
PB129715BSD

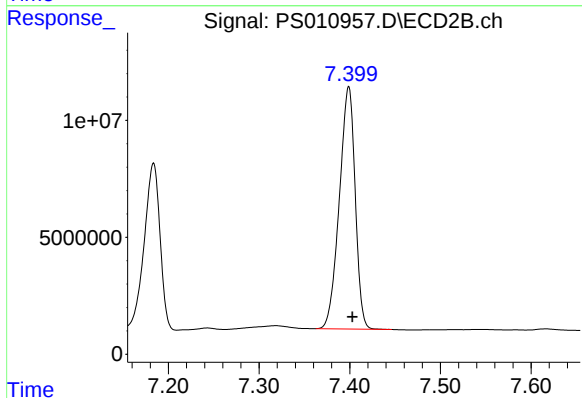


#7 MCPA

R.T.: 7.399 min
Delta R.T.: -0.004 min
Response: 125827397
Conc: 45.59 ug/ml

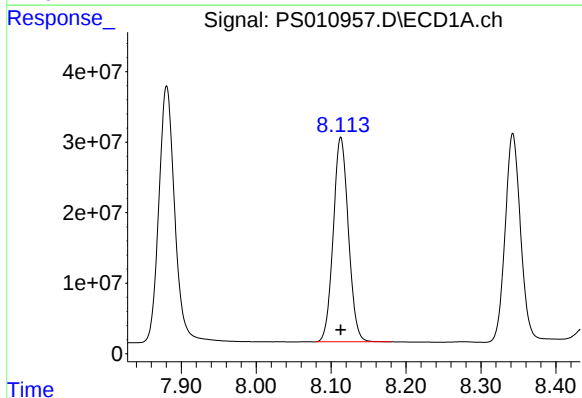


#8 DICHLORPROP

R.T.: 8.113 min
Delta R.T.: 0.000 min
Response: 406682568
Conc: 463.76 ng/ml

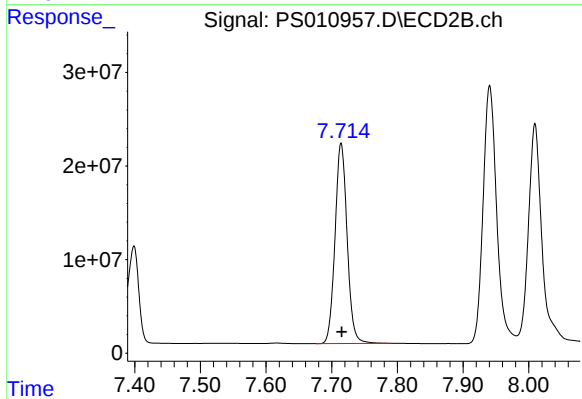

#8 DICHLORPROP


R.T.: 7.714 min
Delta R.T.: 0.000 min
Response: 273828401
Conc: 466.38 ng/ml

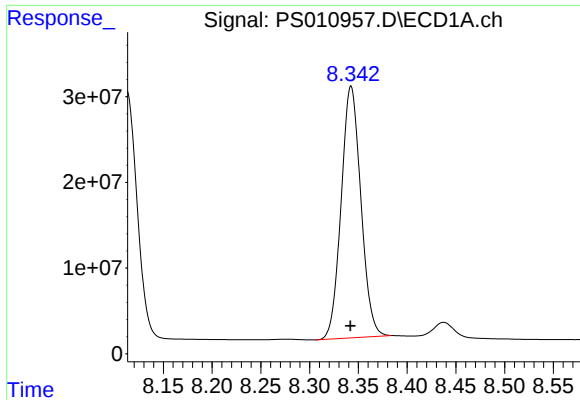

#9 2,4-D


R.T.: 8.343 min
Delta R.T.: 0.000 min
Response: 413309136
Conc: 467.39 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB129715BSD

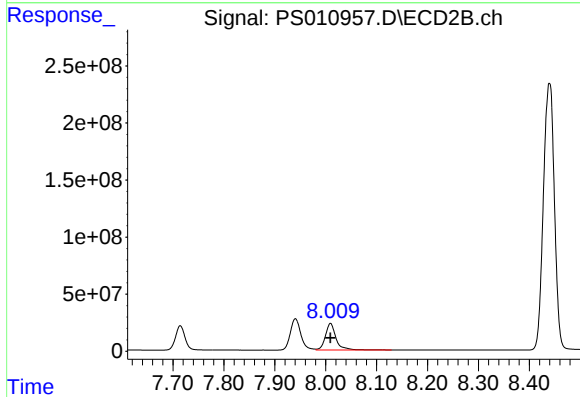


#9 2,4-D

R.T.: 8.009 min
Delta R.T.: 0.000 min
Response: 337753431
Conc: 467.38 ng/ml

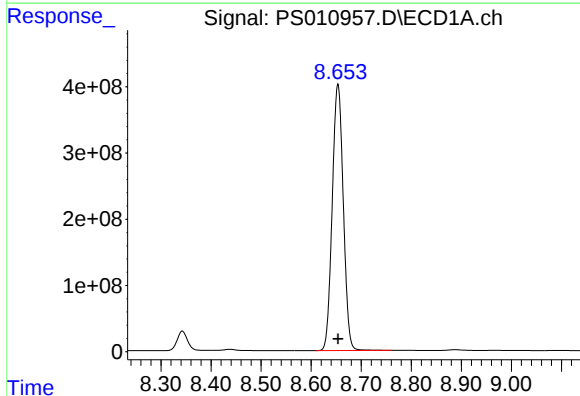


#10 Pentachlorophenol

R.T.: 8.654 min
Delta R.T.: 0.000 min
Response: 6164906749
Conc: 495.80 ng/ml

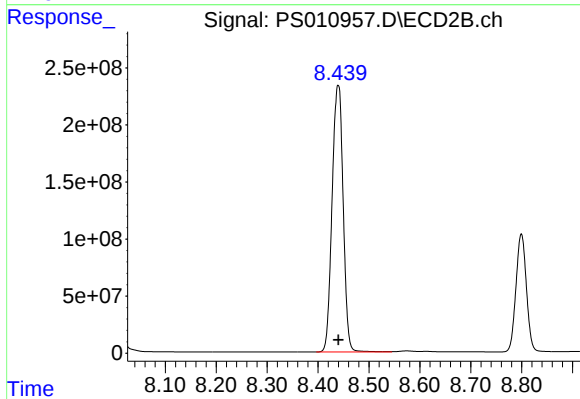

#10 Pentachlorophenol


R.T.: 8.440 min
Delta R.T.: 0.000 min
Response: 3532748005
Conc: 508.04 ng/ml

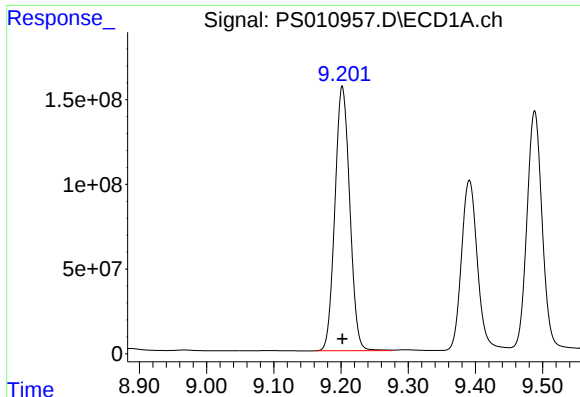

#11 2,4,5-TP (SILVEX)


R.T.: 9.202 min
Delta R.T.: 0.000 min
Response: 2388979780
Conc: 481.13 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB129715BSD

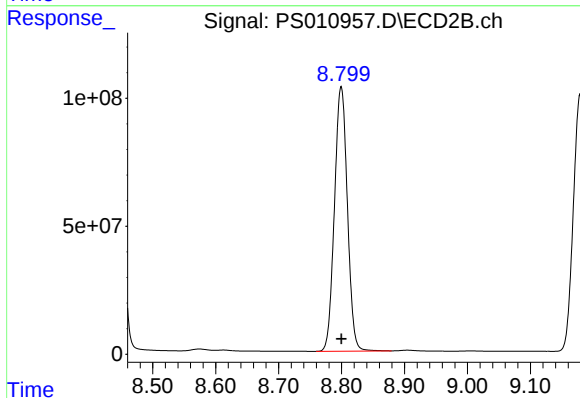


#11 2,4,5-TP (SILVEX)

R.T.: 8.799 min
Delta R.T.: 0.000 min
Response: 1473525785
Conc: 489.72 ng/ml

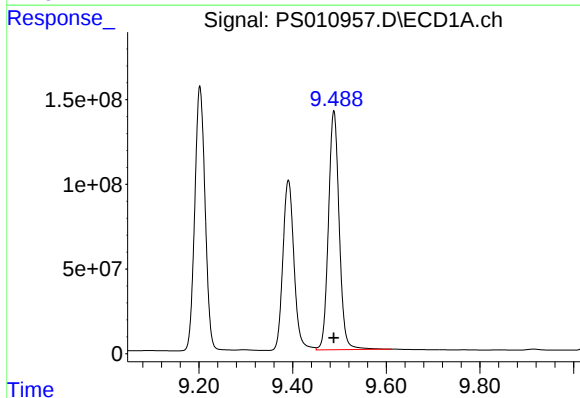


#12 2,4,5-T

R.T.: 9.488 min
Delta R.T.: 0.000 min
Response: 2243491708
Conc: 481.65 ng/ml

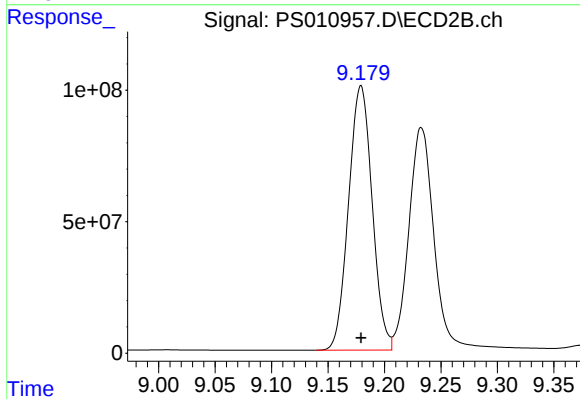

#12 2,4,5-T


R.T.: 9.179 min
Delta R.T.: 0.000 min
Response: 1462901174
Conc: 491.26 ng/ml

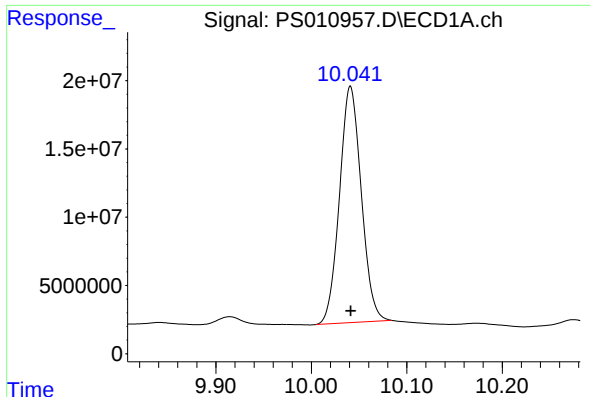

#13 2,4-DB


R.T.: 10.041 min
Delta R.T.: 0.000 min
Response: 274660480
Conc: 462.13 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB129715BSD

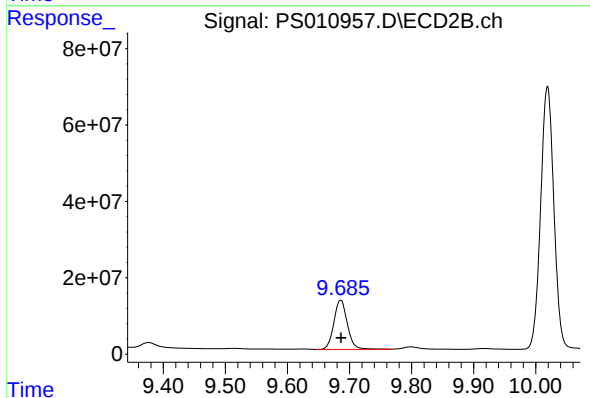


#13 2,4-DB

R.T.: 9.686 min
Delta R.T.: 0.000 min
Response: 194570966
Conc: 473.42 ng/ml

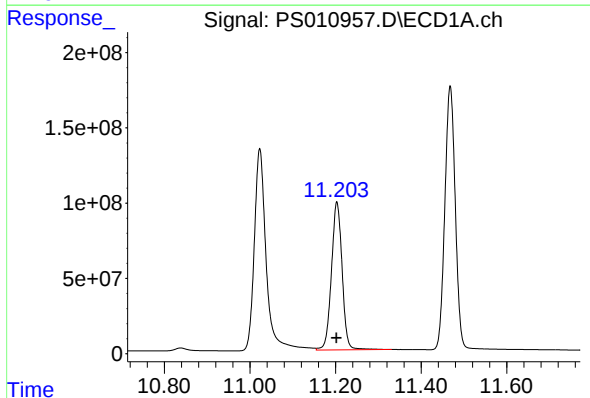


#14 DINOSEB

R.T.: 11.203 min
Delta R.T.: 0.001 min
Response: 1701193244
Conc: 475.00 ng/ml

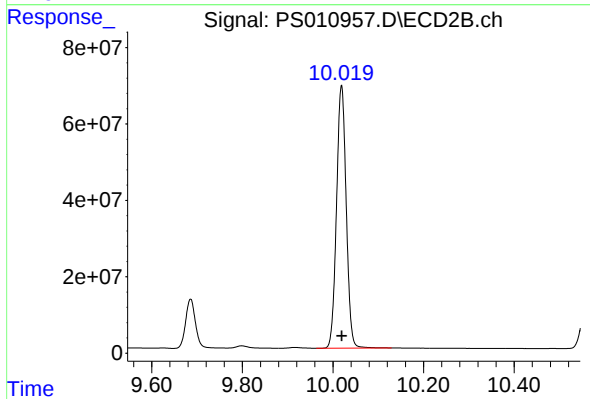

#14 DINOSEB


R.T.: 10.019 min
Delta R.T.: 0.000 min
Response: 1019743262
Conc: 489.76 ng/ml

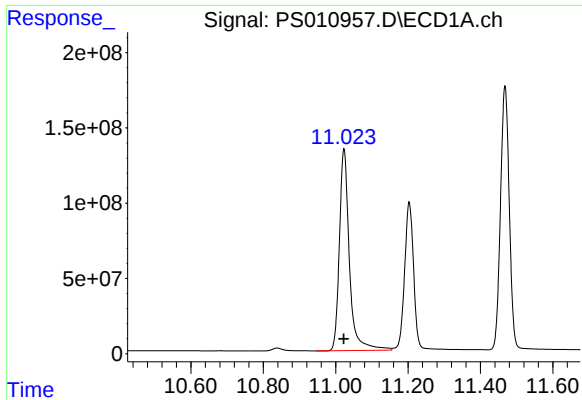

#15 Picloram


R.T.: 11.023 min
Delta R.T.: 0.000 min
Response: 2575271304
Conc: 459.37 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB129715BSD

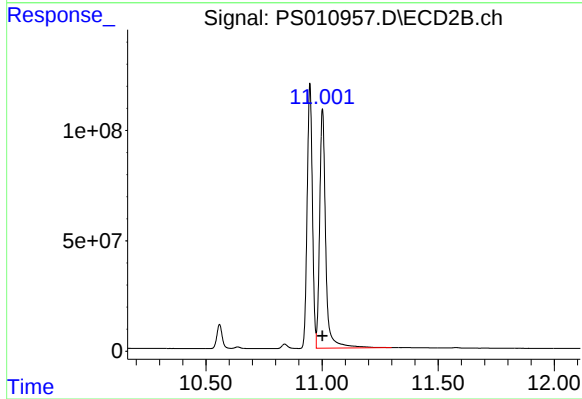


#15 Picloram

R.T.: 11.002 min
Delta R.T.: 0.000 min
Response: 1973753868
Conc: 471.11 ng/ml

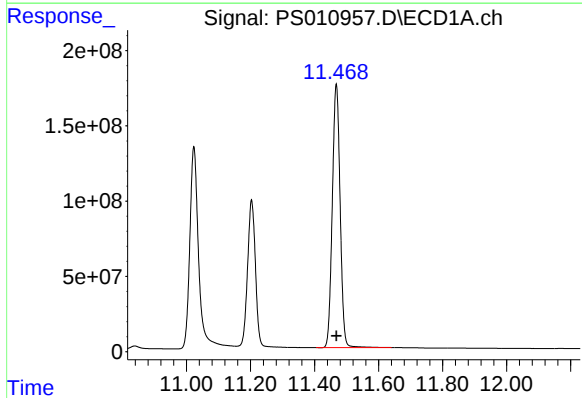

#16 DCPA

R.T.: 11.468 min
Delta R.T.: 0.000 min
Response: 2966923398
Conc: 485.31 ng/ml

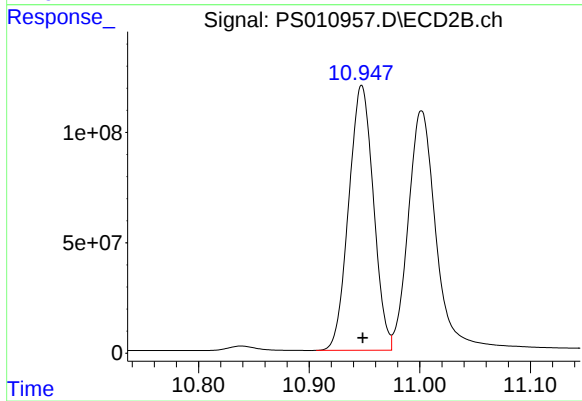

#16 DCPA

R.T.: 10.947 min
Delta R.T.: -0.001 min
Response: 1863589219
Conc: 500.37 ng/ml