

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062623\
 Data File : PS023451.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jun 2023 17:03
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 26 18:37:38 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS060623.M
 Quant Title : 8080.M
 QLast Update : Tue Jun 06 13:00:04 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.479	6.850	1018.3E6	314.7E6	575.566	554.423
Target Compounds							
1) T	Dalapon	2.571	0.000	5240997	0	2.866	N.D. #
3) T	4-Nitroph...	6.313	0.000	12056952	0	9.355	N.D. #
5) T	DICAMBA	6.627	7.014	1494123	989442	<MDL	<MDL #
6) T	MCP	6.816	0.000	1166645	0	<MDL	N.D. #
7) T	MCPA	6.933	0.000	581359	0	<MDL	N.D. #
8) T	DICHLORPROP	7.236	7.654	1978412	1886014	<MDL	3.049 #
9) T	2,4-D	0.000	7.870f	0	838011	N.D.	1.208
10) T	Pentachlo...	7.671	8.356	4799186	4234586	<MDL	<MDL #
11) T	2,4,5-TP ...	8.206	8.716	5407451	821756	<MDL	<MDL #
12) T	2,4,5-T	8.471	9.089	5909306	1917597	<MDL	<MDL #
13) T	2,4-DB	8.977	0.000	12722962	0	5.405	N.D. #
14) T	DINOSEB	10.056	0.000	2521694	0	<MDL	N.D. #
15) T	Picloram	9.881	10.888	177.9E6	36218351	10.252	7.936
16) T	DCPA	10.325	10.888	5212181	36218351	<MDL	9.028 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062623\
Data File : PS023451.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jun 2023 17:03
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 26 18:37:38 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS060623.M
Quant Title : 8080.M
QLast Update : Tue Jun 06 13:00:04 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

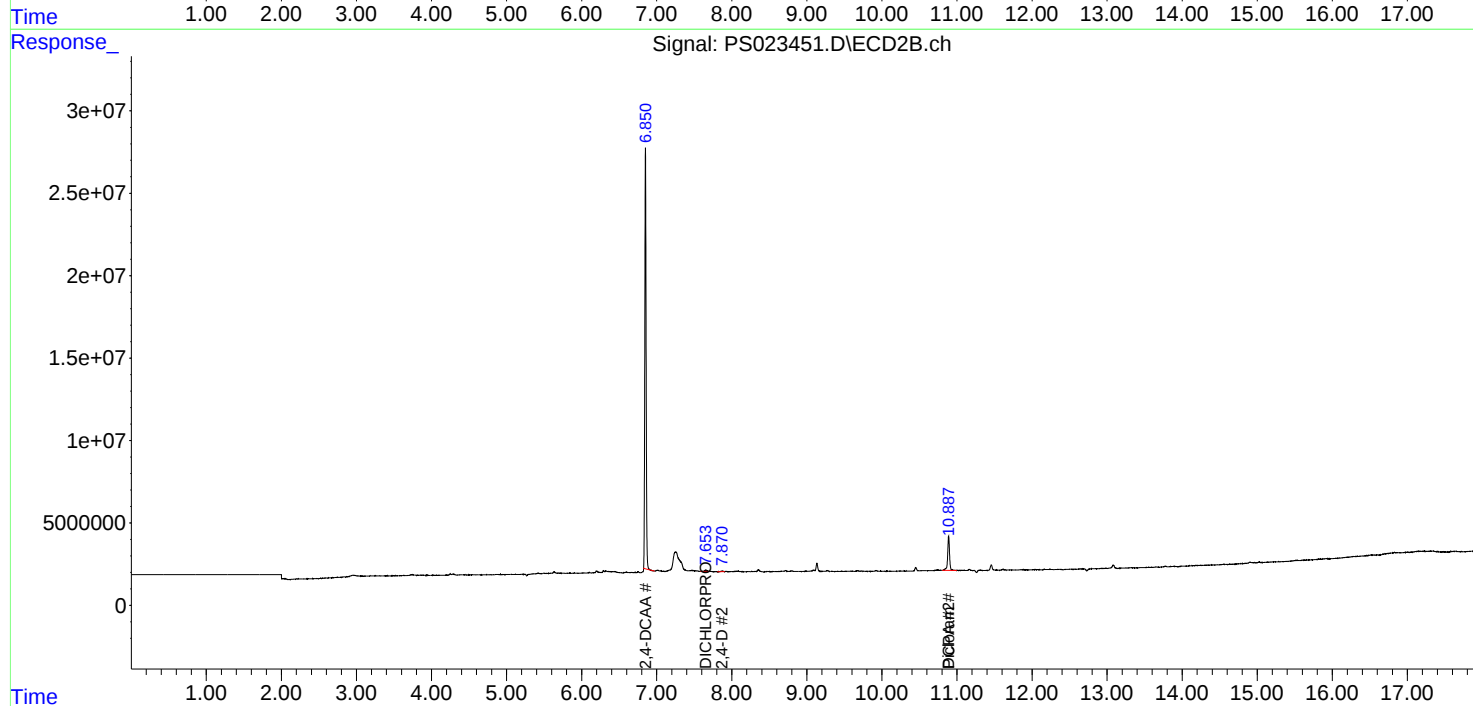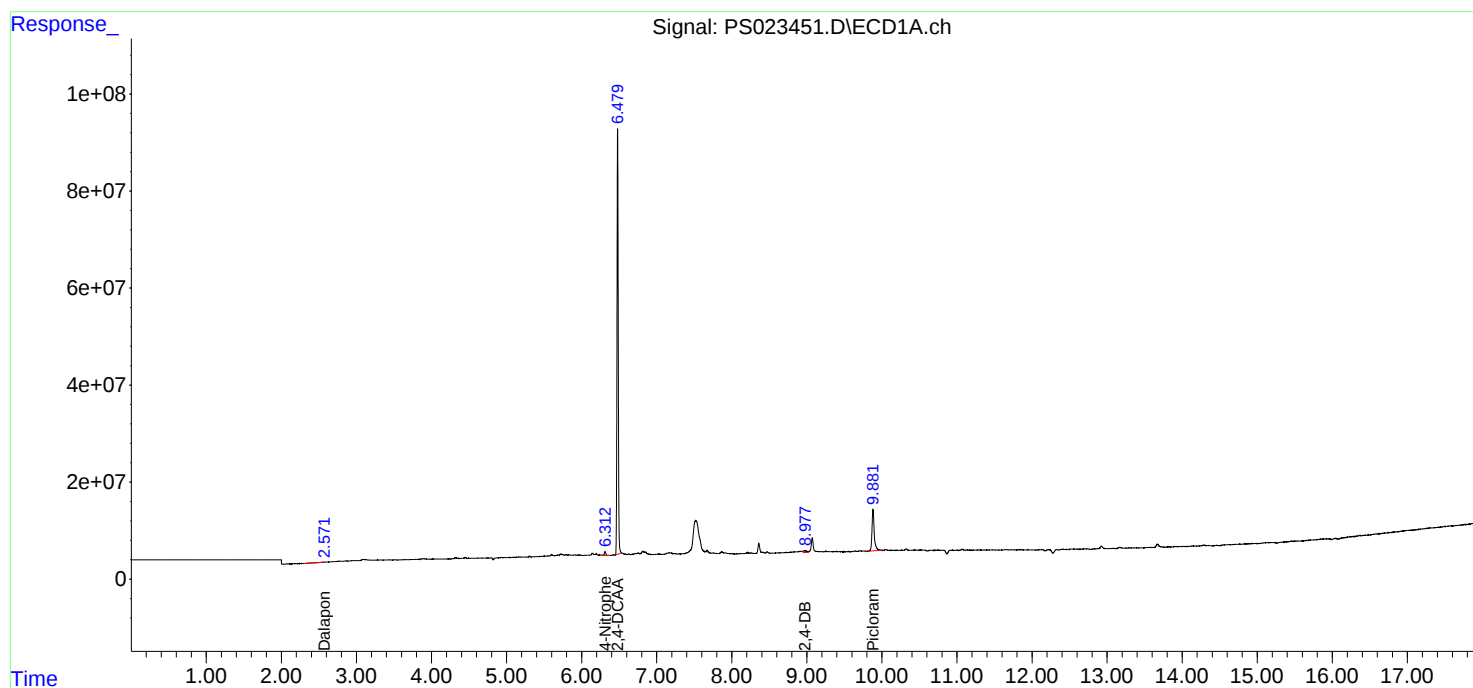


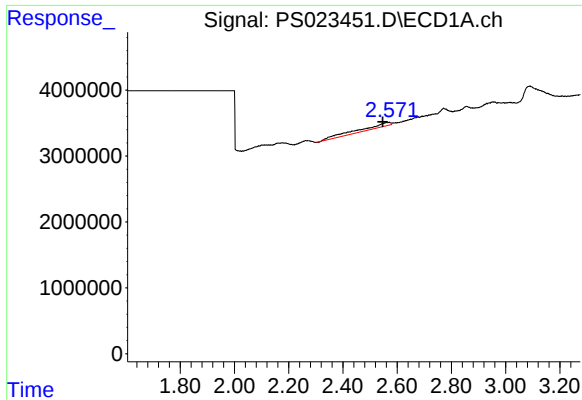

#1 Dalapon


R.T.: 2.571 min
Delta R.T.: 0.024 min
Response: 5240997
Conc: 2.87 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

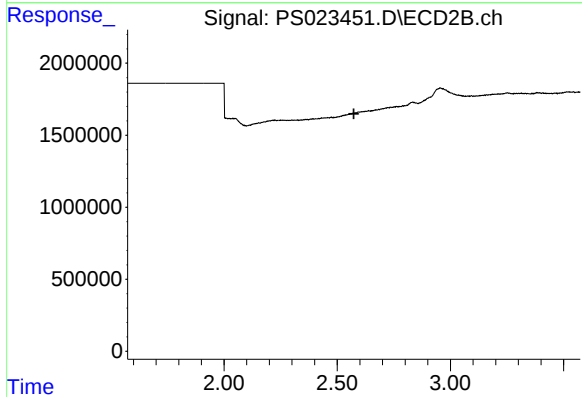


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.574 min
Response: 0
Conc: N.D.

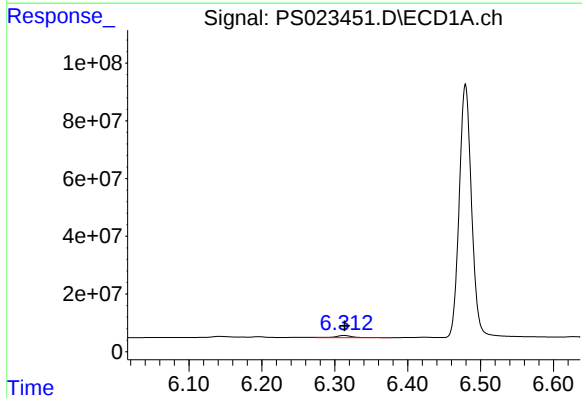


#3 4-Nitrophenol

R.T.: 6.313 min
Delta R.T.: -0.001 min
Response: 12056952
Conc: 9.35 ng/ml

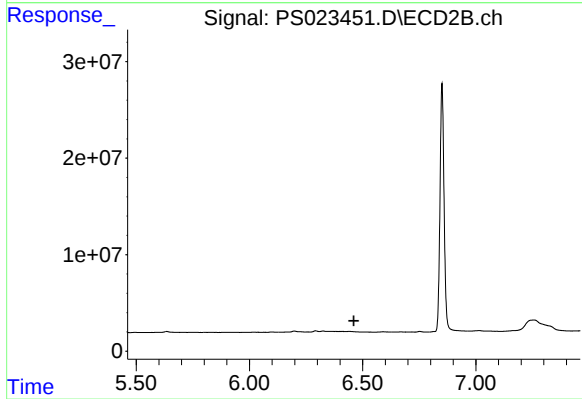

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 6.461 min
Response: 0
Conc: N.D.

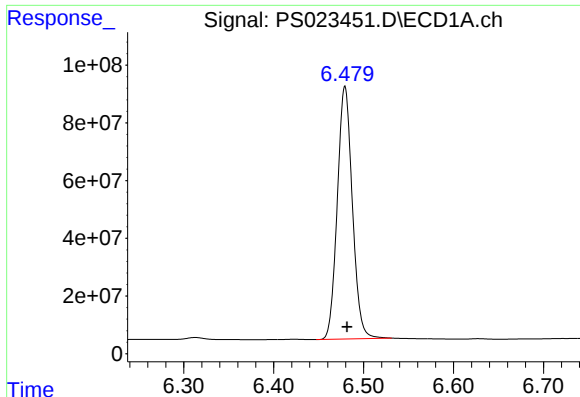

#4 2,4-DCAA


R.T.: 6.479 min
Delta R.T.: -0.002 min
Response: 1018324312
Conc: 575.57 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

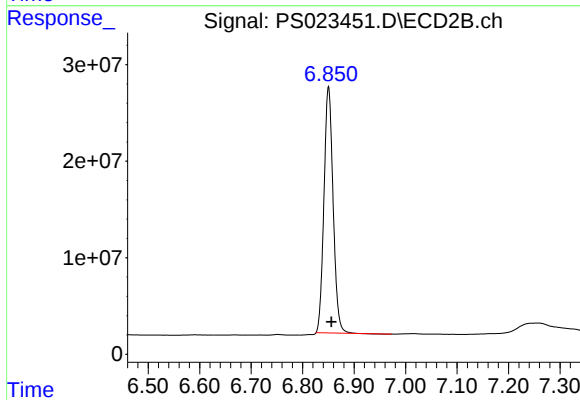


#4 2,4-DCAA

R.T.: 6.850 min
Delta R.T.: -0.006 min
Response: 314743390
Conc: 554.42 ng/ml

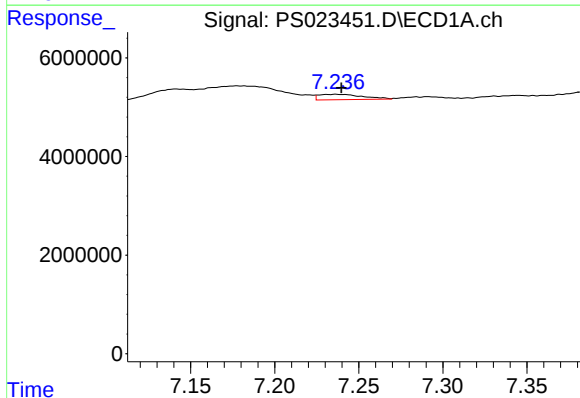


#8 DICHLORPROP

R.T.: 7.236 min
Delta R.T.: -0.003 min
Response: 1978412
Conc: N.D.

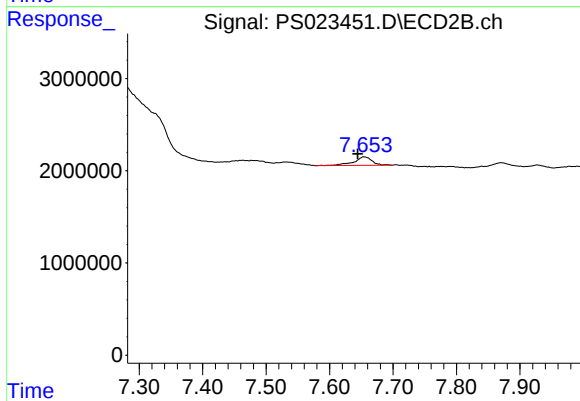

#8 DICHLORPROP


R.T.: 7.654 min
Delta R.T.: 0.010 min
Response: 1886014
Conc: 3.05 ng/ml

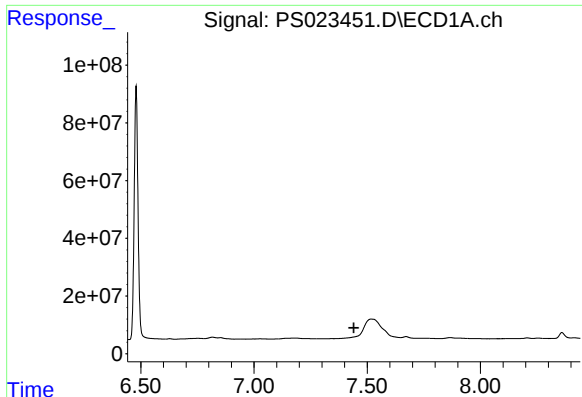

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 7.442 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

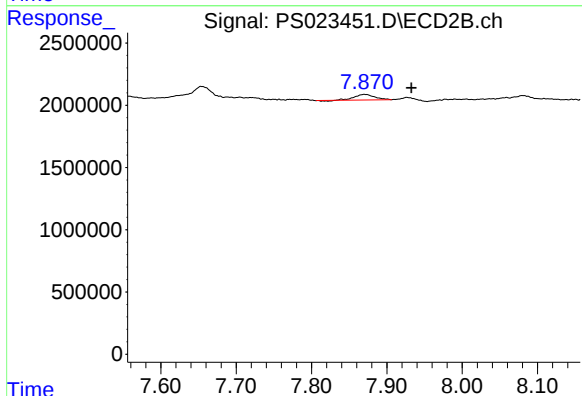


#9 2,4-D

R.T.: 7.870 min
Delta R.T.: -0.063 min
Response: 838011
Conc: 1.21 ng/ml

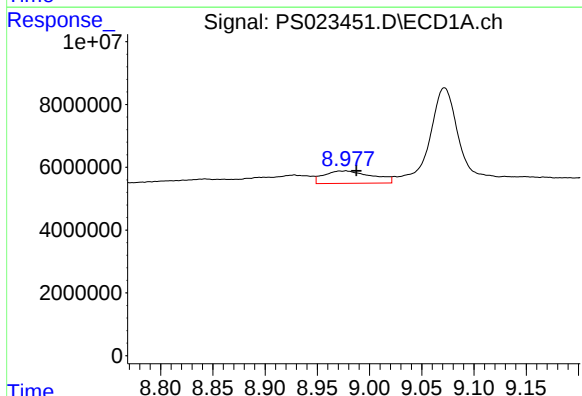


#13 2,4-DB

R.T.: 8.977 min
Delta R.T.: -0.010 min
Response: 12722962
Conc: 5.40 ng/ml

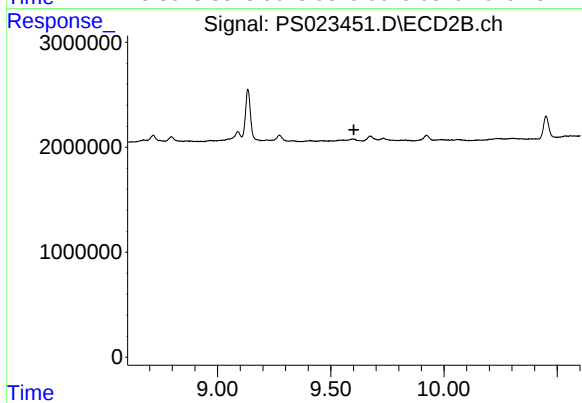

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 9.602 min
Response: 0
Conc: N.D.

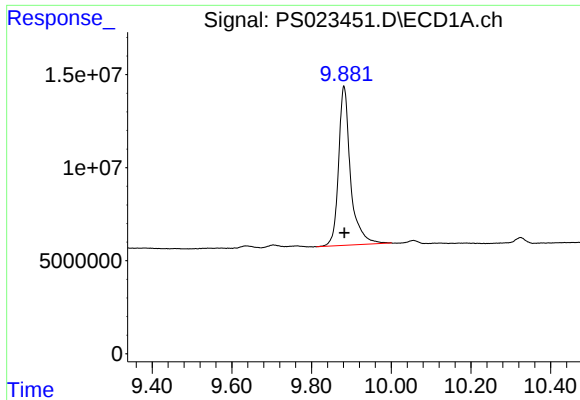

#15 Picloram


R.T.: 9.881 min
Delta R.T.: -0.001 min
Response: 177924688
Conc: 10.25 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

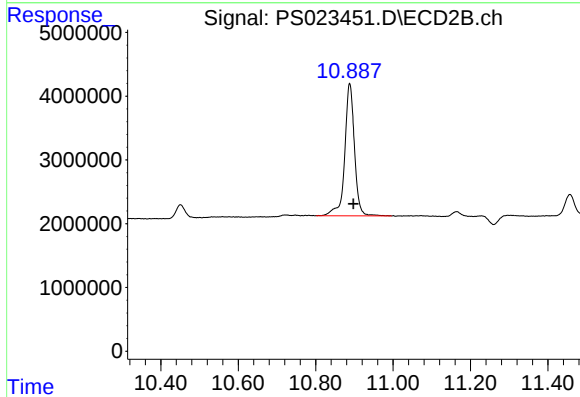


#15 Picloram

R.T.: 10.888 min
Delta R.T.: -0.010 min
Response: 36218351
Conc: 7.94 ng/ml

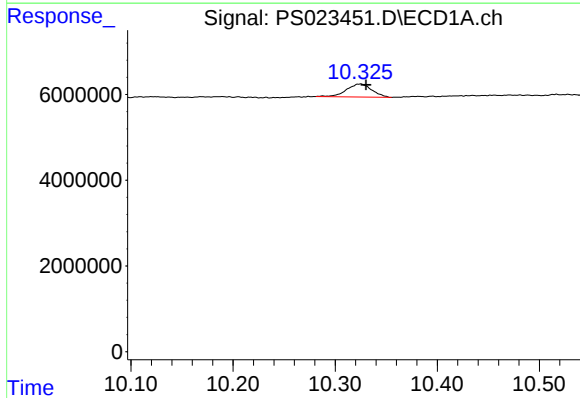

#16 DCPA

R.T.: 10.325 min
Delta R.T.: -0.006 min
Response: 5212181
Conc: N.D.

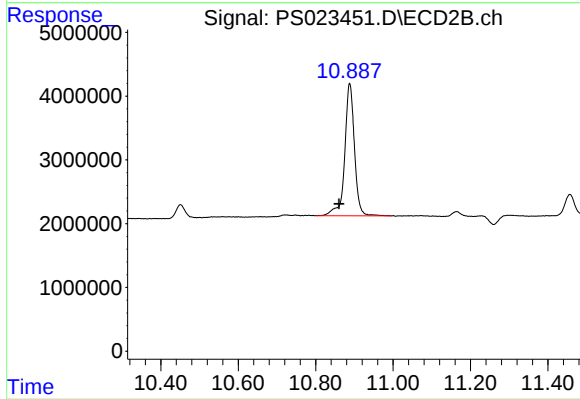

#16 DCPA

R.T.: 10.888 min
Delta R.T.: 0.028 min
Response: 36218351
Conc: 9.03 ng/ml