

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062623\
 Data File : PS023457.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jun 2023 19:53
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 27 00:24:27 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS060623.M
 Quant Title : 8080.M
 QLast Update : Tue Jun 06 13:00:04 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.477	6.851	1027.8E6	323.4E6	580.919	569.656
Target Compounds							
1) T	Dalapon	2.577	0.000	5148459	0	2.816	N.D. #
2) T	3,5-DICHL...	5.797	0.000	924794	0	<MDL	N.D. #
3) T	4-Nitroph...	6.311	0.000	10523359	0	8.165	N.D. #
5) T	DICAMBA	6.623	0.000	241973	0	<MDL	N.D. #
6) T	MCP	6.813	0.000	2909809	0	<MDL	N.D. #
7) T	MCPA	6.927	7.300	118251	18825892	<MDL	7.005 #
8) T	DICHLORPROP	7.226	7.654	1340514	1592217	<MDL	2.574 #
10) T	Pentachlo...	7.668	8.357	553472	1233625	<MDL	<MDL #
11) T	2,4,5-TP ...	8.205	0.000	5242323	0	<MDL	N.D. #
12) T	2,4,5-T	8.472	9.134	1593527	1109193	<MDL	<MDL #
13) T	2,4-DB	8.995	0.000	51293113	0	21.789	N.D. #
14) T	DINOSEB	10.045	0.000	1176811	0	<MDL	N.D. #
15) T	Picloram	9.879	10.888	26921524	4872819	1.551	1.068 #
16) T	DCPA	10.321	10.888	2028792	4872819	<MDL	1.215 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062623\
Data File : PS023457.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jun 2023 19:53
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 27 00:24:27 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS060623.M
Quant Title : 8080.M
QLast Update : Tue Jun 06 13:00:04 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

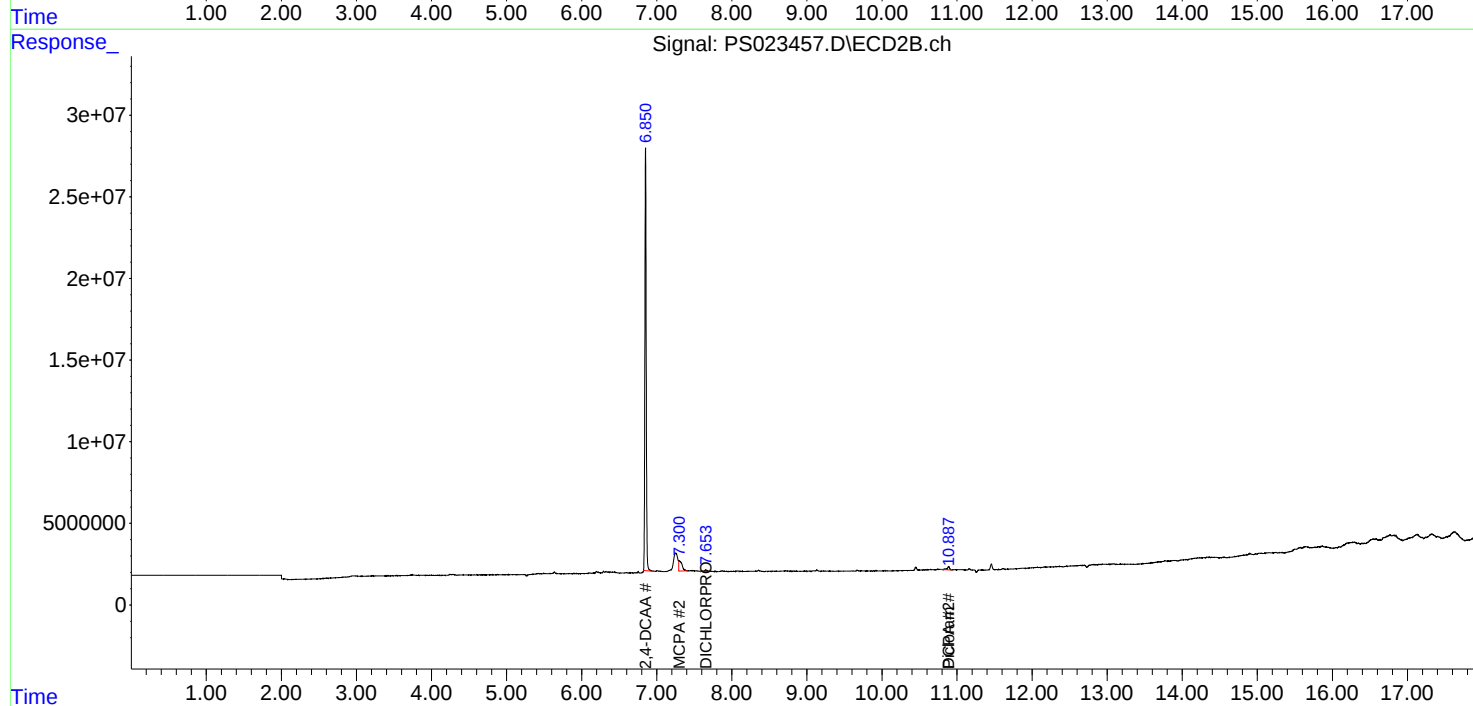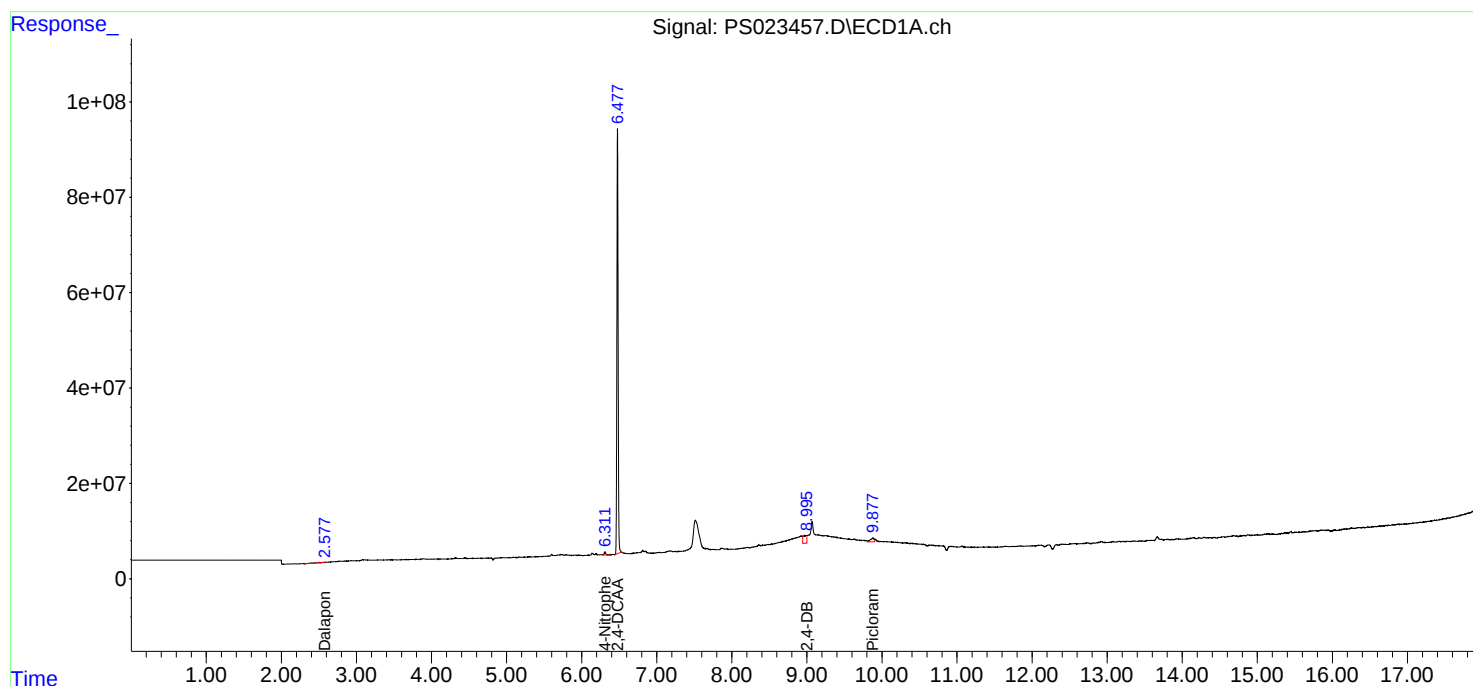


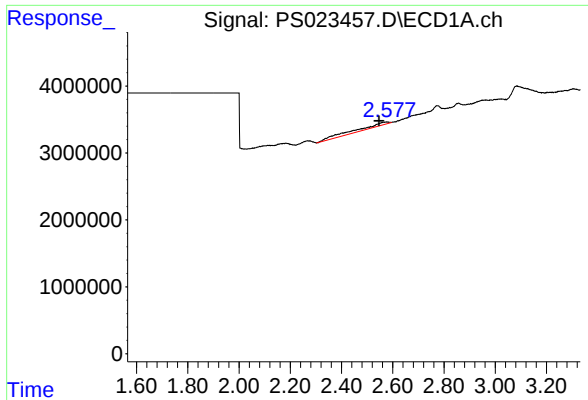

#1 Dalapon


R.T.: 2.577 min
Delta R.T.: 0.030 min
Response: 5148459
Conc: 2.82 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

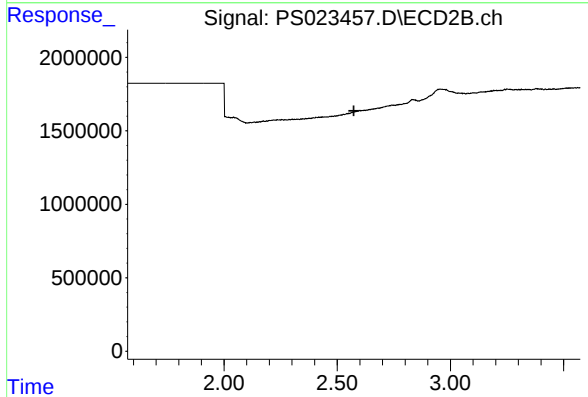


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.574 min
Response: 0
Conc: N.D.

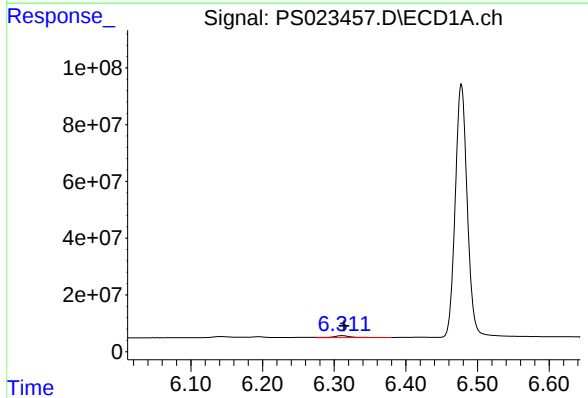


#3 4-Nitrophenol

R.T.: 6.311 min
Delta R.T.: -0.003 min
Response: 10523359
Conc: 8.17 ng/ml

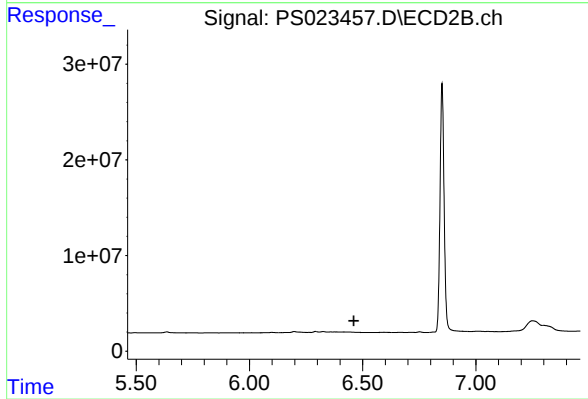

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 6.461 min
Response: 0
Conc: N.D.

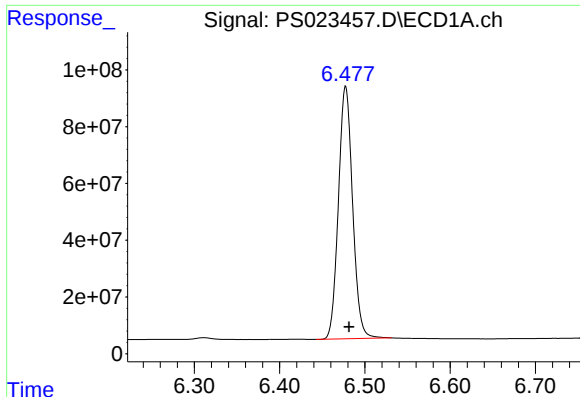

#4 2,4-DCAA


R.T.: 6.477 min
Delta R.T.: -0.004 min
Response: 1027793625
Conc: 580.92 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

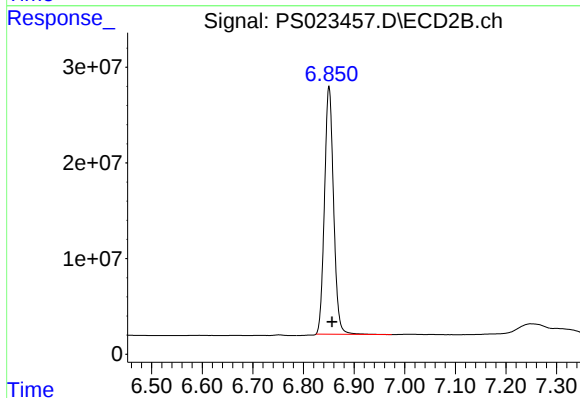


#4 2,4-DCAA

R.T.: 6.851 min
Delta R.T.: -0.006 min
Response: 323390901
Conc: 569.66 ng/ml

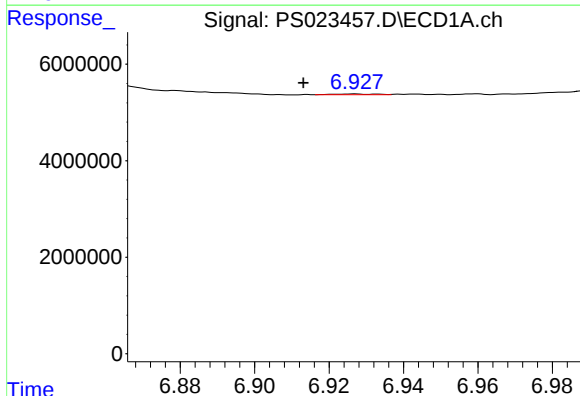


#7 MCPA

R.T.: 6.927 min
Delta R.T.: 0.013 min
Response: 118251
Conc: N.D.

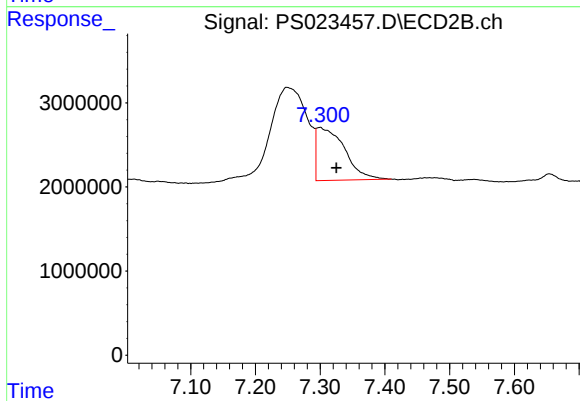

#7 MCPA


R.T.: 7.300 min
Delta R.T.: -0.025 min
Response: 18825892
Conc: 7.00 ug/ml

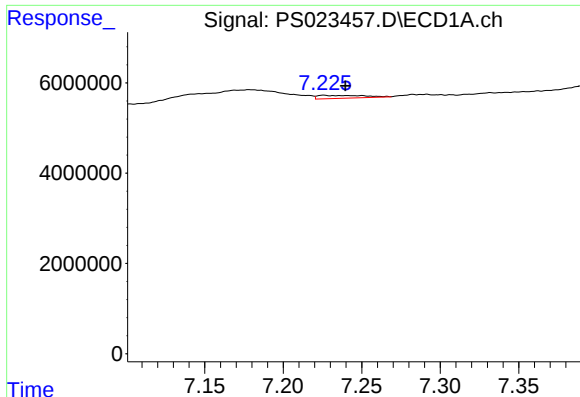

#8 DICHLORPROP


R.T.: 7.226 min
Delta R.T.: -0.014 min
Response: 1340514
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

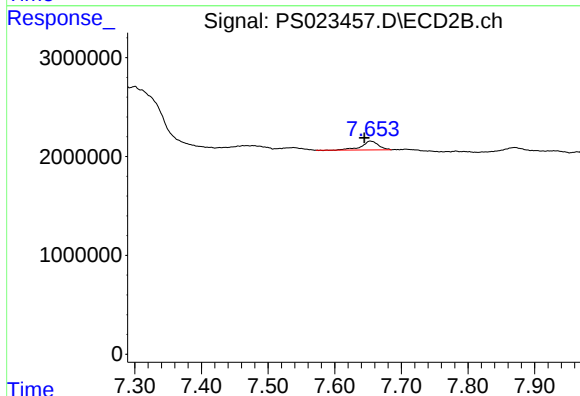


#8 DICHLORPROP

R.T.: 7.654 min
Delta R.T.: 0.009 min
Response: 1592217
Conc: 2.57 ng/ml

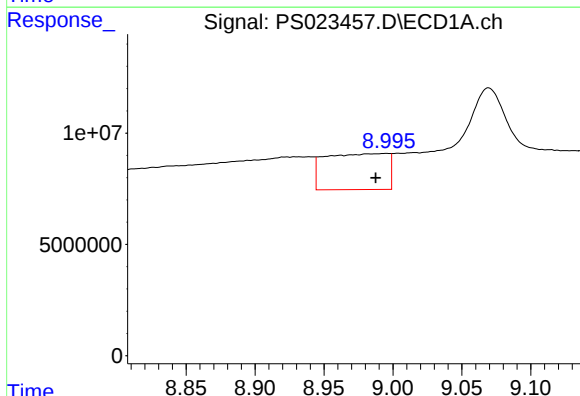


#13 2,4-DB

R.T.: 8.995 min
Delta R.T.: 0.008 min
Response: 51293113
Conc: 21.79 ng/ml

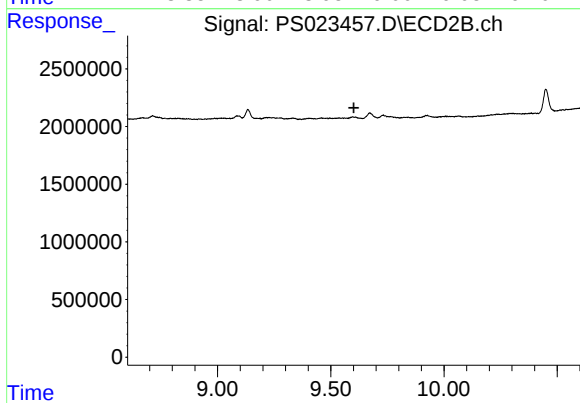

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 9.602 min
Response: 0
Conc: N.D.

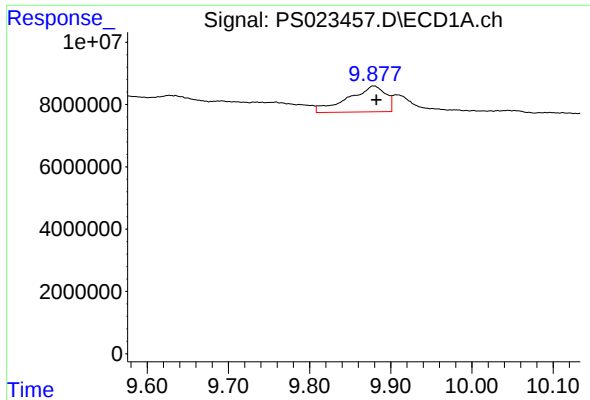

#15 Picloram


R.T.: 9.879 min
Delta R.T.: -0.004 min
Response: 26921524
Conc: 1.55 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

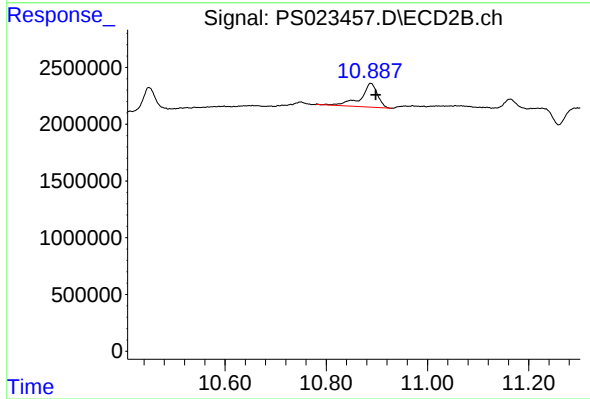


#15 Picloram

R.T.: 10.888 min
Delta R.T.: -0.010 min
Response: 4872819
Conc: 1.07 ng/ml

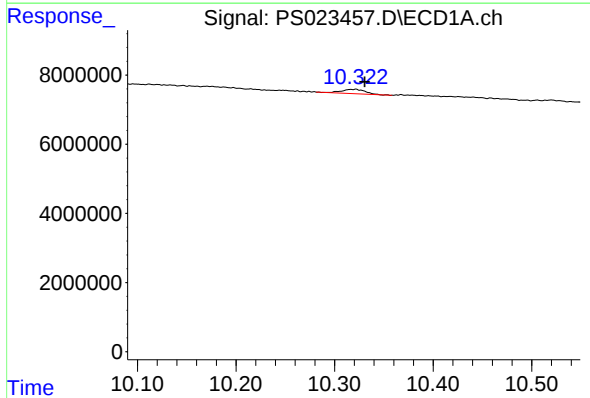

#16 DCPA

R.T.: 10.321 min
Delta R.T.: -0.009 min
Response: 2028792
Conc: N.D.

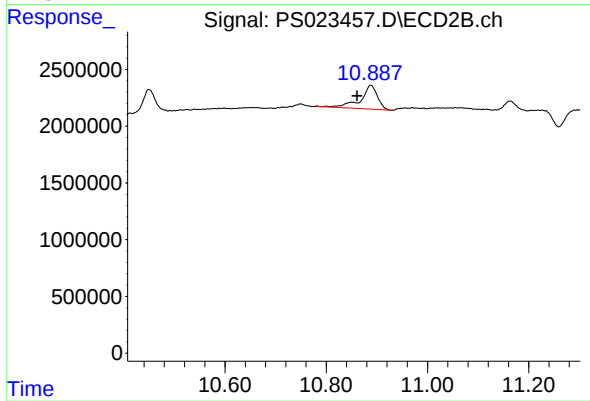

#16 DCPA

R.T.: 10.888 min
Delta R.T.: 0.027 min
Response: 4872819
Conc: 1.21 ng/ml