

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062623\
 Data File : PS023477.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jun 2023 04:48
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 27 07:40:38 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS060623.M
 Quant Title : 8080.M
 QLast Update : Tue Jun 06 13:00:04 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.478	6.849	1046.5E6	323.3E6	591.466	569.576
Target Compounds							
1) T	Dalapon	2.572	0.000	1105809	0	<MDL	N.D. #
2) T	3,5-DICHL...	5.797	0.000	715954	0	<MDL	N.D. #
3) T	4-Nitroph...	6.311	0.000	12184354	0	9.454	N.D. #
5) T	DICAMBA	6.623	0.000	156825	0	<MDL	N.D. #
6) T	MCP	6.813	0.000	2007452	0	<MDL	N.D. #
7) T	MCPA	6.926	0.000	301010	0	<MDL	N.D. #
8) T	DICHLORPROP	7.238	7.654	1068444	1646321	<MDL	2.661 #
9) T	2,4-D	0.000	7.868f	0	1093935	N.D.	1.577
10) T	Pentachlo...	7.669	8.354	2520742	1172392	<MDL	<MDL #
11) T	2,4,5-TP ...	8.206	0.000	4399625	0	<MDL	N.D. #
12) T	2,4,5-T	8.472	9.133	2761387	1115611	<MDL	<MDL #
13) T	2,4-DB	8.992	0.000	1159528	0	<MDL	N.D. #
14) T	DINOSEB	10.053	0.000	996473	0	<MDL	N.D. #
15) T	Picloram	9.883	10.888	20687569	3883355	1.192	<MDL #
16) T	DCPA	10.324	10.888	2654828	3883355	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062623\
Data File : PS023477.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jun 2023 04:48
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 27 07:40:38 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS060623.M
Quant Title : 8080.M
QLast Update : Tue Jun 06 13:00:04 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

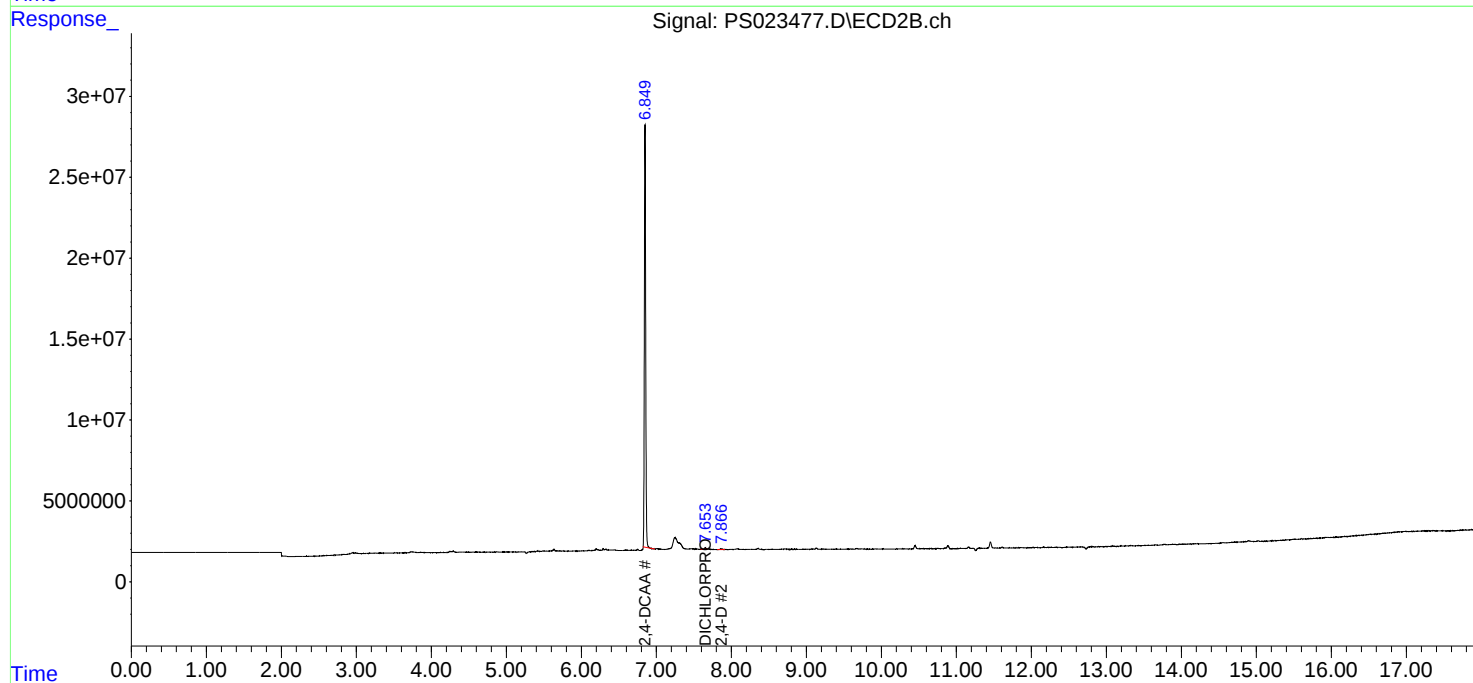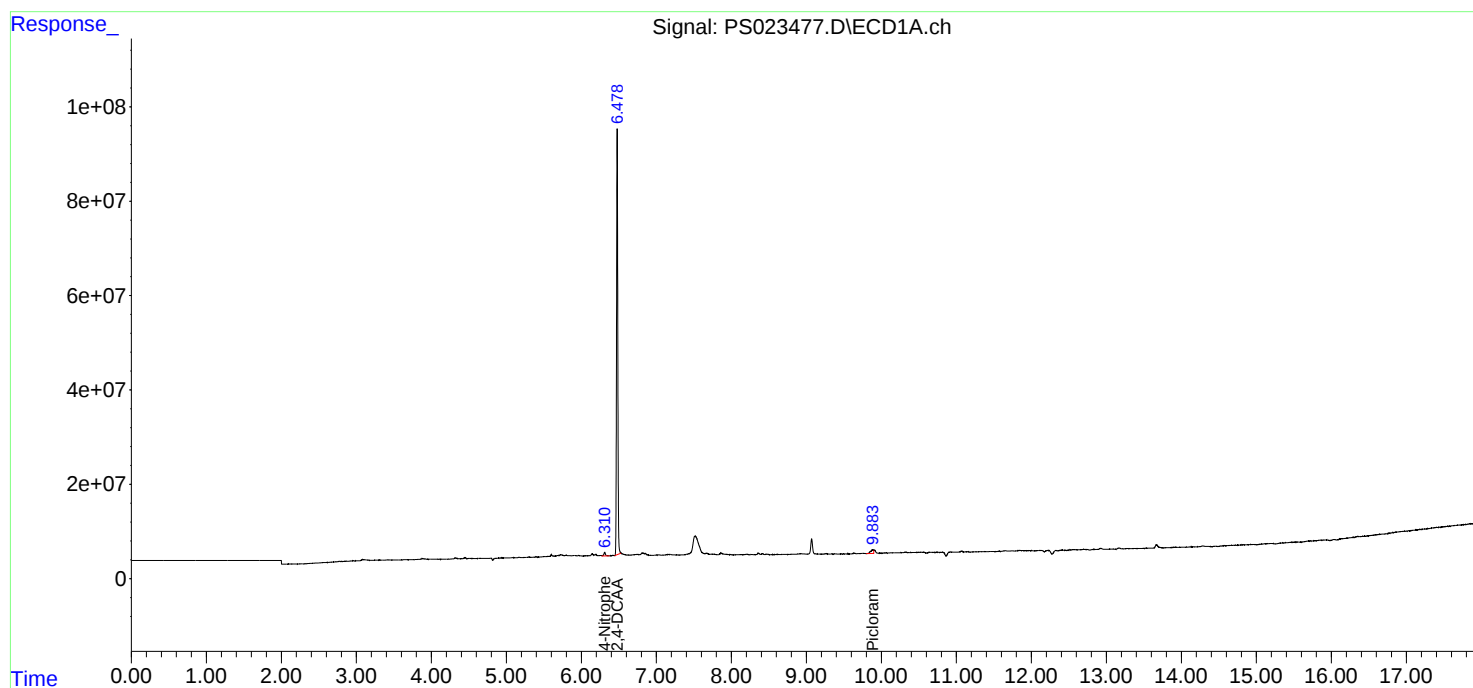


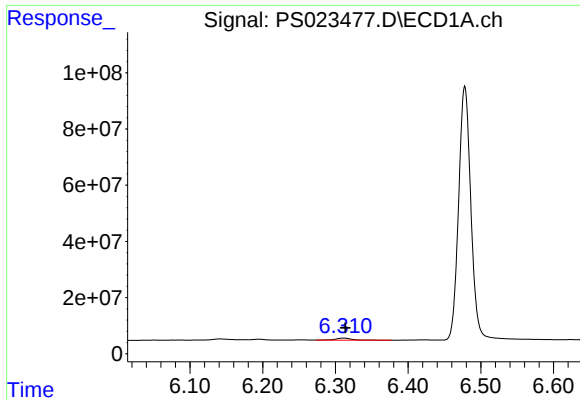

#3 4-Nitrophenol


R.T.: 6.311 min
Delta R.T.: -0.003 min
Response: 12184354
Conc: 9.45 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

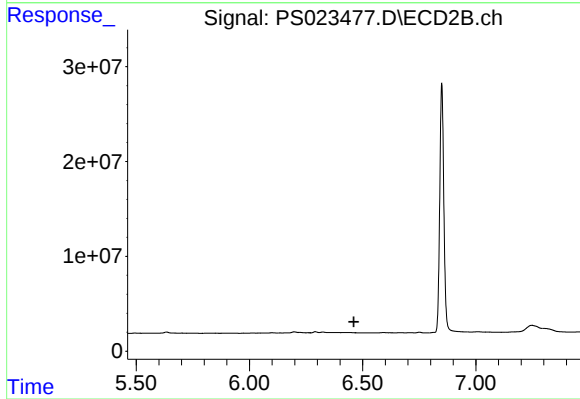


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.461 min
Response: 0
Conc: N.D.

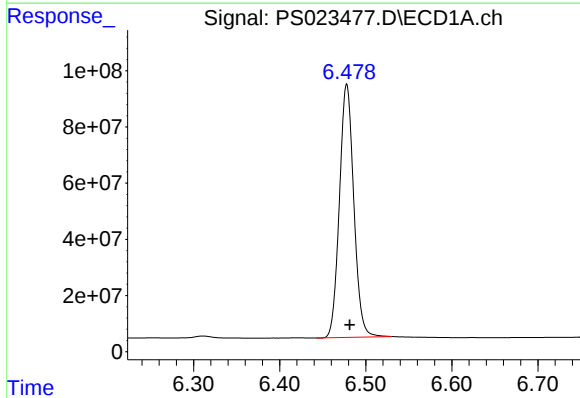


#4 2,4-DCAA

R.T.: 6.478 min
Delta R.T.: -0.004 min
Response: 1046454497
Conc: 591.47 ng/ml

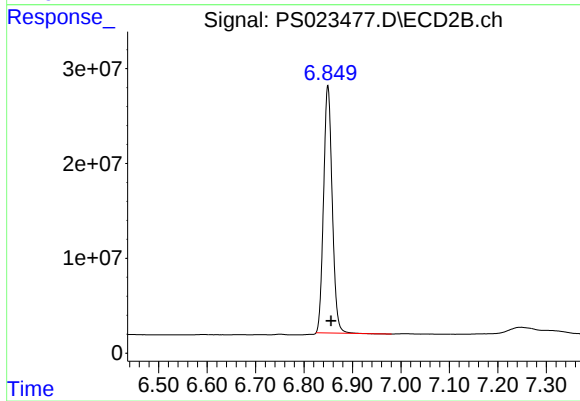

#4 2,4-DCAA


R.T.: 6.849 min
Delta R.T.: -0.007 min
Response: 323345741
Conc: 569.58 ng/ml

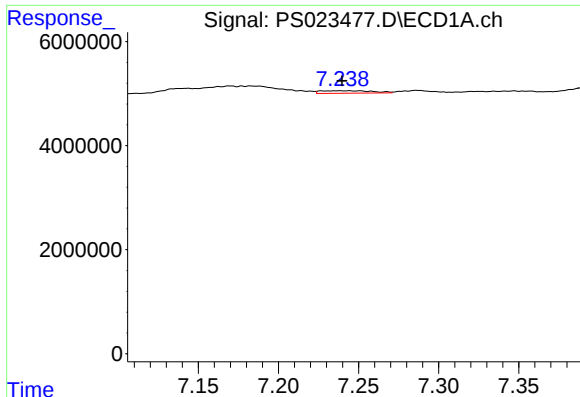

#8 DICHLORPROP


R.T.: 7.238 min
Delta R.T.: -0.001 min
Response: 1068444
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

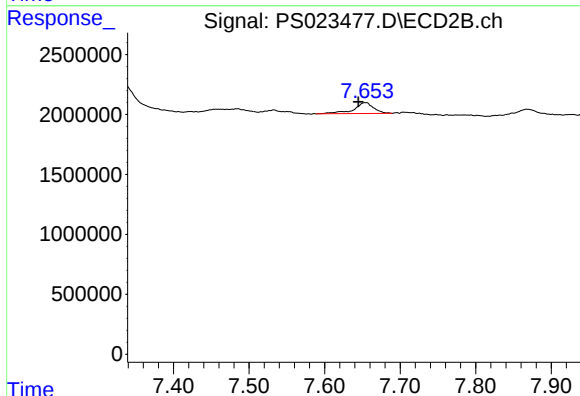


#8 DICHLORPROP

R.T.: 7.654 min
Delta R.T.: 0.009 min
Response: 1646321
Conc: 2.66 ng/ml

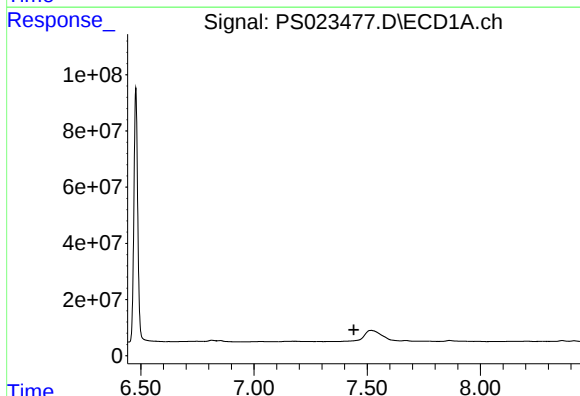


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.442 min
Response: 0
Conc: N.D.

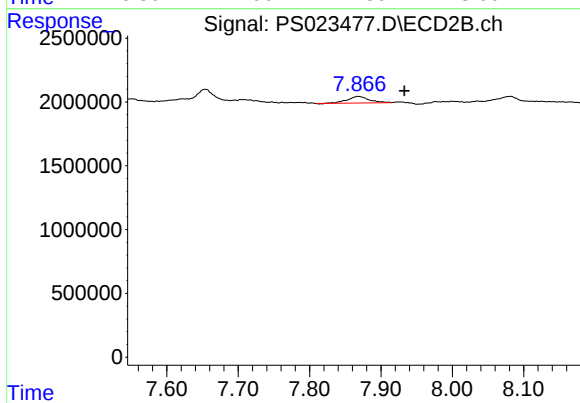

#9 2,4-D


R.T.: 7.868 min
Delta R.T.: -0.065 min
Response: 1093935
Conc: 1.58 ng/ml

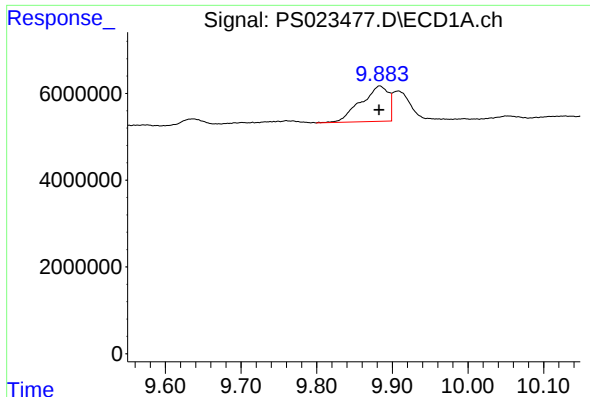

#15 Picloram

R.T.: 9.883 min
Delta R.T.: 0.000 min
Response: 20687569
Conc: 1.19 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

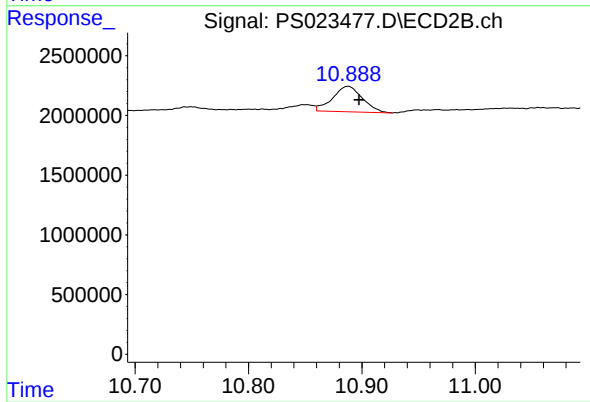

#15 Picloram

R.T.: 10.888 min
Delta R.T.: -0.010 min
Response: 3883355
Conc: N.D.