

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062718\
 Data File : PS000671.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jun 2018 16:59
 Operator : UA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 28 00:52:57 2018
 Quant Method : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061718.M
 Quant Title : 8080.M
 QLast Update : Mon Jun 18 00:27:44 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.799	11.180	191.2E6	160.4E6	507.757	471.260
Target Compounds							
1) T	Dalapon	0.000	2.569	0	20385	N.D.	0.047 #
3) T	4-Nitroph...	11.423	0.000	501481	0	2.133	N.D. #
6) T	MCP	12.479	0.000	1484079	0	1.311	N.D. #
7) T	MCPA	12.773	0.000	185570	0	0.106	N.D. #
8) T	DICHLORPROP	13.342	12.602	838419	143813	2.229	0.447 #
10) T	Pentachlo...	14.070	13.629	755770	478786	0.144	0.101 #
11) T	2,4,5-TP ...	14.928	14.251	1692924	625434	0.780	0.321 #
12) T	2,4,5-T	15.336	14.857	541215	117978	0.251	0.070 #
13) T	2,4-DB	16.167	0.000	120156	0	0.408	N.D. #
14) T	DINOSEB	17.600	15.889	1215866	1106046	0.816	0.848
15) T	Picloram	17.350	17.135	982194	1220541	0.336	0.489 #
16) T	DCPA	17.930	17.135	5345060	1220541	2.086	0.529 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062718\
Data File : PS000671.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jun 2018 16:59
Operator : UA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 28 00:52:57 2018
Quant Method : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061718.M
Quant Title : 8080.M
QLast Update : Mon Jun 18 00:27:44 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

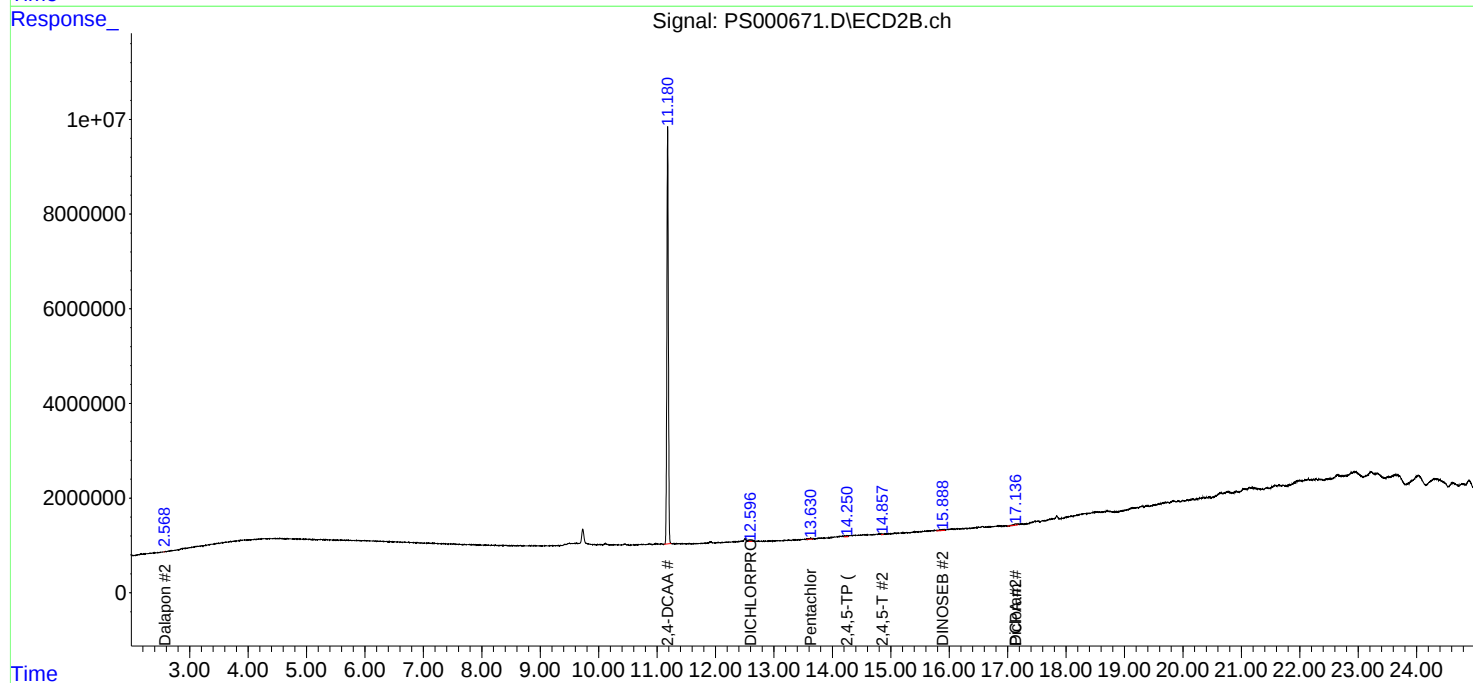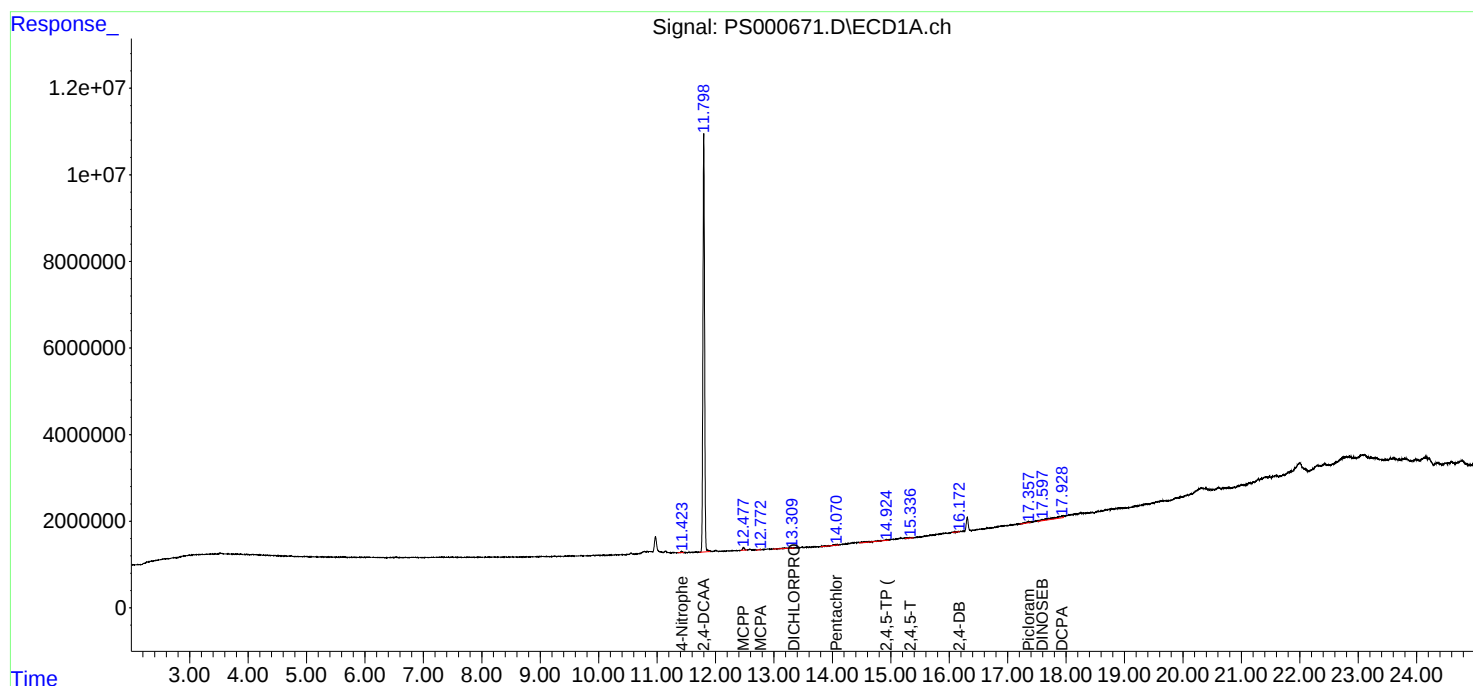


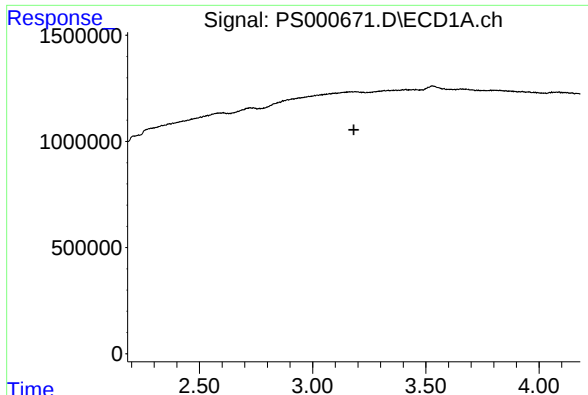

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 3.182 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

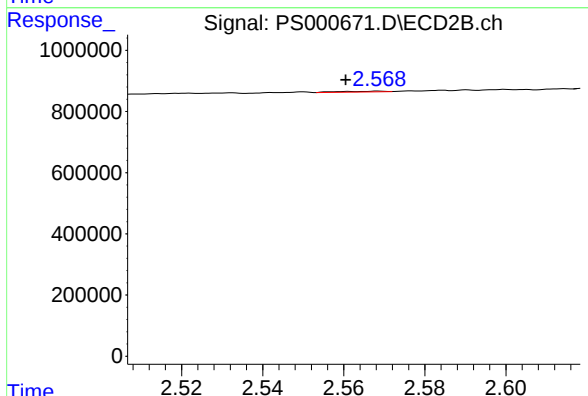


#1 Dalapon

R.T.: 2.569 min
Delta R.T.: 0.008 min
Response: 20385
Conc: 0.05 ng/ml

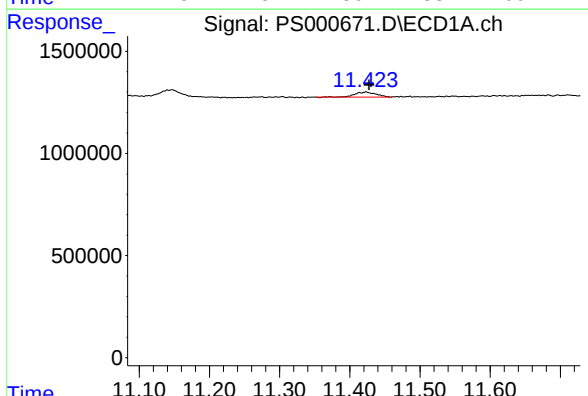


#3 4-Nitrophenol

R.T.: 11.423 min
Delta R.T.: -0.005 min
Response: 501481
Conc: 2.13 ng/ml

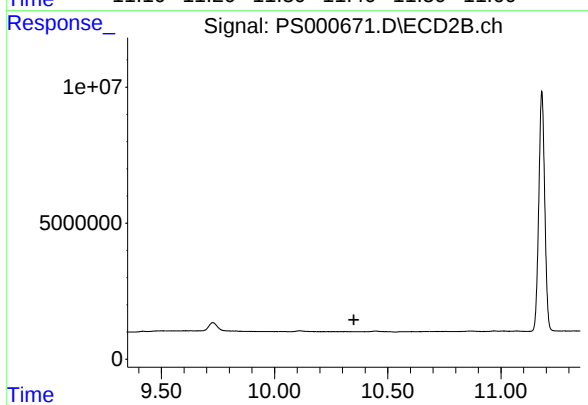

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.350 min
Response: 0
Conc: N.D.

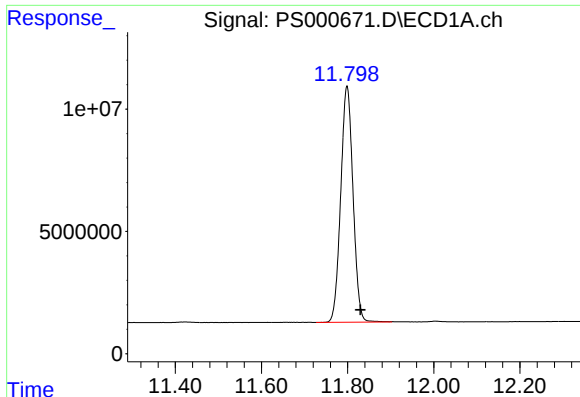

#4 2,4-DCAA


R.T.: 11.799 min
Delta R.T.: -0.031 min
Response: 191249034
Conc: 507.76 ng/ml

Instrument :
ECD_S
ClientSampleId :

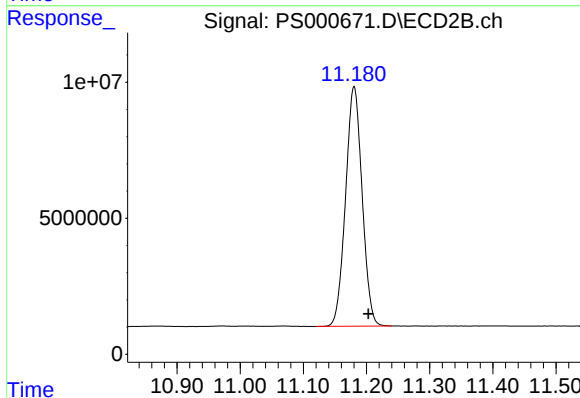


#4 2,4-DCAA

R.T.: 11.180 min
Delta R.T.: -0.023 min
Response: 160374022
Conc: 471.26 ng/ml

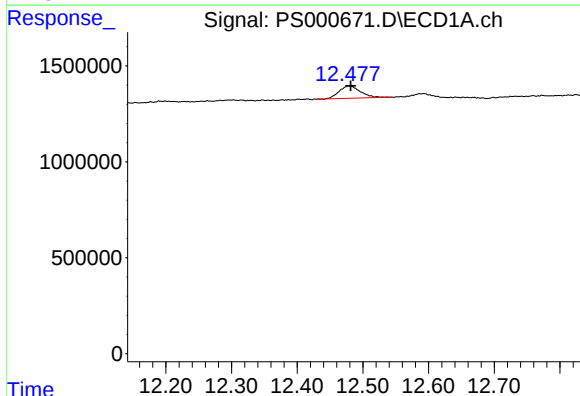


#6 MCP

R.T.: 12.479 min
Delta R.T.: -0.002 min
Response: 1484079
Conc: 1.31 ug/ml

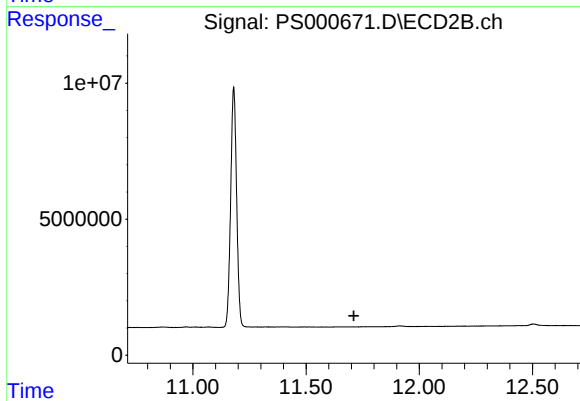

#6 MCP


R.T.: 0.000 min
Exp R.T. : 11.711 min
Response: 0
Conc: N.D.

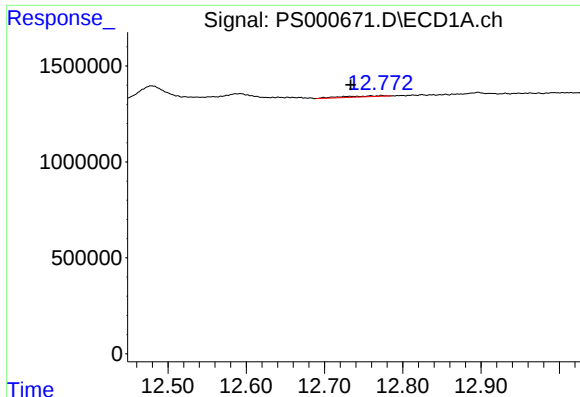

#7 MCPA


R.T.: 12.773 min
Delta R.T.: 0.040 min
Response: 185570
Conc: 0.11 ug/ml

Instrument :
ECD_S
ClientSampleId :

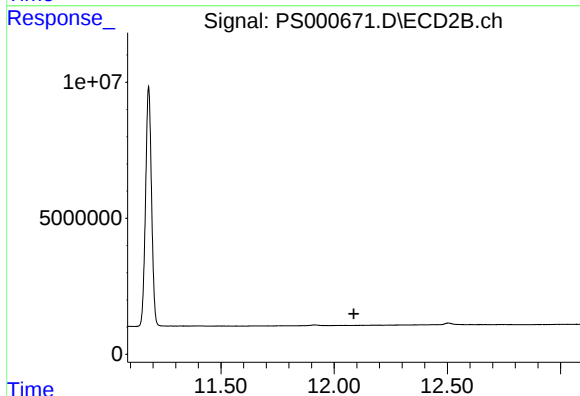


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 12.087 min
Response: 0
Conc: N.D.

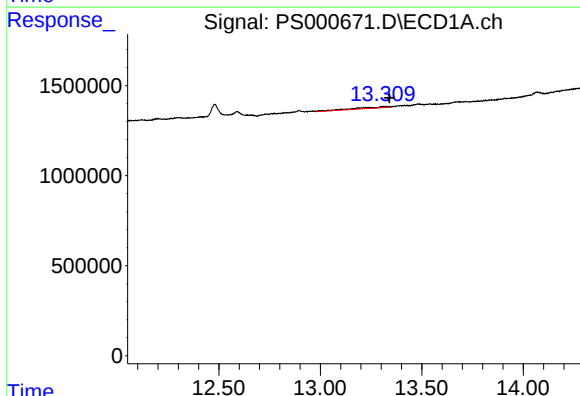


#8 DICHLORPROP

R.T.: 13.342 min
Delta R.T.: 0.001 min
Response: 838419
Conc: 2.23 ng/ml

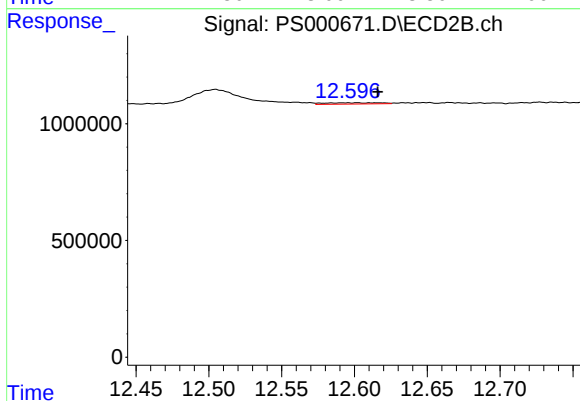

#8 DICHLORPROP


R.T.: 12.602 min
Delta R.T.: -0.014 min
Response: 143813
Conc: 0.45 ng/ml

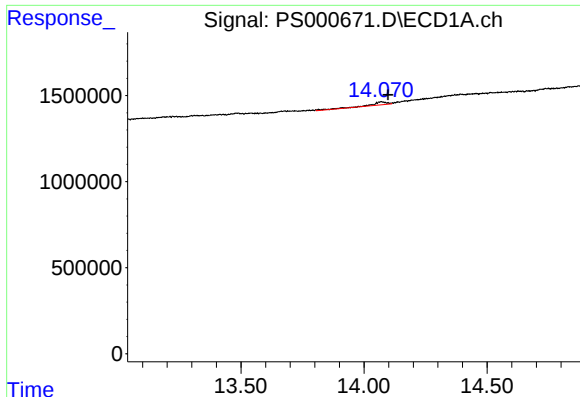

#10 Pentachlorophenol


R.T.: 14.070 min
Delta R.T.: -0.027 min
Response: 755770
Conc: 0.14 ng/ml

Instrument :
ECD_S
ClientSampleId :

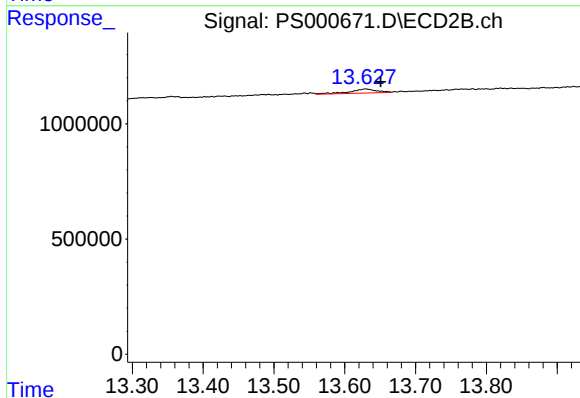


#10 Pentachlorophenol

R.T.: 13.629 min
Delta R.T.: -0.022 min
Response: 478786
Conc: 0.10 ng/ml

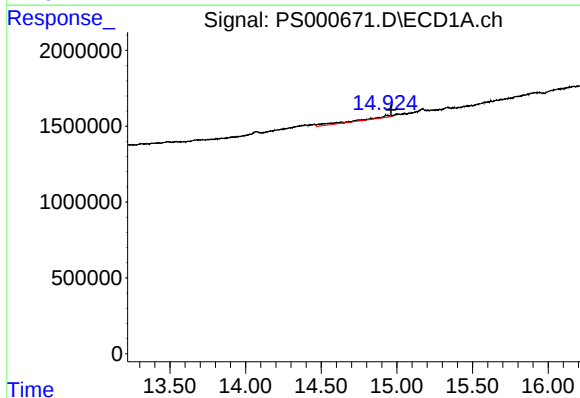


#11 2,4,5-TP (SILVEX)

R.T.: 14.928 min
Delta R.T.: -0.034 min
Response: 1692924
Conc: 0.78 ng/ml

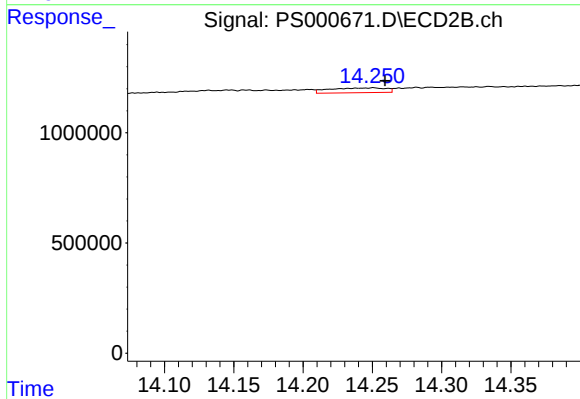

#11 2,4,5-TP (SILVEX)


R.T.: 14.251 min
Delta R.T.: -0.008 min
Response: 625434
Conc: 0.32 ng/ml

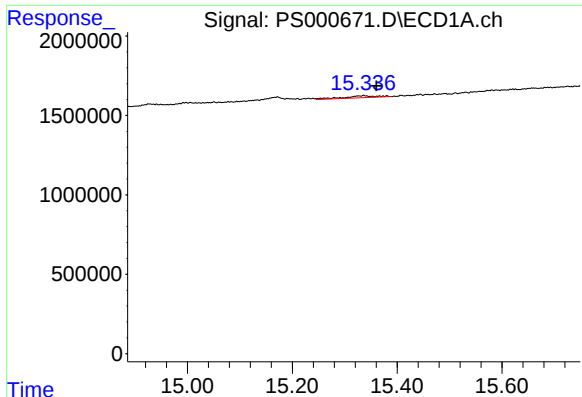

#12 2,4,5-T


R.T.: 15.336 min
Delta R.T.: -0.024 min
Response: 541215
Conc: 0.25 ng/ml

Instrument :
ECD_S
ClientSampleId :

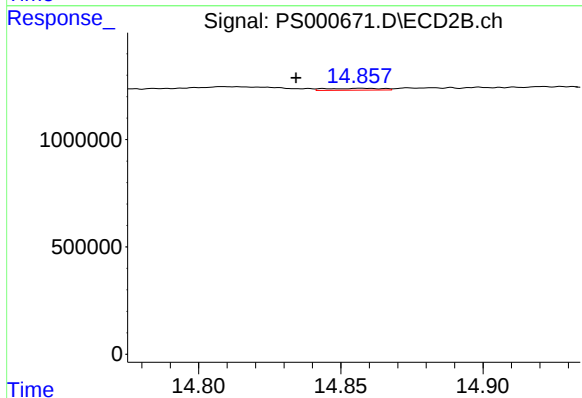


#12 2,4,5-T

R.T.: 14.857 min
Delta R.T.: 0.023 min
Response: 117978
Conc: 0.07 ng/ml

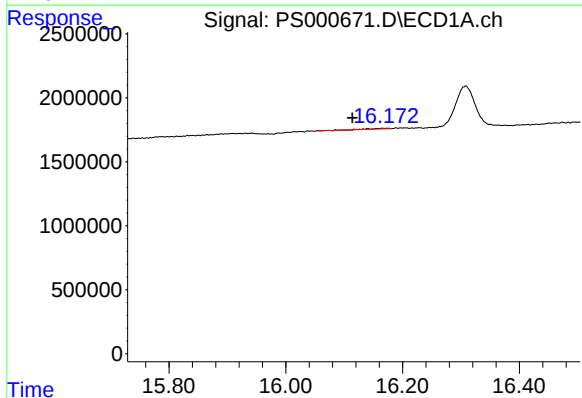


#13 2,4-DB

R.T.: 16.167 min
Delta R.T.: 0.053 min
Response: 120156
Conc: 0.41 ng/ml

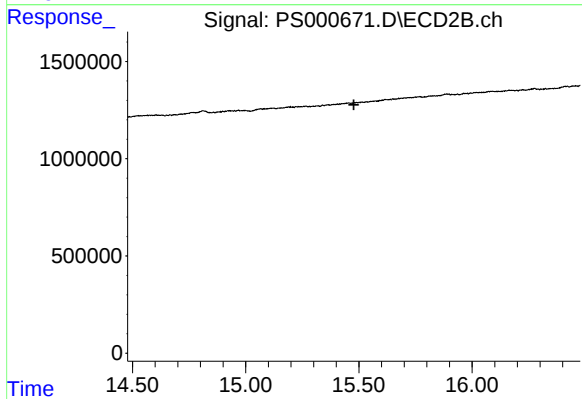

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 15.478 min
Response: 0
Conc: N.D.

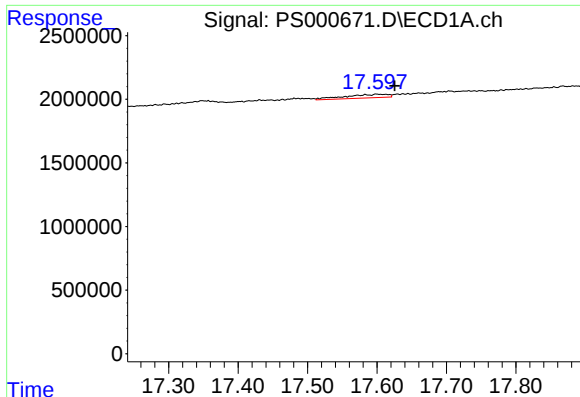

#14 DINOSEB


R.T.: 17.600 min
Delta R.T.: -0.025 min
Response: 1215866
Conc: 0.82 ng/ml

Instrument :
ECD_S
ClientSampleId :

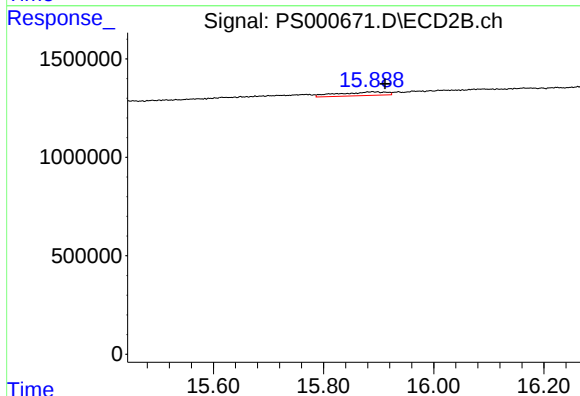


#14 DINOSEB

R.T.: 15.889 min
Delta R.T.: -0.023 min
Response: 1106046
Conc: 0.85 ng/ml

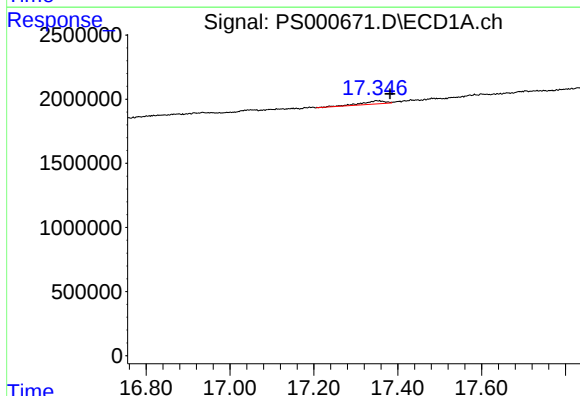


#15 Picloram

R.T.: 17.350 min
Delta R.T.: -0.032 min
Response: 982194
Conc: 0.34 ng/ml

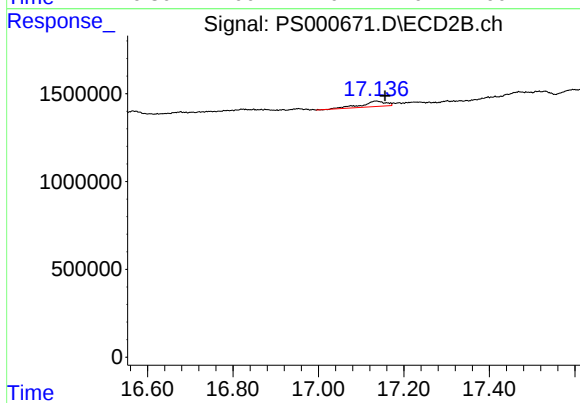

#15 Picloram


R.T.: 17.135 min
Delta R.T.: -0.021 min
Response: 1220541
Conc: 0.49 ng/ml

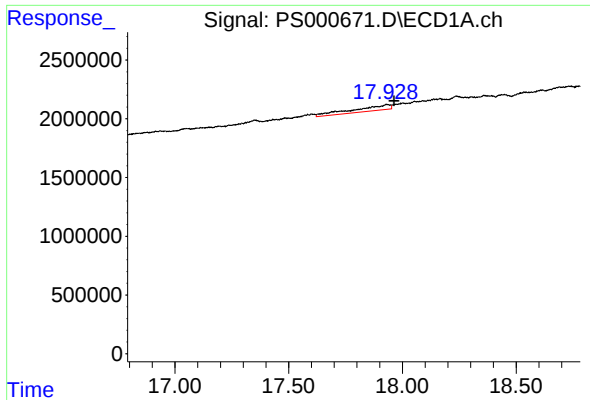

#16 DCPA

R.T.: 17.930 min
Delta R.T.: -0.034 min
Response: 5345060
Conc: 2.09 ng/ml

Instrument :
ECD_S
ClientSampleId :

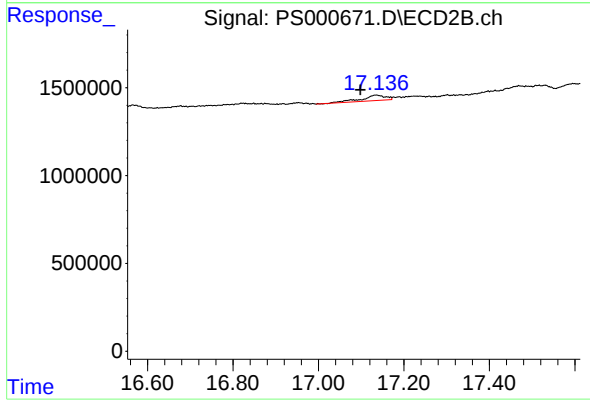

#16 DCPA

R.T.: 17.135 min
Delta R.T.: 0.037 min
Response: 1220541
Conc: 0.53 ng/ml