

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062718\
 Data File : PS000694.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jun 2018 04:50
 Operator : UA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 28 06:56:20 2018
 Quant Method : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061718.M
 Quant Title : 8080.M
 QLast Update : Mon Jun 18 00:27:44 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.794	11.175	197.7E6	165.5E6	524.787	486.189
Target Compounds							
2) T	3,5-DICHL...	0.000	9.414	0	247353	N.D.	0.538 #
3) T	4-Nitroph...	11.418	0.000	595760	0	2.534	N.D. #
6) T	MCP	12.478	0.000	1601847	0	1.415	N.D. #
10) T	Pentachlo...	14.064	0.000	283811	0	0.054	N.D. #
15) T	Picloram	17.349	17.132	808100	54273	0.277	0.022 #
16) T	DCPA	0.000	17.132	0	54273	N.D.	0.024 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062718\
Data File : PS000694.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jun 2018 04:50
Operator : UA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 28 06:56:20 2018
Quant Method : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061718.M
Quant Title : 8080.M
QLast Update : Mon Jun 18 00:27:44 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

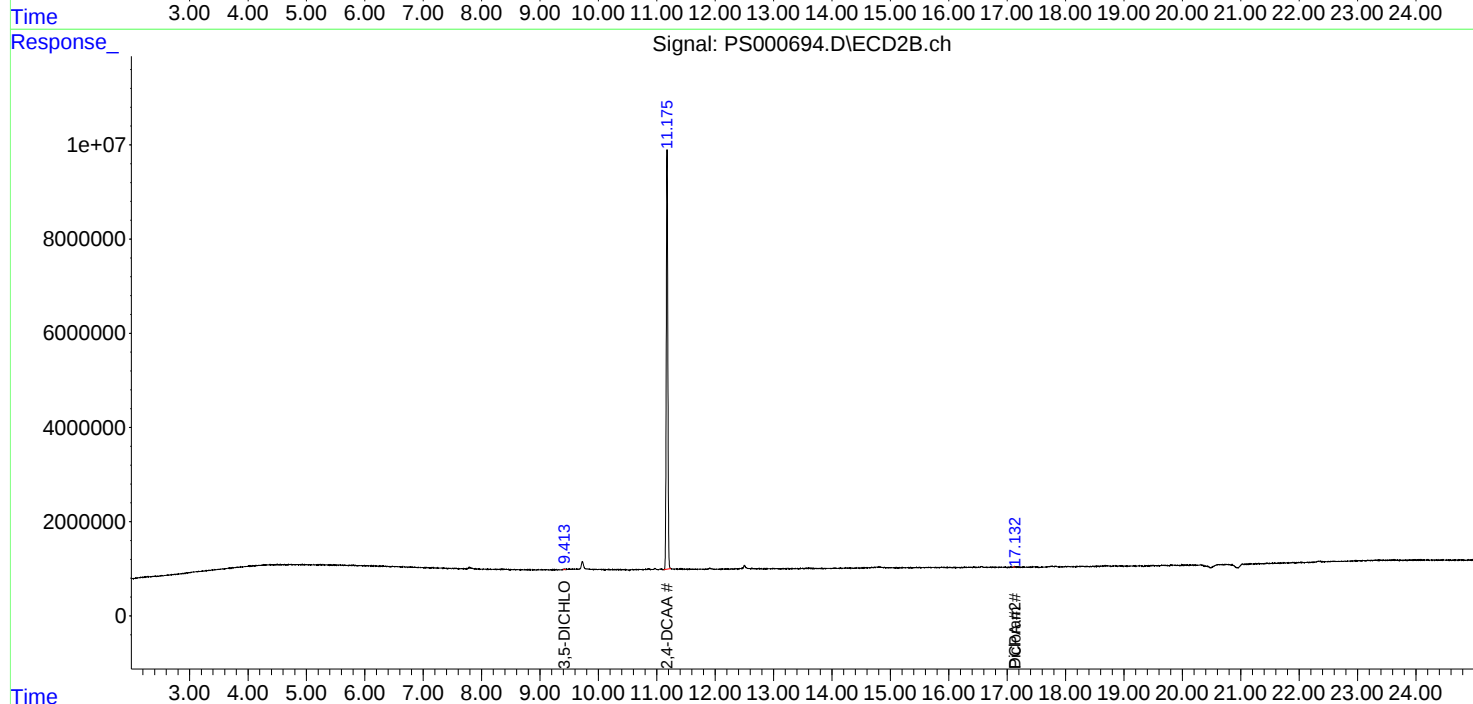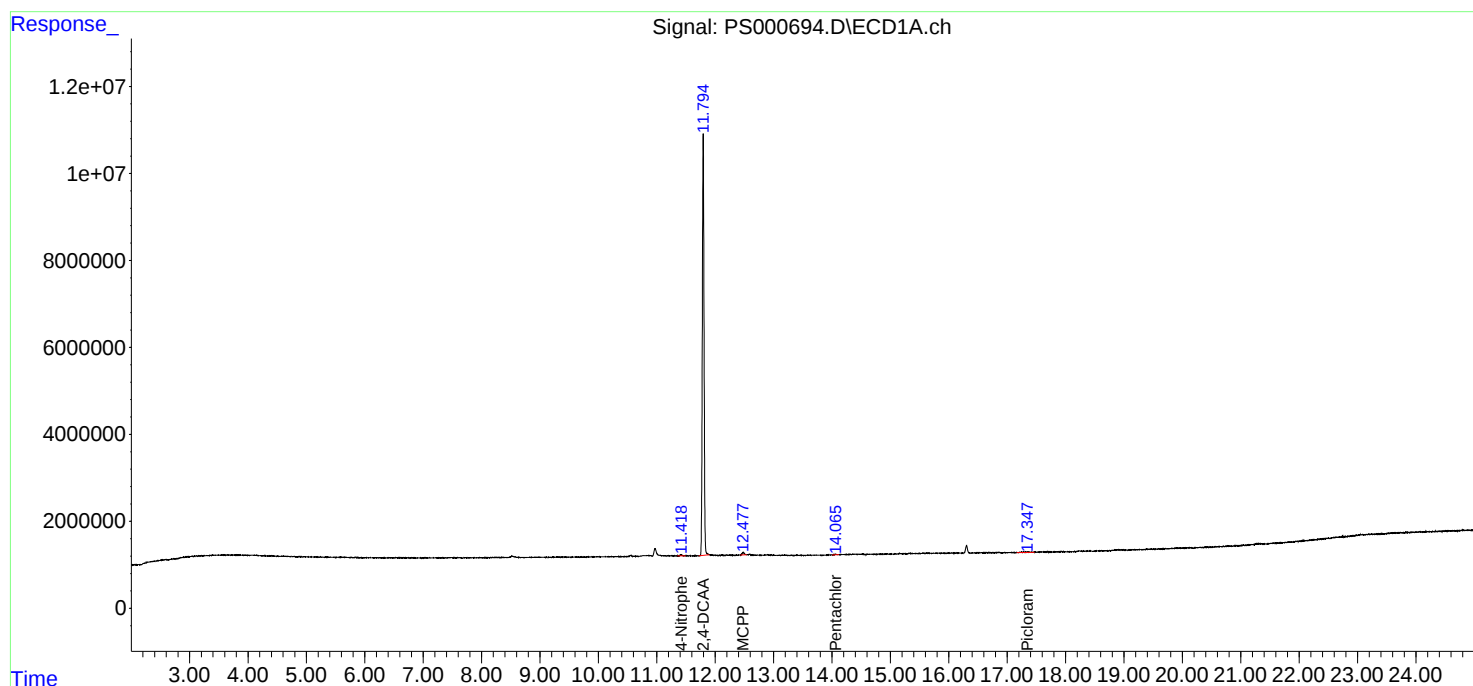


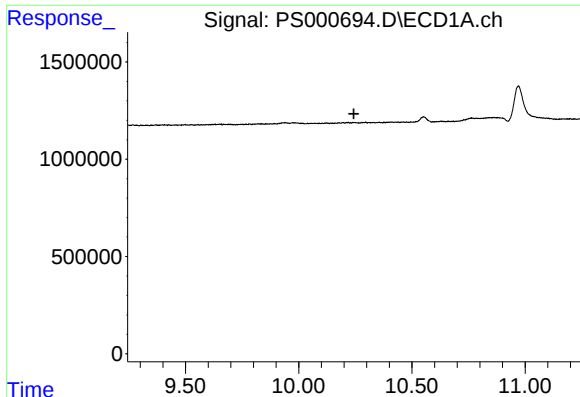

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 10.244 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

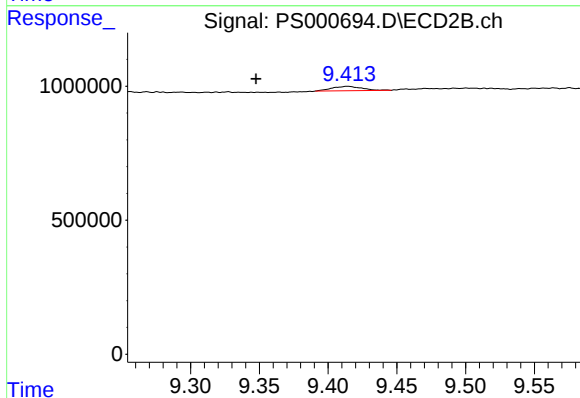


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 9.414 min
Delta R.T.: 0.066 min
Response: 247353
Conc: 0.54 ng/ml

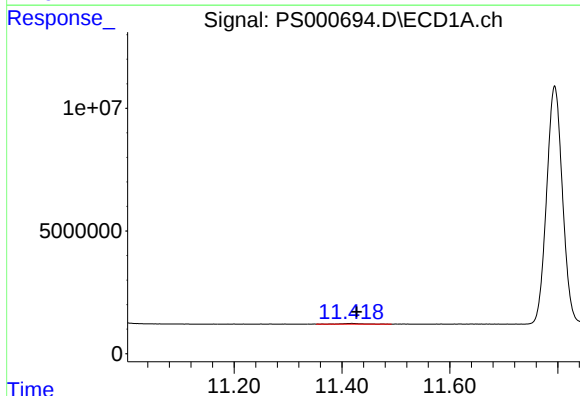


#3 4-Nitrophenol

R.T.: 11.418 min
Delta R.T.: -0.010 min
Response: 595760
Conc: 2.53 ng/ml

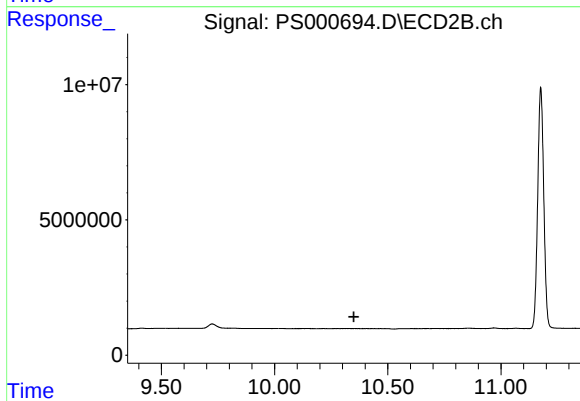

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.350 min
Response: 0
Conc: N.D.

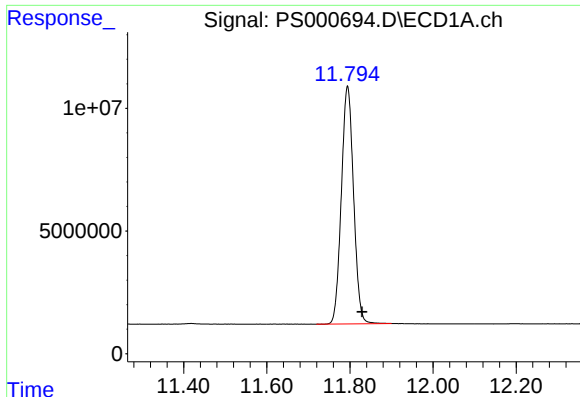

#4 2,4-DCAA


R.T.: 11.794 min
Delta R.T.: -0.035 min
Response: 197663474
Conc: 524.79 ng/ml

Instrument :
ECD_S
ClientSampleId :

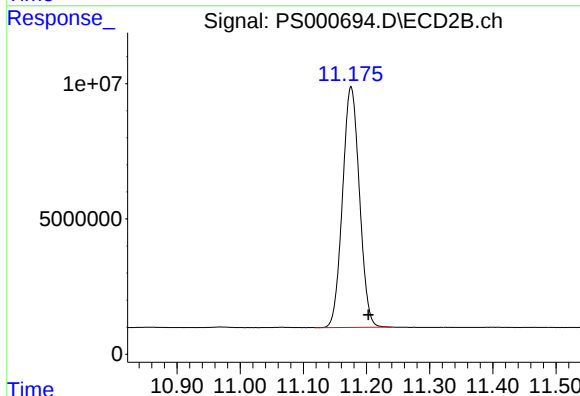


#4 2,4-DCAA

R.T.: 11.175 min
Delta R.T.: -0.027 min
Response: 165454483
Conc: 486.19 ng/ml

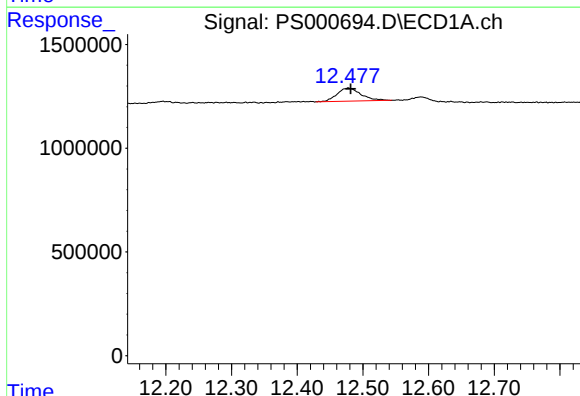


#6 MCP

R.T.: 12.478 min
Delta R.T.: -0.004 min
Response: 1601847
Conc: 1.41 ug/ml

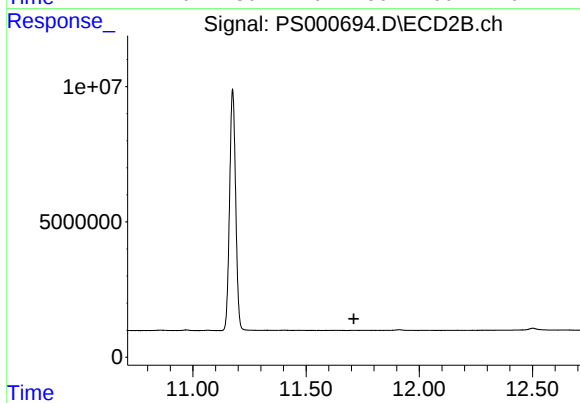

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.711 min
Response: 0
Conc: N.D.

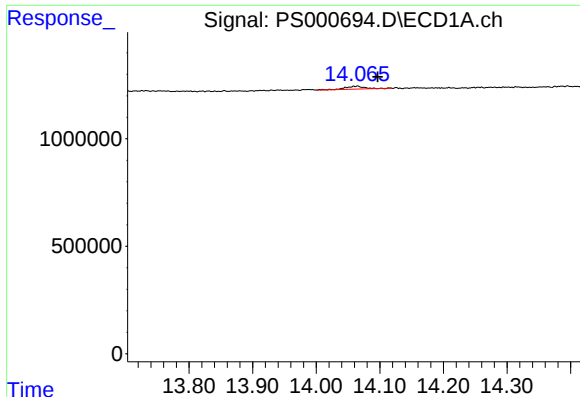

#10 Pentachlorophenol


R.T.: 14.064 min
Delta R.T.: -0.033 min
Response: 283811
Conc: 0.05 ng/ml

Instrument :
ECD_S
ClientSampleId :

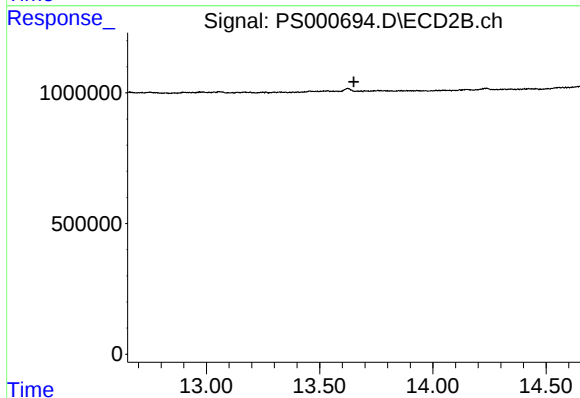


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 13.651 min
Response: 0
Conc: N.D.

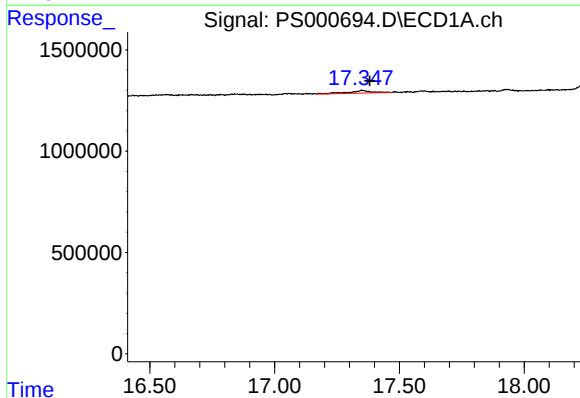


#15 Picloram

R.T.: 17.349 min
Delta R.T.: -0.033 min
Response: 808100
Conc: 0.28 ng/ml

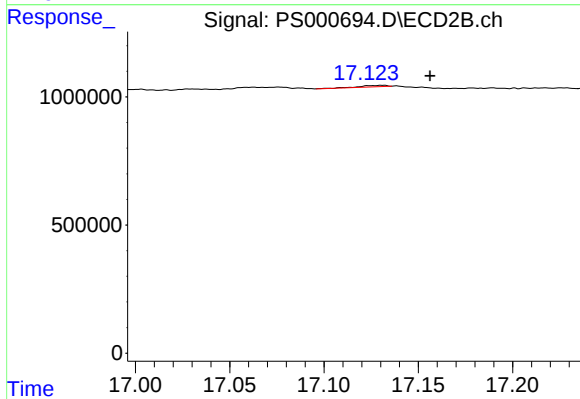

#15 Picloram


R.T.: 17.132 min
Delta R.T.: -0.025 min
Response: 54273
Conc: 0.02 ng/ml

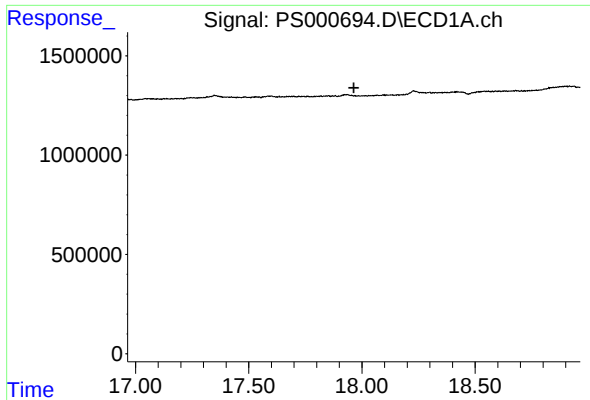

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.964 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

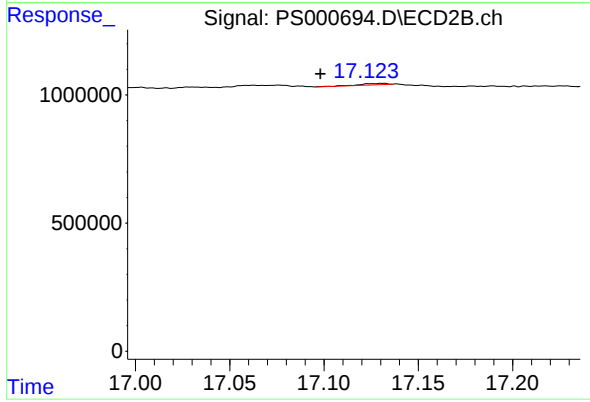

#16 DCPA

R.T.: 17.132 min
Delta R.T.: 0.034 min
Response: 54273
Conc: 0.02 ng/ml