

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062718\
 Data File : PS000668.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jun 2018 15:26
 Operator : UA
 Sample : J3682-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 FK-BPM-01-E5-F5-E5A-F5A

Manual Integrations
 APPROVED

UGO
 6/28/2018 11:48:25 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 27 16:07:17 2018
 Quant Method : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061718.M
 Quant Title : 8080.M
 QLast Update : Mon Jun 18 00:27:44 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	11.831	11.211	109.8E6	87998130	291.446	258.583m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062718\
Data File : PS000668.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jun 2018 15:26
Operator : UA
Sample : J3682-01
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
FK-BPM-01-E5-F5-E5A-F5A


Manual Integrations
APPROVED

UGO
6/28/2018 11:48:25 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 27 16:07:17 2018
Quant Method : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061718.M
Quant Title : 8080.M
QLast Update : Mon Jun 18 00:27:44 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

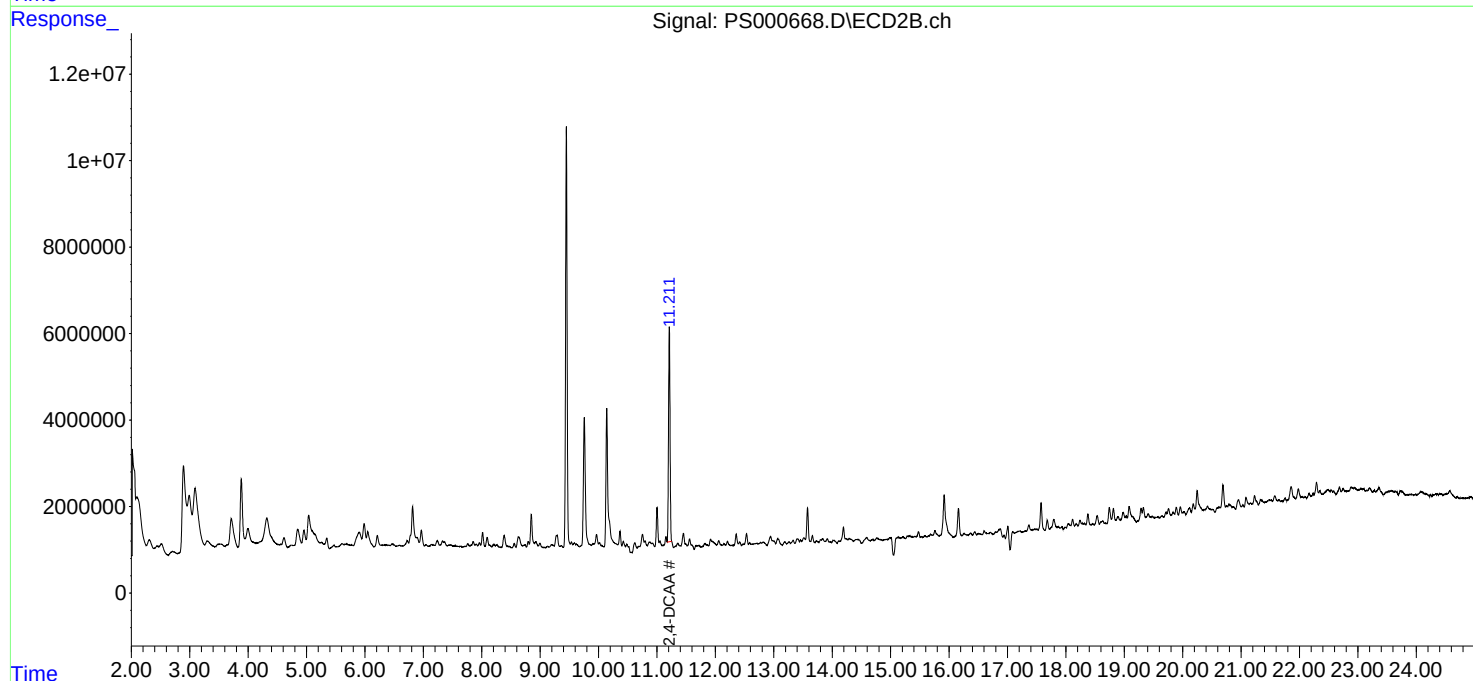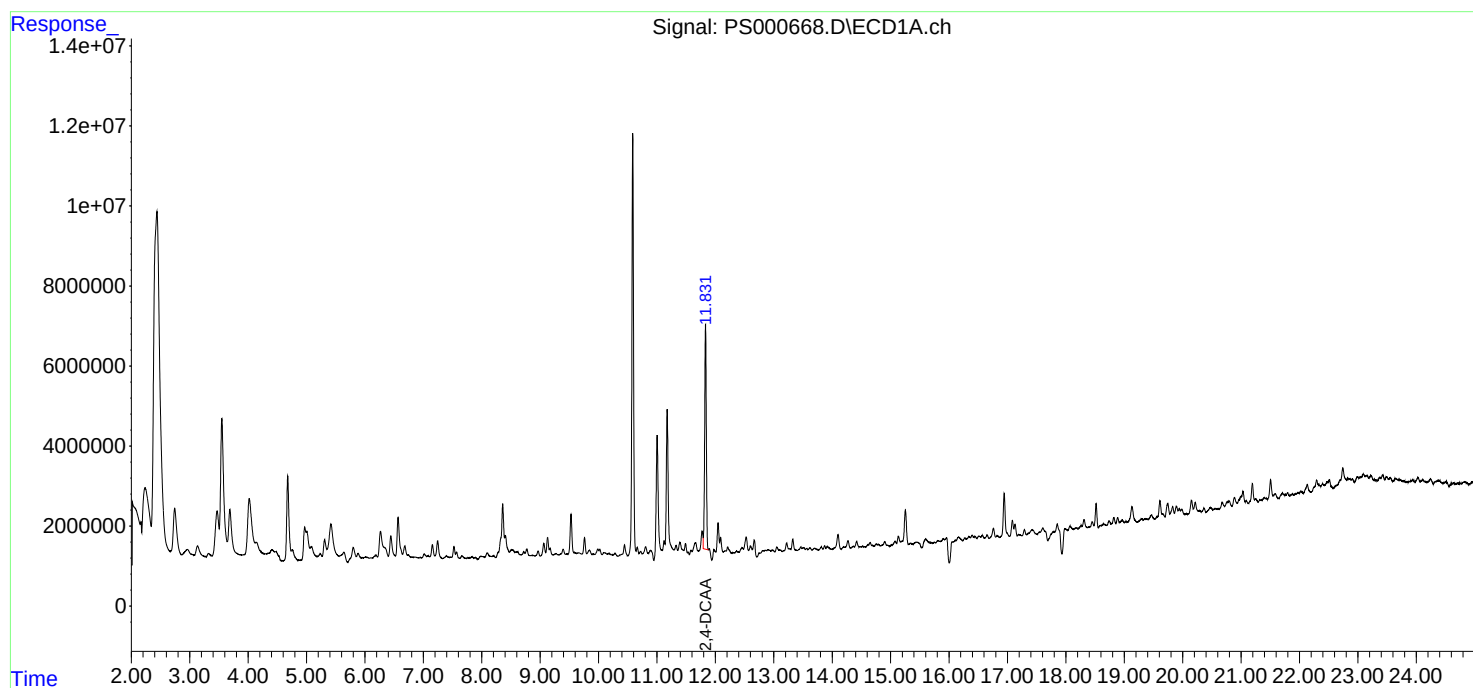

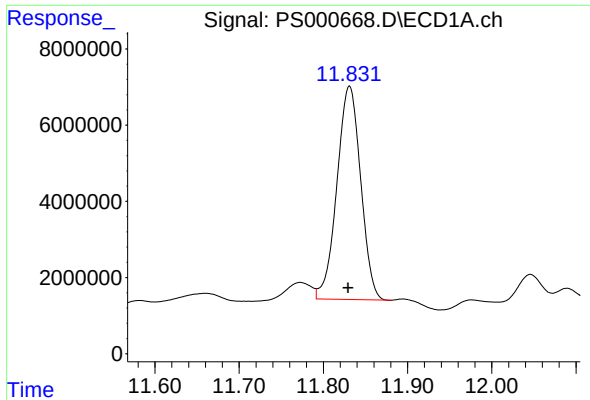


#4 2,4-DCAA

R.T.: 11.831 min
Delta R.T.: 0.002 min
Response: 109774391
Conc: 291.45 ng/ml

Instrument :
ECD_S
ClientSampleId :
FK-BPM-01-E5-F5-E5A-F5A

Manual Integrations
APPROVED

UGO
6/28/2018 11:48:25 AM

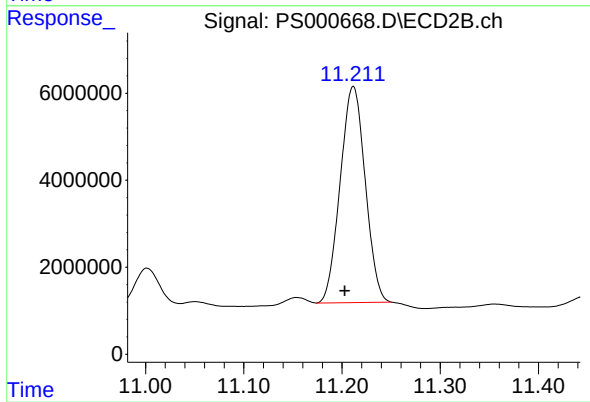

#4 2,4-DCAA

R.T.: 11.211 min
Delta R.T.: 0.008 min
Response: 87998130
Conc: 258.58 ng/ml m