

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062722\
 Data File : PS019817.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jun 2022 01:41
 Operator : AJ\MA
 Sample : HSTDCCC750
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HSTDCCC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 28 01:59:43 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062722.M
 Quant Title : 8080.M
 QLast Update : Mon Jun 27 17:26:48 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.193	6.778	2141.5E6	640.3E6	825.662	788.382
Target Compounds							
1) T	Dalapon	3.010	2.521	3679.9E6	738.7E6	759.171	695.993
2) T	3,5-DICHL...	6.408	5.959	2567.0E6	930.4E6	749.391	728.069
3) T	4-Nitroph...	7.026	6.397	857.8E6	320.3E6	805.948	740.488
5) T	DICAMBA	7.383	6.942	8010.5E6	2695.6E6	780.670	738.919
6) T	MCPD	7.553	7.040	634.9E6	211.7E6	79.140	73.758
7) T	MCPA	7.701	7.252	912.7E6	295.7E6	77.893	73.048
8) T	DICHLORPROP	8.074	7.562	2091.3E6	687.3E6	772.410	730.571
9) T	2,4-D	8.304	7.854	2394.9E6	831.4E6	806.317	737.935
10) T	Pentachlo...	8.609	8.279	28382.2E6	9128.0E6	785.928	739.274
11) T	2,4,5-TP ...	9.160	8.639	12577.9E6	3963.6E6	786.334	747.894
12) T	2,4,5-T	9.446	9.017	13703.1E6	3726.9E6	744.734	762.871
13) T	2,4-DB	9.998	9.522	3103.5E6	490.4E6	775.565	755.136
14) T	DINOSEB	11.150	9.847	12000.9E6	2718.5E6	738.169	762.719
15) T	Picloram	10.976	10.829	24045.7E6	5002.9E6	771.121	769.247
16) T	DCPA	11.419	10.775	19200.3E6	4878.8E6	744.279	752.810



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062722\
Data File : PS019817.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jun 2022 01:41
Operator : AJ\MA
Sample : HSTDCCC750
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 28 01:59:43 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062722.M
Quant Title : 8080.M
QLast Update : Mon Jun 27 17:26:48 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

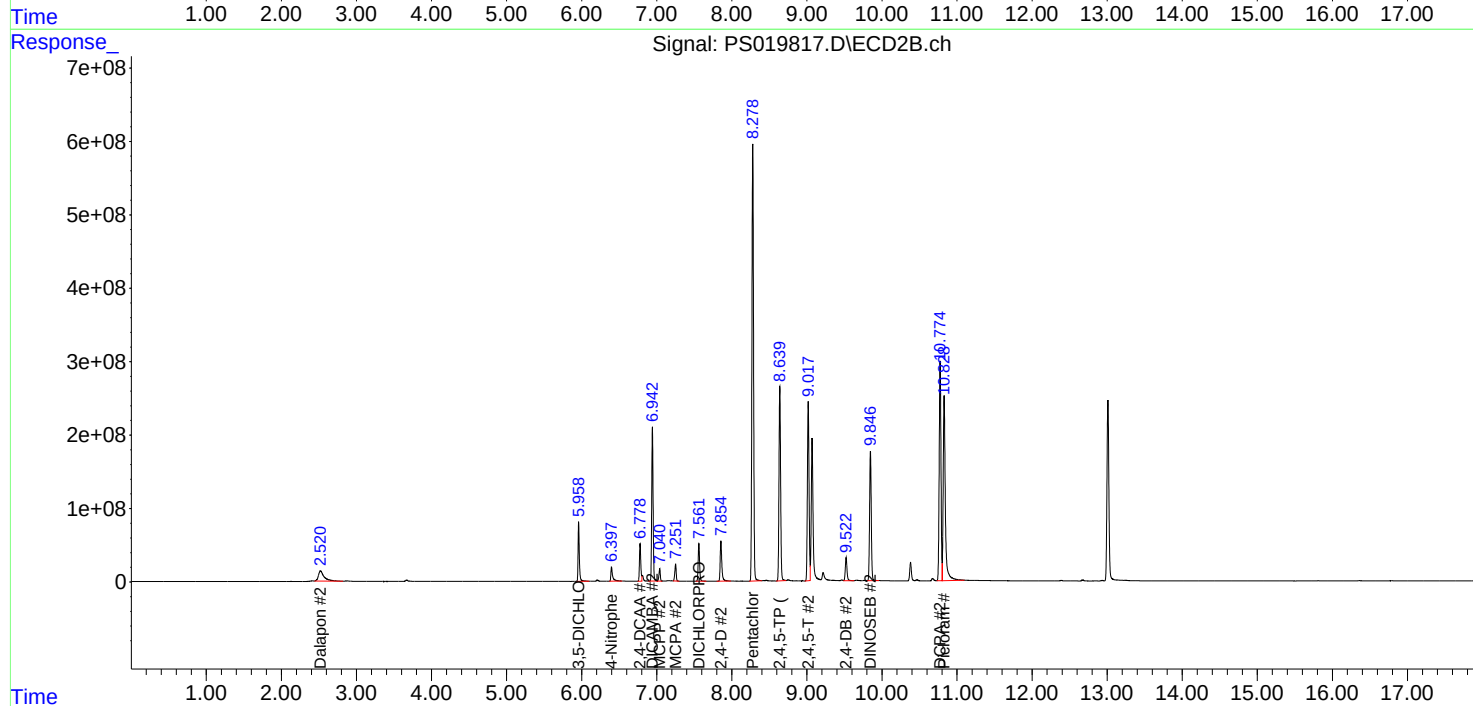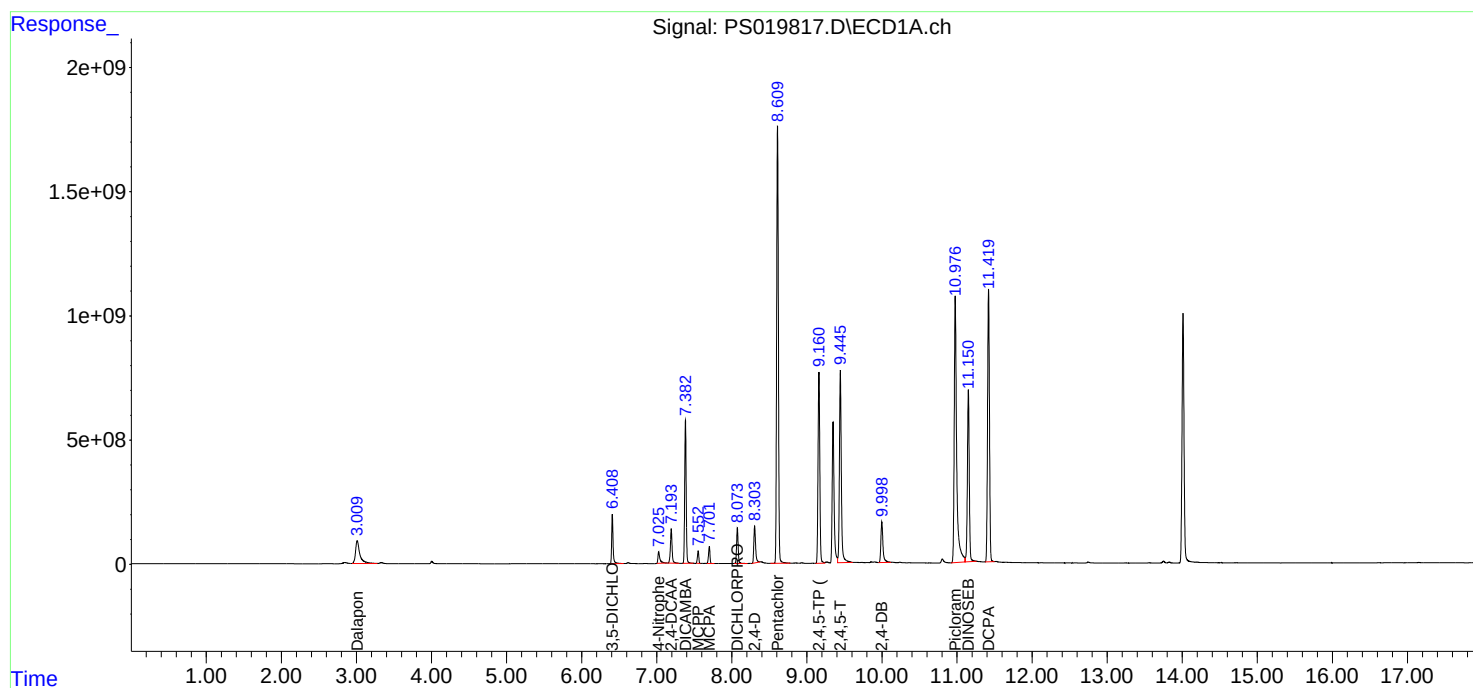


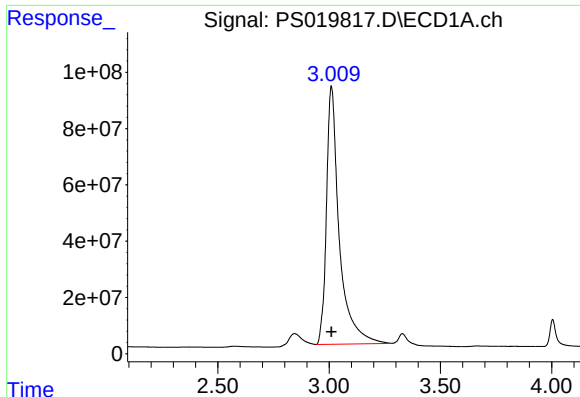

#1 Dalapon


R.T.: 3.010 min
Delta R.T.: 0.000 min
Response: 3679861919
Conc: 759.17 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

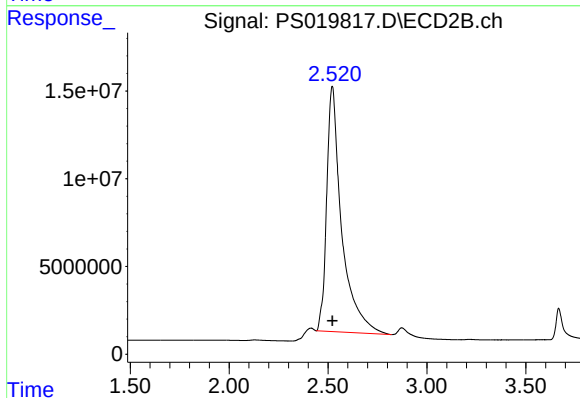


#1 Dalapon

R.T.: 2.521 min
Delta R.T.: 0.000 min
Response: 738695312
Conc: 695.99 ng/ml

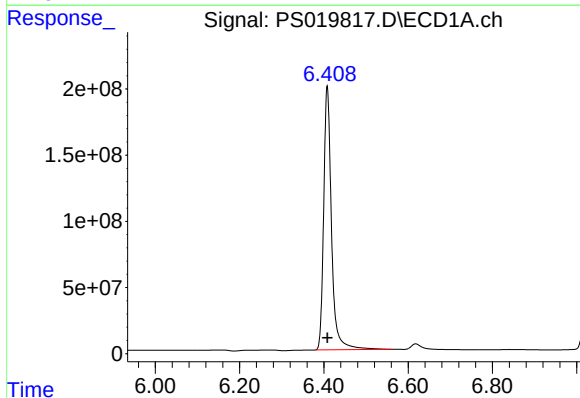


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.408 min
Delta R.T.: 0.000 min
Response: 2566953433
Conc: 749.39 ng/ml

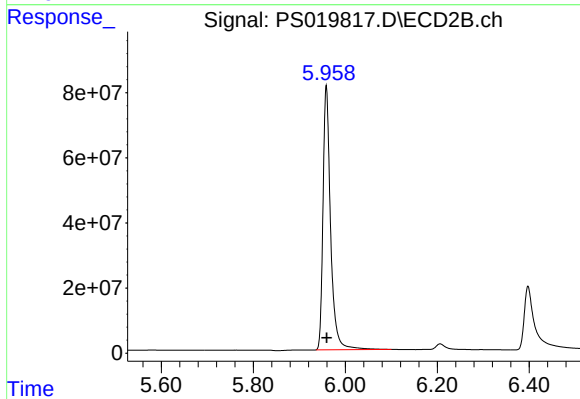

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.959 min
Delta R.T.: 0.000 min
Response: 930373656
Conc: 728.07 ng/ml

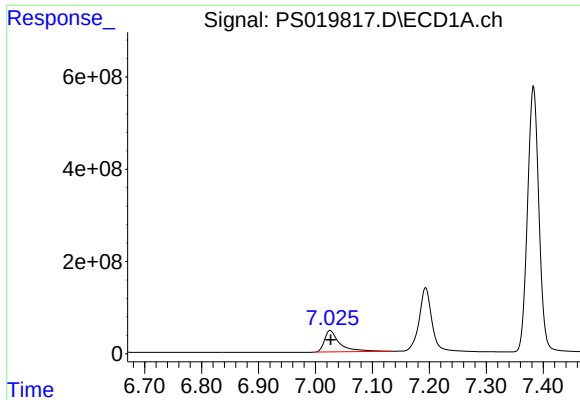

#3 4-Nitrophenol


R.T.: 7.026 min
Delta R.T.: 0.000 min
Response: 857829539
Conc: 805.95 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

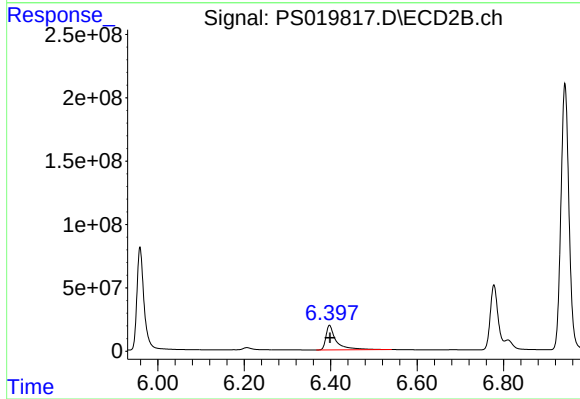


#3 4-Nitrophenol

R.T.: 6.397 min
Delta R.T.: -0.001 min
Response: 320271656
Conc: 740.49 ng/ml

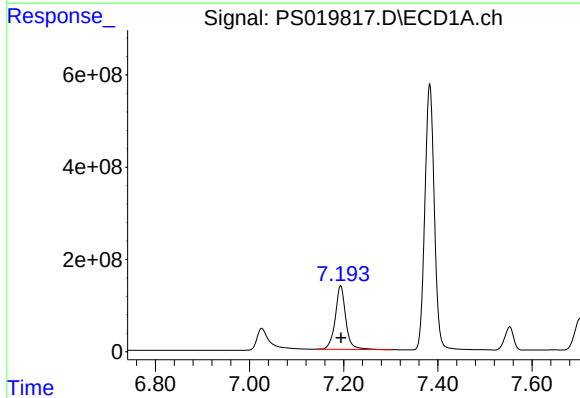


#4 2,4-DCAA

R.T.: 7.193 min
Delta R.T.: 0.000 min
Response: 2141479706
Conc: 825.66 ng/ml

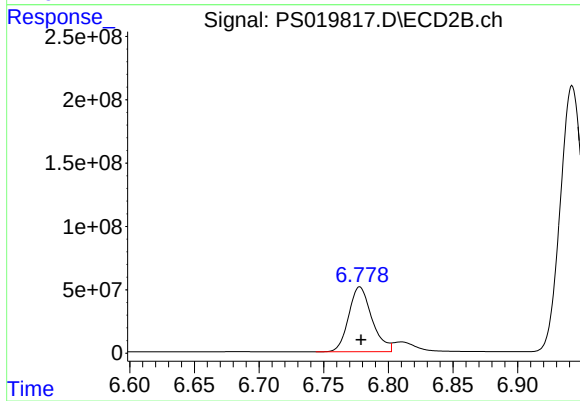

#4 2,4-DCAA


R.T.: 6.778 min
Delta R.T.: 0.000 min
Response: 640281853
Conc: 788.38 ng/ml

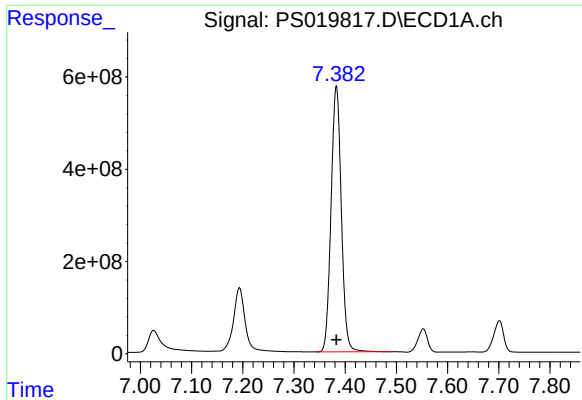

#5 DICAMBA


R.T.: 7.383 min
Delta R.T.: 0.000 min
Response: 8010468489
Conc: 780.67 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

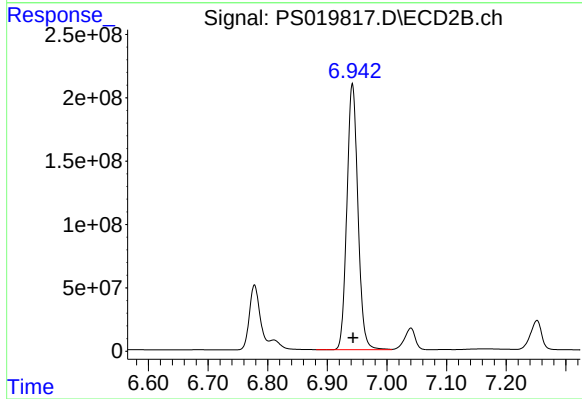


#5 DICAMBA

R.T.: 6.942 min
Delta R.T.: 0.000 min
Response: 2695554766
Conc: 738.92 ng/ml

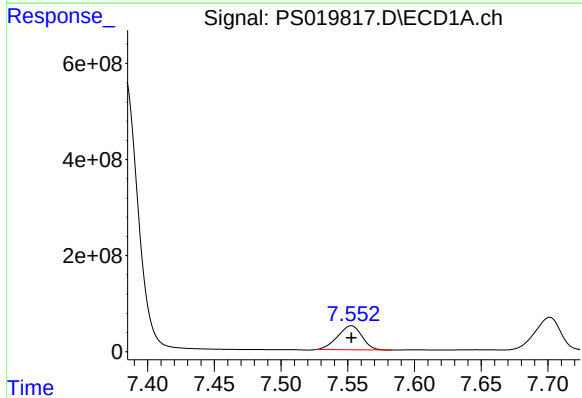


#6 MCP

R.T.: 7.553 min
Delta R.T.: 0.000 min
Response: 634935686
Conc: 79.14 ug/ml

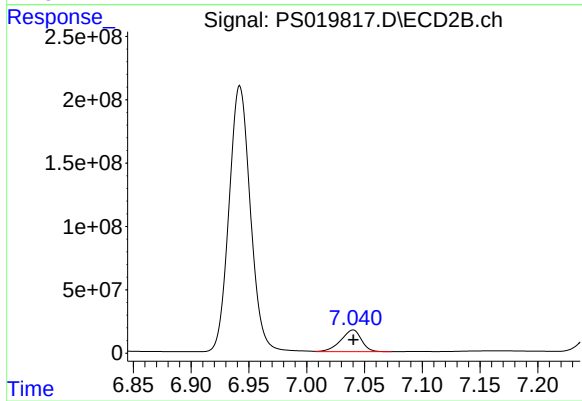

#6 MCP


R.T.: 7.040 min
Delta R.T.: 0.000 min
Response: 211717724
Conc: 73.76 ug/ml

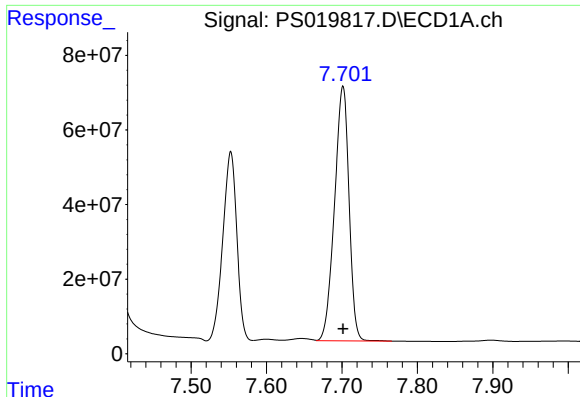

#7 MCPA


R.T.: 7.701 min
Delta R.T.: 0.000 min
Response: 912741549
Conc: 77.89 ug/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

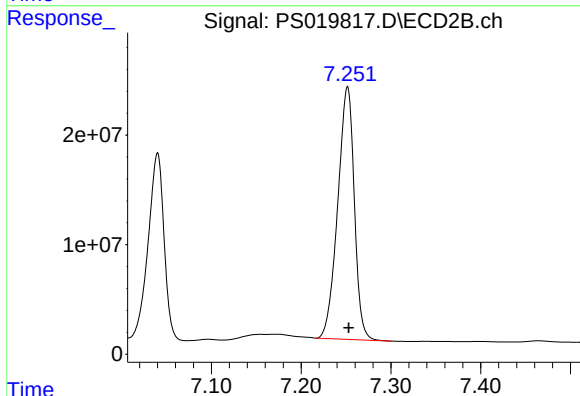


#7 MCPA

R.T.: 7.252 min
Delta R.T.: -0.001 min
Response: 295669698
Conc: 73.05 ug/ml

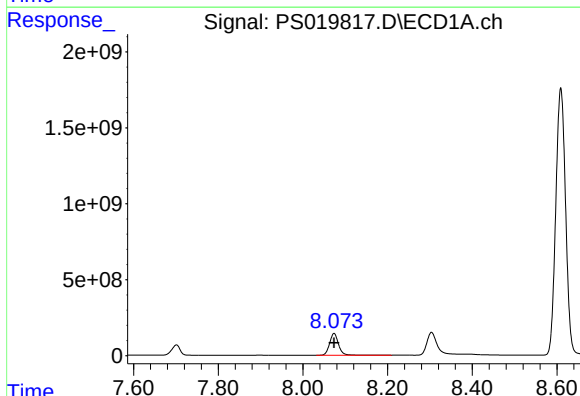


#8 DICHLORPROP

R.T.: 8.074 min
Delta R.T.: 0.000 min
Response: 2091290680
Conc: 772.41 ng/ml

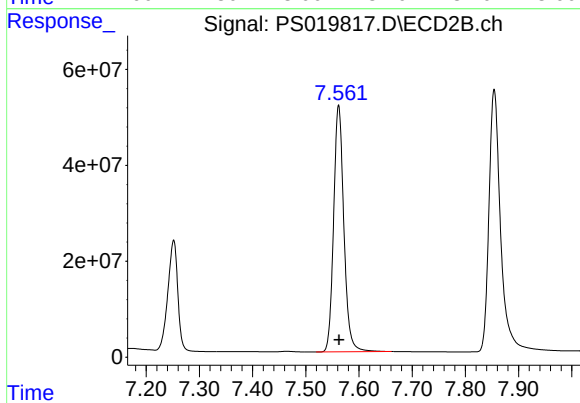

#8 DICHLORPROP


R.T.: 7.562 min
Delta R.T.: -0.001 min
Response: 687263587
Conc: 730.57 ng/ml

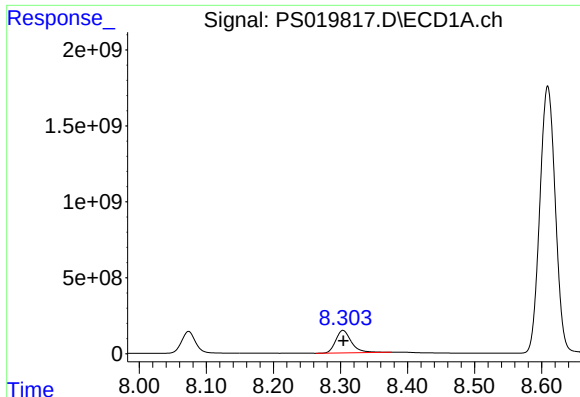

#9 2,4-D


R.T.: 8.304 min
Delta R.T.: 0.000 min
Response: 2394871143
Conc: 806.32 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

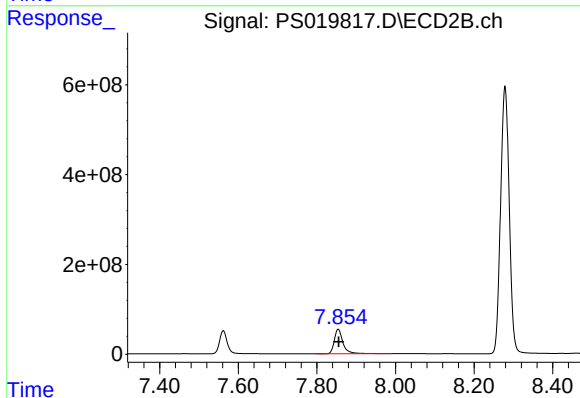


#9 2,4-D

R.T.: 7.854 min
Delta R.T.: -0.001 min
Response: 831434058
Conc: 737.94 ng/ml

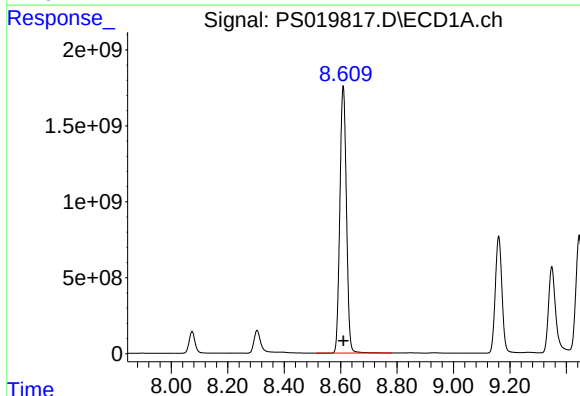


#10 Pentachlorophenol

R.T.: 8.609 min
Delta R.T.: -0.001 min
Response: 28382233904
Conc: 785.93 ng/ml

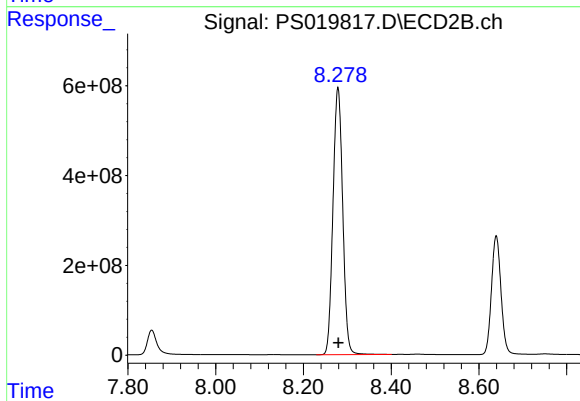

#10 Pentachlorophenol


R.T.: 8.279 min
Delta R.T.: 0.000 min
Response: 9127954961
Conc: 739.27 ng/ml

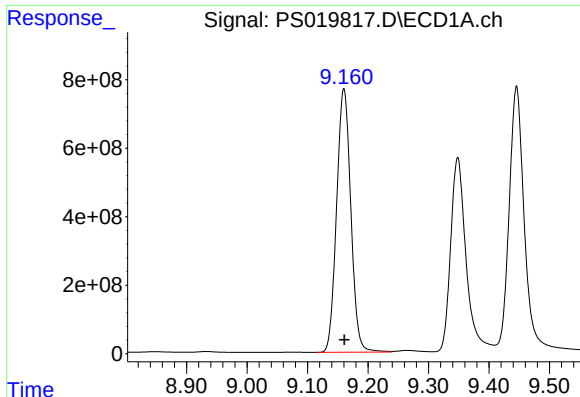

#11 2,4,5-TP (SILVEX)


R.T.: 9.160 min
Delta R.T.: 0.000 min
Response: 12577942134
Conc: 786.33 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

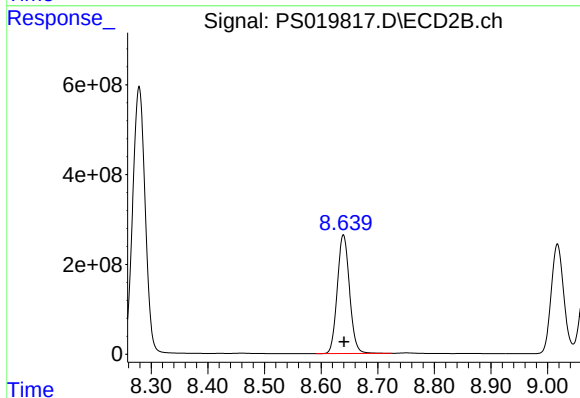


#11 2,4,5-TP (SILVEX)

R.T.: 8.639 min
Delta R.T.: -0.001 min
Response: 3963555170
Conc: 747.89 ng/ml

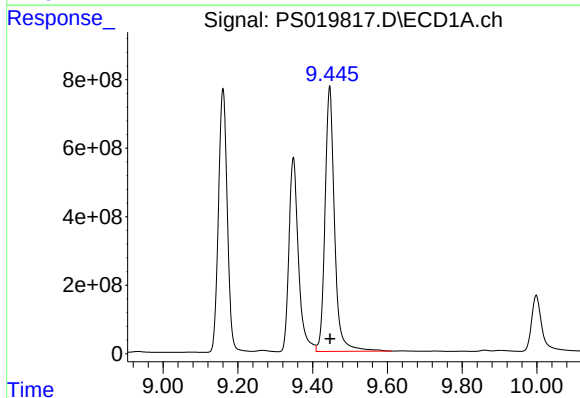


#12 2,4,5-T

R.T.: 9.446 min
Delta R.T.: -0.001 min
Response: 13703138898
Conc: 744.73 ng/ml

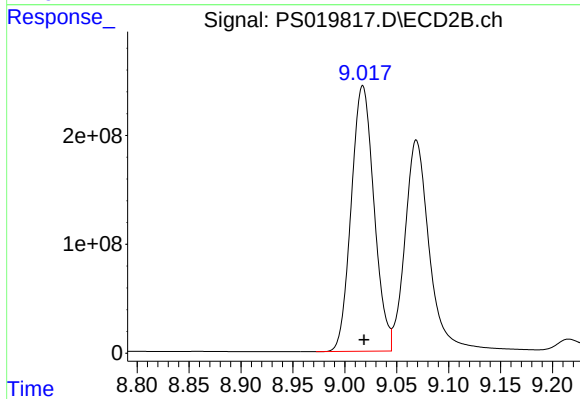

#12 2,4,5-T


R.T.: 9.017 min
Delta R.T.: -0.001 min
Response: 3726880107
Conc: 762.87 ng/ml

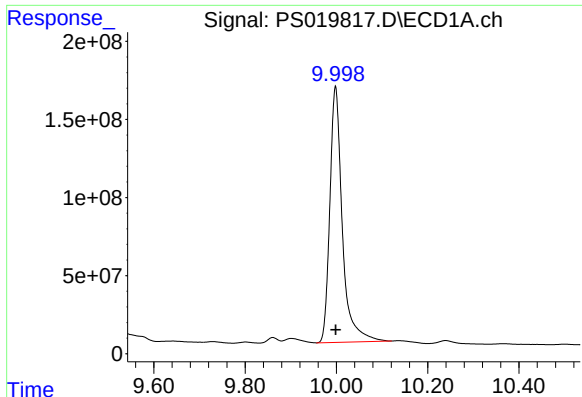

#13 2,4-DB


R.T.: 9.998 min
Delta R.T.: 0.000 min
Response: 3103531507
Conc: 775.57 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

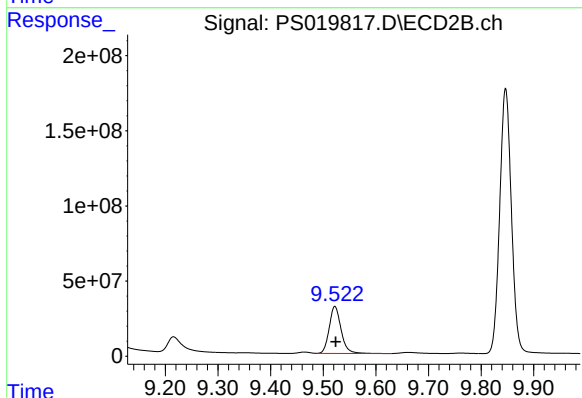


#13 2,4-DB

R.T.: 9.522 min
Delta R.T.: -0.002 min
Response: 490437130
Conc: 755.14 ng/ml

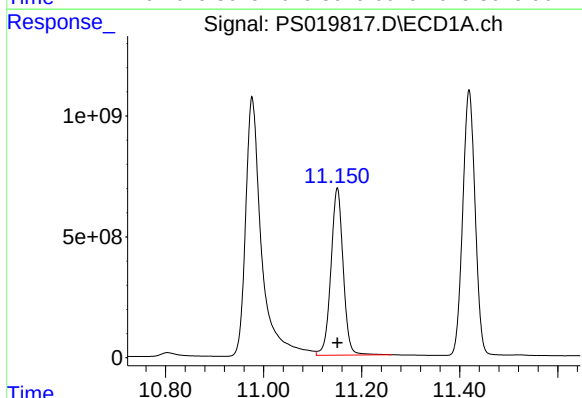


#14 DINOSEB

R.T.: 11.150 min
Delta R.T.: 0.000 min
Response: 12000888962
Conc: 738.17 ng/ml

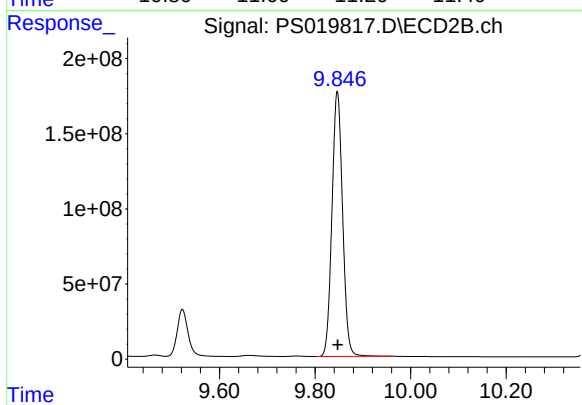

#14 DINOSEB


R.T.: 9.847 min
Delta R.T.: -0.001 min
Response: 2718488101
Conc: 762.72 ng/ml

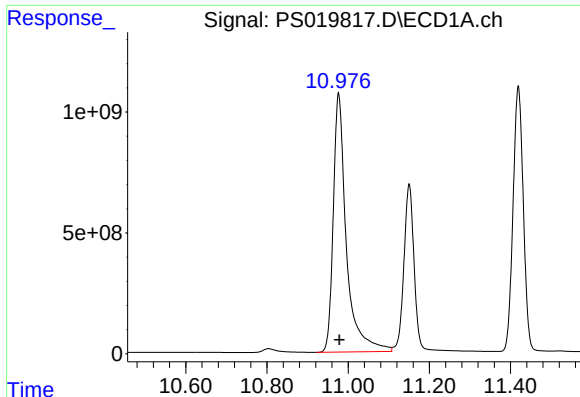

#15 Picloram


R.T.: 10.976 min
Delta R.T.: -0.002 min
Response: 24045724214
Conc: 771.12 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

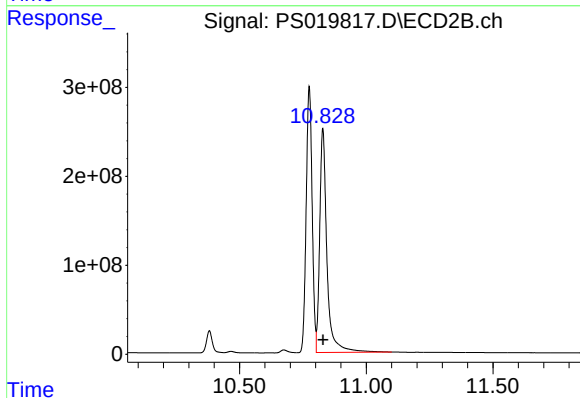


#15 Picloram

R.T.: 10.829 min
Delta R.T.: 0.000 min
Response: 5002874009
Conc: 769.25 ng/ml

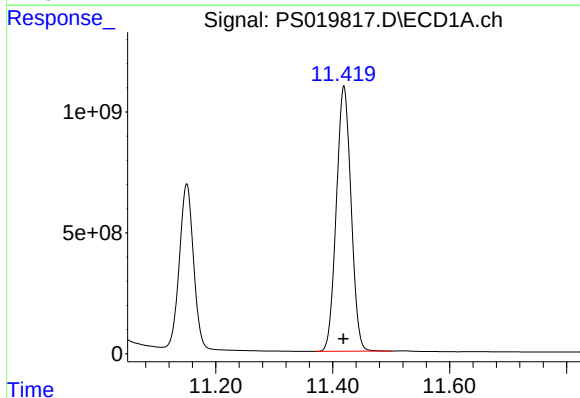

#16 DCPA

R.T.: 11.419 min
Delta R.T.: 0.000 min
Response: 19200275866
Conc: 744.28 ng/ml

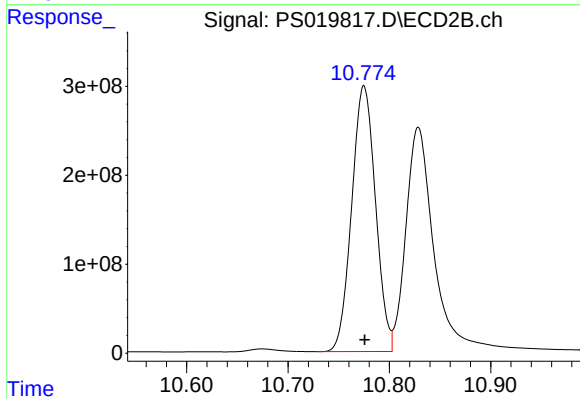

#16 DCPA

R.T.: 10.775 min
Delta R.T.: 0.000 min
Response: 4878828130
Conc: 752.81 ng/ml