

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062723\
 Data File : PS023493.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jun 2023 13:06
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 27 15:50:13 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS060623.M
 Quant Title : 8080.M
 QLast Update : Tue Jun 06 13:00:04 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.480	6.848	1032.7E6	312.3E6	583.704	550.191
Target Compounds							
1) T	Dalapon	2.569	0.000	2661623	0	1.456	N.D. #
3) T	4-Nitroph...	6.312	0.000	13924491	0	10.804	N.D. #
5) T	DICAMBA	6.627	7.013	1716028	1084806	<MDL	<MDL #
6) T	MCP	6.816	0.000	275666	0	<MDL	N.D. #
7) T	MCPA	6.941	0.000	890960	0	<MDL	N.D. #
8) T	DICHLORPROP	7.239	7.651	1964726	1494905	<MDL	2.417 #
9) T	2,4-D	0.000	7.869f	0	783497	N.D.	1.130
10) T	Pentachlo...	7.672	8.352	5417148	2173656	<MDL	<MDL #
11) T	2,4,5-TP ...	8.209	8.712	5807968	1596226	<MDL	<MDL #
12) T	2,4,5-T	8.474	9.087	9637840	1346618	<MDL	<MDL #
13) T	2,4-DB	8.980	0.000	7709761	0	3.275	N.D. #
14) T	DINOSEB	10.057	9.921	2697854	961078	<MDL	<MDL #
15) T	Picloram	9.885	10.886	224.8E6	42468678	12.955	9.306 #
16) T	DCPA	10.326	10.886	6236540	42468678	<MDL	10.586 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062723\
Data File : PS023493.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jun 2023 13:06
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 27 15:50:13 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS060623.M
Quant Title : 8080.M
QLast Update : Tue Jun 06 13:00:04 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

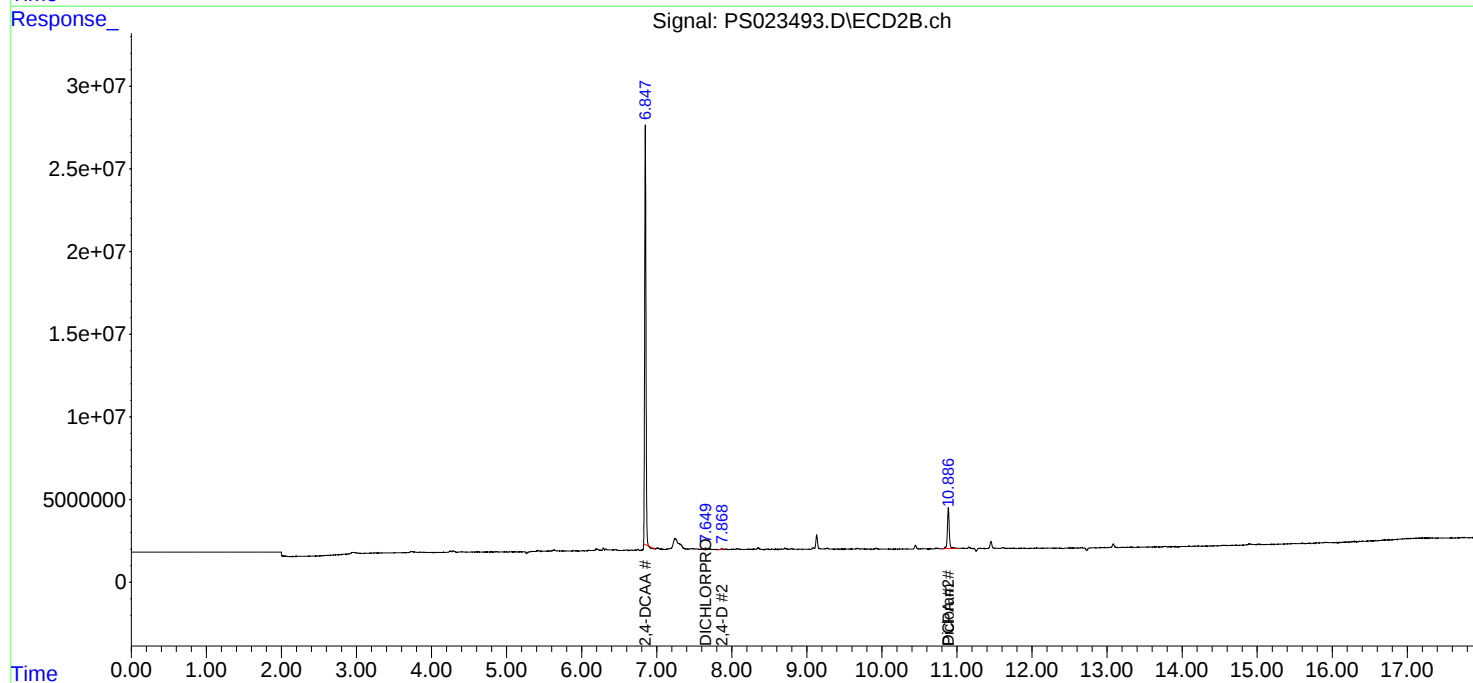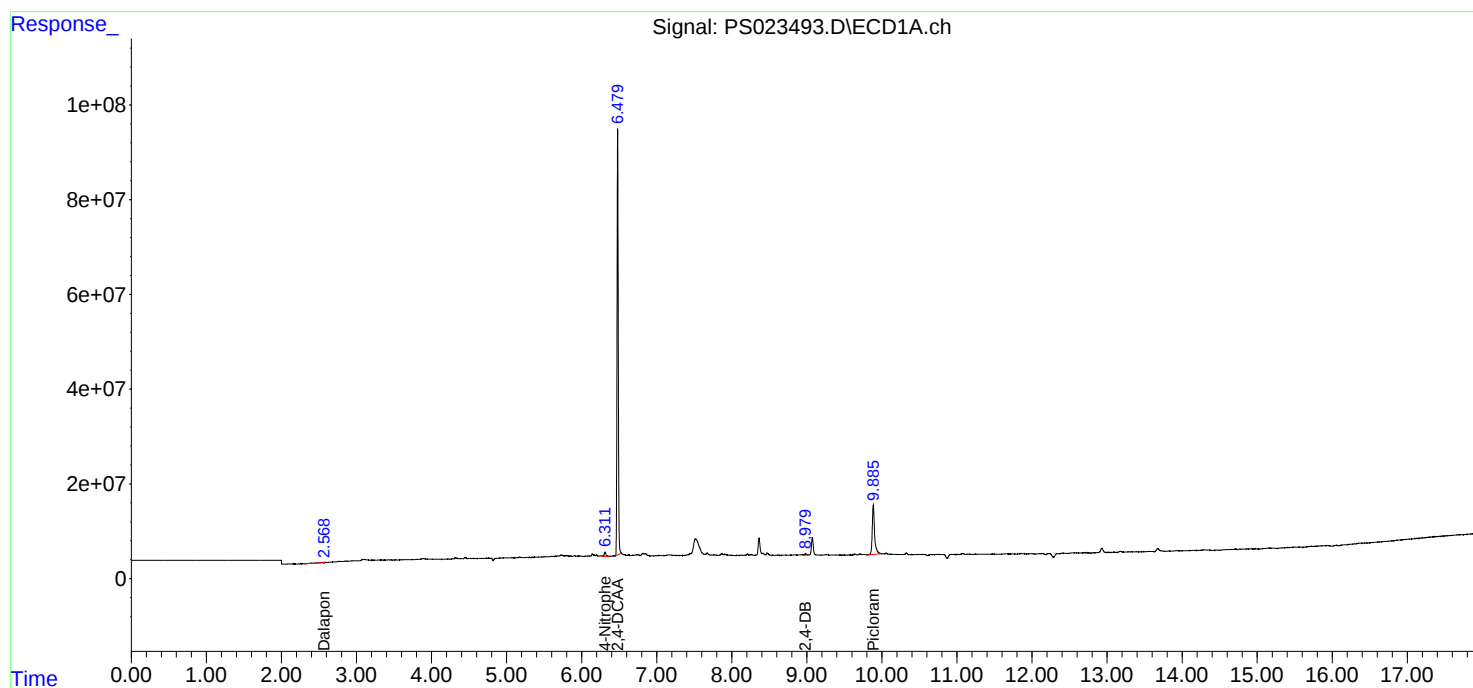


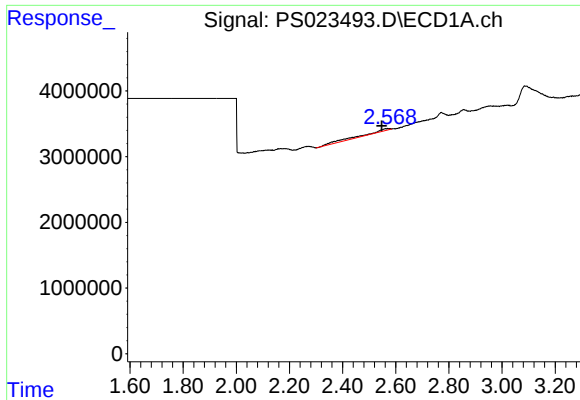

#1 Dalapon


R.T.: 2.569 min
Delta R.T.: 0.022 min
Response: 2661623
Conc: 1.46 ng/ml

Instrument :
ECD_S
ClientSampleId :

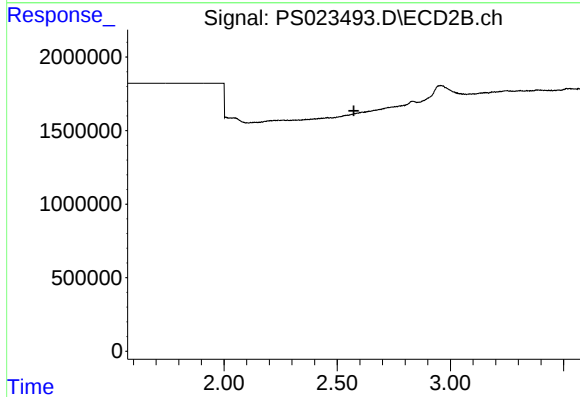


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.574 min
Response: 0
Conc: N.D.

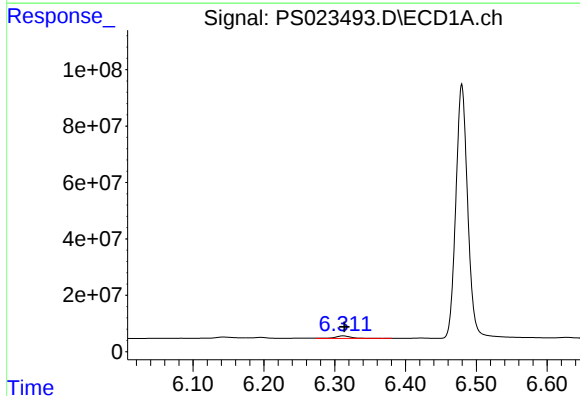


#3 4-Nitrophenol

R.T.: 6.312 min
Delta R.T.: -0.002 min
Response: 13924491
Conc: 10.80 ng/ml

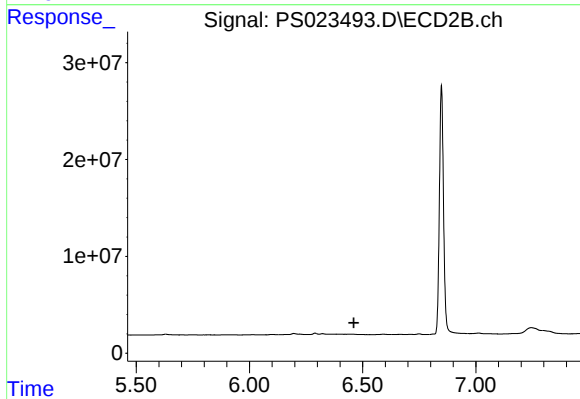

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 6.461 min
Response: 0
Conc: N.D.

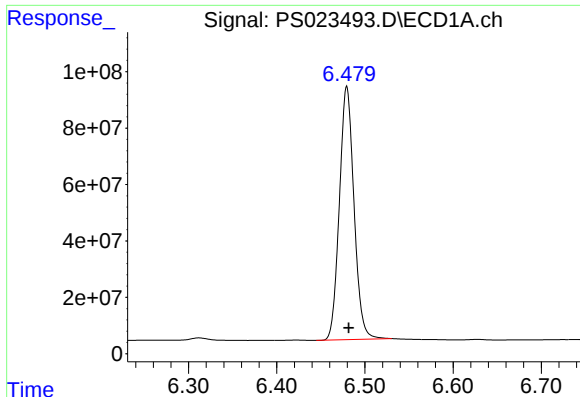

#4 2,4-DCAA


R.T.: 6.480 min
Delta R.T.: -0.002 min
Response: 1032721441
Conc: 583.70 ng/ml

Instrument :
ECD_S
ClientSampleId :

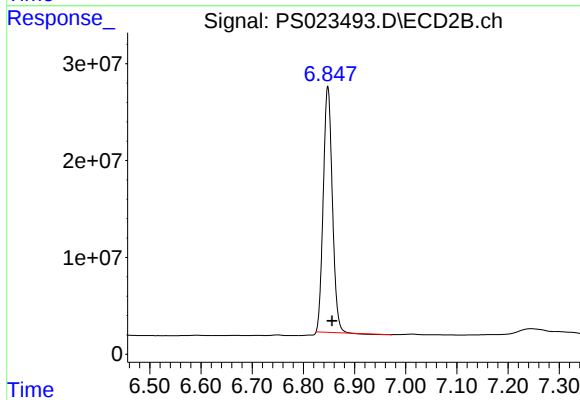


#4 2,4-DCAA

R.T.: 6.848 min
Delta R.T.: -0.008 min
Response: 312341130
Conc: 550.19 ng/ml

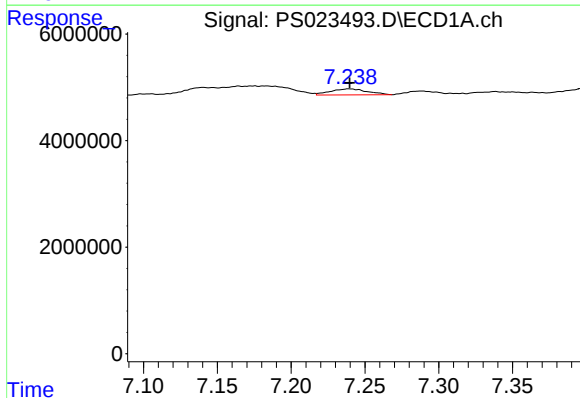


#8 DICHLORPROP

R.T.: 7.239 min
Delta R.T.: 0.000 min
Response: 1964726
Conc: N.D.

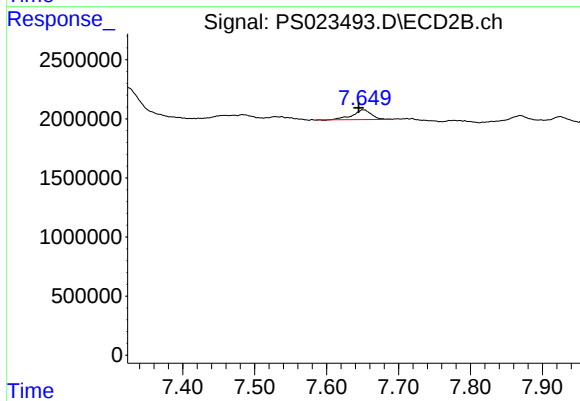

#8 DICHLORPROP


R.T.: 7.651 min
Delta R.T.: 0.006 min
Response: 1494905
Conc: 2.42 ng/ml

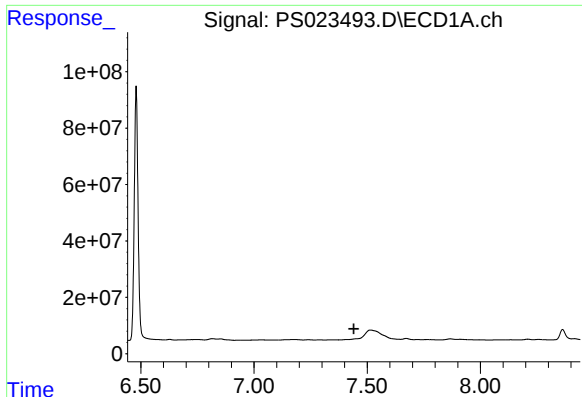

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 7.442 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

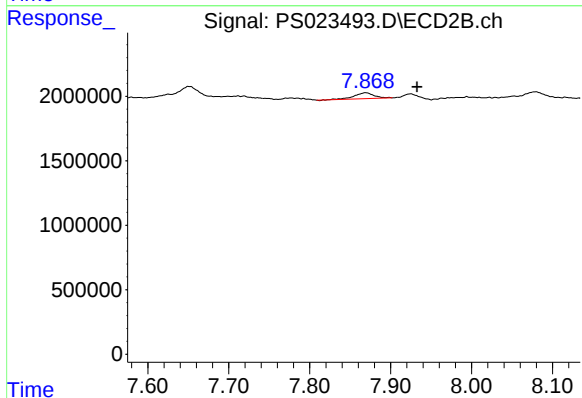


#9 2,4-D

R.T.: 7.869 min
Delta R.T.: -0.064 min
Response: 783497
Conc: 1.13 ng/ml

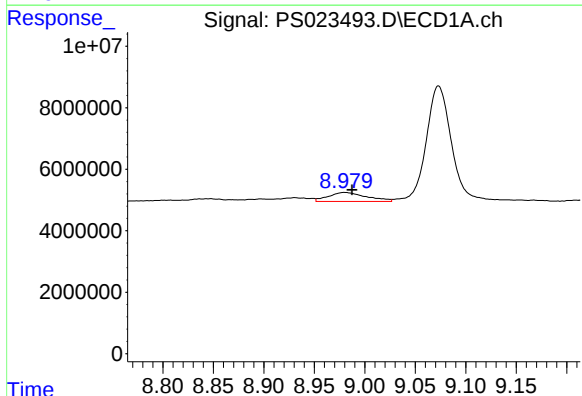


#13 2,4-DB

R.T.: 8.980 min
Delta R.T.: -0.007 min
Response: 7709761
Conc: 3.28 ng/ml

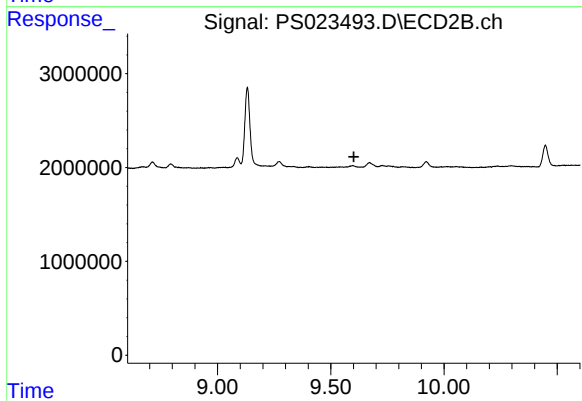

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 9.602 min
Response: 0
Conc: N.D.

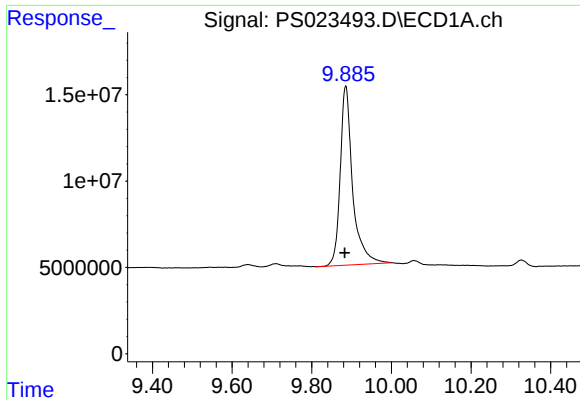

#15 Picloram


R.T.: 9.885 min
Delta R.T.: 0.003 min
Response: 224820690
Conc: 12.95 ng/ml

Instrument :
ECD_S
ClientSampleId :

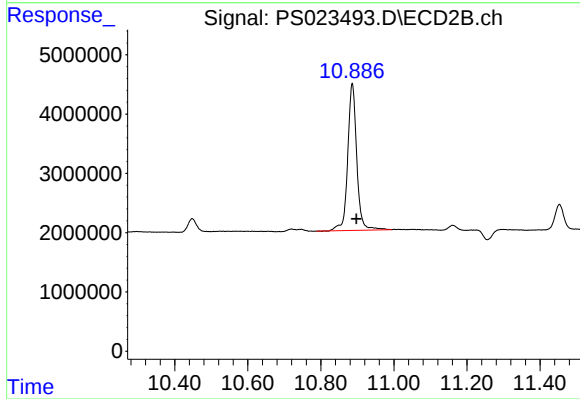


#15 Picloram

R.T.: 10.886 min
Delta R.T.: -0.012 min
Response: 42468678
Conc: 9.31 ng/ml

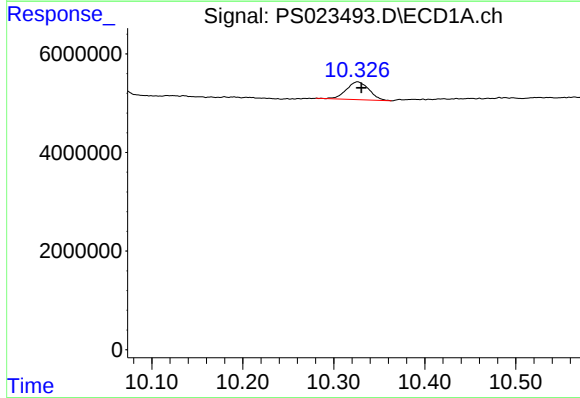

#16 DCPA

R.T.: 10.326 min
Delta R.T.: -0.004 min
Response: 6236540
Conc: N.D.

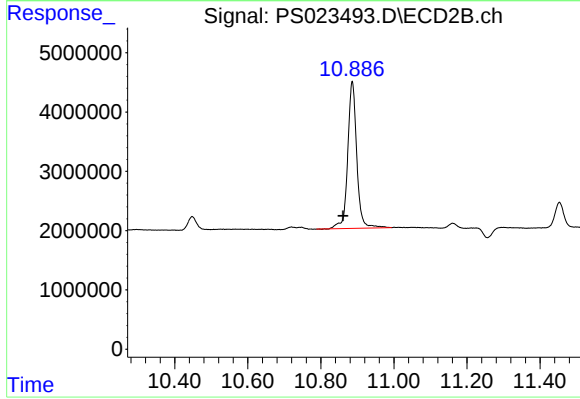

#16 DCPA

R.T.: 10.886 min
Delta R.T.: 0.025 min
Response: 42468678
Conc: 10.59 ng/ml