

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062723\
 Data File : PS023503.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jun 2023 17:10
 Operator : AR\AJ
 Sample : 03362-14
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 COMPOSIT-SB-19-20

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 27 18:08:23 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS060623.M
 Quant Title : 8080.M
 QLast Update : Tue Jun 06 13:00:04 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.425f	0.000	1335481	0	<MDL	N.D. #
Target Compounds							
1) T	Dalapon	2.542	0.000	78414	0	<MDL	N.D. #
3) T	4-Nitroph...	6.314	0.000	1401947	0	1.088	N.D. #
6) T	MCP	6.817	0.000	765937	0	<MDL	N.D. #
8) T	DICHLORPROP	7.177f	0.000	10983318	0	5.323	N.D. #
10) T	Pentachlo...	7.740f	0.000	464548	0	<MDL	N.D. #
11) T	2,4,5-TP ...	8.205	0.000	2584507	0	<MDL	N.D. #
12) T	2,4,5-T	8.464	0.000	1238856	0	<MDL	N.D. #
13) T	2,4-DB	8.942f	0.000	2080430	0	<MDL	N.D. #
14) T	DINOSEB	10.044	0.000	476819	0	<MDL	N.D. #
15) T	Picloram	9.878	0.000	1189824	0	<MDL	N.D. #
16) T	DCPA	10.320	0.000	772177	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062723\
Data File : PS023503.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jun 2023 17:10
Operator : AR\AJ
Sample : 03362-14
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
COMPOSIT-SB-19-20

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 27 18:08:23 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS060623.M
Quant Title : 8080.M
QLast Update : Tue Jun 06 13:00:04 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

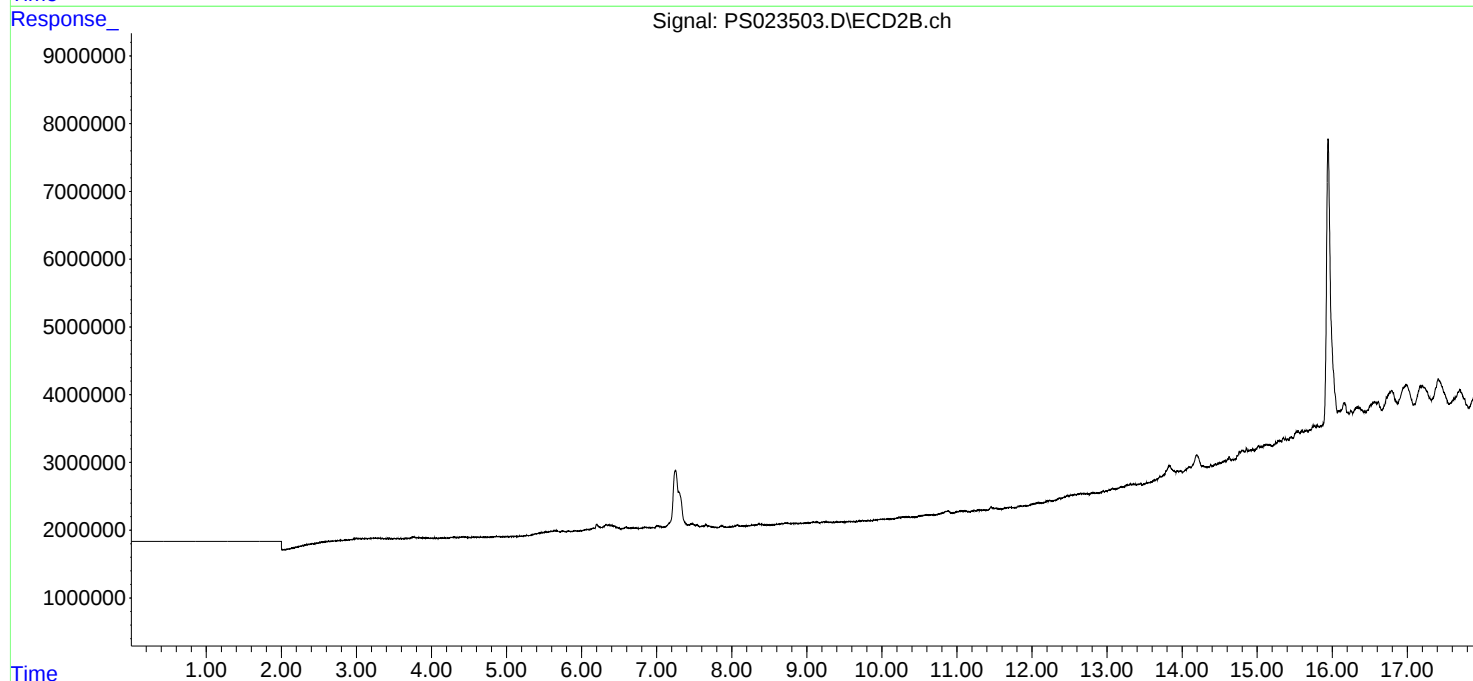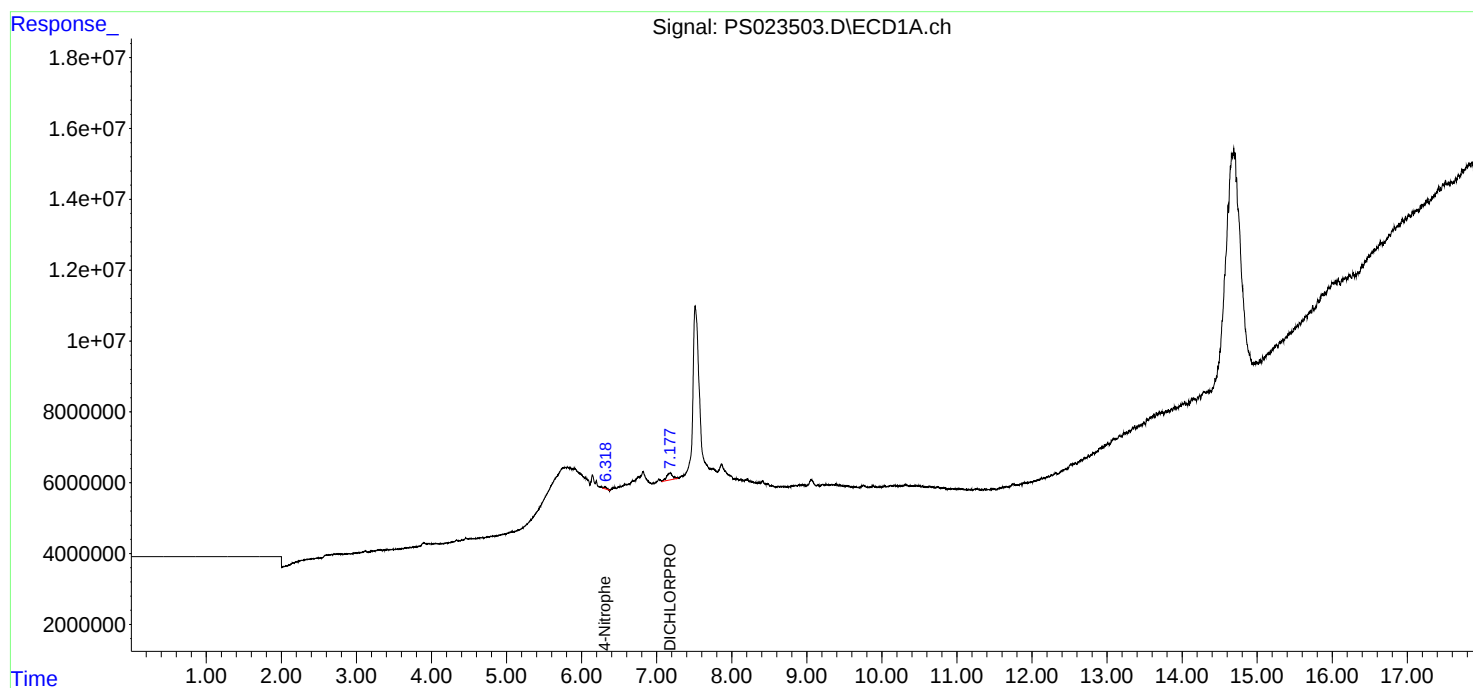


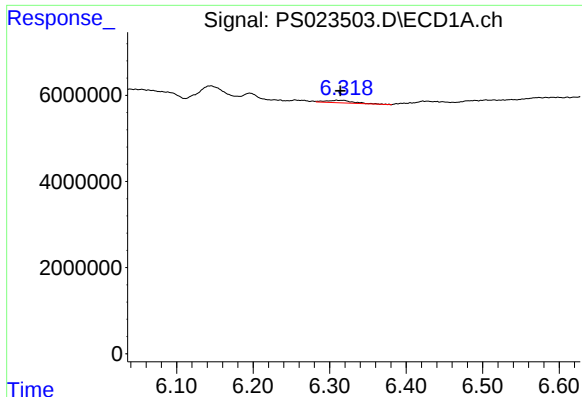

#3 4-Nitrophenol


R.T.: 6.314 min
Delta R.T.: 0.000 min
Response: 1401947
Conc: 1.09 ng/ml

Instrument :
ECD_S
ClientSampleId :
COMPOSIT-SB-19-20

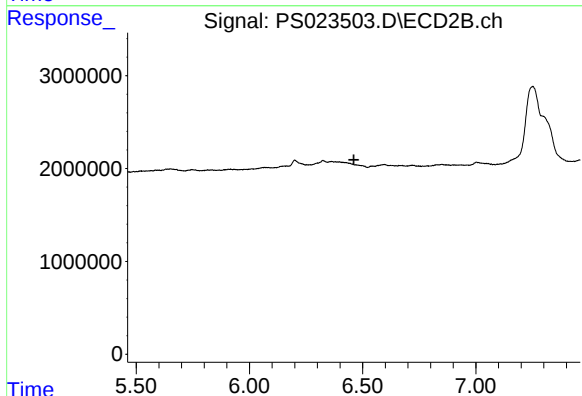


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.461 min
Response: 0
Conc: N.D.

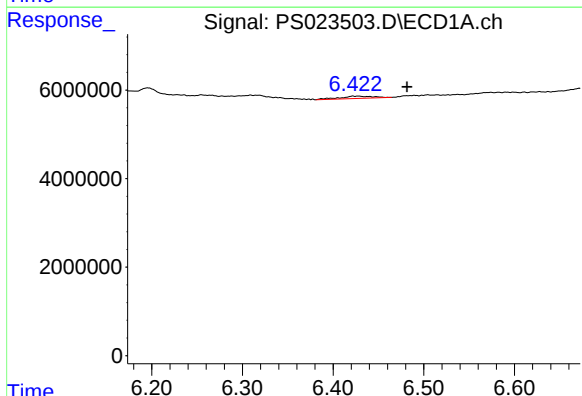


#4 2,4-DCAA

R.T.: 6.425 min
Delta R.T.: -0.056 min
Response: 1335481
Conc: N.D.

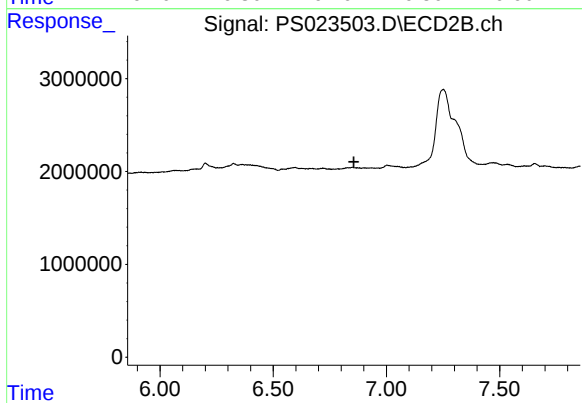

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 6.856 min
Response: 0
Conc: N.D.

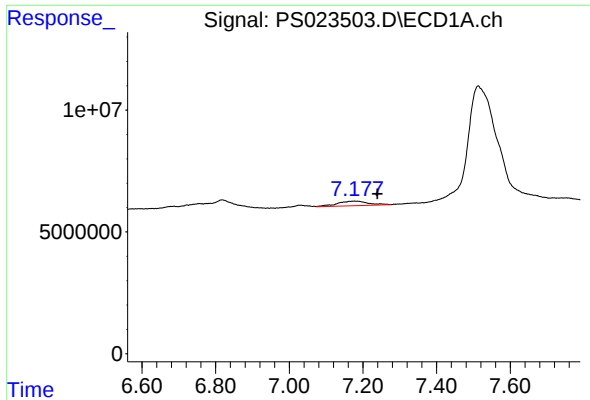

#8 DICHLORPROP

R.T.: 7.177 min
Delta R.T.: -0.063 min
Response: 10983318
Conc: 5.32 ng/ml

Instrument :
ECD_S
ClientSampleId :
COMPOSIT-SB-19-20

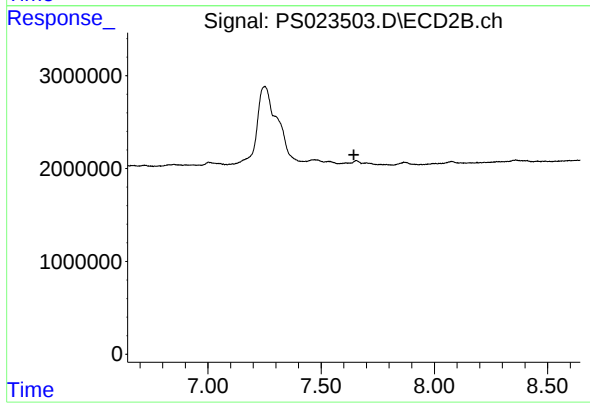

#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 7.645 min
Response: 0
Conc: N.D.