

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062723\
 Data File : PS023517.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jun 2023 00:03
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 28 02:57:31 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS060623.M
 Quant Title : 8080.M
 QLast Update : Tue Jun 06 13:00:04 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.477	6.847	954.5E6	285.0E6	539.511	502.016
Target Compounds							
1) T	Dalapon	2.563	0.000	2048124	0	1.120	N.D. #
3) T	4-Nitroph...	6.312	0.000	9328028	0	7.238	N.D. #
5) T	DICAMBA	6.624	0.000	1198275	0	<MDL	N.D. #
6) T	MCP	6.812	0.000	13070967	0	2.372	N.D. #
7) T	MCPA	6.936	7.299	-1109606	9807581	N.D.	3.649
8) T	DICHLORPROP	7.241	7.652	1295210	7828635	<MDL	12.656 #
9) T	2,4-D	7.400f	7.867f	1554675	1176477	<MDL	1.696 #
10) T	Pentachlo...	7.668	8.354	4646379	1840837	<MDL	<MDL #
11) T	2,4,5-TP ...	8.204	0.000	6022148	0	<MDL	N.D. #
12) T	2,4,5-T	8.465	9.130	6346889	1825315	<MDL	<MDL #
13) T	2,4-DB	8.978	0.000	10237709	0	4.349	N.D. #
14) T	DINOSEB	10.054	0.000	917090	0	<MDL	N.D. #
15) T	Picloram	9.878	10.883	31931069	6342491	1.840	1.390
16) T	DCPA	10.319	10.851	3390293	2085113	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062723\
Data File : PS023517.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jun 2023 00:03
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 28 02:57:31 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS060623.M
Quant Title : 8080.M
QLast Update : Tue Jun 06 13:00:04 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

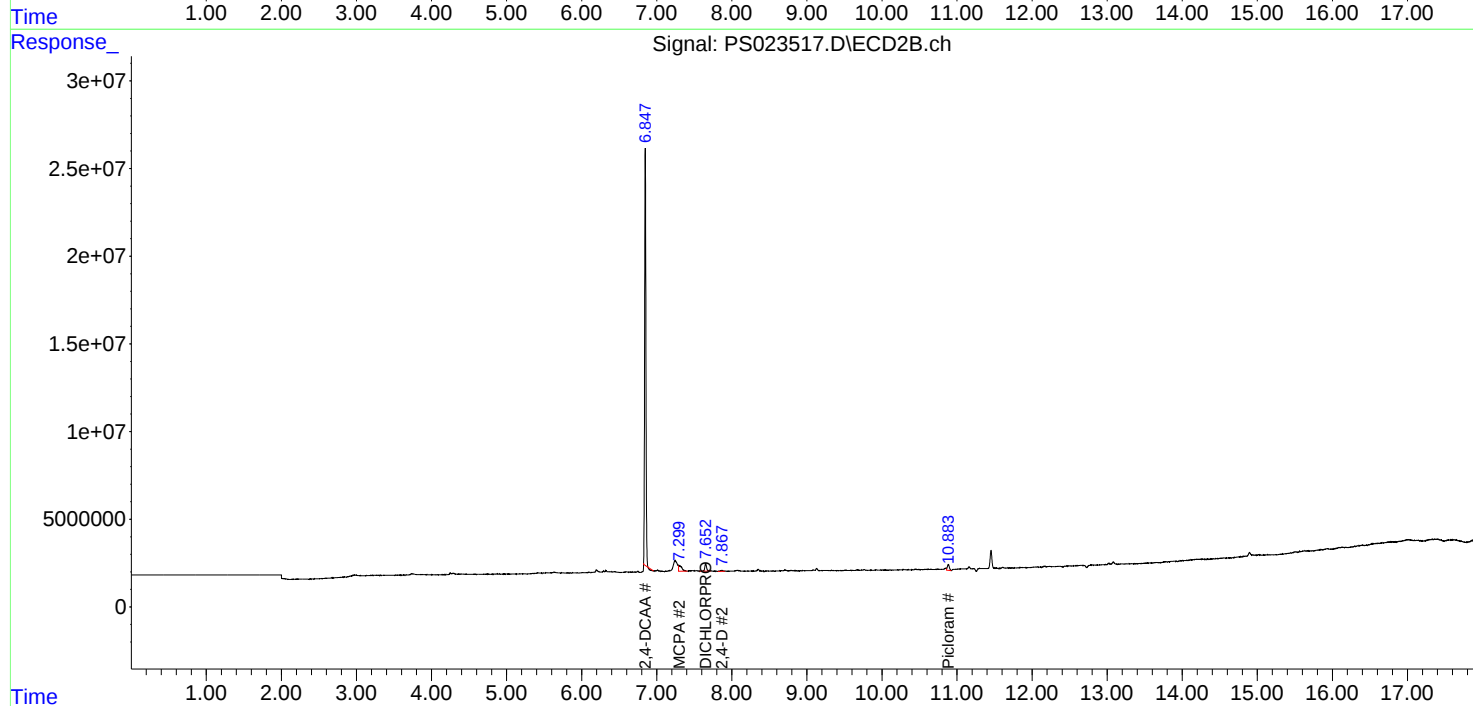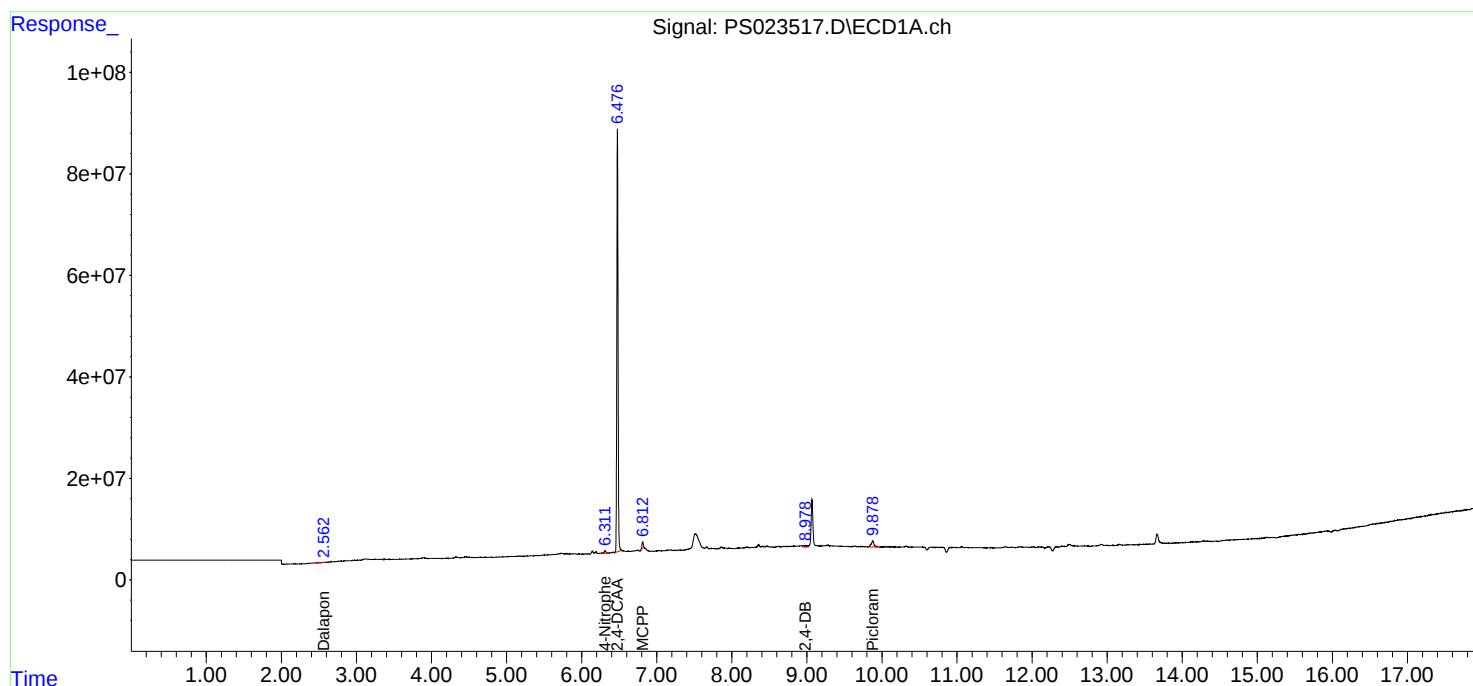


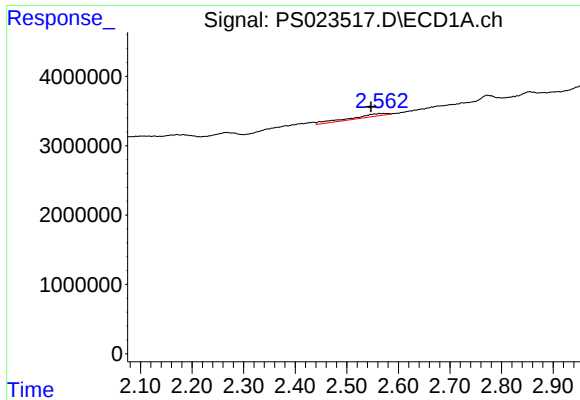

#1 Dalapon


R.T.: 2.563 min
Delta R.T.: 0.016 min
Response: 2048124
Conc: 1.12 ng/ml

Instrument :
ECD_S
ClientSampleId :

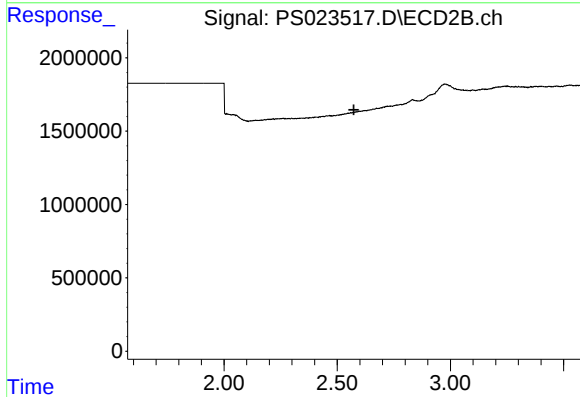


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.574 min
Response: 0
Conc: N.D.

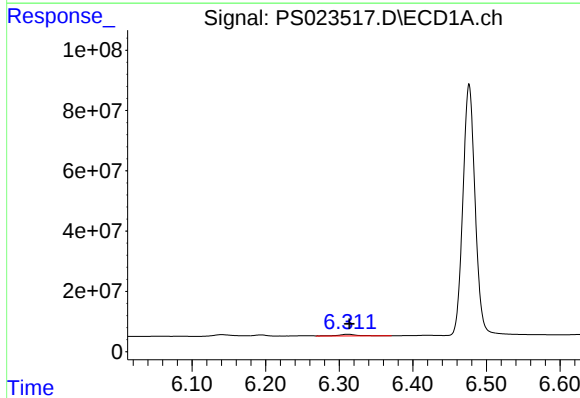


#3 4-Nitrophenol

R.T.: 6.312 min
Delta R.T.: -0.002 min
Response: 9328028
Conc: 7.24 ng/ml

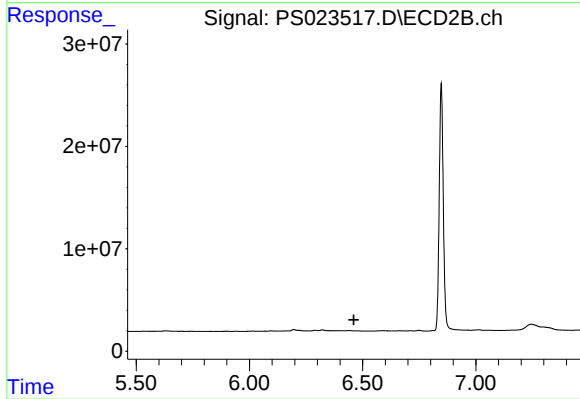

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 6.461 min
Response: 0
Conc: N.D.

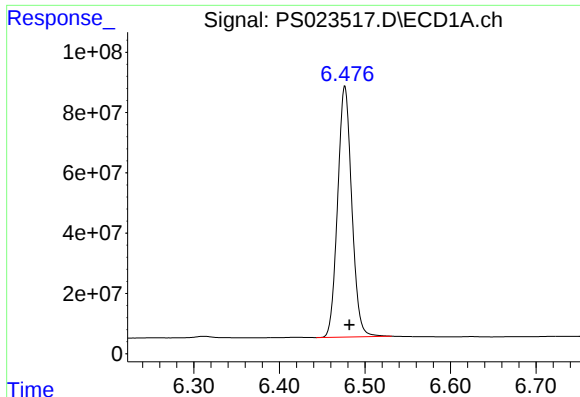

#4 2,4-DCAA


R.T.: 6.477 min
Delta R.T.: -0.005 min
Response: 954532710
Conc: 539.51 ng/ml

Instrument :
ECD_S
ClientSampleId :

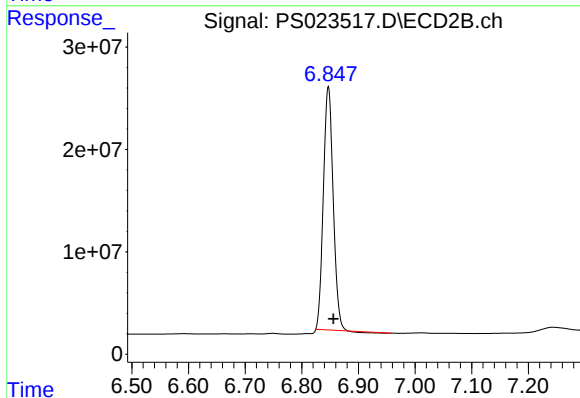


#4 2,4-DCAA

R.T.: 6.847 min
Delta R.T.: -0.009 min
Response: 284992148
Conc: 502.02 ng/ml

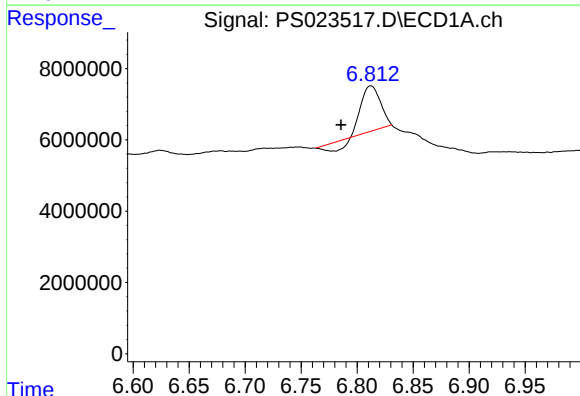


#6 MCP

R.T.: 6.812 min
Delta R.T.: 0.027 min
Response: 13070967
Conc: 2.37 ug/ml

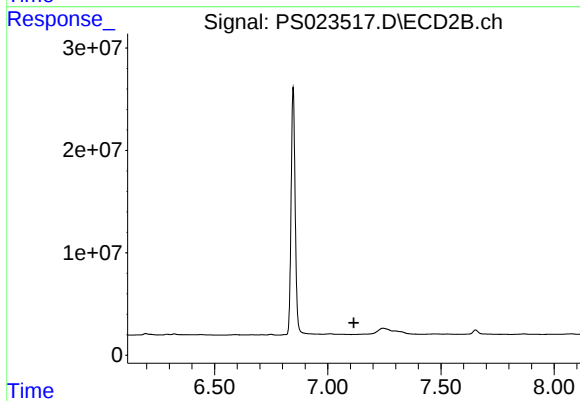

#6 MCP


R.T.: 0.000 min
Exp R.T. : 7.115 min
Response: 0
Conc: N.D.

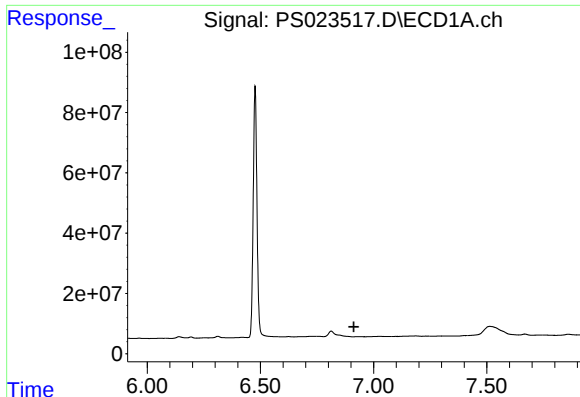

#7 MCPA


R.T.: 6.936 min
Delta R.T.: 0.023 min
Response: -1109606
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

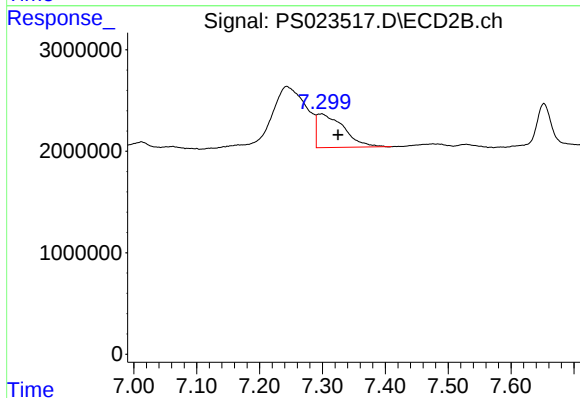


#7 MCPA

R.T.: 7.299 min
Delta R.T.: -0.026 min
Response: 9807581
Conc: 3.65 ug/ml

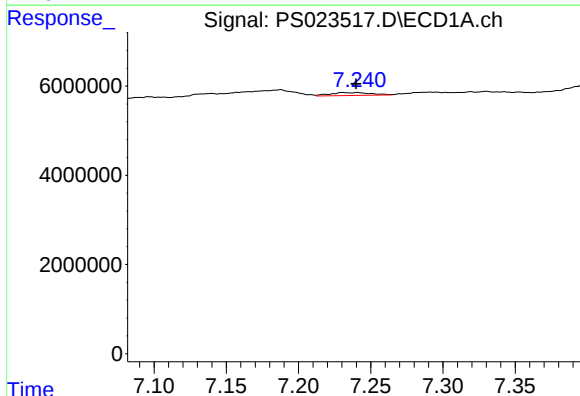


#8 DICHLORPROP

R.T.: 7.241 min
Delta R.T.: 0.001 min
Response: 1295210
Conc: N.D.

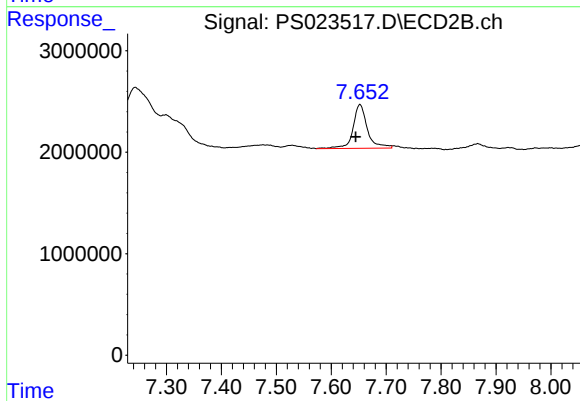

#8 DICHLORPROP


R.T.: 7.652 min
Delta R.T.: 0.008 min
Response: 7828635
Conc: 12.66 ng/ml

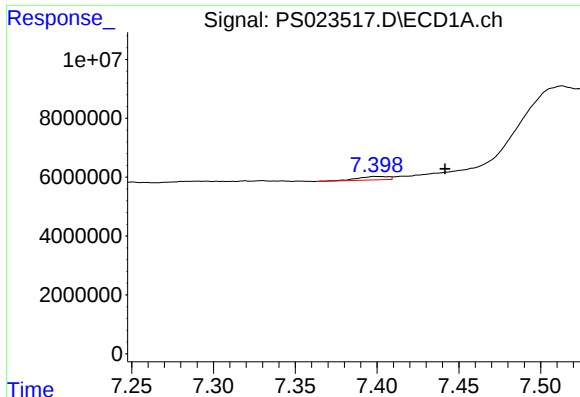

#9 2,4-D


R.T.: 7.400 min
Delta R.T.: -0.042 min
Response: 1554675
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

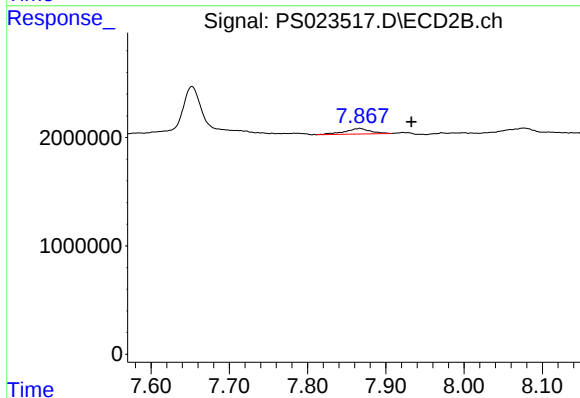


#9 2,4-D

R.T.: 7.867 min
Delta R.T.: -0.066 min
Response: 1176477
Conc: 1.70 ng/ml

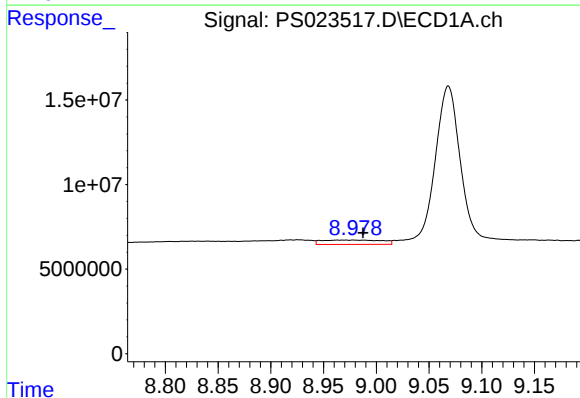


#13 2,4-DB

R.T.: 8.978 min
Delta R.T.: -0.009 min
Response: 10237709
Conc: 4.35 ng/ml

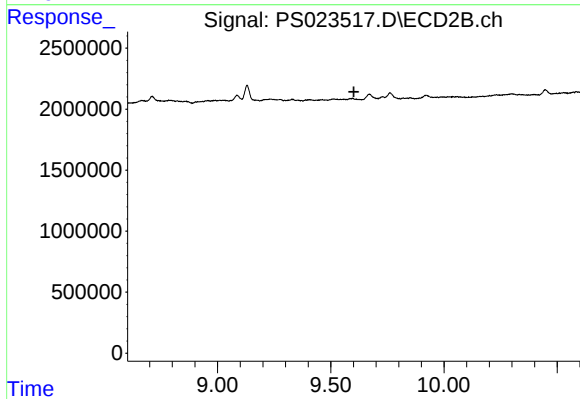

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 9.602 min
Response: 0
Conc: N.D.

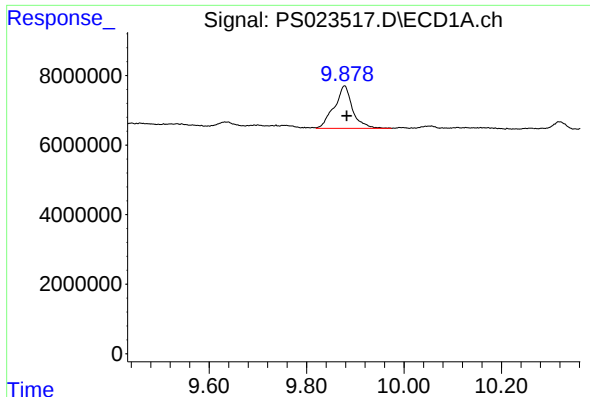

#15 Picloram

R.T.: 9.878 min
Delta R.T.: -0.005 min
Response: 31931069
Conc: 1.84 ng/ml

Instrument :
ECD_S
ClientSampleId :

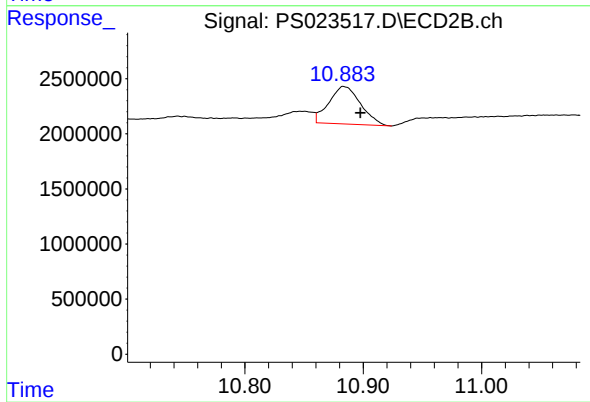

#15 Picloram

R.T.: 10.883 min
Delta R.T.: -0.014 min
Response: 6342491
Conc: 1.39 ng/ml