

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062725\
 Data File : PS030849.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jun 2025 21:29
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 27 23:25:44 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061825.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 19 05:11:26 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.340	7.766	1955.7E6	614.5E6	532.246	573.208
Target Compounds							
1) T	Dalapon	2.750f	2.659f	5778738	42551857	<MDL	15.520 #
2) T	3,5-DICHL...	6.493	0.000	49248068	0	9.158	N.D. #
3) T	4-Nitroph...	7.121f	0.000	39889352	0	25.298	N.D. #
5) T	DICAMBA	7.527	7.974	1383362	6507820	<MDL	<MDL #
6) T	MCPD	7.773f	8.084	45566106	6996411	4.853	3.336 #
7) T	MCPA	7.880	0.000	1957087	0	<MDL	N.D. #
8) T	DICHLORPROP	8.212f	8.681	27459003	4262314	7.331	2.711 #
9) T	2,4-D	0.000	8.983f	0	3506176	N.D.	2.063
10) T	Pentachlo...	8.782	9.548	7521020	22952909	<MDL	<MDL #
11) T	2,4,5-TP ...	9.360	9.927	17838499	11429325	<MDL	<MDL #
12) T	2,4,5-T	9.658	10.360	4993987	3735460	<MDL	<MDL #
13) T	2,4-DB	0.000	10.957f	0	37202209	N.D.	31.450
14) T	DINOSEB	11.460	0.000	3510119	0	<MDL	N.D. #
15) T	Picloram	11.264	12.422	8970664	20537041	<MDL	<MDL #
16) T	DCPA	11.754	12.366	13048545	9129773	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062725\
Data File : PS030849.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jun 2025 21:29
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 27 23:25:44 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061825.M
Quant Title : 8080.M
QLast Update : Thu Jun 19 05:11:26 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

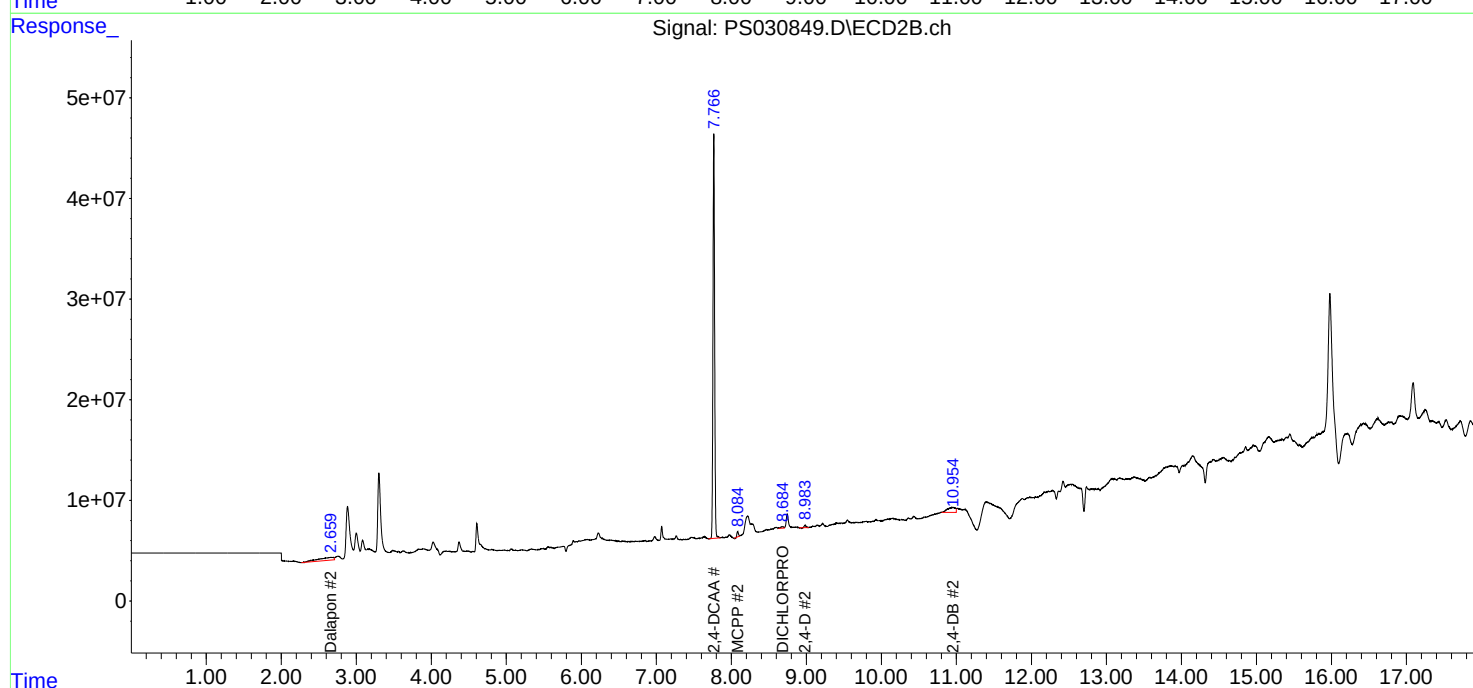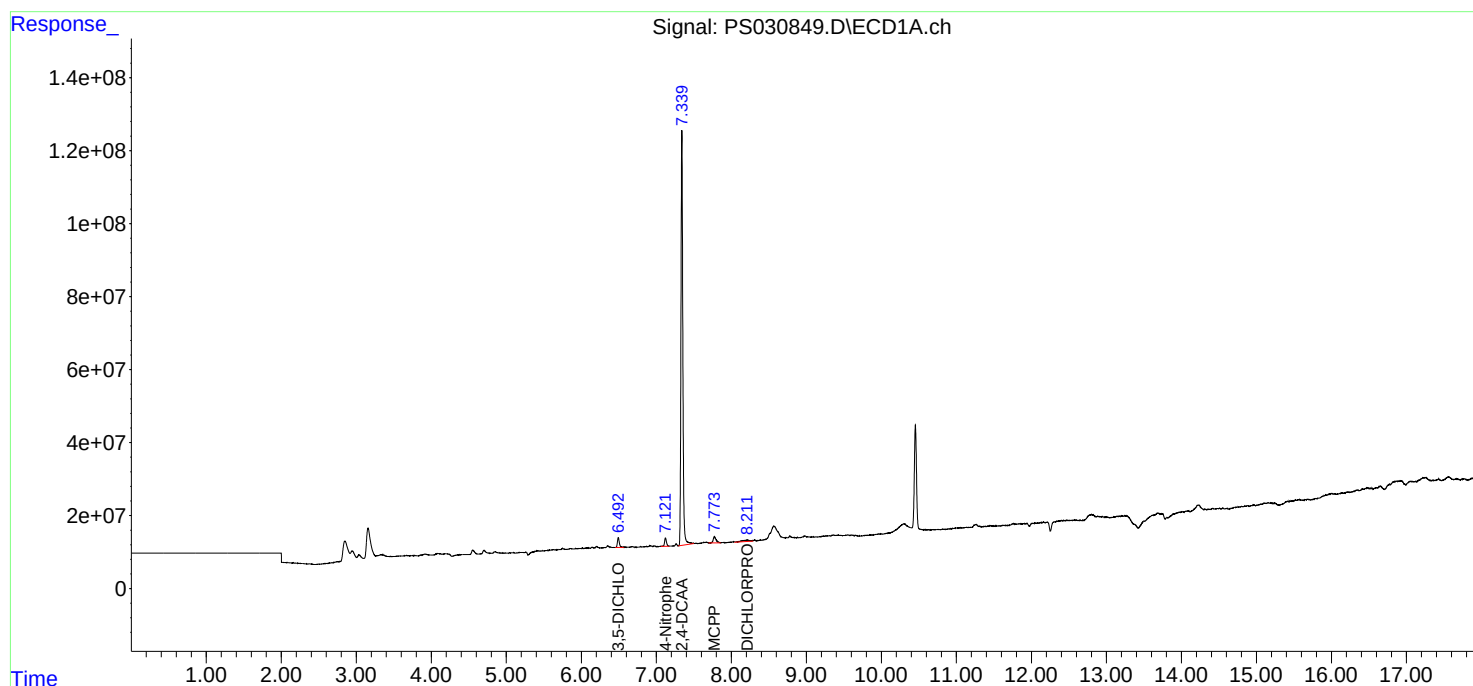


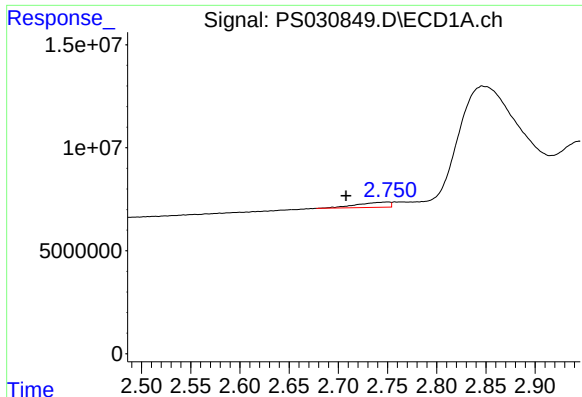

#1 Dalapon


R.T.: 2.750 min
Delta R.T.: 0.042 min
Response: 5778738
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

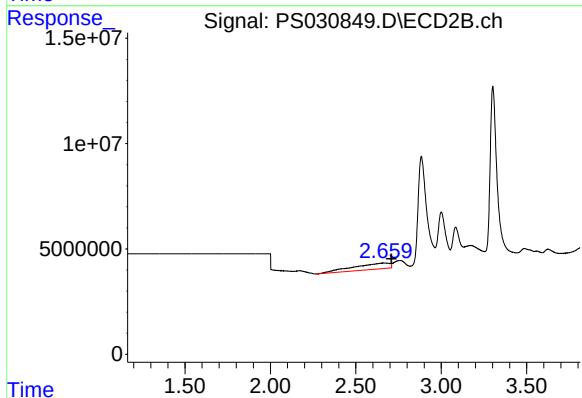


#1 Dalapon

R.T.: 2.659 min
Delta R.T.: -0.048 min
Response: 42551857
Conc: 15.52 ng/ml

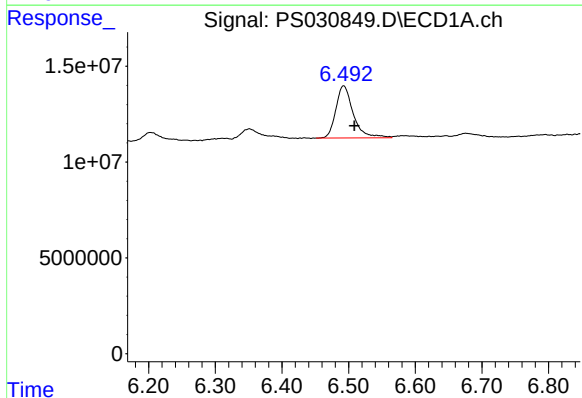


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.493 min
Delta R.T.: -0.016 min
Response: 49248068
Conc: 9.16 ng/ml

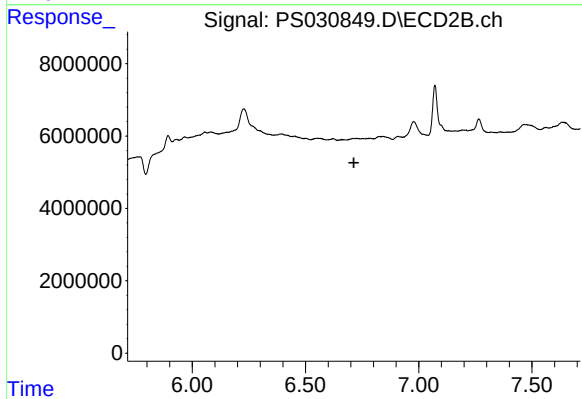

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.713 min
Response: 0
Conc: N.D.

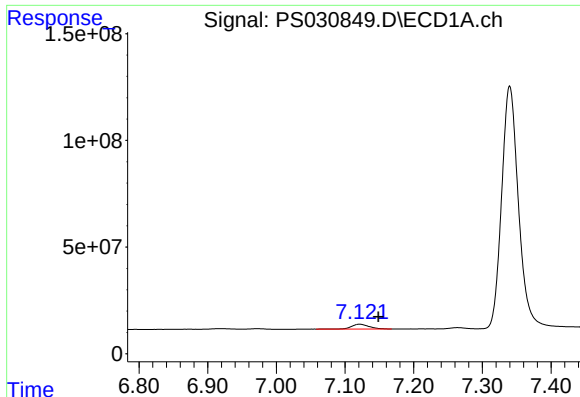

#3 4-Nitrophenol


R.T.: 7.121 min
Delta R.T.: -0.027 min
Response: 39889352
Conc: 25.30 ng/ml

Instrument :
ECD_S
ClientSampleId :

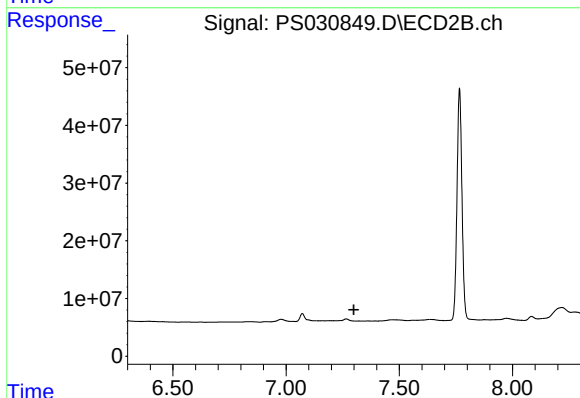


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 7.299 min
Response: 0
Conc: N.D.

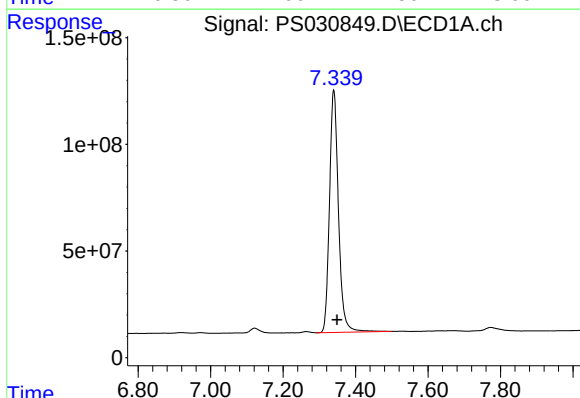


#4 2,4-DCAA

R.T.: 7.340 min
Delta R.T.: -0.010 min
Response: 1955682047
Conc: 532.25 ng/ml

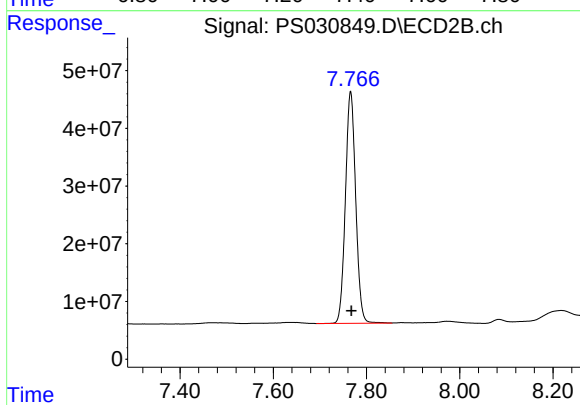

#4 2,4-DCAA


R.T.: 7.766 min
Delta R.T.: -0.002 min
Response: 614457895
Conc: 573.21 ng/ml

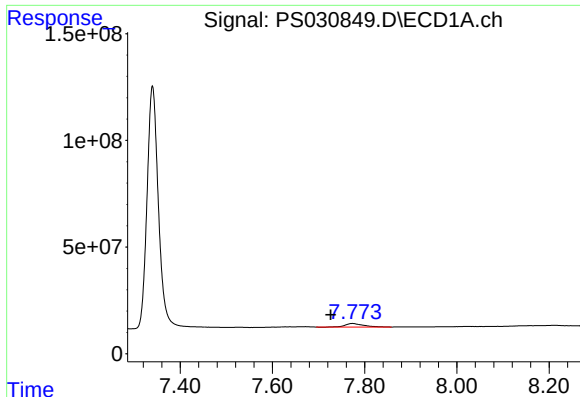

#6 MCP


R.T.: 7.773 min
Delta R.T.: 0.047 min
Response: 45566106
Conc: 4.85 ug/ml

Instrument :
ECD_S
ClientSampleId :

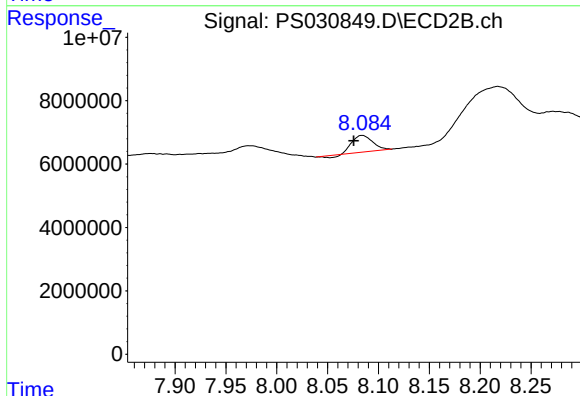


#6 MCP

R.T.: 8.084 min
Delta R.T.: 0.008 min
Response: 6996411
Conc: 3.34 ug/ml

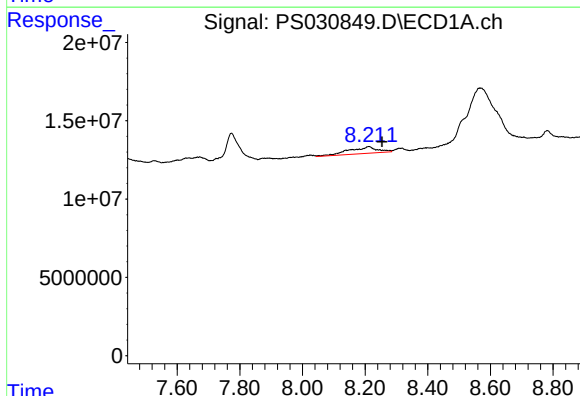


#8 DICHLORPROP

R.T.: 8.212 min
Delta R.T.: -0.043 min
Response: 27459003
Conc: 7.33 ng/ml

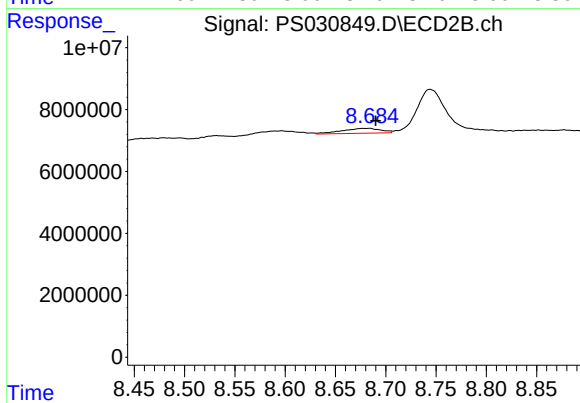

#8 DICHLORPROP


R.T.: 8.681 min
Delta R.T.: -0.009 min
Response: 4262314
Conc: 2.71 ng/ml

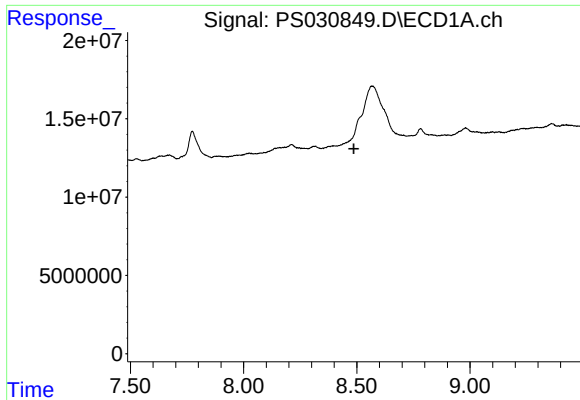

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.487 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

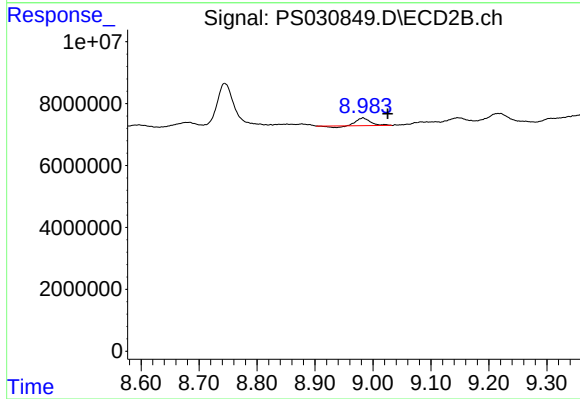


#9 2,4-D

R.T.: 8.983 min
Delta R.T.: -0.043 min
Response: 3506176
Conc: 2.06 ng/ml

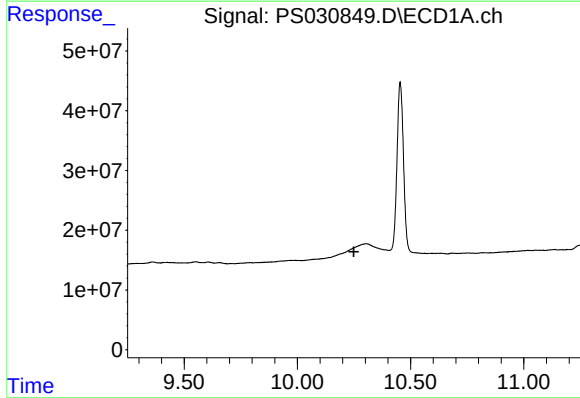

#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 10.250 min
Response: 0
Conc: N.D.

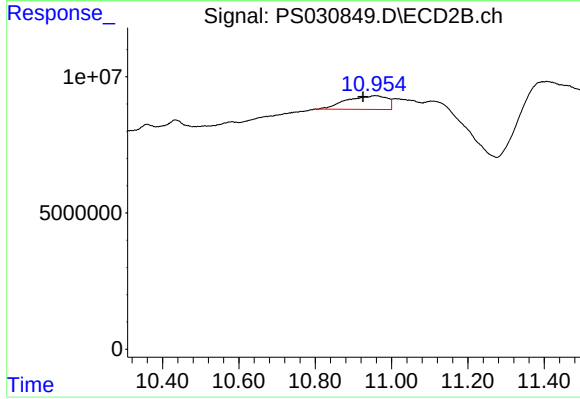

#13 2,4-DB

R.T.: 10.957 min
Delta R.T.: 0.031 min
Response: 37202209
Conc: 31.45 ng/ml