

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062821\
 Data File : PS015940.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jun 2021 09:07
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 28 14:36:53 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061521.M
 Quant Title : 8080.M
 QLast Update : Tue Jun 15 18:15:49 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
8) T	DICHLORPROP	0.000	7.565	0	6733643	N.D. 13.006
10) T	Pentachlo...	8.613	0.000	9346714	0	<MDL N.D. #
12) T	2,4,5-T	9.447	9.054f	14498879	21448908	1.642 7.605 #
13) T	2,4-DB	9.990	0.000	8759356	0	4.282 N.D. #
14) T	DINOSEB	11.158	0.000	8182190	0	1.263 N.D. #
15) T	Picloram	10.975	10.815	215.1E6	82461226	15.734 19.608
16) T	DCPA	11.424	10.815	32052145	82461226	2.423 19.614 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062821\
Data File : PS015940.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jun 2021 09:07
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 28 14:36:53 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061521.M
Quant Title : 8080.M
QLast Update : Tue Jun 15 18:15:49 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

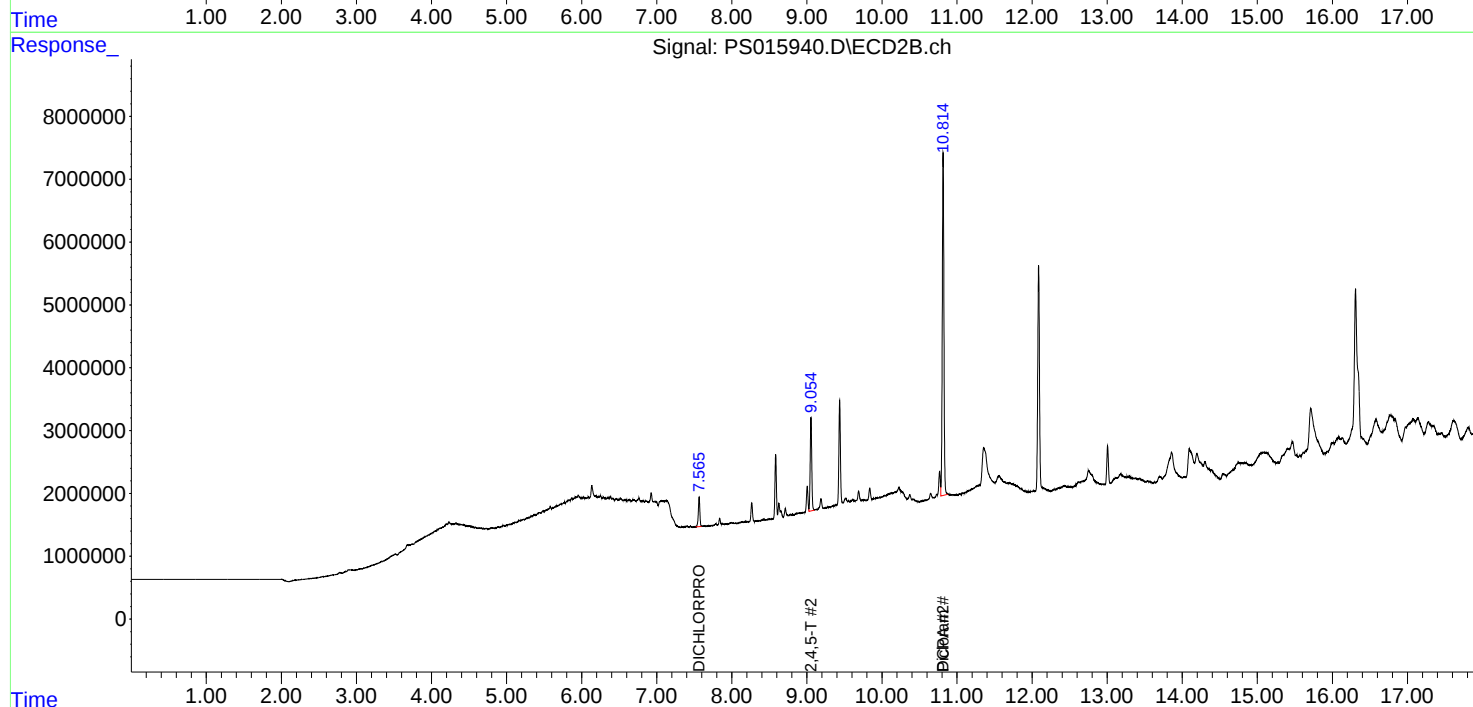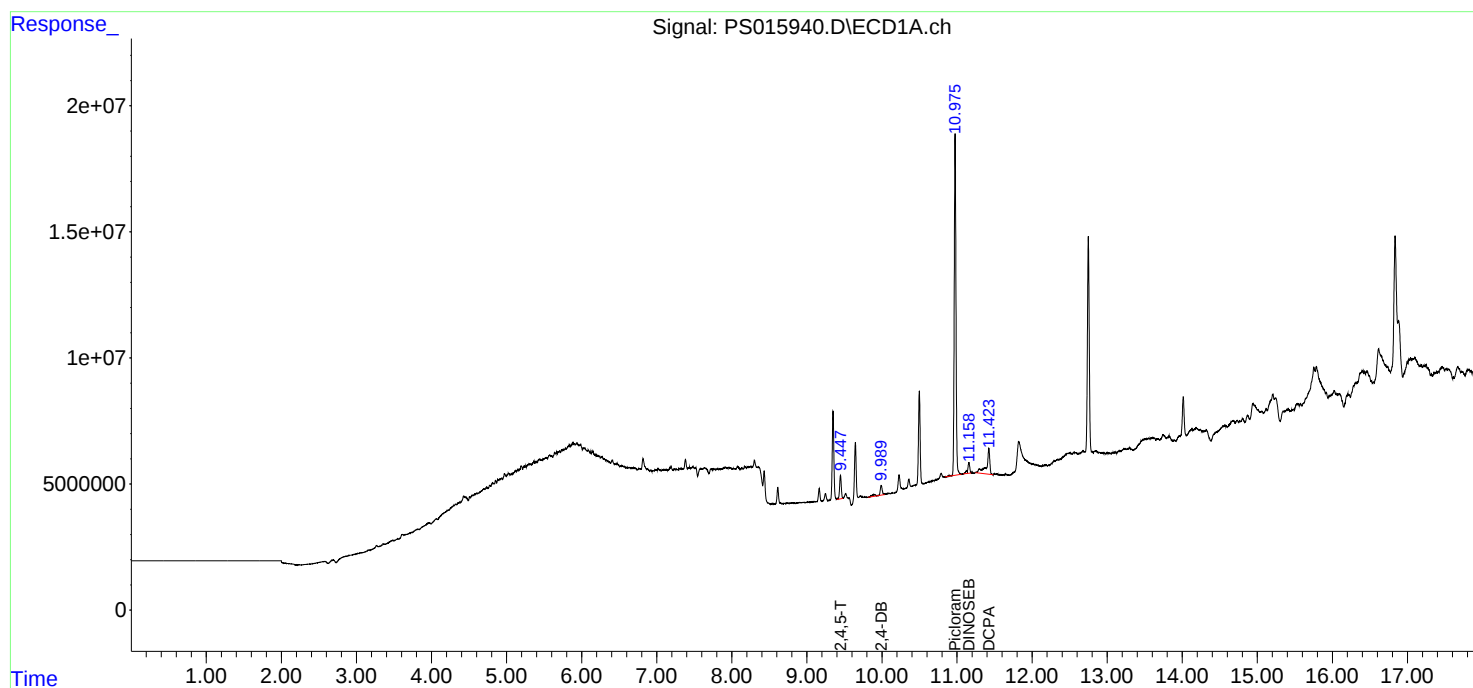


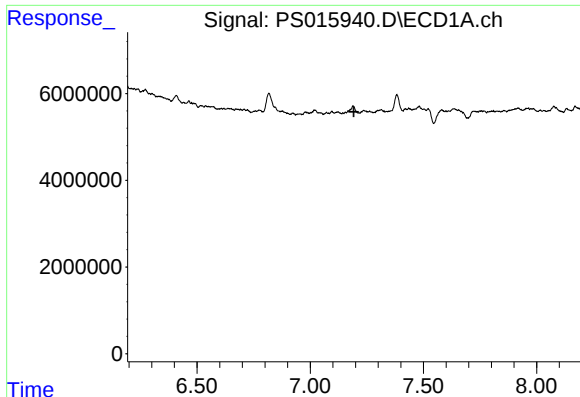

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 7.193 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

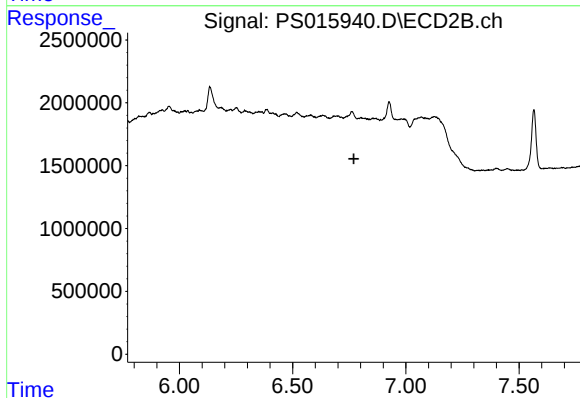


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 6.771 min
Response: 0
Conc: N.D.

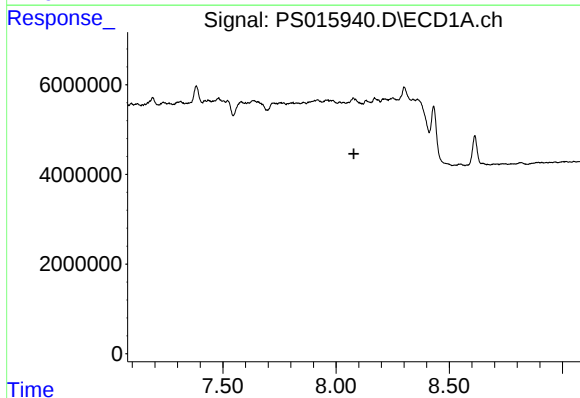


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.079 min
Response: 0
Conc: N.D.

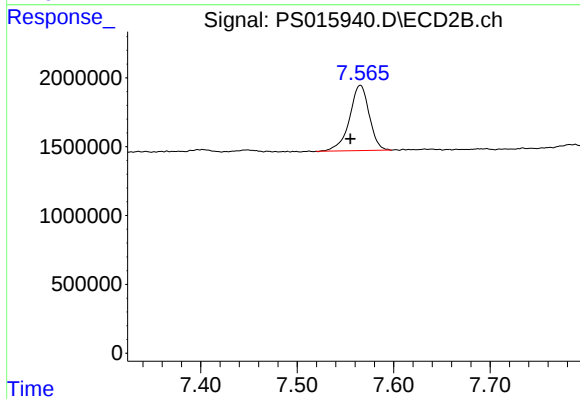

#8 DICHLORPROP


R.T.: 7.565 min
Delta R.T.: 0.010 min
Response: 6733643
Conc: 13.01 ng/ml

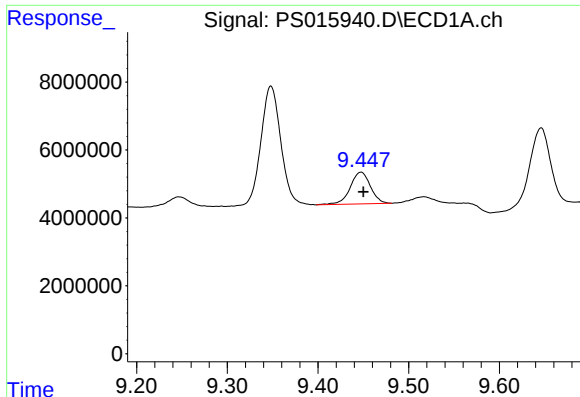

#12 2,4,5-T


R.T.: 9.447 min
Delta R.T.: -0.003 min
Response: 14498879
Conc: 1.64 ng/ml

Instrument :
ECD_S
ClientSampleId :

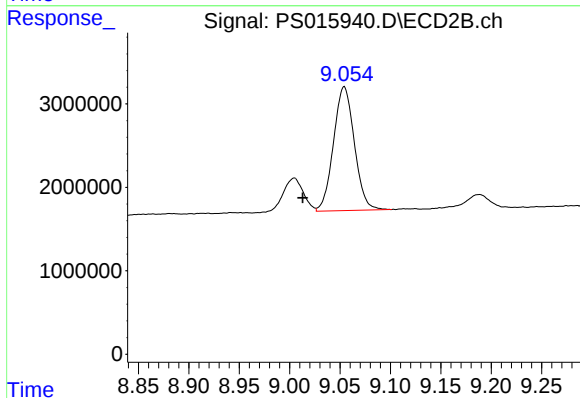


#12 2,4,5-T

R.T.: 9.054 min
Delta R.T.: 0.041 min
Response: 21448908
Conc: 7.60 ng/ml

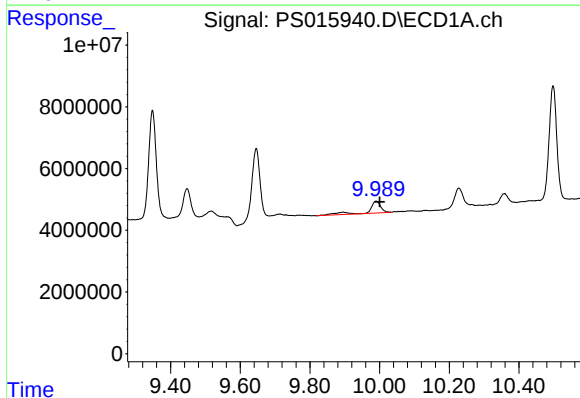


#13 2,4-DB

R.T.: 9.990 min
Delta R.T.: -0.010 min
Response: 8759356
Conc: 4.28 ng/ml

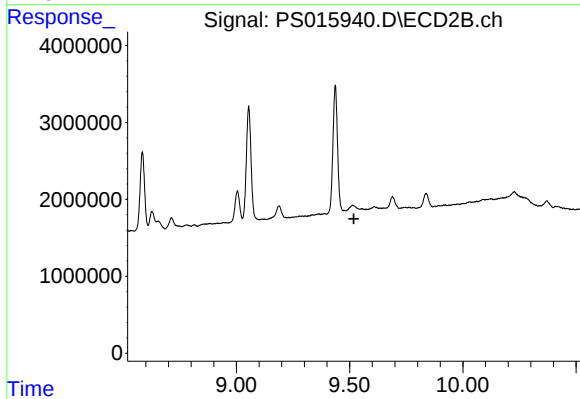

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 9.519 min
Response: 0
Conc: N.D.

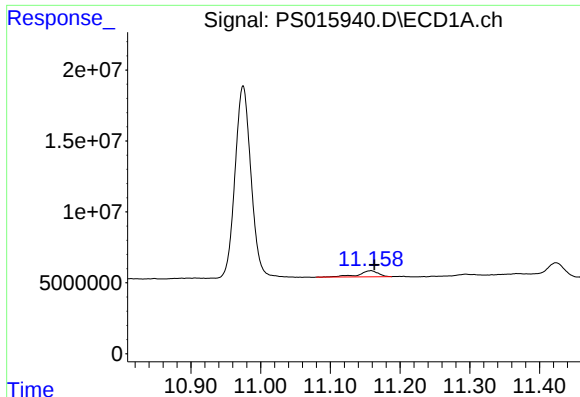

#14 DINOSEB


R.T.: 11.158 min
Delta R.T.: -0.006 min
Response: 8182190
Conc: 1.26 ng/ml

Instrument :
ECD_S
ClientSampleId :

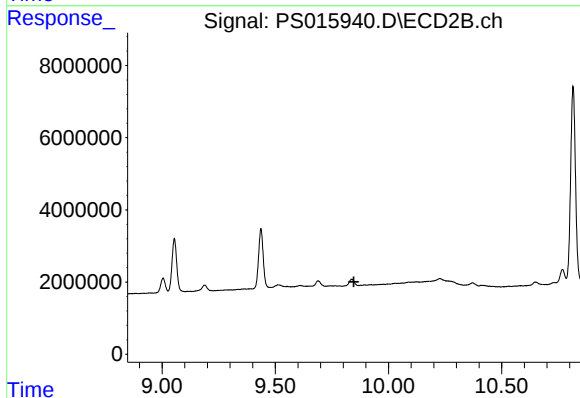


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 9.847 min
Response: 0
Conc: N.D.

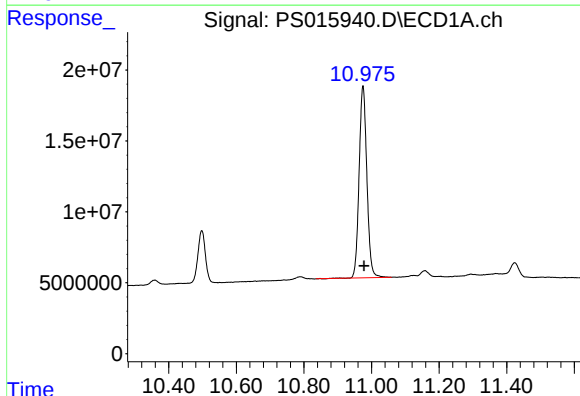


#15 Picloram

R.T.: 10.975 min
Delta R.T.: -0.003 min
Response: 215099235
Conc: 15.73 ng/ml

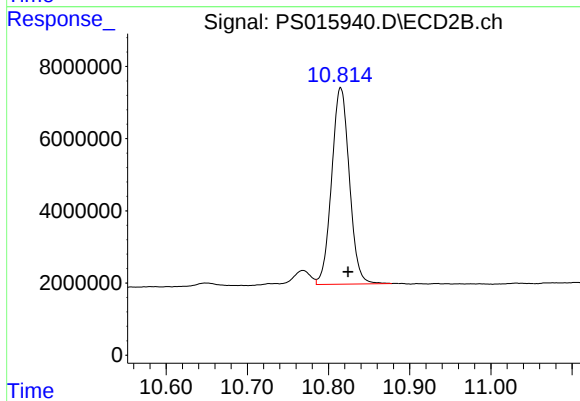

#15 Picloram


R.T.: 10.815 min
Delta R.T.: -0.009 min
Response: 82461226
Conc: 19.61 ng/ml

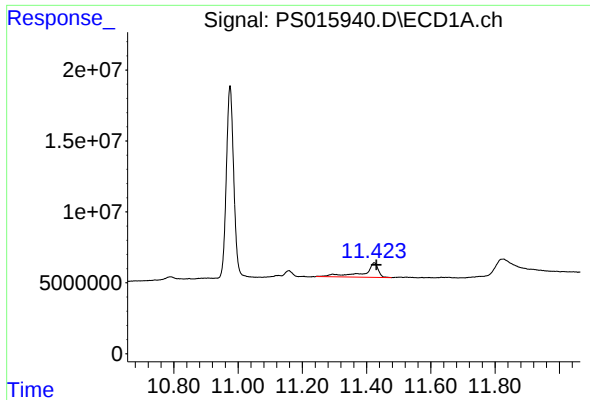

#16 DCPA

R.T.: 11.424 min
Delta R.T.: -0.007 min
Response: 32052145
Conc: 2.42 ng/ml

Instrument :
ECD_S
ClientSampleId :

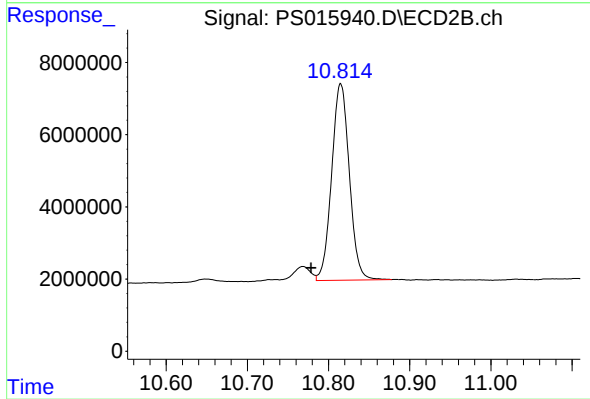

#16 DCPA

R.T.: 10.815 min
Delta R.T.: 0.036 min
Response: 82461226
Conc: 19.61 ng/ml