

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062821\
 Data File : PS015941.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jun 2021 09:31
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 28 14:37:04 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061521.M
 Quant Title : 8080.M
 QLast Update : Tue Jun 15 18:15:49 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.189	6.765	651.7E6	240.8E6	392.249	477.891
Target Compounds							
8) T	DICHLORPROP	0.000	7.568	0	8190500	N.D.	15.820
9) T	2,4-D	8.374f	0.000	30986655	0	17.681	N.D. #
12) T	2,4,5-T	9.448	9.058f	7823555	10969431	<MDL	3.889 #
15) T	Picloram	10.979	10.818	131.5E6	52684980	9.622	12.527 #
16) T	DCPA	0.000	10.818	0	52684980	N.D.	12.531



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062821\
Data File : PS015941.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jun 2021 09:31
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 28 14:37:04 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061521.M
Quant Title : 8080.M
QLast Update : Tue Jun 15 18:15:49 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

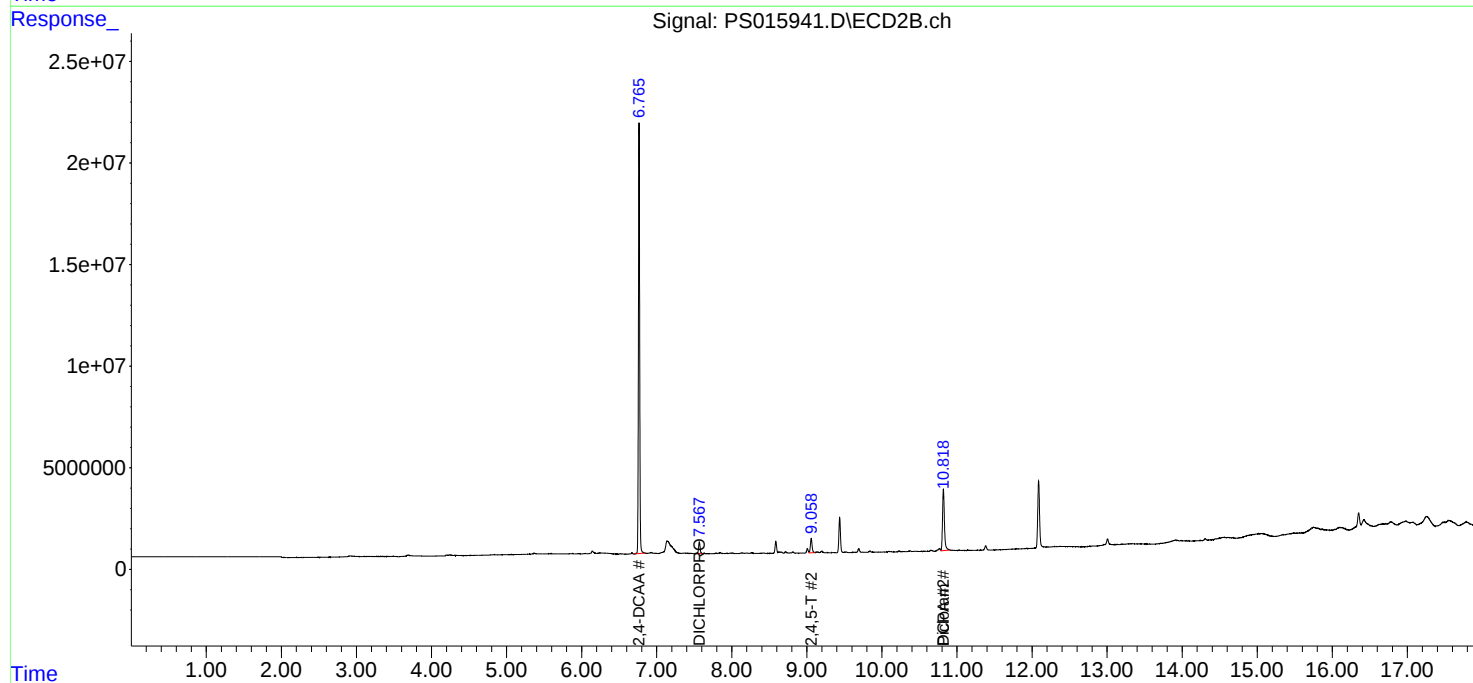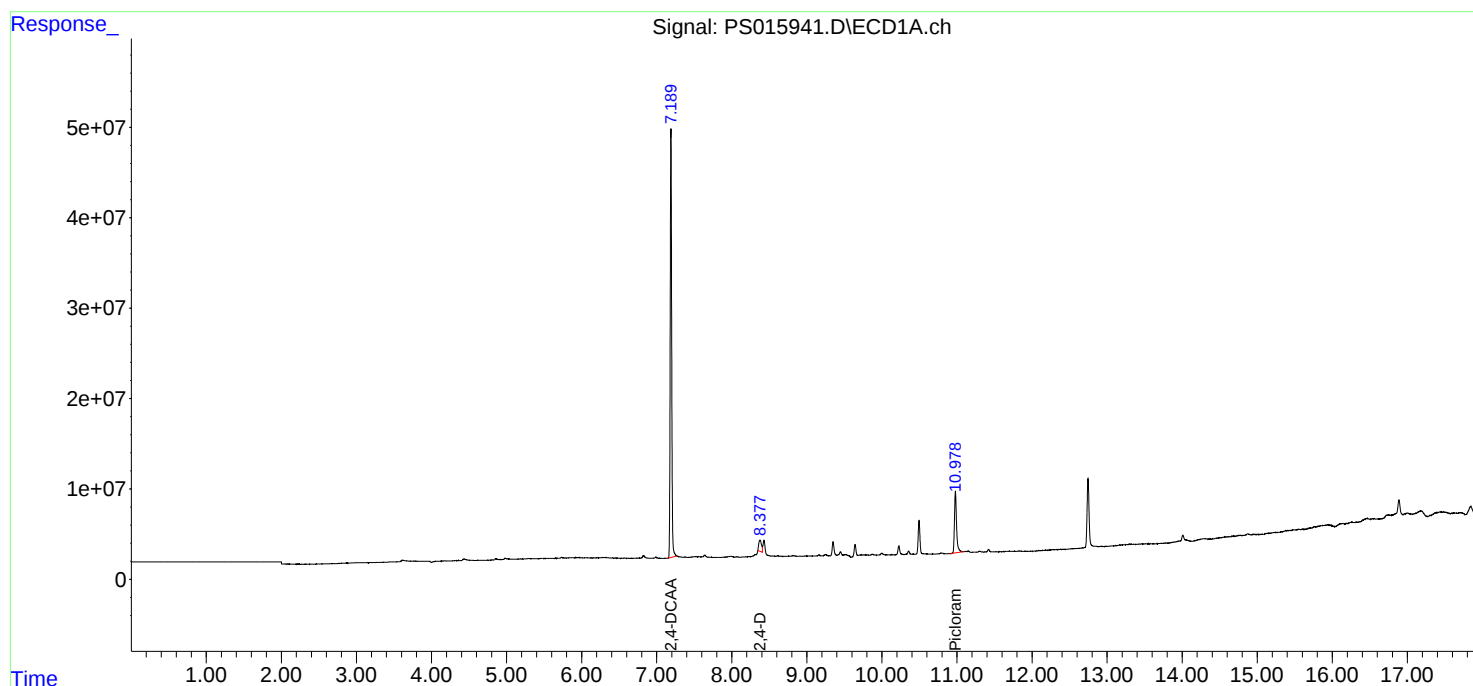


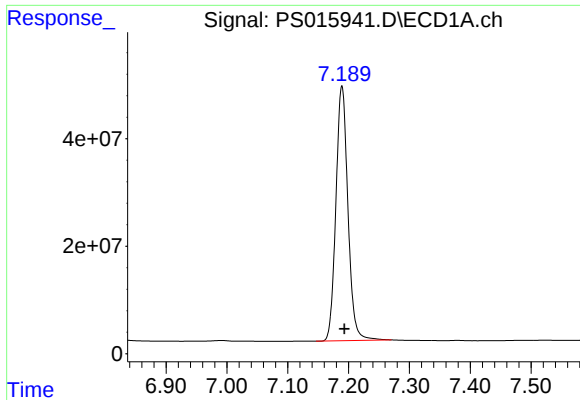

#4 2,4-DCAA


R.T.: 7.189 min
Delta R.T.: -0.004 min
Response: 651700756
Conc: 392.25 ng/ml

Instrument :
ECD_S
ClientSampleId :

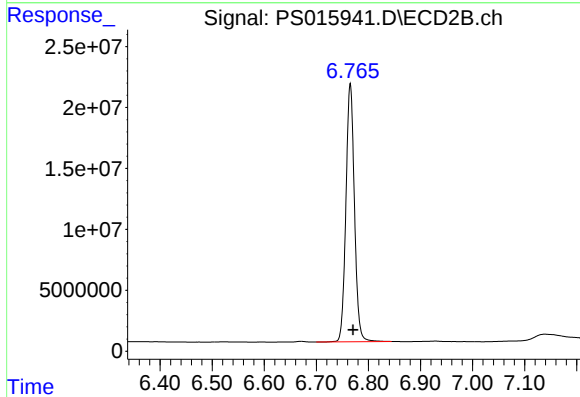


#4 2,4-DCAA

R.T.: 6.765 min
Delta R.T.: -0.005 min
Response: 240786394
Conc: 477.89 ng/ml

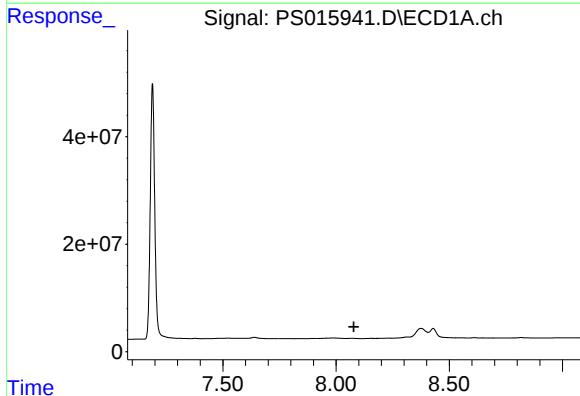


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.079 min
Response: 0
Conc: N.D.

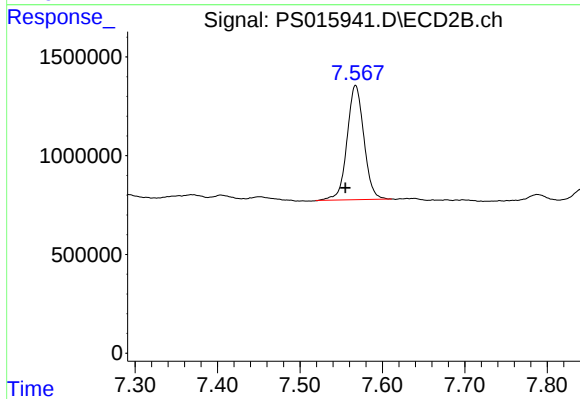

#8 DICHLORPROP


R.T.: 7.568 min
Delta R.T.: 0.012 min
Response: 8190500
Conc: 15.82 ng/ml

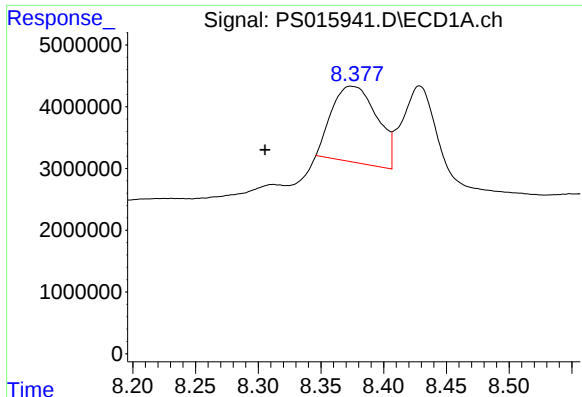

#9 2,4-D


R.T.: 8.374 min
Delta R.T.: 0.069 min
Response: 30986655
Conc: 17.68 ng/ml

Instrument :
ECD_S
ClientSampleId :

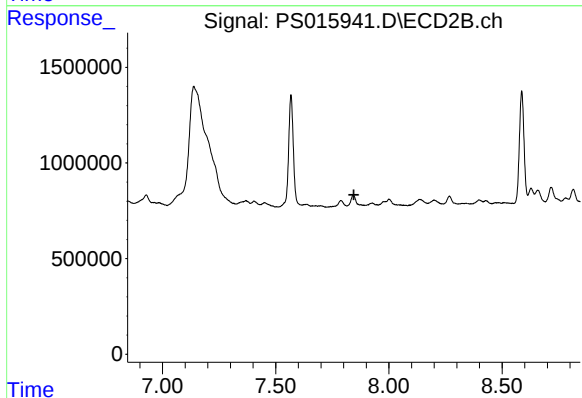


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.845 min
Response: 0
Conc: N.D.

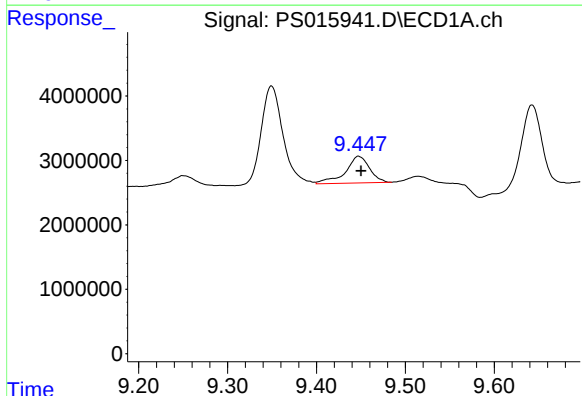


#12 2,4,5-T

R.T.: 9.448 min
Delta R.T.: -0.002 min
Response: 7823555
Conc: N.D.

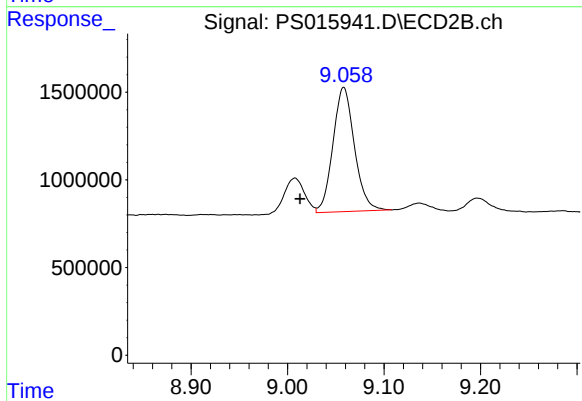

#12 2,4,5-T


R.T.: 9.058 min
Delta R.T.: 0.045 min
Response: 10969431
Conc: 3.89 ng/ml

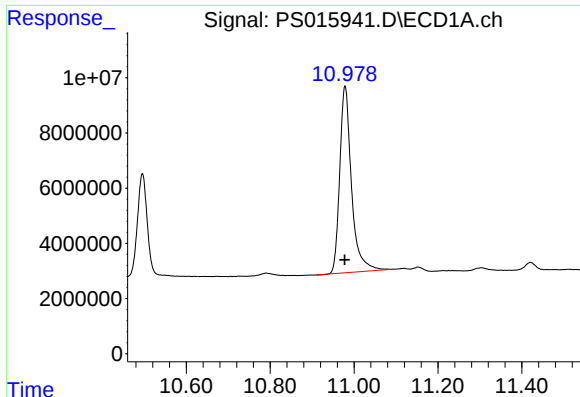

#15 Picloram


R.T.: 10.979 min
Delta R.T.: 0.000 min
Response: 131545137
Conc: 9.62 ng/ml

Instrument :
ECD_S
ClientSampleId :

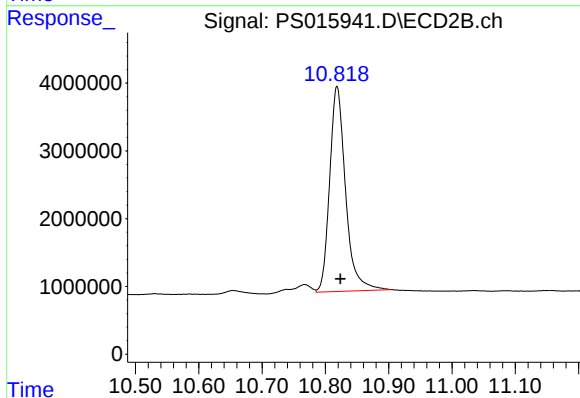


#15 Picloram

R.T.: 10.818 min
Delta R.T.: -0.006 min
Response: 52684980
Conc: 12.53 ng/ml

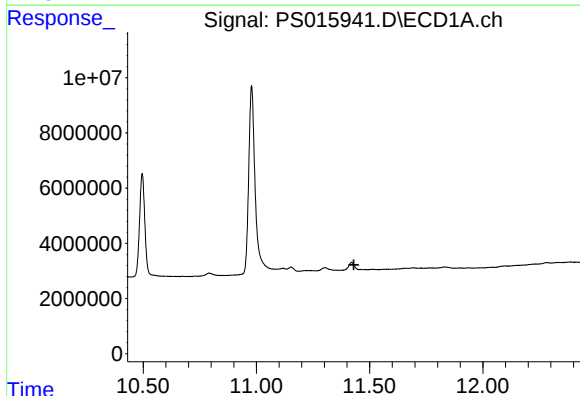

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.431 min
Response: 0
Conc: N.D.

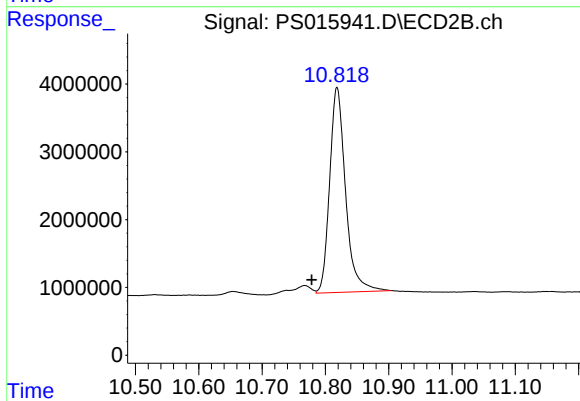

#16 DCPA

R.T.: 10.818 min
Delta R.T.: 0.040 min
Response: 52684980
Conc: 12.53 ng/ml