

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062822\
 Data File : PS019819.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jun 2022 09:13
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 12 03:46:31 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062722.M
 Quant Title : 8080.M
 QLast Update : Mon Jun 27 17:26:48 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.197	6.780	1432.0E6	486.1E6	552.118	598.530
Target Compounds							
1) T	Dalapon	3.046	0.000	1070513	0	<MDL	N.D. #
2) T	3,5-DICHL...	6.438	0.000	352671	0	<MDL	N.D. #
7) T	MCPA	7.656f	0.000	3212968	0	<MDL	N.D. #
8) T	DICHLORPROP	8.089	7.578	1056200	495609	<MDL	<MDL #
9) T	2,4-D	0.000	7.918f	0	1199940	N.D.	1.065
10) T	Pentachlo...	8.615	8.283	8327174	2790217	<MDL	<MDL #
11) T	2,4,5-TP ...	9.175	8.651	6885544	2717281	<MDL	<MDL #
12) T	2,4,5-T	9.403f	9.051	183.3E6	1987723	9.962	<MDL #
13) T	2,4-DB	9.986	9.563	485174	328751	<MDL	<MDL #
14) T	DINOSEB	0.000	9.853	0	1955401	N.D.	<MDL
15) T	Picloram	10.974	10.869	3629900	133.1E6	<MDL	20.464 #
16) T	DCPA	11.422	10.778	14940449	6244872	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062822\
Data File : PS019819.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jun 2022 09:13
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 12 03:46:31 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062722.M
Quant Title : 8080.M
QLast Update : Mon Jun 27 17:26:48 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

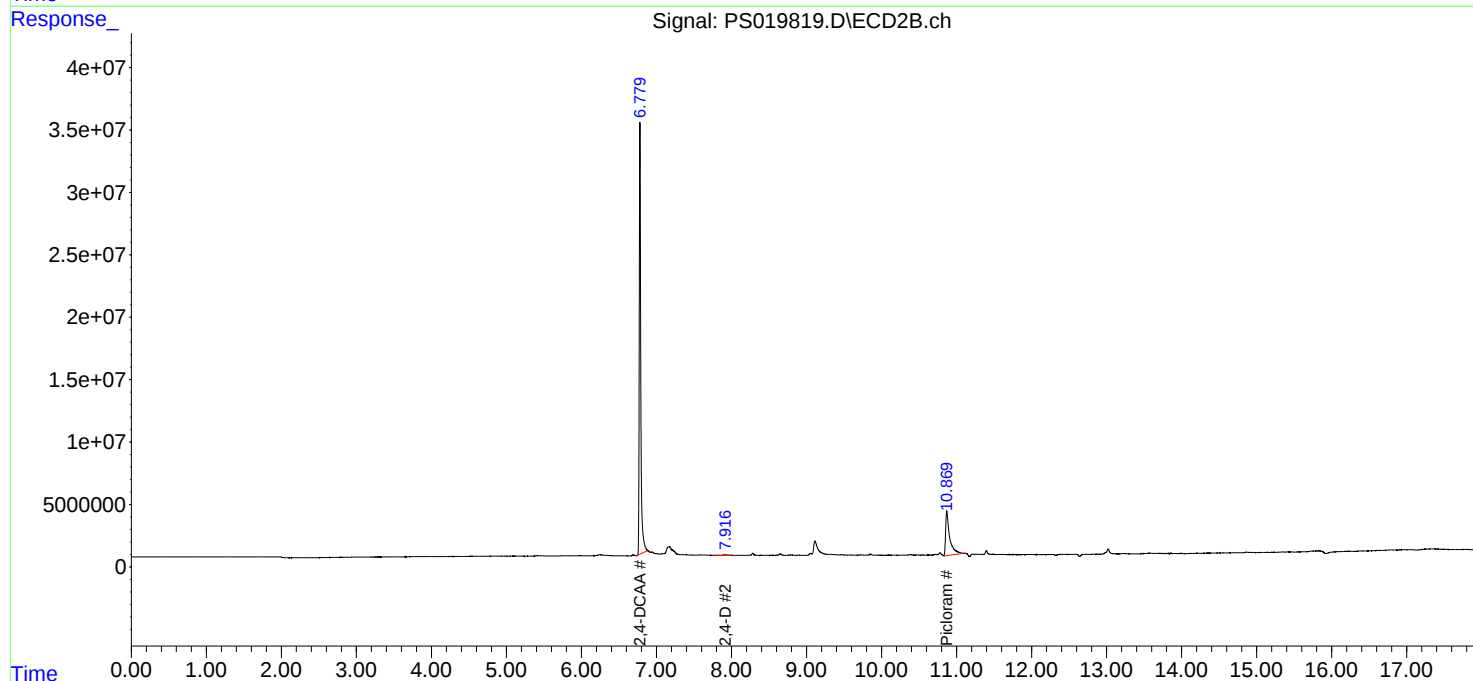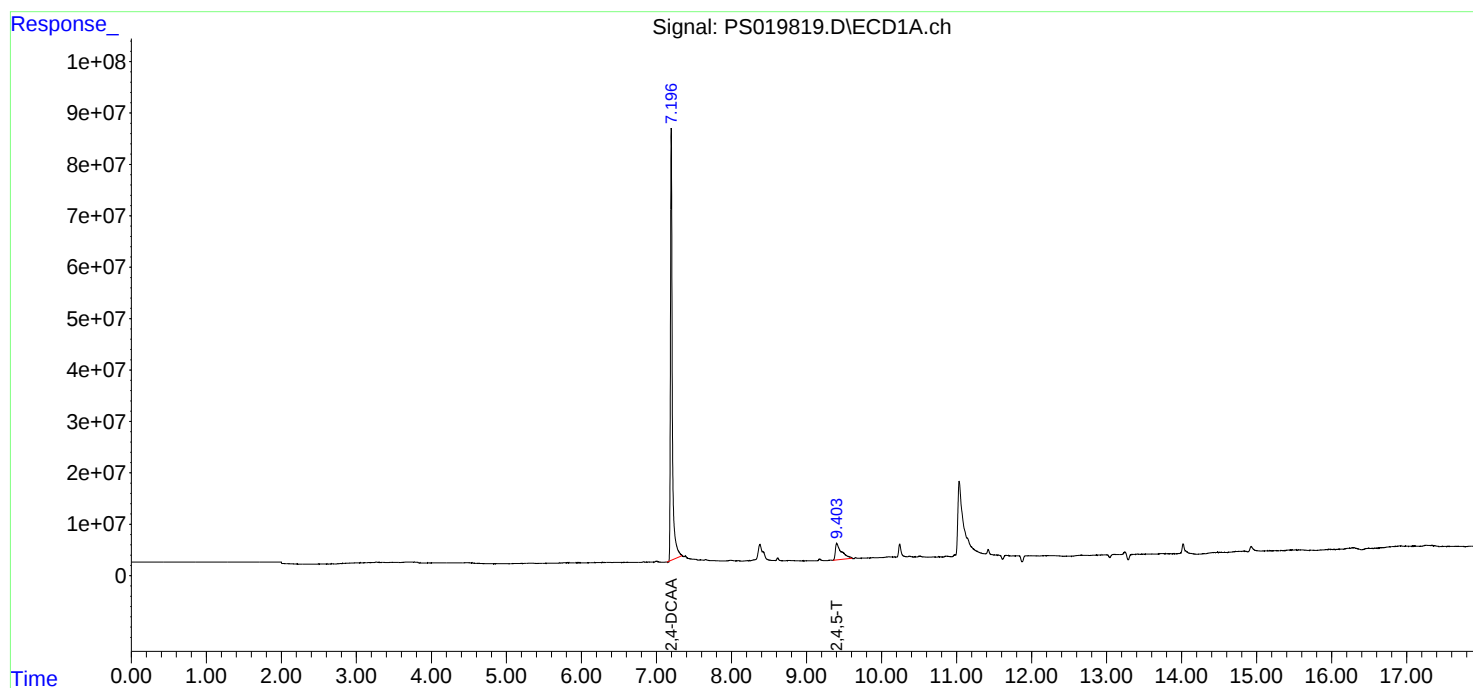


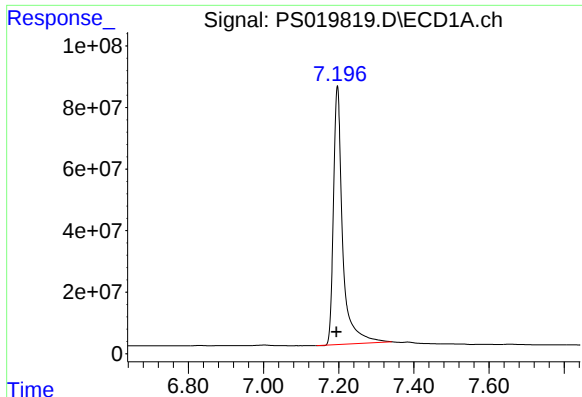

#4 2,4-DCAA


R.T.: 7.197 min
Delta R.T.: 0.003 min
Response: 1432001007
Conc: 552.12 ng/ml

Instrument :
ECD_S
ClientSampleId :

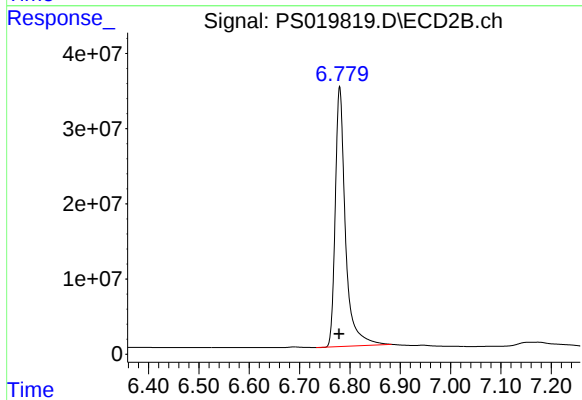


#4 2,4-DCAA

R.T.: 6.780 min
Delta R.T.: 0.001 min
Response: 486093586
Conc: 598.53 ng/ml

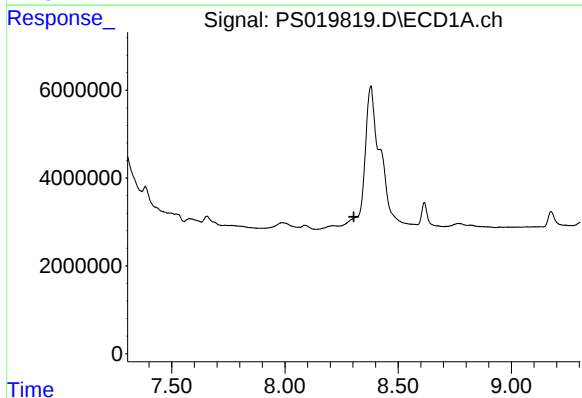


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 8.304 min
Response: 0
Conc: N.D.

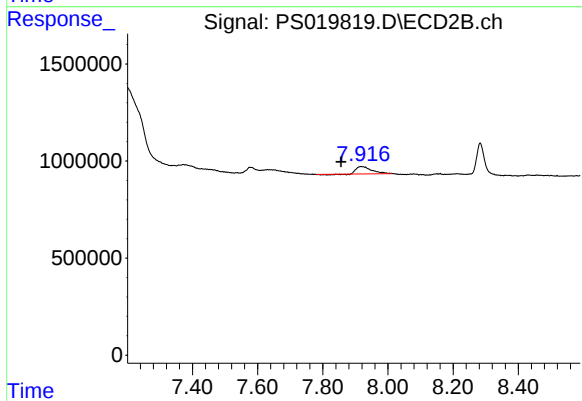

#9 2,4-D


R.T.: 7.918 min
Delta R.T.: 0.062 min
Response: 1199940
Conc: 1.07 ng/ml

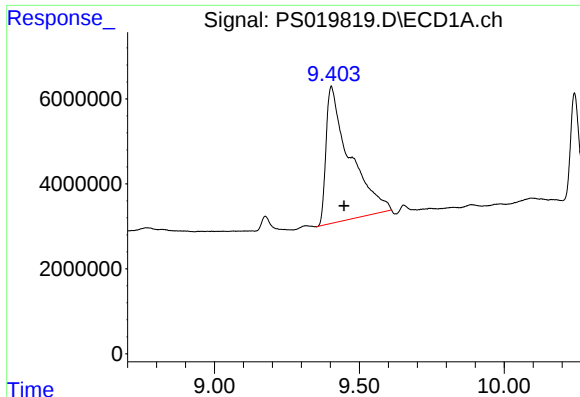

#12 2,4,5-T


R.T.: 9.403 min
Delta R.T.: -0.044 min
Response: 183310361
Conc: 9.96 ng/ml

Instrument :
ECD_S
ClientSampleId :

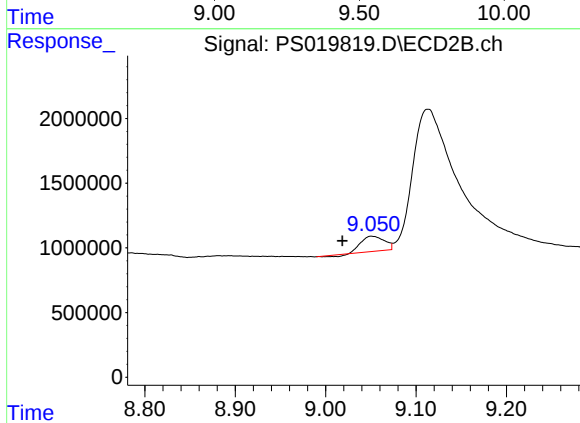


#12 2,4,5-T

R.T.: 9.051 min
Delta R.T.: 0.033 min
Response: 1987723
Conc: N.D.

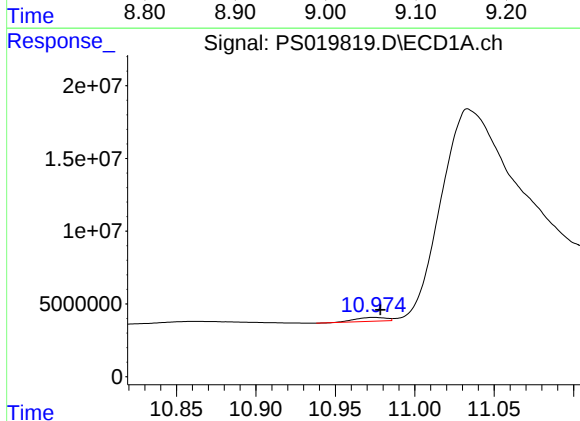

#15 Picloram

R.T.: 10.974 min
Delta R.T.: -0.004 min
Response: 3629900
Conc: N.D.

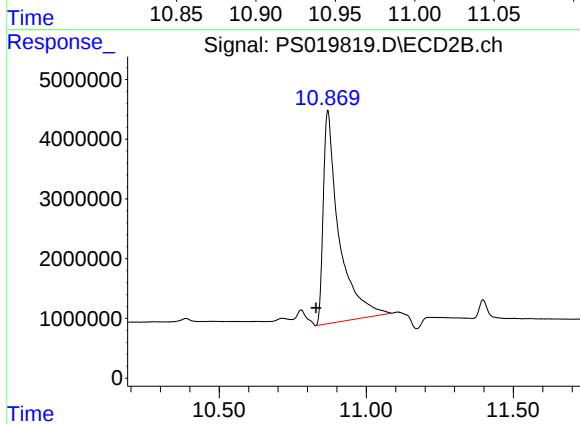

#15 Picloram

R.T.: 10.869 min
Delta R.T.: 0.040 min
Response: 133086570
Conc: 20.46 ng/ml