

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062822\
 Data File : PS019831.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jun 2022 14:06
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 12 03:50:11 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062722.M
 Quant Title : 8080.M
 QLast Update : Mon Jun 27 17:26:48 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.195	6.780	1430.0E6	499.3E6	551.357	614.810
Target Compounds							
1) T	Dalapon	3.049	0.000	911998	0	<MDL	N.D. #
2) T	3,5-DICHL...	6.454f	5.988	3296997	222308	<MDL	<MDL #
5) T	DICAMBA	0.000	7.006f	0	1178471	N.D.	<MDL
6) T	MCP	0.000	7.006	0	1178471	N.D.	<MDL
7) T	MCPA	7.693	0.000	3884408	0	<MDL	N.D. #
8) T	DICHLORPROP	0.000	7.574	0	36504	N.D.	<MDL
9) T	2,4-D	0.000	7.825	0	300424	N.D.	<MDL
10) T	Pentachlo...	8.613	8.283	3661394	1578225	<MDL	<MDL #
11) T	2,4,5-TP ...	9.171	8.647	2319184	568141	<MDL	<MDL #
12) T	2,4,5-T	9.427	9.050	16643643	601885	<MDL	<MDL #
13) T	2,4-DB	9.974	9.464f	10049766	2354918	2.511	3.626 #
14) T	DINOSEB	11.131	9.853	20599360	1391412	1.267	<MDL #
15) T	Picloram	10.967	10.881f	34250354	16085723	1.098	2.473 #
16) T	DCPA	11.422	10.777	4551707	9500511	<MDL	1.466 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062822\
Data File : PS019831.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jun 2022 14:06
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 12 03:50:11 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062722.M
Quant Title : 8080.M
QLast Update : Mon Jun 27 17:26:48 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

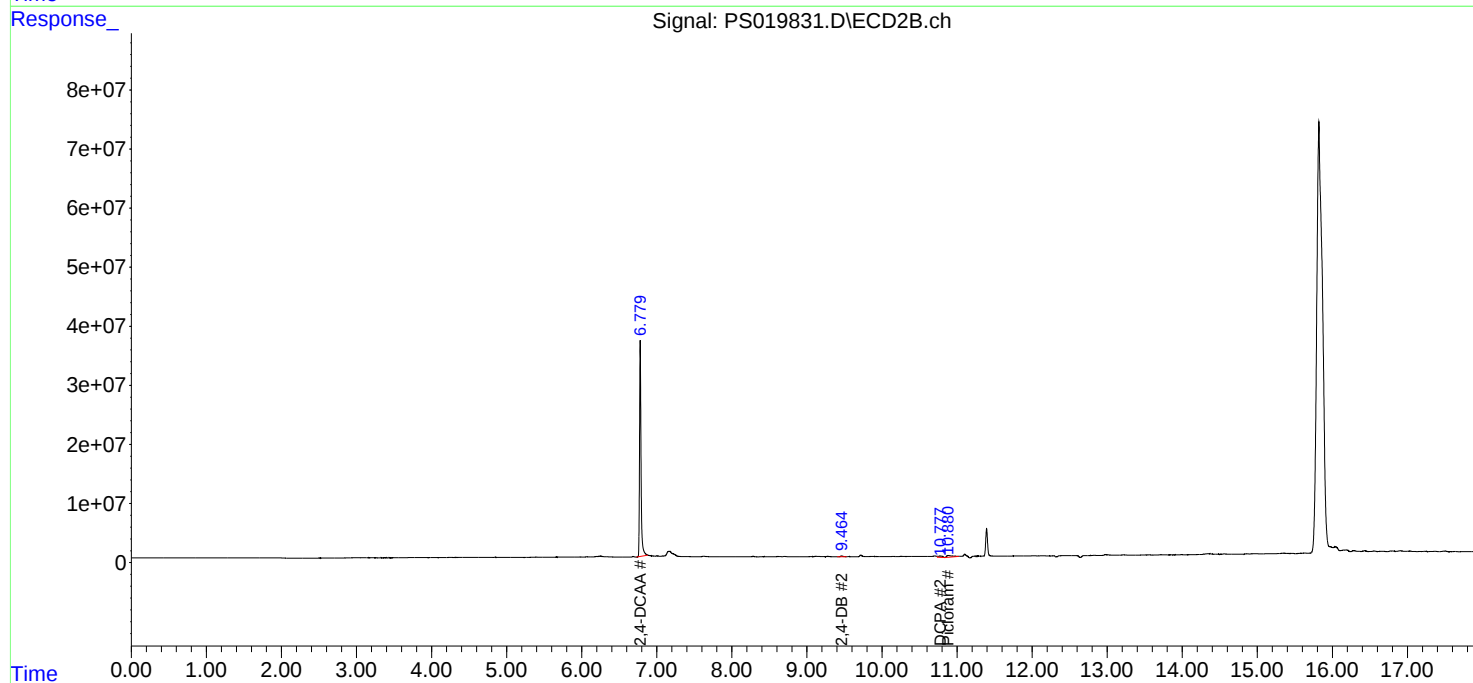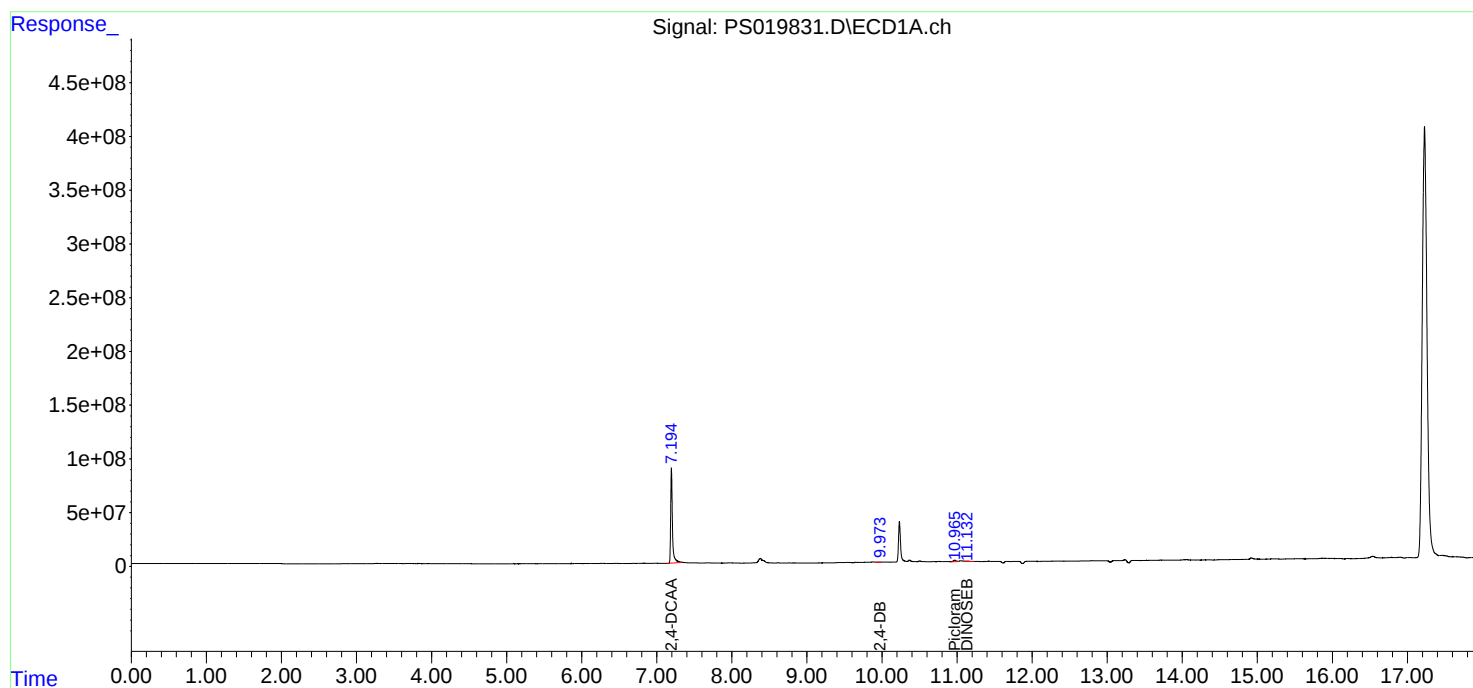


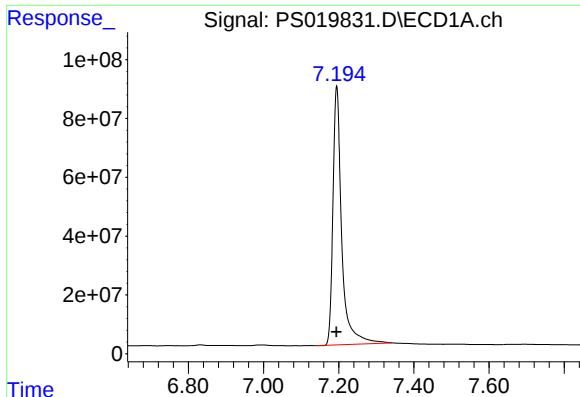

#4 2,4-DCAA


R.T.: 7.195 min
Delta R.T.: 0.000 min
Response: 1430028408
Conc: 551.36 ng/ml

Instrument :
ECD_S
ClientSampleId :

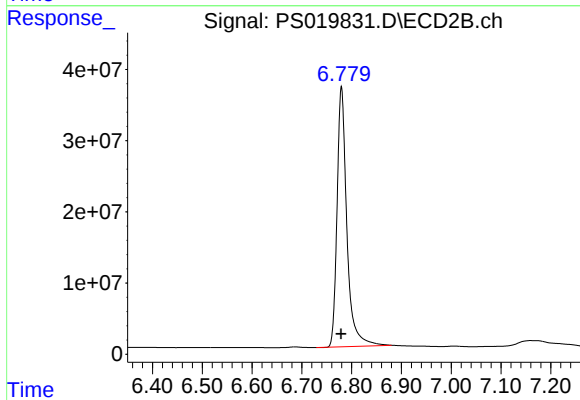


#4 2,4-DCAA

R.T.: 6.780 min
Delta R.T.: 0.000 min
Response: 499315668
Conc: 614.81 ng/ml

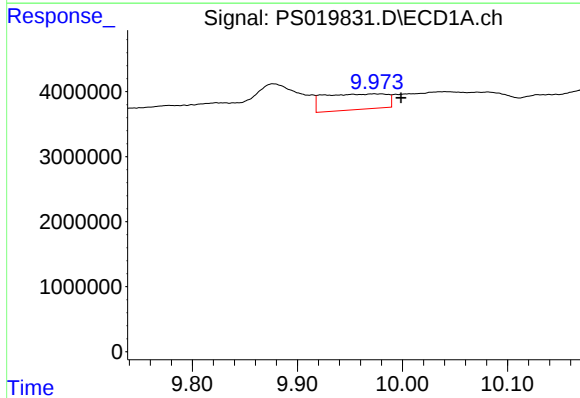


#13 2,4-DB

R.T.: 9.974 min
Delta R.T.: -0.025 min
Response: 10049766
Conc: 2.51 ng/ml

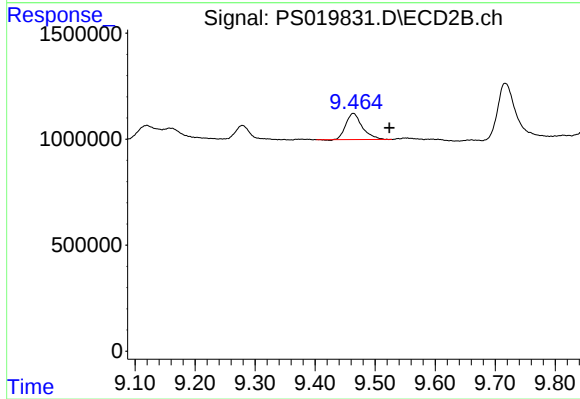

#13 2,4-DB


R.T.: 9.464 min
Delta R.T.: -0.060 min
Response: 2354918
Conc: 3.63 ng/ml

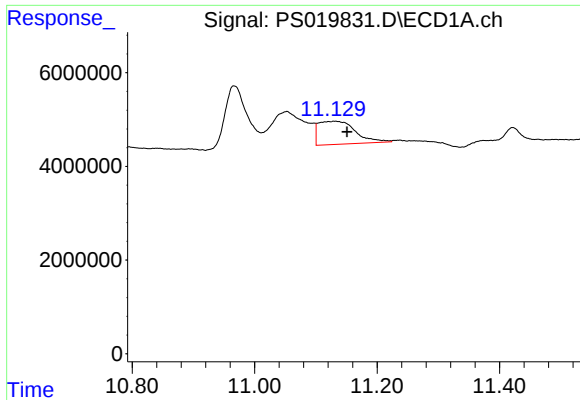

#14 DINOSEB


R.T.: 11.131 min
Delta R.T.: -0.020 min
Response: 20599360
Conc: 1.27 ng/ml

Instrument :
ECD_S
ClientSampleId :

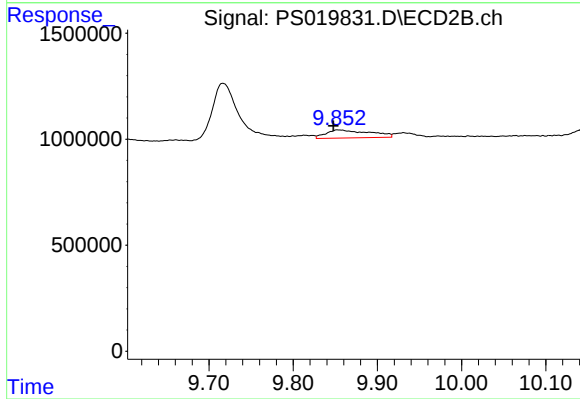


#14 DINOSEB

R.T.: 9.853 min
Delta R.T.: 0.005 min
Response: 1391412
Conc: N.D.

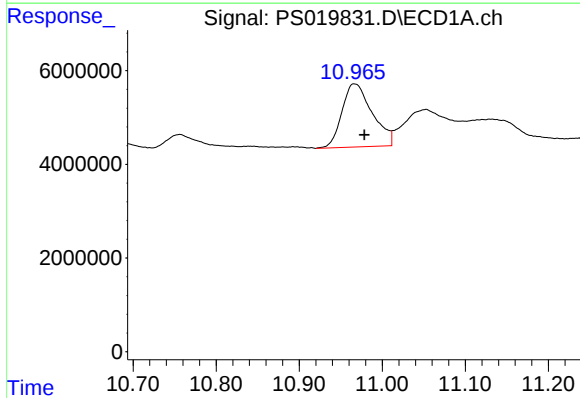


#15 Picloram

R.T.: 10.967 min
Delta R.T.: -0.011 min
Response: 34250354
Conc: 1.10 ng/ml

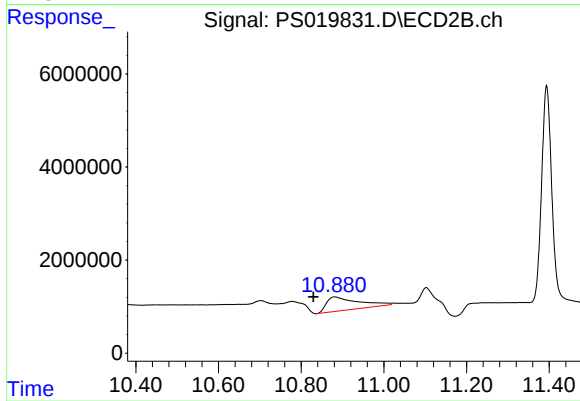

#15 Picloram


R.T.: 10.881 min
Delta R.T.: 0.052 min
Response: 16085723
Conc: 2.47 ng/ml

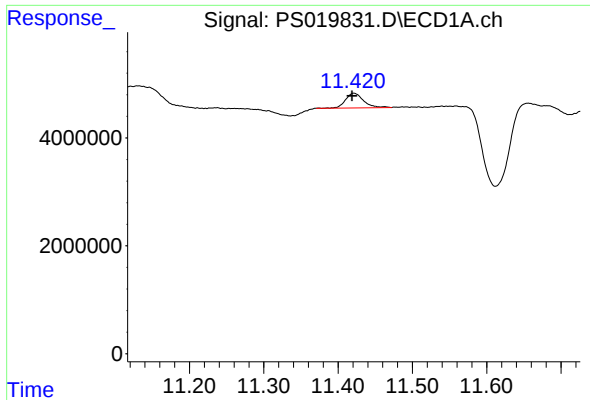

#16 DCPA

R.T.: 11.422 min
Delta R.T.: 0.003 min
Response: 4551707
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

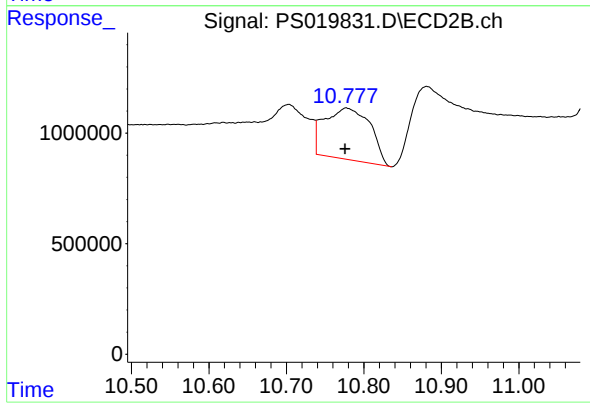

#16 DCPA

R.T.: 10.777 min
Delta R.T.: 0.001 min
Response: 9500511
Conc: 1.47 ng/ml