

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062822\
 Data File : PS019820.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jun 2022 09:37
 Operator : AJ\MA
 Sample : HSTDCCC750 (Sig #1); HSTDICC200 (Sig #2)
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HSTDCCC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 12 03:46:44 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062722.M
 Quant Title : 8080.M
 QLast Update : Mon Jun 27 17:26:48 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.194	6.780	1939.5E6	628.0E6	747.782	773.219
Target Compounds							
1) T	Dalapon	3.010	2.522	3589.8E6	716.2E6	740.599	674.806
2) T	3,5-DICHL...	6.409	5.960	2361.1E6	912.4E6	689.296	713.975
3) T	4-Nitroph...	7.027	6.399	766.5E6	309.5E6	720.101	715.624
5) T	DICAMBA	7.384	6.944	7243.5E6	2658.0E6	705.922	728.624
6) T	MCPD	7.553	7.041	577.7E6	209.1E6	72.004	72.840
7) T	MCPA	7.702	7.254	822.1E6	291.2E6	70.155	71.937
8) T	DICHLORPROP	8.075	7.563	1913.2E6	675.0E6	706.630	717.486
9) T	2,4-D	8.305	7.856	2175.8E6	812.7E6	732.542	721.292
10) T	Pentachlo...	8.611	8.280	26020.7E6	8994.5E6	720.537	728.466
11) T	2,4,5-TP ...	9.161	8.641	11487.2E6	3909.8E6	718.142	737.745
12) T	2,4,5-T	9.446	9.019	13246.7E6	3656.9E6	719.926	748.539
13) T	2,4-DB	9.999	9.524	2972.5E6	480.6E6	742.823	739.920
14) T	DINOSEB	11.151	9.848	11912.3E6	2669.5E6	732.718	748.961
15) T	Picloram	10.977	10.830	23168.5E6	4822.8E6	742.989	741.561
16) T	DCPA	11.420	10.777	19016.8E6	4796.5E6	737.168	740.110


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062822\
Data File : PS019820.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jun 2022 09:37
Operator : AJ\MA
Sample : HSTDCCC750 (Sig #1); HSTDICC200 (Sig #2)
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 12 03:46:44 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062722.M
Quant Title : 8080.M
QLast Update : Mon Jun 27 17:26:48 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

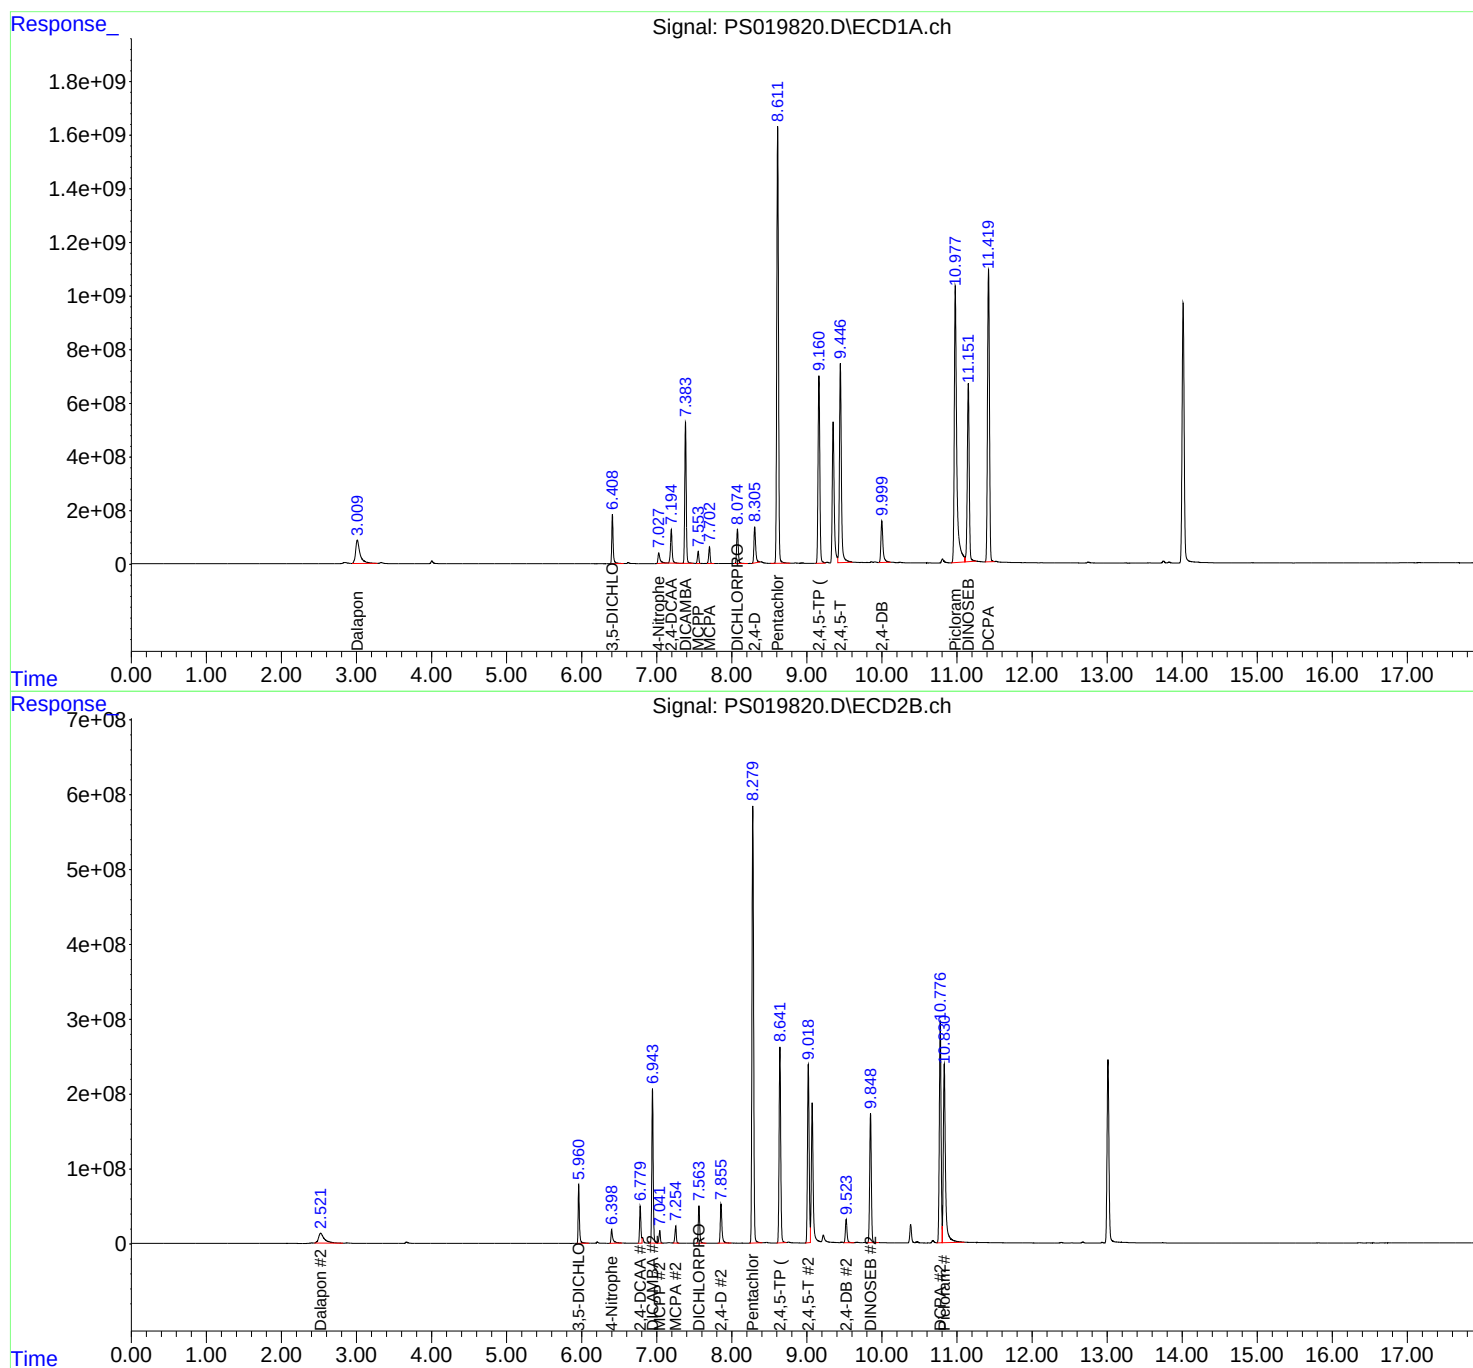


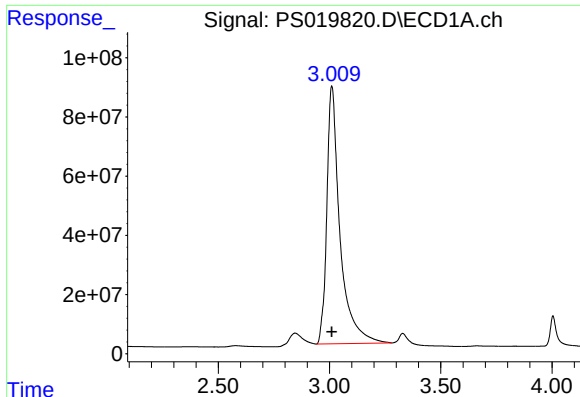

#1 Dalapon


R.T.: 3.010 min
Delta R.T.: 0.000 min
Response: 3589842625
Conc: 740.60 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

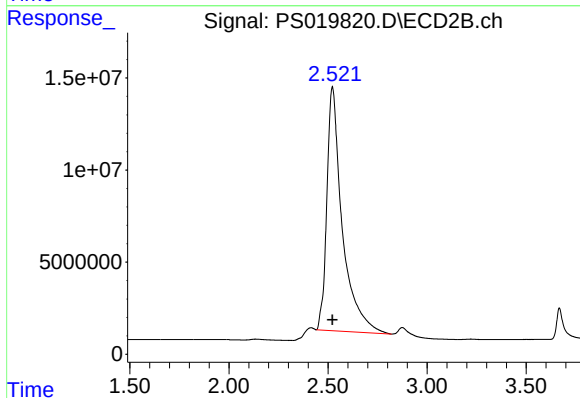


#1 Dalapon

R.T.: 2.522 min
Delta R.T.: 0.000 min
Response: 716207763
Conc: 674.81 ng/ml

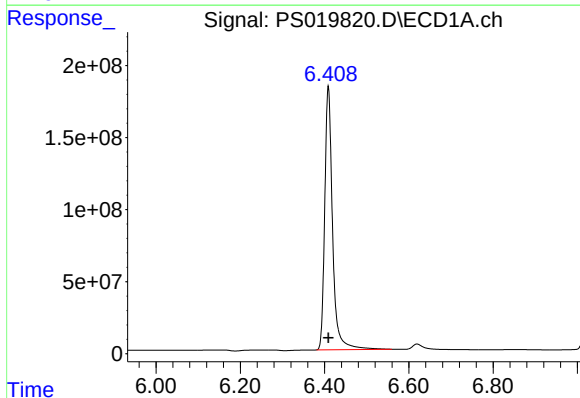


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.409 min
Delta R.T.: 0.000 min
Response: 2361106130
Conc: 689.30 ng/ml

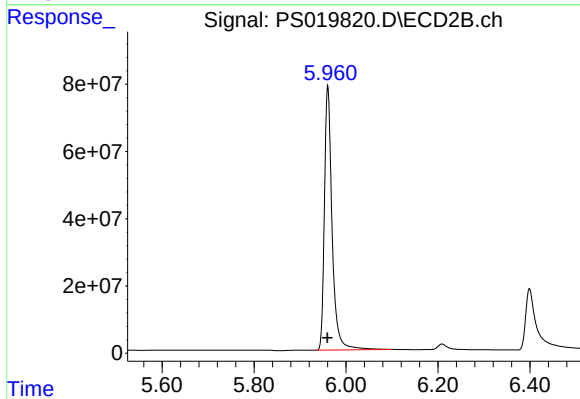

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.960 min
Delta R.T.: 0.000 min
Response: 912363753
Conc: 713.97 ng/ml

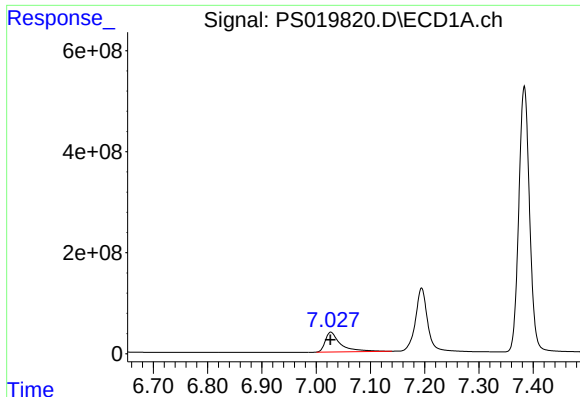

#3 4-Nitrophenol


R.T.: 7.027 min
Delta R.T.: 0.000 min
Response: 766457228
Conc: 720.10 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

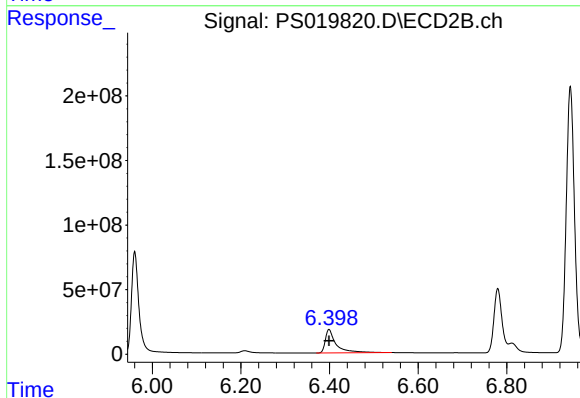


#3 4-Nitrophenol

R.T.: 6.399 min
Delta R.T.: 0.000 min
Response: 309517523
Conc: 715.62 ng/ml

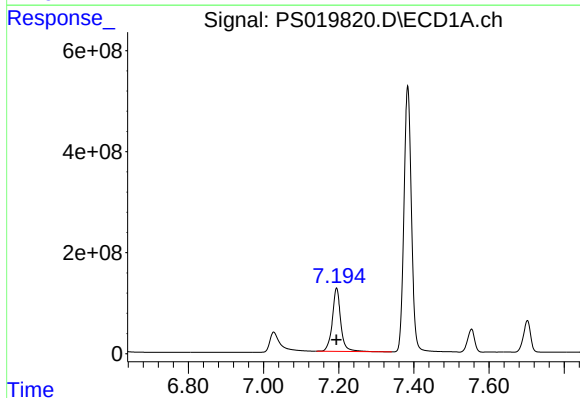


#4 2,4-DCAA

R.T.: 7.194 min
Delta R.T.: 0.000 min
Response: 1939486110
Conc: 747.78 ng/ml

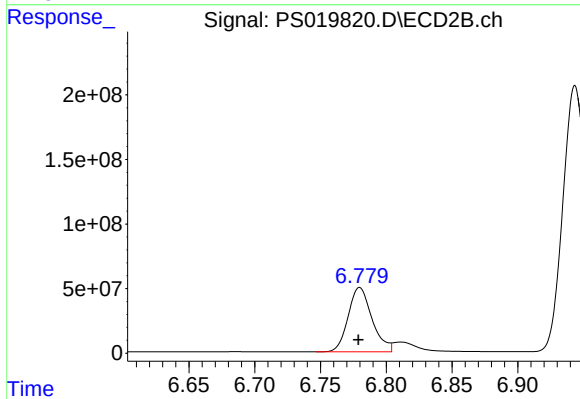

#4 2,4-DCAA


R.T.: 6.780 min
Delta R.T.: 0.000 min
Response: 627966584
Conc: 773.22 ng/ml

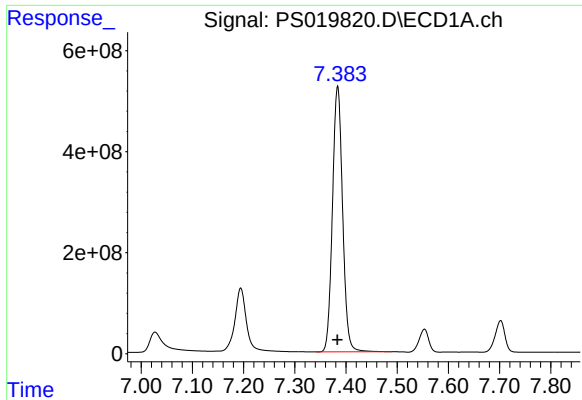

#5 DICAMBA


R.T.: 7.384 min
Delta R.T.: 0.000 min
Response: 7243481476
Conc: 705.92 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

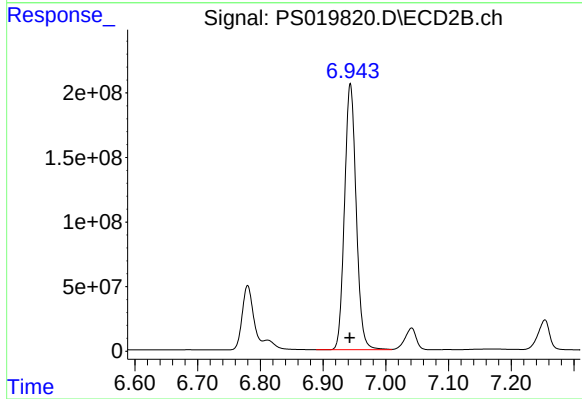


#5 DICAMBA

R.T.: 6.944 min
Delta R.T.: 0.000 min
Response: 2657999150
Conc: 728.62 ng/ml

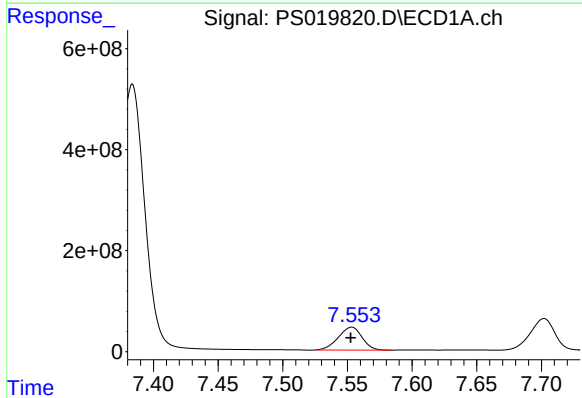


#6 MCP

R.T.: 7.553 min
Delta R.T.: 0.000 min
Response: 577689554
Conc: 72.00 ug/ml

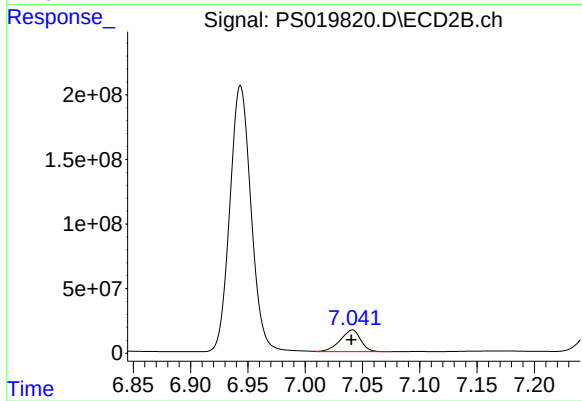

#6 MCP


R.T.: 7.041 min
Delta R.T.: 0.000 min
Response: 209080685
Conc: 72.84 ug/ml

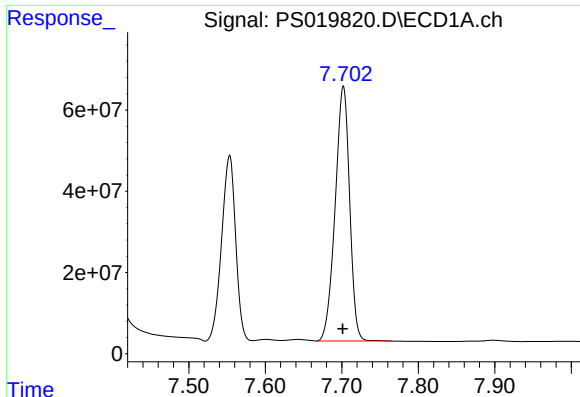

#7 MCPA


R.T.: 7.702 min
Delta R.T.: 0.000 min
Response: 822068757
Conc: 70.15 ug/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

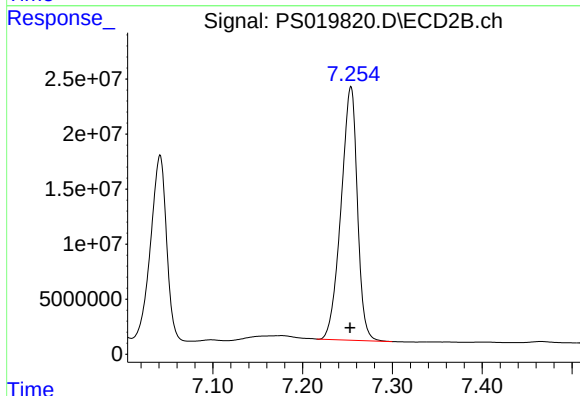


#7 MCPA

R.T.: 7.254 min
Delta R.T.: 0.000 min
Response: 291173611
Conc: 71.94 ug/ml

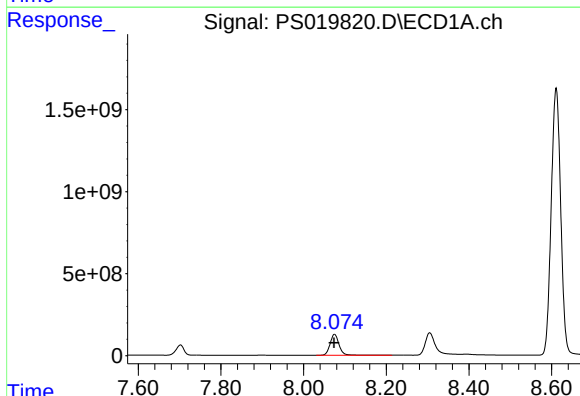


#8 DICHLORPROP

R.T.: 8.075 min
Delta R.T.: 0.000 min
Response: 1913191689
Conc: 706.63 ng/ml

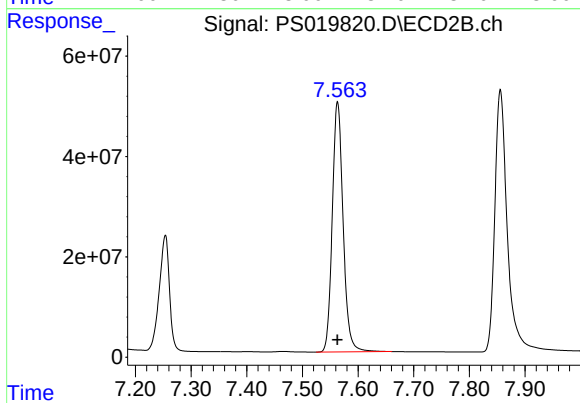

#8 DICHLORPROP


R.T.: 7.563 min
Delta R.T.: 0.000 min
Response: 674953624
Conc: 717.49 ng/ml

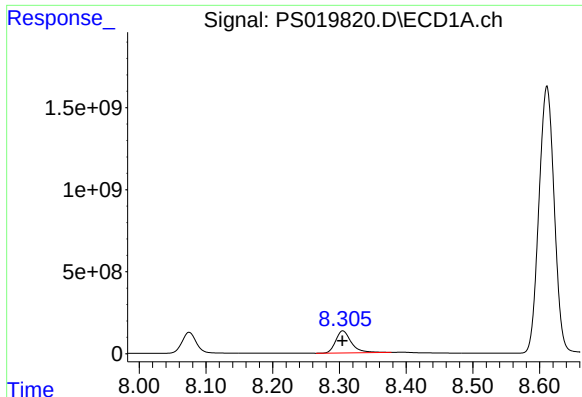

#9 2,4-D


R.T.: 8.305 min
Delta R.T.: 0.000 min
Response: 2175750219
Conc: 732.54 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

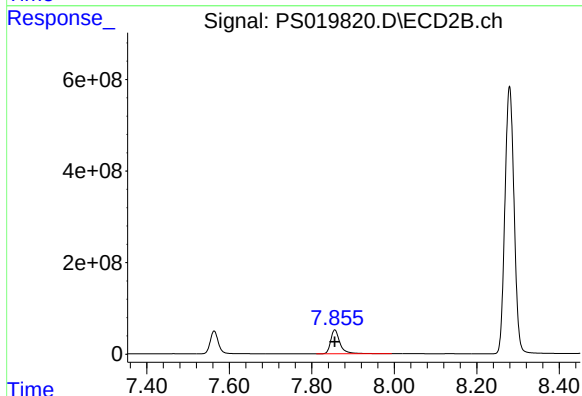


#9 2,4-D

R.T.: 7.856 min
Delta R.T.: 0.000 min
Response: 812681655
Conc: 721.29 ng/ml

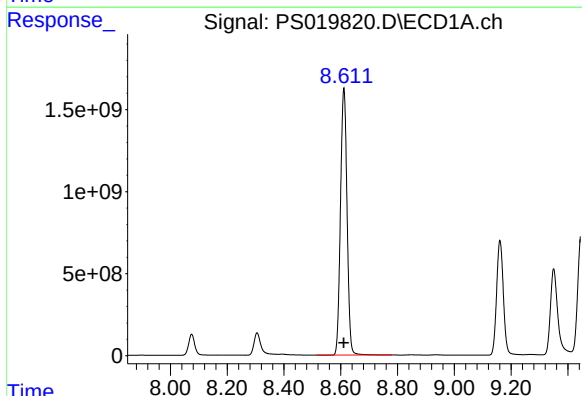


#10 Pentachlorophenol

R.T.: 8.611 min
Delta R.T.: 0.000 min
Response: 26020744911
Conc: 720.54 ng/ml

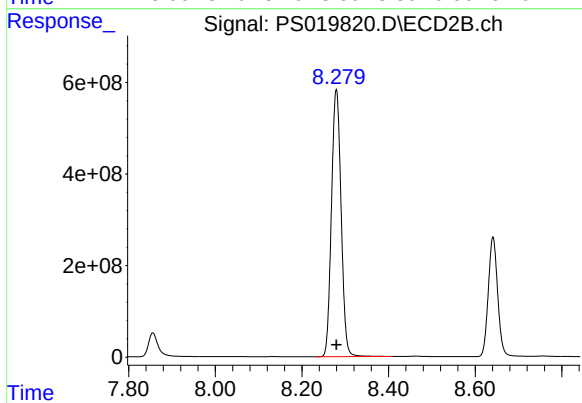

#10 Pentachlorophenol


R.T.: 8.280 min
Delta R.T.: 0.000 min
Response: 8994510624
Conc: 728.47 ng/ml

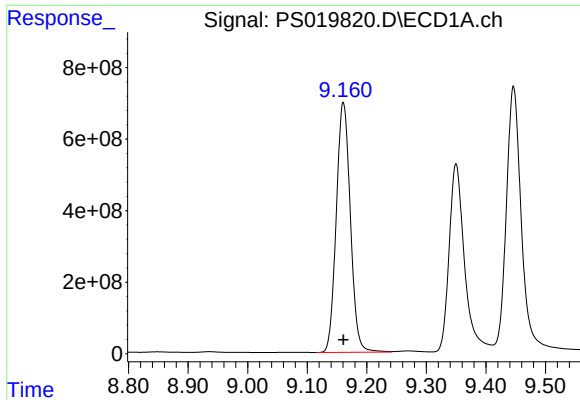

#11 2,4,5-TP (SILVEX)


R.T.: 9.161 min
Delta R.T.: 0.000 min
Response: 11487156628
Conc: 718.14 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

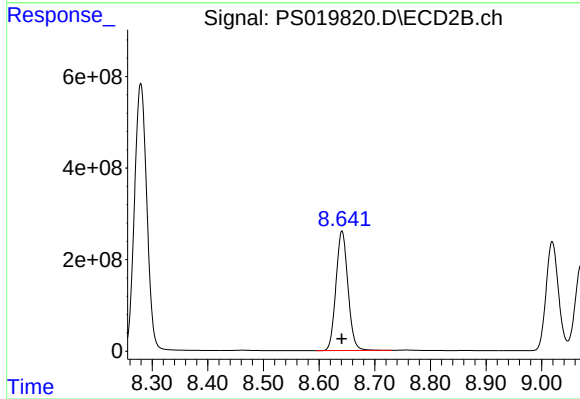


#11 2,4,5-TP (SILVEX)

R.T.: 8.641 min
Delta R.T.: 0.000 min
Response: 3909769507
Conc: 737.74 ng/ml

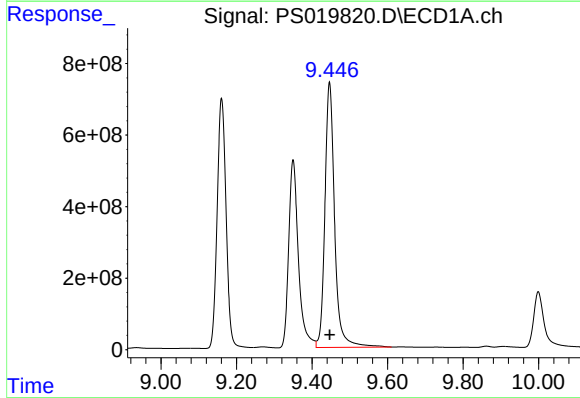


#12 2,4,5-T

R.T.: 9.446 min
Delta R.T.: 0.000 min
Response: 13246676507
Conc: 719.93 ng/ml

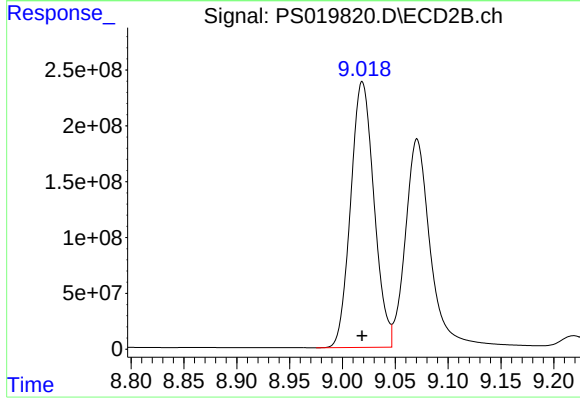

#12 2,4,5-T


R.T.: 9.019 min
Delta R.T.: 0.000 min
Response: 3656859286
Conc: 748.54 ng/ml

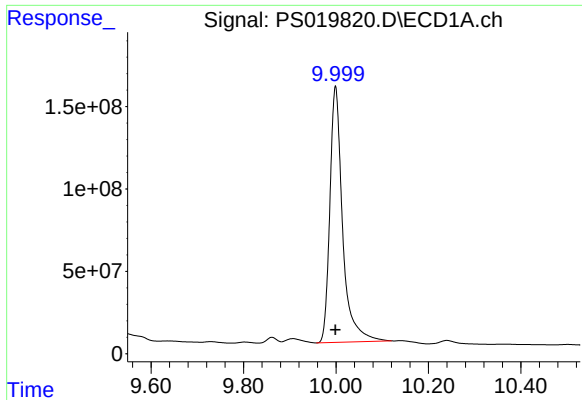

#13 2,4-DB


R.T.: 9.999 min
Delta R.T.: 0.000 min
Response: 2972506223
Conc: 742.82 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

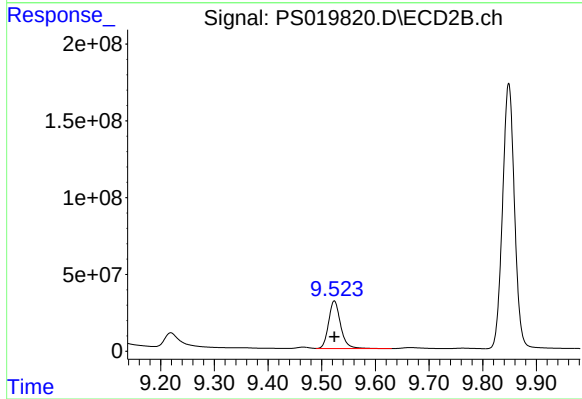


#13 2,4-DB

R.T.: 9.524 min
Delta R.T.: 0.000 min
Response: 480554981
Conc: 739.92 ng/ml

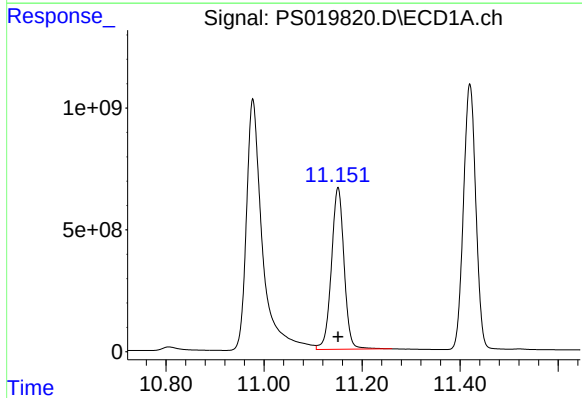


#14 DINOSEB

R.T.: 11.151 min
Delta R.T.: 0.000 min
Response: 11912276876
Conc: 732.72 ng/ml

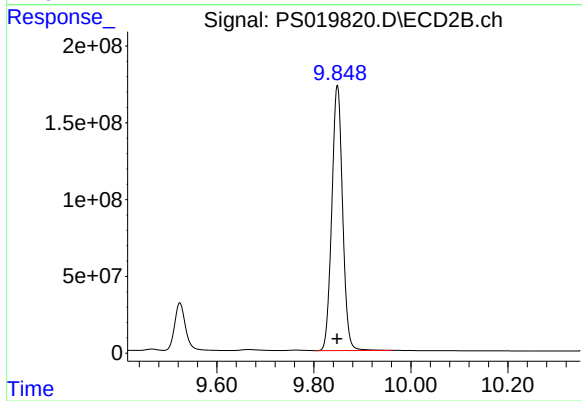

#14 DINOSEB


R.T.: 9.848 min
Delta R.T.: 0.000 min
Response: 2669451799
Conc: 748.96 ng/ml

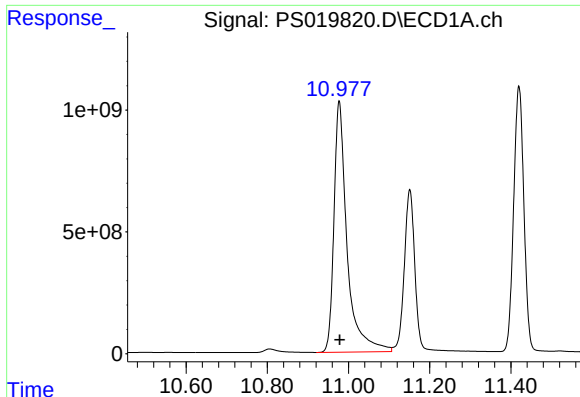

#15 Picloram


R.T.: 10.977 min
Delta R.T.: -0.001 min
Response: 23168513367
Conc: 742.99 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

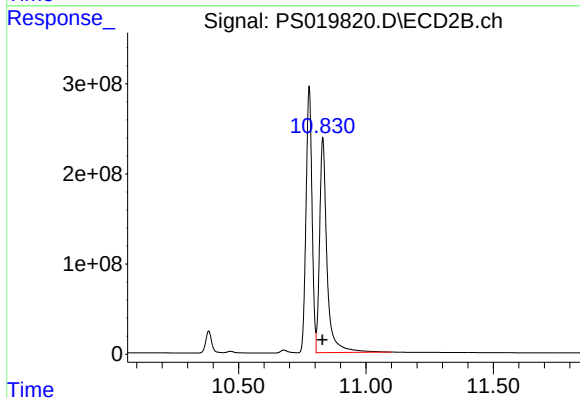


#15 Picloram

R.T.: 10.830 min
Delta R.T.: 0.000 min
Response: 4822816264
Conc: 741.56 ng/ml

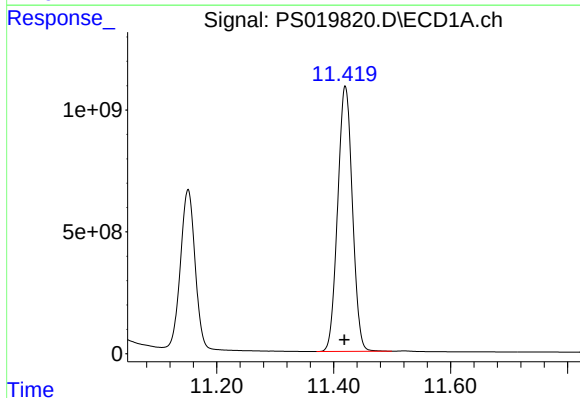

#16 DCPA

R.T.: 11.420 min
Delta R.T.: 0.001 min
Response: 19016845665
Conc: 737.17 ng/ml

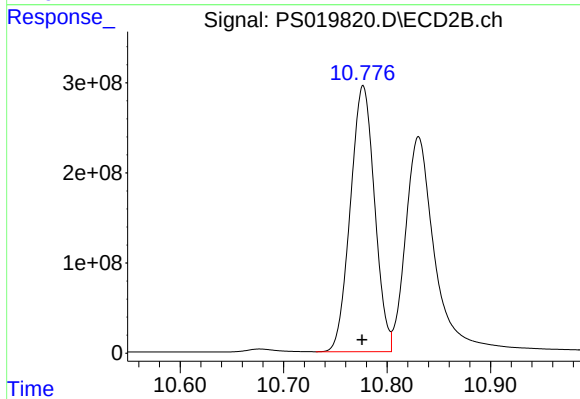

#16 DCPA

R.T.: 10.777 min
Delta R.T.: 0.001 min
Response: 4796524174
Conc: 740.11 ng/ml