

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062823\
 Data File : PS023532.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jun 2023 11:20
 Operator : AR\AJ
 Sample : 03393-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 SF-9

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 28 18:19:16 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS060623.M
 Quant Title : 8080.M
 QLast Update : Tue Jun 06 13:00:04 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.476	6.846	202.5E6	45799885	114.481	80.677 #
Target Compounds							
1) T	Dalapon	2.516	2.540	28548147	42080720	15.613	45.907 #
2) T	3,5-DICHL...	5.852	6.039	873536	855724	<MDL	<MDL #
3) T	4-Nitroph...	6.304	0.000	24766100	0	19.216	N.D. #
5) T	DICAMBA	6.654	7.049	-1763914	2621435	N.D.	1.023
6) T	MCP	6.806	7.097	107.8E6	3460520	19.553	1.936 #
7) T	MCPA	6.944	7.314	27269452	24953836	3.483	9.285 #
8) T	DICHLORPROP	7.254	7.647	27813551	35148779	13.479	56.821 #
9) T	2,4-D	7.438	7.951	4536579	449069	1.857	<MDL #
10) T	Pentachlo...	7.666	8.349	6945823	2896000	<MDL	<MDL #
11) T	2,4,5-TP ...	8.204	8.731	39018436	8797229	3.374	2.636
12) T	2,4,5-T	8.480	9.075	65019578	7058321	5.723	2.302 #
13) T	2,4-DB	8.995	9.598	155.4E6	7357752	66.007	19.843 #
15) T	Picloram	9.876	10.883	43447078	28939049	2.503	6.341 #
16) T	DCPA	10.322	10.883	29900593	28939049	2.145	7.213 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062823\
Data File : PS023532.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jun 2023 11:20
Operator : AR\AJ
Sample : 03393-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
SF-9

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 28 18:19:16 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS060623.M
Quant Title : 8080.M
QLast Update : Tue Jun 06 13:00:04 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

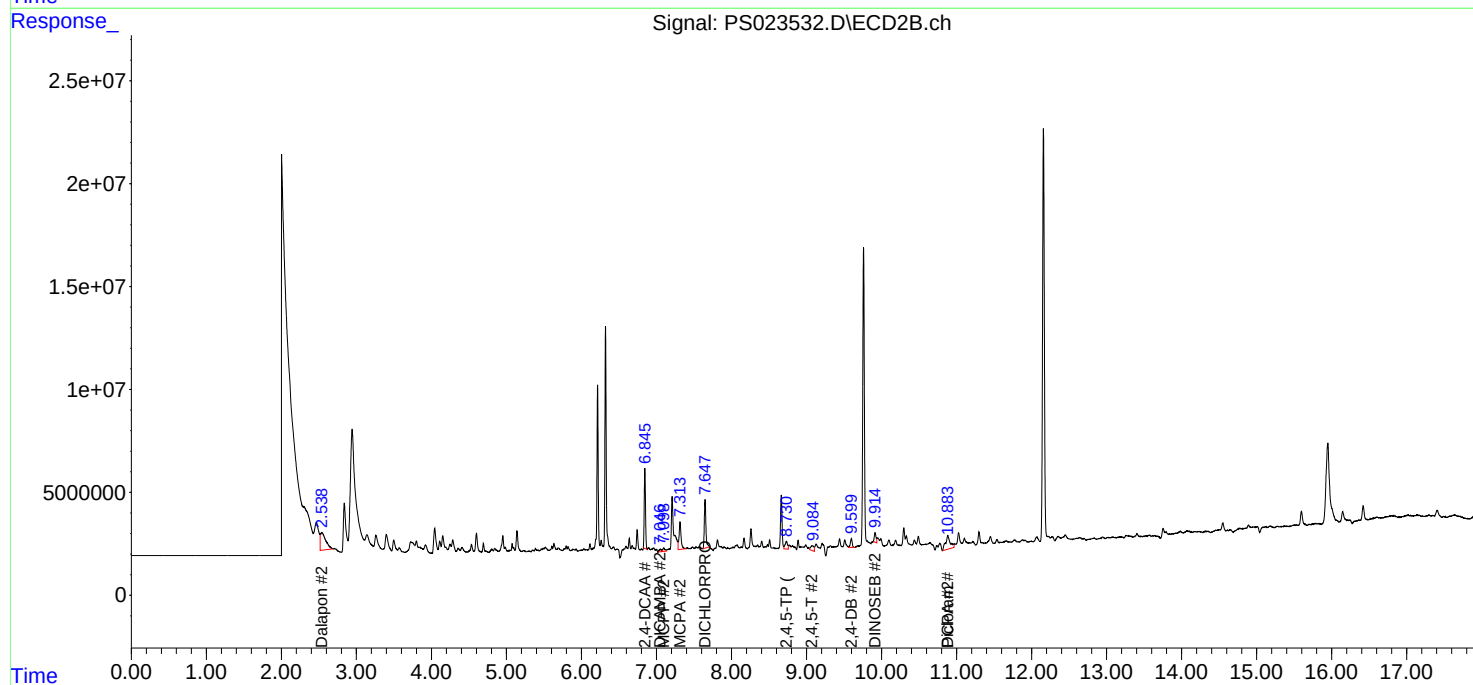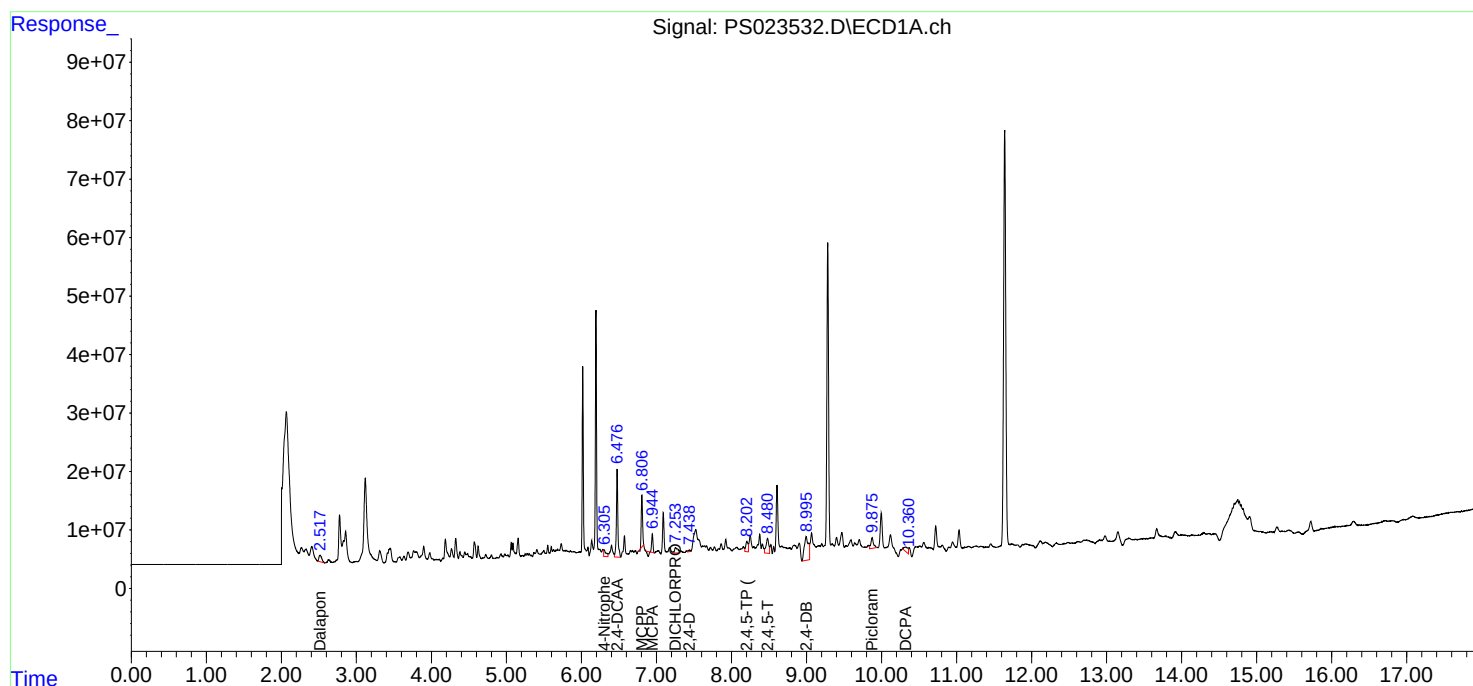


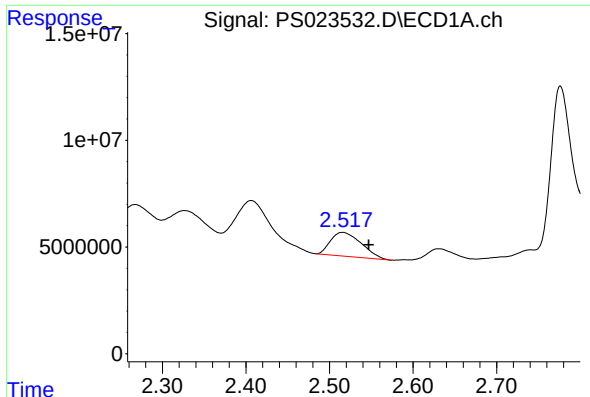

#1 Dalapon


R.T.: 2.516 min
Delta R.T.: -0.031 min
Response: 28548147
Conc: 15.61 ng/ml

Instrument :
ECD_S
ClientSampleId :
SF-9

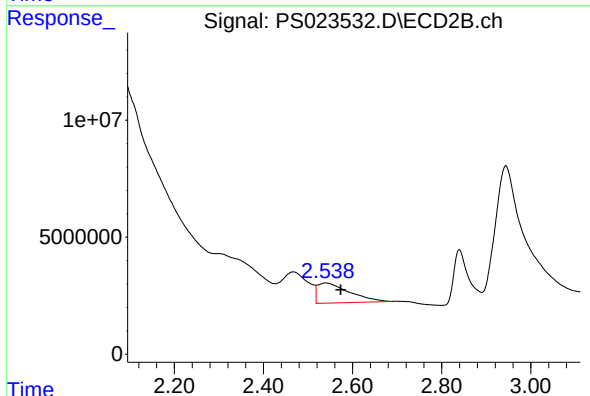


#1 Dalapon

R.T.: 2.540 min
Delta R.T.: -0.034 min
Response: 42080720
Conc: 45.91 ng/ml

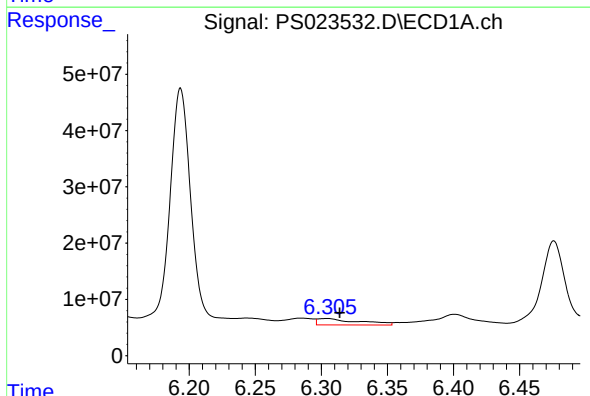


#3 4-Nitrophenol

R.T.: 6.304 min
Delta R.T.: -0.010 min
Response: 24766100
Conc: 19.22 ng/ml

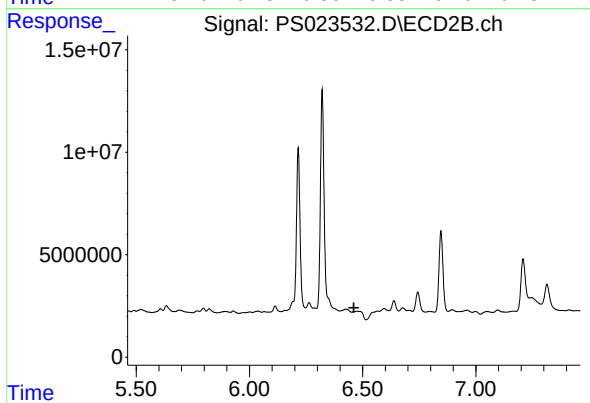

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 6.461 min
Response: 0
Conc: N.D.

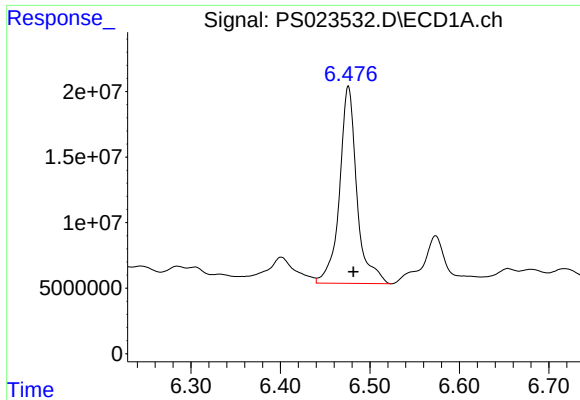

#4 2,4-DCAA


R.T.: 6.476 min
Delta R.T.: -0.006 min
Response: 202545974
Conc: 114.48 ng/ml

Instrument :
ECD_S
ClientSampleId :
SF-9

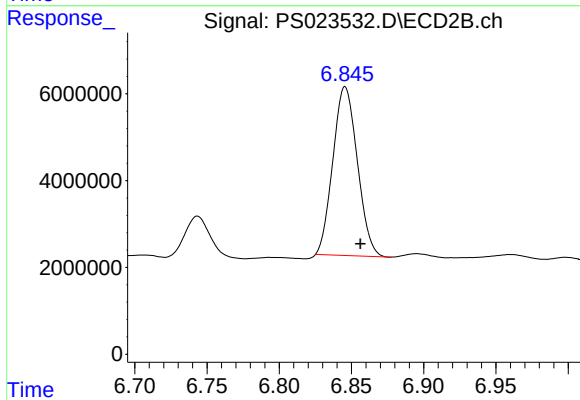


#4 2,4-DCAA

R.T.: 6.846 min
Delta R.T.: -0.010 min
Response: 45799885
Conc: 80.68 ng/ml

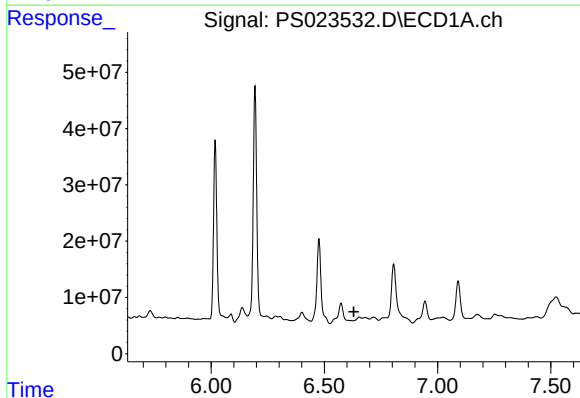


#5 DICAMBA

R.T.: 6.654 min
Delta R.T.: 0.024 min
Response: -1763914
Conc: N.D.

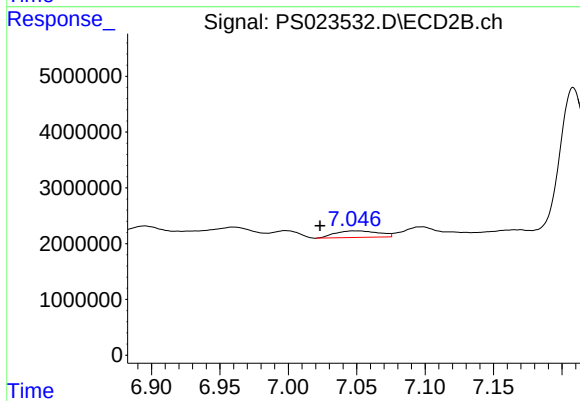

#5 DICAMBA


R.T.: 7.049 min
Delta R.T.: 0.026 min
Response: 2621435
Conc: 1.02 ng/ml

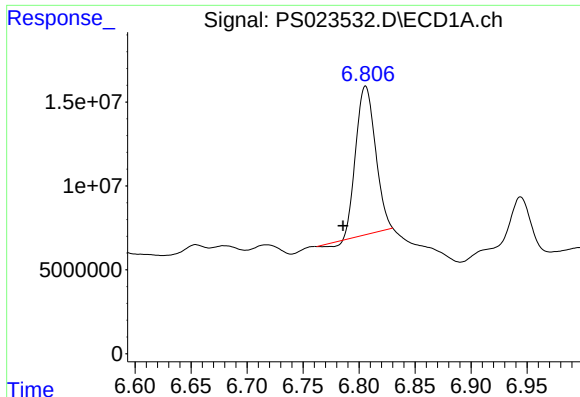

#6 MCP


R.T.: 6.806 min
Delta R.T.: 0.020 min
Response: 107768700
Conc: 19.55 ug/ml

Instrument :
ECD_S
ClientSampleId :
SF-9

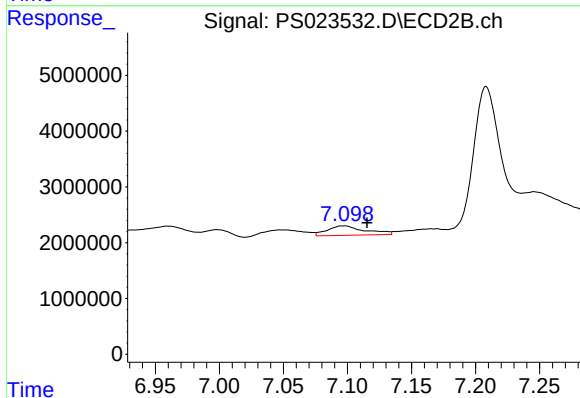


#6 MCP

R.T.: 7.097 min
Delta R.T.: -0.018 min
Response: 3460520
Conc: 1.94 ug/ml

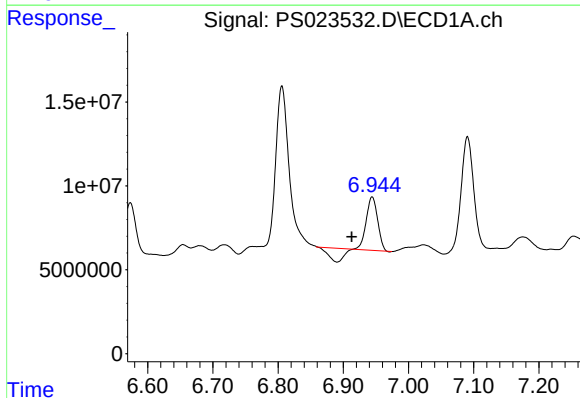


#7 MCP

R.T.: 6.944 min
Delta R.T.: 0.031 min
Response: 27269452
Conc: 3.48 ug/ml

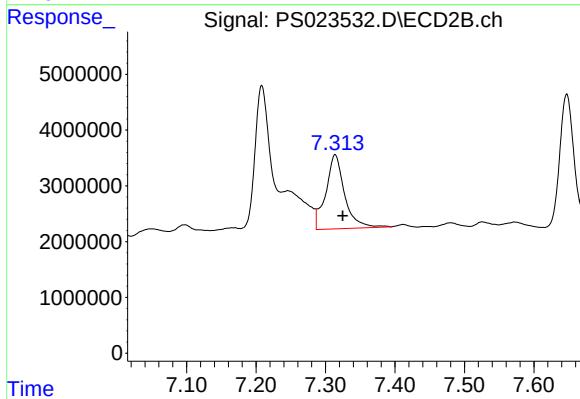

#7 MCP


R.T.: 7.314 min
Delta R.T.: -0.011 min
Response: 24953836
Conc: 9.28 ug/ml

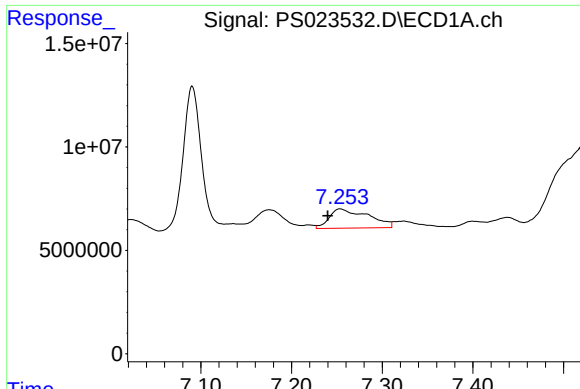

#8 DICHLORPROP


R.T.: 7.254 min
Delta R.T.: 0.014 min
Response: 27813551
Conc: 13.48 ng/ml

Instrument :
ECD_S
ClientSampleId :
SF-9

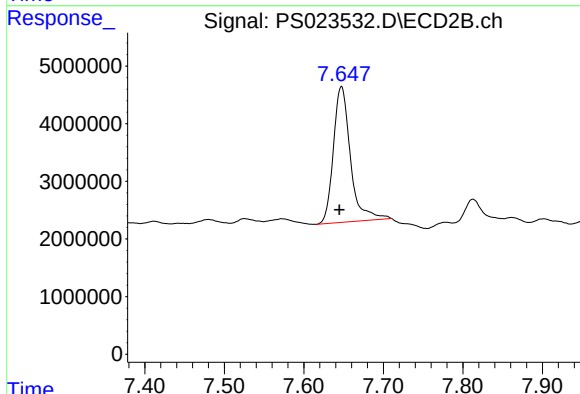


#8 DICHLORPROP

R.T.: 7.647 min
Delta R.T.: 0.003 min
Response: 35148779
Conc: 56.82 ng/ml

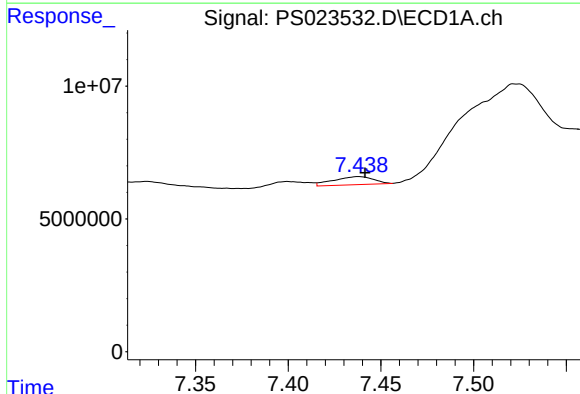


#9 2,4-D

R.T.: 7.438 min
Delta R.T.: -0.004 min
Response: 4536579
Conc: 1.86 ng/ml

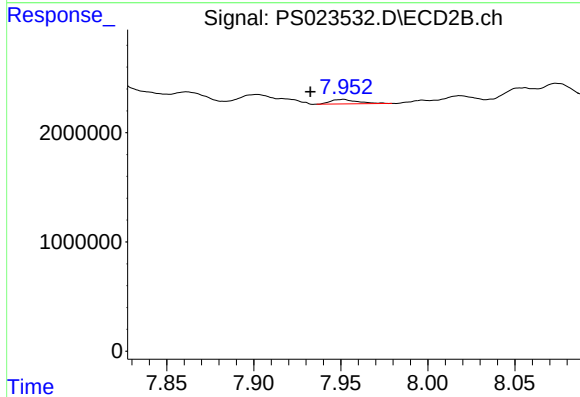

#9 2,4-D


R.T.: 7.951 min
Delta R.T.: 0.018 min
Response: 449069
Conc: N.D.

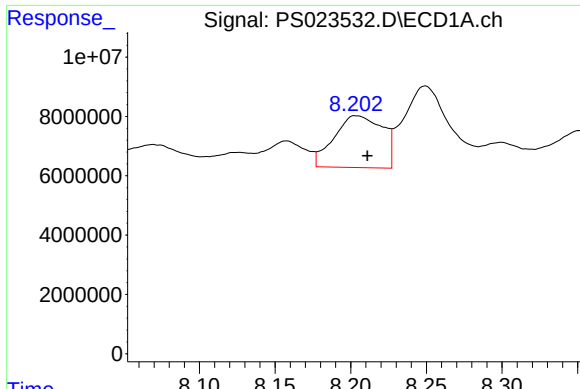

#11 2,4,5-TP (SILVEX)


R.T.: 8.204 min
Delta R.T.: -0.007 min
Response: 39018436
Conc: 3.37 ng/ml

Instrument :
ECD_S
ClientSampleId :
SF-9

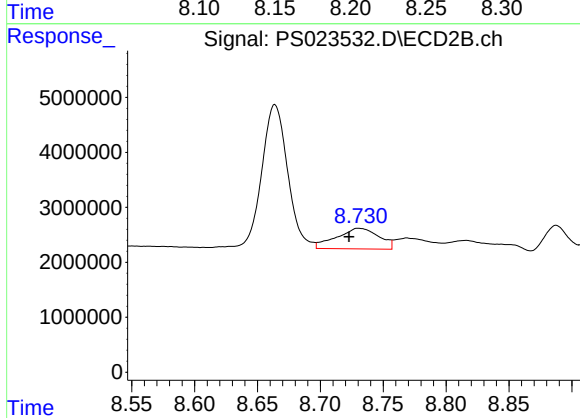


#11 2,4,5-TP (SILVEX)

R.T.: 8.731 min
Delta R.T.: 0.008 min
Response: 8797229
Conc: 2.64 ng/ml

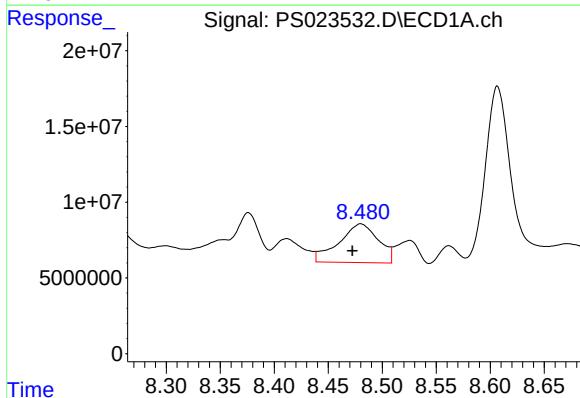


#12 2,4,5-T

R.T.: 8.480 min
Delta R.T.: 0.008 min
Response: 65019578
Conc: 5.72 ng/ml

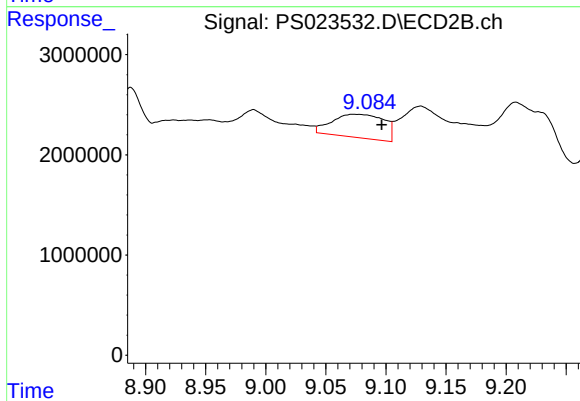

#12 2,4,5-T


R.T.: 9.075 min
Delta R.T.: -0.022 min
Response: 7058321
Conc: 2.30 ng/ml

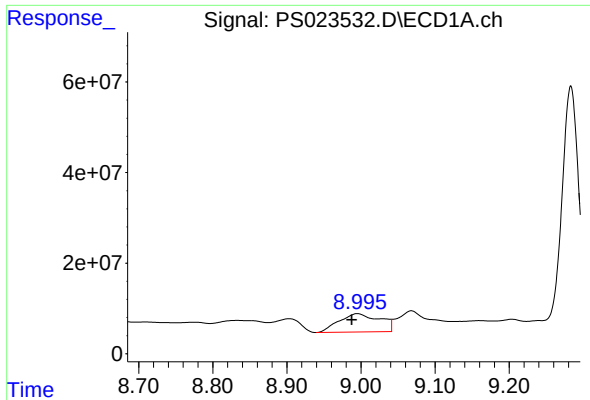

#13 2,4-DB


R.T.: 8.995 min
Delta R.T.: 0.008 min
Response: 155387279
Conc: 66.01 ng/ml

Instrument :
ECD_S
ClientSampleId :
SF-9

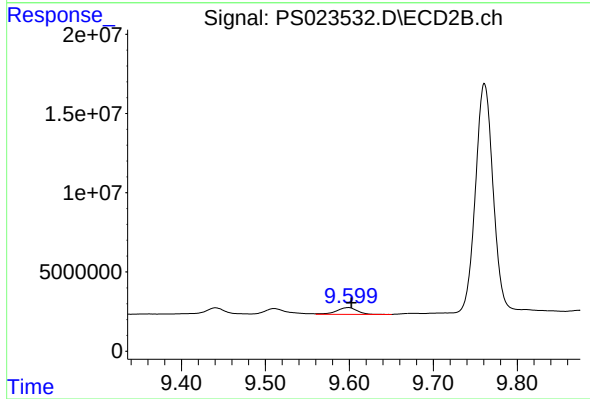


#13 2,4-DB

R.T.: 9.598 min
Delta R.T.: -0.004 min
Response: 7357752
Conc: 19.84 ng/ml

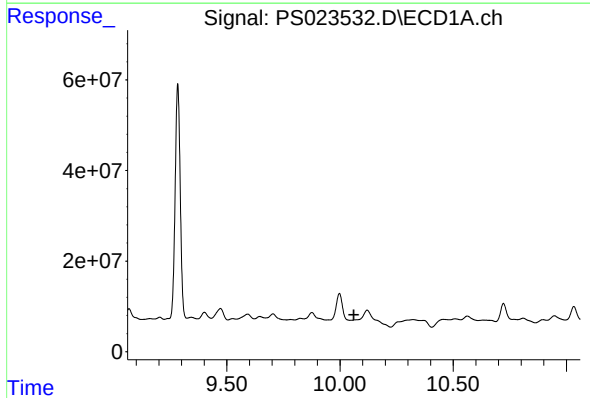


#14 DINOSEB

R.T.: 10.120 min
Delta R.T.: 0.058 min
Response: -40080772
Conc: N.D.

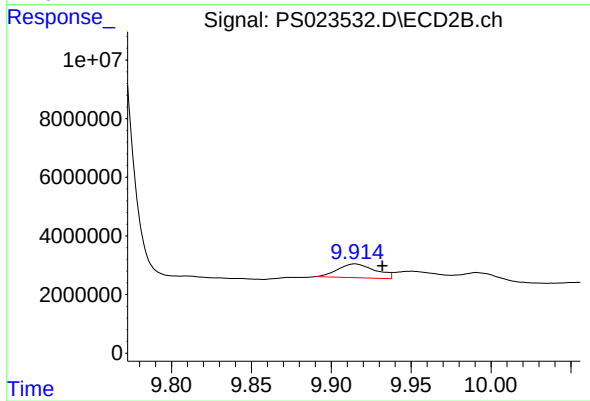

#14 DINOSEB


R.T.: 9.915 min
Delta R.T.: -0.017 min
Response: 7683047
Conc: 3.24 ng/ml

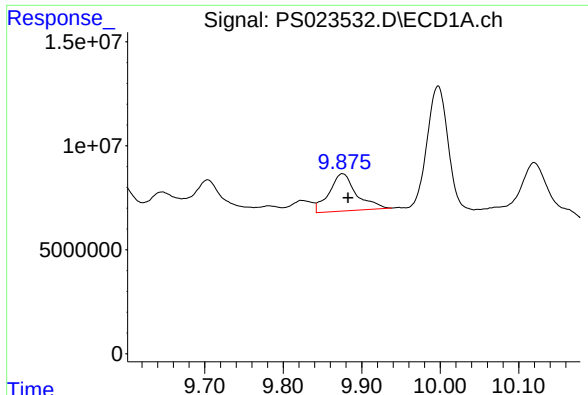

#15 Picloram


R.T.: 9.876 min
Delta R.T.: -0.007 min
Response: 43447078
Conc: 2.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
SF-9

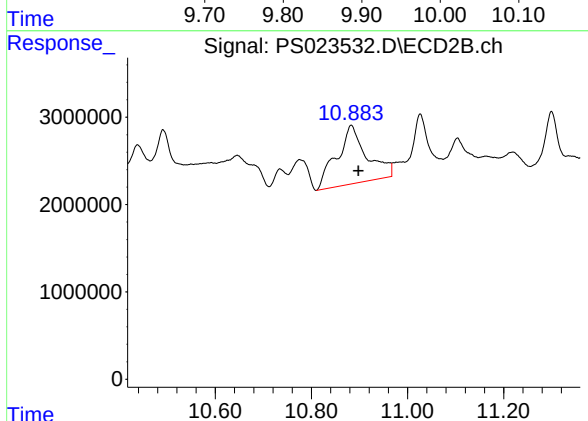


#15 Picloram

R.T.: 10.883 min
Delta R.T.: -0.015 min
Response: 28939049
Conc: 6.34 ng/ml

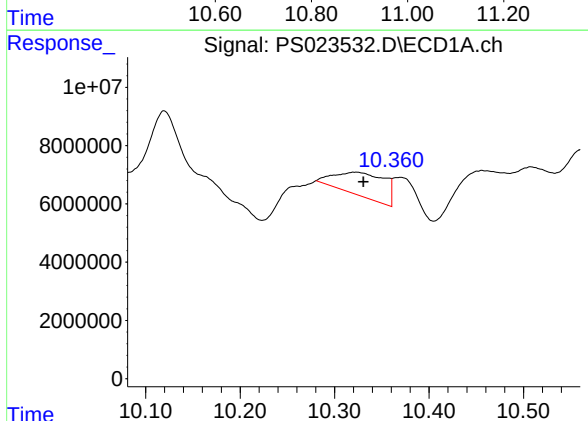

#16 DCPA

R.T.: 10.322 min
Delta R.T.: -0.008 min
Response: 29900593
Conc: 2.14 ng/ml

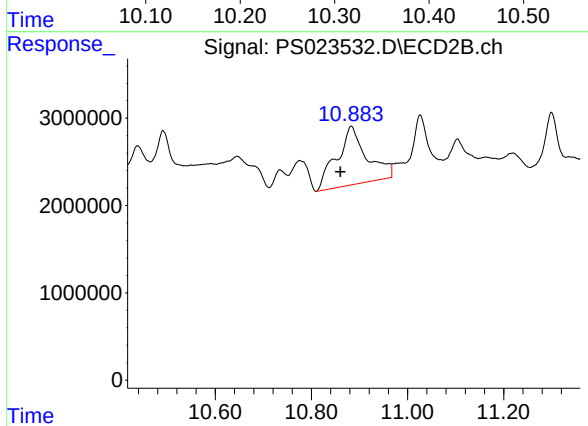

#16 DCPA

R.T.: 10.883 min
Delta R.T.: 0.022 min
Response: 28939049
Conc: 7.21 ng/ml