

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062920\
 Data File : PS010990.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jun 2020 08:53
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 29 12:15:10 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062420.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 25 02:45:12 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds									
10)	T	Pentachlo...	8.658	0.000	6628060	0	<MDL	N.D.	#
12)	T	2,4,5-T	9.493	9.233	7955571	22333150	1.708	7.500	#
15)	T	Picloram	11.027	11.001	92296035	78491139	16.463	18.735	
16)	T	DCPA	11.473	11.001	7900405	78491139	1.292	21.075	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062920\
Data File : PS010990.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jun 2020 08:53
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 29 12:15:10 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062420.M
Quant Title : 8080.M
QLast Update : Thu Jun 25 02:45:12 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

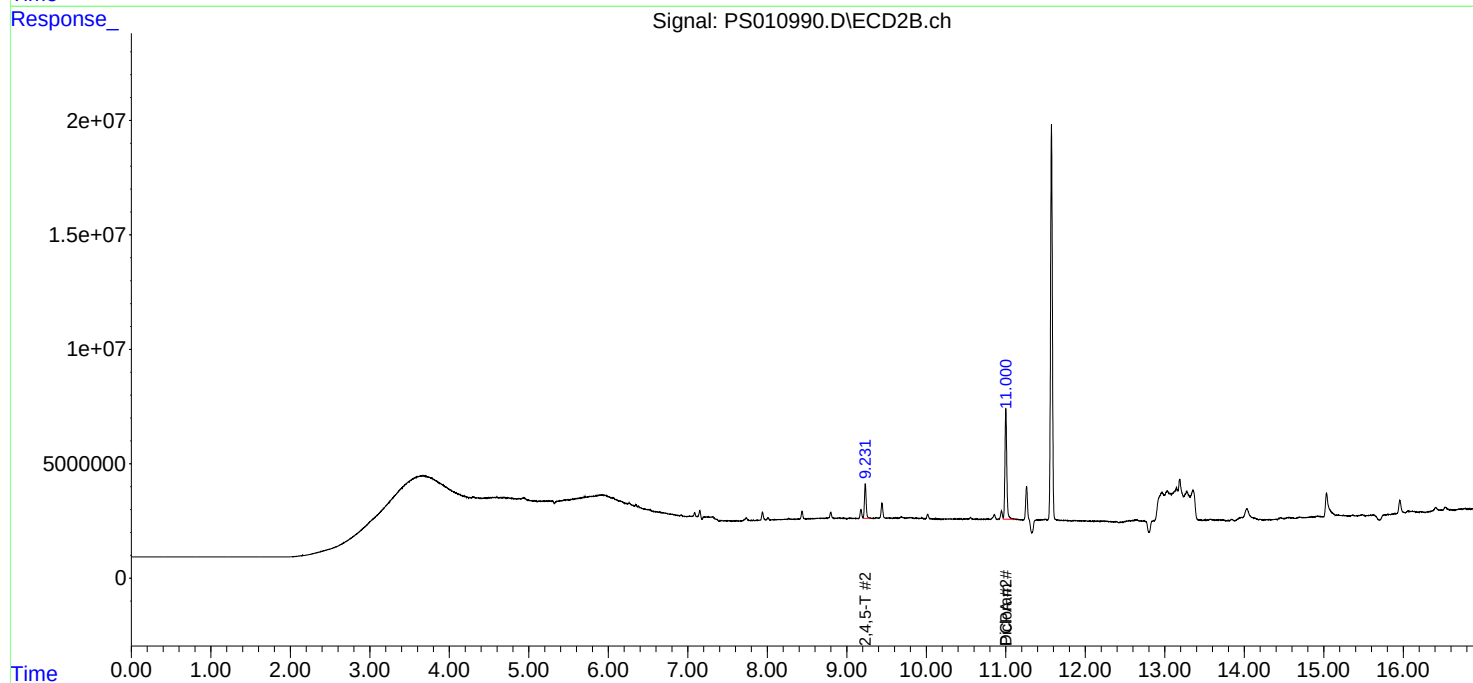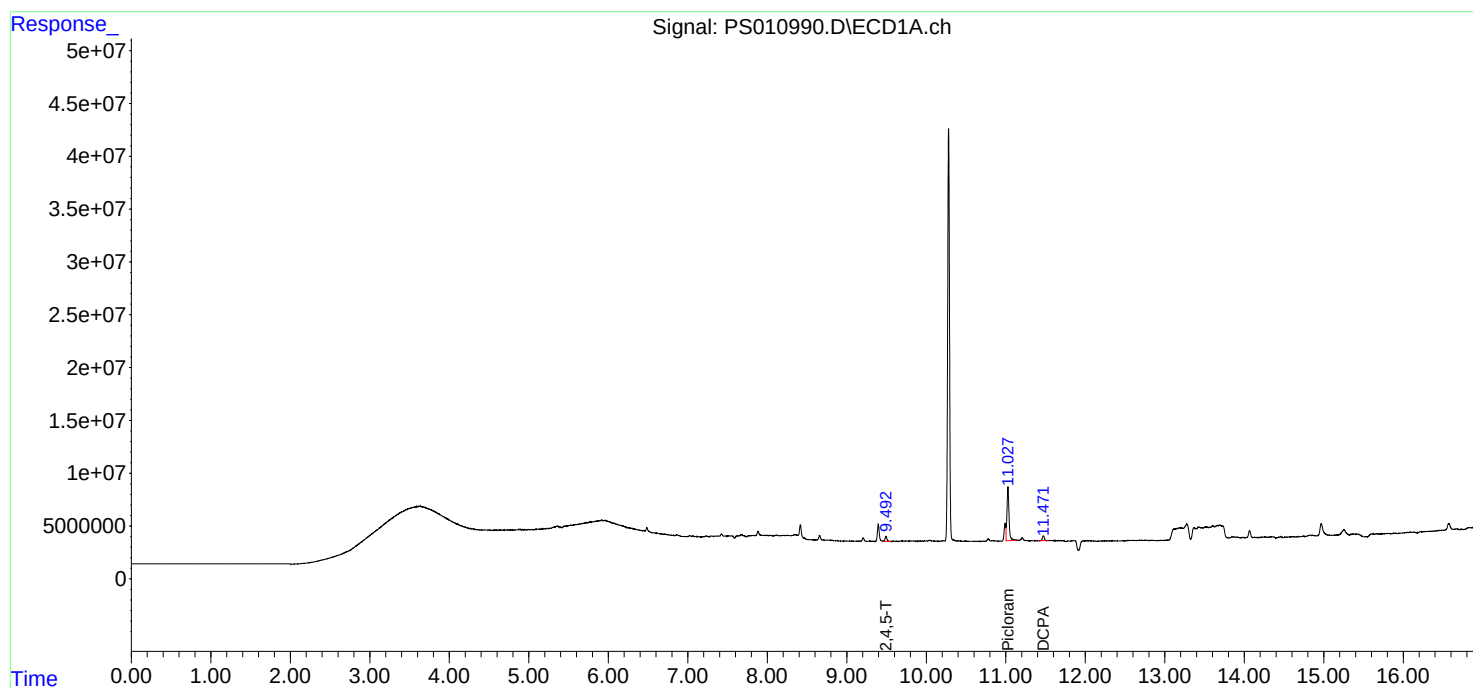


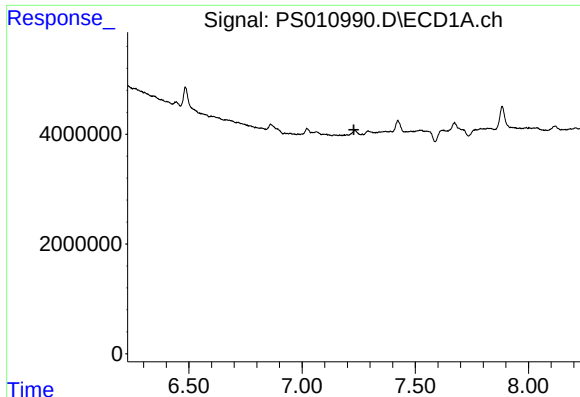

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 7.228 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

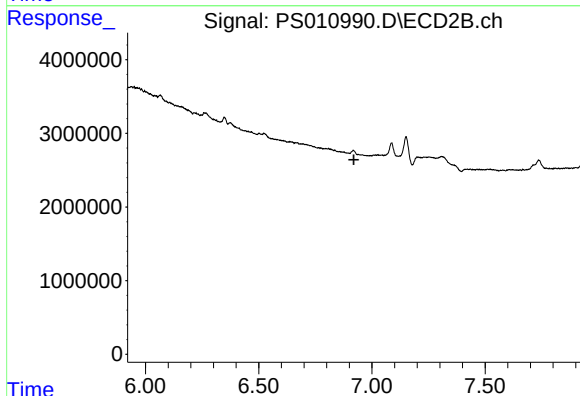


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 6.920 min
Response: 0
Conc: N.D.

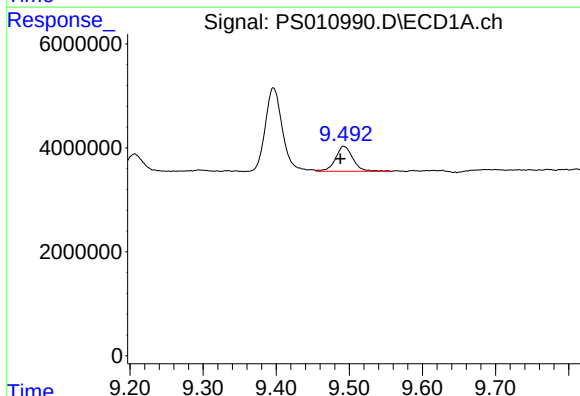


#12 2,4,5-T

R.T.: 9.493 min
Delta R.T.: 0.005 min
Response: 7955571
Conc: 1.71 ng/ml

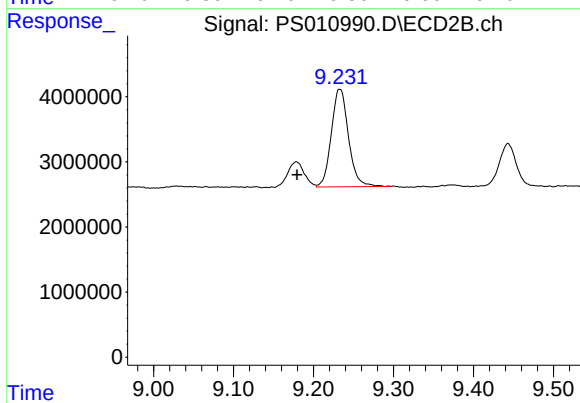

#12 2,4,5-T


R.T.: 9.233 min
Delta R.T.: 0.053 min
Response: 22333150
Conc: 7.50 ng/ml

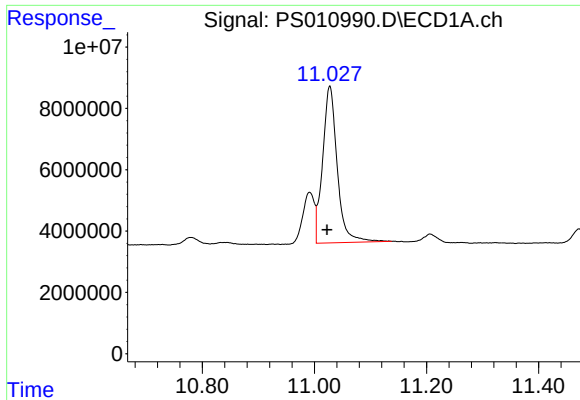

#15 Picloram


R.T.: 11.027 min
Delta R.T.: 0.005 min
Response: 92296035
Conc: 16.46 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

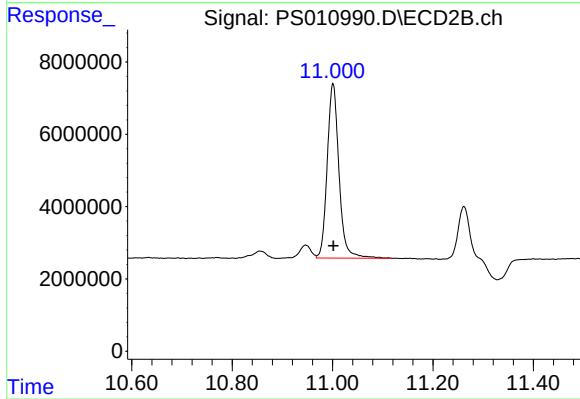


#15 Picloram

R.T.: 11.001 min
Delta R.T.: -0.001 min
Response: 78491139
Conc: 18.73 ng/ml

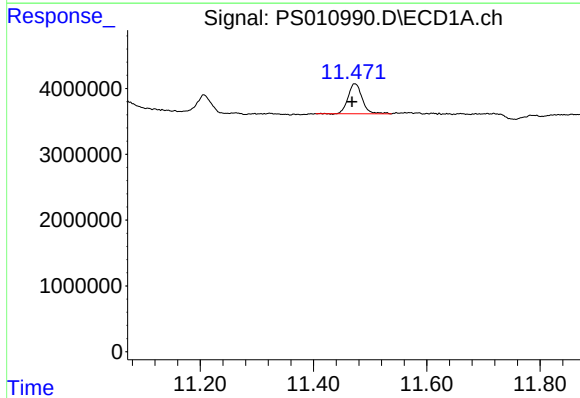

#16 DCPA

R.T.: 11.473 min
Delta R.T.: 0.005 min
Response: 7900405
Conc: 1.29 ng/ml

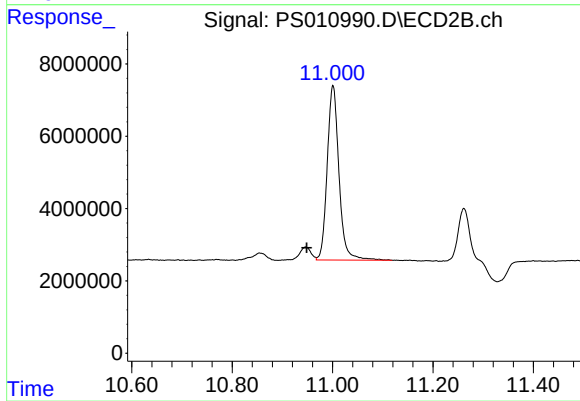

#16 DCPA

R.T.: 11.001 min
Delta R.T.: 0.052 min
Response: 78491139
Conc: 21.07 ng/ml