

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062920\
 Data File : PS010991.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jun 2020 09:16
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 29 12:15:25 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062420.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 25 02:45:12 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.230	6.919	441.1E6	311.2E6	486.471	561.705
Target Compounds							
12) T	2,4,5-T	0.000	9.242	0	12888448	N.D.	4.328
15) T	Picloram	11.035	11.010	53738853	53834755	9.586	12.850 #
16) T	DCPA	0.000	11.010	0	53834755	N.D.	14.455



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062920\
Data File : PS010991.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jun 2020 09:16
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 29 12:15:25 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062420.M
Quant Title : 8080.M
QLast Update : Thu Jun 25 02:45:12 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

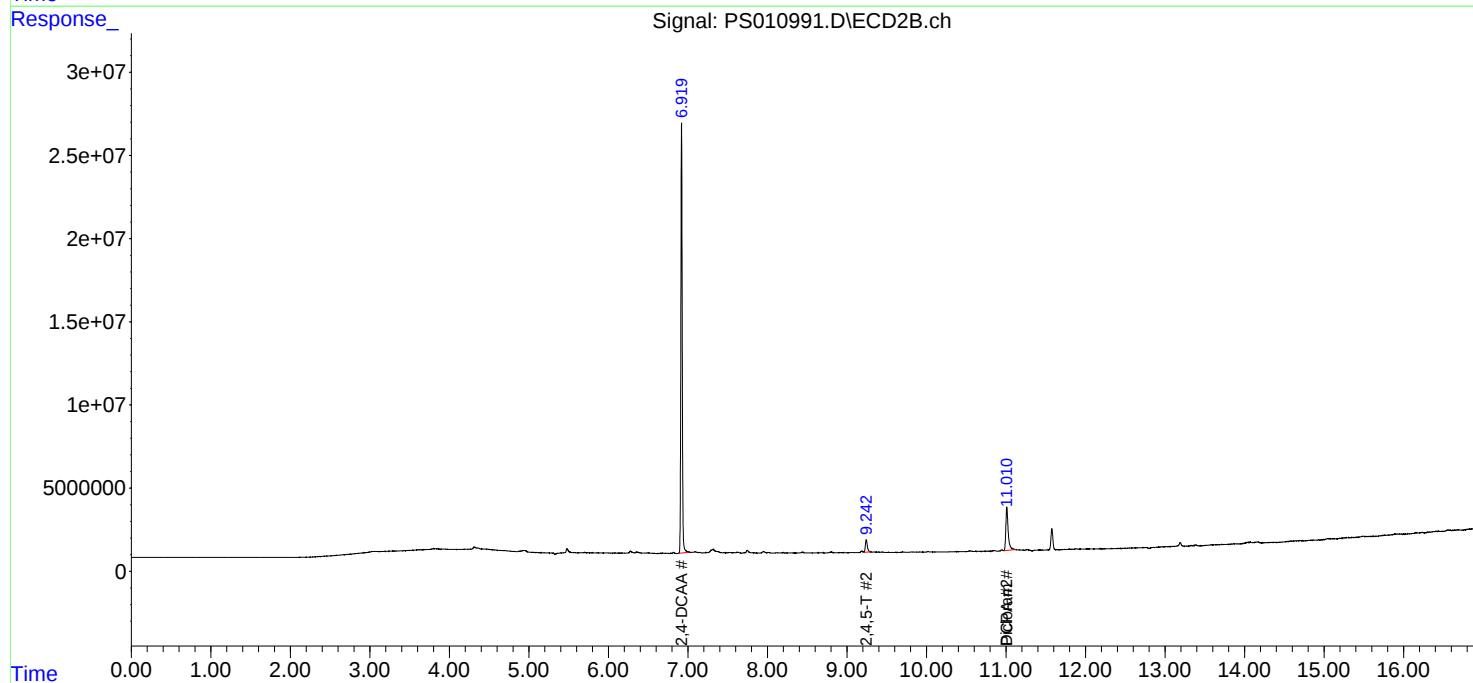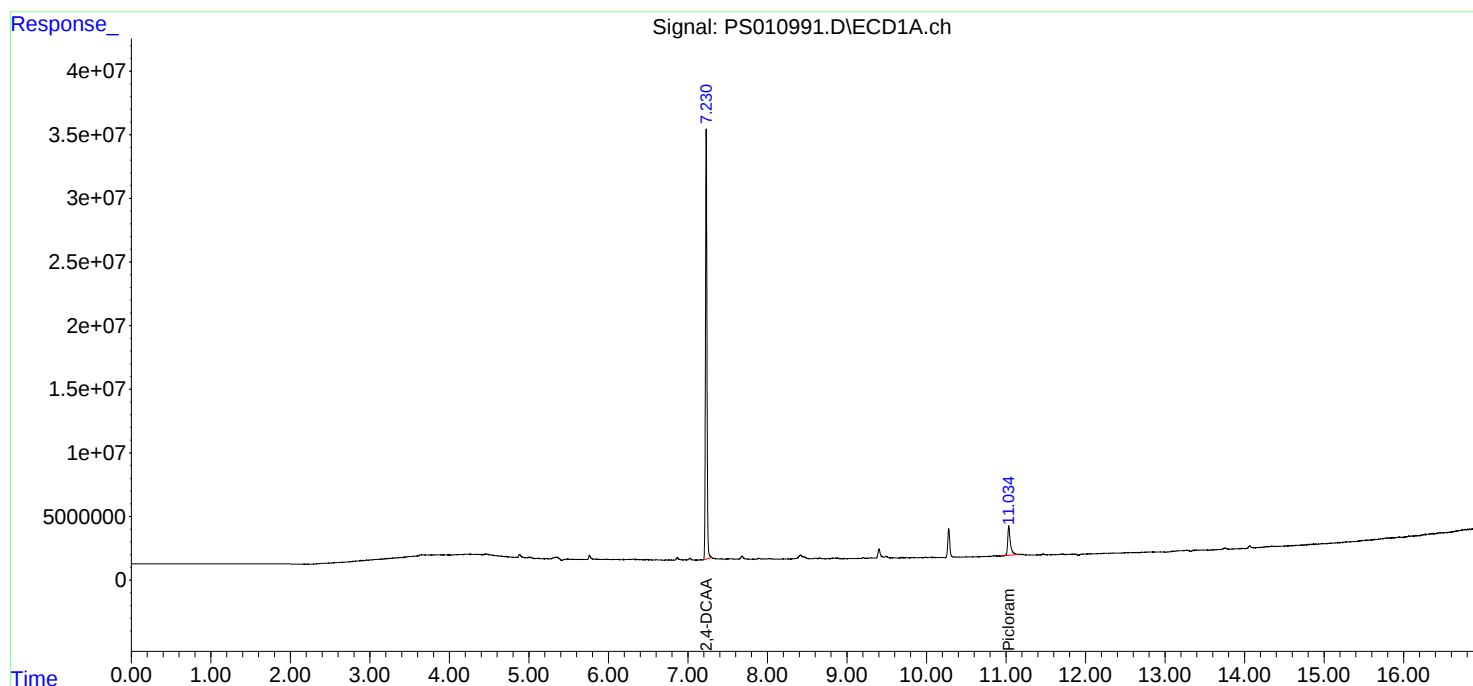


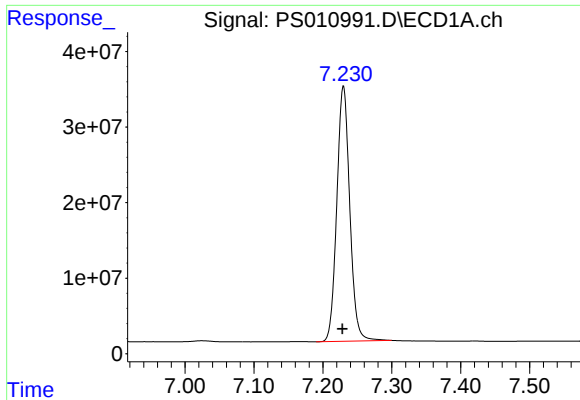

#4 2,4-DCAA


R.T.: 7.230 min
Delta R.T.: 0.002 min
Response: 441141338
Conc: 486.47 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

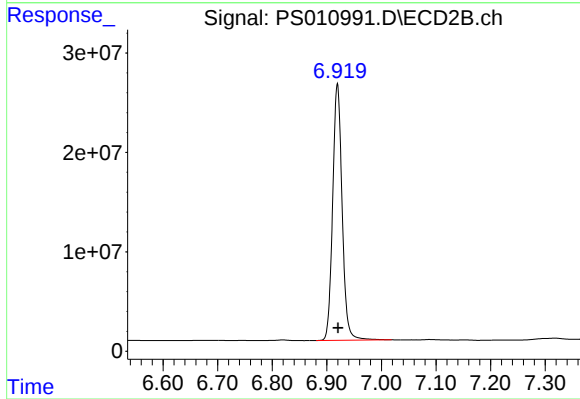


#4 2,4-DCAA

R.T.: 6.919 min
Delta R.T.: 0.000 min
Response: 311227643
Conc: 561.71 ng/ml

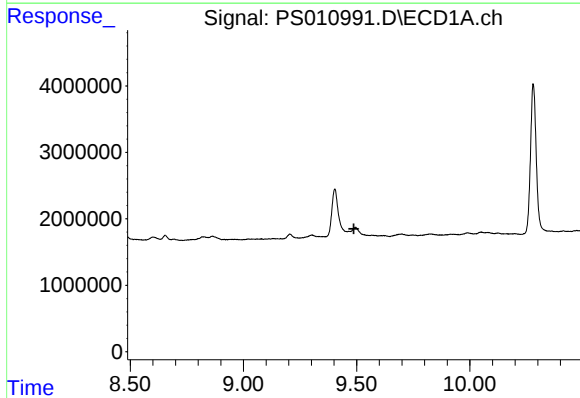


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.488 min
Response: 0
Conc: N.D.

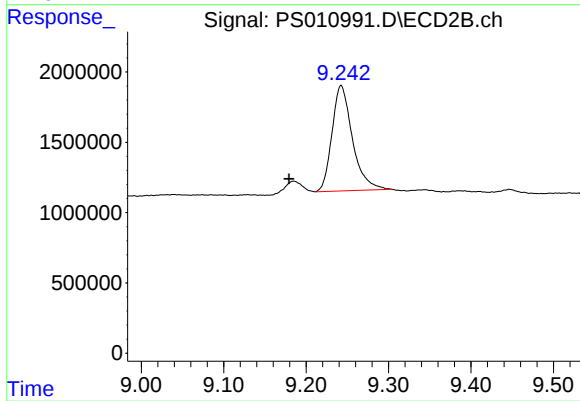

#12 2,4,5-T


R.T.: 9.242 min
Delta R.T.: 0.063 min
Response: 12888448
Conc: 4.33 ng/ml

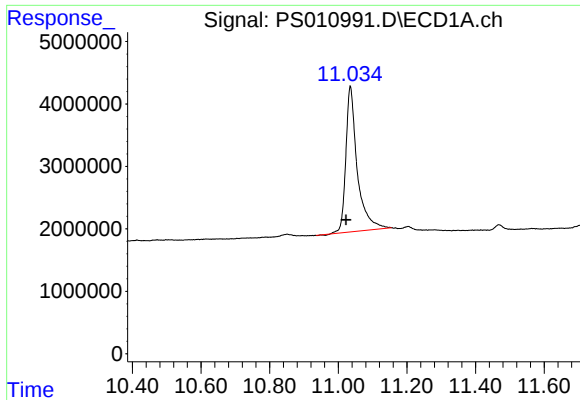

#15 Picloram


R.T.: 11.035 min
Delta R.T.: 0.013 min
Response: 53738853
Conc: 9.59 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

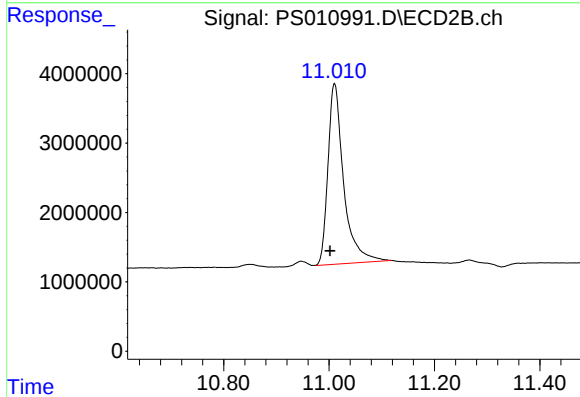


#15 Picloram

R.T.: 11.010 min
Delta R.T.: 0.008 min
Response: 53834755
Conc: 12.85 ng/ml

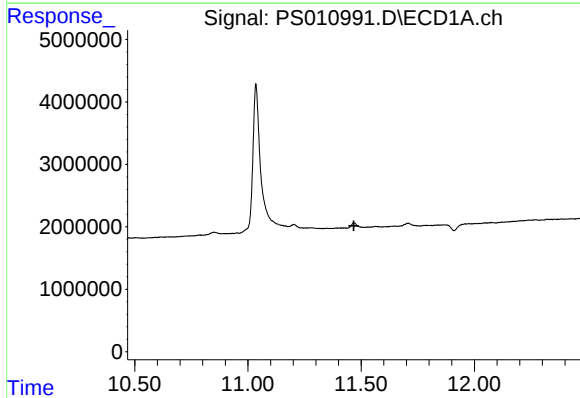

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.468 min
Response: 0
Conc: N.D.

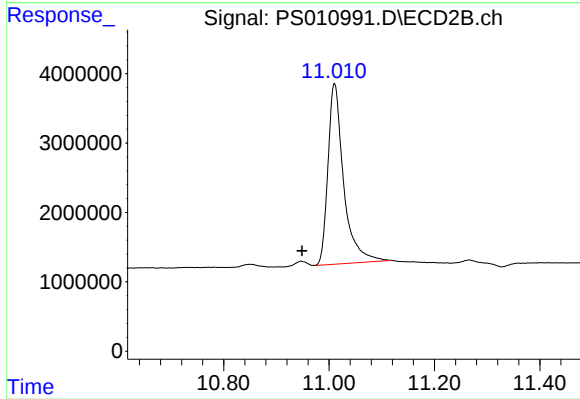

#16 DCPA

R.T.: 11.010 min
Delta R.T.: 0.062 min
Response: 53834755
Conc: 14.45 ng/ml