

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062920\
 Data File : PS010994.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jun 2020 11:17
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 29 12:16:22 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062420.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 25 02:45:12 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.233	6.919	447.9E6	315.7E6	493.945	569.824
Target Compounds							
9) T	2,4-D	0.000	7.950	0	6834518	N.D.	9.458
12) T	2,4,5-T	9.501	9.186	11466316	6801869	2.462	2.284
15) T	Picloram	11.040	11.011	138.8E6	132.0E6	24.761	31.513 #
16) T	DCPA	0.000	11.011	0	132.0E6	N.D.	35.449



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062920\
Data File : PS010994.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jun 2020 11:17
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 29 12:16:22 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062420.M
Quant Title : 8080.M
QLast Update : Thu Jun 25 02:45:12 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

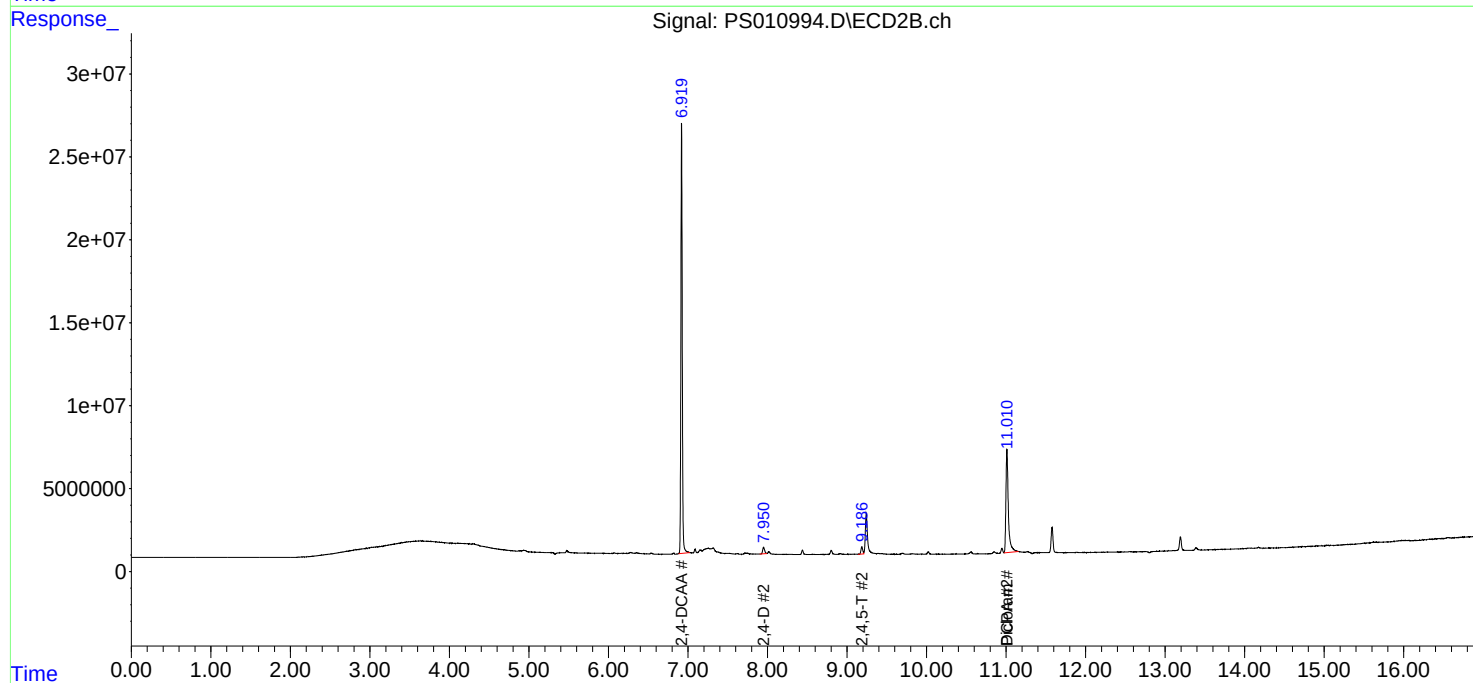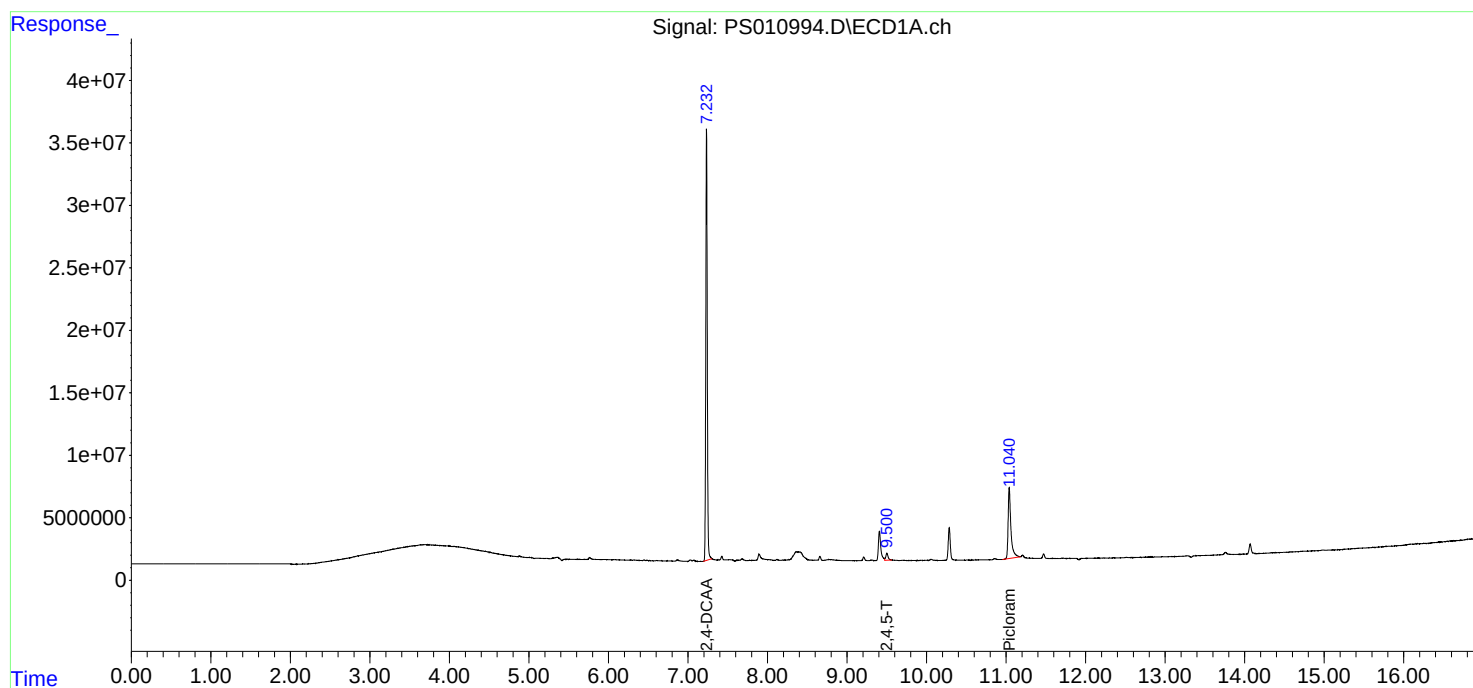


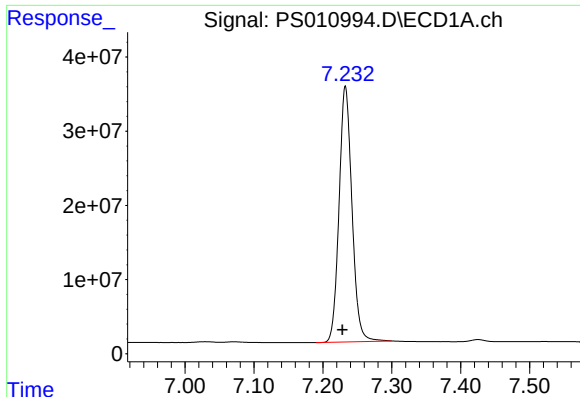

#4 2,4-DCAA


R.T.: 7.233 min
Delta R.T.: 0.004 min
Response: 447918830
Conc: 493.95 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

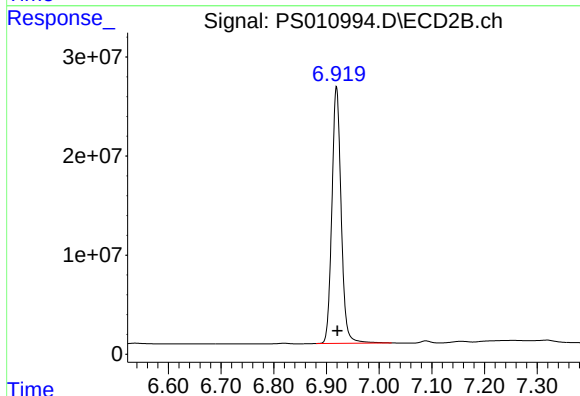


#4 2,4-DCAA

R.T.: 6.919 min
Delta R.T.: -0.001 min
Response: 315725646
Conc: 569.82 ng/ml

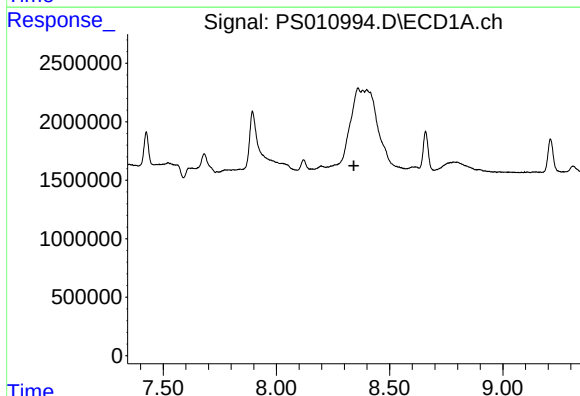


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 8.342 min
Response: 0
Conc: N.D.

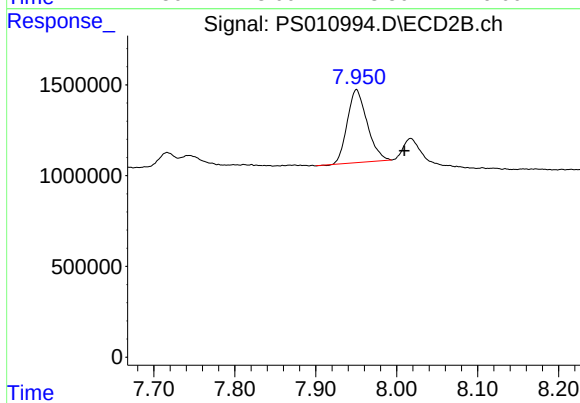

#9 2,4-D


R.T.: 7.950 min
Delta R.T.: -0.059 min
Response: 6834518
Conc: 9.46 ng/ml

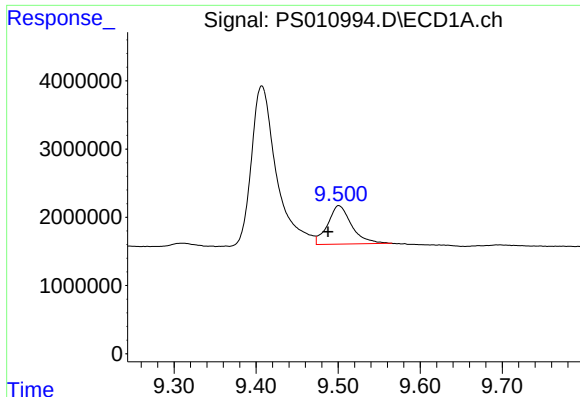

#12 2,4,5-T


R.T.: 9.501 min
Delta R.T.: 0.013 min
Response: 11466316
Conc: 2.46 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

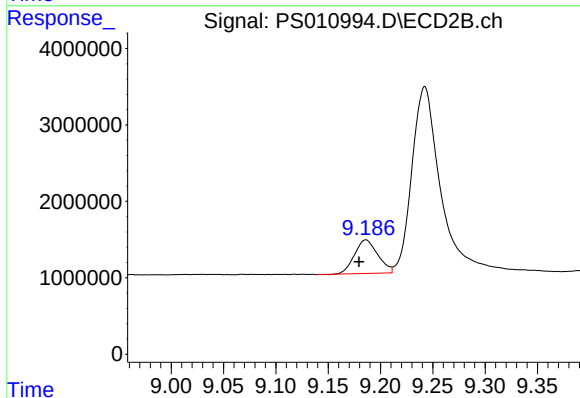


#12 2,4,5-T

R.T.: 9.186 min
Delta R.T.: 0.007 min
Response: 6801869
Conc: 2.28 ng/ml

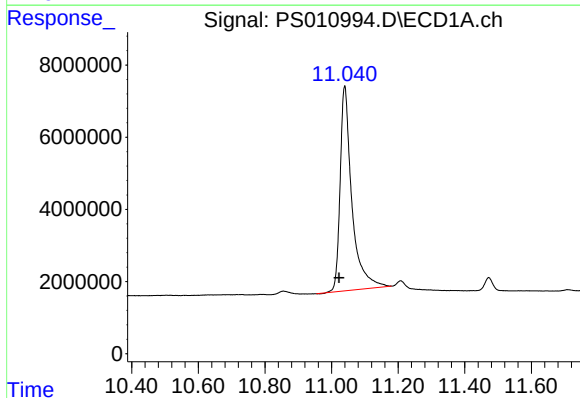


#15 Picloram

R.T.: 11.040 min
Delta R.T.: 0.017 min
Response: 138814692
Conc: 24.76 ng/ml

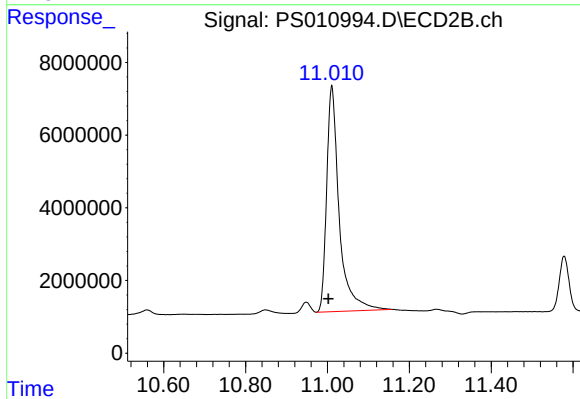

#15 Picloram


R.T.: 11.011 min
Delta R.T.: 0.009 min
Response: 132027049
Conc: 31.51 ng/ml

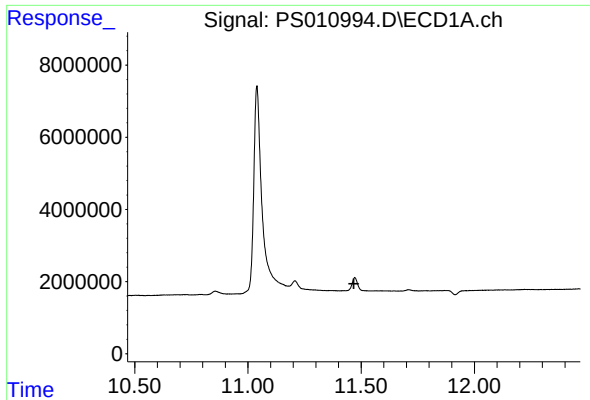

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.468 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

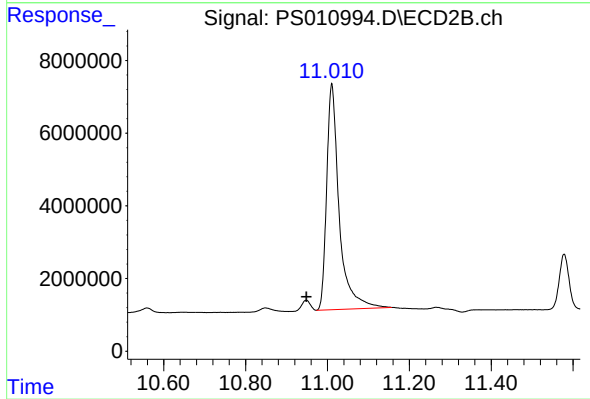

#16 DCPA

R.T.: 11.011 min
Delta R.T.: 0.062 min
Response: 132027049
Conc: 35.45 ng/ml