

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062921\
 Data File : PS015960.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jun 2021 08:56
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 29 13:51:33 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061521.M
 Quant Title : 8080.M
 QLast Update : Tue Jun 15 18:15:49 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
8) T	DICHLORPROP	0.000	7.566	0	8366411	N.D. 16.159
10) T	Pentachlo...	8.613	0.000	12481548	0	<MDL N.D. #
11) T	2,4,5-TP ...	9.164	8.585f	9175567	-1198131	1.050 N.D. #
12) T	2,4,5-T	9.448	9.005	16672243	5881628	1.888 2.085
13) T	2,4-DB	9.992	0.000	8331649	0	4.073 N.D. #
14) T	DINOSEB	11.158	0.000	6472215	0	<MDL N.D. #
15) T	Picloram	10.977	10.816	269.1E6	98887380	19.684 23.513
16) T	DCPA	11.424	10.769	86315516	7727582	6.526 1.838 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062921\
Data File : PS015960.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jun 2021 08:56
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 29 13:51:33 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061521.M
Quant Title : 8080.M
QLast Update : Tue Jun 15 18:15:49 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

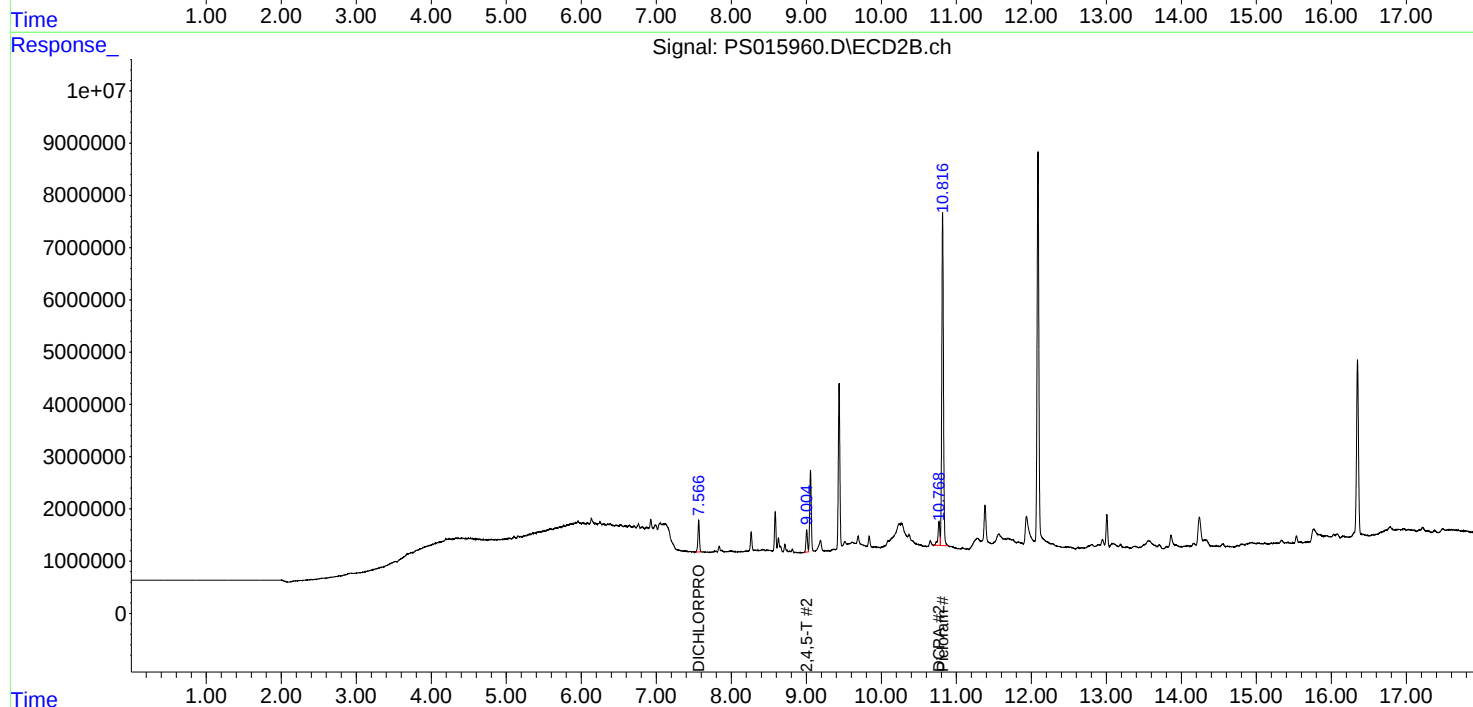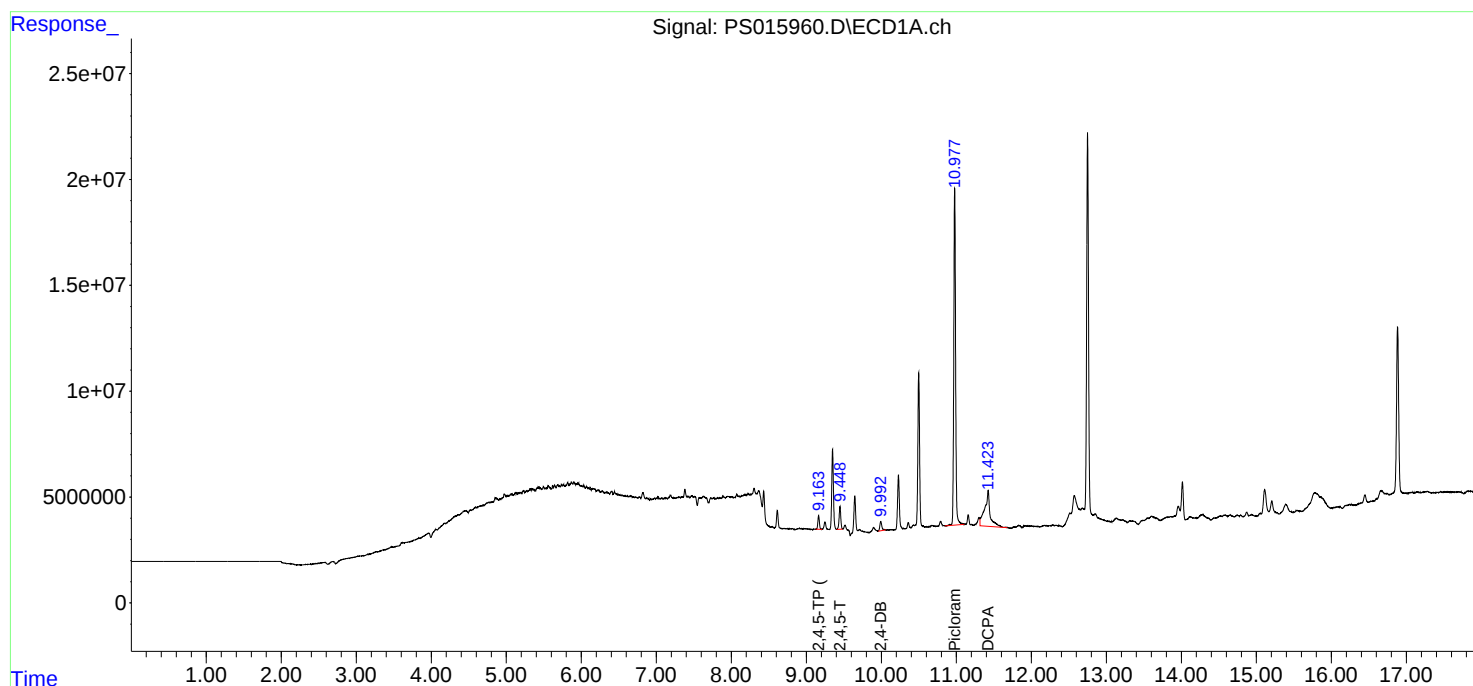


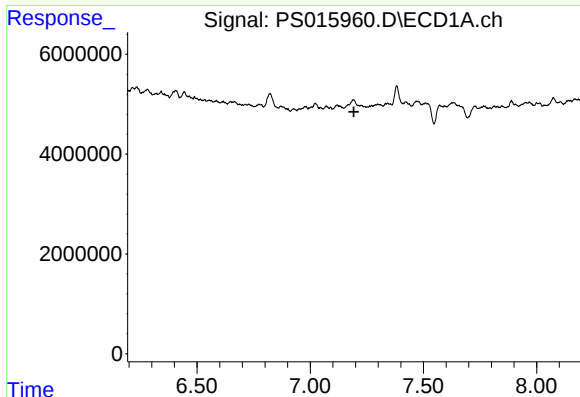

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 7.193 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

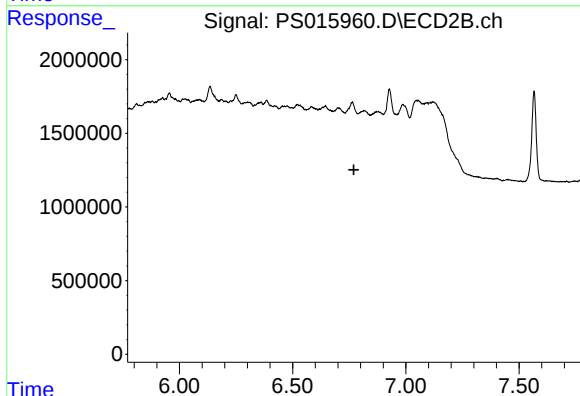


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 6.771 min
Response: 0
Conc: N.D.

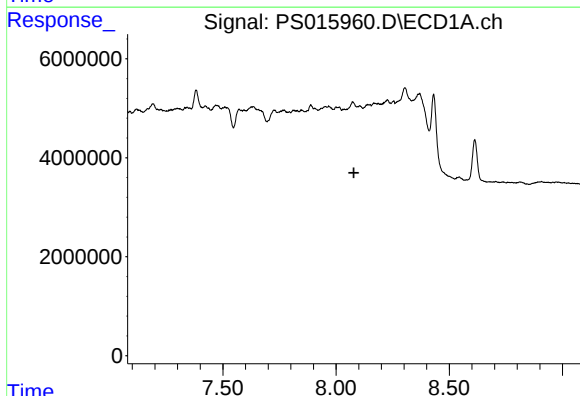


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.079 min
Response: 0
Conc: N.D.

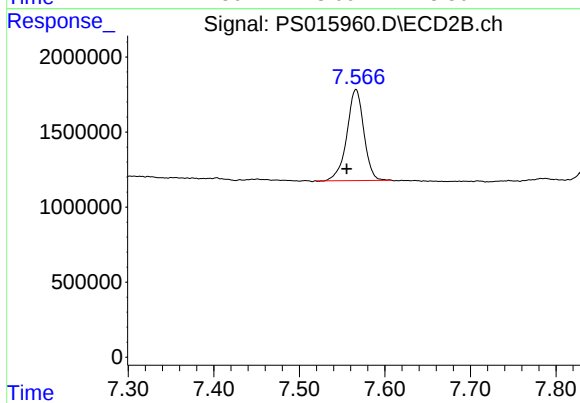

#8 DICHLORPROP


R.T.: 7.566 min
Delta R.T.: 0.011 min
Response: 8366411
Conc: 16.16 ng/ml

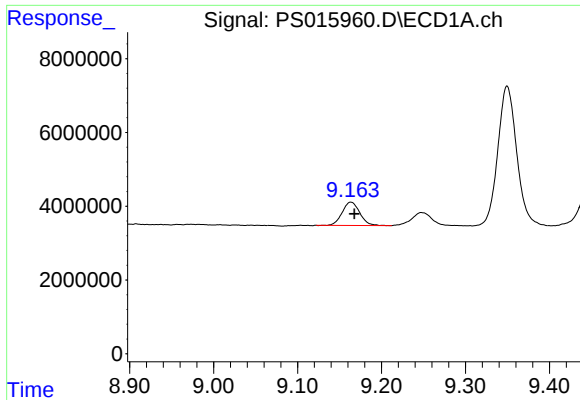

#11 2,4,5-TP (SILVEX)


R.T.: 9.164 min
Delta R.T.: -0.004 min
Response: 9175567
Conc: 1.05 ng/ml

Instrument :
ECD_S
ClientSampleId :

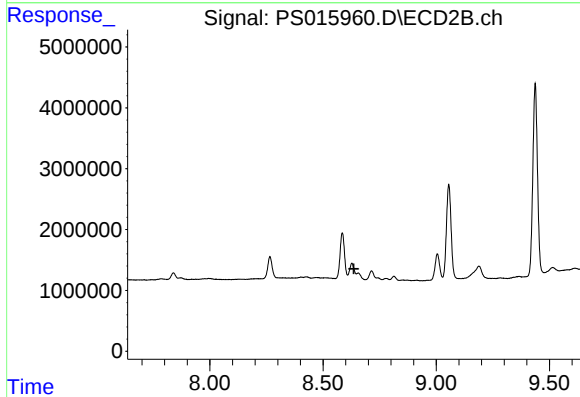


#11 2,4,5-TP (SILVEX)

R.T.: 8.585 min
Delta R.T.: -0.051 min
Response: -1198131
Conc: N.D.

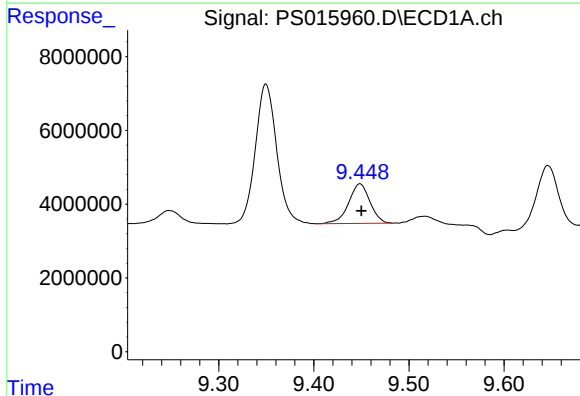


#12 2,4,5-T

R.T.: 9.448 min
Delta R.T.: -0.002 min
Response: 16672243
Conc: 1.89 ng/ml

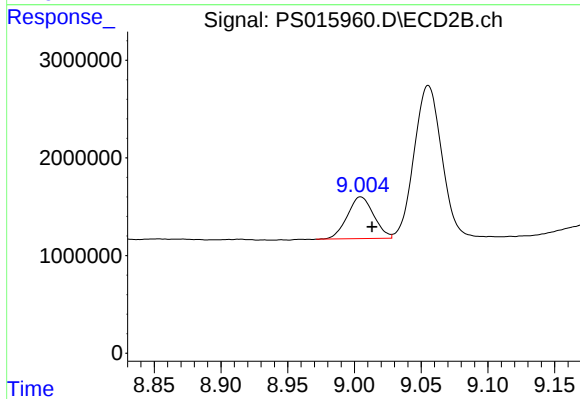

#12 2,4,5-T


R.T.: 9.005 min
Delta R.T.: -0.008 min
Response: 5881628
Conc: 2.09 ng/ml

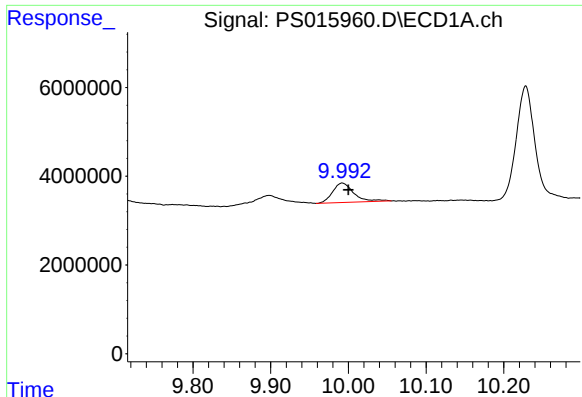

#13 2,4-DB


R.T.: 9.992 min
Delta R.T.: -0.008 min
Response: 8331649
Conc: 4.07 ng/ml

Instrument :
ECD_S
ClientSampleId :

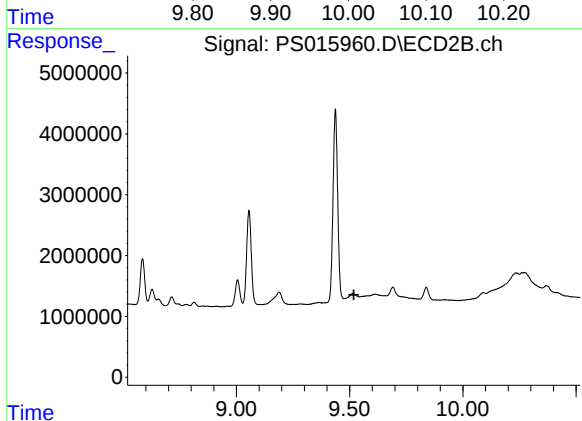


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.519 min
Response: 0
Conc: N.D.

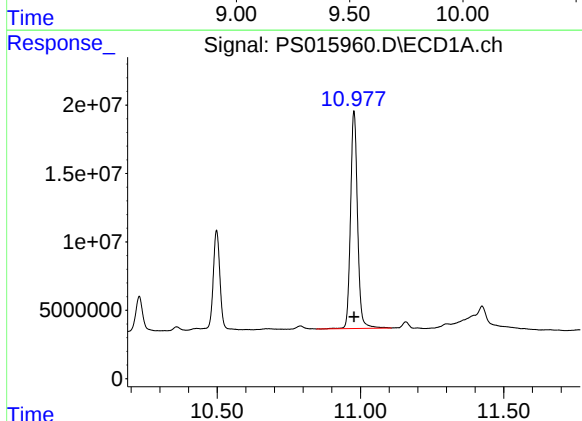


#15 Picloram

R.T.: 10.977 min
Delta R.T.: 0.000 min
Response: 269090151
Conc: 19.68 ng/ml

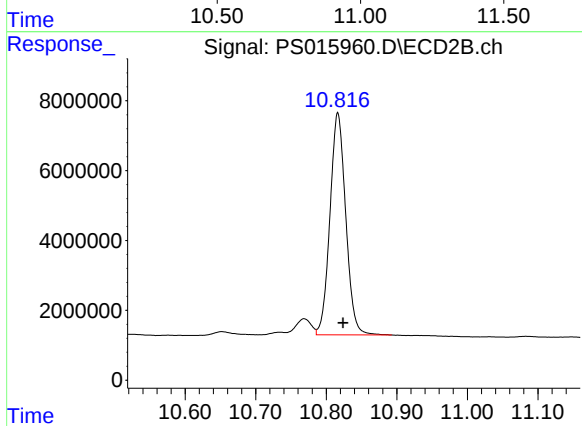

#15 Picloram


R.T.: 10.816 min
Delta R.T.: -0.007 min
Response: 98887380
Conc: 23.51 ng/ml

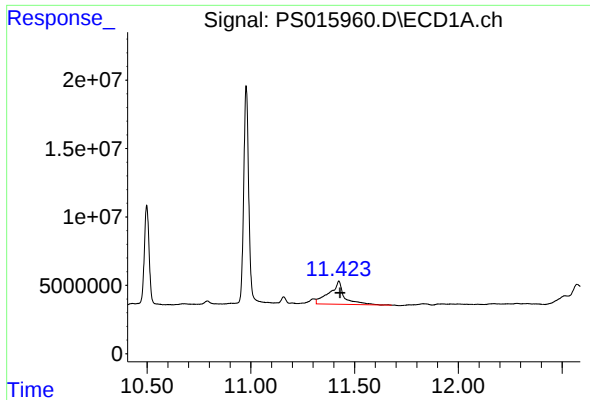

#16 DCPA

R.T.: 11.424 min
Delta R.T.: -0.007 min
Response: 86315516
Conc: 6.53 ng/ml

Instrument :
ECD_S
ClientSampleId :

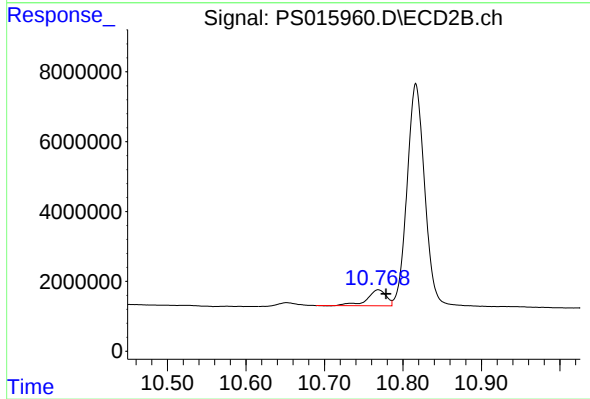

#16 DCPA

R.T.: 10.769 min
Delta R.T.: -0.010 min
Response: 7727582
Conc: 1.84 ng/ml