

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062921\
 Data File : PS015961.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jun 2021 09:20
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 29 13:51:51 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061521.M
 Quant Title : 8080.M
 QLast Update : Tue Jun 15 18:15:49 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.189	6.766	669.1E6	249.4E6	402.737	495.074
Target Compounds							
8) T	DICHLORPROP	0.000	7.569	0	13215419	N.D.	25.525
9) T	2,4-D	8.374f	0.000	33495888	0	19.113	N.D. #
12) T	2,4,5-T	0.000	9.061f	0	13389987	N.D.	4.747
15) T	Picloram	10.983	10.821	179.9E6	71687397	13.162	17.046 #
16) T	DCPA	0.000	10.821f	0	71687397	N.D.	17.051



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062921\
Data File : PS015961.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jun 2021 09:20
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 29 13:51:51 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061521.M
Quant Title : 8080.M
QLast Update : Tue Jun 15 18:15:49 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

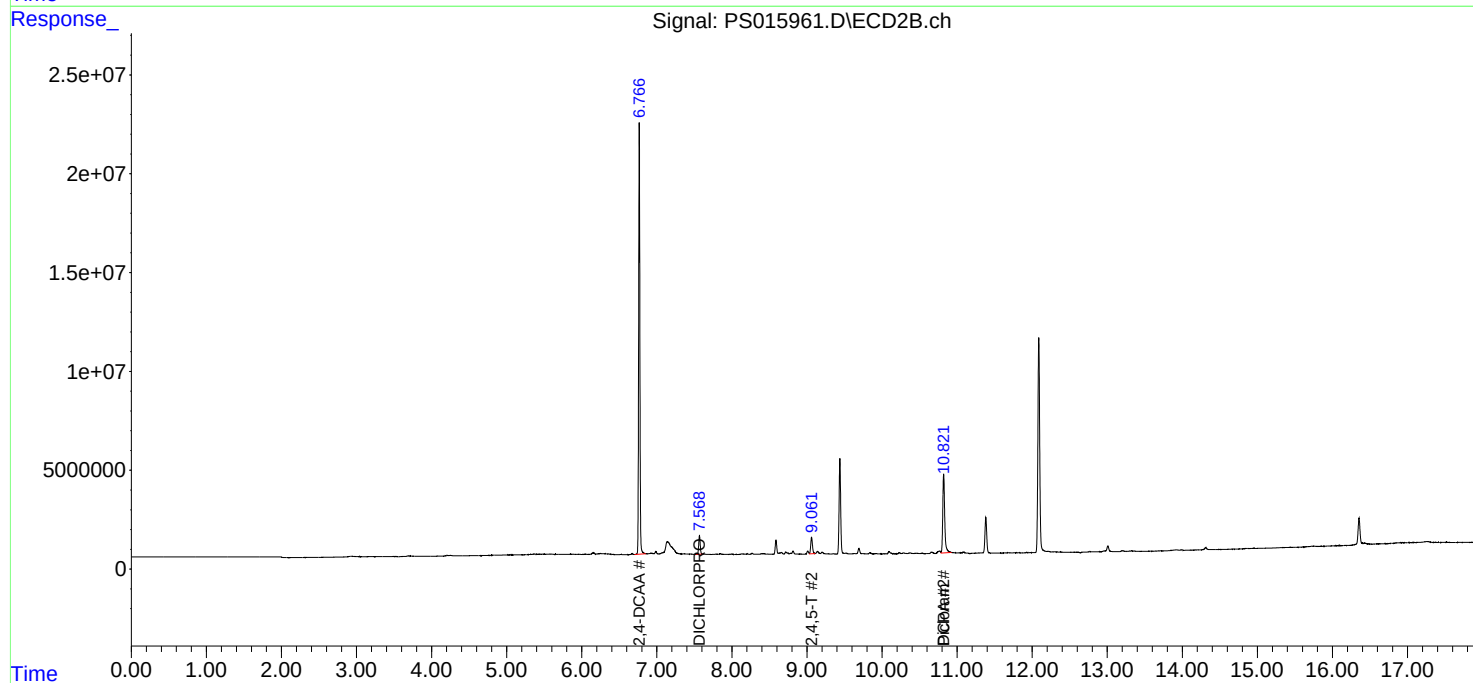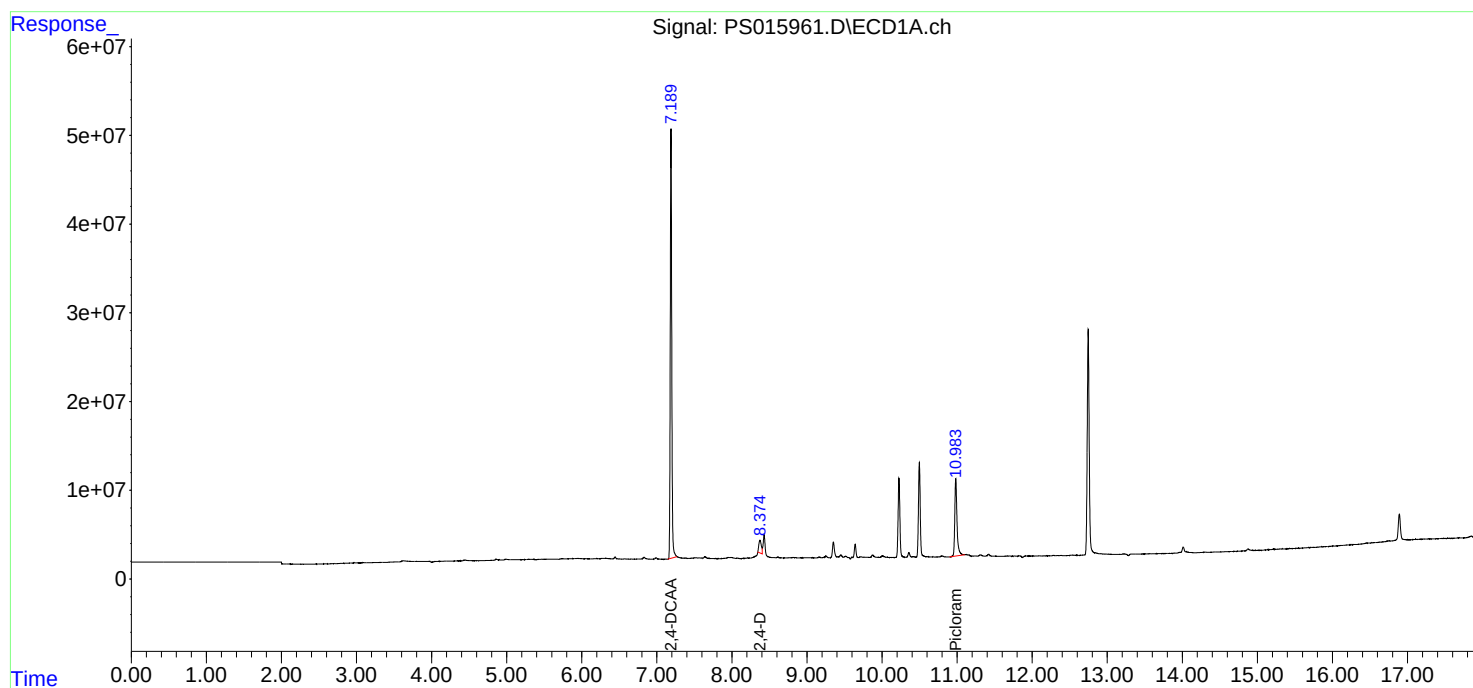


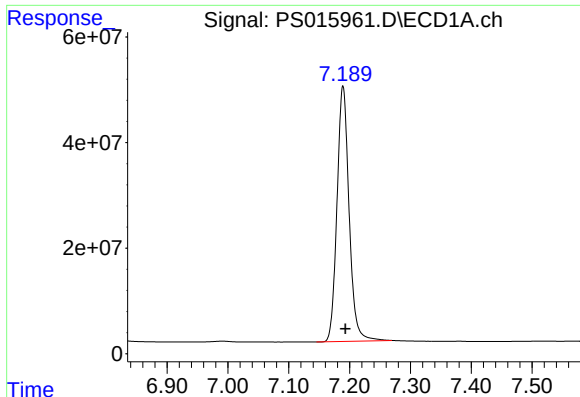

#4 2,4-DCAA


R.T.: 7.189 min
Delta R.T.: -0.004 min
Response: 669126341
Conc: 402.74 ng/ml

Instrument :
ECD_S
ClientSampleId :

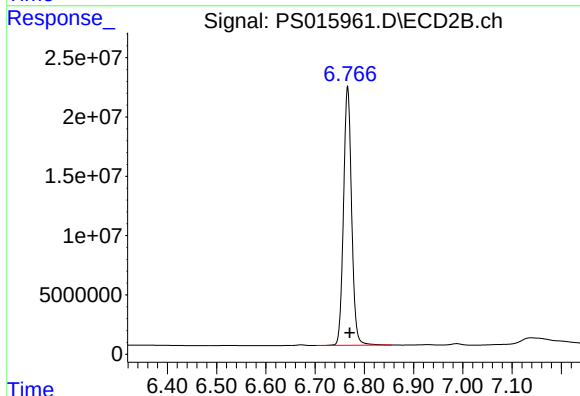


#4 2,4-DCAA

R.T.: 6.766 min
Delta R.T.: -0.004 min
Response: 249444138
Conc: 495.07 ng/ml

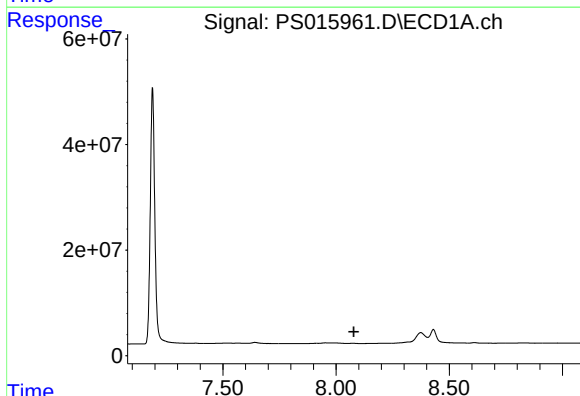


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.079 min
Response: 0
Conc: N.D.

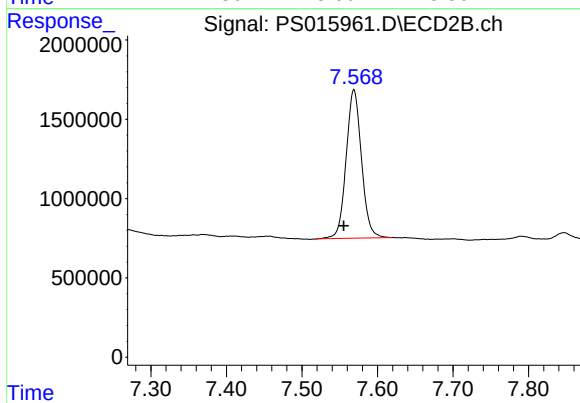

#8 DICHLORPROP


R.T.: 7.569 min
Delta R.T.: 0.014 min
Response: 13215419
Conc: 25.52 ng/ml

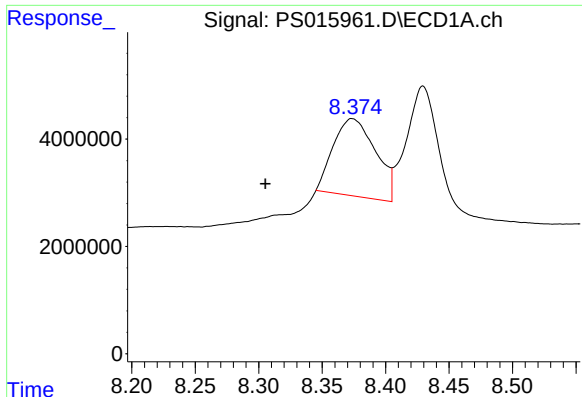

#9 2,4-D


R.T.: 8.374 min
Delta R.T.: 0.068 min
Response: 33495888
Conc: 19.11 ng/ml

Instrument :
ECD_S
ClientSampleId :

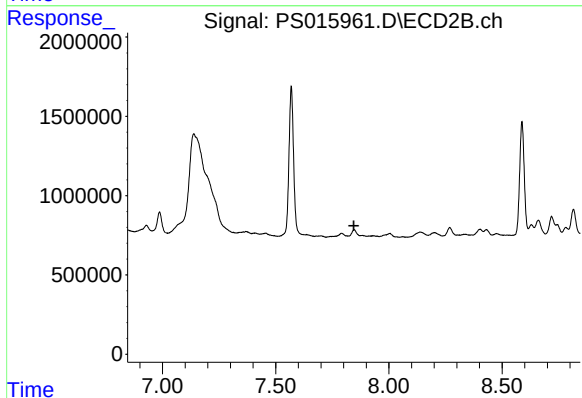


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.845 min
Response: 0
Conc: N.D.

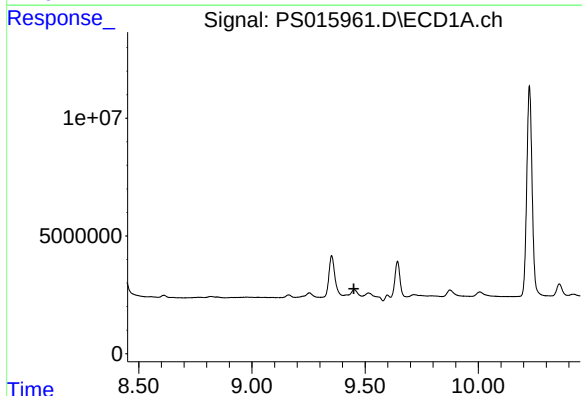


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.450 min
Response: 0
Conc: N.D.

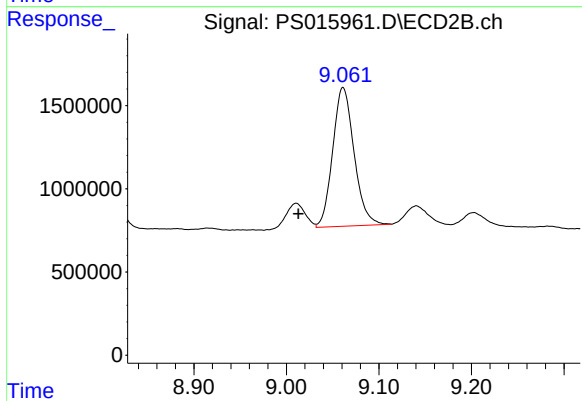

#12 2,4,5-T


R.T.: 9.061 min
Delta R.T.: 0.048 min
Response: 13389987
Conc: 4.75 ng/ml

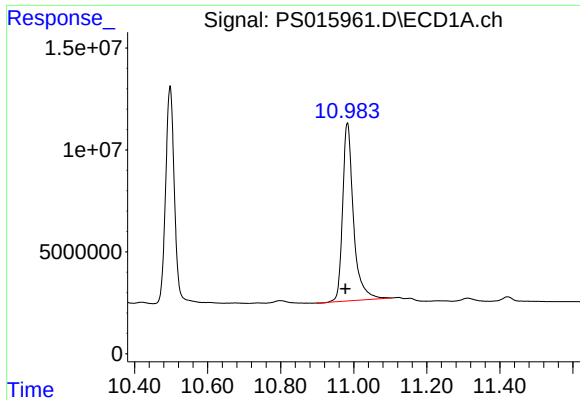

#15 Picloram


R.T.: 10.983 min
Delta R.T.: 0.005 min
Response: 179933406
Conc: 13.16 ng/ml

Instrument :
ECD_S
ClientSampleId :

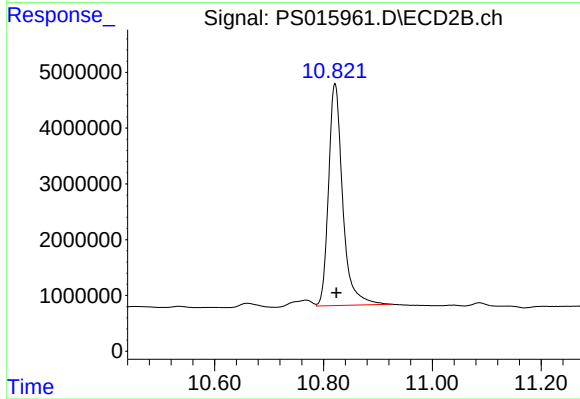


#15 Picloram

R.T.: 10.821 min
Delta R.T.: -0.003 min
Response: 71687397
Conc: 17.05 ng/ml

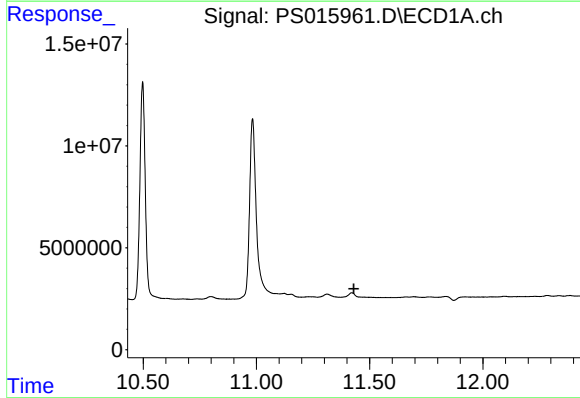

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.431 min
Response: 0
Conc: N.D.

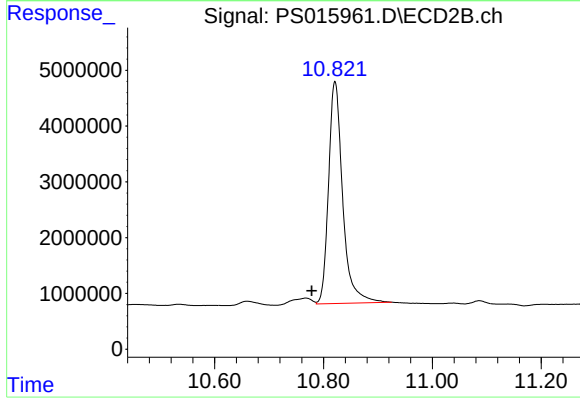

#16 DCPA

R.T.: 10.821 min
Delta R.T.: 0.043 min
Response: 71687397
Conc: 17.05 ng/ml