

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062923\
 Data File : PS023554.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jun 2023 07:58
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 29 15:46:05 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS060623.M
 Quant Title : 8080.M
 QLast Update : Tue Jun 06 13:00:04 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.489	0.000	1352223	0	<MDL	N.D. #
Target Compounds							
1) T	Dalapon	2.592f	0.000	660034	0	<MDL	N.D. #
2) T	3,5-DICHL...	5.867	0.000	258861	0	<MDL	N.D. #
3) T	4-Nitroph...	6.323	0.000	11904431	0	9.237	N.D. #
5) T	DICAMBA	6.636	7.006	155880	1204581	<MDL	<MDL #
6) T	MCPD	6.771	7.061f	508799	2084241	<MDL	1.166 #
7) T	MCPA	6.908	0.000	408164	0	<MDL	N.D. #
8) T	DICHLORPROP	7.266	7.645	21637415	2724230	10.486	4.404 #
9) T	2,4-D	7.462	0.000	32758396	0	13.407	N.D. #
10) T	Pentachlo...	7.699	0.000	2803519	0	<MDL	N.D. #
11) T	2,4,5-TP ...	8.201	0.000	159794	0	<MDL	N.D. #
12) T	2,4,5-T	8.497	9.082	3715253	2826917	<MDL	<MDL #
13) T	2,4-DB	8.993	0.000	8586580	0	3.647	N.D. #
14) T	DINOSEB	10.053	0.000	303021	0	<MDL	N.D. #
15) T	Picloram	9.907	10.879	163.0E6	49343284	9.391	10.812
16) T	DCPA	10.339	10.879	822464	49343284	<MDL	12.299 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062923\
Data File : PS023554.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jun 2023 07:58
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 29 15:46:05 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS060623.M
Quant Title : 8080.M
QLast Update : Tue Jun 06 13:00:04 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

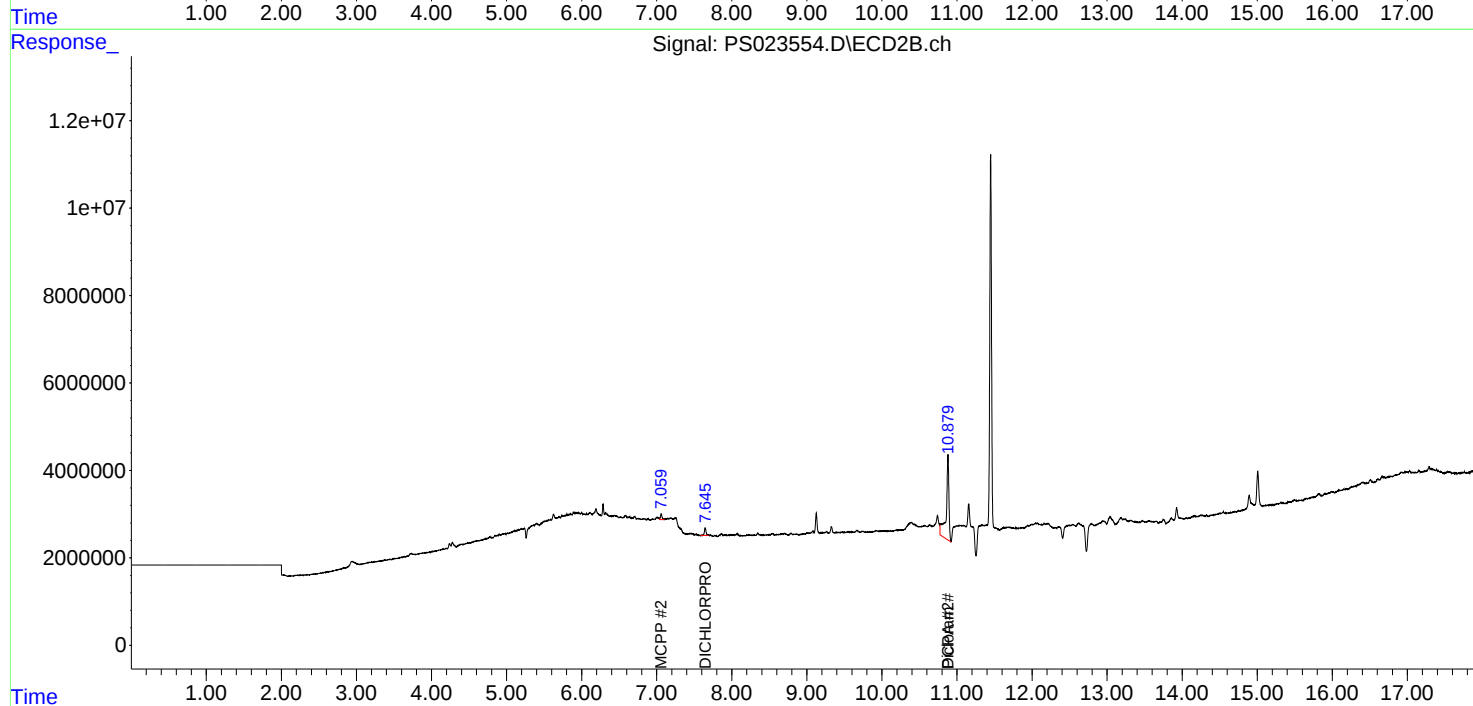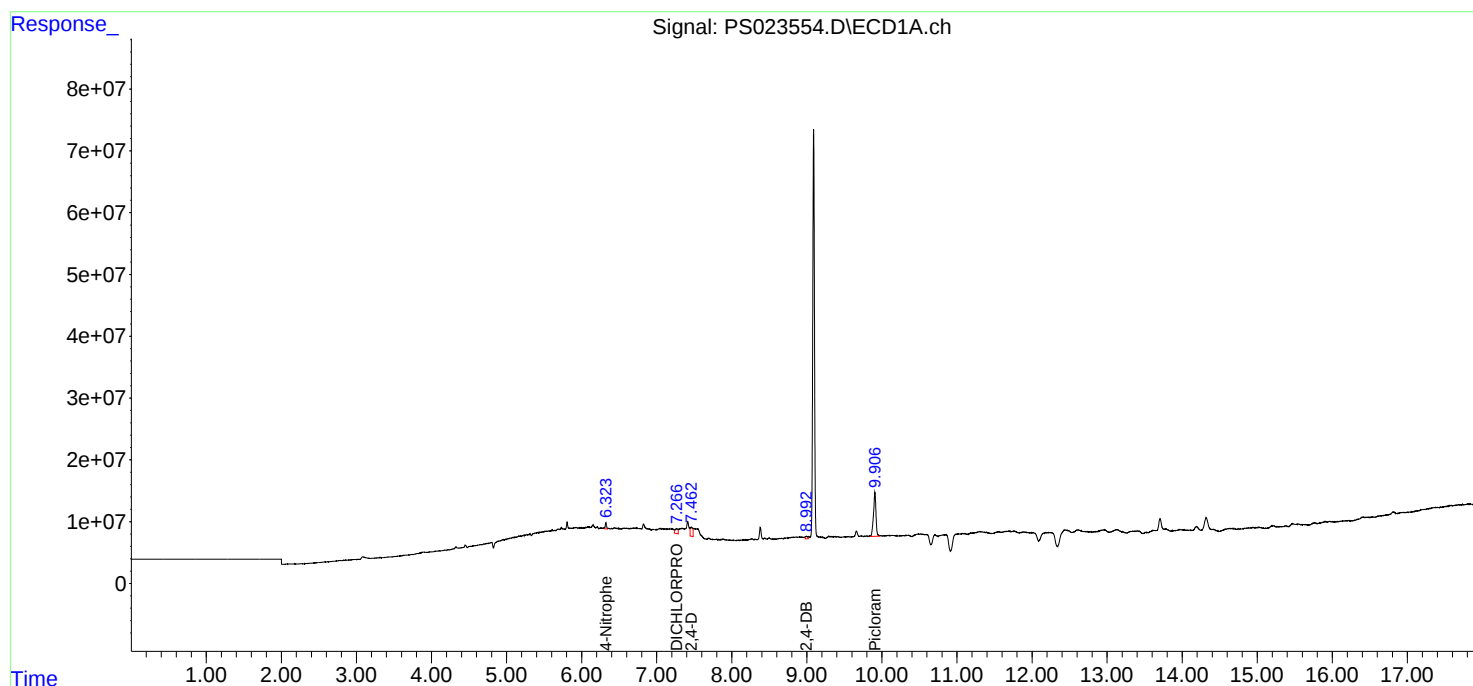


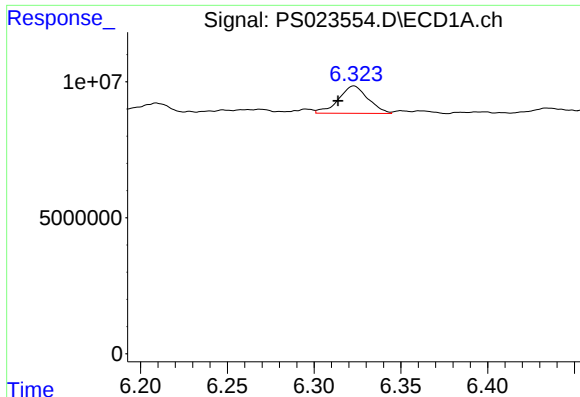

#3 4-Nitrophenol


R.T.: 6.323 min
Delta R.T.: 0.009 min
Response: 11904431
Conc: 9.24 ng/ml

Instrument :
ECD_S
ClientSampleId :

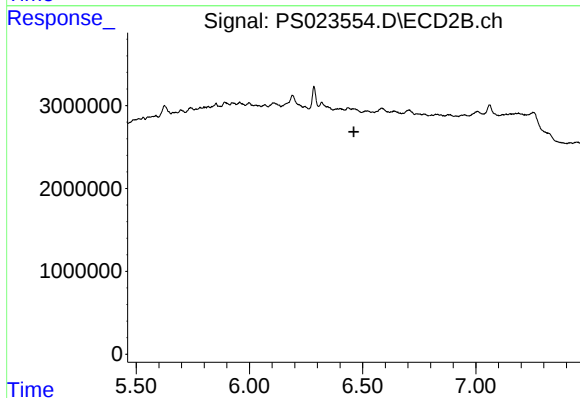


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.461 min
Response: 0
Conc: N.D.

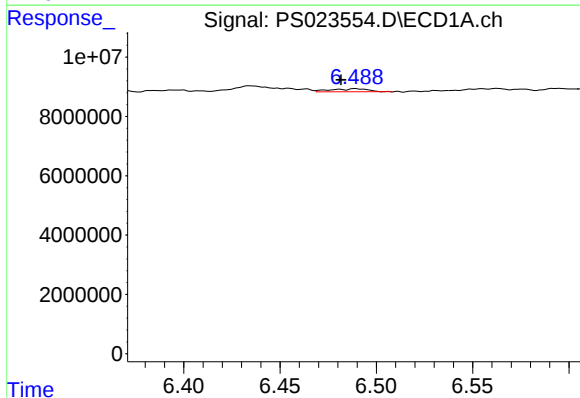


#4 2,4-DCAA

R.T.: 6.489 min
Delta R.T.: 0.007 min
Response: 1352223
Conc: N.D.

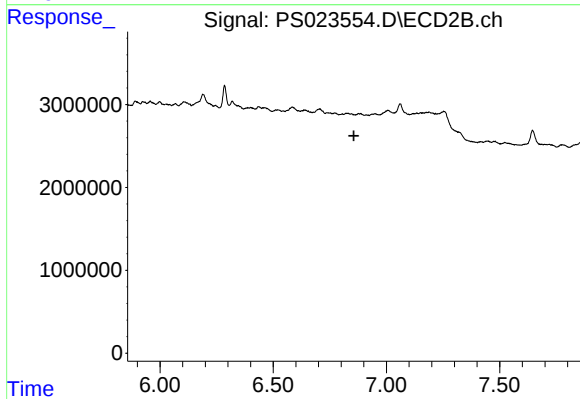

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 6.856 min
Response: 0
Conc: N.D.

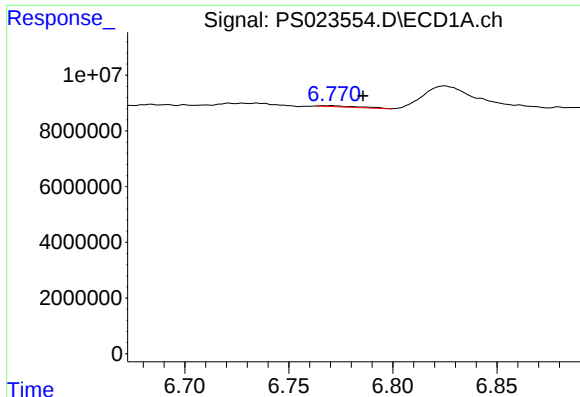

#6 MCPP


R.T.: 6.771 min
Delta R.T.: -0.015 min
Response: 508799
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

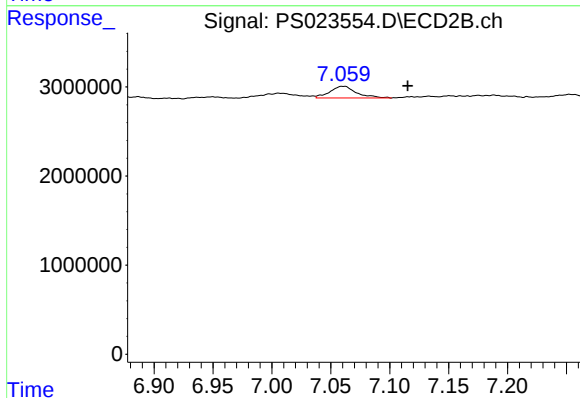


#6 MCPP

R.T.: 7.061 min
Delta R.T.: -0.055 min
Response: 2084241
Conc: 1.17 ug/ml

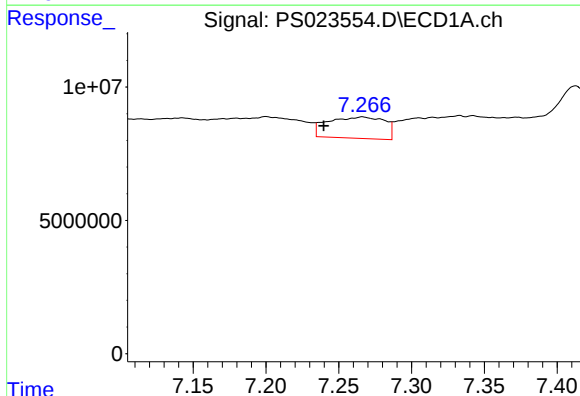


#8 DICHLORPROP

R.T.: 7.266 min
Delta R.T.: 0.027 min
Response: 21637415
Conc: 10.49 ng/ml

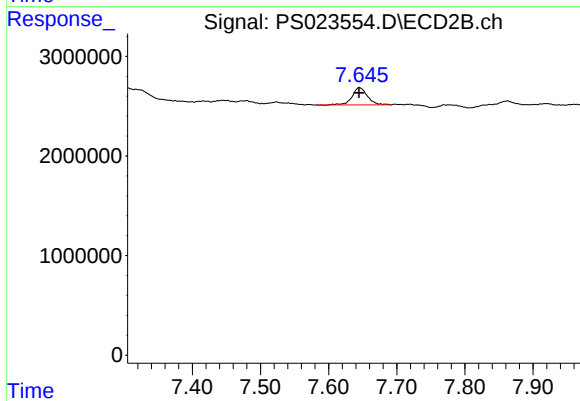

#8 DICHLORPROP


R.T.: 7.645 min
Delta R.T.: 0.000 min
Response: 2724230
Conc: 4.40 ng/ml

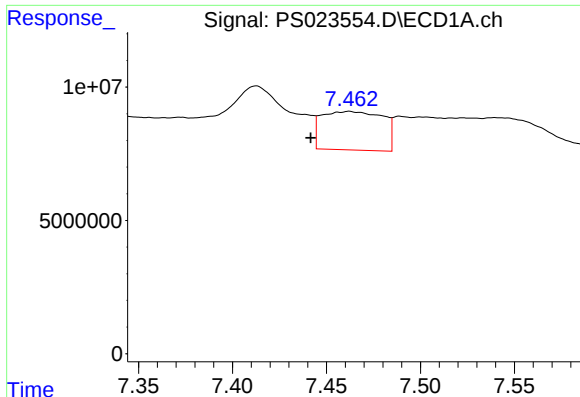

#9 2,4-D


R.T.: 7.462 min
Delta R.T.: 0.021 min
Response: 32758396
Conc: 13.41 ng/ml

Instrument :
ECD_S
ClientSampleId :

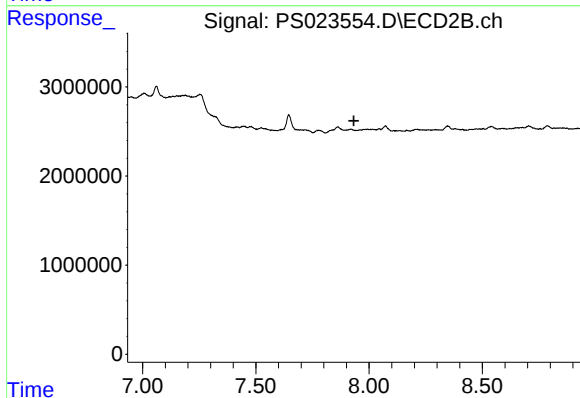


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.933 min
Response: 0
Conc: N.D.

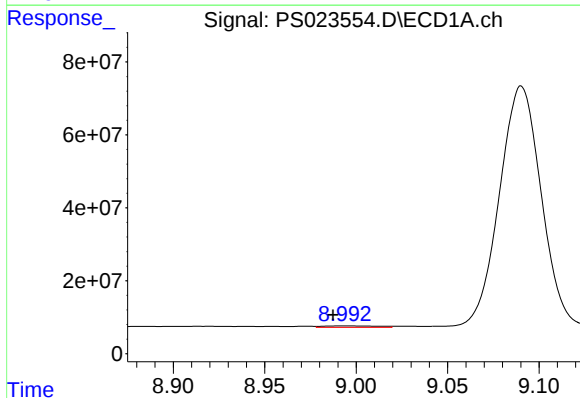


#13 2,4-DB

R.T.: 8.993 min
Delta R.T.: 0.006 min
Response: 8586580
Conc: 3.65 ng/ml

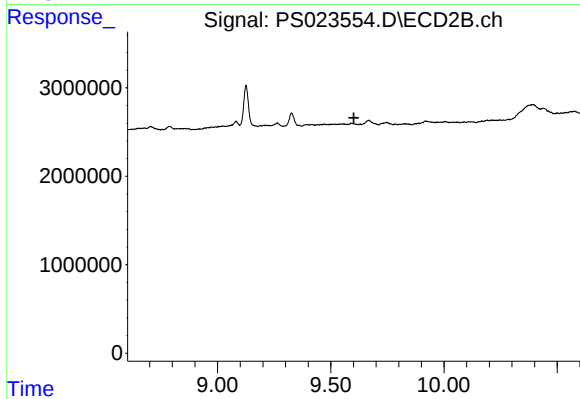

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 9.602 min
Response: 0
Conc: N.D.

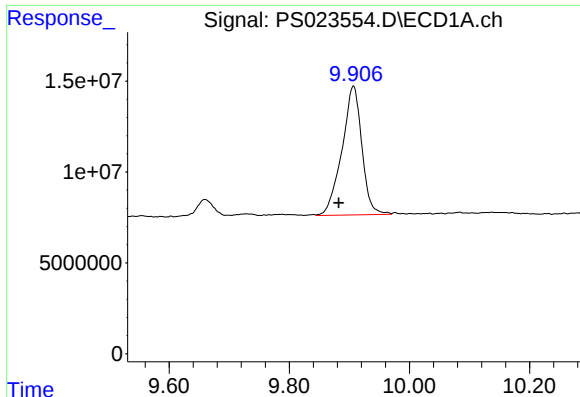

#15 Picloram


R.T.: 9.907 min
Delta R.T.: 0.024 min
Response: 162973874
Conc: 9.39 ng/ml

Instrument :
ECD_S
ClientSampleId :

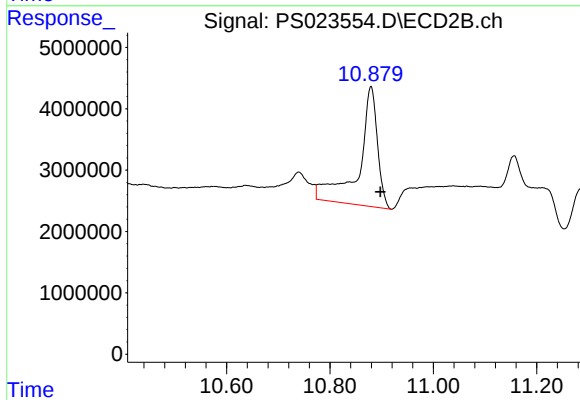


#15 Picloram

R.T.: 10.879 min
Delta R.T.: -0.018 min
Response: 49343284
Conc: 10.81 ng/ml

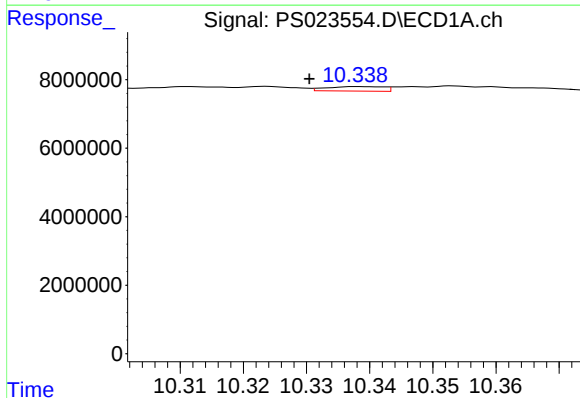

#16 DCPA

R.T.: 10.339 min
Delta R.T.: 0.008 min
Response: 822464
Conc: N.D.

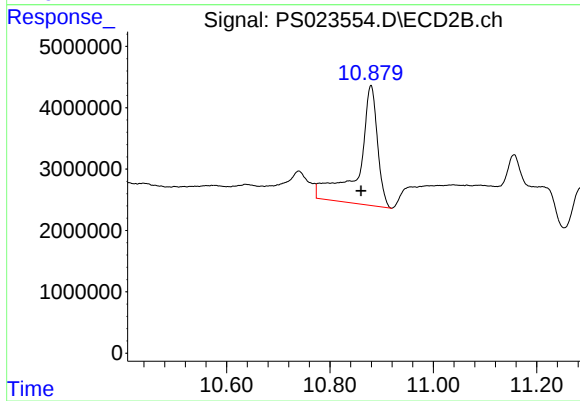

#16 DCPA

R.T.: 10.879 min
Delta R.T.: 0.019 min
Response: 49343284
Conc: 12.30 ng/ml