

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062923\
 Data File : PS023555.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jun 2023 08:22
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 29 15:46:23 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS060623.M
 Quant Title : 8080.M
 QLast Update : Tue Jun 06 13:00:04 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.479	6.845	964.7E6	264.7E6	545.242	466.210
Target Compounds							
1) T	Dalapon	2.570	0.000	950325	0	<MDL	N.D. #
2) T	3,5-DICHL...	5.799	0.000	3768066	0	1.403	N.D. #
3) T	4-Nitroph...	6.312	0.000	10543248	0	8.180	N.D. #
5) T	DICAMBA	6.626	7.062	180170	1549468	<MDL	<MDL #
6) T	MCP	6.813	7.062f	3348892	1549468	<MDL	<MDL #
7) T	MCPA	6.925	0.000	130816	0	<MDL	N.D. #
8) T	DICHLORPROP	7.238	7.647	2150739	2460147	1.042	3.977 #
9) T	2,4-D	7.401f	7.865f	16875491	1383858	6.907	1.995 #
10) T	Pentachlo...	7.672	0.000	1955911	0	<MDL	N.D. #
11) T	2,4,5-TP ...	8.210	0.000	3518646	0	<MDL	N.D. #
12) T	2,4,5-T	8.472	9.127	2859657	3800519	<MDL	1.240 #
13) T	2,4-DB	8.976	0.000	5635011	0	2.394	N.D. #
14) T	DINOSEB	10.056	0.000	813398	0	<MDL	N.D. #
15) T	Picloram	9.883	10.881	112.7E6	25076046	6.491	5.495
16) T	DCPA	10.326	10.881	3648563	25076046	<MDL	6.250 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062923\
Data File : PS023555.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jun 2023 08:22
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 29 15:46:23 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS060623.M
Quant Title : 8080.M
QLast Update : Tue Jun 06 13:00:04 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

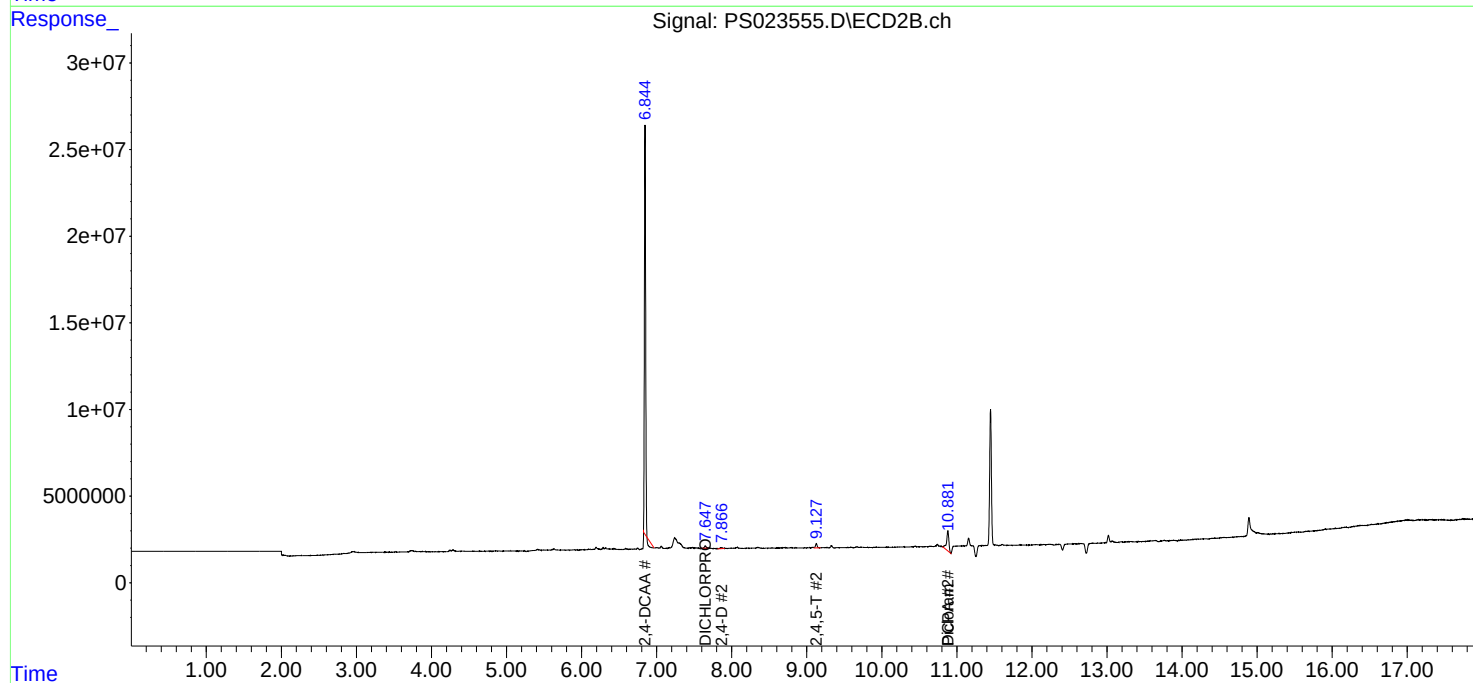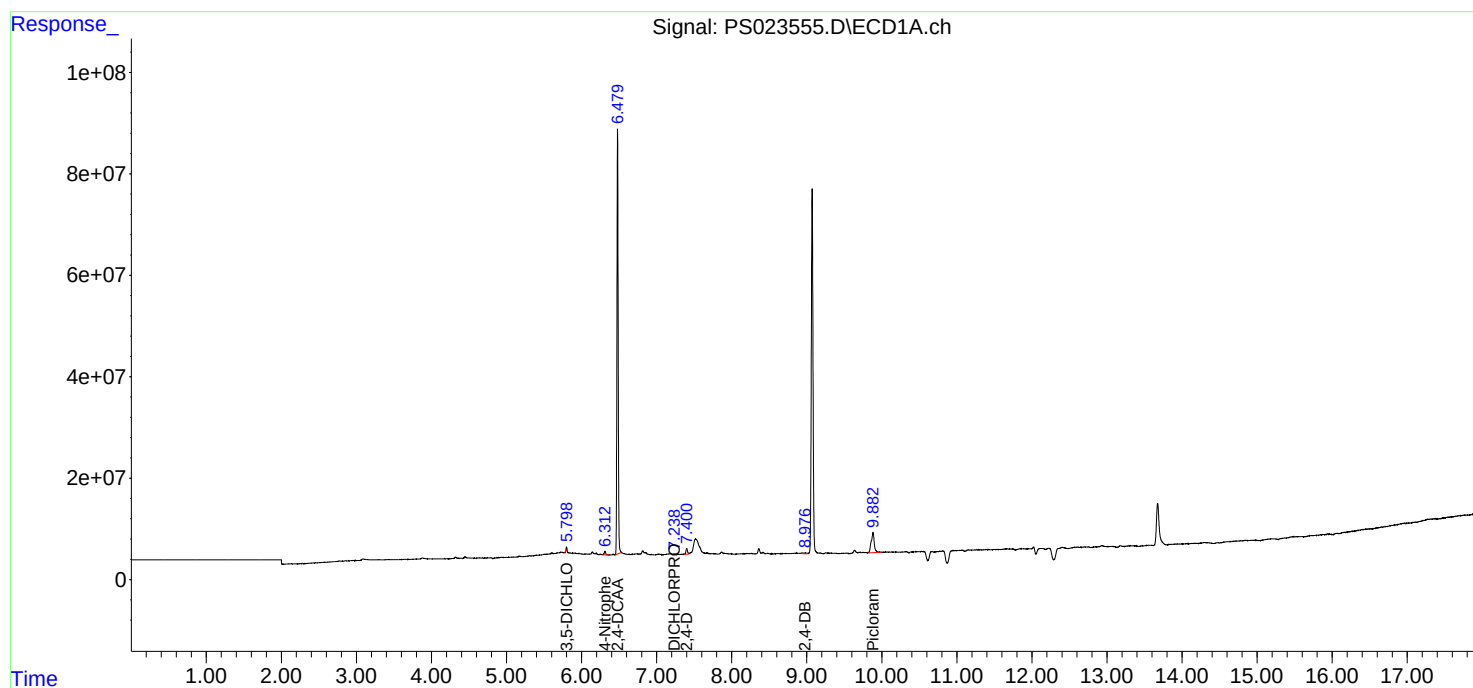


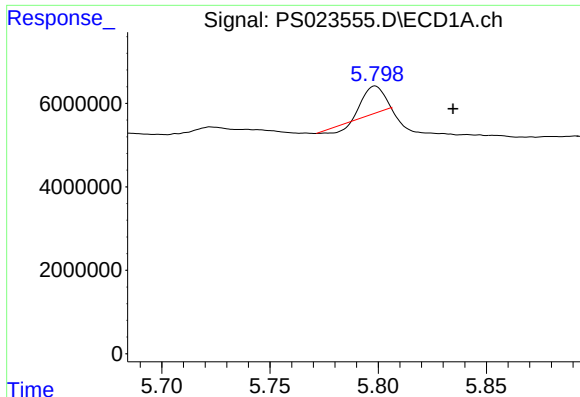

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.799 min
Delta R.T.: -0.036 min
Response: 3768066
Conc: 1.40 ng/ml

Instrument :
ECD_S
ClientSampleId :

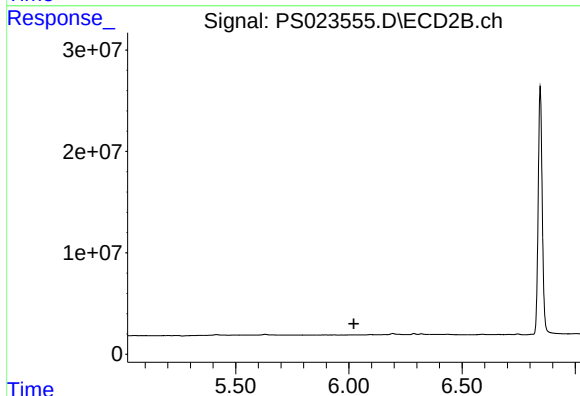


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.022 min
Response: 0
Conc: N.D.

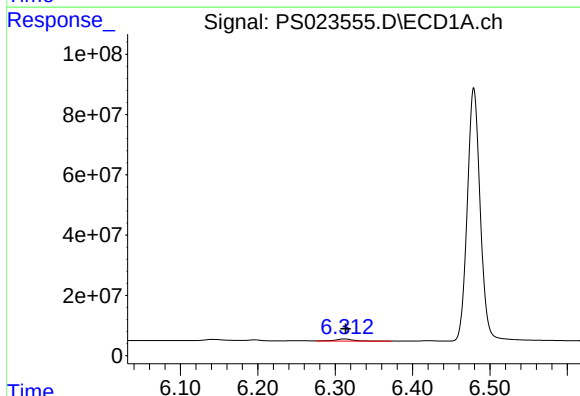


#3 4-Nitrophenol

R.T.: 6.312 min
Delta R.T.: -0.002 min
Response: 10543248
Conc: 8.18 ng/ml

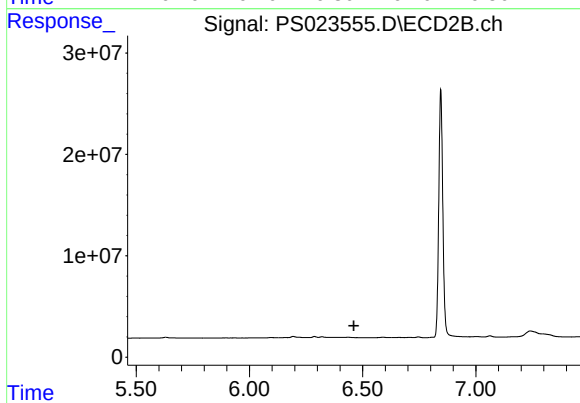

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 6.461 min
Response: 0
Conc: N.D.

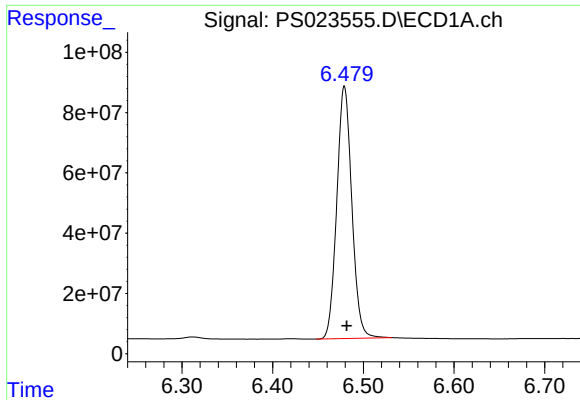

#4 2,4-DCAA


R.T.: 6.479 min
Delta R.T.: -0.002 min
Response: 964672177
Conc: 545.24 ng/ml

Instrument :
ECD_S
ClientSampleId :

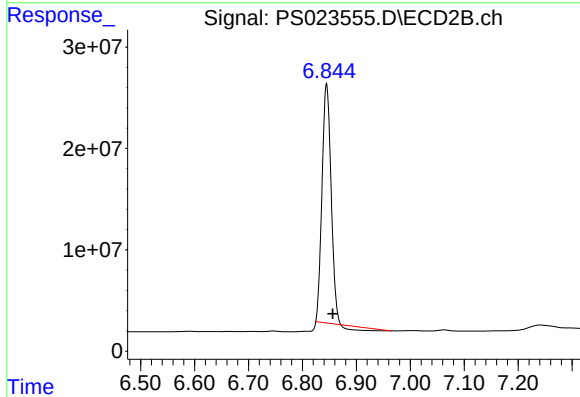


#4 2,4-DCAA

R.T.: 6.845 min
Delta R.T.: -0.011 min
Response: 264665125
Conc: 466.21 ng/ml

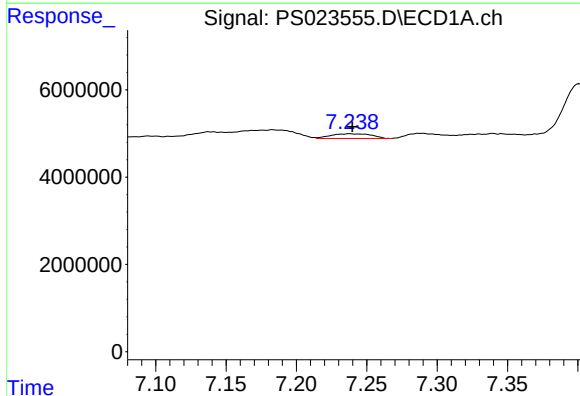


#8 DICHLORPROP

R.T.: 7.238 min
Delta R.T.: -0.002 min
Response: 2150739
Conc: 1.04 ng/ml

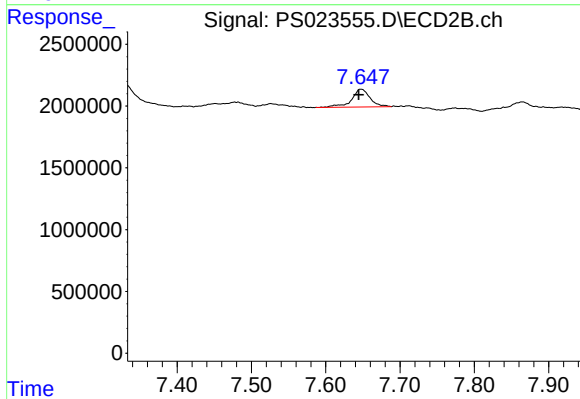

#8 DICHLORPROP


R.T.: 7.647 min
Delta R.T.: 0.003 min
Response: 2460147
Conc: 3.98 ng/ml

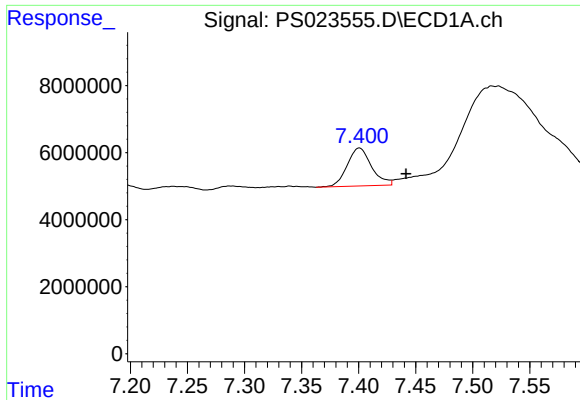

#9 2,4-D


R.T.: 7.401 min
Delta R.T.: -0.041 min
Response: 16875491
Conc: 6.91 ng/ml

Instrument :
ECD_S
ClientSampleId :

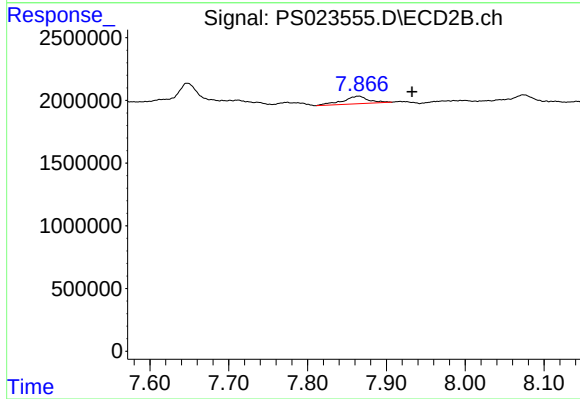


#9 2,4-D

R.T.: 7.865 min
Delta R.T.: -0.068 min
Response: 1383858
Conc: 2.00 ng/ml

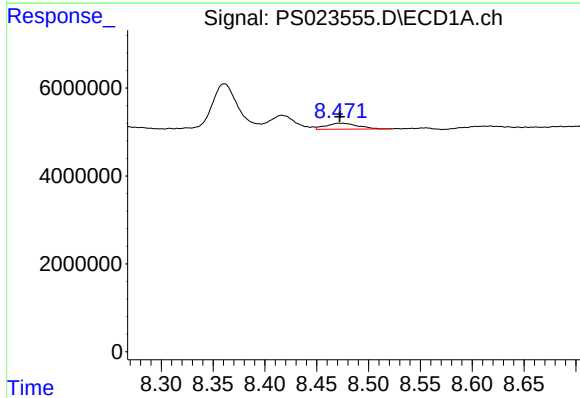


#12 2,4,5-T

R.T.: 8.472 min
Delta R.T.: 0.000 min
Response: 2859657
Conc: N.D.

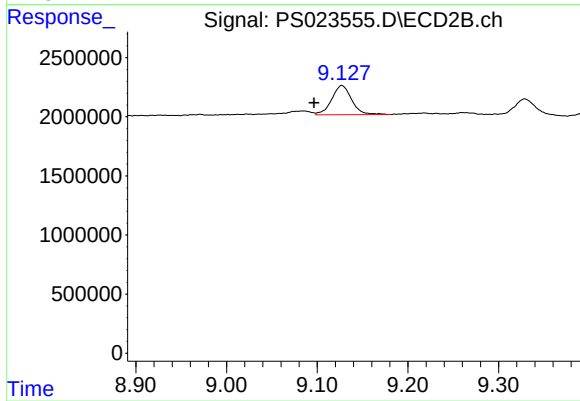

#12 2,4,5-T


R.T.: 9.127 min
Delta R.T.: 0.031 min
Response: 3800519
Conc: 1.24 ng/ml

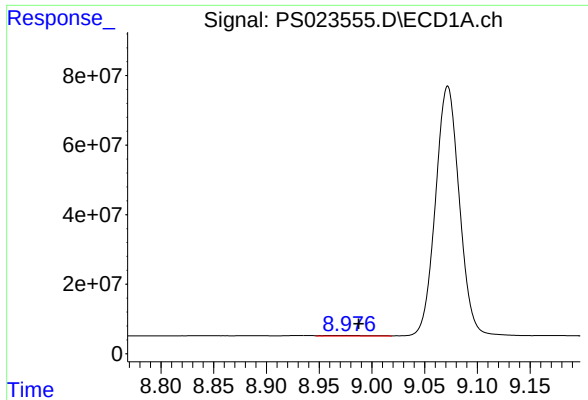

#13 2,4-DB


R.T.: 8.976 min
Delta R.T.: -0.011 min
Response: 5635011
Conc: 2.39 ng/ml

Instrument :
ECD_S
ClientSampleId :

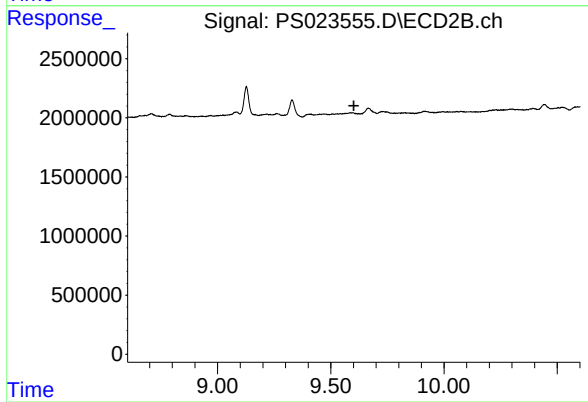


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.602 min
Response: 0
Conc: N.D.

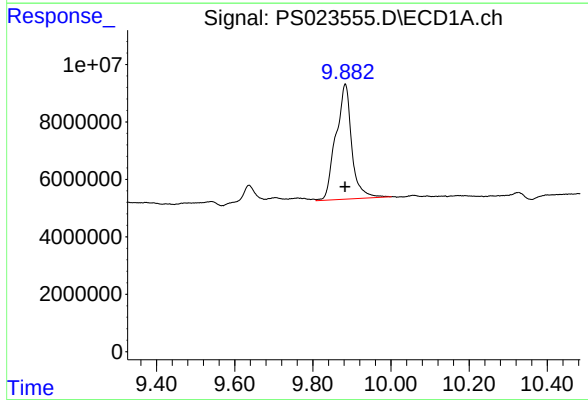


#15 Picloram

R.T.: 9.883 min
Delta R.T.: 0.000 min
Response: 112652423
Conc: 6.49 ng/ml

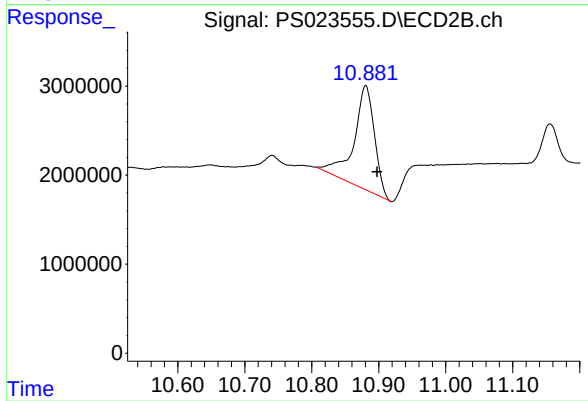

#15 Picloram


R.T.: 10.881 min
Delta R.T.: -0.017 min
Response: 25076046
Conc: 5.49 ng/ml

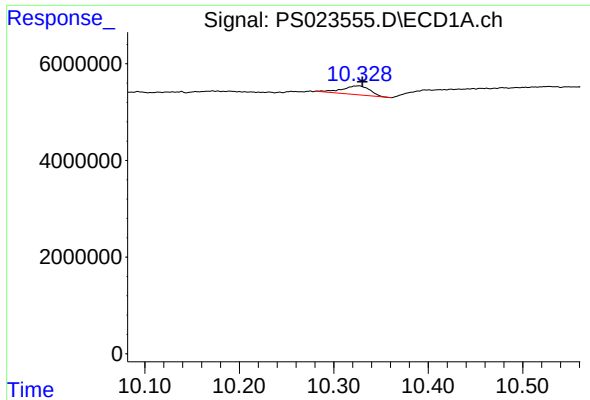

#16 DCPA

R.T.: 10.326 min
Delta R.T.: -0.004 min
Response: 3648563
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

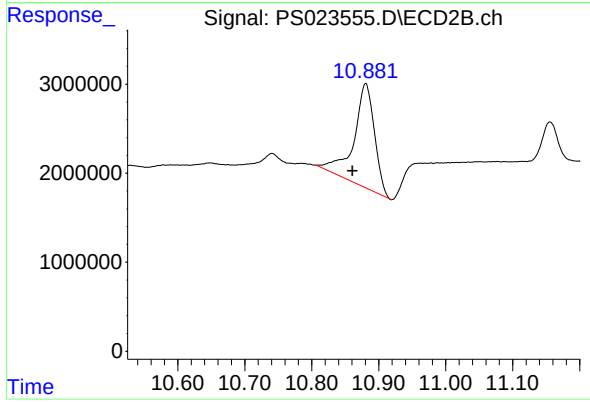

#16 DCPA

R.T.: 10.881 min
Delta R.T.: 0.020 min
Response: 25076046
Conc: 6.25 ng/ml