

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS063020\
 Data File : PS011002.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Jun 2020 15:49
 Operator : DD\AJ
 Sample : L2806-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 30 18:26:56 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062420.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 25 02:45:12 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.229	6.920	313.6E6	227.8E6	345.879	411.193
Target Compounds							
1) T	Dalapon	2.996	2.586	36819774	107.4E6	32.883	142.332 #
2) T	3,5-DICHL...	0.000	6.101	0	74319167	N.D.	89.237
5) T	DICAMBA	7.408	7.055	5582070	5735467	1.531	2.525 #
7) T	MCPA	7.694	7.465	56701876	50532451	14.238	18.309 #
8) T	DICHLORPROP	0.000	7.741	0	7740553	N.D.	13.184
10) T	Pentachlo...	8.710	0.000	9427395	0	<MDL	N.D. #
12) T	2,4,5-T	9.428	0.000	28702372	0	6.162	N.D. #
14) T	DINOSEB	11.168	0.000	9992833	0	2.790	N.D. #
15) T	Picloram	10.995	0.000	26736630	0	4.769	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS063020\
Data File : PS011002.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Jun 2020 15:49
Operator : DD\AJ
Sample : L2806-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 30 18:26:56 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062420.M
Quant Title : 8080.M
QLast Update : Thu Jun 25 02:45:12 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

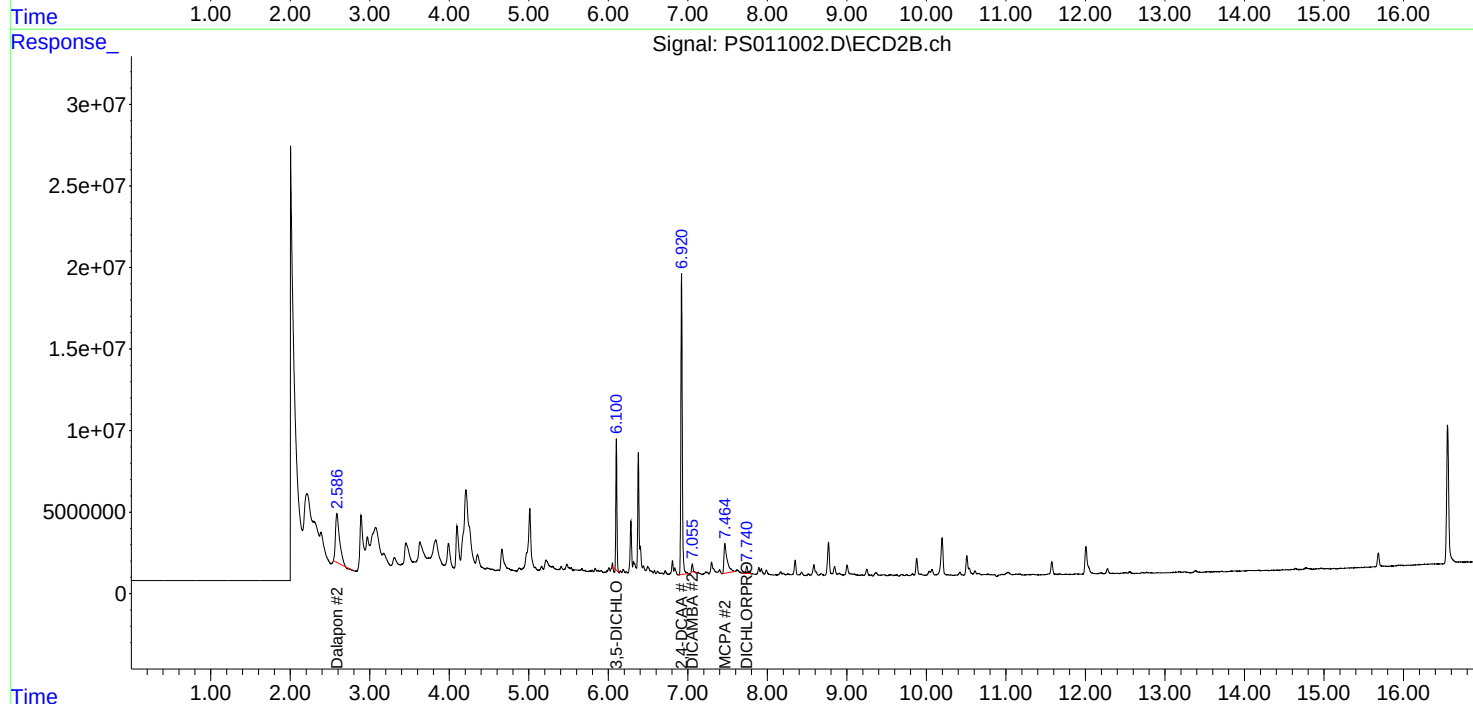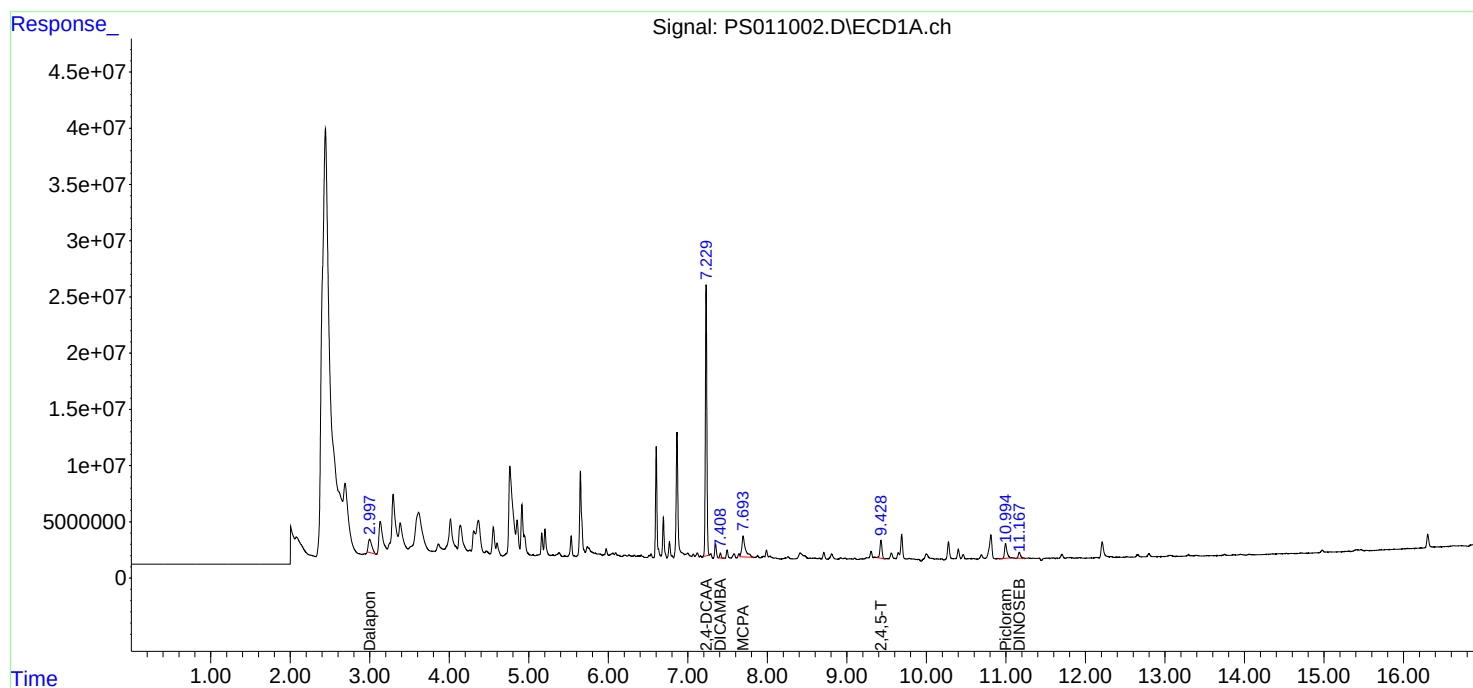


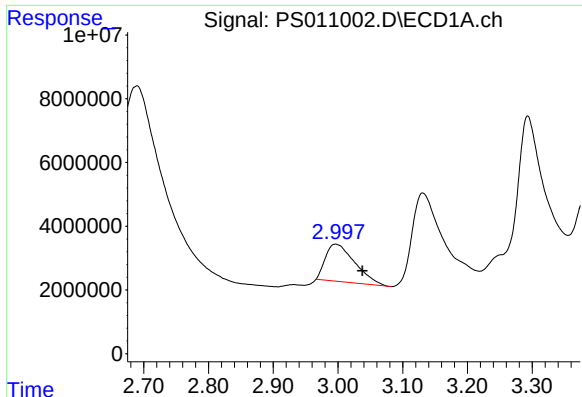

#1 Dalapon


R.T.: 2.996 min
Delta R.T.: -0.042 min
Response: 36819774
Conc: 32.88 ng/ml

Instrument :
ECD_S
ClientSampleId :

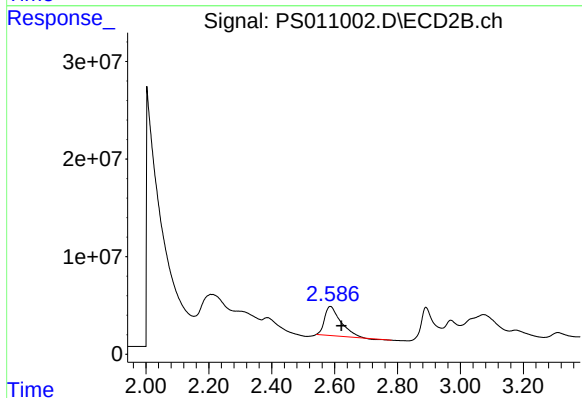


#1 Dalapon

R.T.: 2.586 min
Delta R.T.: -0.036 min
Response: 107369921
Conc: 142.33 ng/ml

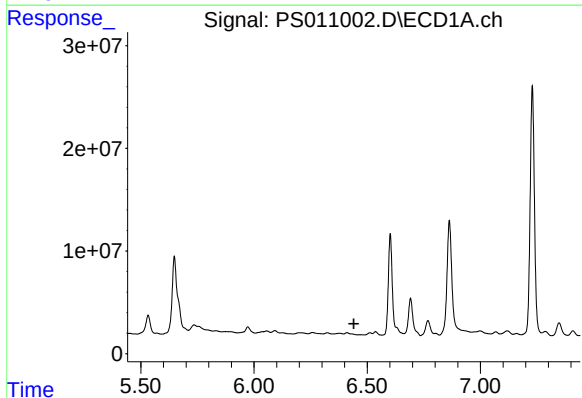


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.441 min
Response: 0
Conc: N.D.

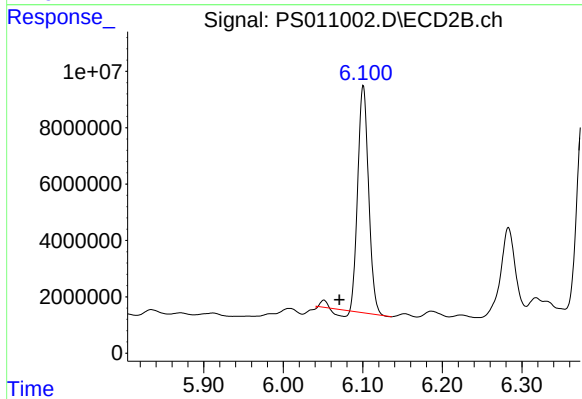

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.101 min
Delta R.T.: 0.030 min
Response: 74319167
Conc: 89.24 ng/ml

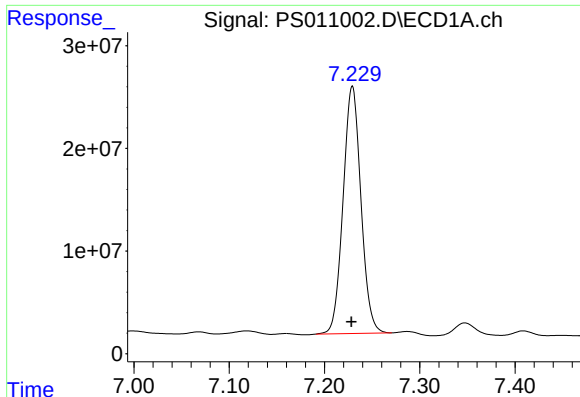

#4 2,4-DCAA


R.T.: 7.229 min
Delta R.T.: 0.000 min
Response: 313649458
Conc: 345.88 ng/ml

Instrument :
ECD_S
ClientSampleId :

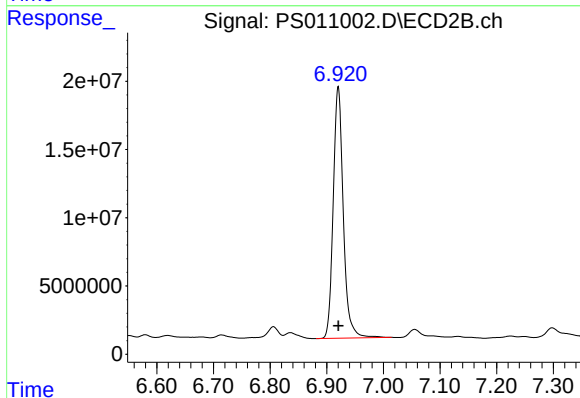


#4 2,4-DCAA

R.T.: 6.920 min
Delta R.T.: 0.000 min
Response: 227832043
Conc: 411.19 ng/ml

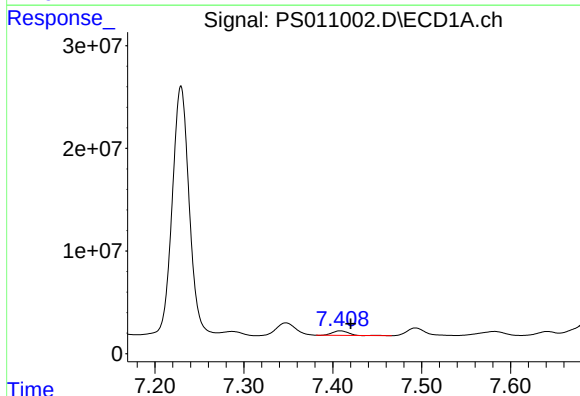


#5 DICAMBA

R.T.: 7.408 min
Delta R.T.: -0.012 min
Response: 5582070
Conc: 1.53 ng/ml

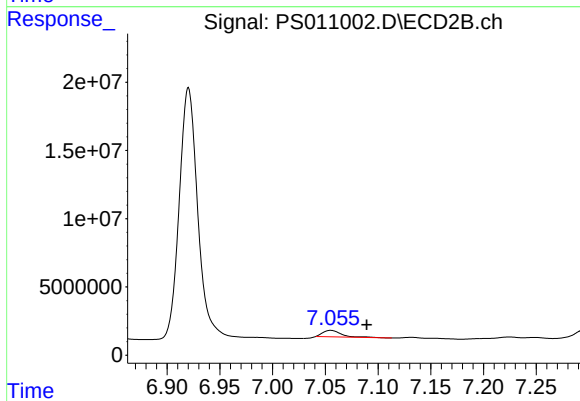

#5 DICAMBA


R.T.: 7.055 min
Delta R.T.: -0.034 min
Response: 5735467
Conc: 2.53 ng/ml

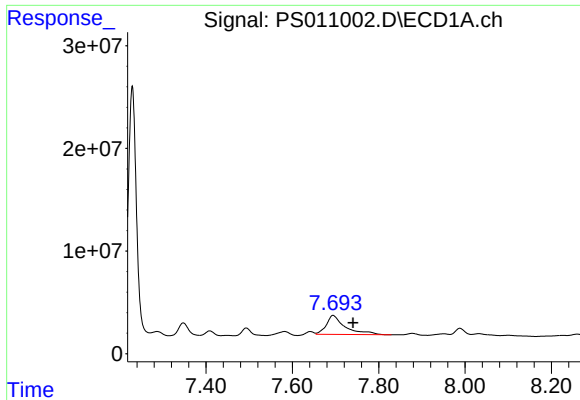

#7 MCPA


R.T.: 7.694 min
Delta R.T.: -0.046 min
Response: 56701876
Conc: 14.24 ug/ml

Instrument :
ECD_S
ClientSampleId :

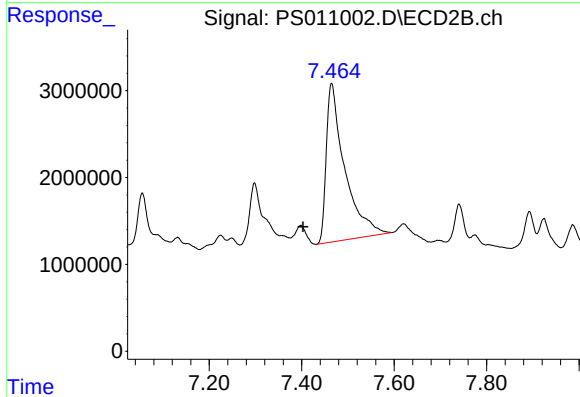


#7 MCPA

R.T.: 7.465 min
Delta R.T.: 0.062 min
Response: 50532451
Conc: 18.31 ug/ml

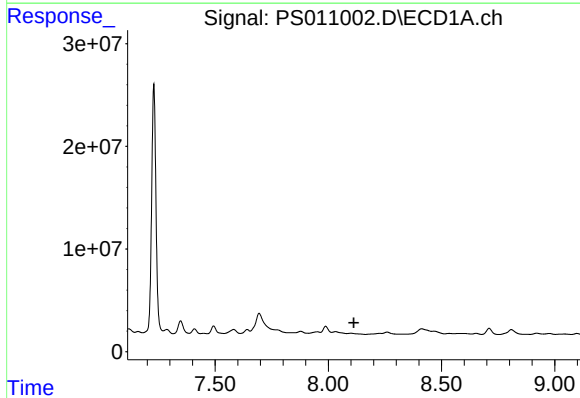


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.113 min
Response: 0
Conc: N.D.

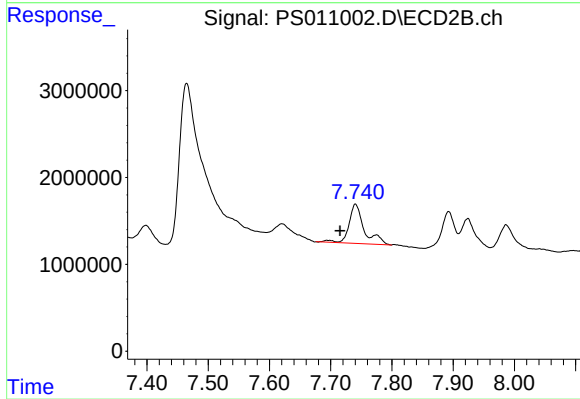

#8 DICHLORPROP


R.T.: 7.741 min
Delta R.T.: 0.025 min
Response: 7740553
Conc: 13.18 ng/ml

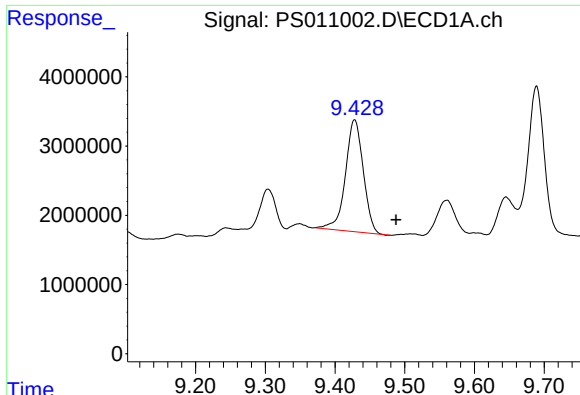

#12 2,4,5-T


R.T.: 9.428 min
Delta R.T.: -0.060 min
Response: 28702372
Conc: 6.16 ng/ml

Instrument :
ECD_S
ClientSampleId :

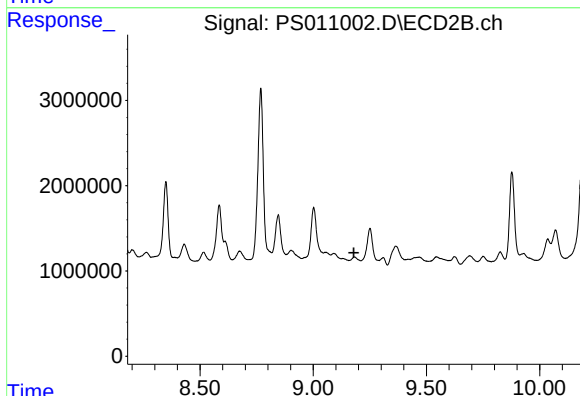


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.179 min
Response: 0
Conc: N.D.

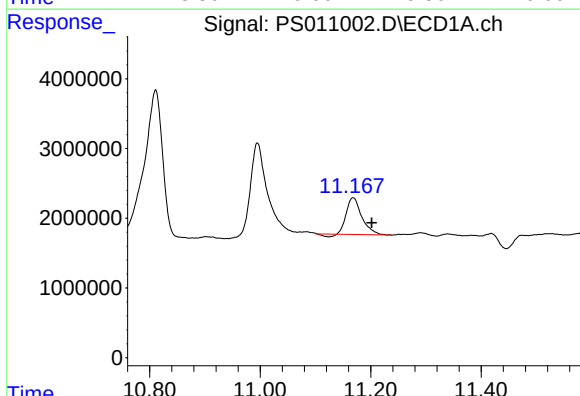


#14 DINOSEB

R.T.: 11.168 min
Delta R.T.: -0.034 min
Response: 9992833
Conc: 2.79 ng/ml

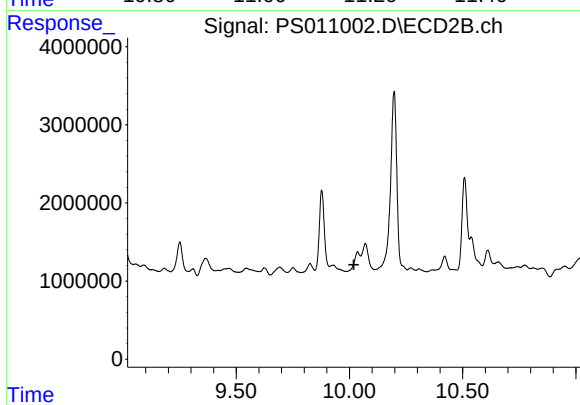

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 10.020 min
Response: 0
Conc: N.D.

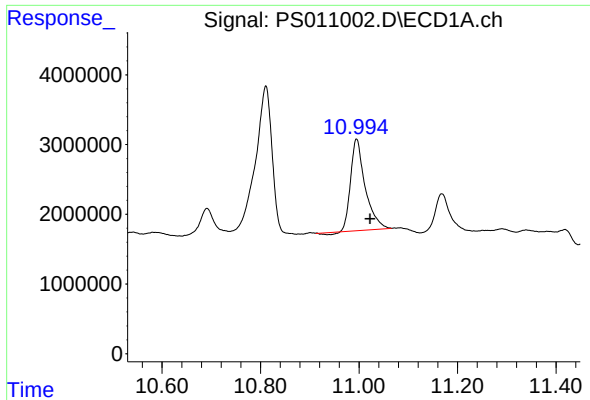

#15 Picloram

R.T.: 10.995 min
Delta R.T.: -0.027 min
Response: 26736630
Conc: 4.77 ng/ml

Instrument :
ECD_S
ClientSampleId :

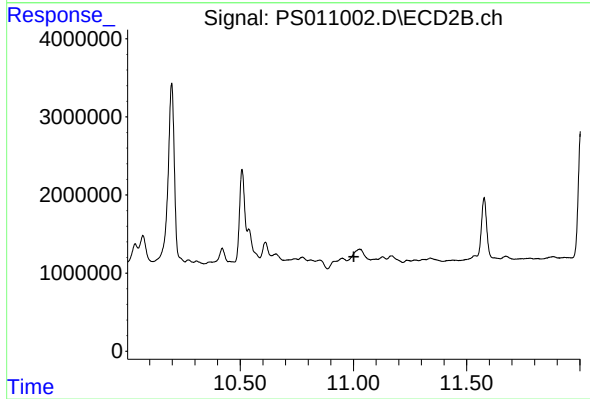

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 11.002 min
Response: 0
Conc: N.D.