

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS063020\
 Data File : PS011003.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Jun 2020 16:12
 Operator : DD\AJ
 Sample : L2819-08
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 30 18:27:09 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062420.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 25 02:45:12 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.229	6.920	310.3E6	224.3E6	342.161	404.777
Target Compounds							
1) T	Dalapon	2.997	2.585	39887943	100.6E6	35.623	133.421 #
2) T	3,5-DICHL...	0.000	6.101	0	76576273	N.D.	91.948
3) T	4-Nitroph...	7.120	0.000	7468570	0	18.710	N.D. #
5) T	DICAMBA	7.408	7.055	5444621	5421138	1.493	2.387 #
7) T	MCPA	7.696	7.466	51133387	45148670	12.840	16.358 #
10) T	Pentachlo...	8.710	0.000	9876578	0	<MDL	N.D. #
12) T	2,4,5-T	9.427	0.000	34478517	0	7.402	N.D. #
14) T	DINOSEB	11.168	10.066	10560497	11486747	2.949	5.517 #
15) T	Picloram	10.995	0.000	28526901	0	5.089	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS063020\
Data File : PS011003.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Jun 2020 16:12
Operator : DD\AJ
Sample : L2819-08
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 30 18:27:09 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062420.M
Quant Title : 8080.M
QLast Update : Thu Jun 25 02:45:12 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

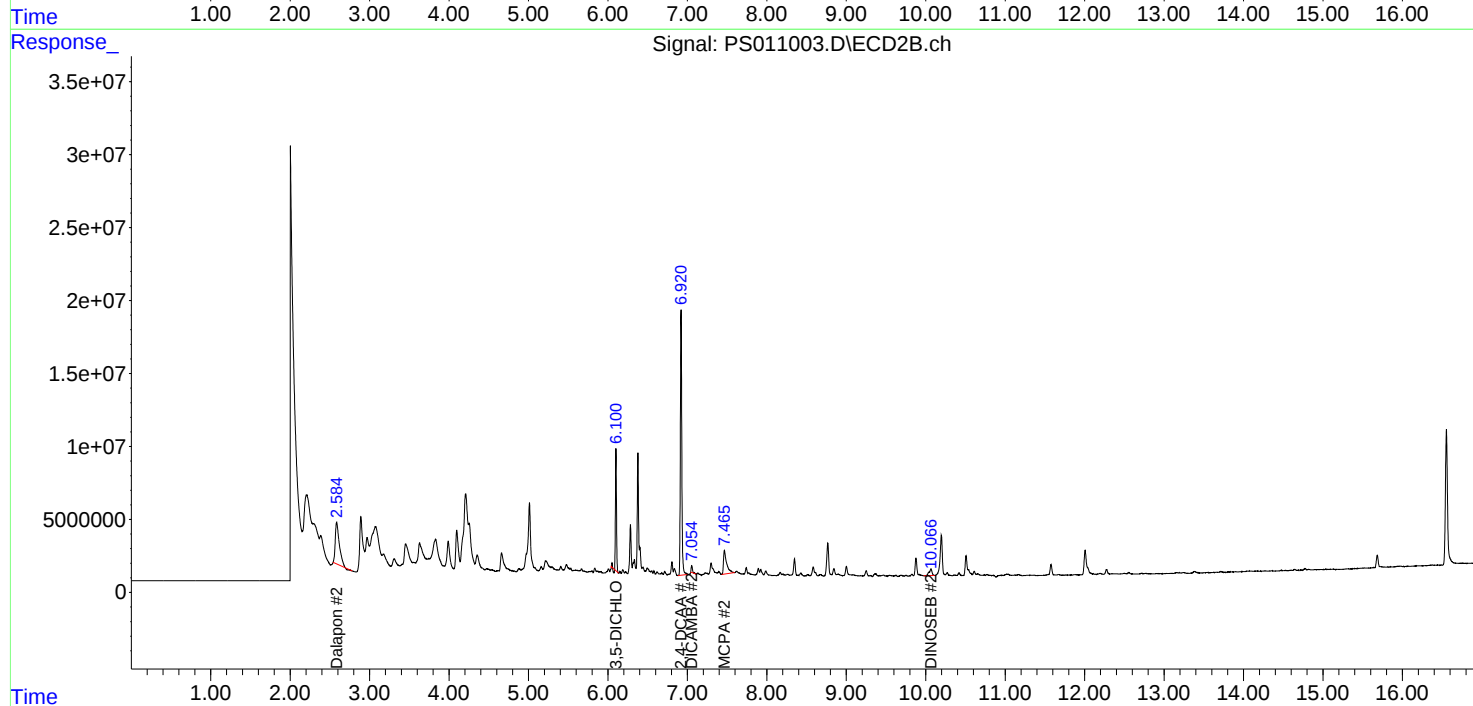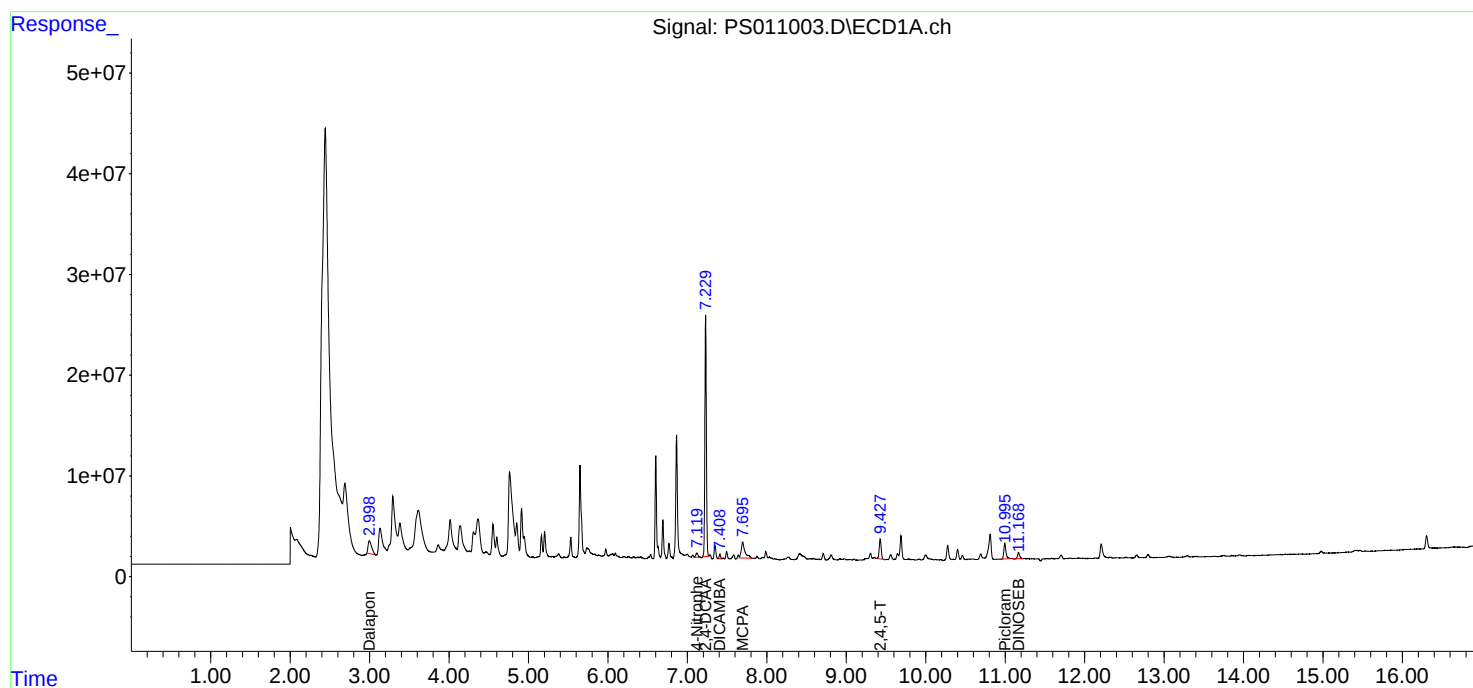


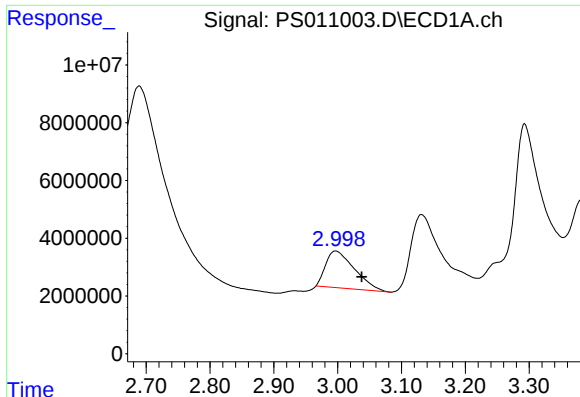

#1 Dalapon


R.T.: 2.997 min
Delta R.T.: -0.041 min
Response: 39887943
Conc: 35.62 ng/ml

Instrument :
ECD_S
ClientSampleId :

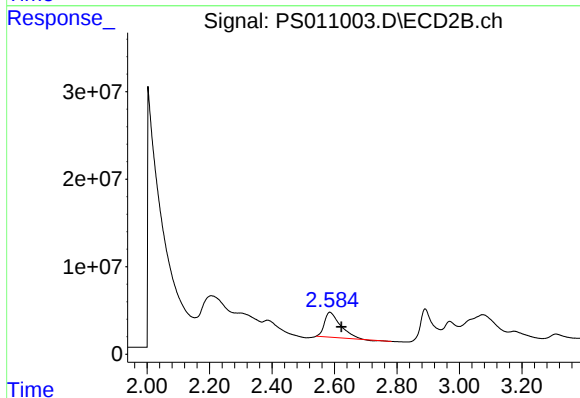


#1 Dalapon

R.T.: 2.585 min
Delta R.T.: -0.037 min
Response: 100647549
Conc: 133.42 ng/ml

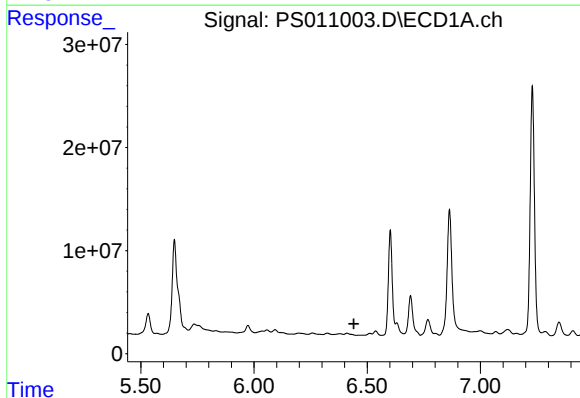


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.441 min
Response: 0
Conc: N.D.

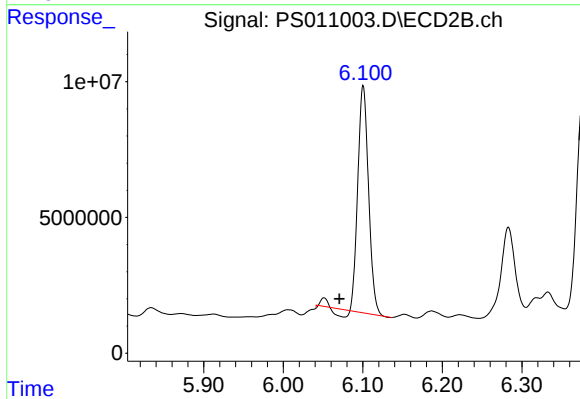

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.101 min
Delta R.T.: 0.030 min
Response: 76576273
Conc: 91.95 ng/ml

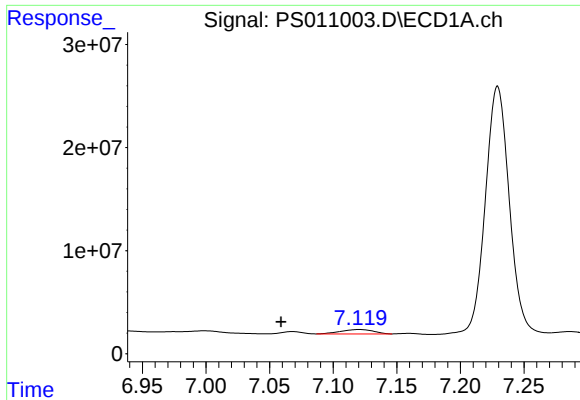

#3 4-Nitrophenol


R.T.: 7.120 min
Delta R.T.: 0.062 min
Response: 7468570
Conc: 18.71 ng/ml

Instrument :
ECD_S
ClientSampleId :

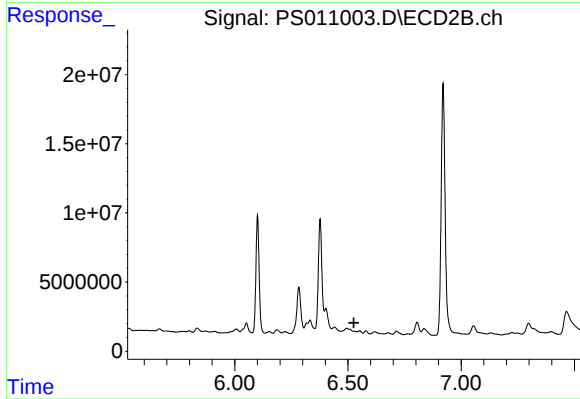


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.526 min
Response: 0
Conc: N.D.

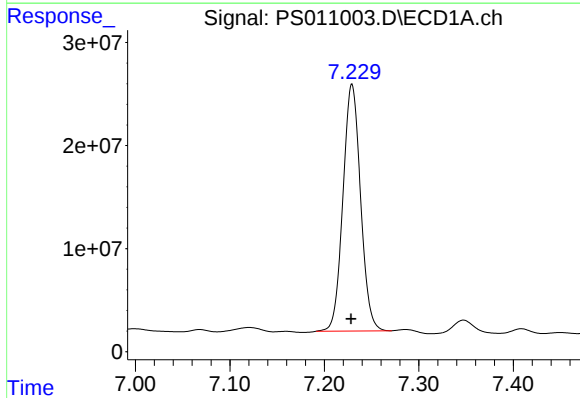


#4 2,4-DCAA

R.T.: 7.229 min
Delta R.T.: 0.000 min
Response: 310277939
Conc: 342.16 ng/ml

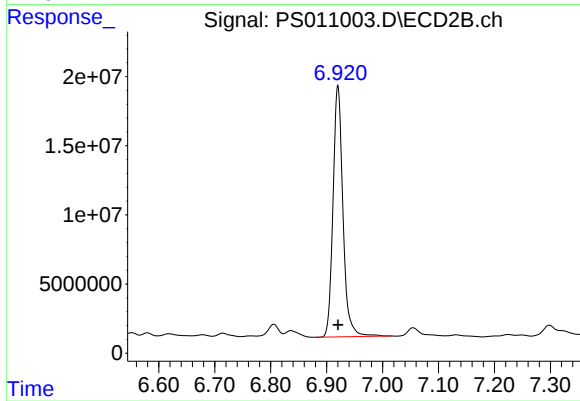

#4 2,4-DCAA


R.T.: 6.920 min
Delta R.T.: 0.000 min
Response: 224277096
Conc: 404.78 ng/ml

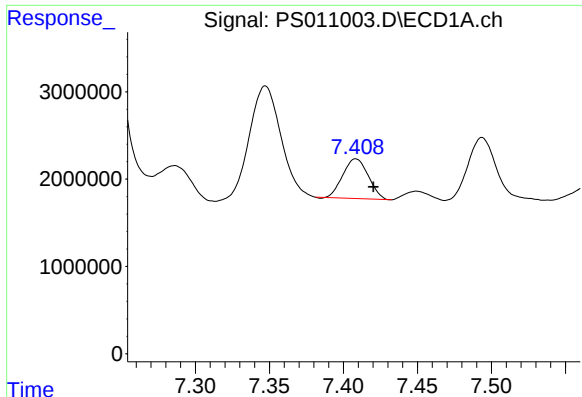

#5 DICAMBA


R.T.: 7.408 min
Delta R.T.: -0.012 min
Response: 5444621
Conc: 1.49 ng/ml

Instrument :
ECD_S
ClientSampleId :

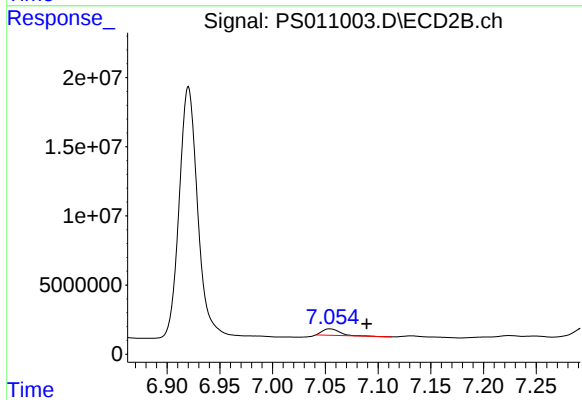


#5 DICAMBA

R.T.: 7.055 min
Delta R.T.: -0.035 min
Response: 5421138
Conc: 2.39 ng/ml

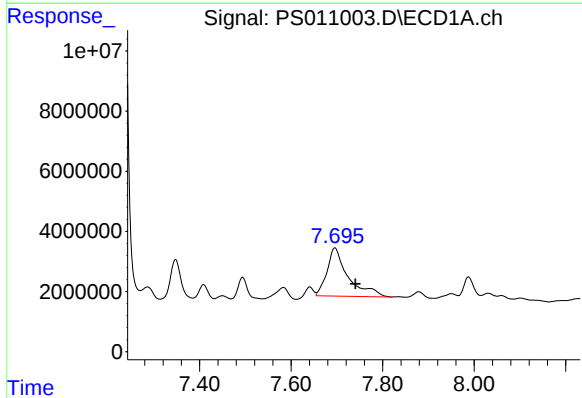


#7 MCPA

R.T.: 7.696 min
Delta R.T.: -0.045 min
Response: 51133387
Conc: 12.84 ug/ml

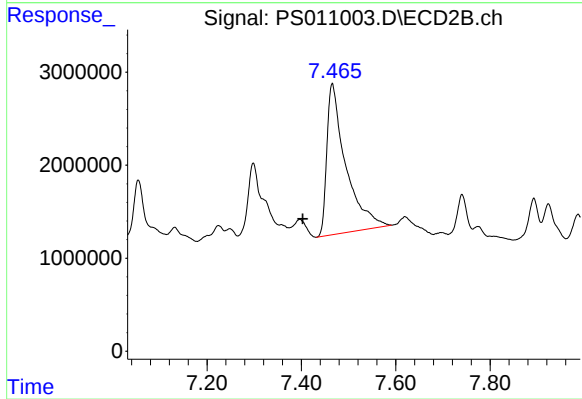

#7 MCPA


R.T.: 7.466 min
Delta R.T.: 0.063 min
Response: 45148670
Conc: 16.36 ug/ml

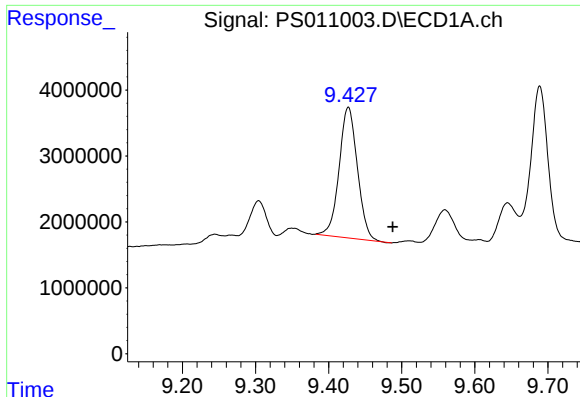

#12 2,4,5-T


R.T.: 9.427 min
Delta R.T.: -0.061 min
Response: 34478517
Conc: 7.40 ng/ml

Instrument :
ECD_S
ClientSampleId :

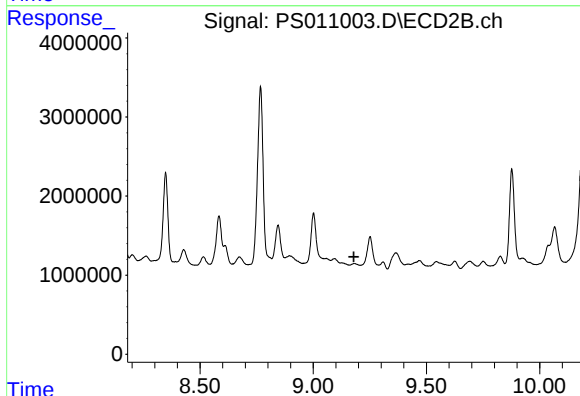


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.179 min
Response: 0
Conc: N.D.

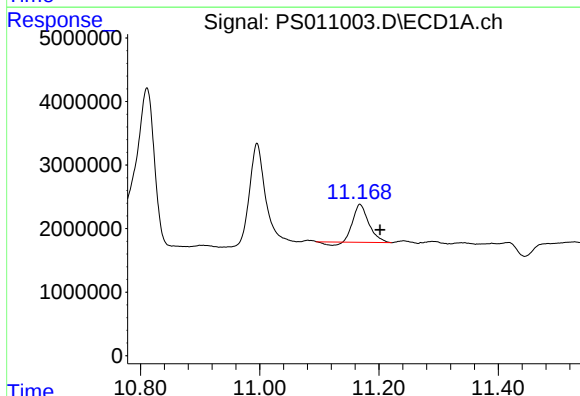


#14 DINOSEB

R.T.: 11.168 min
Delta R.T.: -0.034 min
Response: 10560497
Conc: 2.95 ng/ml

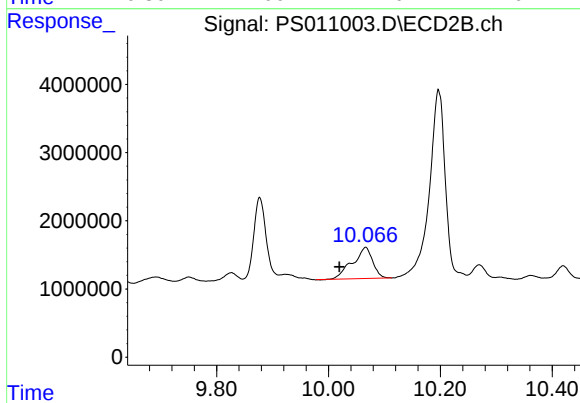

#14 DINOSEB


R.T.: 10.066 min
Delta R.T.: 0.047 min
Response: 11486747
Conc: 5.52 ng/ml

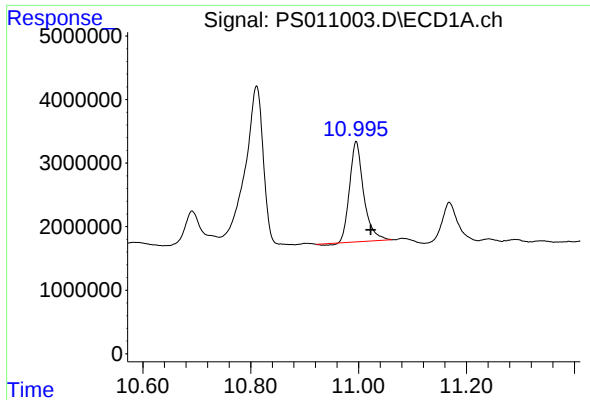

#15 Picloram

R.T.: 10.995 min
Delta R.T.: -0.027 min
Response: 28526901
Conc: 5.09 ng/ml

Instrument :
ECD_S
ClientSampleId :

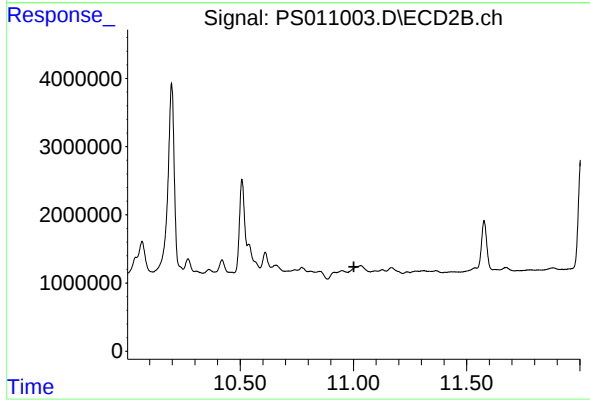

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 11.002 min
Response: 0
Conc: N.D.