

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS063020\
 Data File : PS011006.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Jun 2020 17:21
 Operator : DD\AJ
 Sample : PB129859BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 30 18:37:36 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062420.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 25 02:45:12 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.229	6.920	470.2E6	320.0E6	518.550	577.559
Target Compounds							
1) T	Dalapon	2.995	2.585	39428304	132.0E6	35.213	175.042 #
2) T	3,5-DICHL...	0.000	6.100	0	61177889	N.D.	73.458
3) T	4-Nitroph...	7.004	0.000	5340488	0	13.379	N.D. #
6) T	MCP	7.583	0.000	6512740	0	2.284	N.D. #
7) T	MCPA	7.777	7.384	56306480	45784251	14.139	16.589
9) T	2,4-D	0.000	7.986	0	7416908	N.D.	10.263
10) T	Pentachlo...	8.709	0.000	15624340	0	1.257	N.D. #
12) T	2,4,5-T	9.508	0.000	7520135	0	1.614	N.D. #
14) T	DINOSEB	11.169	0.000	12990879	0	3.627	N.D. #
15) T	Picloram	10.995	0.000	20235450	0	3.610	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS063020\
Data File : PS011006.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Jun 2020 17:21
Operator : DD\AJ
Sample : PB129859BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 30 18:37:36 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062420.M
Quant Title : 8080.M
QLast Update : Thu Jun 25 02:45:12 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

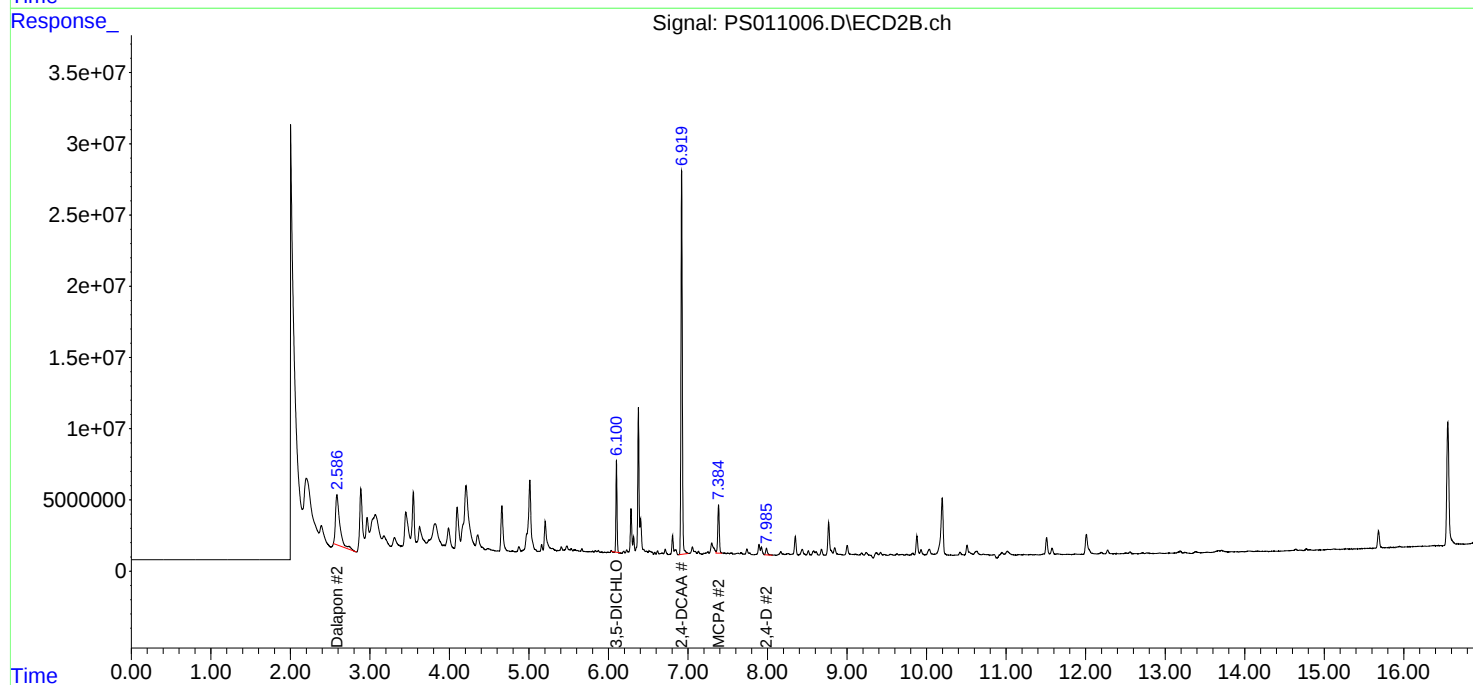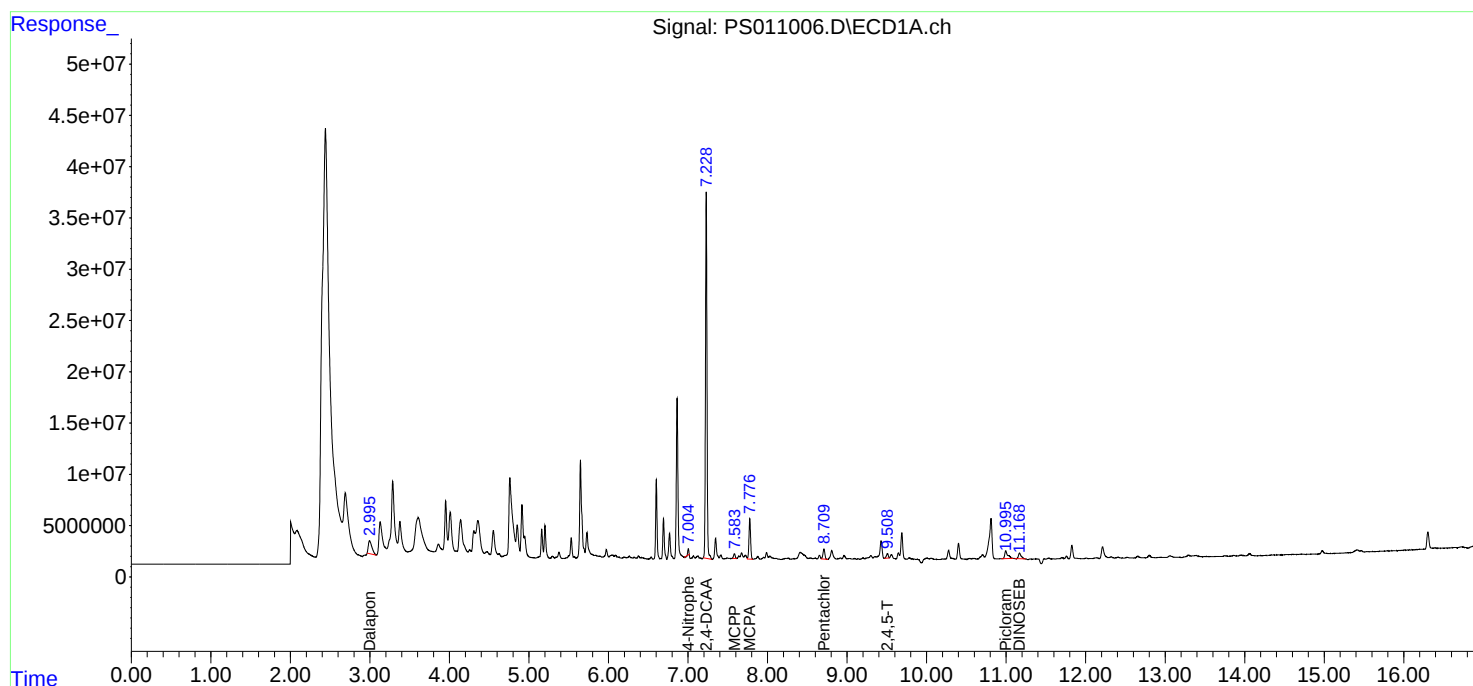


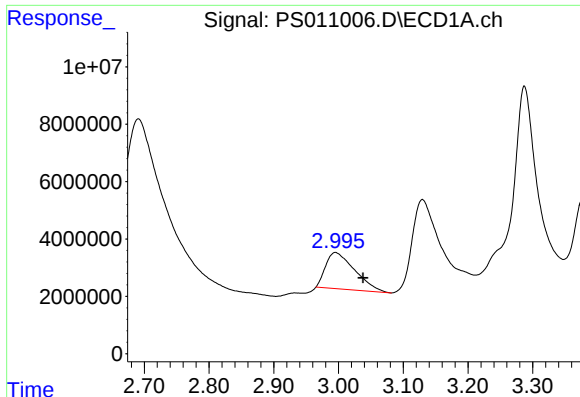

#1 Dalapon


R.T.: 2.995 min
Delta R.T.: -0.043 min
Response: 39428304
Conc: 35.21 ng/ml

Instrument :
ECD_S
ClientSampleId :

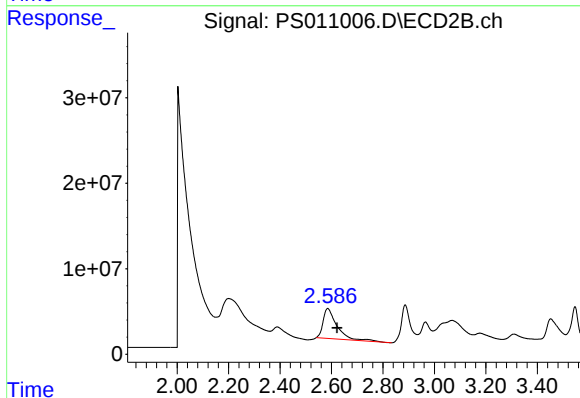


#1 Dalapon

R.T.: 2.585 min
Delta R.T.: -0.036 min
Response: 132044962
Conc: 175.04 ng/ml

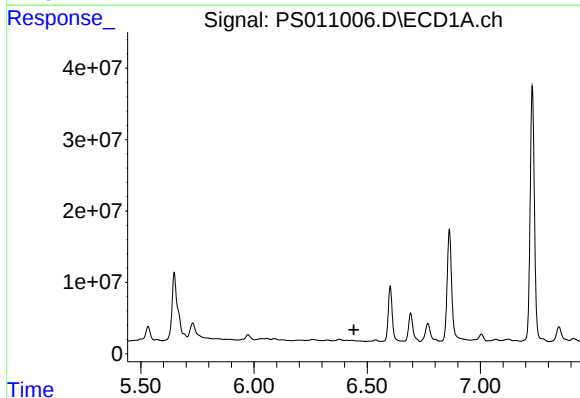


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.441 min
Response: 0
Conc: N.D.

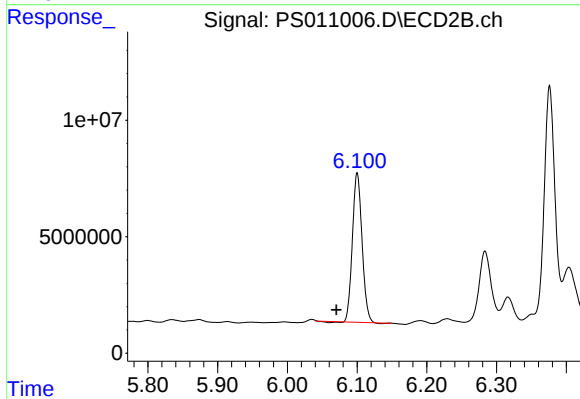

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.100 min
Delta R.T.: 0.030 min
Response: 61177889
Conc: 73.46 ng/ml

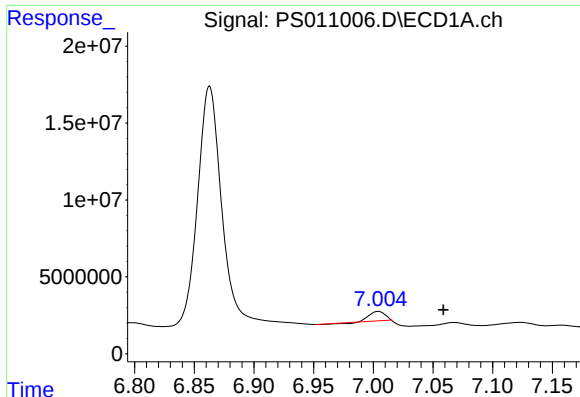

#3 4-Nitrophenol


R.T.: 7.004 min
Delta R.T.: -0.055 min
Response: 5340488
Conc: 13.38 ng/ml

Instrument :
ECD_S
ClientSampleId :

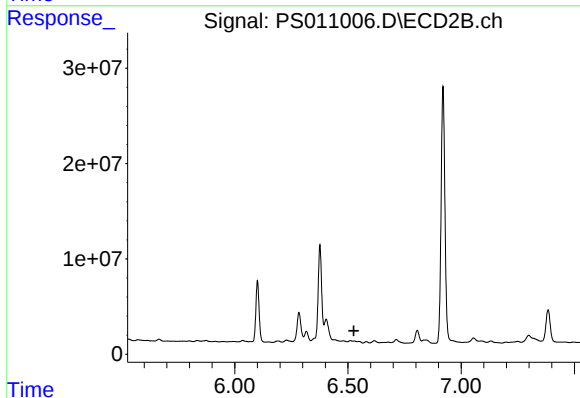


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.526 min
Response: 0
Conc: N.D.

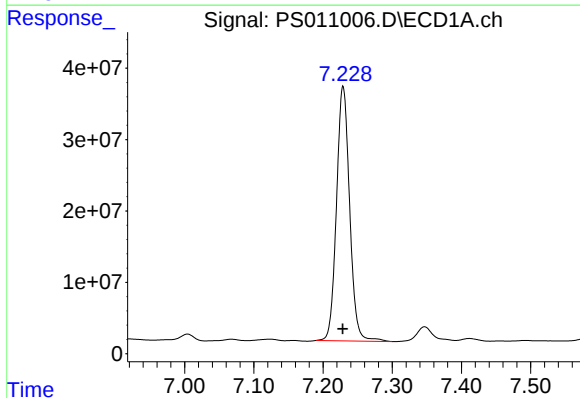


#4 2,4-DCAA

R.T.: 7.229 min
Delta R.T.: 0.000 min
Response: 470230966
Conc: 518.55 ng/ml

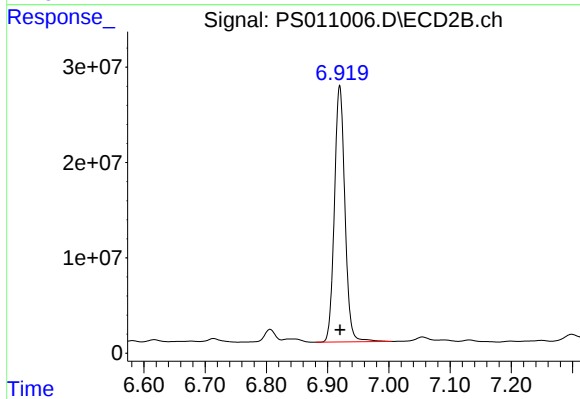

#4 2,4-DCAA


R.T.: 6.920 min
Delta R.T.: 0.000 min
Response: 320011533
Conc: 577.56 ng/ml

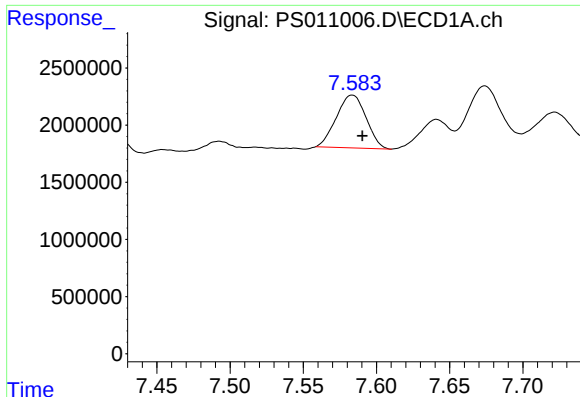

#6 MCPP


R.T.: 7.583 min
Delta R.T.: -0.007 min
Response: 6512740
Conc: 2.28 ug/ml

Instrument :
ECD_S
ClientSampleId :

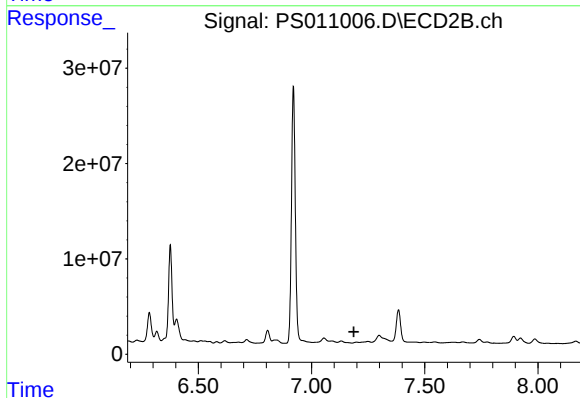


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 7.187 min
Response: 0
Conc: N.D.

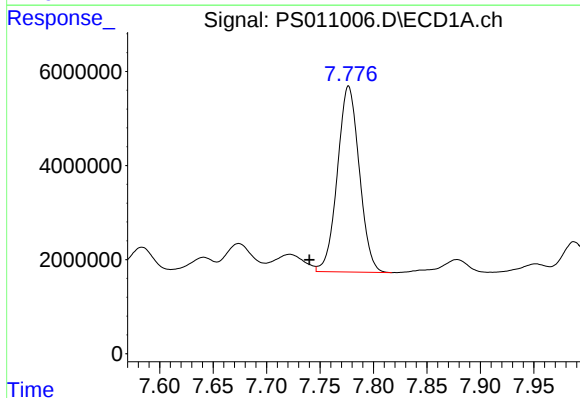


#7 MCPA

R.T.: 7.777 min
Delta R.T.: 0.037 min
Response: 56306480
Conc: 14.14 ug/ml

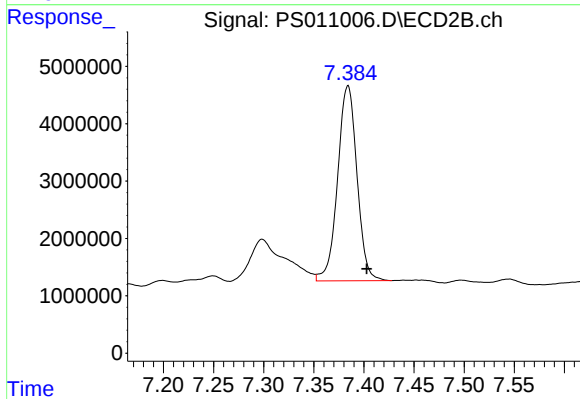

#7 MCPA


R.T.: 7.384 min
Delta R.T.: -0.019 min
Response: 45784251
Conc: 16.59 ug/ml

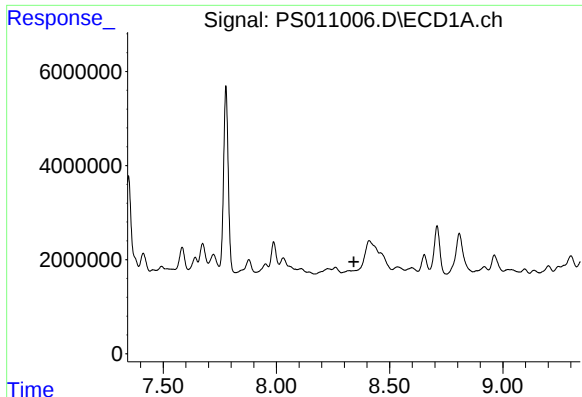

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.342 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

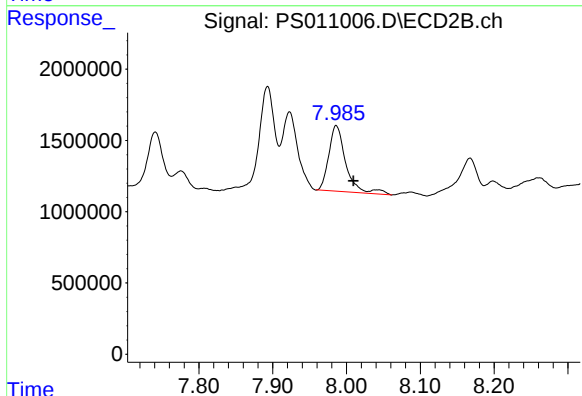


#9 2,4-D

R.T.: 7.986 min
Delta R.T.: -0.023 min
Response: 7416908
Conc: 10.26 ng/ml

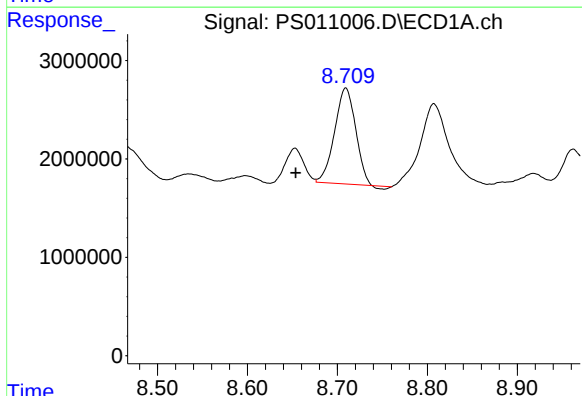


#10 Pentachlorophenol

R.T.: 8.709 min
Delta R.T.: 0.056 min
Response: 15624340
Conc: 1.26 ng/ml

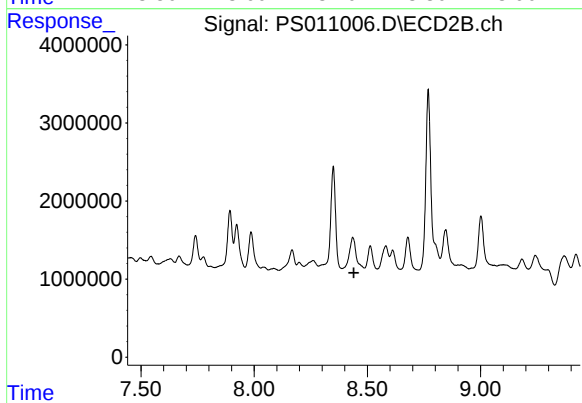

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 8.440 min
Response: 0
Conc: N.D.

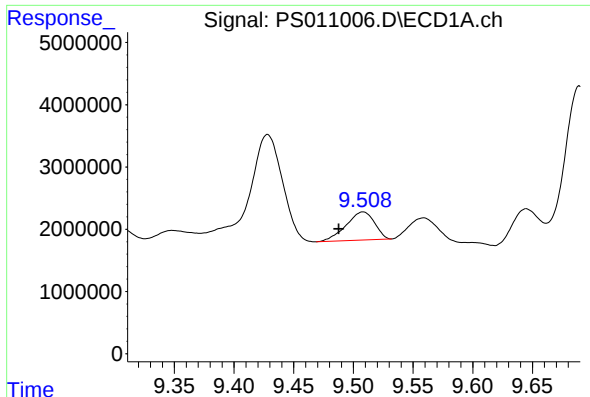

#12 2,4,5-T


R.T.: 9.508 min
Delta R.T.: 0.020 min
Response: 7520135
Conc: 1.61 ng/ml

Instrument :
ECD_S
ClientSampleId :

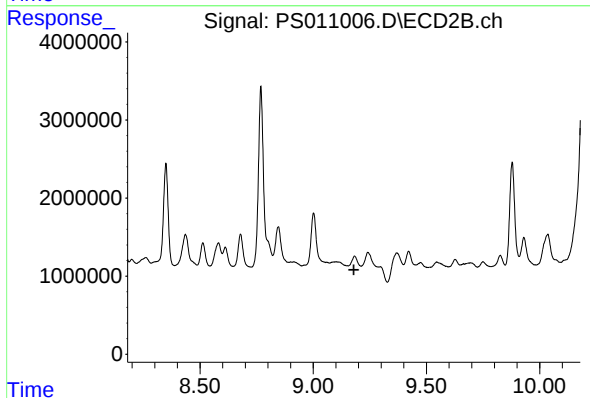


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.179 min
Response: 0
Conc: N.D.

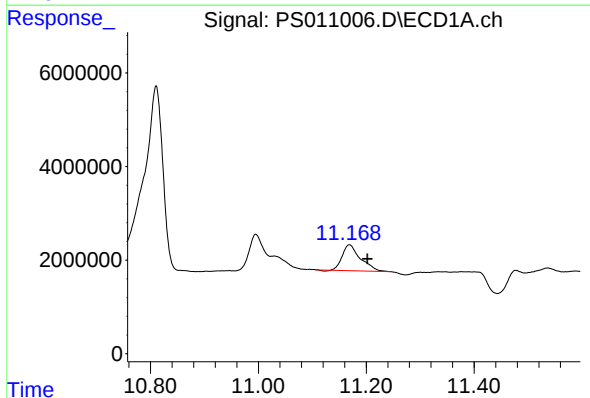


#14 DINOSEB

R.T.: 11.169 min
Delta R.T.: -0.033 min
Response: 12990879
Conc: 3.63 ng/ml

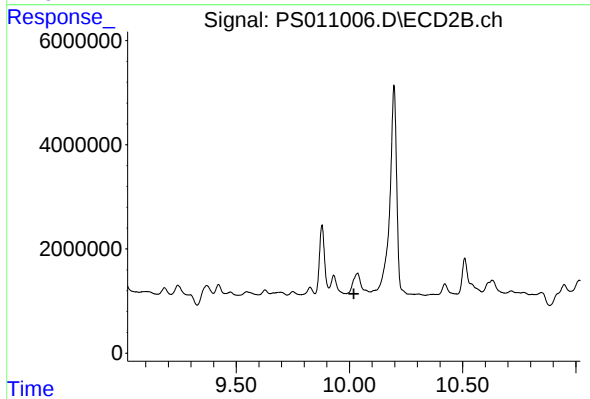

#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 10.020 min
Response: 0
Conc: N.D.

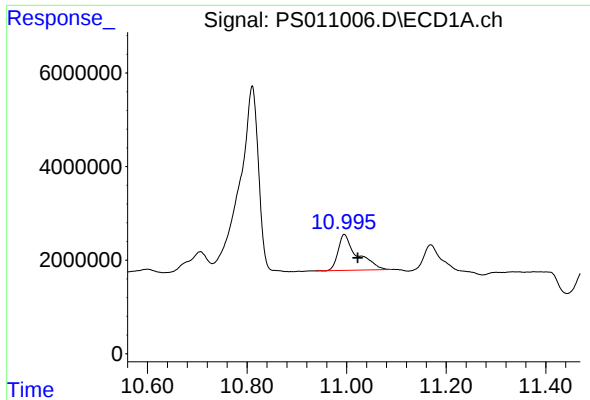

#15 Picloram


R.T.: 10.995 min

Delta R.T.: -0.027 min

Response: 20235450

Conc: 3.61 ng/ml

Instrument :
ECD_S
ClientSampleId :

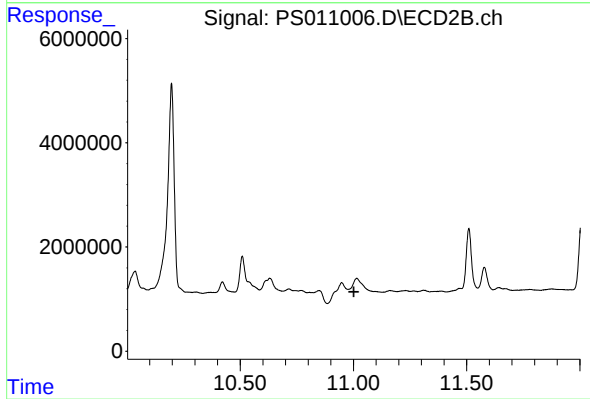

#15 Picloram

R.T.: 0.000 min

Exp R.T. : 11.002 min

Response: 0

Conc: N.D.