

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS063021\
 Data File : PS015968.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jun 2021 16:18
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 30 00:34:17 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS063021.M
 Quant Title : 8080.M
 QLast Update : Wed Jun 30 00:31:48 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

7) T	MCPA	7.634f	0.000	19387609	0	3.049	N.D.	#
8) T	DICHLORPROP	0.000	7.572	0	6510325	N.D.	12.363	
9) T	2,4-D	8.305	0.000	13248969	0	8.265	N.D.	#
11) T	2,4,5-TP ...	9.160	8.587f	5653780	25243281	<MDL	8.947	#
12) T	2,4,5-T	9.445	9.007	30314511	9500299	3.882	3.293	
14) T	DINOSEB	11.152	0.000	9783935	0	1.785	N.D.	#
15) T	Picloram	10.975	10.818	172.8E6	61262881	15.710	14.725	
16) T	DCPA	11.421	10.769	19624476	10309587	1.819	2.397	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS063021\
Data File : PS015968.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jun 2021 16:18
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 30 00:34:17 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS063021.M
Quant Title : 8080.M
QLast Update : Wed Jun 30 00:31:48 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

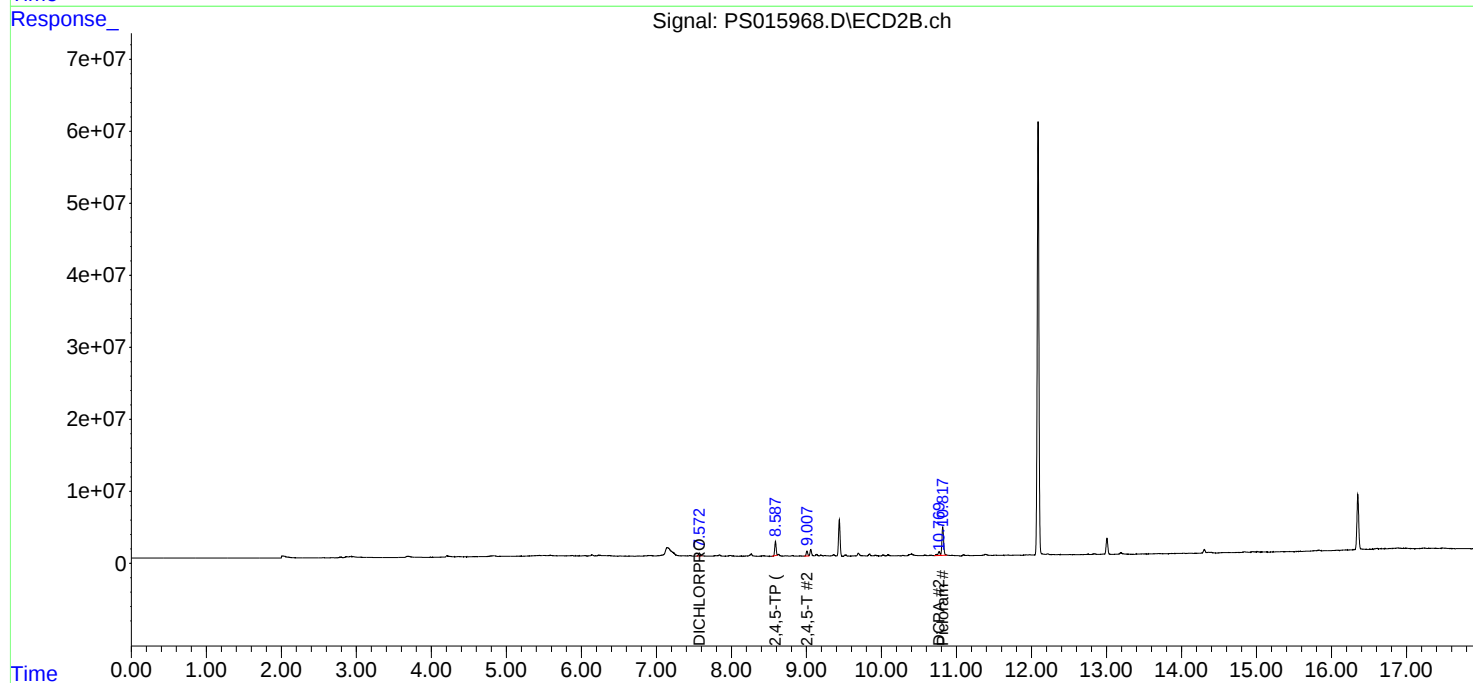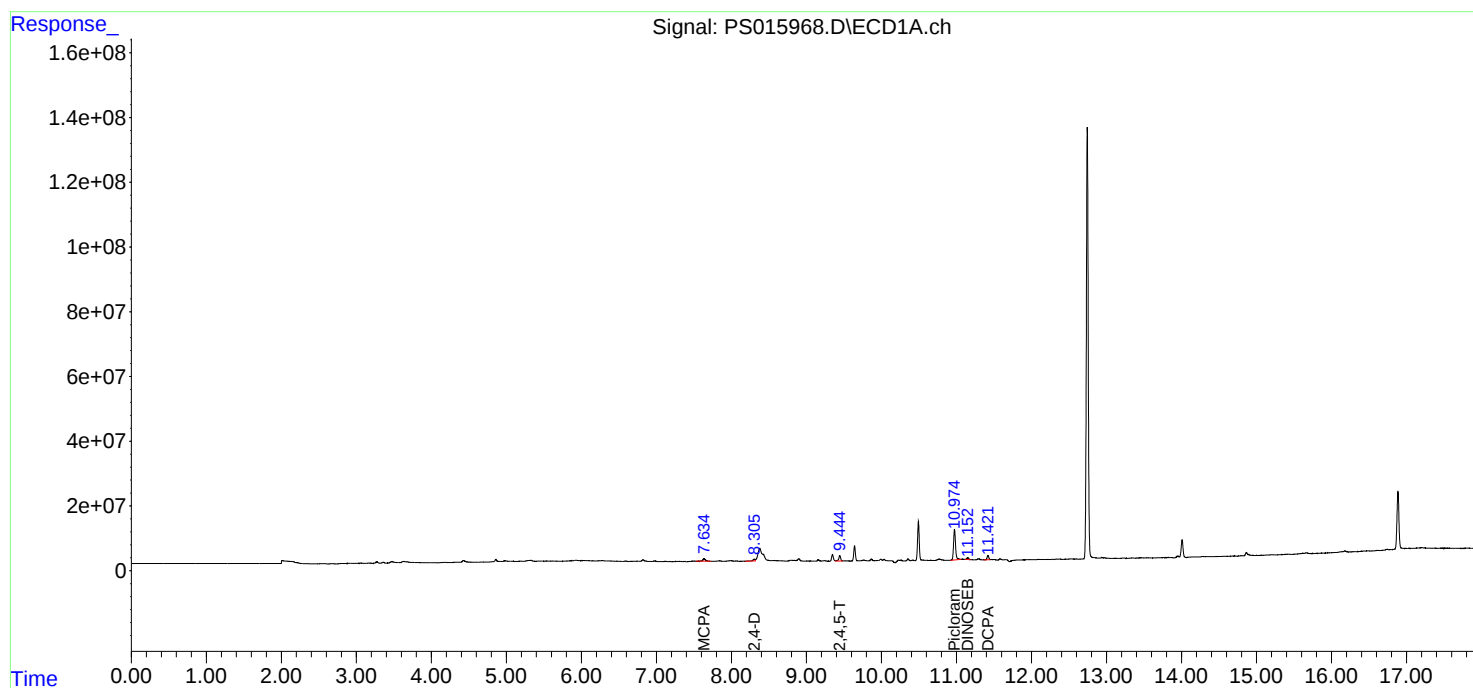


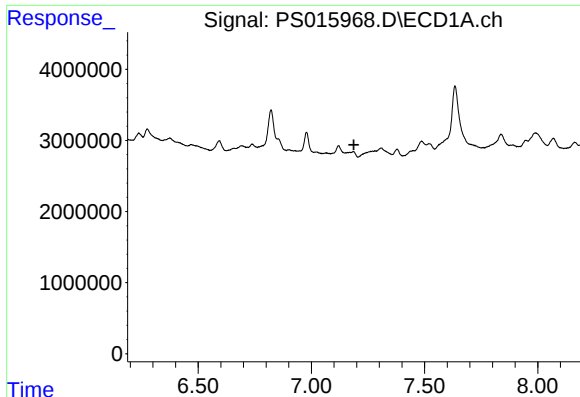

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 7.188 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

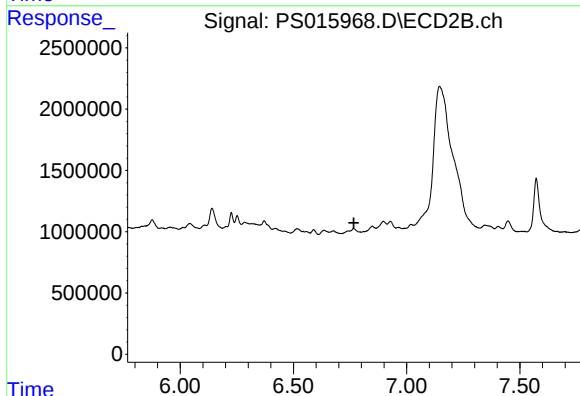


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 6.767 min
Response: 0
Conc: N.D.

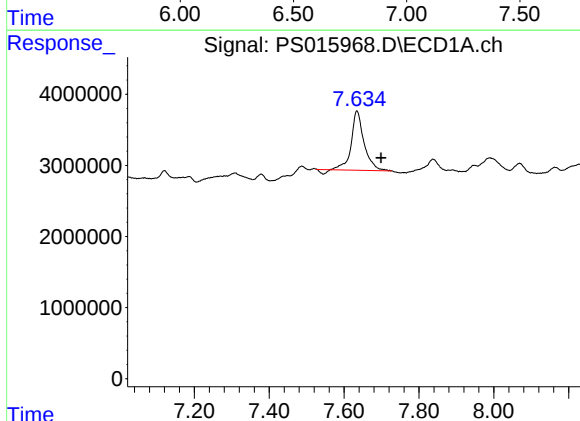


#7 MCPA

R.T.: 7.634 min
Delta R.T.: -0.064 min
Response: 19387609
Conc: 3.05 ug/ml

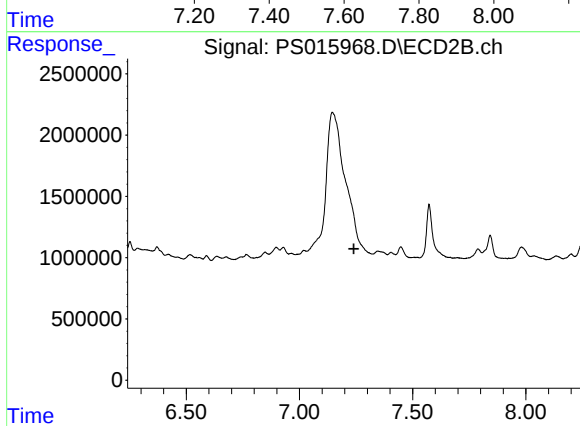

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 7.240 min
Response: 0
Conc: N.D.

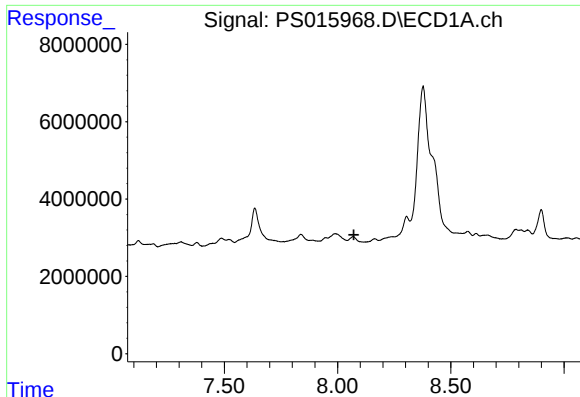

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.072 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

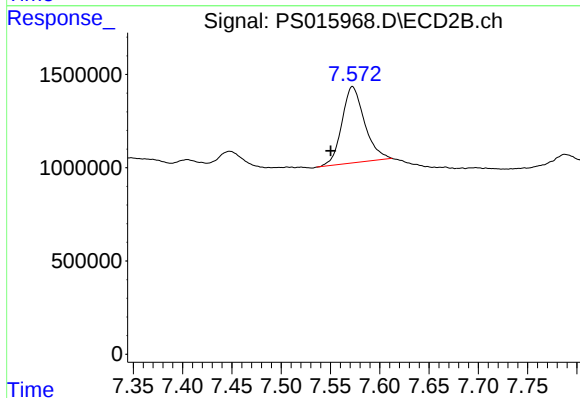


#8 DICHLORPROP

R.T.: 7.572 min
Delta R.T.: 0.022 min
Response: 6510325
Conc: 12.36 ng/ml

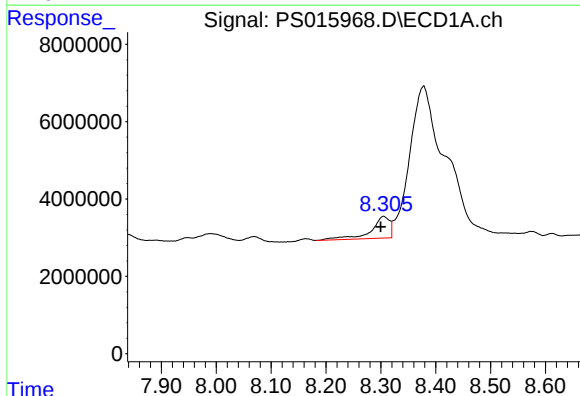


#9 2,4-D

R.T.: 8.305 min
Delta R.T.: 0.005 min
Response: 13248969
Conc: 8.26 ng/ml

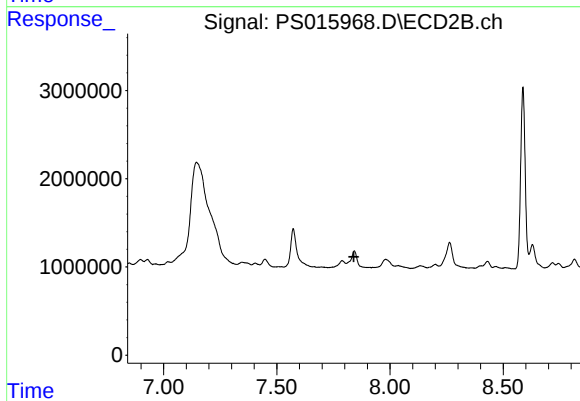

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 7.841 min
Response: 0
Conc: N.D.

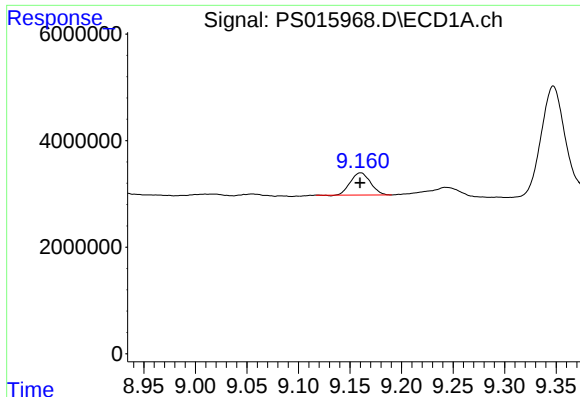

#11 2,4,5-TP (SILVEX)


R.T.: 9.160 min
Delta R.T.: 0.000 min
Response: 5653780
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

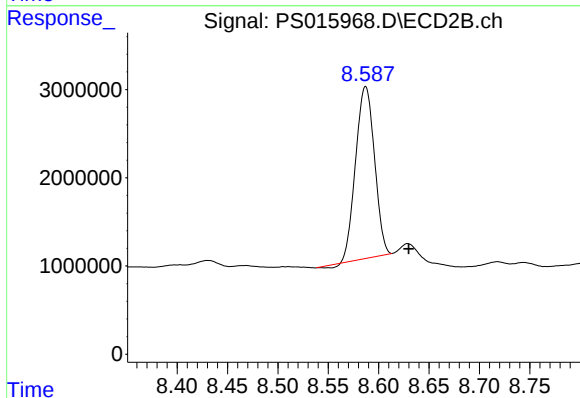


#11 2,4,5-TP (SILVEX)

R.T.: 8.587 min
Delta R.T.: -0.043 min
Response: 25243281
Conc: 8.95 ng/ml

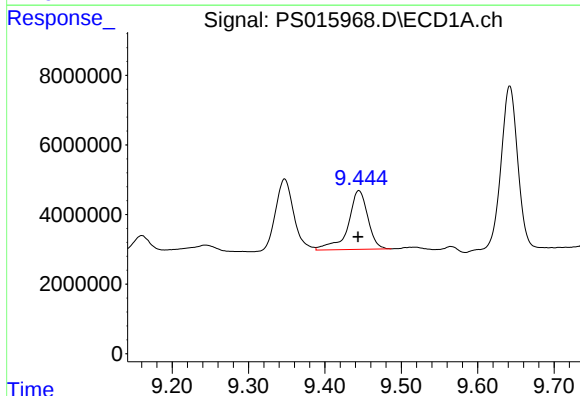


#12 2,4,5-T

R.T.: 9.445 min
Delta R.T.: 0.001 min
Response: 30314511
Conc: 3.88 ng/ml

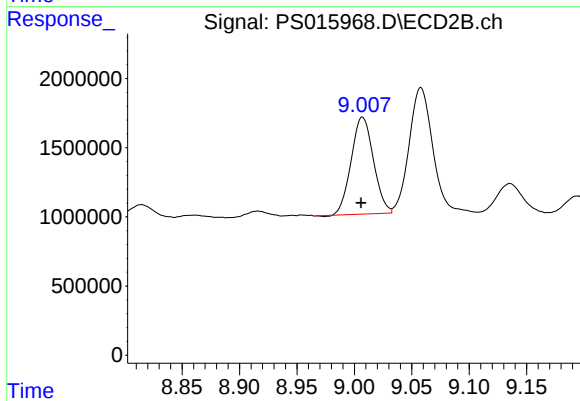

#12 2,4,5-T


R.T.: 9.007 min
Delta R.T.: 0.001 min
Response: 9500299
Conc: 3.29 ng/ml

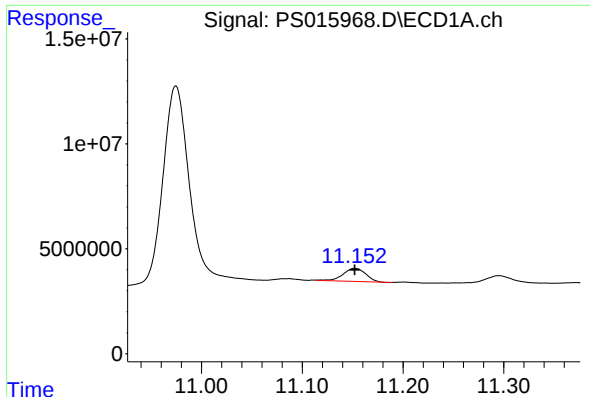

#14 DINOSEB


R.T.: 11.152 min
Delta R.T.: 0.000 min
Response: 9783935
Conc: 1.78 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

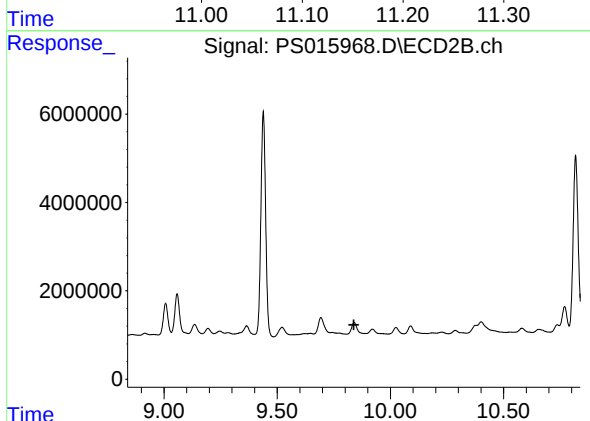


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 9.839 min
Response: 0
Conc: N.D.

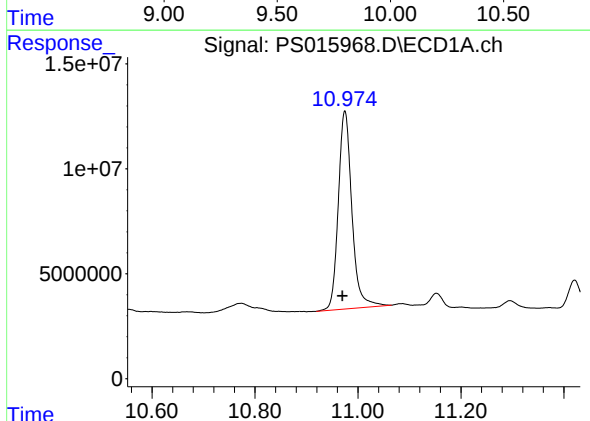


#15 Picloram

R.T.: 10.975 min
Delta R.T.: 0.005 min
Response: 172807958
Conc: 15.71 ng/ml

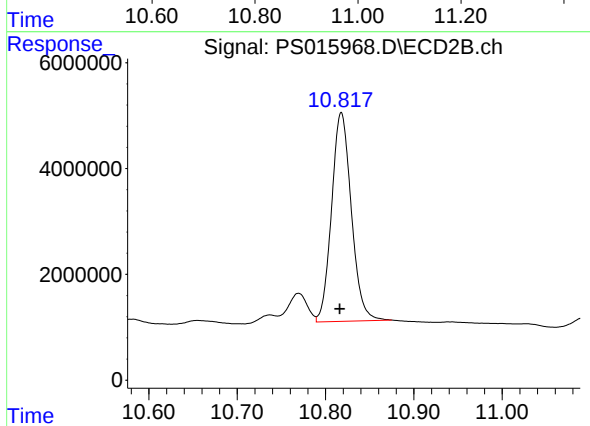

#15 Picloram


R.T.: 10.818 min
Delta R.T.: 0.002 min
Response: 61262881
Conc: 14.72 ng/ml

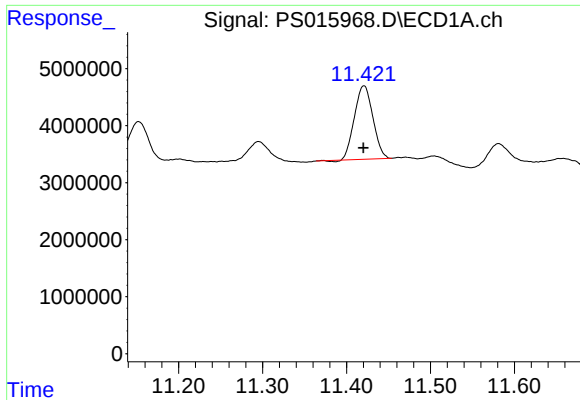

#16 DCPA

R.T.: 11.421 min
Delta R.T.: 0.000 min
Response: 19624476
Conc: 1.82 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

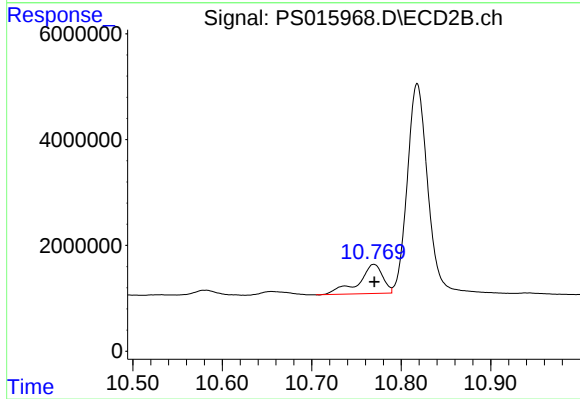

#16 DCPA

R.T.: 10.769 min
Delta R.T.: 0.000 min
Response: 10309587
Conc: 2.40 ng/ml