

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS063021\
 Data File : PS015969.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jun 2021 16:42
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 30 00:34:40 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS063021.M
 Quant Title : 8080.M
 QLast Update : Wed Jun 30 00:31:48 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.188	6.767	639.5E6	238.2E6	416.548	464.049
Target Compounds							
7) T	MCPA	7.632f	0.000	17934302	0	2.820	N.D. #
9) T	2,4-D	8.305	0.000	9353116	0	5.835	N.D. #
11) T	2,4,5-TP ...	9.160	8.587f	8769573	23480327	1.182	8.322 #
12) T	2,4,5-T	9.445	9.007	34797264	11884119	4.456	4.120
13) T	2,4-DB	10.035f	0.000	7112036	0	4.282	N.D. #
14) T	DINOSEB	11.152	0.000	13842416	0	2.525	N.D. #
15) T	Picloram	10.975	10.819	127.8E6	45545759	11.622	10.947
16) T	DCPA	11.420	10.769	27718337	13335990	2.570	3.101



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS063021\
Data File : PS015969.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jun 2021 16:42
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 30 00:34:40 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS063021.M
Quant Title : 8080.M
QLast Update : Wed Jun 30 00:31:48 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

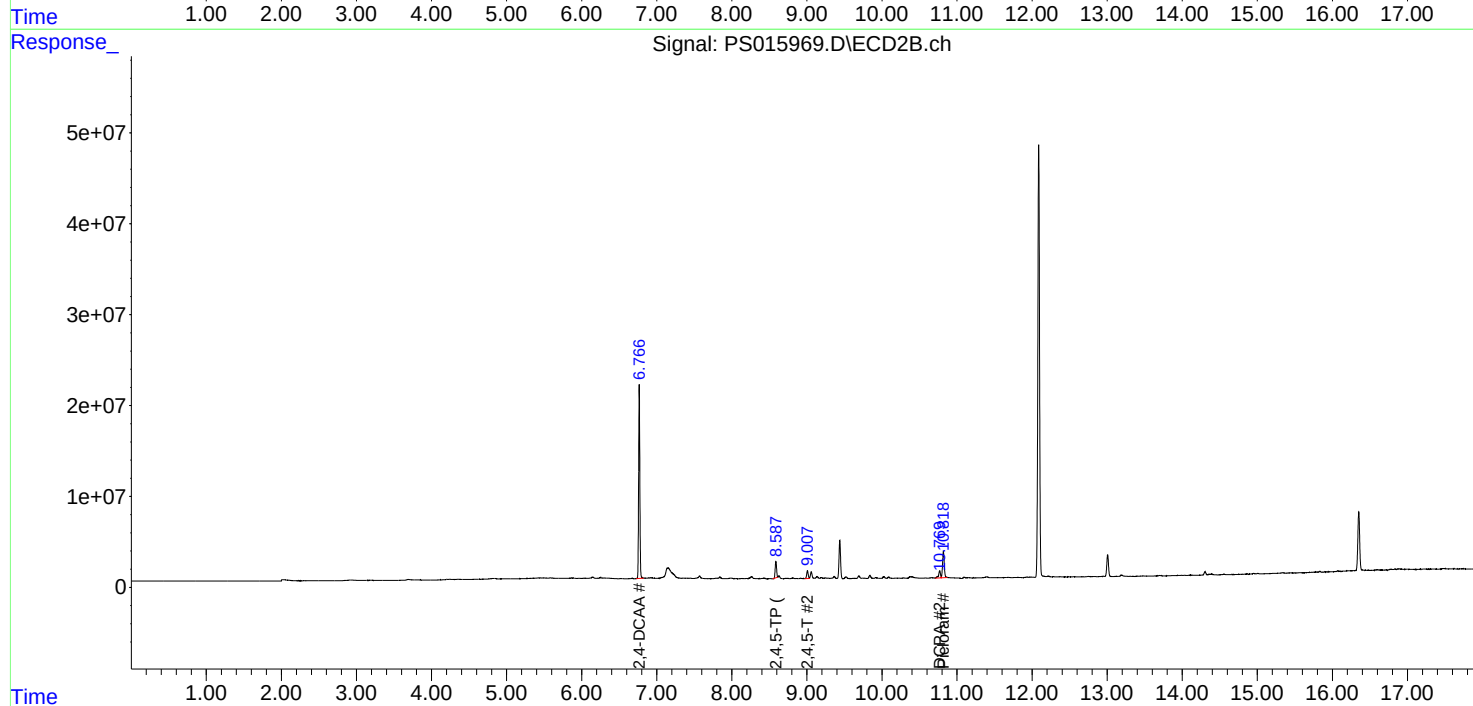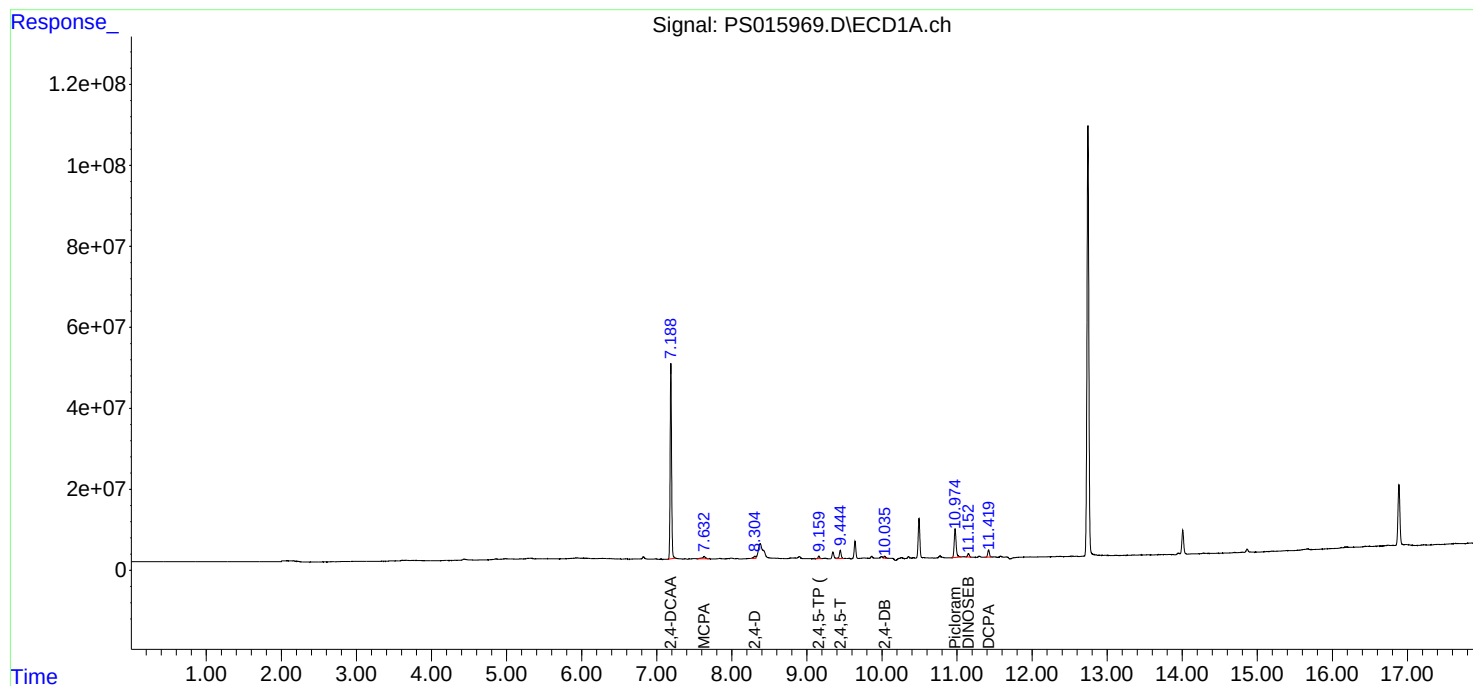


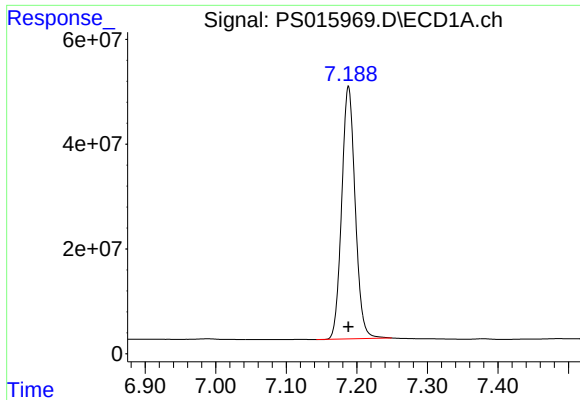

#4 2,4-DCAA


R.T.: 7.188 min
Delta R.T.: 0.000 min
Response: 639484503
Conc: 416.55 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

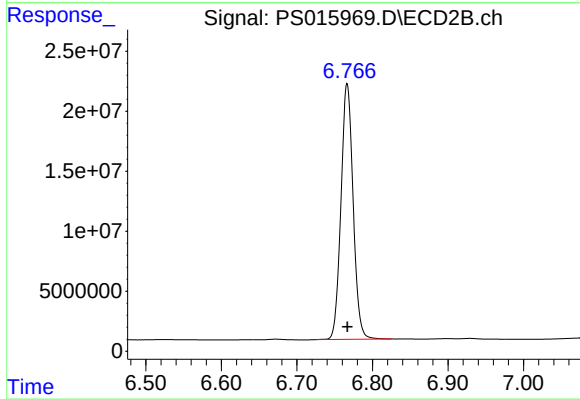


#4 2,4-DCAA

R.T.: 6.767 min
Delta R.T.: 0.000 min
Response: 238204372
Conc: 464.05 ng/ml

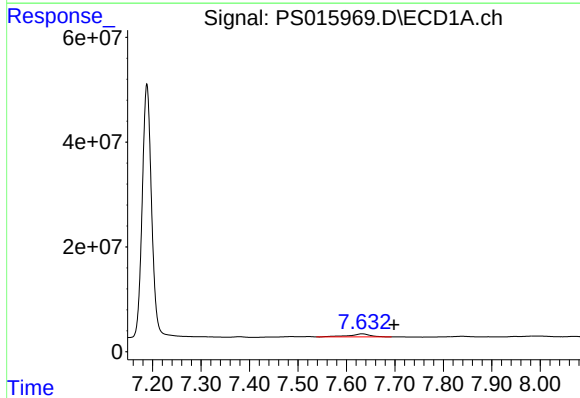


#7 MCPA

R.T.: 7.632 min
Delta R.T.: -0.066 min
Response: 17934302
Conc: 2.82 ug/ml

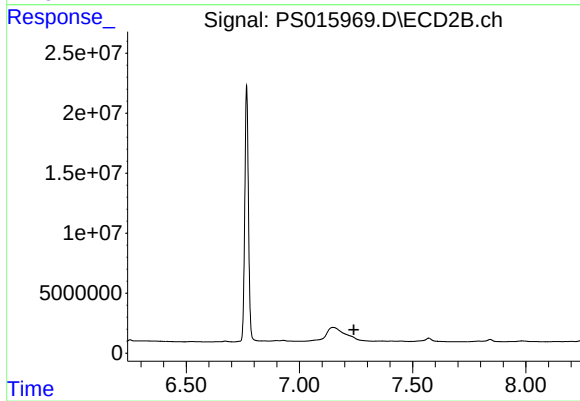

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 7.240 min
Response: 0
Conc: N.D.

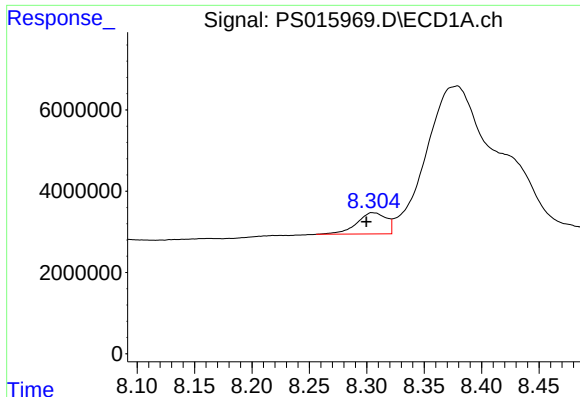

#9 2,4-D


R.T.: 8.305 min
Delta R.T.: 0.005 min
Response: 9353116
Conc: 5.83 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

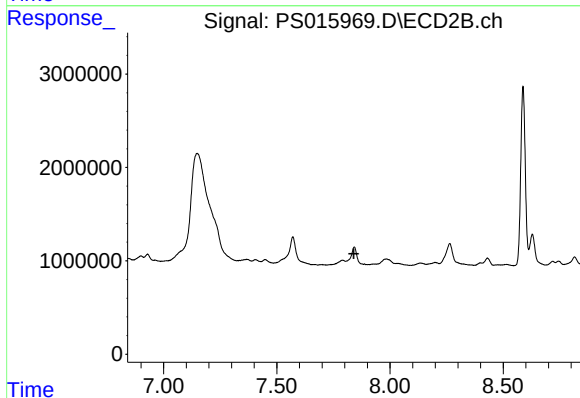


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.841 min
Response: 0
Conc: N.D.

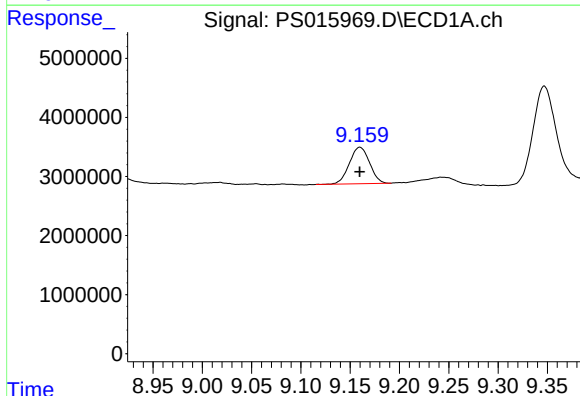


#11 2,4,5-TP (SILVEX)

R.T.: 9.160 min
Delta R.T.: 0.000 min
Response: 8769573
Conc: 1.18 ng/ml

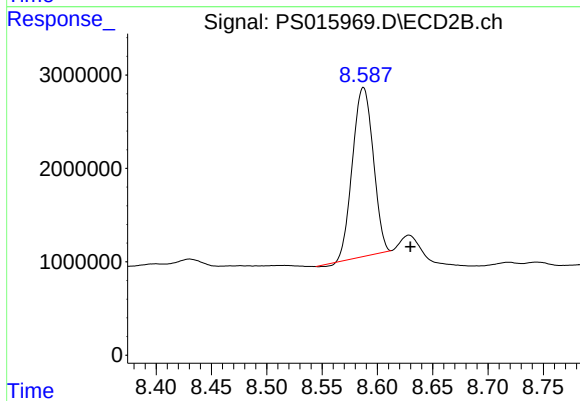

#11 2,4,5-TP (SILVEX)


R.T.: 8.587 min
Delta R.T.: -0.042 min
Response: 23480327
Conc: 8.32 ng/ml

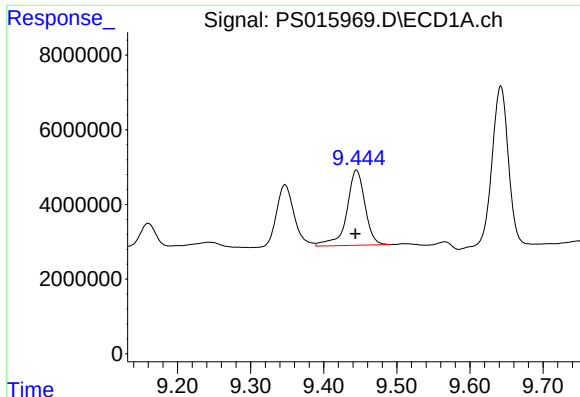

#12 2,4,5-T


R.T.: 9.445 min
Delta R.T.: 0.001 min
Response: 34797264
Conc: 4.46 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

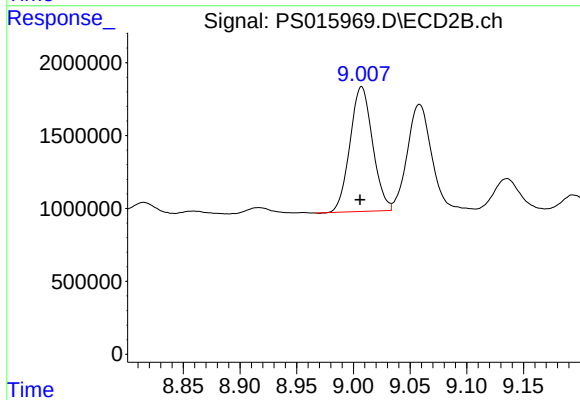


#12 2,4,5-T

R.T.: 9.007 min
Delta R.T.: 0.001 min
Response: 11884119
Conc: 4.12 ng/ml

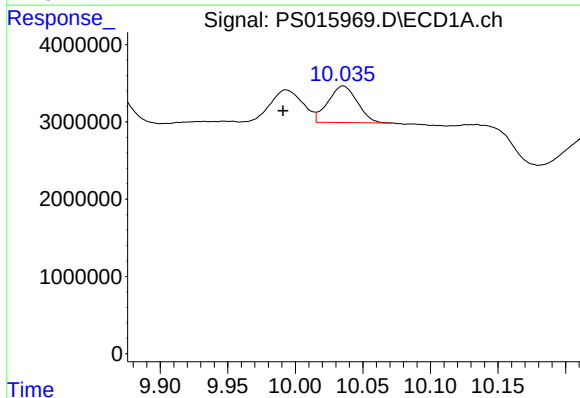


#13 2,4-DB

R.T.: 10.035 min
Delta R.T.: 0.045 min
Response: 7112036
Conc: 4.28 ng/ml

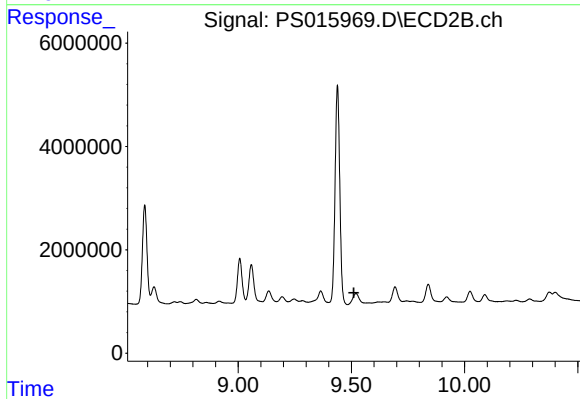

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 9.512 min
Response: 0
Conc: N.D.

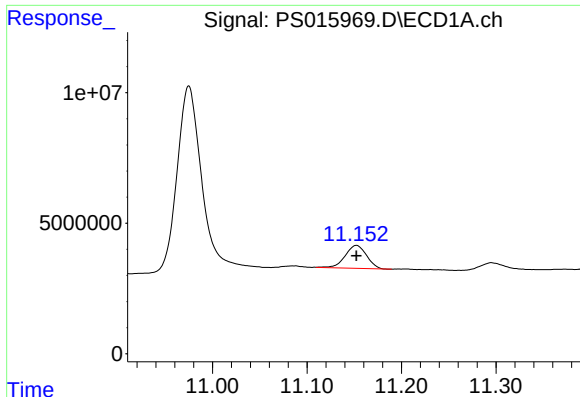

#14 DINOSEB


R.T.: 11.152 min
Delta R.T.: 0.000 min
Response: 13842416
Conc: 2.52 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

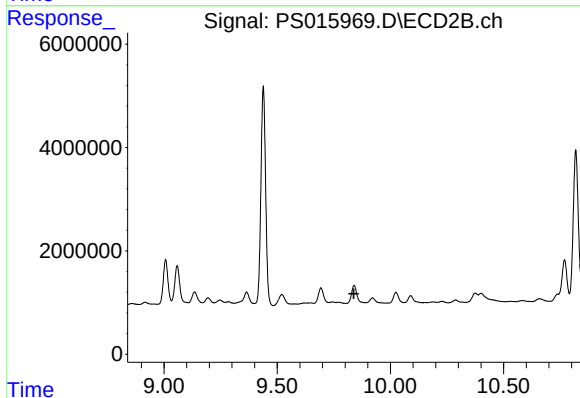


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 9.839 min
Response: 0
Conc: N.D.

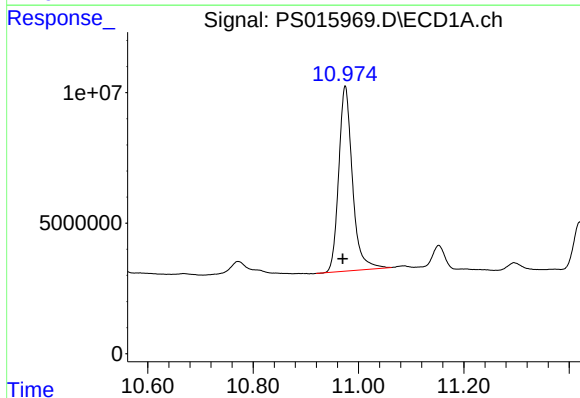


#15 Picloram

R.T.: 10.975 min
Delta R.T.: 0.005 min
Response: 127843411
Conc: 11.62 ng/ml

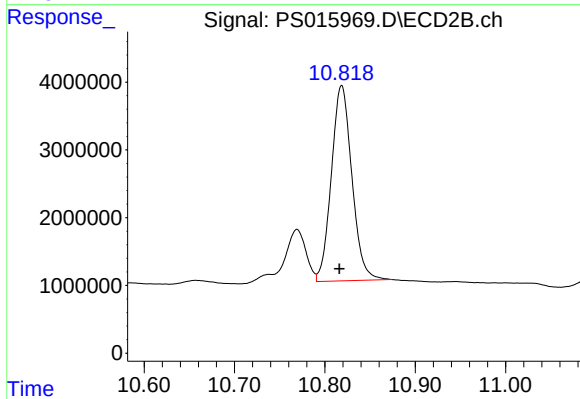

#15 Picloram


R.T.: 10.819 min
Delta R.T.: 0.002 min
Response: 45545759
Conc: 10.95 ng/ml

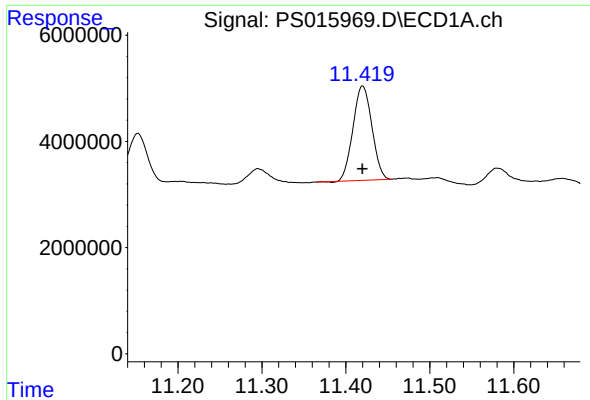

#16 DCPA

R.T.: 11.420 min
Delta R.T.: 0.000 min
Response: 27718337
Conc: 2.57 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

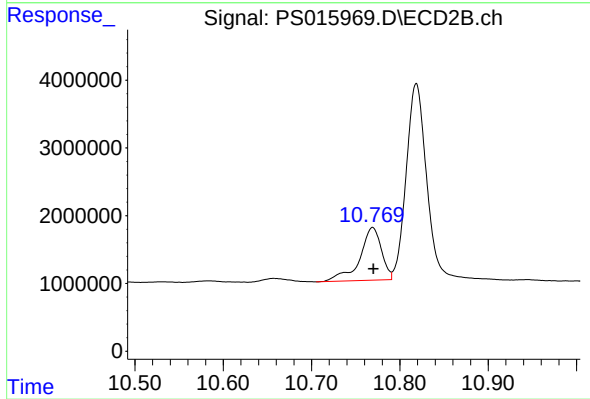

#16 DCPA

R.T.: 10.769 min
Delta R.T.: 0.000 min
Response: 13335990
Conc: 3.10 ng/ml