

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS063021\
 Data File : PS015976.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jun 2021 19:31
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 30 00:35:22 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS063021.M
 Quant Title : 8080.M
 QLast Update : Wed Jun 30 00:31:48 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.188	6.766	642.1E6	242.8E6	418.248	473.044
Target Compounds							
11) T	2,4,5-TP ...	0.000	8.588f	0	8916206	N.D.	3.160
12) T	2,4,5-T	9.447	9.060f	8769627	12418729	1.123	4.305 #
15) T	Picloram	10.977	10.820	185.9E6	69609935	16.899	16.731
16) T	DCPA	11.421	10.820f	8386544	69609935	<MDL	16.187 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS063021\
Data File : PS015976.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jun 2021 19:31
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 30 00:35:22 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS063021.M
Quant Title : 8080.M
QLast Update : Wed Jun 30 00:31:48 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

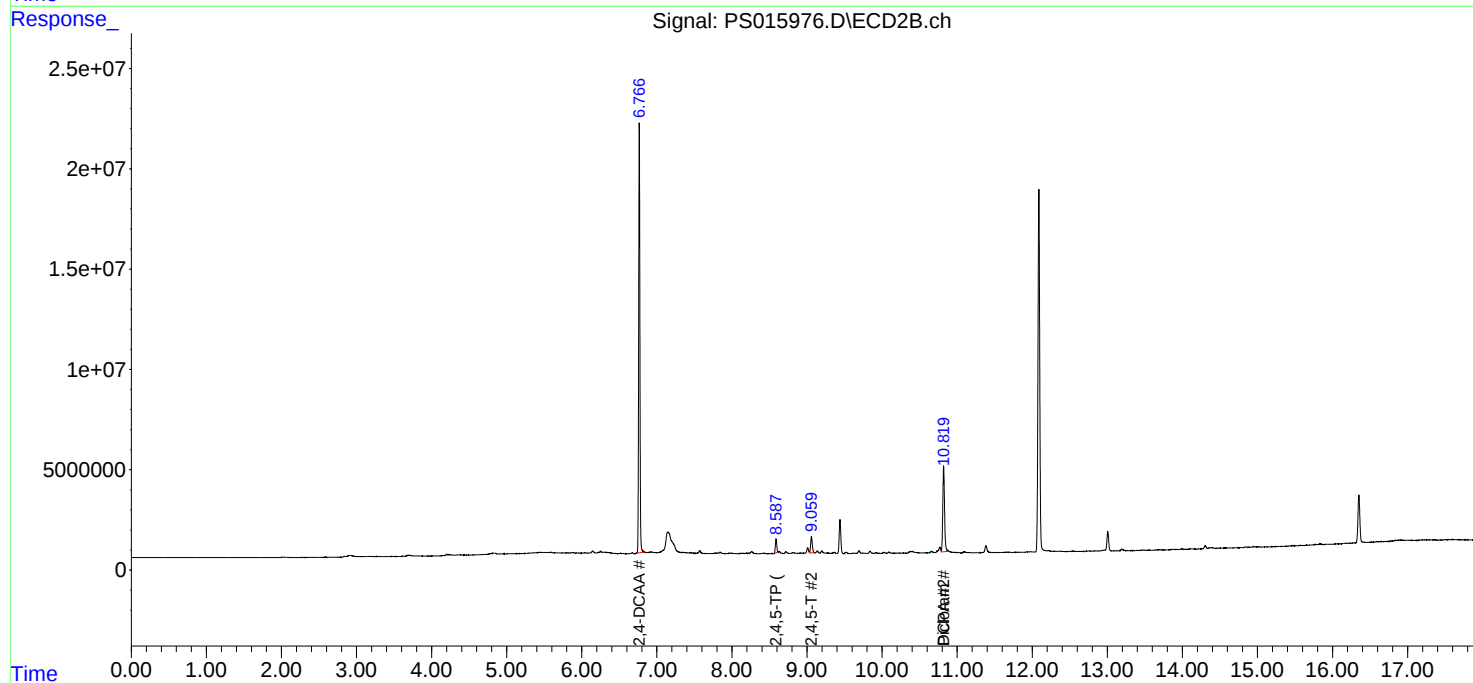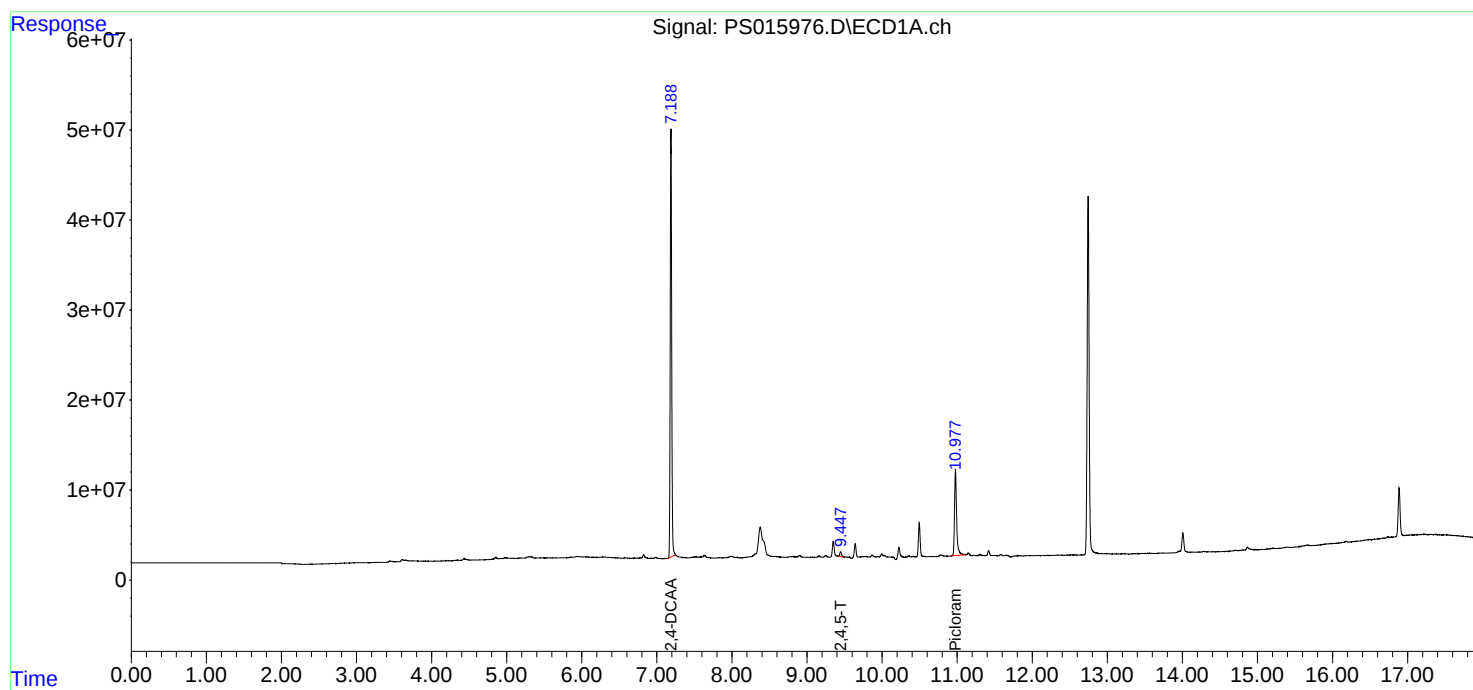


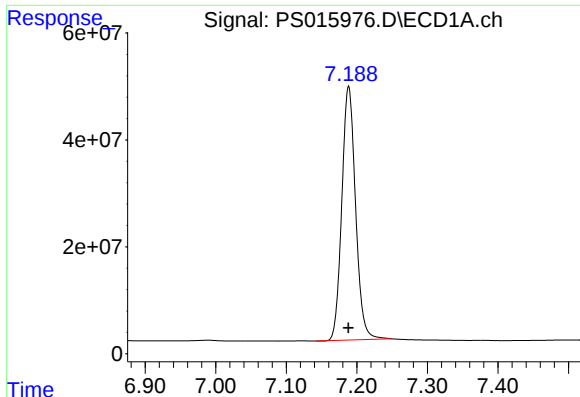

#4 2,4-DCAA


R.T.: 7.188 min
Delta R.T.: 0.000 min
Response: 642094458
Conc: 418.25 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

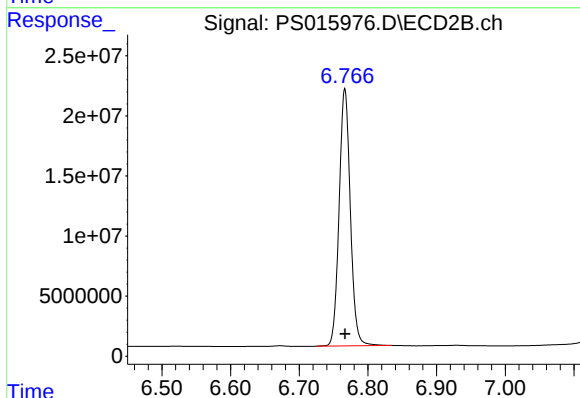


#4 2,4-DCAA

R.T.: 6.766 min
Delta R.T.: 0.000 min
Response: 242821426
Conc: 473.04 ng/ml

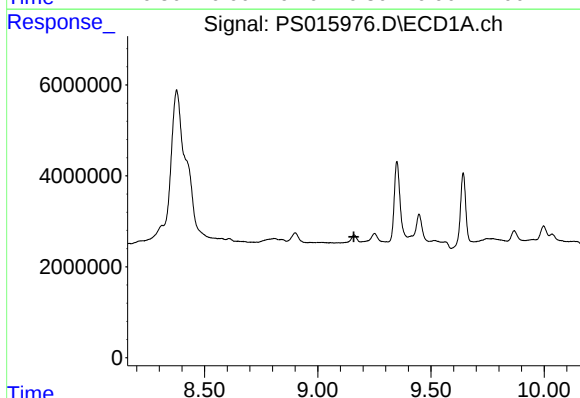


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 9.160 min
Response: 0
Conc: N.D.

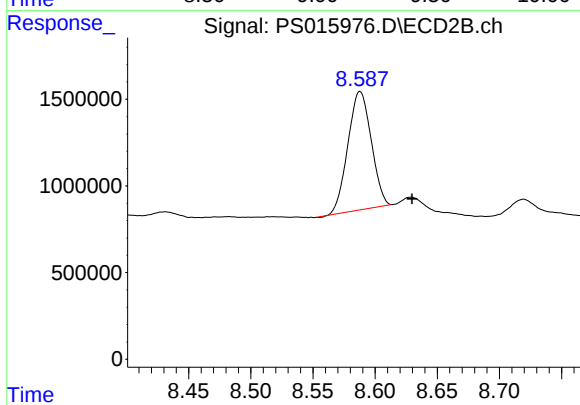

#11 2,4,5-TP (SILVEX)


R.T.: 8.588 min
Delta R.T.: -0.042 min
Response: 8916206
Conc: 3.16 ng/ml

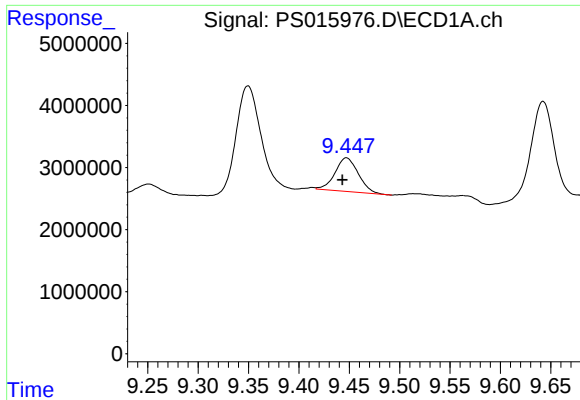

#12 2,4,5-T


R.T.: 9.447 min
Delta R.T.: 0.004 min
Response: 8769627
Conc: 1.12 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

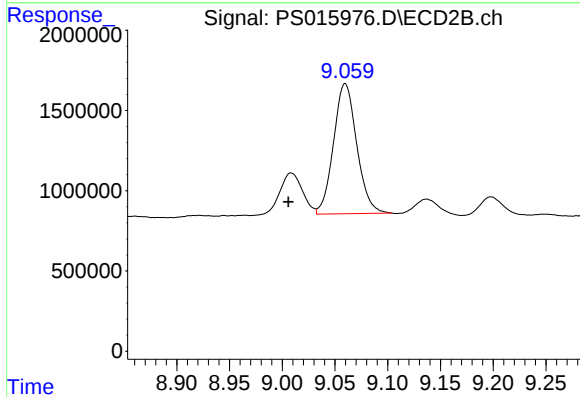


#12 2,4,5-T

R.T.: 9.060 min
Delta R.T.: 0.054 min
Response: 12418729
Conc: 4.30 ng/ml

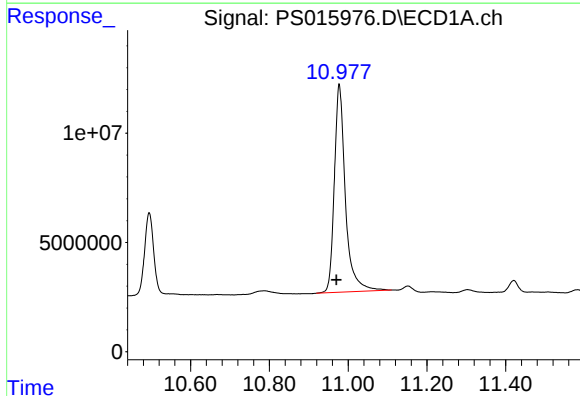


#15 Picloram

R.T.: 10.977 min
Delta R.T.: 0.007 min
Response: 185895215
Conc: 16.90 ng/ml

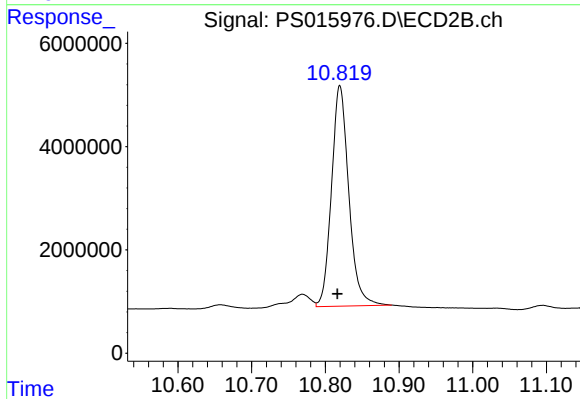

#15 Picloram


R.T.: 10.820 min
Delta R.T.: 0.004 min
Response: 69609935
Conc: 16.73 ng/ml

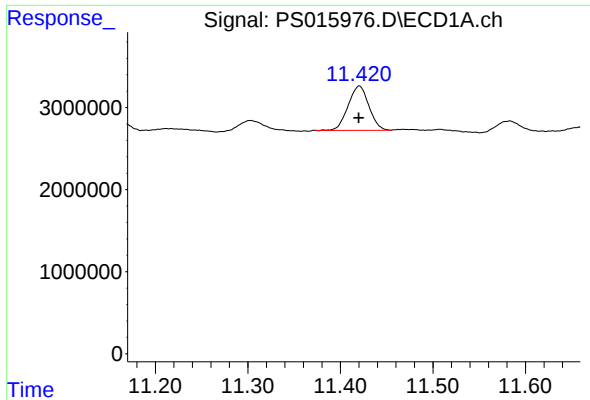

#16 DCPA

R.T.: 11.421 min
Delta R.T.: 0.000 min
Response: 8386544
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

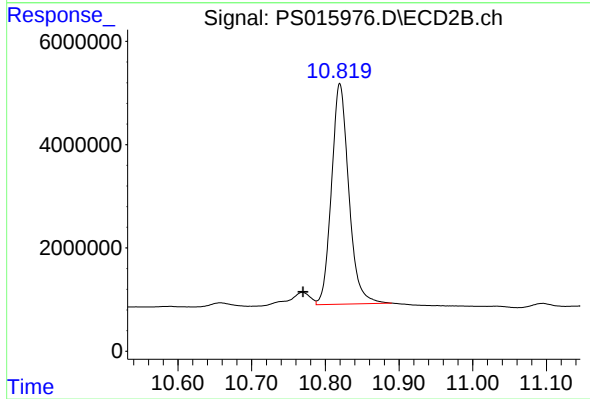

#16 DCPA

R.T.: 10.820 min
Delta R.T.: 0.050 min
Response: 69609935
Conc: 16.19 ng/ml