

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS063021\
 Data File : PS015993.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Jun 2021 03:11
 Operator : DD\AJ
 Sample : M2834-01MS
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 FK-BPM-01-B8-C8-B8A-C8AMS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 30 05:24:17 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS063021.M
 Quant Title : 8080.M
 QLast Update : Wed Jun 30 00:31:48 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.187	6.765	642.1E6	210.8E6	418.239	410.638
Target Compounds							
1) T	Dalapon	3.014	2.519	556.2E6	179.2E6	256.437	256.424
2) T	3,5-DICHL...	6.405	5.957	588.3E6	226.7E6	271.236	294.491
3) T	4-Nitroph...	7.014	6.386	212.7E6	87336446	240.556	276.709
5) T	DICAMBA	7.378	6.929	1542.2E6	550.6E6	269.177	261.371
6) T	MCPD	7.544	7.022	121.1E6	39741640	27.612	23.954
7) T	MCPA	7.691	7.232	196.8E6	68895447	30.943	26.138
8) T	DICHLORPROP	8.070	7.549	431.7E6	129.1E6	310.318	245.214
9) T	2,4-D	8.299	7.840	586.2E6	197.6E6	365.677	313.402
10) T	Pentachlo...	8.608	8.267	4190.6E6	1556.8E6	211.466	216.418
11) T	2,4,5-TP ...	9.159	8.629	1937.5E6	771.3E6	261.103	273.354
12) T	2,4,5-T	9.442	9.006	1929.0E6	753.0E6	247.033	261.035
13) T	2,4-DB	9.995	9.517	222.3E6	187.8E6	133.809	499.526 #
14) T	DINOSEB	11.150	9.839	89720011	65961845	16.366	32.305 #
15) T	Picloram	10.969	10.815	3172.9E6	1200.2E6	288.442	288.470
16) T	DCPA	11.420	10.769	2364.8E6	1091.9E6	219.235	253.914



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS063021\
Data File : PS015993.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Jun 2021 03:11
Operator : DD\AJ
Sample : M2834-01MS
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
FK-BPM-01-B8-C8-B8A-C8AMS

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 30 05:24:17 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS063021.M
Quant Title : 8080.M
QLast Update : Wed Jun 30 00:31:48 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

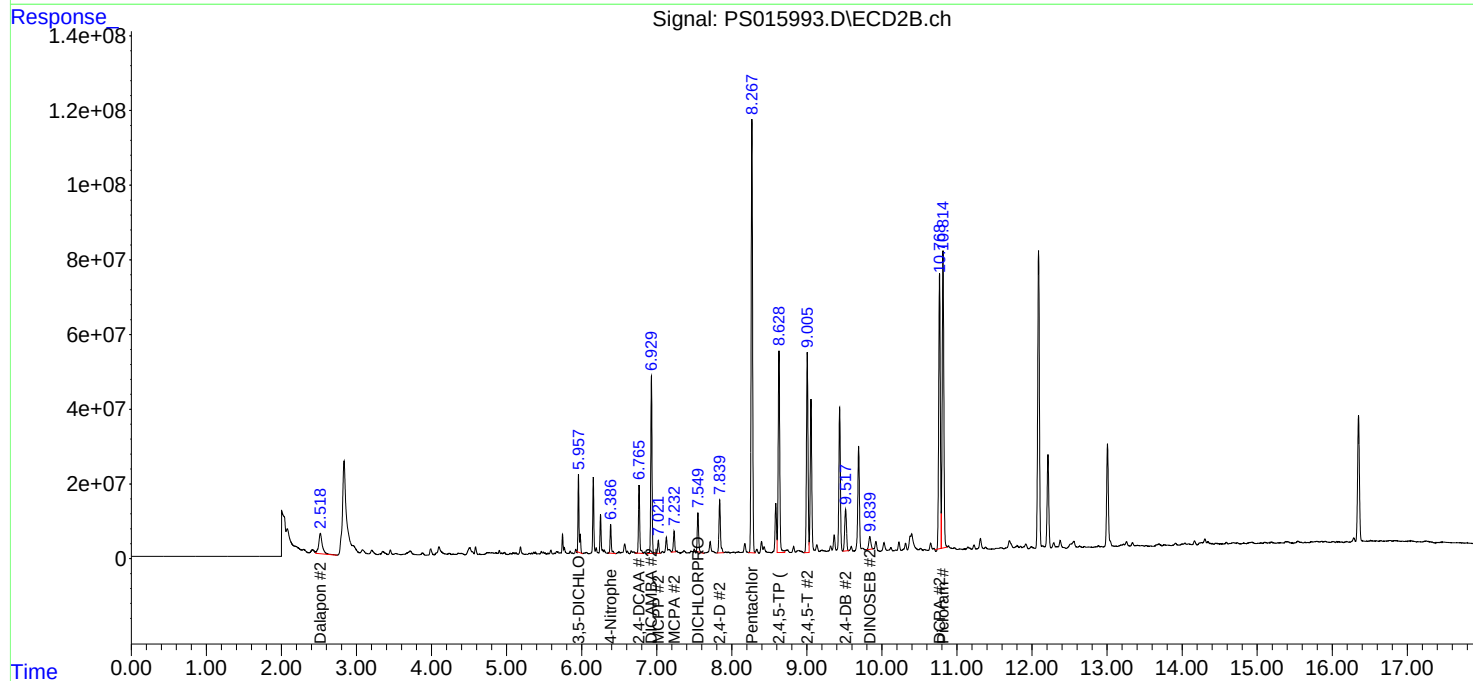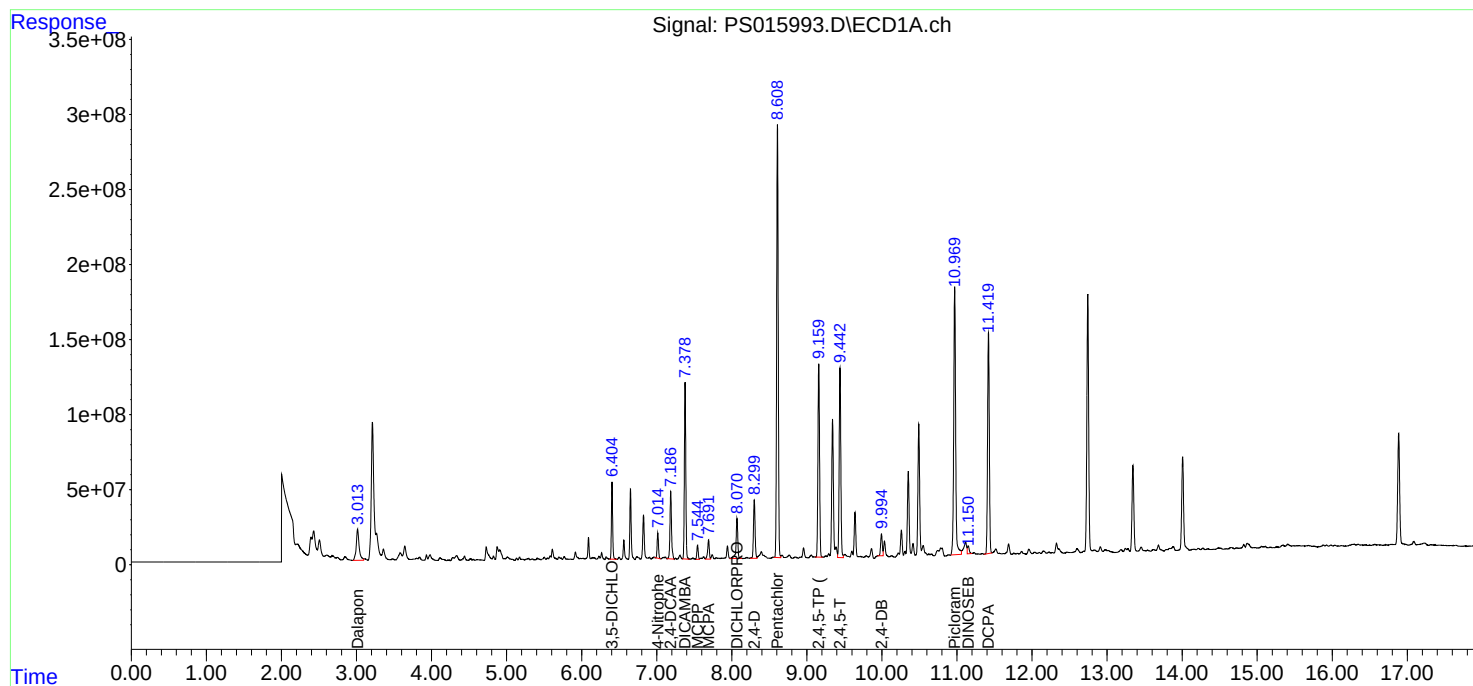


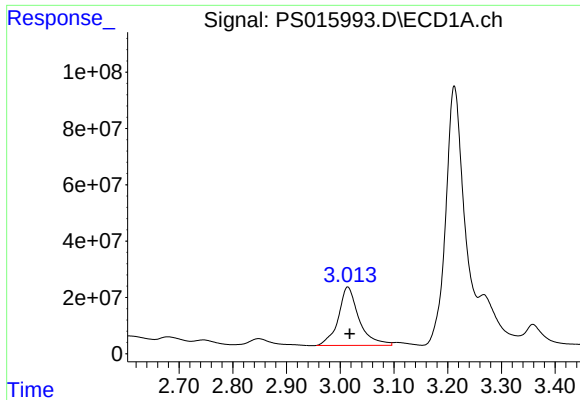

#1 Dalapon


R.T.: 3.014 min
Delta R.T.: -0.004 min
Response: 556179833
Conc: 256.44 ng/ml

Instrument :
ECD_S
ClientSampleId :
FK-BPM-01-B8-C8-B8A-C8AMS

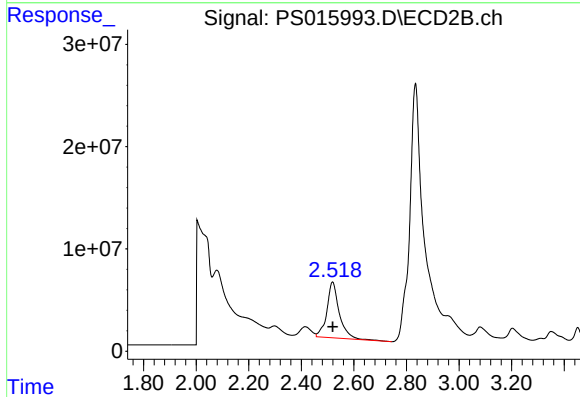


#1 Dalapon

R.T.: 2.519 min
Delta R.T.: 0.000 min
Response: 179220933
Conc: 256.42 ng/ml

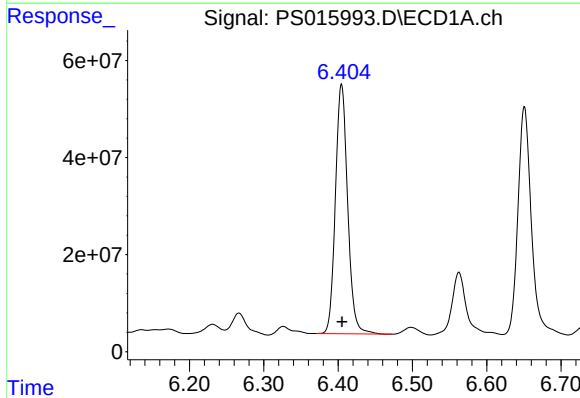


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.405 min
Delta R.T.: 0.000 min
Response: 588299299
Conc: 271.24 ng/ml

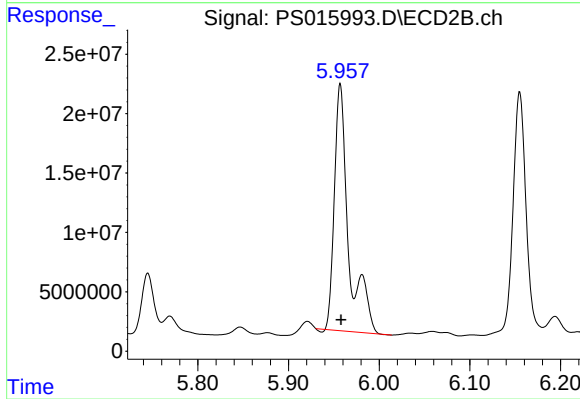

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.957 min
Delta R.T.: 0.000 min
Response: 226681595
Conc: 294.49 ng/ml

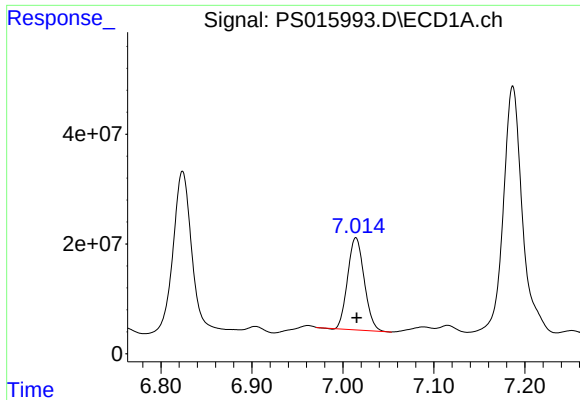

#3 4-Nitrophenol


R.T.: 7.014 min
Delta R.T.: 0.000 min
Response: 212729965
Conc: 240.56 ng/ml

Instrument :
ECD_S
ClientSampleId :
FK-BPM-01-B8-C8-B8A-C8AMS

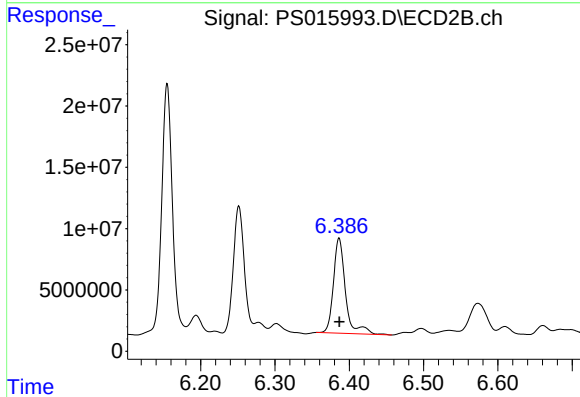


#3 4-Nitrophenol

R.T.: 6.386 min
Delta R.T.: 0.000 min
Response: 87336446
Conc: 276.71 ng/ml

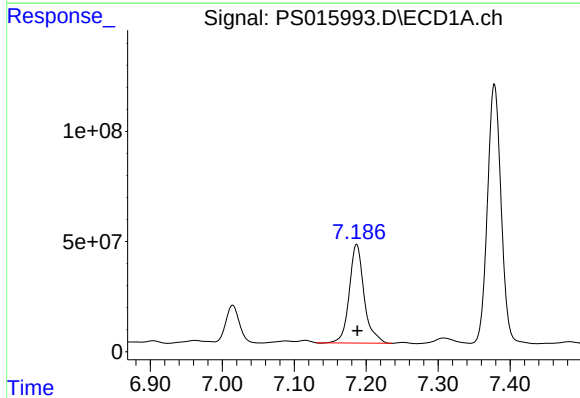


#4 2,4-DCAA

R.T.: 7.187 min
Delta R.T.: -0.001 min
Response: 642080278
Conc: 418.24 ng/ml

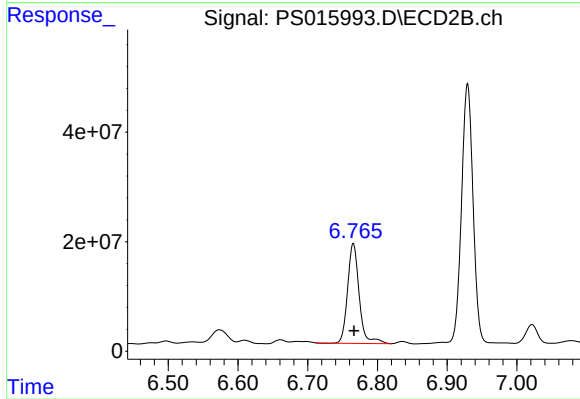

#4 2,4-DCAA


R.T.: 6.765 min
Delta R.T.: -0.001 min
Response: 210787641
Conc: 410.64 ng/ml

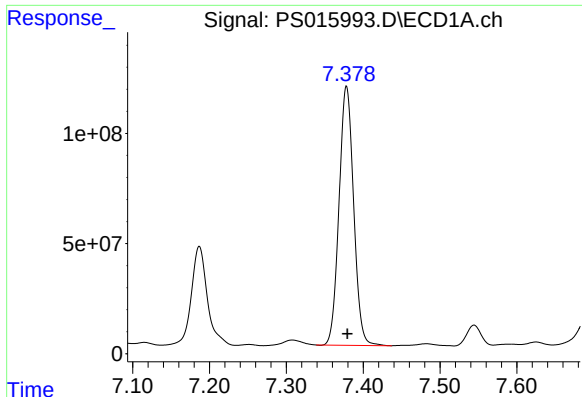

#5 DICAMBA


R.T.: 7.378 min
Delta R.T.: -0.001 min
Response: 1542162605
Conc: 269.18 ng/ml

Instrument :
ECD_S
ClientSampleId :
FK-BPM-01-B8-C8-B8A-C8AMS

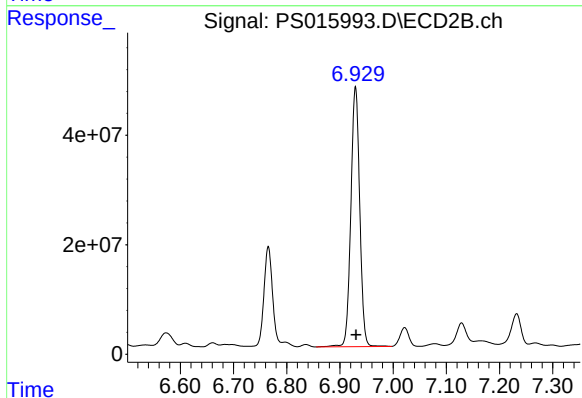


#5 DICAMBA

R.T.: 6.929 min
Delta R.T.: -0.001 min
Response: 550552265
Conc: 261.37 ng/ml

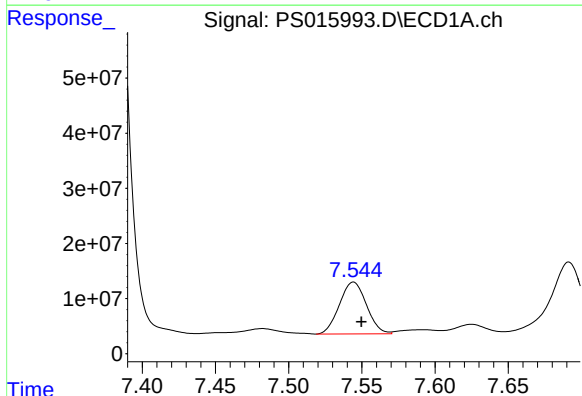


#6 MCP

R.T.: 7.544 min
Delta R.T.: -0.006 min
Response: 121050407
Conc: 27.61 ug/ml

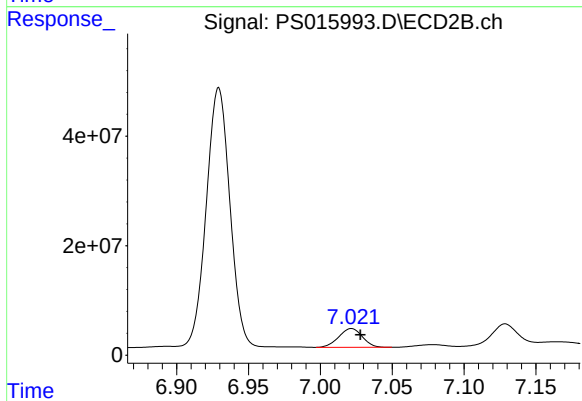

#6 MCP


R.T.: 7.022 min
Delta R.T.: -0.006 min
Response: 39741640
Conc: 23.95 ug/ml

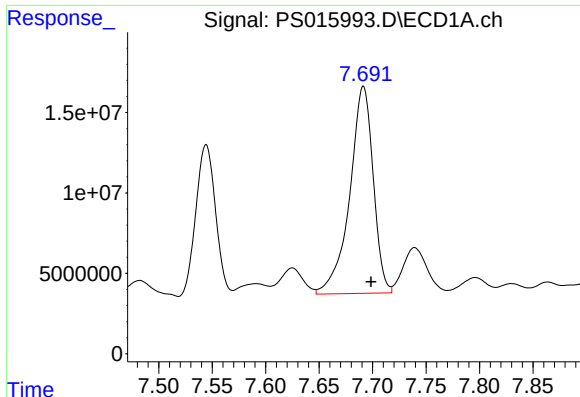

#7 MCPA


R.T.: 7.691 min
Delta R.T.: -0.007 min
Response: 196768800
Conc: 30.94 ug/ml

Instrument :
ECD_S
ClientSampleId :
FK-BPM-01-B8-C8-B8A-C8AMS

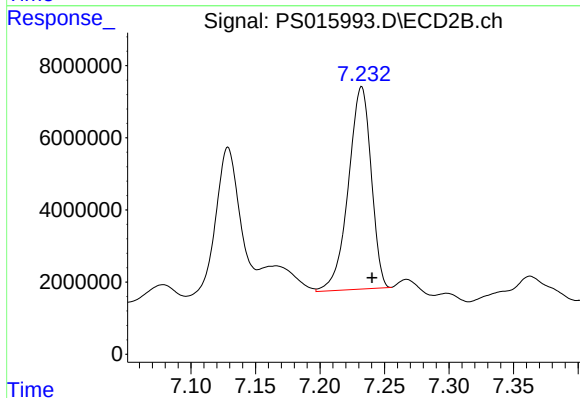


#7 MCPA

R.T.: 7.232 min
Delta R.T.: -0.008 min
Response: 68895447
Conc: 26.14 ug/ml

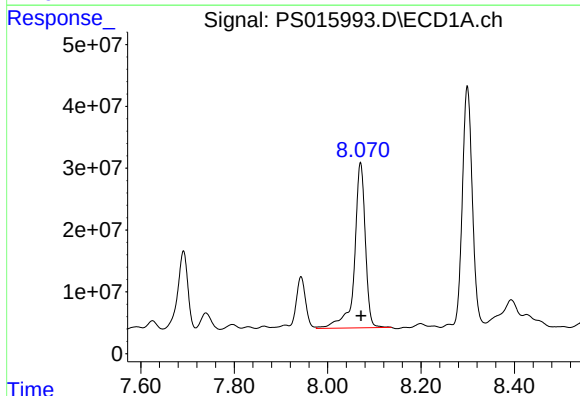


#8 DICHLORPROP

R.T.: 8.070 min
Delta R.T.: -0.001 min
Response: 431652562
Conc: 310.32 ng/ml

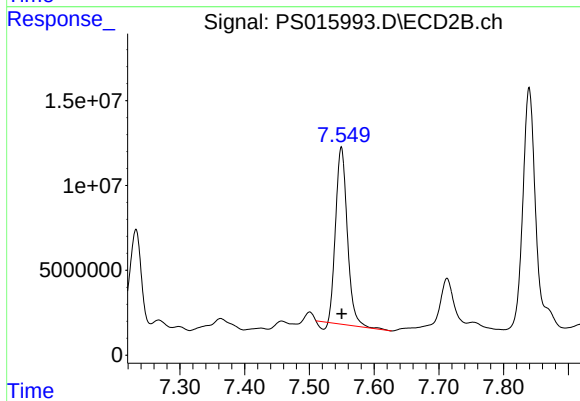

#8 DICHLORPROP


R.T.: 7.549 min
Delta R.T.: 0.000 min
Response: 129126177
Conc: 245.21 ng/ml

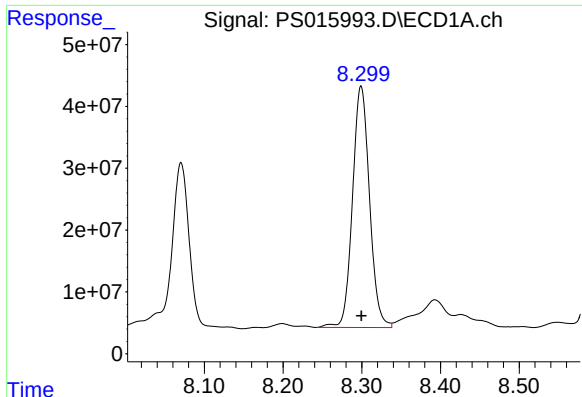

#9 2,4-D


R.T.: 8.299 min
Delta R.T.: 0.000 min
Response: 586201698
Conc: 365.68 ng/ml

Instrument :
ECD_S
ClientSampleId :
FK-BPM-01-B8-C8-B8A-C8AMS

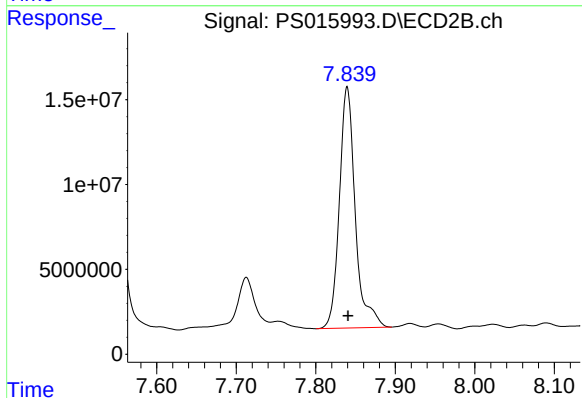


#9 2,4-D

R.T.: 7.840 min
Delta R.T.: -0.001 min
Response: 197636093
Conc: 313.40 ng/ml

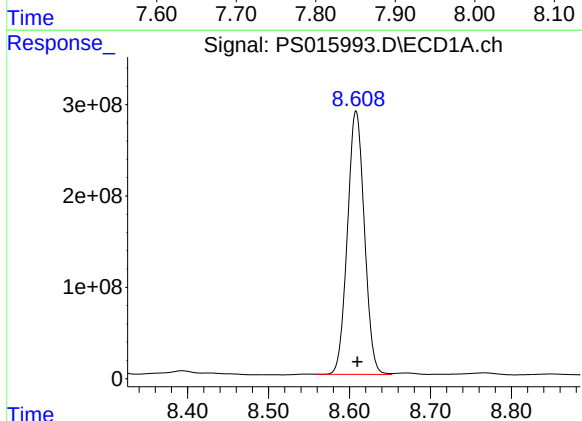


#10 Pentachlorophenol

R.T.: 8.608 min
Delta R.T.: -0.002 min
Response: 4190601308
Conc: 211.47 ng/ml

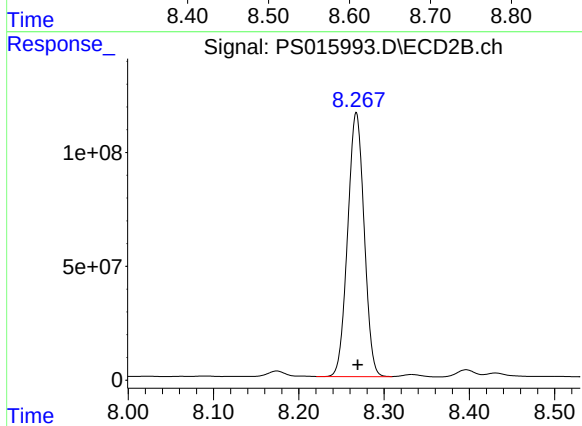

#10 Pentachlorophenol


R.T.: 8.267 min
Delta R.T.: -0.002 min
Response: 1556753888
Conc: 216.42 ng/ml

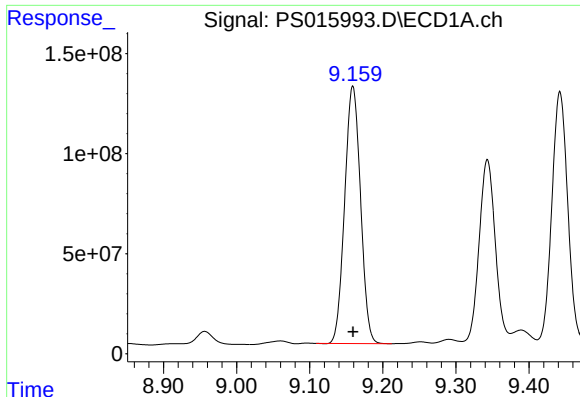

#11 2,4,5-TP (SILVEX)


R.T.: 9.159 min
Delta R.T.: 0.000 min
Response: 1937474465
Conc: 261.10 ng/ml

Instrument :
ECD_S
ClientSampleId :
FK-BPM-01-B8-C8-B8A-C8AMS

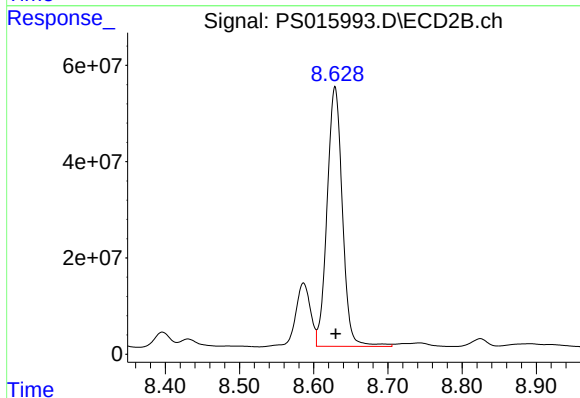


#11 2,4,5-TP (SILVEX)

R.T.: 8.629 min
Delta R.T.: -0.001 min
Response: 771287300
Conc: 273.35 ng/ml

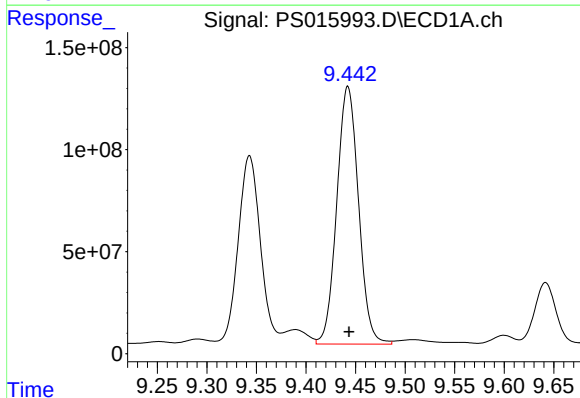


#12 2,4,5-T

R.T.: 9.442 min
Delta R.T.: -0.001 min
Response: 1929000978
Conc: 247.03 ng/ml

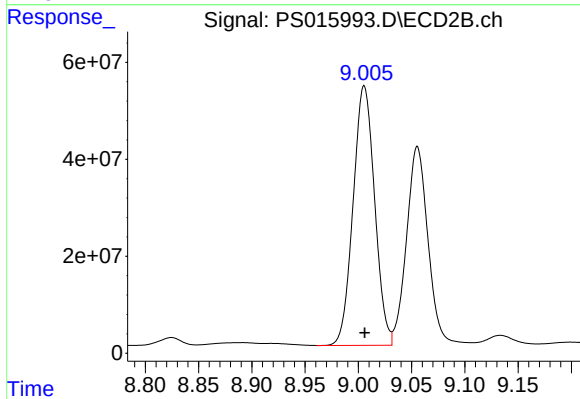

#12 2,4,5-T


R.T.: 9.006 min
Delta R.T.: 0.000 min
Response: 753016253
Conc: 261.03 ng/ml

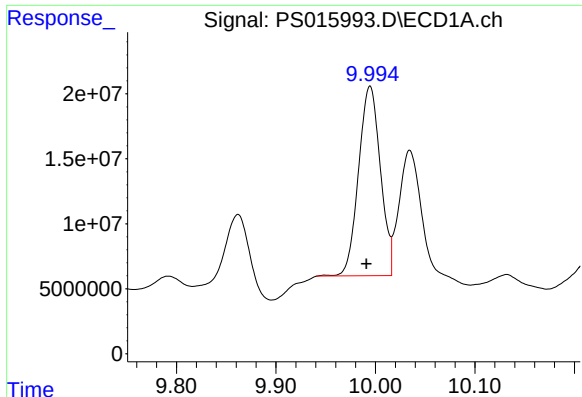

#13 2,4-DB


R.T.: 9.995 min
Delta R.T.: 0.004 min
Response: 22268527
Conc: 133.81 ng/ml

Instrument :
ECD_S
ClientSampleId :
FK-BPM-01-B8-C8-B8A-C8AMS

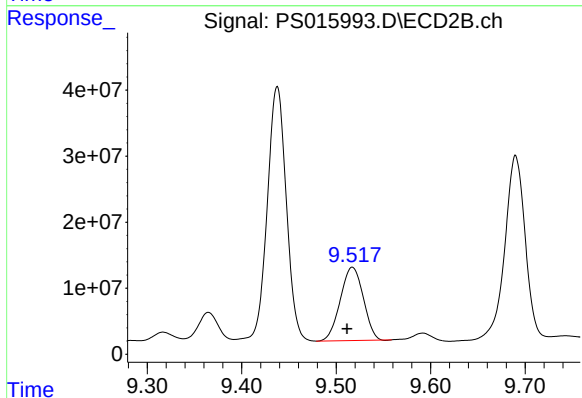


#13 2,4-DB

R.T.: 9.517 min
Delta R.T.: 0.006 min
Response: 187790658
Conc: 499.53 ng/ml

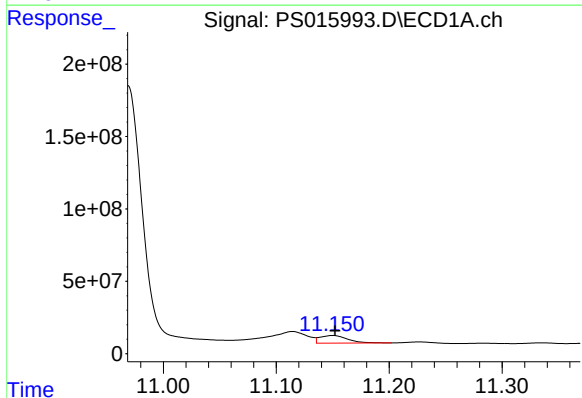


#14 DINOSEB

R.T.: 11.150 min
Delta R.T.: -0.002 min
Response: 89720011
Conc: 16.37 ng/ml

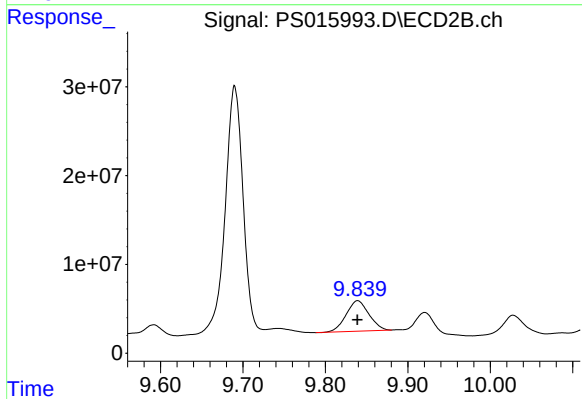

#14 DINOSEB


R.T.: 9.839 min
Delta R.T.: 0.000 min
Response: 65961845
Conc: 32.31 ng/ml

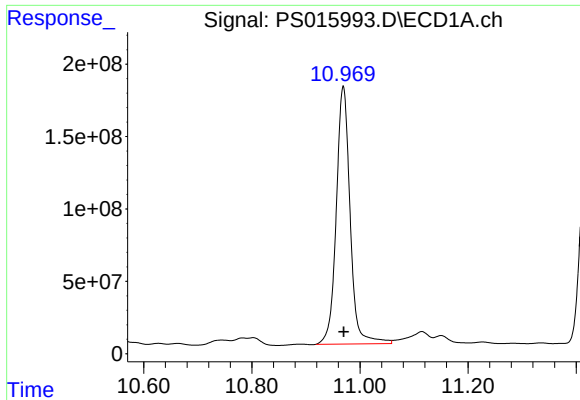

#15 Picloram


R.T.: 10.969 min
Delta R.T.: 0.000 min
Response: 3172928784
Conc: 288.44 ng/ml

Instrument :
ECD_S
ClientSampleId :
FK-BPM-01-B8-C8-B8A-C8AMS

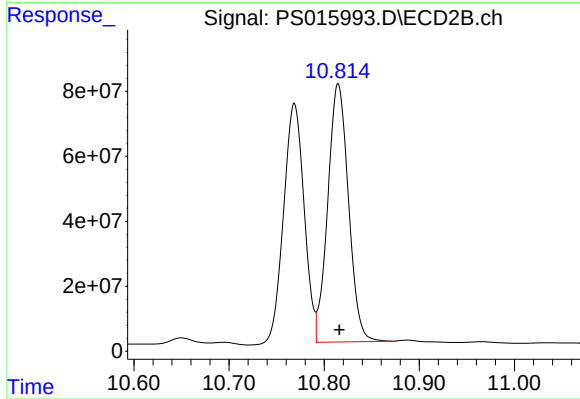


#15 Picloram

R.T.: 10.815 min
Delta R.T.: -0.001 min
Response: 1200204577
Conc: 288.47 ng/ml

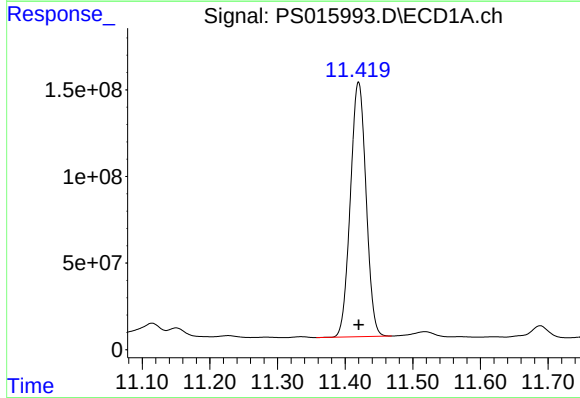

#16 DCPA

R.T.: 11.420 min
Delta R.T.: 0.000 min
Response: 2364843263
Conc: 219.23 ng/ml

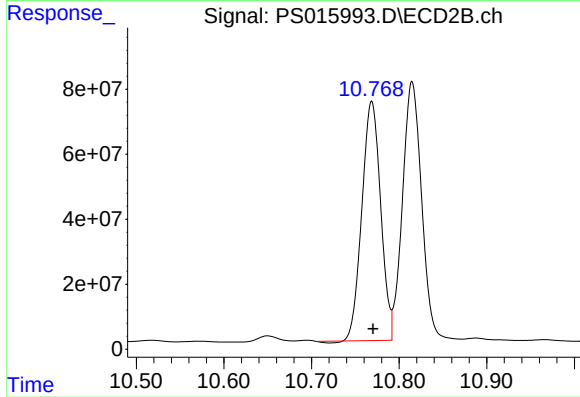

#16 DCPA

R.T.: 10.769 min
Delta R.T.: -0.001 min
Response: 1091939885
Conc: 253.91 ng/ml