

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS063021\
 Data File : PS015972.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jun 2021 17:54
 Operator : DD\AJ
 Sample : HSTDICC750
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HSTDICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 30 00:23:26 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS063021.M
 Quant Title : 8080.M
 QLast Update : Wed Jun 30 00:22:11 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.188	6.767	1184.1E6	396.7E6	750.000	750.000
Target Compounds							
1) T	Dalapon	3.018	2.519	1530.1E6	496.8E6	682.500	682.500
2) T	3,5-DICHL...	6.406	5.958	1557.0E6	557.2E6	697.500	697.500
3) T	4-Nitroph...	7.015	6.387	619.3E6	222.3E6	682.500	682.500
5) T	DICAMBA	7.380	6.930	4198.3E6	1550.8E6	705.000	705.000
6) T	MCPD	7.550	7.028	323.7E6	121.6E6	70.500	70.500
7) T	MCPA	7.699	7.240	459.4E6	185.5E6	69.750	69.750
8) T	DICHLORPROP	8.072	7.550	1007.9E6	380.7E6	705.000	705.000
9) T	2,4-D	8.300	7.841	1162.1E6	459.5E6	705.000	705.000
10) T	Pentachlo...	8.610	8.269	14609.0E6	5324.6E6	712.500	712.500
11) T	2,4,5-TP ...	9.160	8.630	5492.8E6	2093.1E6	712.500	712.500
12) T	2,4,5-T	9.443	9.006	5794.6E6	2144.1E6	712.500	712.500
13) T	2,4-DB	9.991	9.512	1227.3E6	277.7E6	712.500	712.500
14) T	DINOSEB	11.152	9.839	4011.4E6	1511.2E6	705.000	705.000
15) T	Picloram	10.970	10.816	8176.5E6	3113.7E6	712.500	712.500
16) T	DCPA	11.420	10.770	8025.1E6	3226.2E6	720.000	720.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS063021\
Data File : PS015972.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jun 2021 17:54
Operator : DD\AJ
Sample : HSTDICC750
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 30 00:23:26 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS063021.M
Quant Title : 8080.M
QLast Update : Wed Jun 30 00:22:11 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

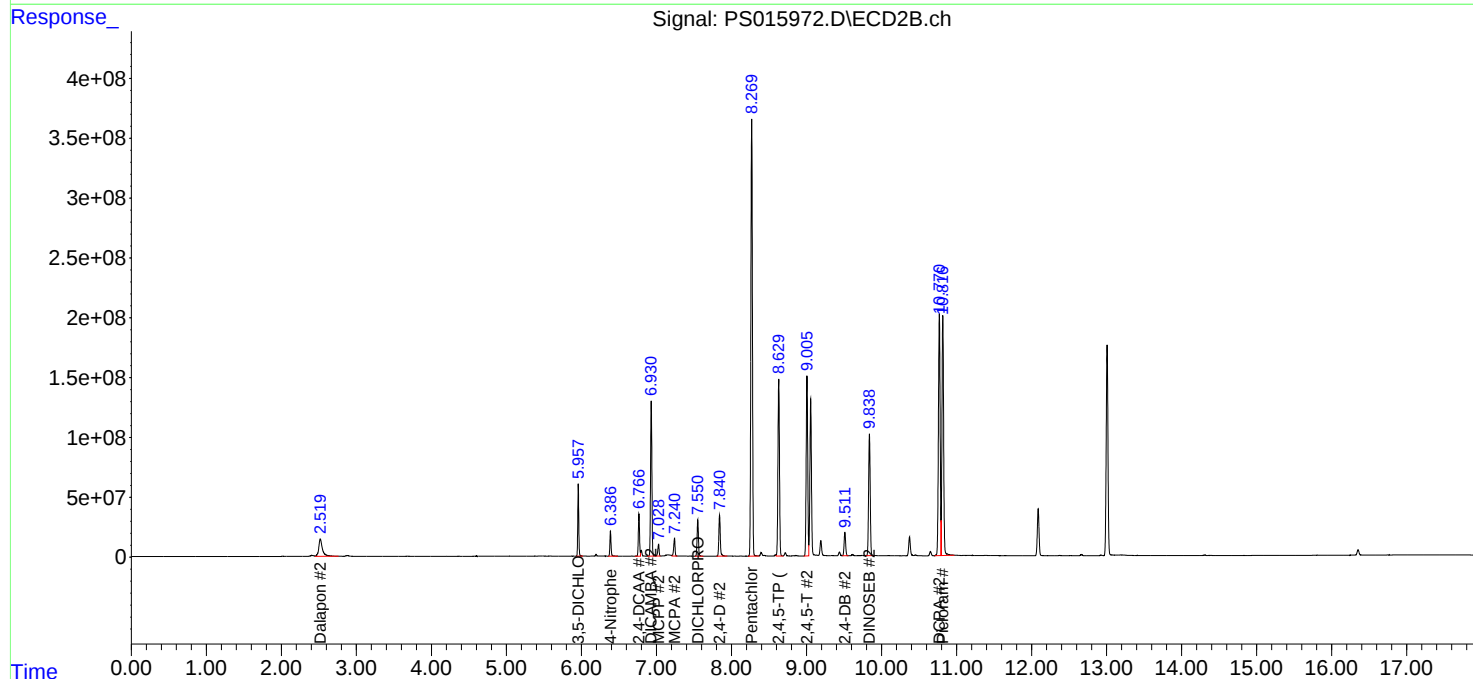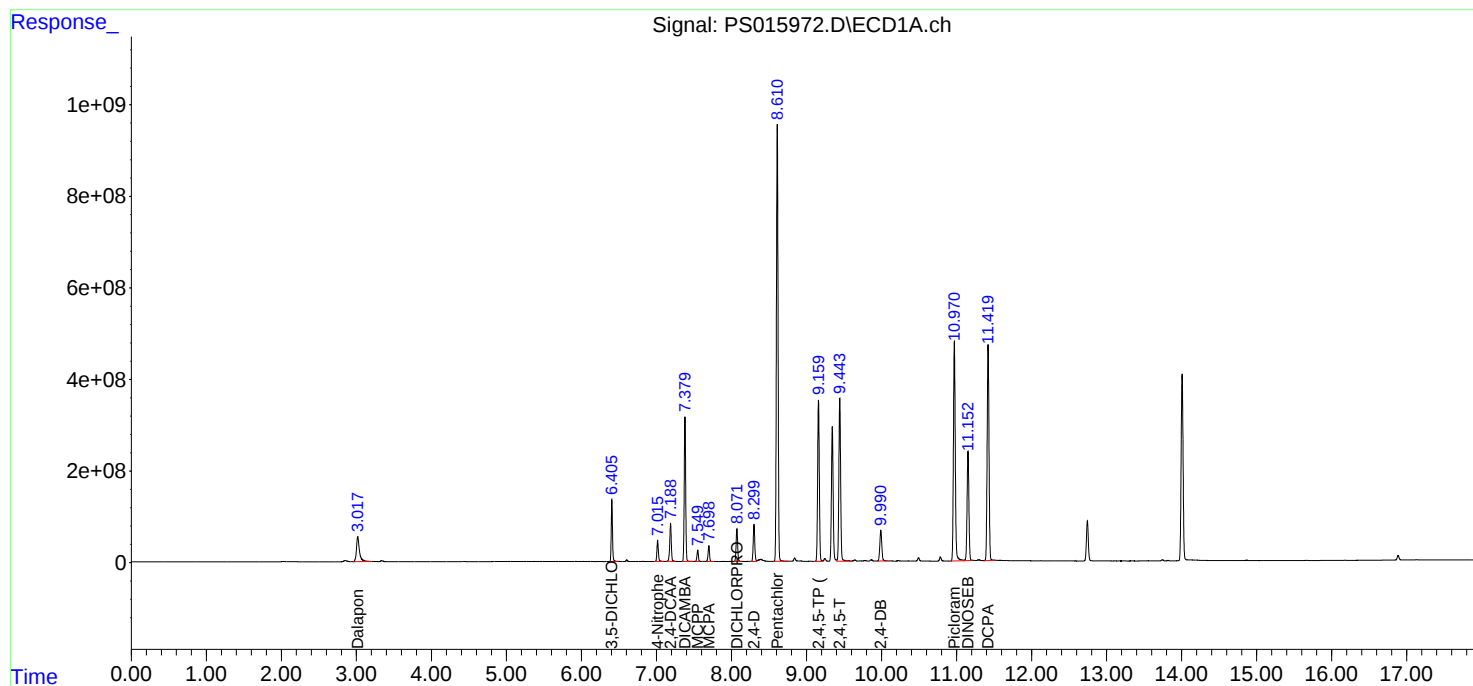


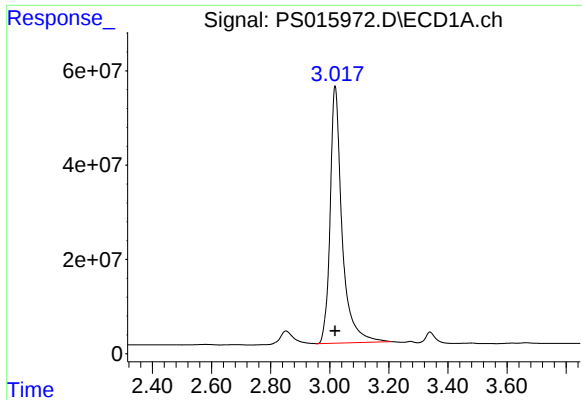

#1 Dalapon


R.T.: 3.018 min
Delta R.T.: 0.000 min
Response: 1530124846
Conc: 682.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

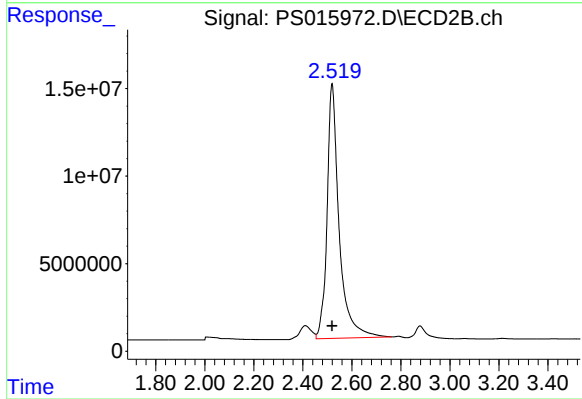


#1 Dalapon

R.T.: 2.519 min
Delta R.T.: 0.000 min
Response: 496753343
Conc: 682.50 ng/ml

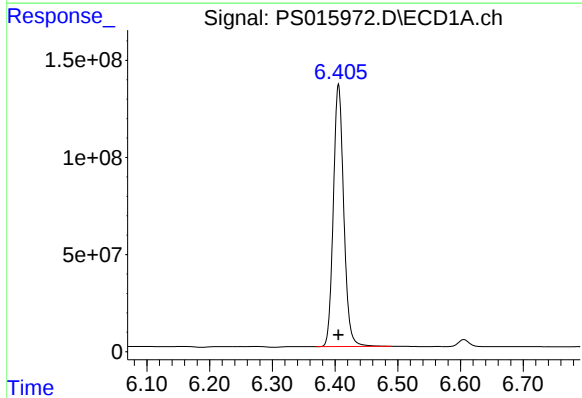


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.406 min
Delta R.T.: 0.000 min
Response: 1556980115
Conc: 697.50 ng/ml

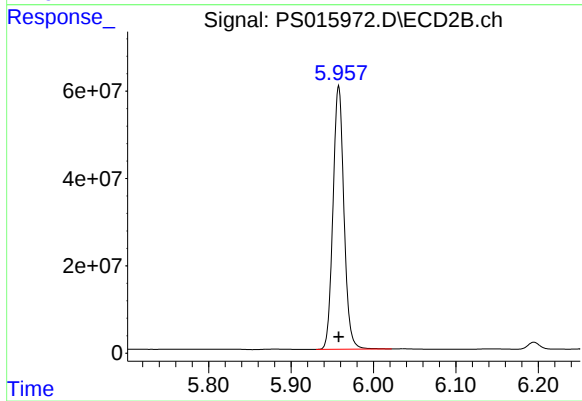

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.958 min
Delta R.T.: 0.000 min
Response: 557184495
Conc: 697.50 ng/ml

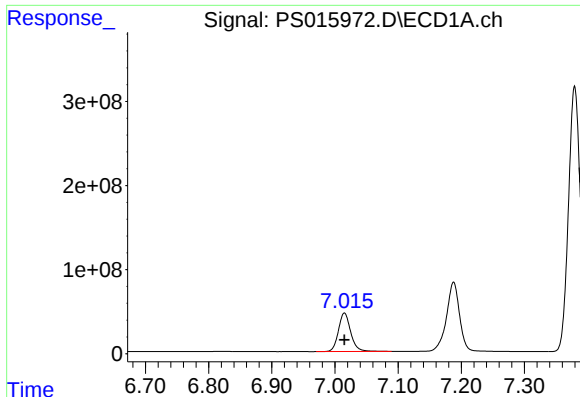

#3 4-Nitrophenol


R.T.: 7.015 min
Delta R.T.: 0.000 min
Response: 619334874
Conc: 682.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

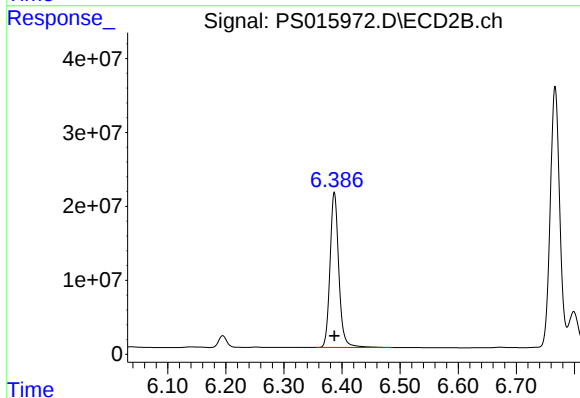


#3 4-Nitrophenol

R.T.: 6.387 min
Delta R.T.: 0.000 min
Response: 222269767
Conc: 682.50 ng/ml

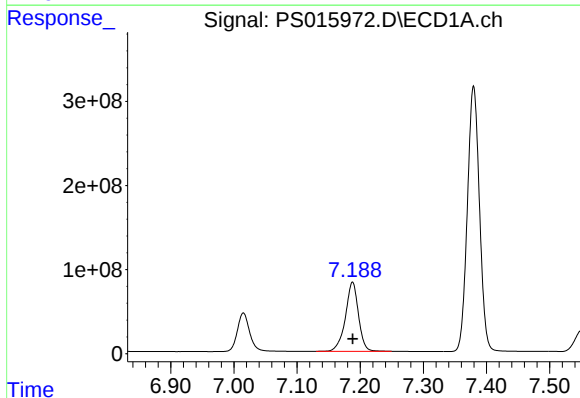


#4 2,4-DCAA

R.T.: 7.188 min
Delta R.T.: 0.000 min
Response: 1184134553
Conc: 750.00 ng/ml

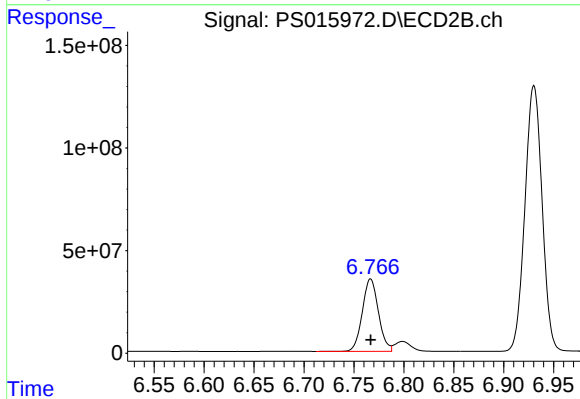

#4 2,4-DCAA


R.T.: 6.767 min
Delta R.T.: 0.000 min
Response: 396695669
Conc: 750.00 ng/ml

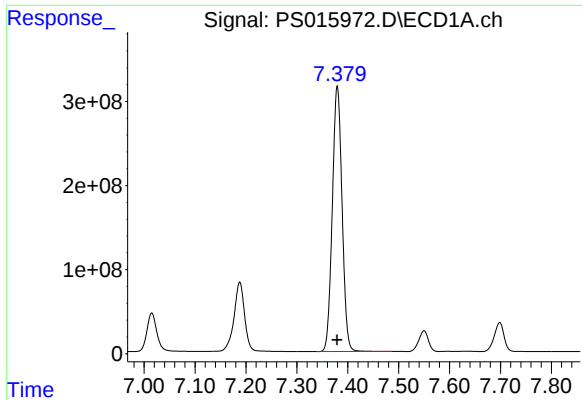

#5 DICAMBA


R.T.: 7.380 min
Delta R.T.: 0.000 min
Response: 4198327442
Conc: 705.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

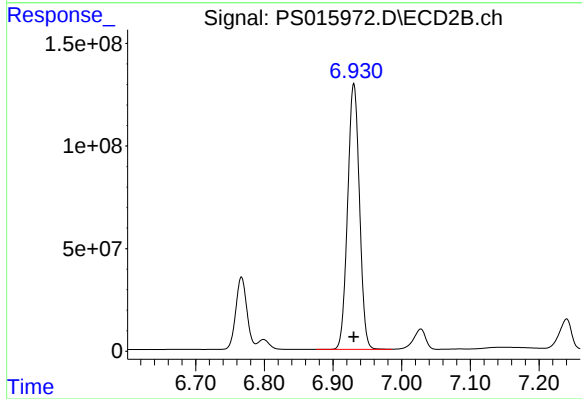


#5 DICAMBA

R.T.: 6.930 min
Delta R.T.: 0.000 min
Response: 1550807694
Conc: 705.00 ng/ml

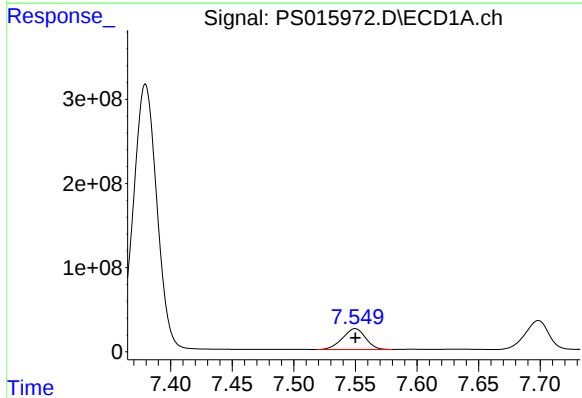


#6 MCP

R.T.: 7.550 min
Delta R.T.: 0.000 min
Response: 323692581
Conc: 70.50 ug/ml

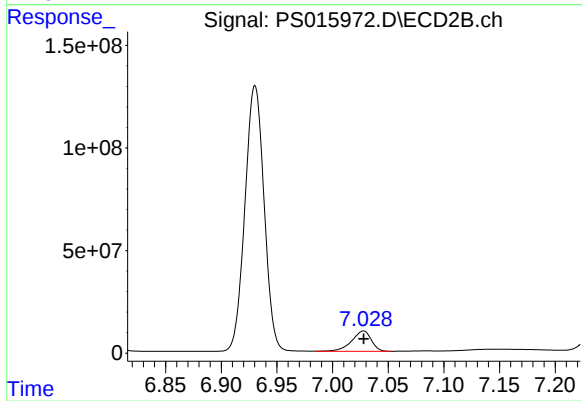

#6 MCP


R.T.: 7.028 min
Delta R.T.: 0.000 min
Response: 121647518
Conc: 70.50 ug/ml

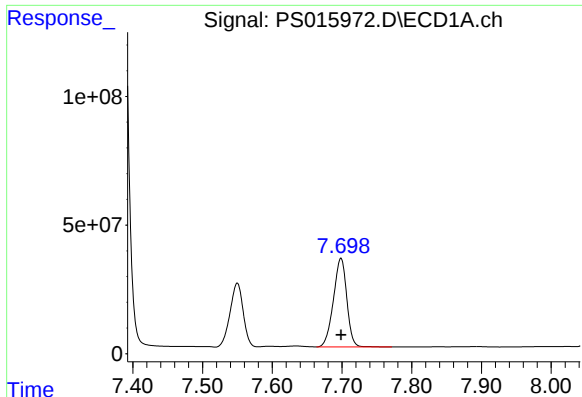

#7 MCPA


R.T.: 7.699 min
Delta R.T.: 0.000 min
Response: 459355577
Conc: 69.75 ug/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

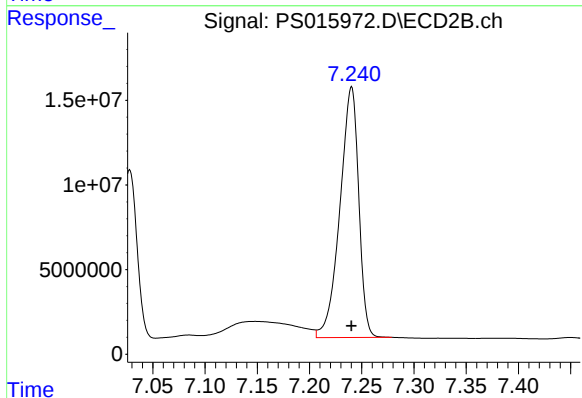


#7 MCPA

R.T.: 7.240 min
Delta R.T.: 0.000 min
Response: 185545402
Conc: 69.75 ug/ml

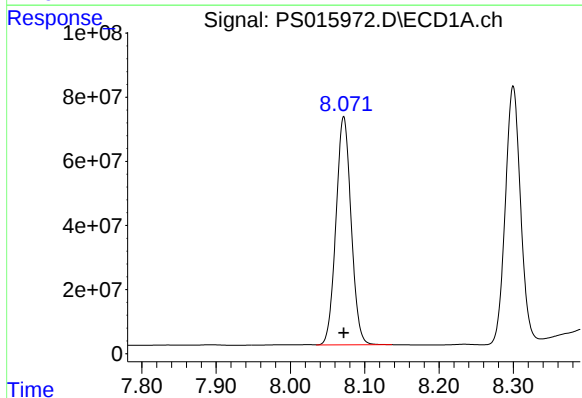


#8 DICHLORPROP

R.T.: 8.072 min
Delta R.T.: 0.000 min
Response: 1007906110
Conc: 705.00 ng/ml

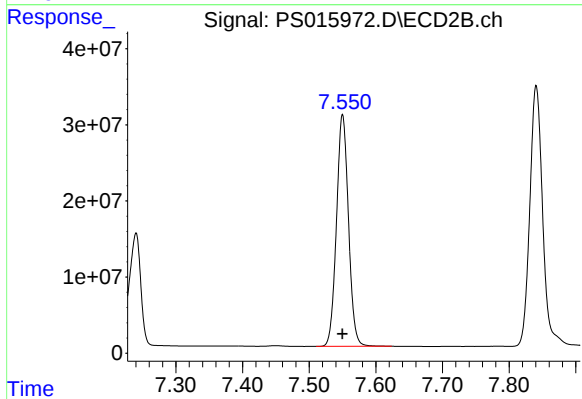

#8 DICHLORPROP


R.T.: 7.550 min
Delta R.T.: 0.000 min
Response: 380700083
Conc: 705.00 ng/ml

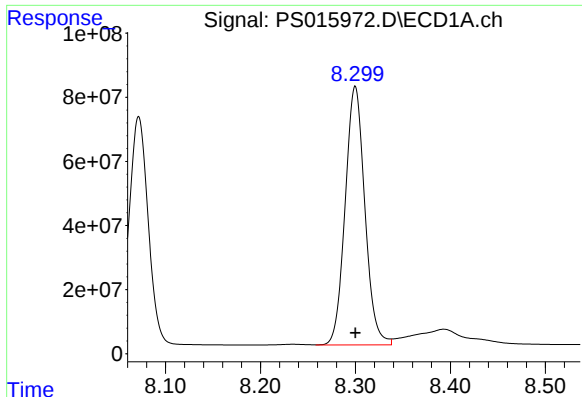

#9 2,4-D


R.T.: 8.300 min
Delta R.T.: 0.000 min
Response: 1162137183
Conc: 705.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

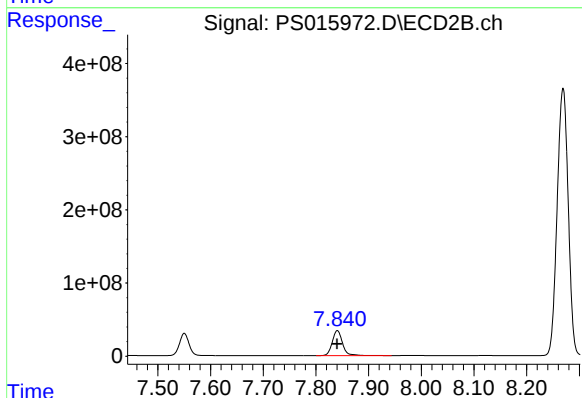


#9 2,4-D

R.T.: 7.841 min
Delta R.T.: 0.000 min
Response: 459484813
Conc: 705.00 ng/ml

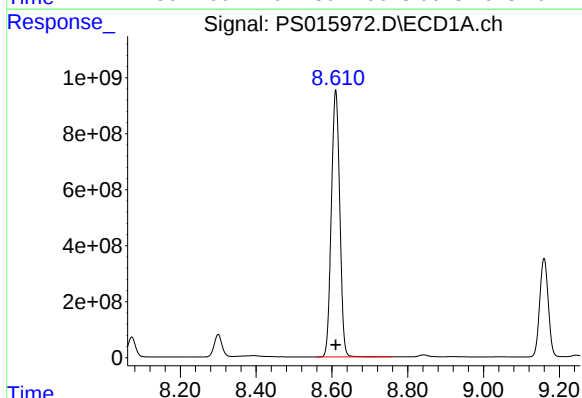


#10 Pentachlorophenol

R.T.: 8.610 min
Delta R.T.: 0.000 min
Response: 14609037390
Conc: 712.50 ng/ml

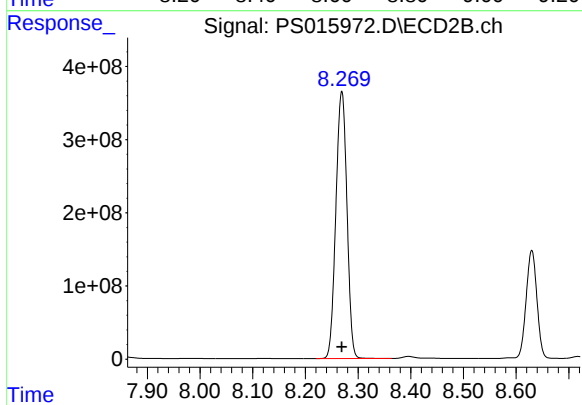

#10 Pentachlorophenol


R.T.: 8.269 min
Delta R.T.: 0.000 min
Response: 5324589171
Conc: 712.50 ng/ml

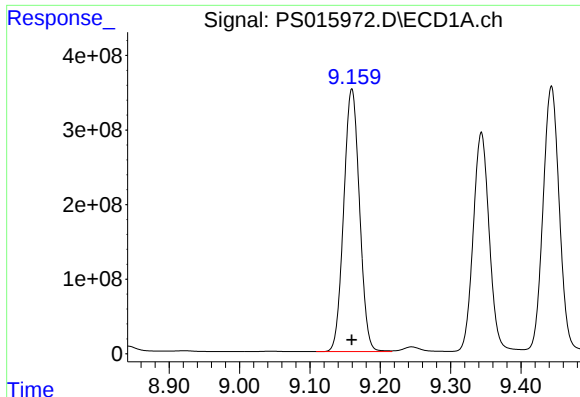

#11 2,4,5-TP (SILVEX)


R.T.: 9.160 min
Delta R.T.: 0.000 min
Response: 5492845001
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

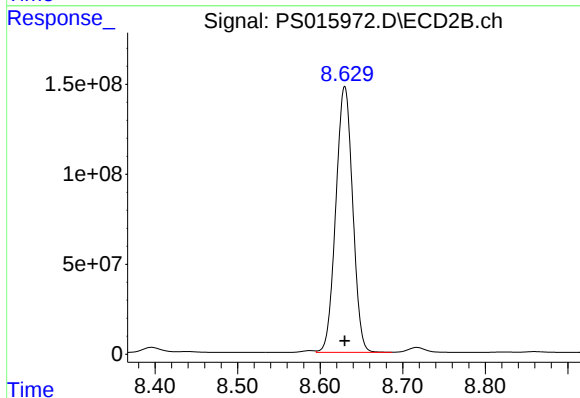


#11 2,4,5-TP (SILVEX)

R.T.: 8.630 min
Delta R.T.: 0.000 min
Response: 2093104783
Conc: 712.50 ng/ml

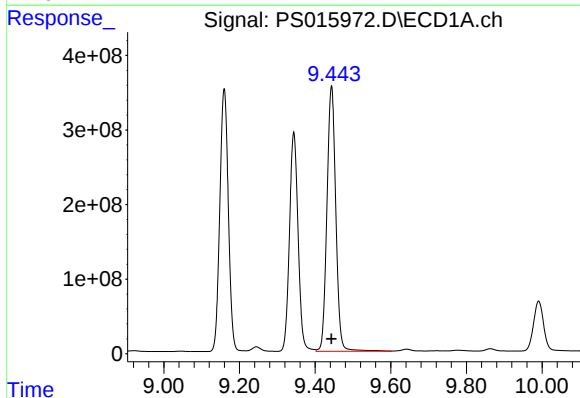


#12 2,4,5-T

R.T.: 9.443 min
Delta R.T.: 0.000 min
Response: 5794562977
Conc: 712.50 ng/ml

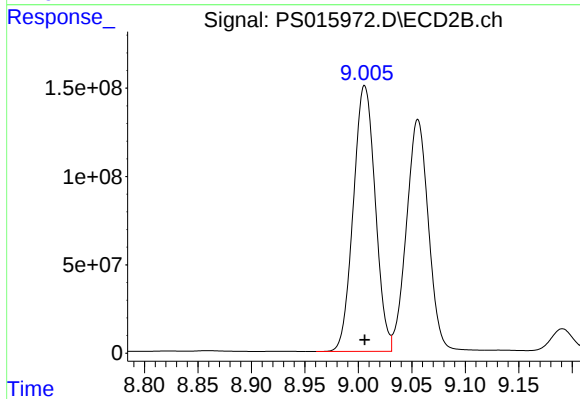

#12 2,4,5-T


R.T.: 9.006 min
Delta R.T.: 0.000 min
Response: 2144148750
Conc: 712.50 ng/ml

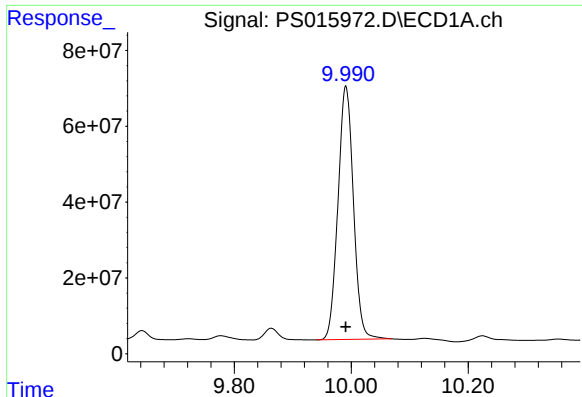

#13 2,4-DB


R.T.: 9.991 min
Delta R.T.: 0.000 min
Response: 1227255825
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

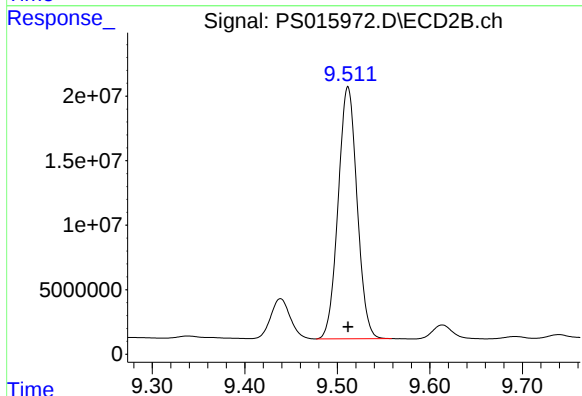


#13 2,4-DB

R.T.: 9.512 min
Delta R.T.: 0.000 min
Response: 277650292
Conc: 712.50 ng/ml

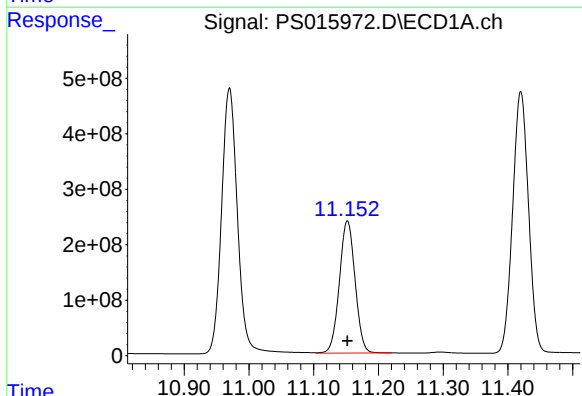


#14 DINOSEB

R.T.: 11.152 min
Delta R.T.: 0.000 min
Response: 4011353654
Conc: 705.00 ng/ml

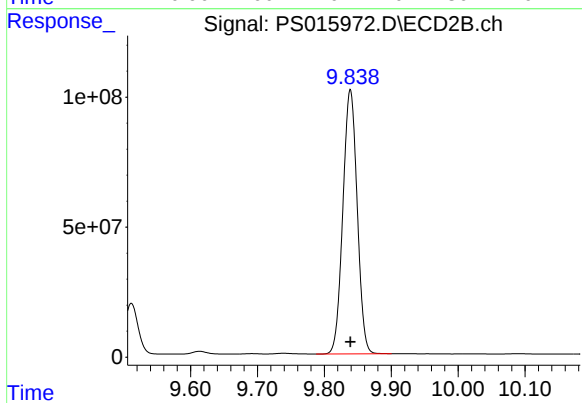

#14 DINOSEB


R.T.: 9.839 min
Delta R.T.: 0.000 min
Response: 1511201313
Conc: 705.00 ng/ml

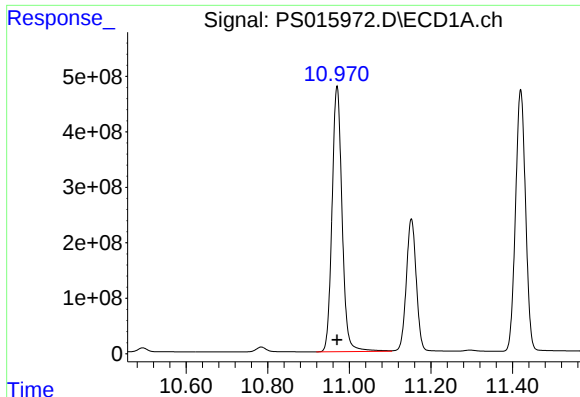

#15 Picloram


R.T.: 10.970 min
Delta R.T.: 0.000 min
Response: 8176479781
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

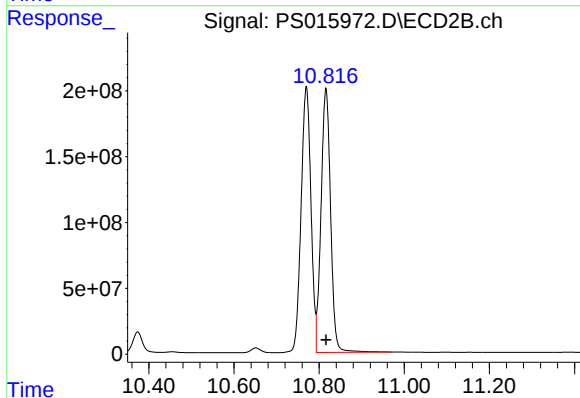


#15 Picloram

R.T.: 10.816 min
Delta R.T.: 0.000 min
Response: 3113742840
Conc: 712.50 ng/ml

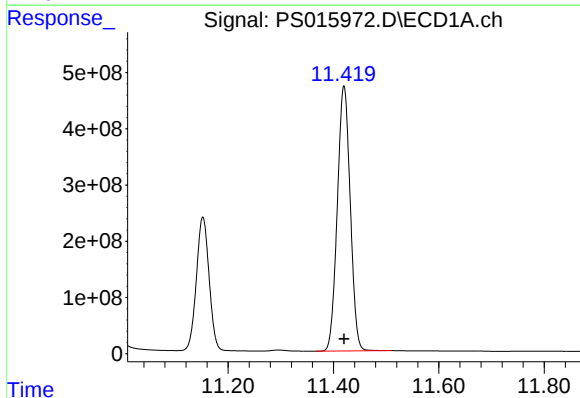

#16 DCPA

R.T.: 11.420 min
Delta R.T.: 0.000 min
Response: 8025103524
Conc: 720.00 ng/ml

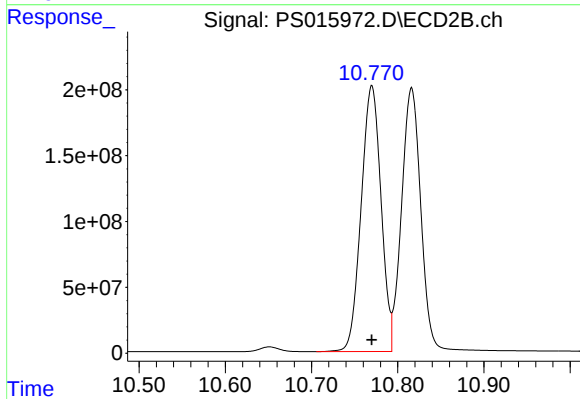

#16 DCPA

R.T.: 10.770 min
Delta R.T.: 0.000 min
Response: 3226223813
Conc: 720.00 ng/ml