

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS063021\
 Data File : PS015992.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Jun 2021 02:47
 Operator : DD\AJ
 Sample : M2834-01
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 FK-BPM-01-B8-C8-B8A-C8A

Manual Integrations
 APPROVED

mohammad
 6/30/2021 2:04:22 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 30 05:24:03 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS063021.M
 Quant Title : 8080.M
 QLast Update : Wed Jun 30 00:31:48 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	7.187	6.765	817.6E6	230.9E6	532.557m	449.853m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS063021\
Data File : PS015992.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Jun 2021 02:47
Operator : DD\AJ
Sample : M2834-01
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
FK-BPM-01-B8-C8-B8A-C8A


Manual Integrations
APPROVED

mohammad
6/30/2021 2:04:22 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 30 05:24:03 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS063021.M
Quant Title : 8080.M
QLast Update : Wed Jun 30 00:31:48 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

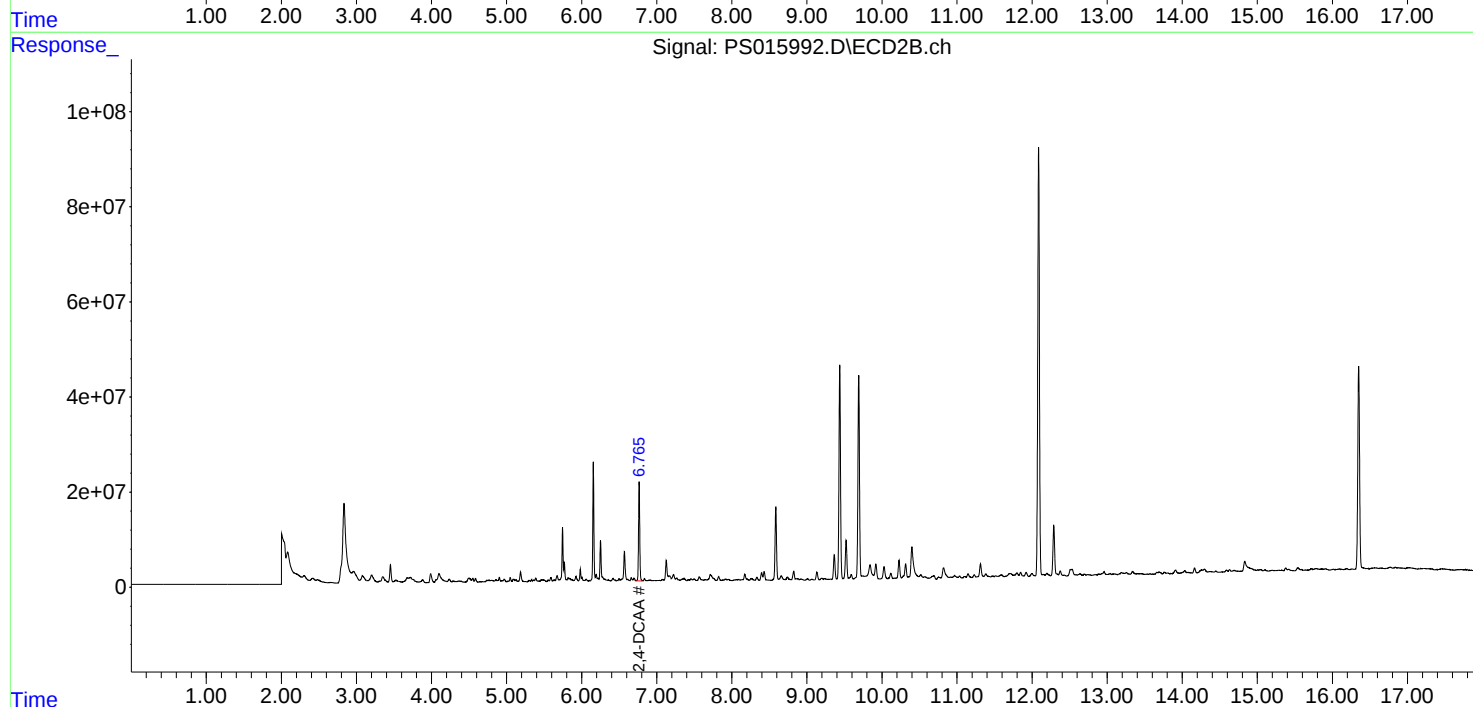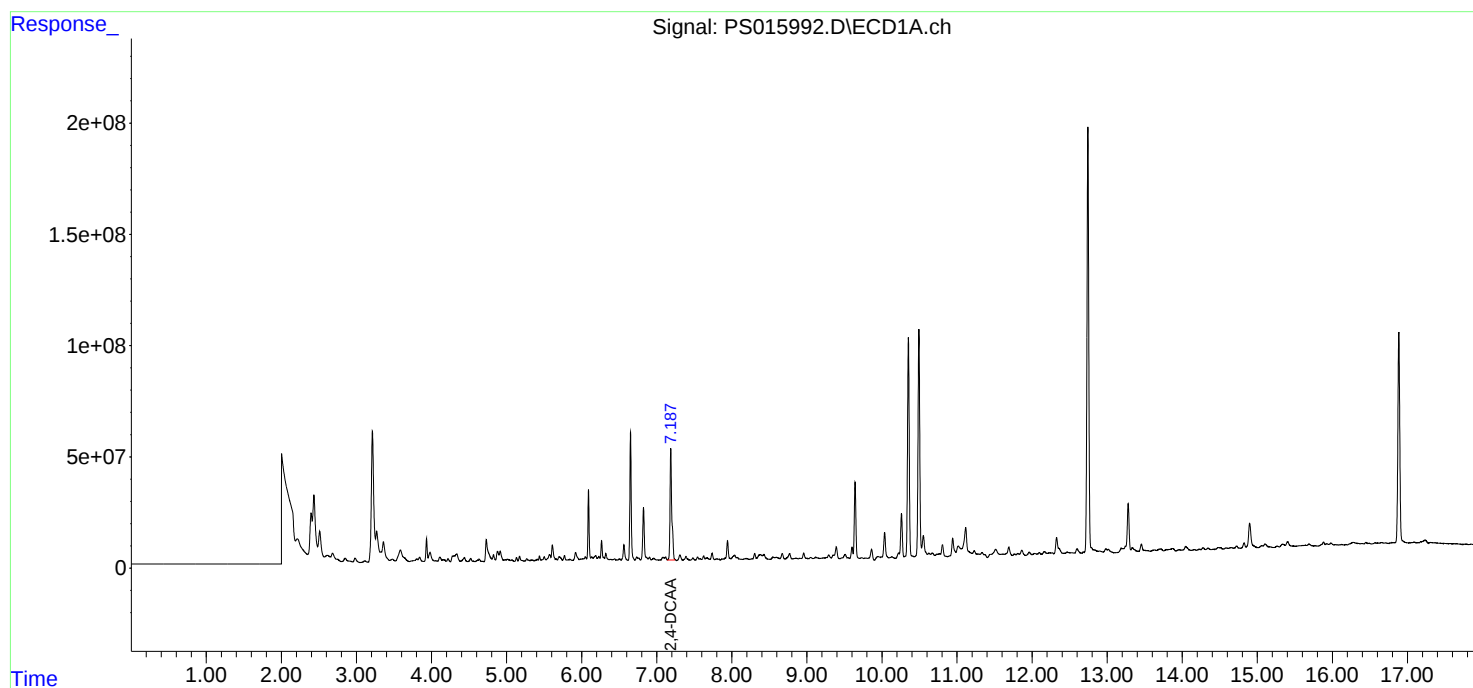

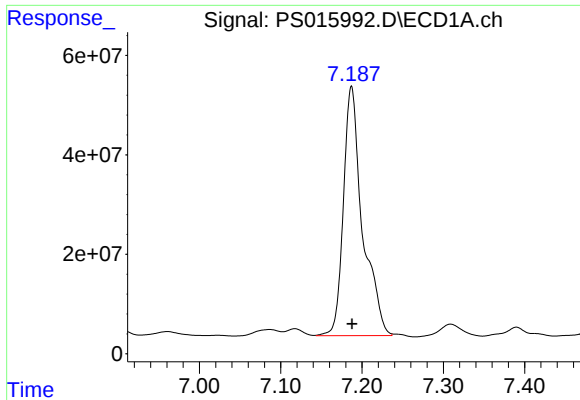


#4 2,4-DCAA

R.T.: 7.187 min
Delta R.T.: -0.001 min
Response: 817580535
Conc: 532.56 ng/ml m

Instrument :
ECD_S
ClientSampleId :
FK-BPM-01-B8-C8-B8A-C8A

Manual Integrations
APPROVED

mohammad
6/30/2021 2:04:22 PM

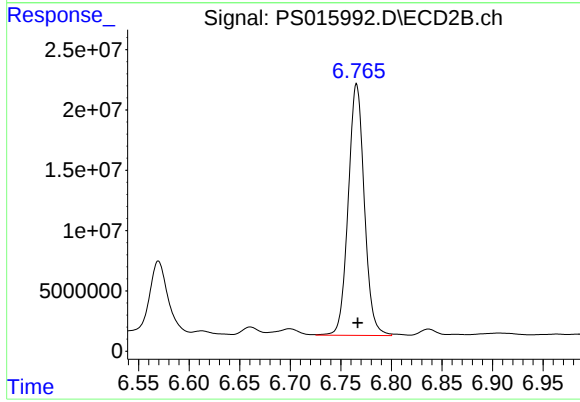

#4 2,4-DCAA

R.T.: 6.765 min
Delta R.T.: -0.002 min
Response: 230917371
Conc: 449.85 ng/ml m