

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS063022\
 Data File : PS019857.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Jun 2022 14:14
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 12 04:42:30 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062722.M
 Quant Title : 8080.M
 QLast Update : Mon Jun 27 17:26:48 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.200	6.780	1359.9E6	453.5E6	524.322	558.421
Target Compounds							
1) T	Dalapon	3.018	0.000	666595	0	<MDL	N.D. #
2) T	3,5-DICHL...	6.447	5.991	2178393	306021	<MDL	<MDL #
5) T	DICAMBA	7.391	6.947	10468116	4754214	1.020	1.303 #
7) T	MCPA	7.655f	0.000	4198508	0	<MDL	N.D. #
8) T	DICHLORPROP	8.095	7.579	3585004	2329295	1.324	2.476 #
10) T	Pentachlo...	8.621	8.285	18055016	6246130	<MDL	<MDL #
11) T	2,4,5-TP ...	9.184	8.657	29609414	8418602	1.851	1.589
12) T	2,4,5-T	9.413	9.055	348.4E6	8187436	18.935	1.676 #
13) T	2,4-DB	9.970	9.576f	899427	1099978	<MDL	1.694 #
14) T	DINOSEB	11.156	9.855	222.8E6	9793893	13.703	2.748 #
15) T	Picloram	10.976	10.870f	24893421	253.4E6	<MDL	38.965 #
16) T	DCPA	11.427	10.780	89008624	17851000	3.450	2.754



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS063022\
Data File : PS019857.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Jun 2022 14:14
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 12 04:42:30 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062722.M
Quant Title : 8080.M
QLast Update : Mon Jun 27 17:26:48 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

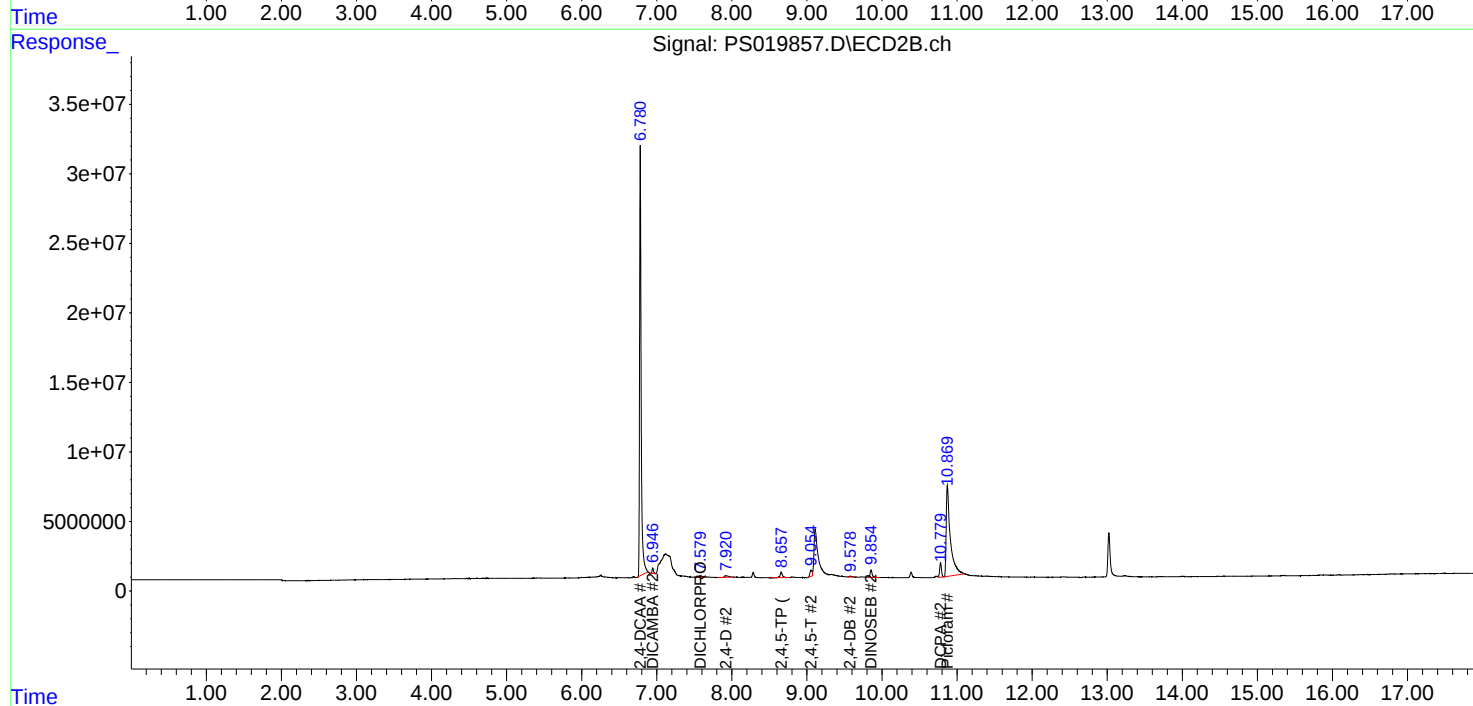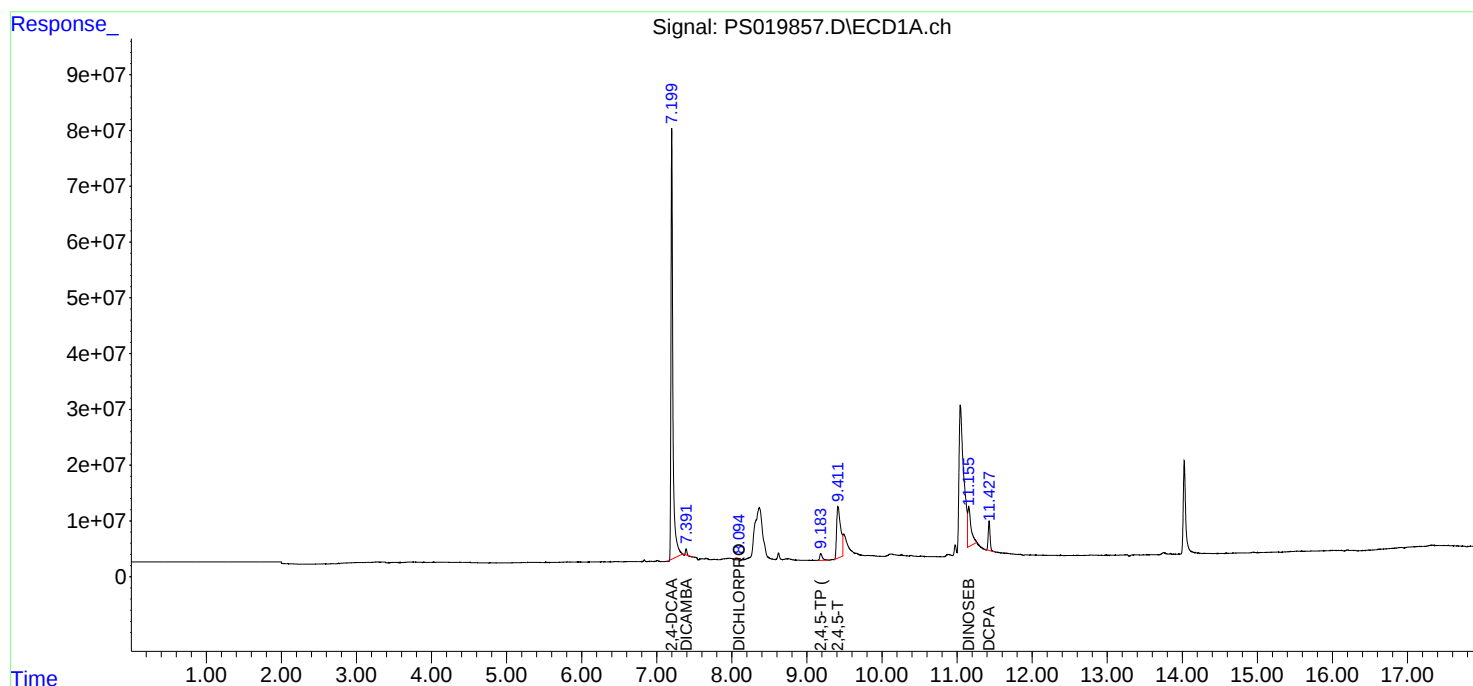


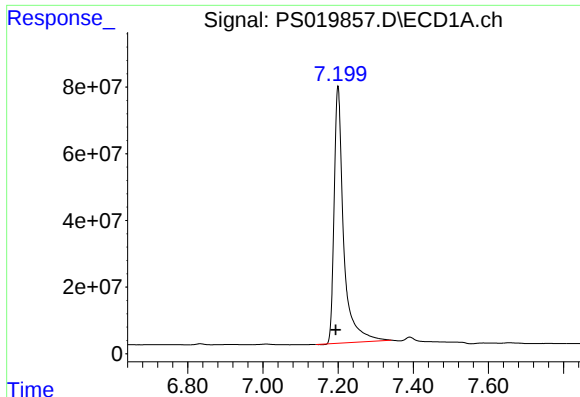

#4 2,4-DCAA


R.T.: 7.200 min
Delta R.T.: 0.006 min
Response: 1359908983
Conc: 524.32 ng/ml

Instrument :
ECD_S
ClientSampleId :

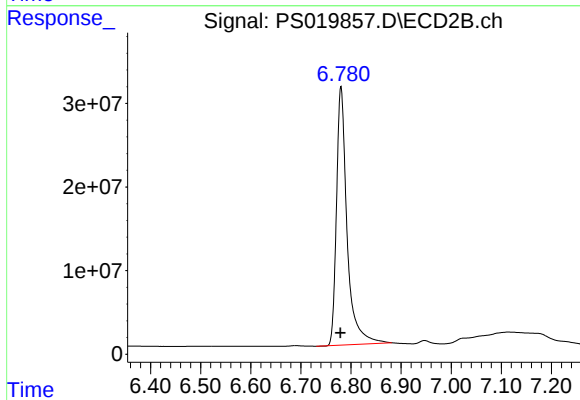


#4 2,4-DCAA

R.T.: 6.780 min
Delta R.T.: 0.001 min
Response: 453519826
Conc: 558.42 ng/ml

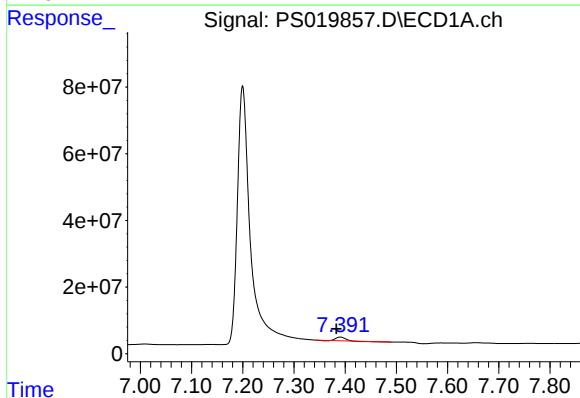


#5 DICAMBA

R.T.: 7.391 min
Delta R.T.: 0.008 min
Response: 10468116
Conc: 1.02 ng/ml

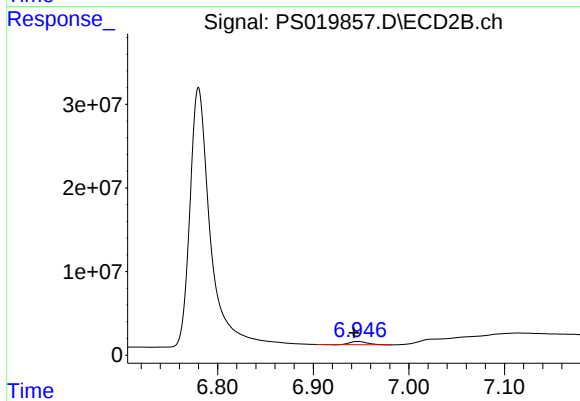

#5 DICAMBA


R.T.: 6.947 min
Delta R.T.: 0.004 min
Response: 4754214
Conc: 1.30 ng/ml

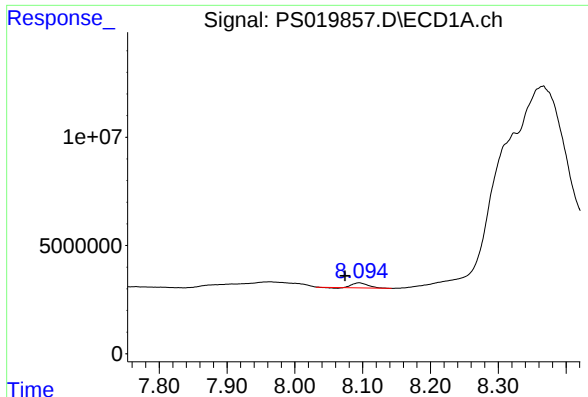

#8 DICHLORPROP


R.T.: 8.095 min
Delta R.T.: 0.021 min
Response: 3585004
Conc: 1.32 ng/ml

Instrument :
ECD_S
ClientSampleId :

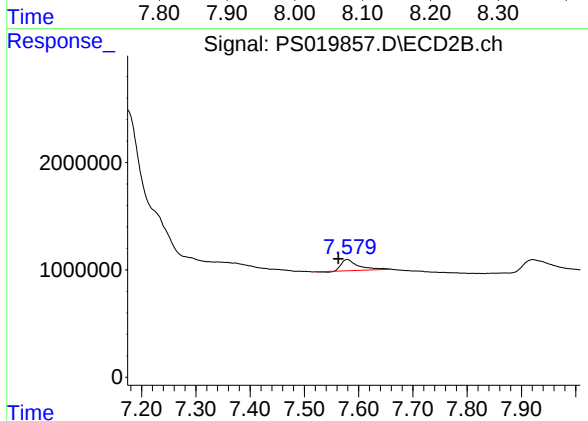


#8 DICHLORPROP

R.T.: 7.579 min
Delta R.T.: 0.016 min
Response: 2329295
Conc: 2.48 ng/ml

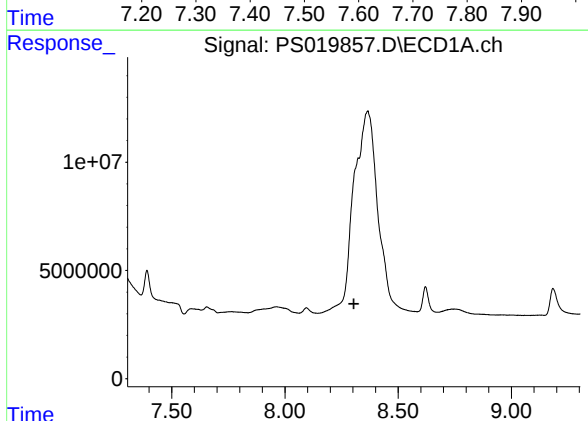


#9 2,4-D

R.T.: 8.365 min
Delta R.T.: 0.061 min
Response: -86476656
Conc: N.D.

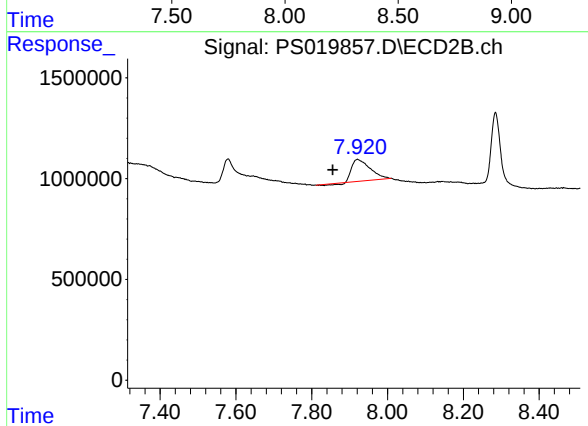

#9 2,4-D


R.T.: 7.921 min
Delta R.T.: 0.065 min
Response: 3519240
Conc: 3.12 ng/ml

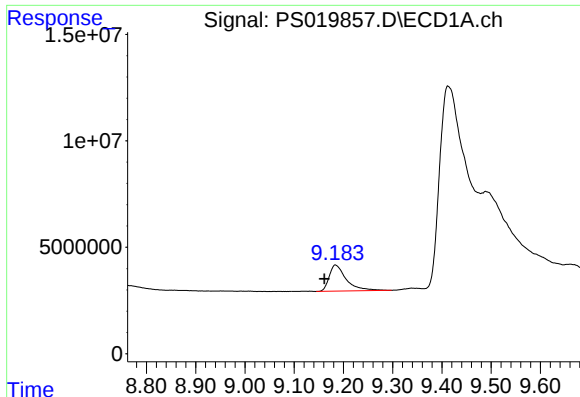

#11 2,4,5-TP (SILVEX)


R.T.: 9.184 min
Delta R.T.: 0.023 min
Response: 29609414
Conc: 1.85 ng/ml

Instrument :
ECD_S
ClientSampleId :

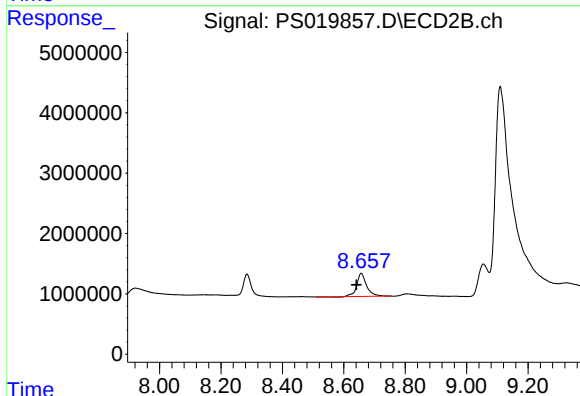


#11 2,4,5-TP (SILVEX)

R.T.: 8.657 min
Delta R.T.: 0.016 min
Response: 8418602
Conc: 1.59 ng/ml

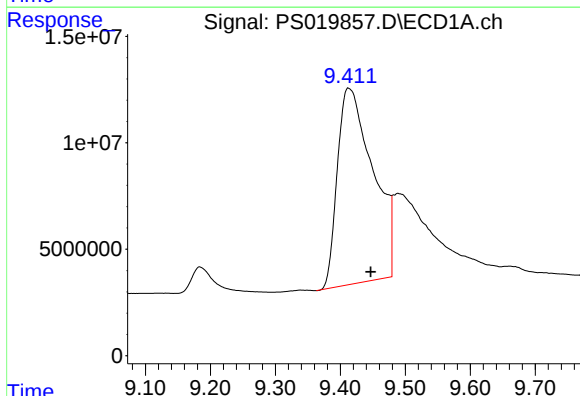


#12 2,4,5-T

R.T.: 9.413 min
Delta R.T.: -0.034 min
Response: 348397234
Conc: 18.93 ng/ml

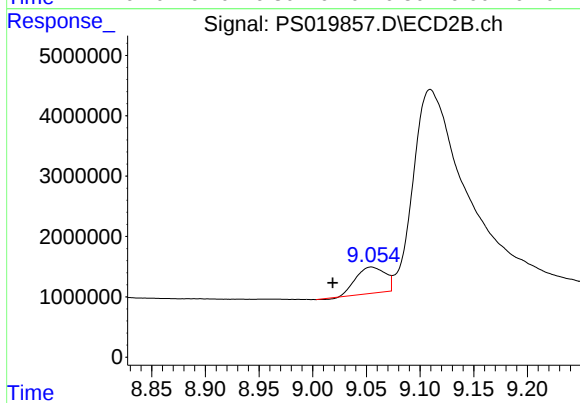

#12 2,4,5-T


R.T.: 9.055 min
Delta R.T.: 0.036 min
Response: 8187436
Conc: 1.68 ng/ml

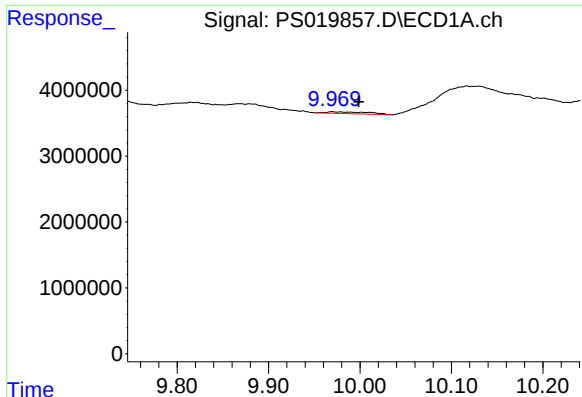

#13 2,4-DB


R.T.: 9.970 min
Delta R.T.: -0.029 min
Response: 899427
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

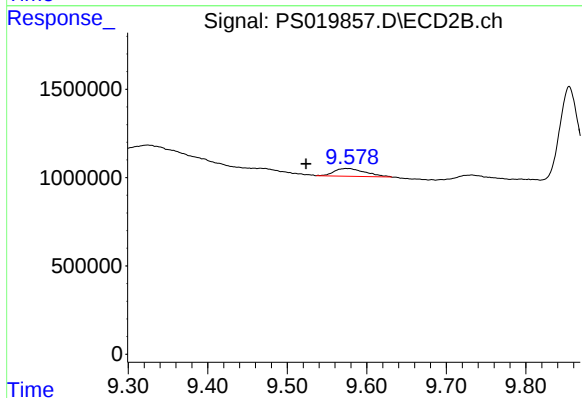


#13 2,4-DB

R.T.: 9.576 min
Delta R.T.: 0.052 min
Response: 1099978
Conc: 1.69 ng/ml

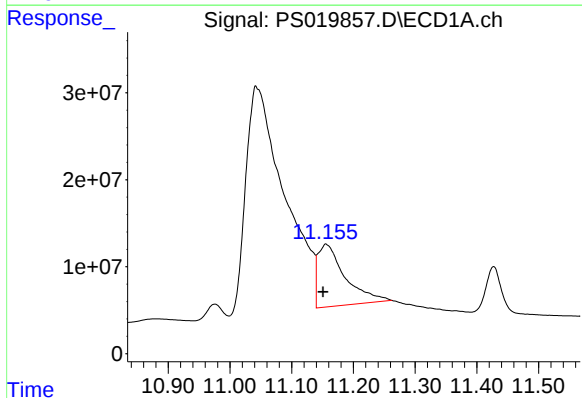


#14 DINOSEB

R.T.: 11.156 min
Delta R.T.: 0.005 min
Response: 222775531
Conc: 13.70 ng/ml

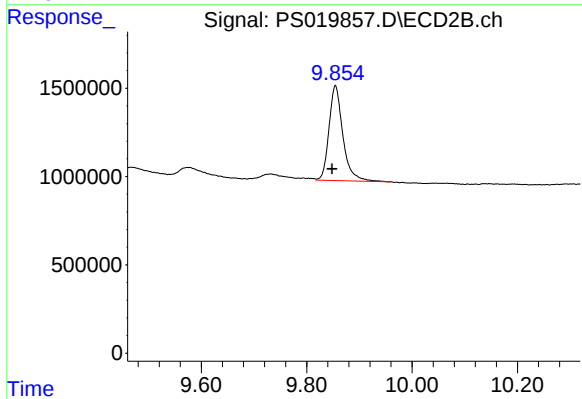

#14 DINOSEB


R.T.: 9.855 min
Delta R.T.: 0.007 min
Response: 9793893
Conc: 2.75 ng/ml

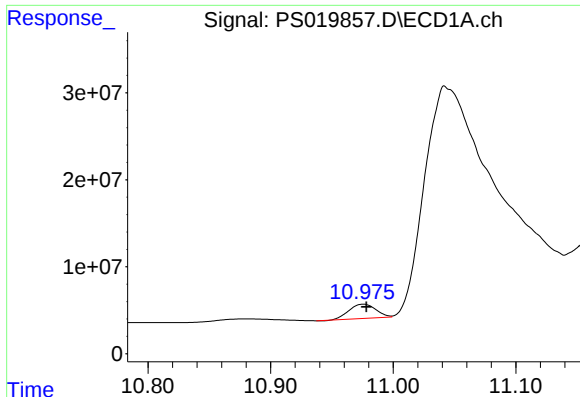

#15 Picloram


R.T.: 10.976 min
Delta R.T.: -0.003 min
Response: 24893421
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

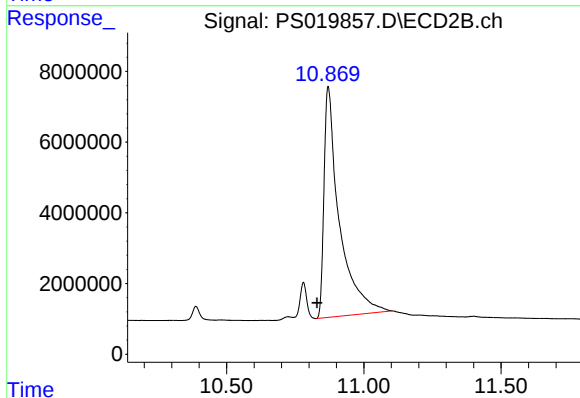


#15 Picloram

R.T.: 10.870 min
Delta R.T.: 0.041 min
Response: 253414191
Conc: 38.97 ng/ml

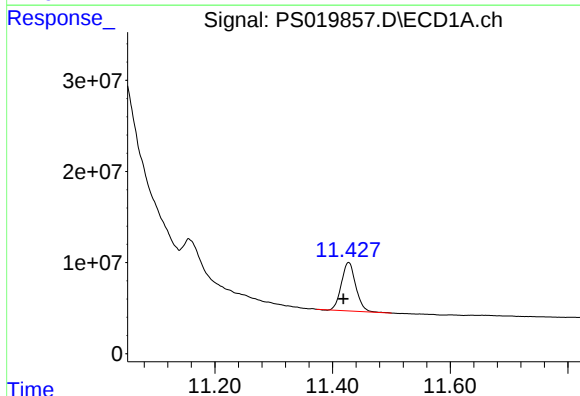

#16 DCPA

R.T.: 11.427 min
Delta R.T.: 0.009 min
Response: 89008624
Conc: 3.45 ng/ml

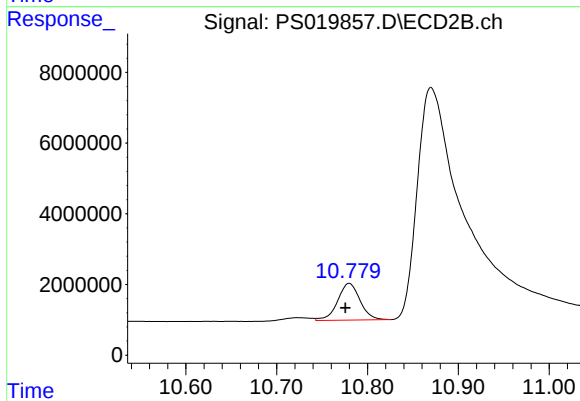

#16 DCPA

R.T.: 10.780 min
Delta R.T.: 0.004 min
Response: 17851000
Conc: 2.75 ng/ml