

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070120\
 Data File : PS011020.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Jul 2020 12:42
 Operator : DD\AJ
 Sample : L3148-07
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 01 15:49:29 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062420.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 25 02:45:12 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.229	6.919	226.7E6	168.9E6	249.943	304.882
Target Compounds							
1) T	Dalapon	2.997	2.584	42080003	125.5E6	37.581	166.413 #
2) T	3,5-DICHL...	0.000	6.099	0	83214297	N.D.	99.918
3) T	4-Nitroph...	6.997	6.551	5196842	3523650	13.019	10.966
5) T	DICAMBA	7.409	0.000	5525295	0	1.515	N.D. #
7) T	MCPA	7.693	7.463	81733238	78229241	20.523	28.344 #
8) T	DICHLORPROP	0.000	7.739	0	4958114	N.D.	8.445
10) T	Pentachlo...	8.709	0.000	11204456	0	<MDL	N.D. #
12) T	2,4,5-T	9.427	0.000	33474820	0	7.187	N.D. #
14) T	DINOSEB	11.167	0.000	15149917	0	4.230	N.D. #
15) T	Picloram	10.994	0.000	30042862	0	5.359	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070120\
Data File : PS011020.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Jul 2020 12:42
Operator : DD\AJ
Sample : L3148-07
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 01 15:49:29 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062420.M
Quant Title : 8080.M
QLast Update : Thu Jun 25 02:45:12 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

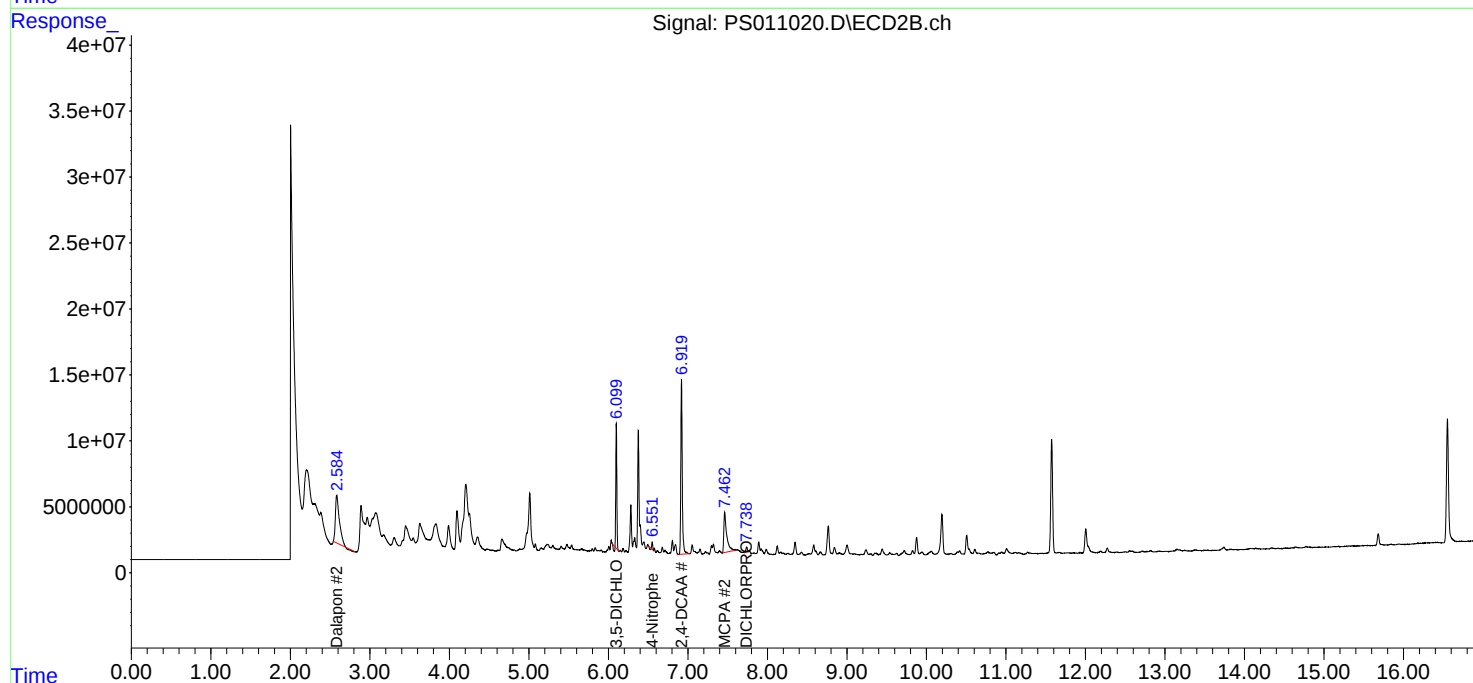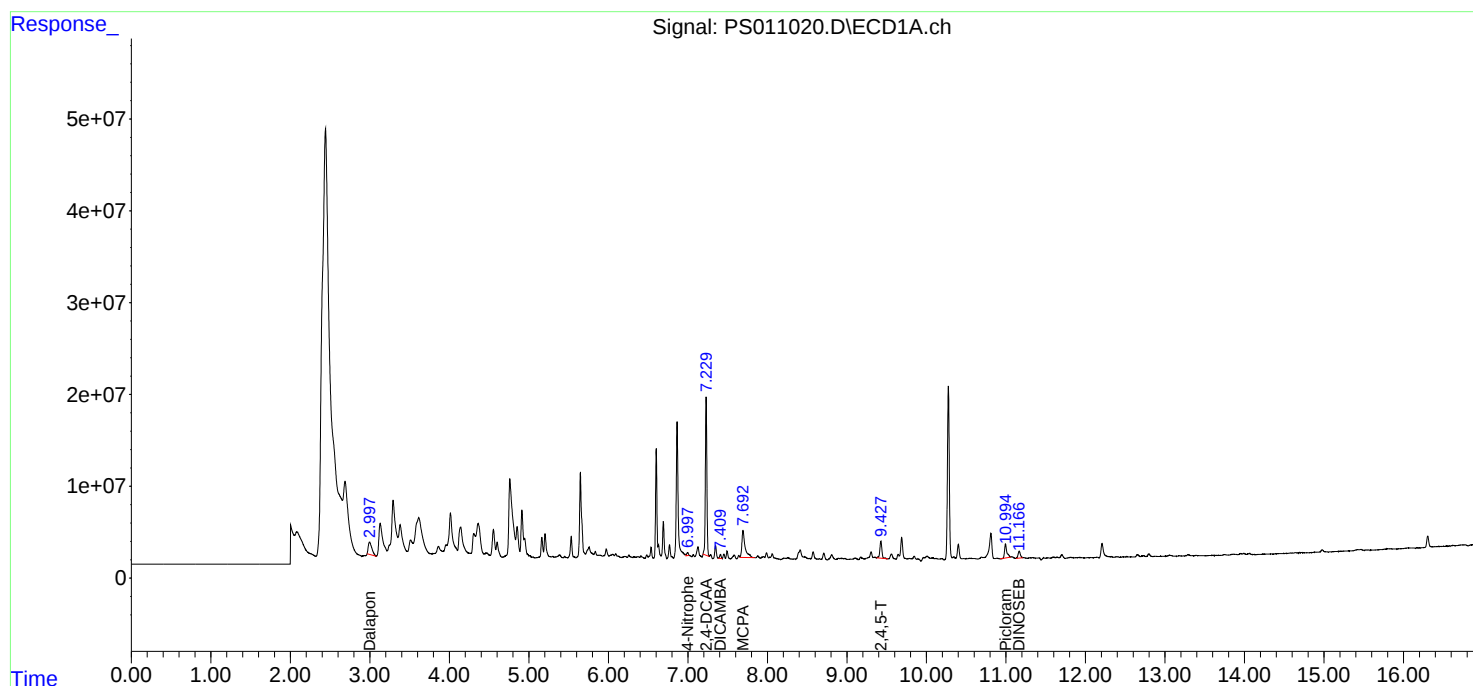


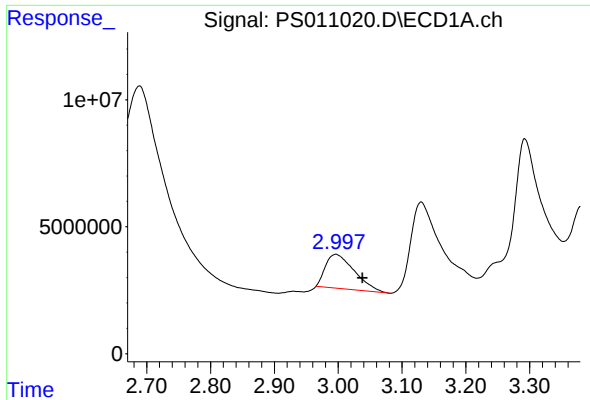

#1 Dalapon


R.T.: 2.997 min
Delta R.T.: -0.041 min
Response: 42080003
Conc: 37.58 ng/ml

Instrument :
ECD_S
ClientSampleId :

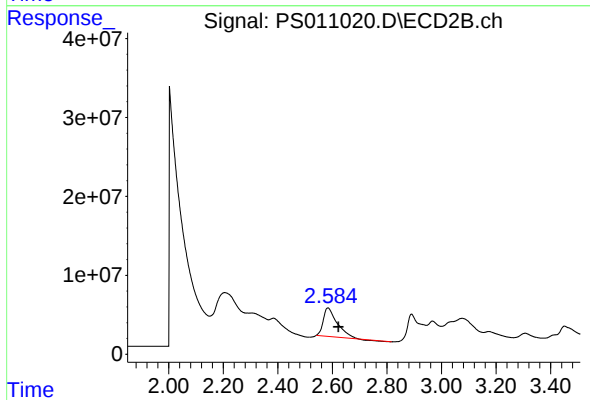


#1 Dalapon

R.T.: 2.584 min
Delta R.T.: -0.038 min
Response: 125535767
Conc: 166.41 ng/ml

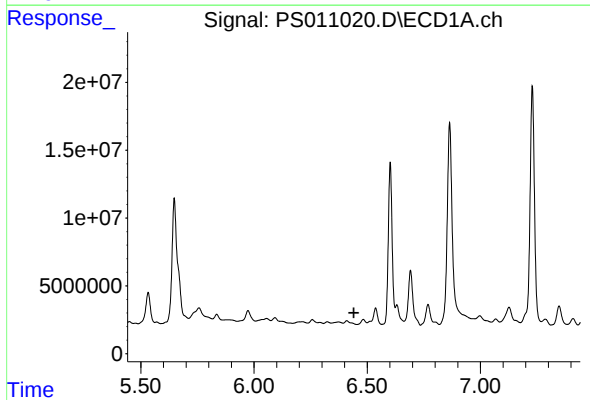


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.441 min
Response: 0
Conc: N.D.

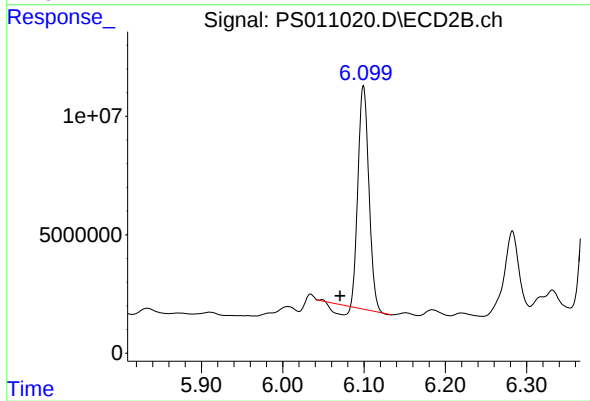

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.099 min
Delta R.T.: 0.029 min
Response: 83214297
Conc: 99.92 ng/ml

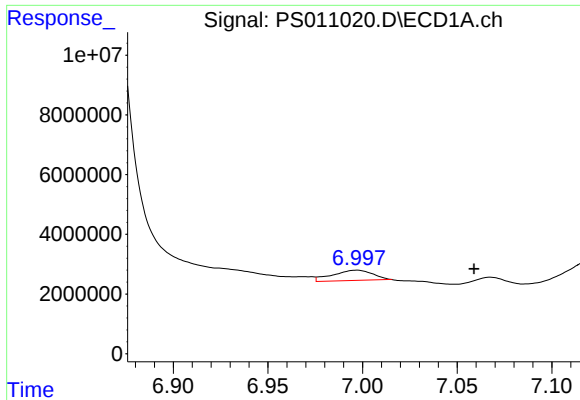

#3 4-Nitrophenol


R.T.: 6.997 min
Delta R.T.: -0.062 min
Response: 5196842
Conc: 13.02 ng/ml

Instrument :
ECD_S
ClientSampleId :

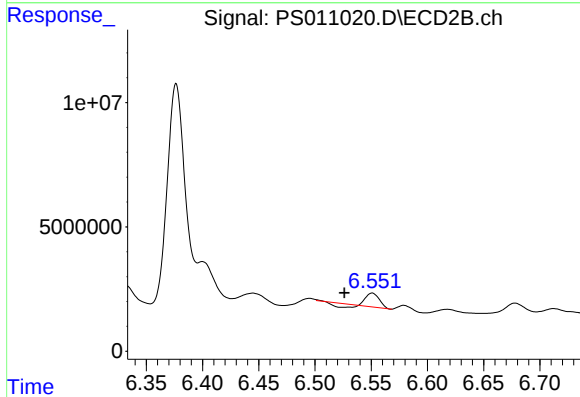


#3 4-Nitrophenol

R.T.: 6.551 min
Delta R.T.: 0.025 min
Response: 3523650
Conc: 10.97 ng/ml

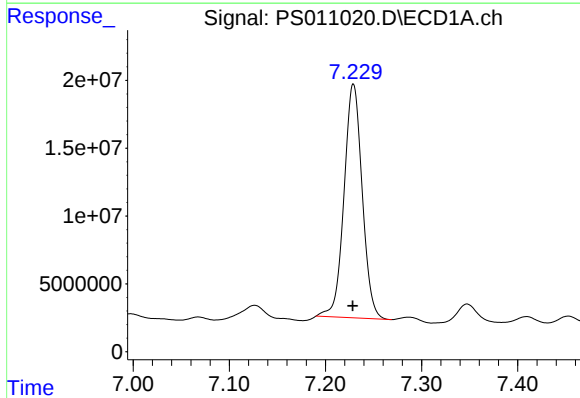


#4 2,4-DCAA

R.T.: 7.229 min
Delta R.T.: 0.000 min
Response: 226652573
Conc: 249.94 ng/ml

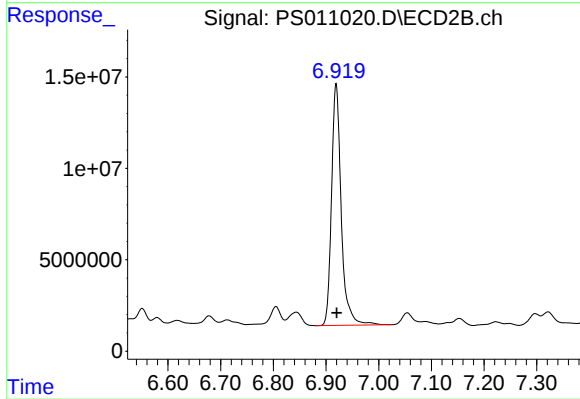

#4 2,4-DCAA


R.T.: 6.919 min
Delta R.T.: -0.001 min
Response: 168927658
Conc: 304.88 ng/ml

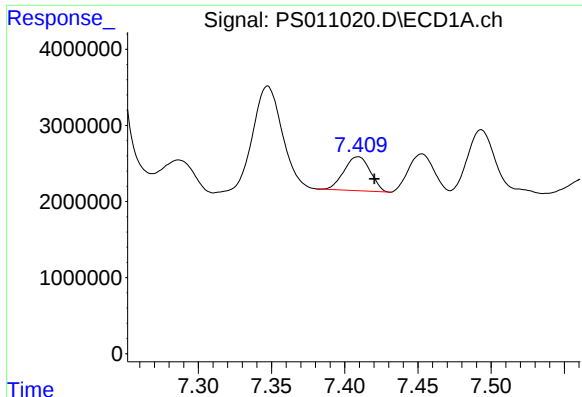

#5 DICAMBA


R.T.: 7.409 min
Delta R.T.: -0.011 min
Response: 5525295
Conc: 1.52 ng/ml

Instrument :
ECD_S
ClientSampleId :

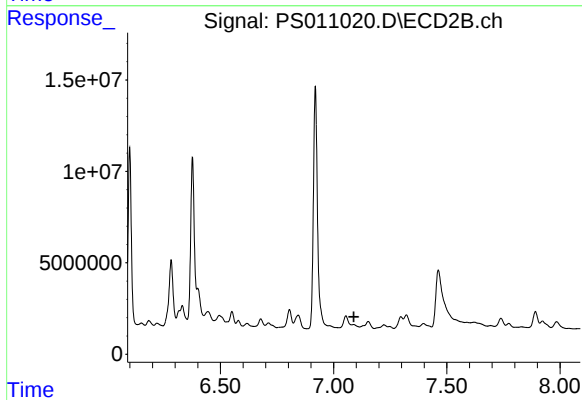


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.089 min
Response: 0
Conc: N.D.

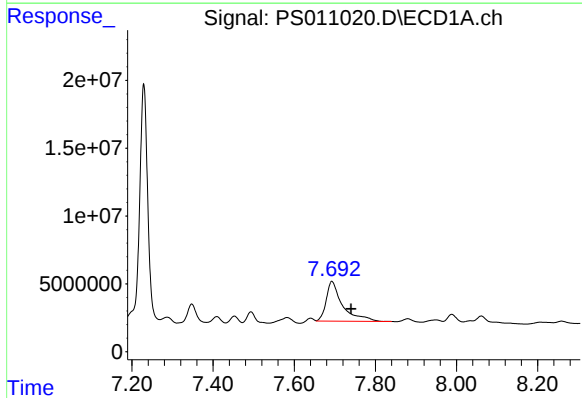


#7 MCPA

R.T.: 7.693 min
Delta R.T.: -0.047 min
Response: 81733238
Conc: 20.52 ug/ml

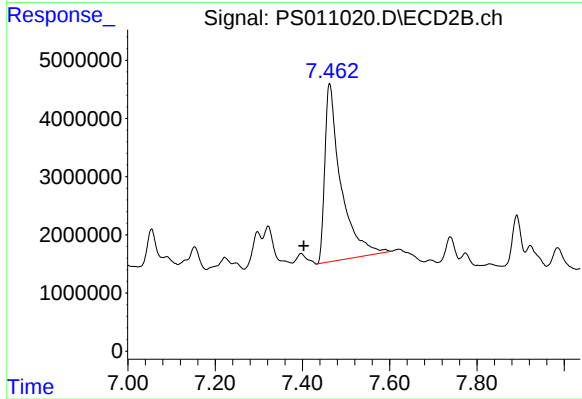

#7 MCPA


R.T.: 7.463 min
Delta R.T.: 0.060 min
Response: 78229241
Conc: 28.34 ug/ml

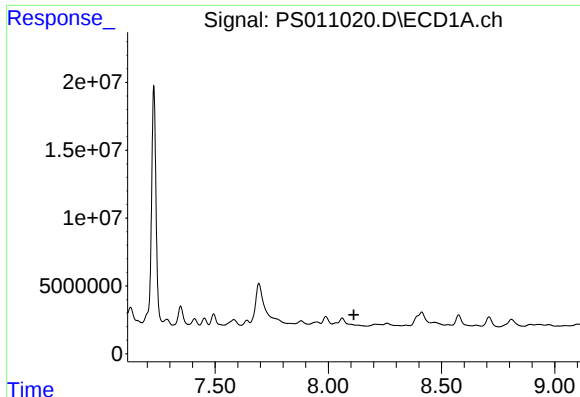

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.113 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

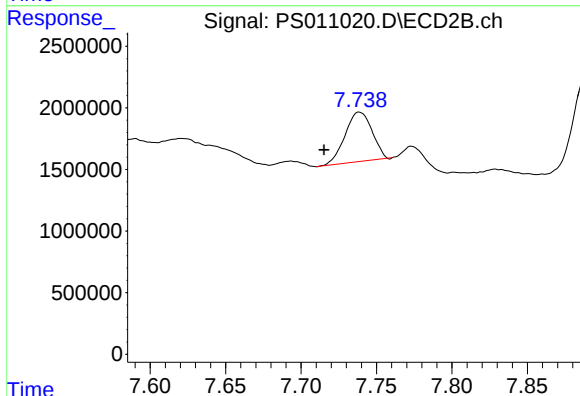


#8 DICHLORPROP

R.T.: 7.739 min
Delta R.T.: 0.024 min
Response: 4958114
Conc: 8.44 ng/ml

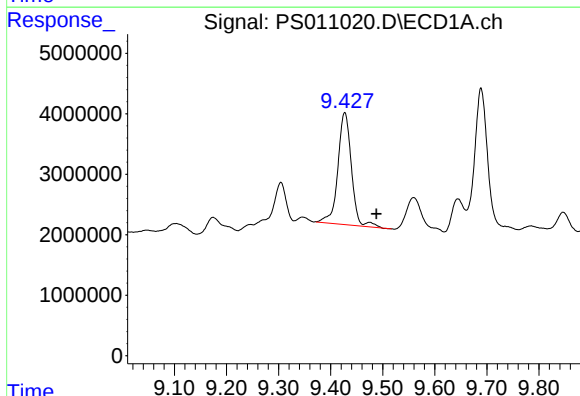


#12 2,4,5-T

R.T.: 9.427 min
Delta R.T.: -0.061 min
Response: 33474820
Conc: 7.19 ng/ml

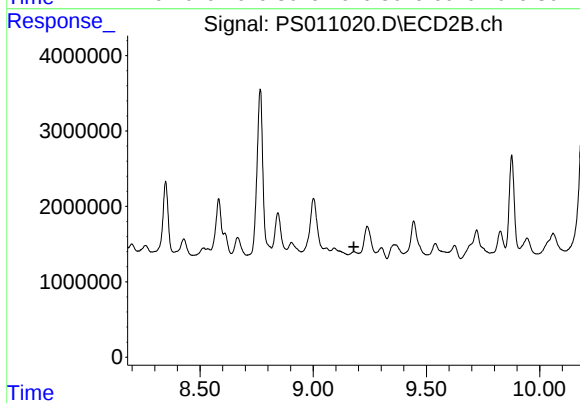

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.179 min
Response: 0
Conc: N.D.

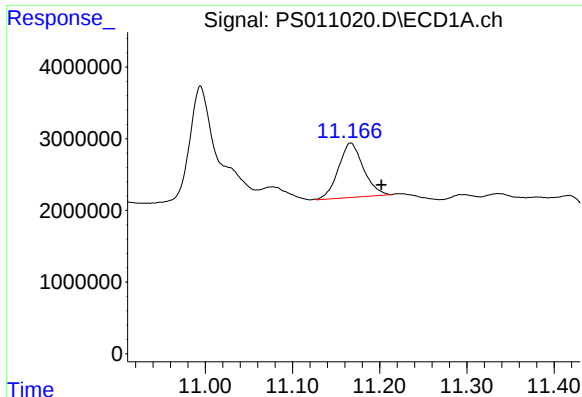

#14 DINOSEB


R.T.: 11.167 min
Delta R.T.: -0.035 min
Response: 15149917
Conc: 4.23 ng/ml

Instrument :
ECD_S
ClientSampleId :

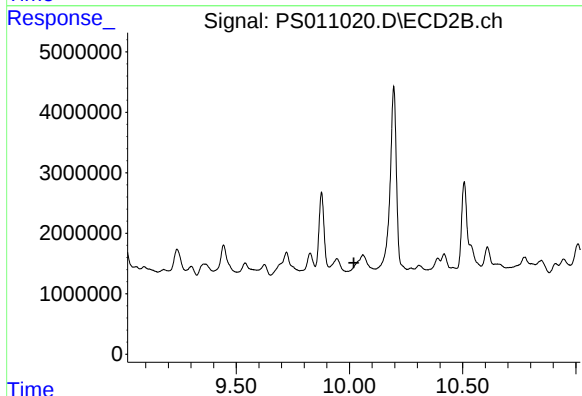


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 10.020 min
Response: 0
Conc: N.D.

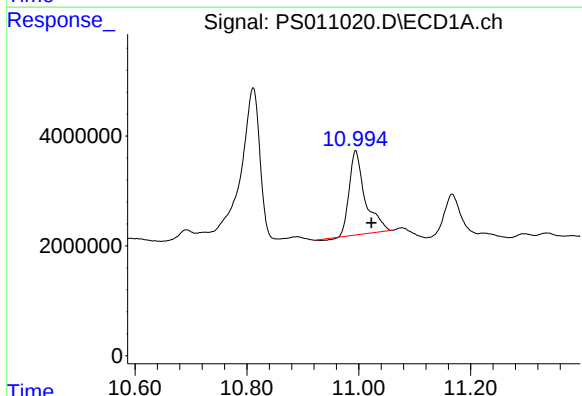

#15 Picloram

R.T.: 10.994 min
Delta R.T.: -0.028 min
Response: 30042862
Conc: 5.36 ng/ml

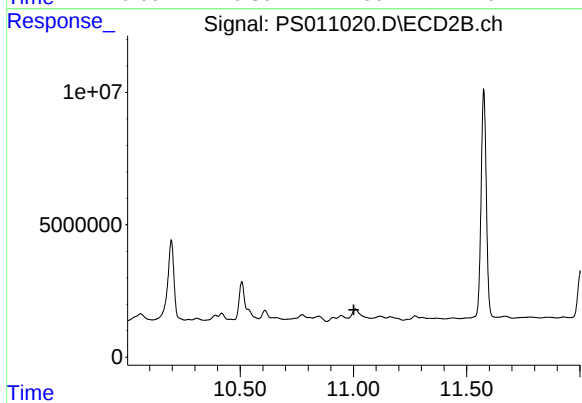

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 11.002 min
Response: 0
Conc: N.D.