

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070120\
 Data File : PS011026.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Jul 2020 14:59
 Operator : DD\AJ
 Sample : L3153-08
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 01 15:51:23 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062420.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 25 02:45:12 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.230	6.921	245.4E6	176.3E6	270.654	318.128
Target Compounds							
1) T	Dalapon	2.996	2.585	42773180	104.3E6	38.200	138.255 #
2) T	3,5-DICHL...	0.000	6.101	0	72324936	N.D.	86.843
3) T	4-Nitroph...	6.998	0.000	5223980	0	13.087	N.D. #
5) T	DICAMBA	0.000	7.056	0	7391704	N.D.	3.254
7) T	MCPA	7.693	7.463	119.8E6	96332939	30.091	34.903
10) T	Pentachlo...	8.710	0.000	9834315	0	<MDL	N.D. #
12) T	2,4,5-T	9.428	0.000	28860469	0	6.196	N.D. #
14) T	DINOSEB	11.170	0.000	16389485	0	4.576	N.D. #
15) T	Picloram	10.996	0.000	30888569	0	5.510	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070120\
Data File : PS011026.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Jul 2020 14:59
Operator : DD\AJ
Sample : L3153-08
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 01 15:51:23 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062420.M
Quant Title : 8080.M
QLast Update : Thu Jun 25 02:45:12 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

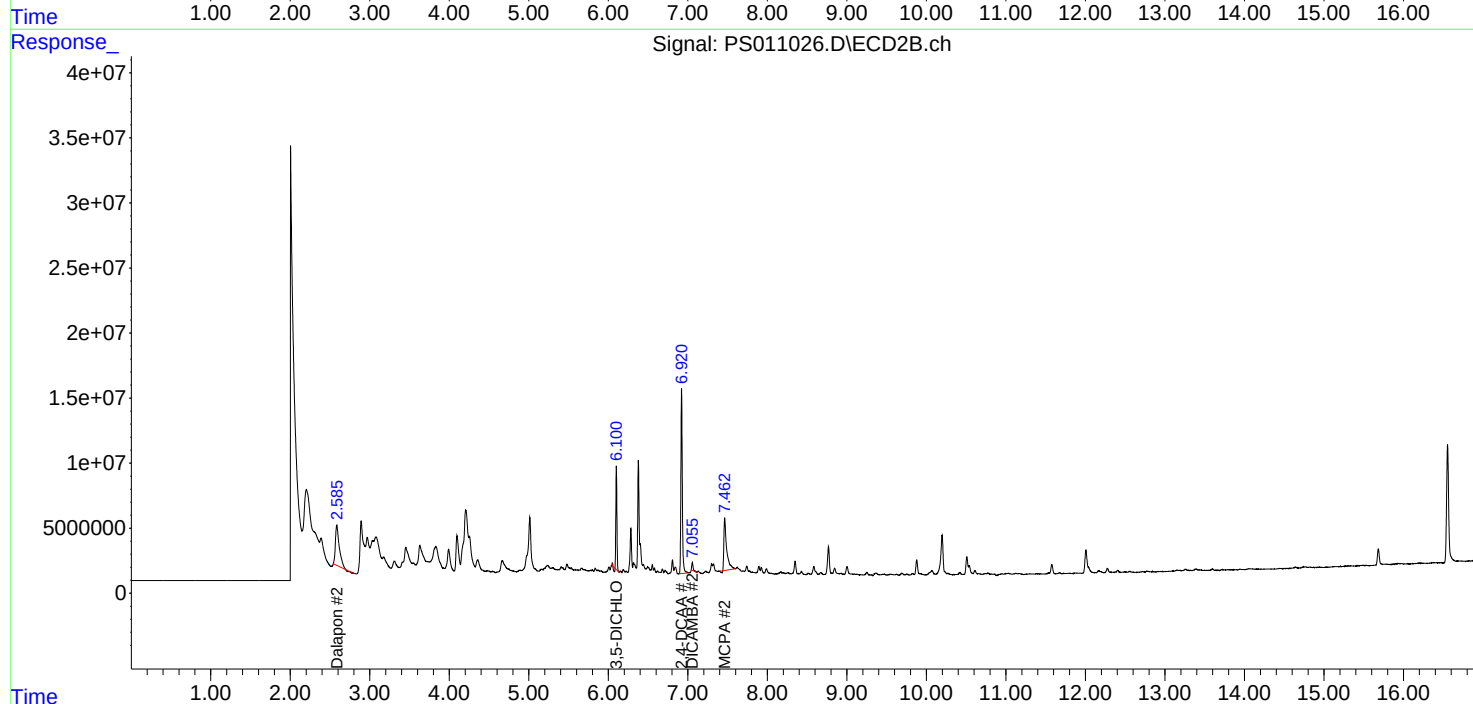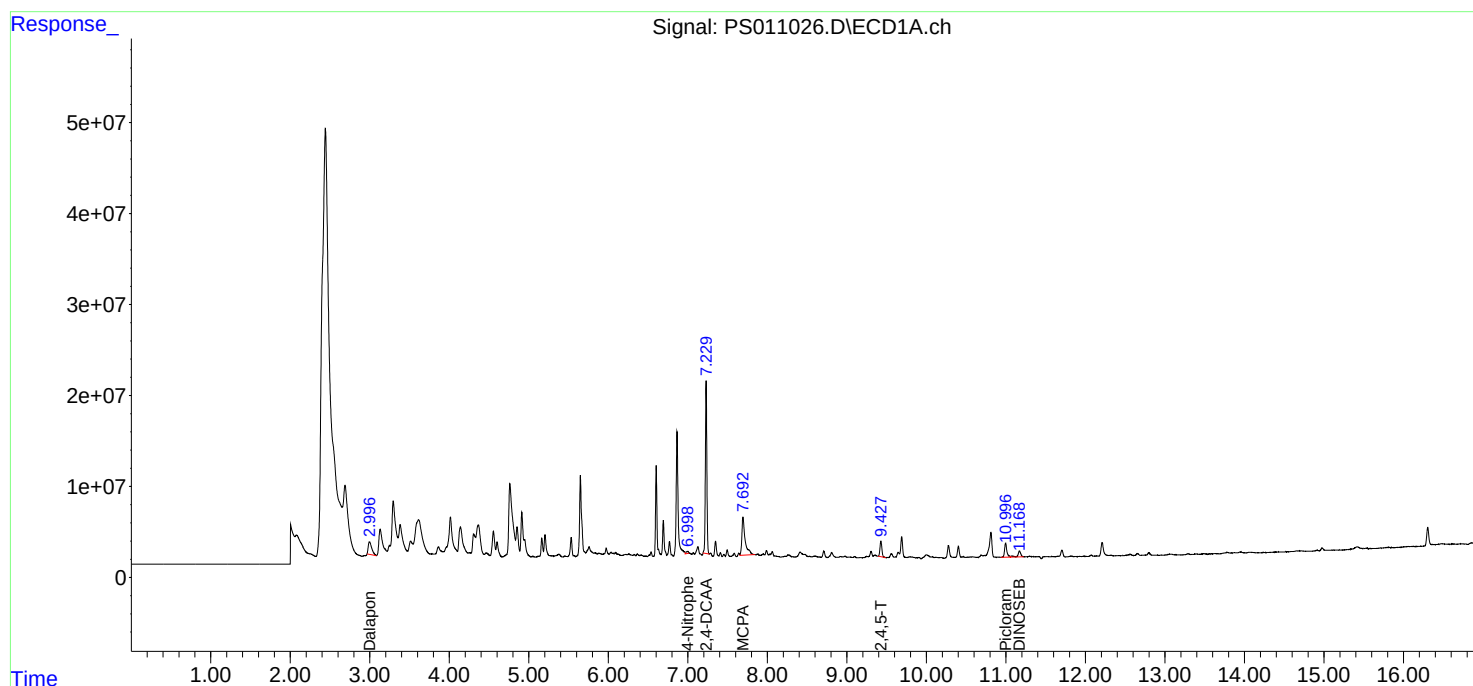


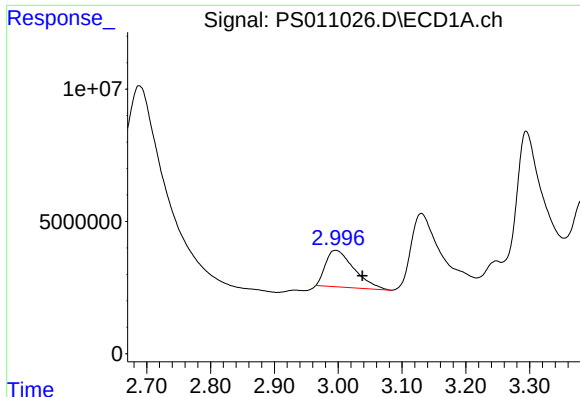

#1 Dalapon


R.T.: 2.996 min
Delta R.T.: -0.042 min
Response: 42773180
Conc: 38.20 ng/ml

Instrument :
ECD_S
ClientSampleId :

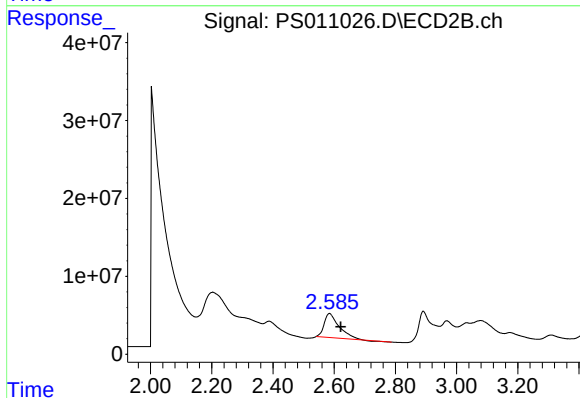


#1 Dalapon

R.T.: 2.585 min
Delta R.T.: -0.037 min
Response: 104294406
Conc: 138.26 ng/ml

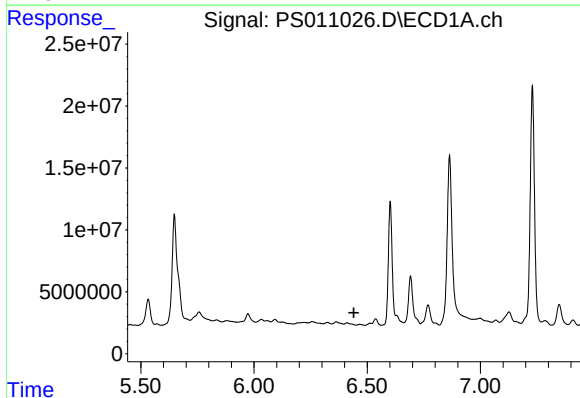


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.441 min
Response: 0
Conc: N.D.

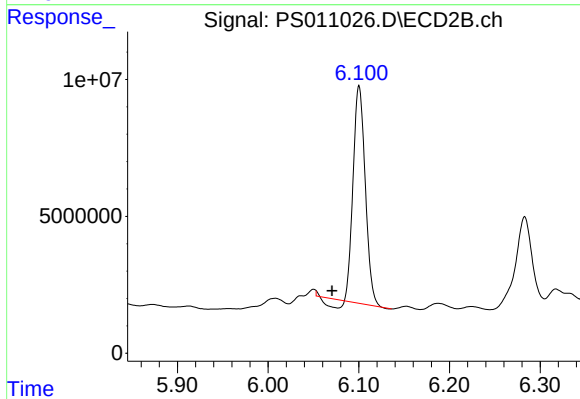

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.101 min
Delta R.T.: 0.030 min
Response: 72324936
Conc: 86.84 ng/ml

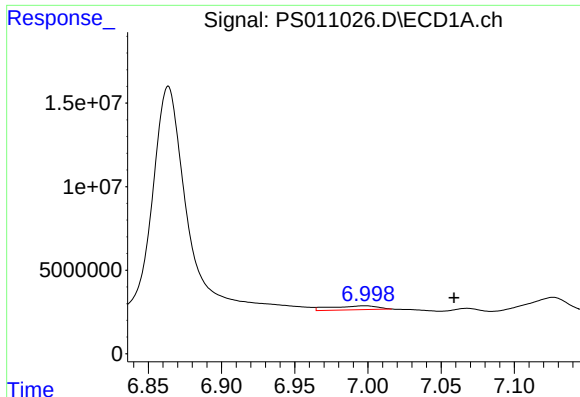

#3 4-Nitrophenol


R.T.: 6.998 min
Delta R.T.: -0.061 min
Response: 5223980
Conc: 13.09 ng/ml

Instrument :
ECD_S
ClientSampleId :

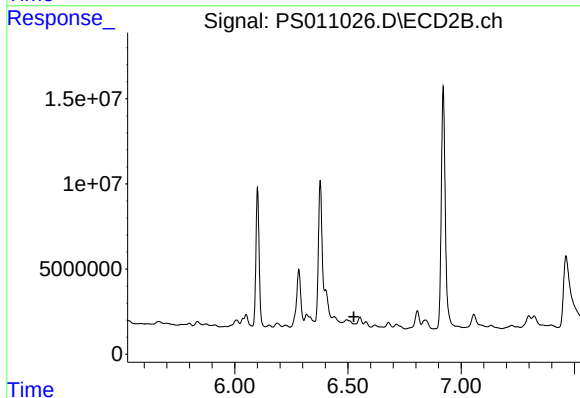


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.526 min
Response: 0
Conc: N.D.

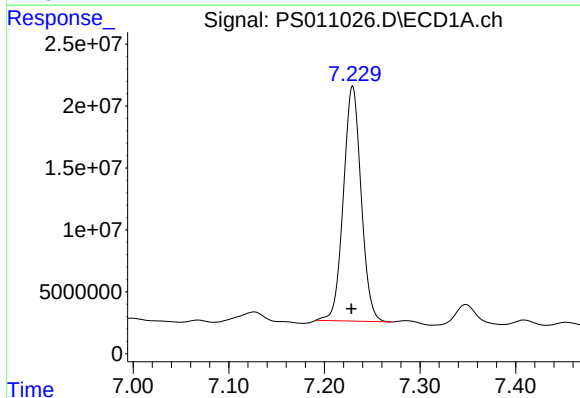


#4 2,4-DCAA

R.T.: 7.230 min
Delta R.T.: 0.001 min
Response: 245434407
Conc: 270.65 ng/ml

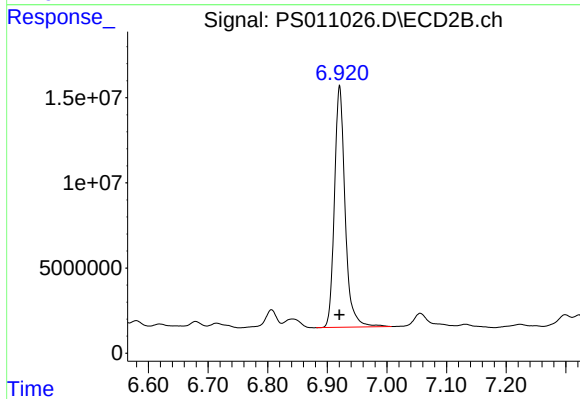

#4 2,4-DCAA


R.T.: 6.921 min
Delta R.T.: 0.000 min
Response: 176266924
Conc: 318.13 ng/ml

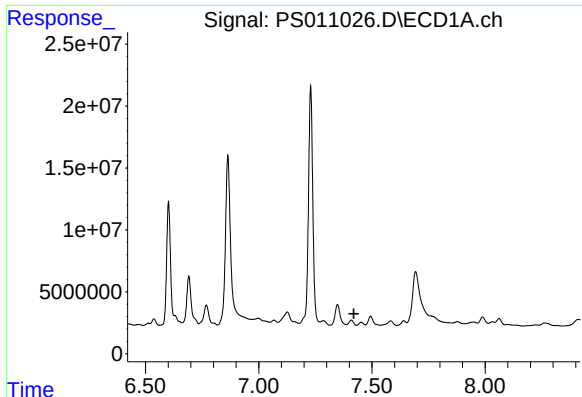

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 7.420 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

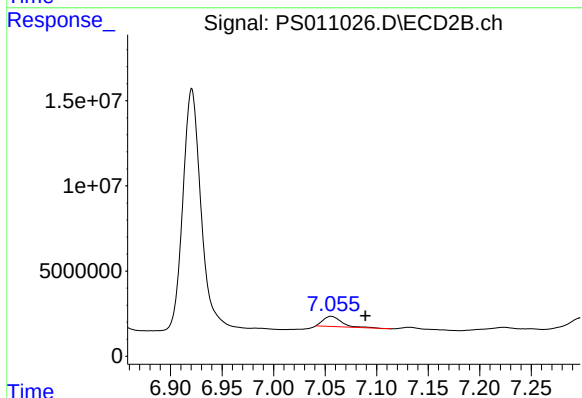


#5 DICAMBA

R.T.: 7.056 min
Delta R.T.: -0.033 min
Response: 7391704
Conc: 3.25 ng/ml

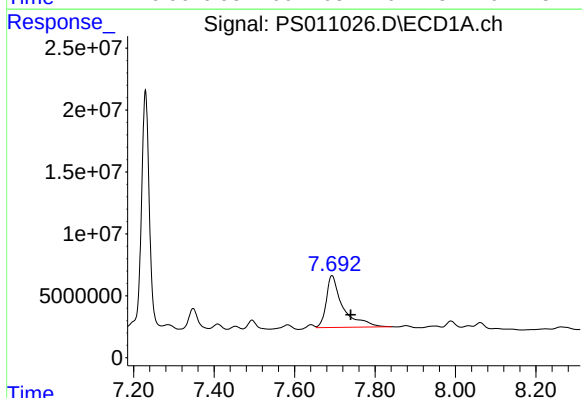


#7 MCPA

R.T.: 7.693 min
Delta R.T.: -0.047 min
Response: 119834457
Conc: 30.09 ug/ml

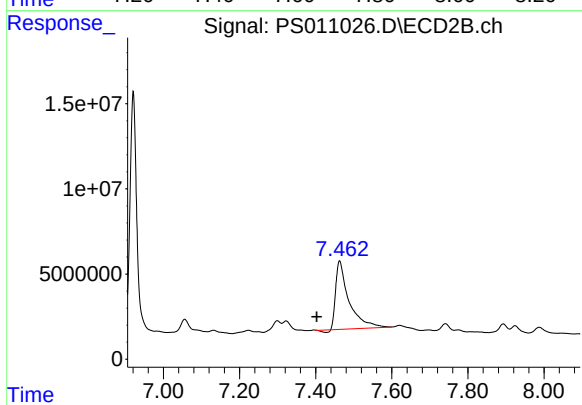

#7 MCPA


R.T.: 7.463 min
Delta R.T.: 0.060 min
Response: 96332939
Conc: 34.90 ug/ml

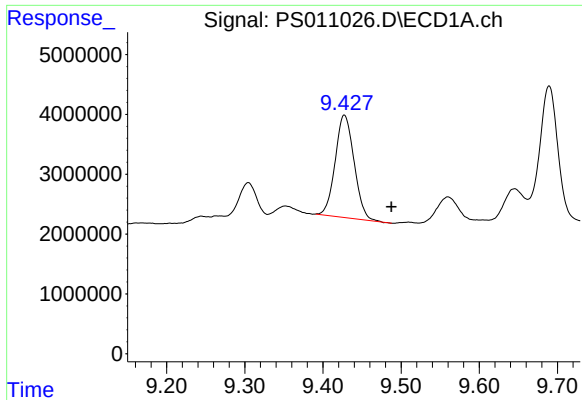

#12 2,4,5-T


R.T.: 9.428 min
Delta R.T.: -0.060 min
Response: 28860469
Conc: 6.20 ng/ml

Instrument :
ECD_S
ClientSampleId :

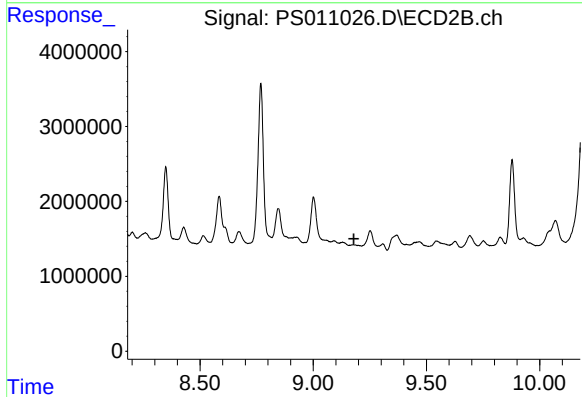


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.179 min
Response: 0
Conc: N.D.

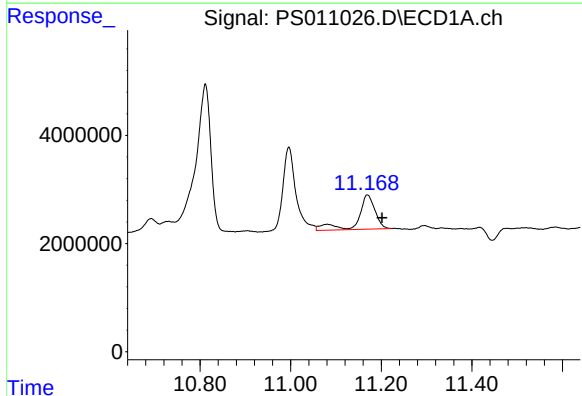


#14 DINOSEB

R.T.: 11.170 min
Delta R.T.: -0.033 min
Response: 16389485
Conc: 4.58 ng/ml

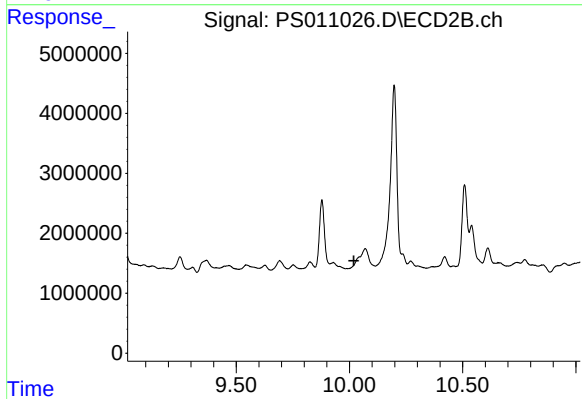

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 10.020 min
Response: 0
Conc: N.D.

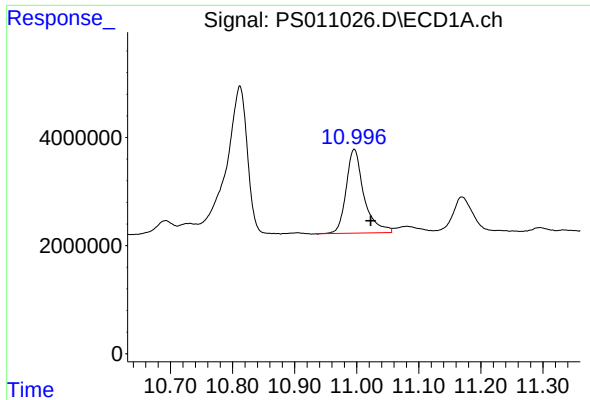

#15 Picloram

R.T.: 10.996 min
Delta R.T.: -0.027 min
Response: 30888569
Conc: 5.51 ng/ml

Instrument :
ECD_S
ClientSampleId :

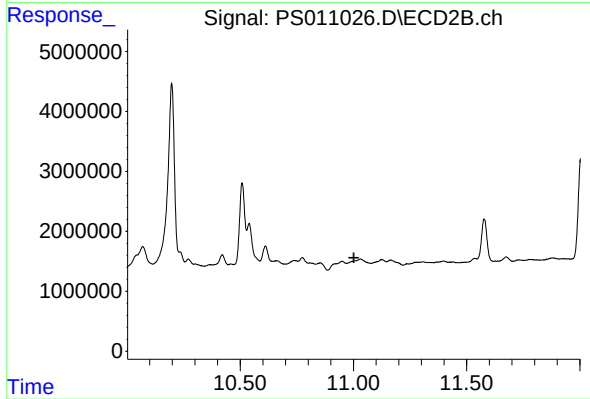

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 11.002 min
Response: 0
Conc: N.D.