

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070120\
 Data File : PS011033.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Jul 2020 17:40
 Operator : DD\AJ
 Sample : L3153-23
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 02 05:03:33 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062420.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 25 02:45:12 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.229	6.920	247.7E6	179.4E6	273.139	323.742
Target Compounds							
1) T	Dalapon	2.994	2.586	40178378	134.2E6	35.882	177.873 #
2) T	3,5-DICHL...	0.000	6.101	0	67084178	N.D.	80.550
3) T	4-Nitroph...	6.996	0.000	7690934	0	19.267	N.D. #
5) T	DICAMBA	0.000	7.055	0	5975721	N.D.	2.631
7) T	MCPA	7.690	7.459	160.6E6	151.6E6	40.336	54.944 #
8) T	DICHLORPROP	0.000	7.740	0	8371543	N.D.	14.258
10) T	Pentachlo...	8.709	0.000	11528258	0	<MDL	N.D. #
12) T	2,4,5-T	9.427	0.000	29012821	0	6.229	N.D. #
14) T	DINOSEB	11.169	10.066	11431736	15602721	3.192	7.494 #
15) T	Picloram	10.995	0.000	32094526	0	5.725	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070120\
Data File : PS011033.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Jul 2020 17:40
Operator : DD\AJ
Sample : L3153-23
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 02 05:03:33 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062420.M
Quant Title : 8080.M
QLast Update : Thu Jun 25 02:45:12 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

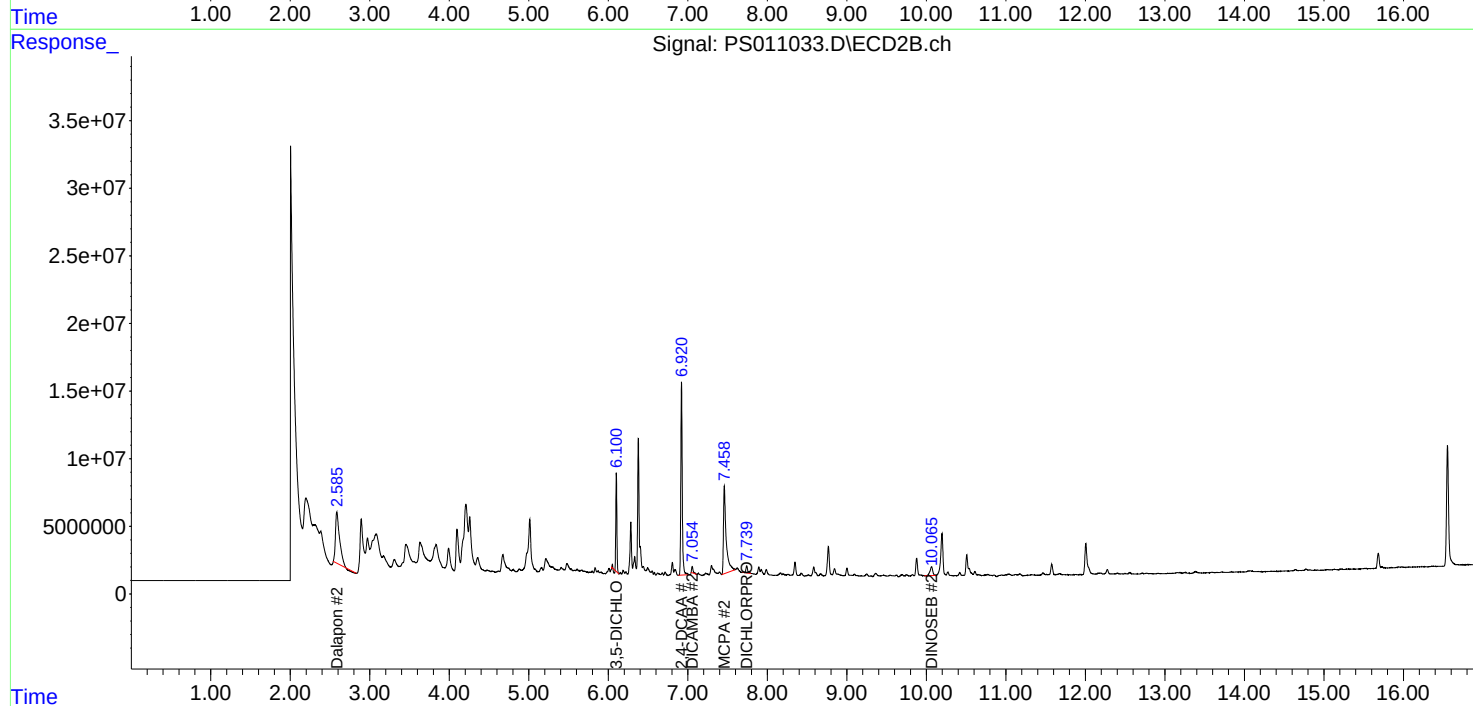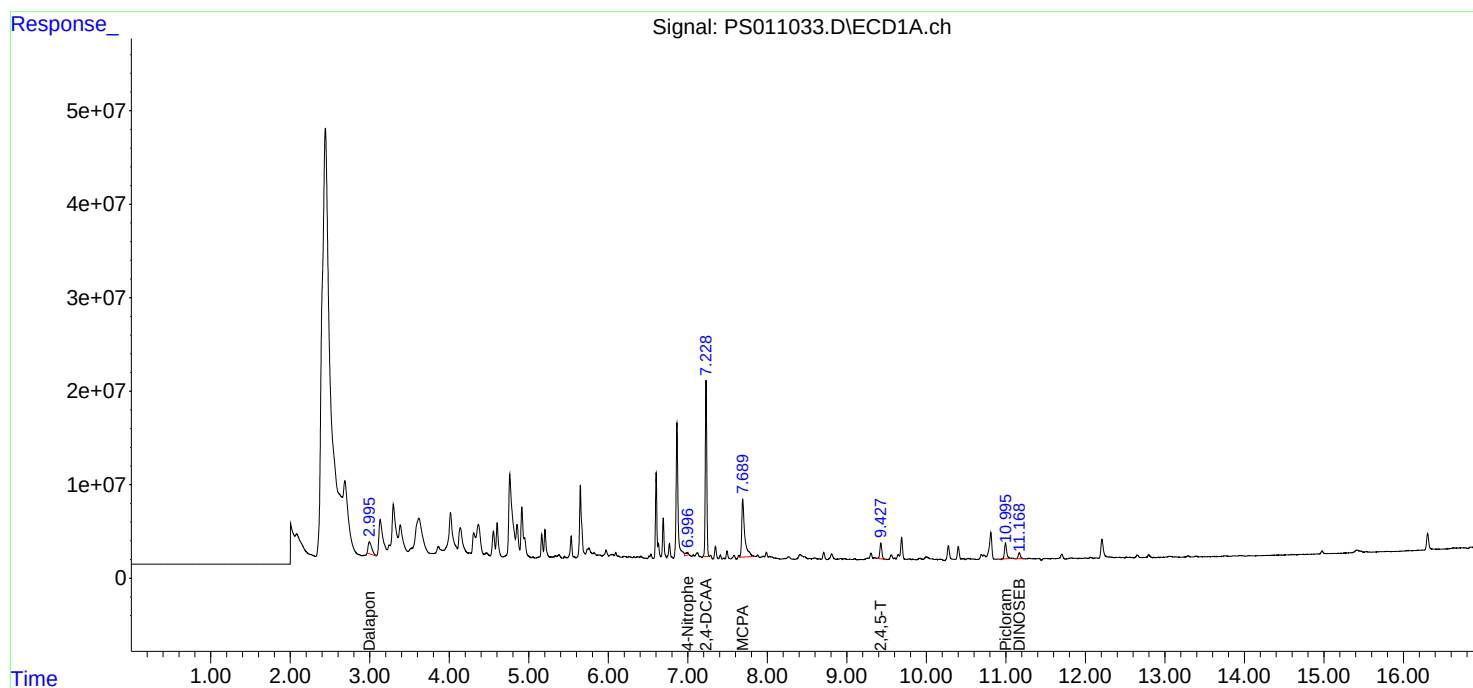


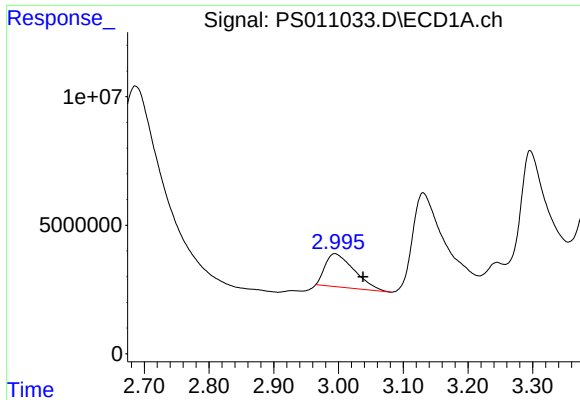

#1 Dalapon


R.T.: 2.994 min
Delta R.T.: -0.044 min
Response: 40178378
Conc: 35.88 ng/ml

Instrument :
ECD_S
ClientSampleId :

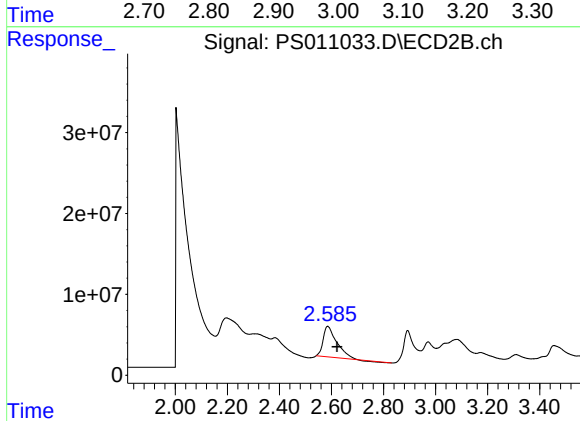


#1 Dalapon

R.T.: 2.586 min
Delta R.T.: -0.036 min
Response: 134180539
Conc: 177.87 ng/ml

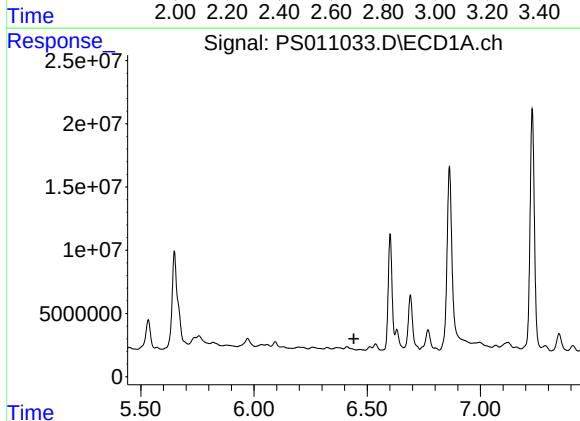


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.441 min
Response: 0
Conc: N.D.

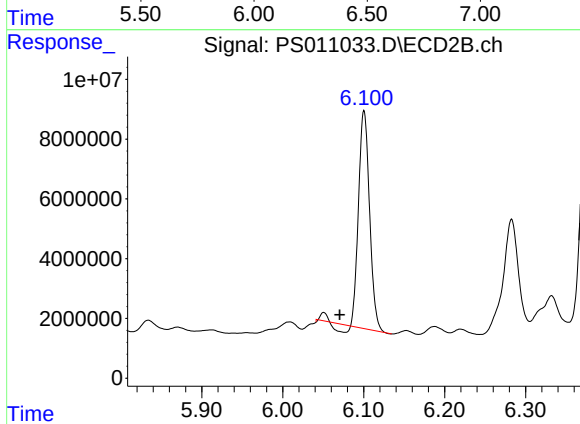

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.101 min
Delta R.T.: 0.030 min
Response: 67084178
Conc: 80.55 ng/ml

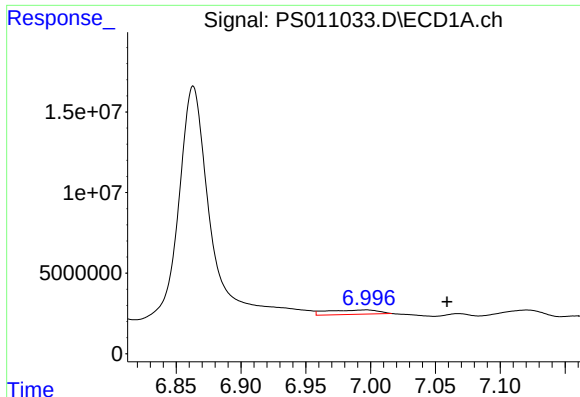

#3 4-Nitrophenol


R.T.: 6.996 min
Delta R.T.: -0.063 min
Response: 7690934
Conc: 19.27 ng/ml

Instrument :
ECD_S
ClientSampleId :

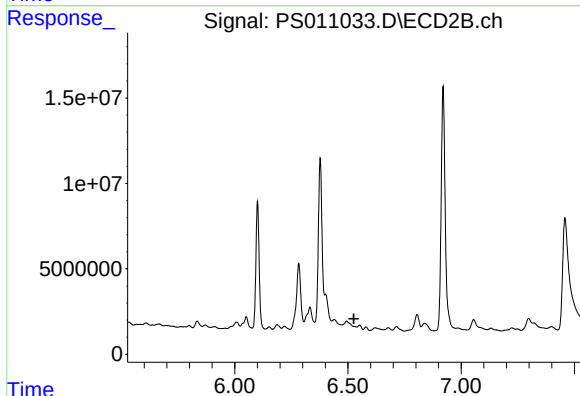


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.526 min
Response: 0
Conc: N.D.

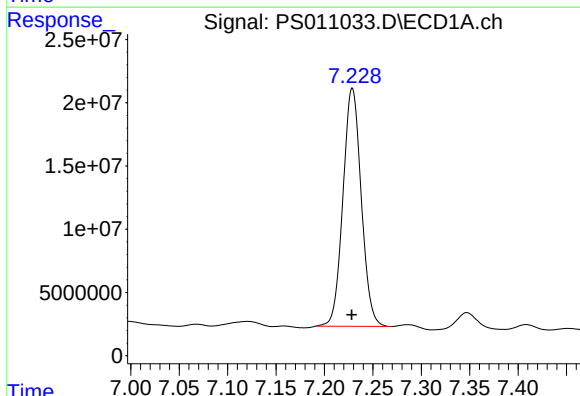


#4 2,4-DCAA

R.T.: 7.229 min
Delta R.T.: 0.000 min
Response: 247687511
Conc: 273.14 ng/ml

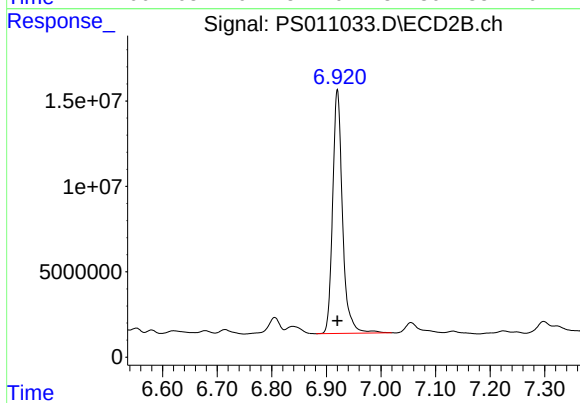

#4 2,4-DCAA


R.T.: 6.920 min
Delta R.T.: 0.000 min
Response: 179377502
Conc: 323.74 ng/ml

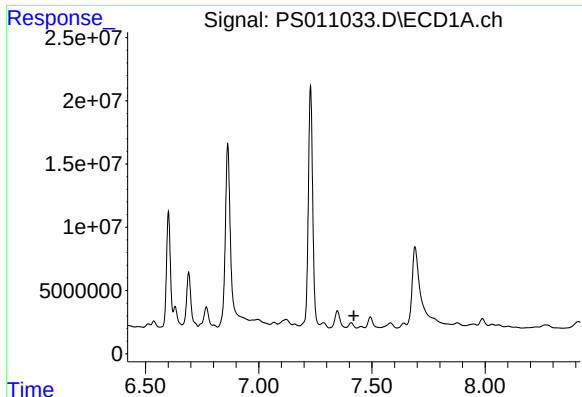

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 7.420 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

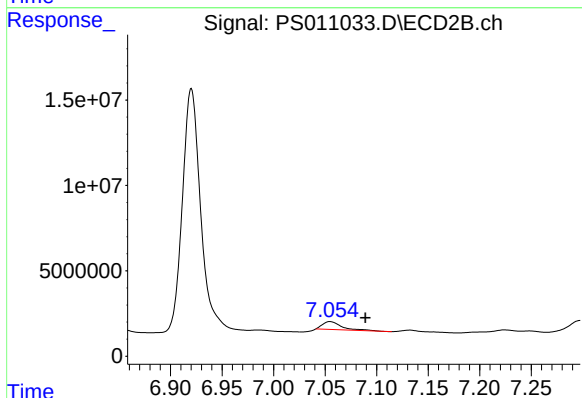


#5 DICAMBA

R.T.: 7.055 min
Delta R.T.: -0.034 min
Response: 5975721
Conc: 2.63 ng/ml

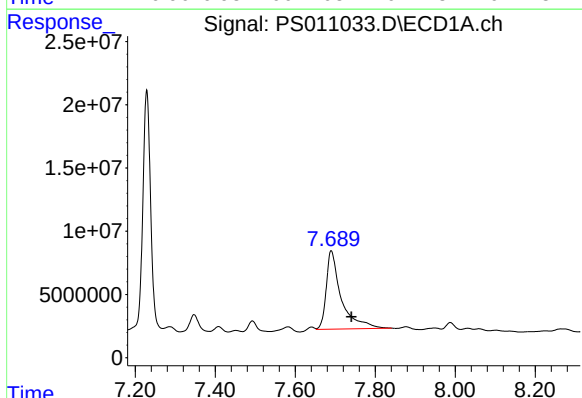


#7 MCPA

R.T.: 7.690 min
Delta R.T.: -0.050 min
Response: 160636517
Conc: 40.34 ug/ml

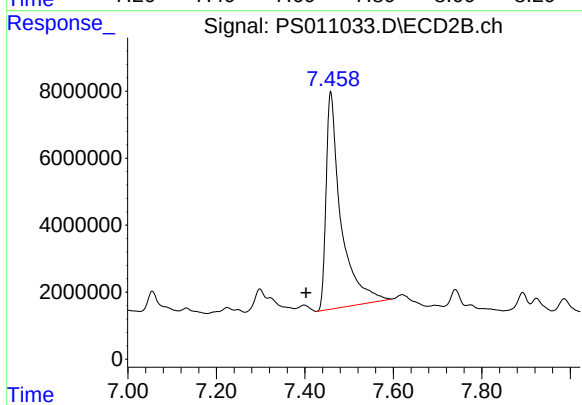

#7 MCPA


R.T.: 7.459 min
Delta R.T.: 0.056 min
Response: 151645093
Conc: 54.94 ug/ml

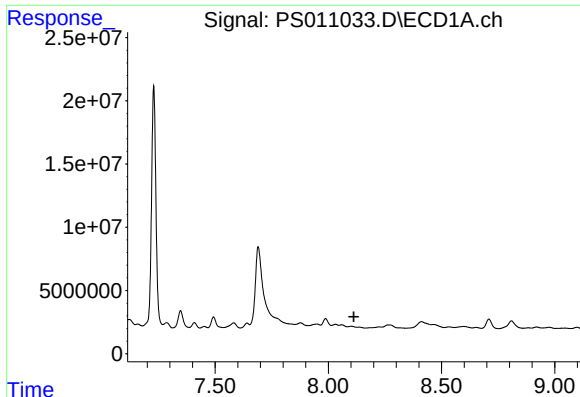

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.113 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

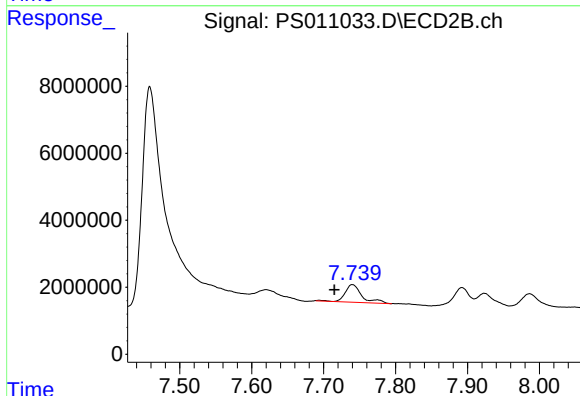


#8 DICHLORPROP

R.T.: 7.740 min
Delta R.T.: 0.025 min
Response: 8371543
Conc: 14.26 ng/ml

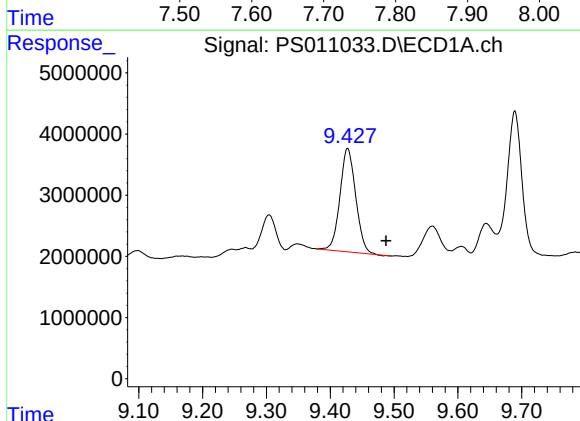


#12 2,4,5-T

R.T.: 9.427 min
Delta R.T.: -0.060 min
Response: 29012821
Conc: 6.23 ng/ml

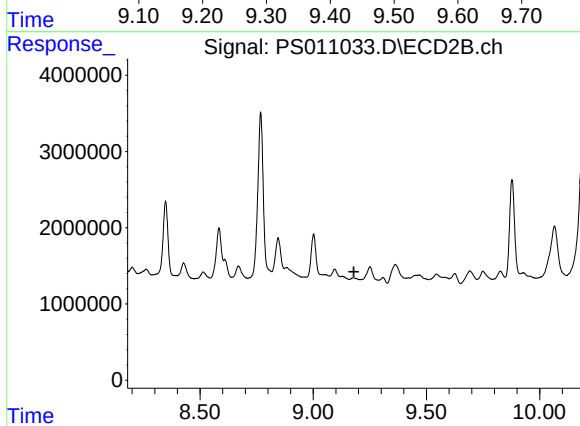

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.179 min
Response: 0
Conc: N.D.

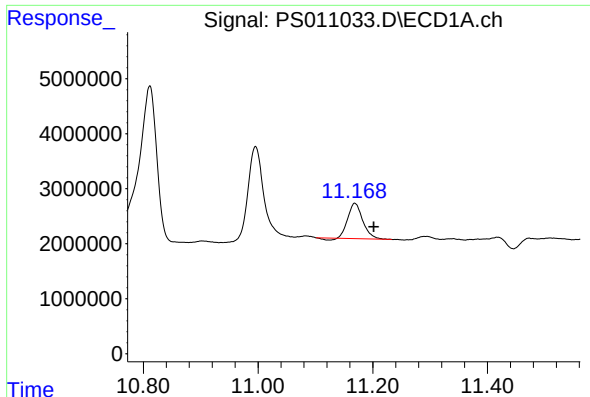

#14 DINOSEB


R.T.: 11.169 min
Delta R.T.: -0.033 min
Response: 11431736
Conc: 3.19 ng/ml

Instrument :
ECD_S
ClientSampleId :

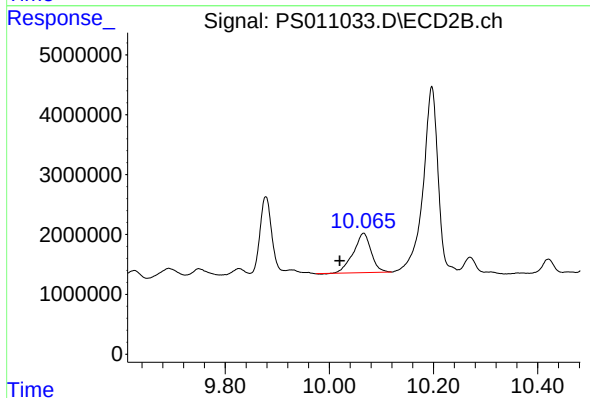


#14 DINOSEB

R.T.: 10.066 min
Delta R.T.: 0.046 min
Response: 15602721
Conc: 7.49 ng/ml

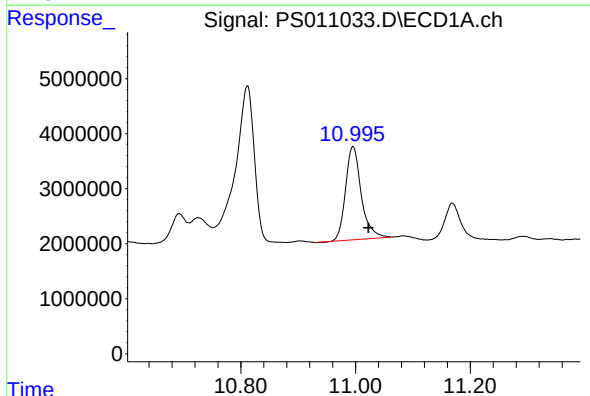

#15 Picloram

R.T.: 10.995 min
Delta R.T.: -0.027 min
Response: 32094526
Conc: 5.72 ng/ml

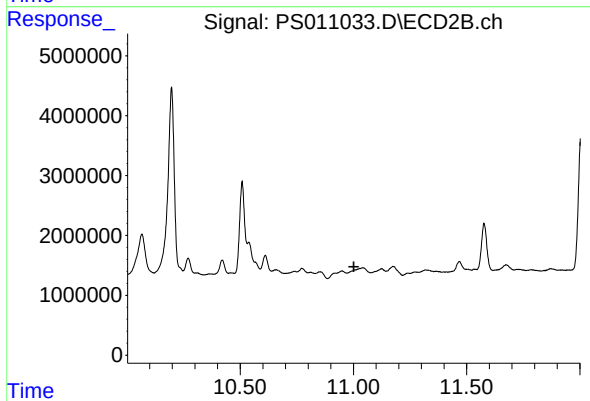

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 11.002 min
Response: 0
Conc: N.D.