

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070120\
 Data File : PS011034.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Jul 2020 18:03
 Operator : DD\AJ
 Sample : L3153-26
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 02 05:03:50 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062420.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 25 02:45:12 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.229	6.920	245.3E6	176.7E6	270.534	318.949
Target Compounds							
1) T	Dalapon	2.995	2.586	42514248	136.6E6	37.969	181.094 #
2) T	3,5-DICHL...	0.000	6.100	0	75223566	N.D.	90.323
3) T	4-Nitroph...	6.998	0.000	5583125	0	13.987	N.D. #
5) T	DICAMBA	7.409	0.000	5479992	0	1.503	N.D. #
7) T	MCPA	7.693	7.462	116.4E6	108.1E6	29.231	39.177 #
10) T	Pentachlo...	8.710	0.000	9786414	0	<MDL	N.D. #
12) T	2,4,5-T	9.427	0.000	34452081	0	7.396	N.D. #
14) T	DINOSEB	11.169	10.065	10829960	13888268	3.024	6.670 #
15) T	Picloram	10.996	0.000	28895232	0	5.154	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070120\
Data File : PS011034.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Jul 2020 18:03
Operator : DD\AJ
Sample : L3153-26
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 02 05:03:50 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062420.M
Quant Title : 8080.M
QLast Update : Thu Jun 25 02:45:12 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

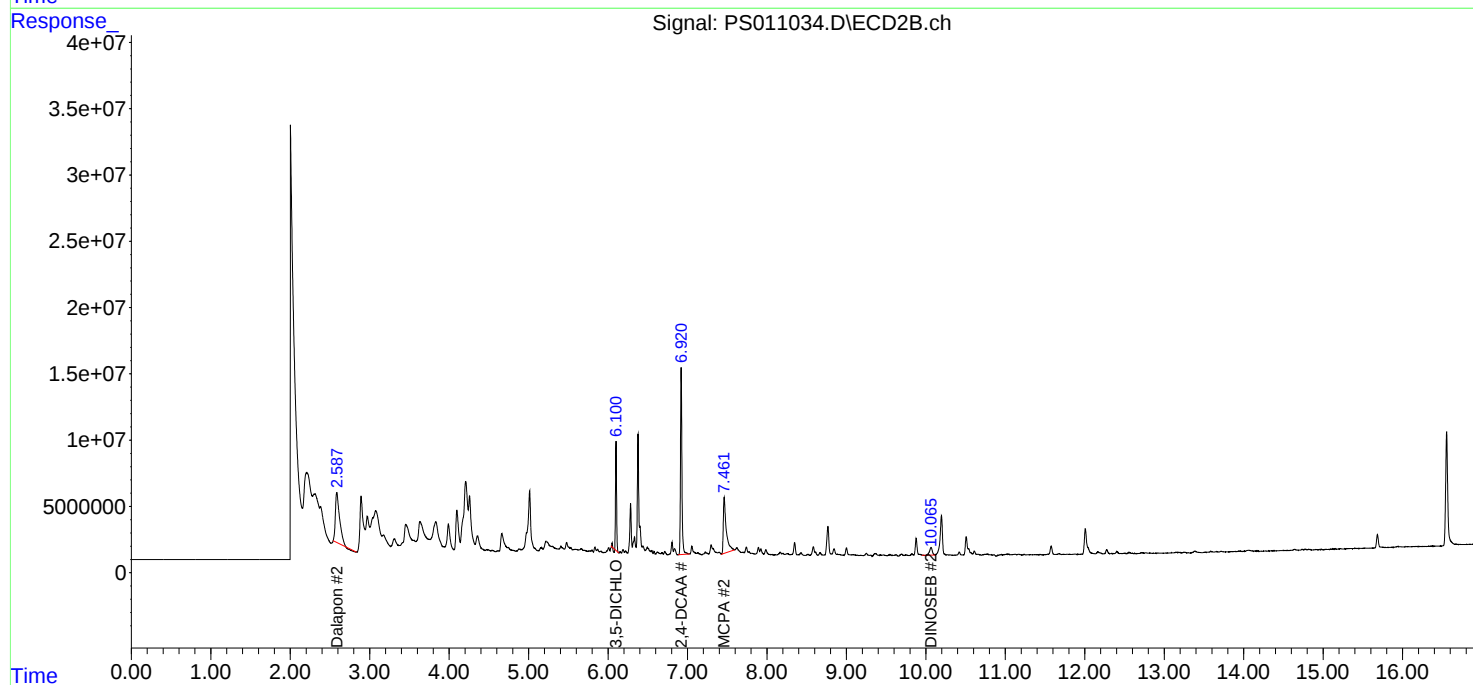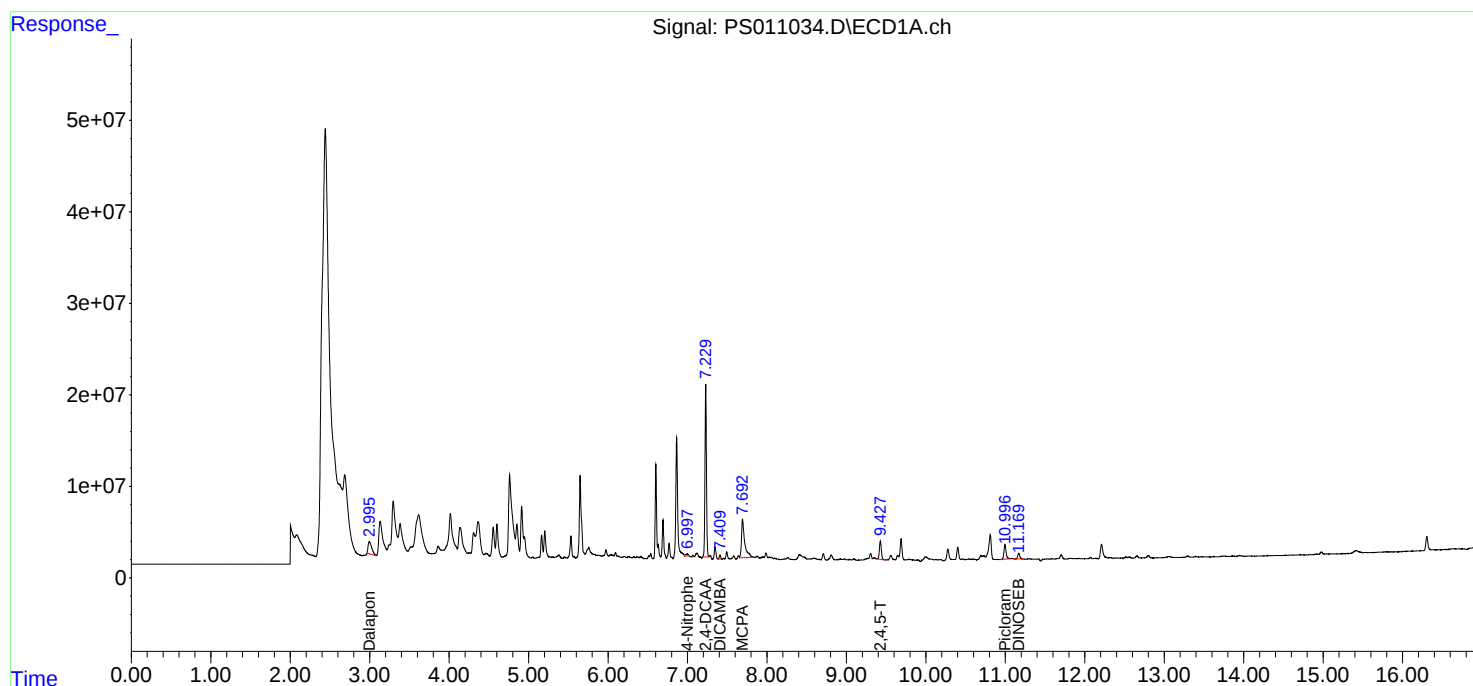


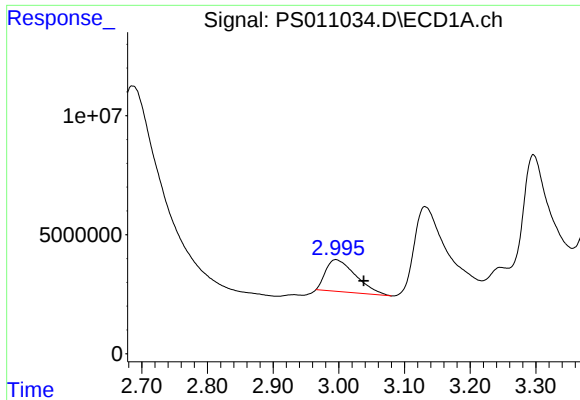

#1 Dalapon


R.T.: 2.995 min
Delta R.T.: -0.043 min
Response: 42514248
Conc: 37.97 ng/ml

Instrument :
ECD_S
ClientSampleId :

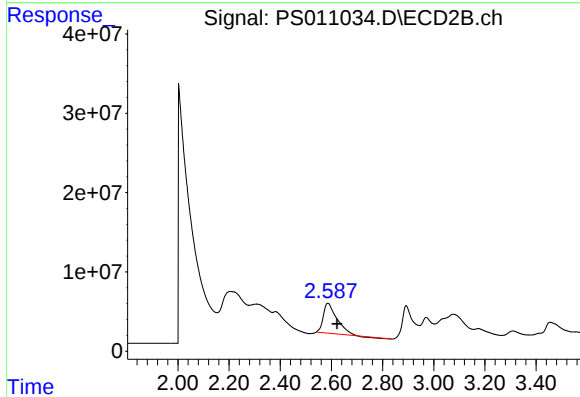


#1 Dalapon

R.T.: 2.586 min
Delta R.T.: -0.036 min
Response: 136610122
Conc: 181.09 ng/ml

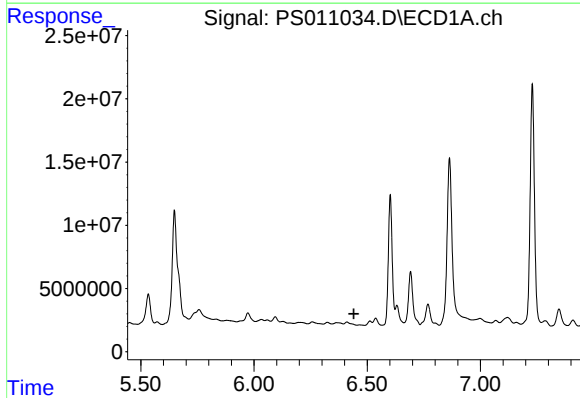


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.441 min
Response: 0
Conc: N.D.

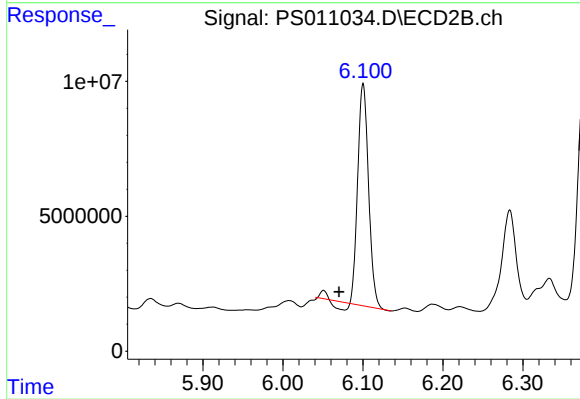

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.100 min
Delta R.T.: 0.030 min
Response: 75223566
Conc: 90.32 ng/ml

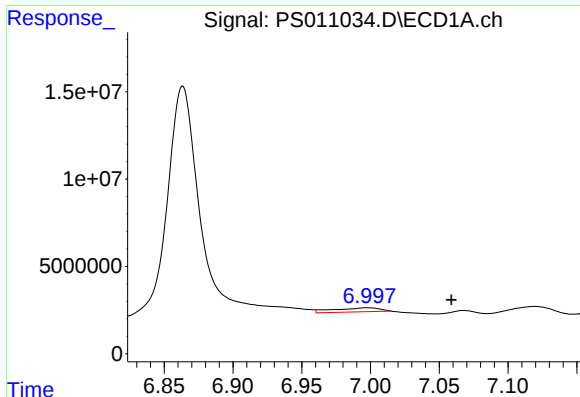

#3 4-Nitrophenol


R.T.: 6.998 min
Delta R.T.: -0.061 min
Response: 5583125
Conc: 13.99 ng/ml

Instrument :
ECD_S
ClientSampleId :

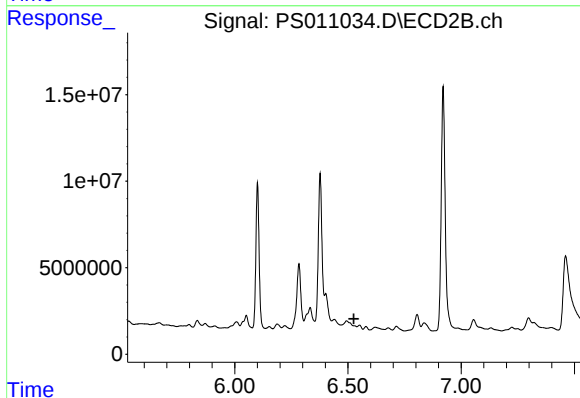


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.526 min
Response: 0
Conc: N.D.

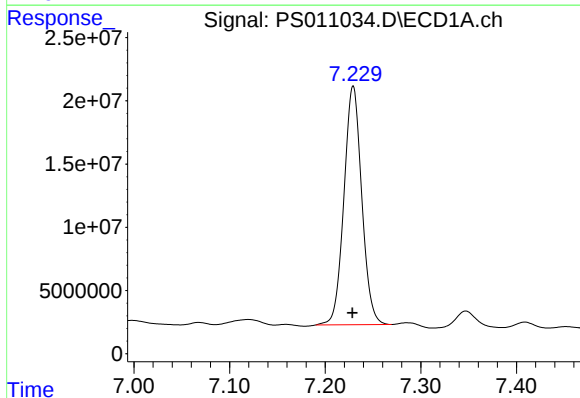


#4 2,4-DCAA

R.T.: 7.229 min
Delta R.T.: 0.000 min
Response: 245325424
Conc: 270.53 ng/ml

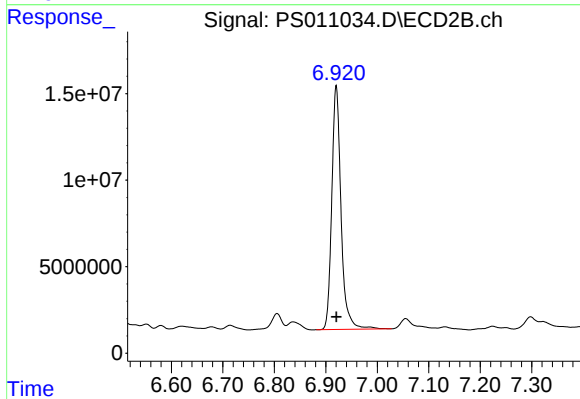

#4 2,4-DCAA


R.T.: 6.920 min
Delta R.T.: 0.000 min
Response: 176722133
Conc: 318.95 ng/ml

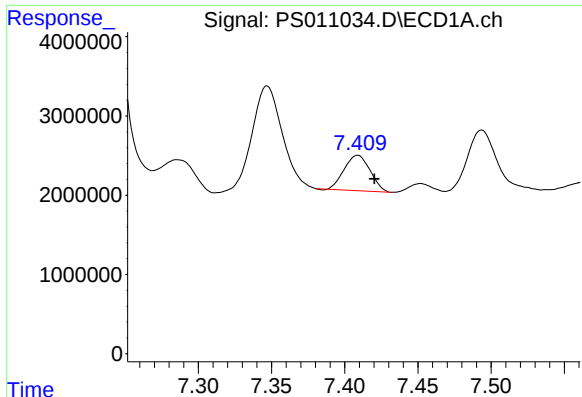

#5 DICAMBA


R.T.: 7.409 min
Delta R.T.: -0.011 min
Response: 5479992
Conc: 1.50 ng/ml

Instrument :
ECD_S
ClientSampleId :

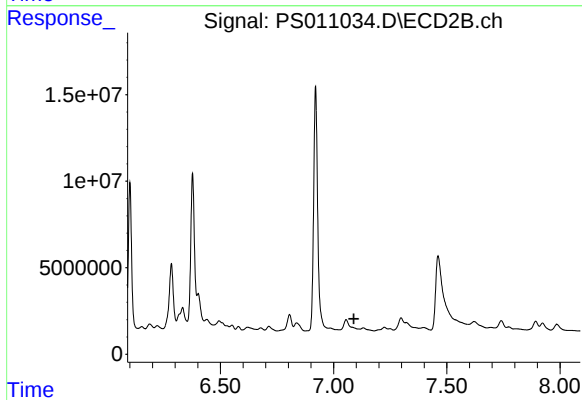


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.089 min
Response: 0
Conc: N.D.

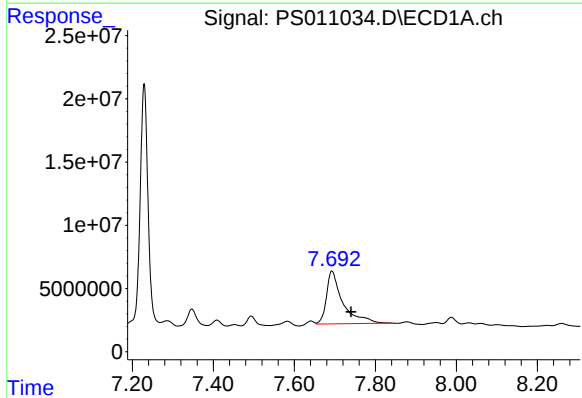


#7 MCPA

R.T.: 7.693 min
Delta R.T.: -0.047 min
Response: 116408942
Conc: 29.23 ug/ml

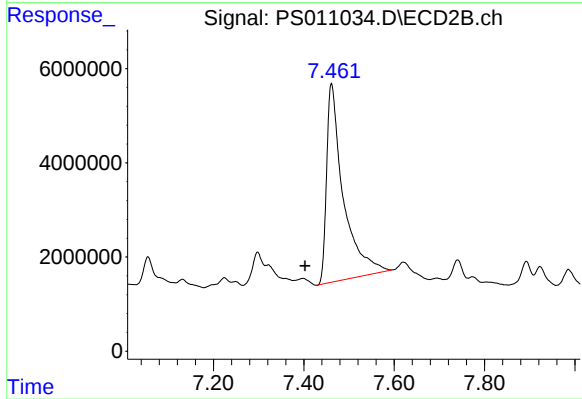

#7 MCPA


R.T.: 7.462 min
Delta R.T.: 0.059 min
Response: 108129086
Conc: 39.18 ug/ml

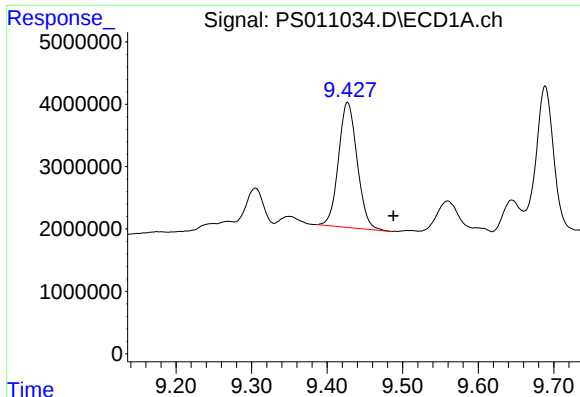

#12 2,4,5-T


R.T.: 9.427 min
Delta R.T.: -0.061 min
Response: 34452081
Conc: 7.40 ng/ml

Instrument :
ECD_S
ClientSampleId :

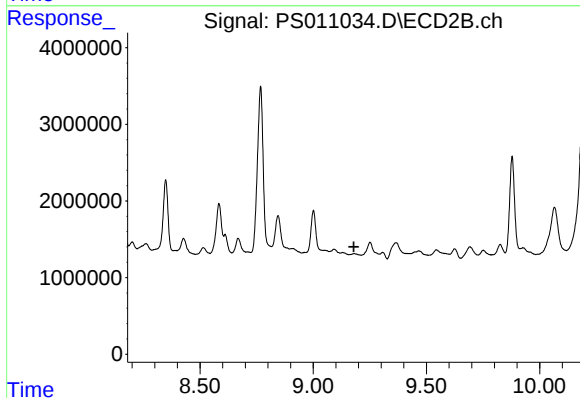


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.179 min
Response: 0
Conc: N.D.

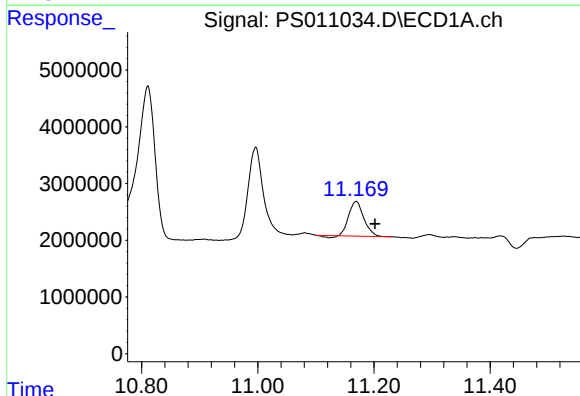


#14 DINOSEB

R.T.: 11.169 min
Delta R.T.: -0.033 min
Response: 10829960
Conc: 3.02 ng/ml

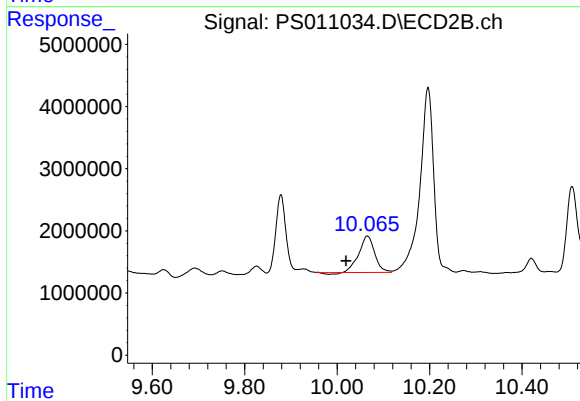

#14 DINOSEB


R.T.: 10.065 min
Delta R.T.: 0.046 min
Response: 13888268
Conc: 6.67 ng/ml

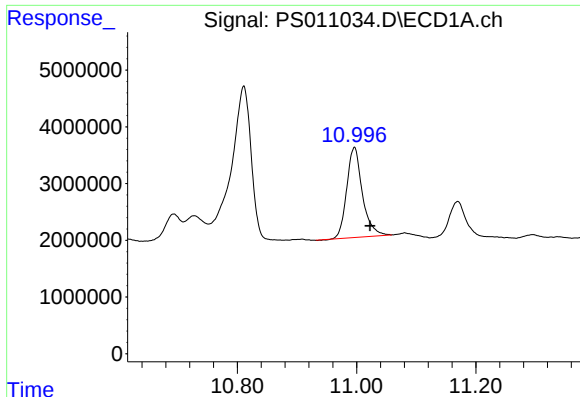

#15 Picloram

R.T.: 10.996 min
Delta R.T.: -0.026 min
Response: 28895232
Conc: 5.15 ng/ml

Instrument :
ECD_S
ClientSampleId :

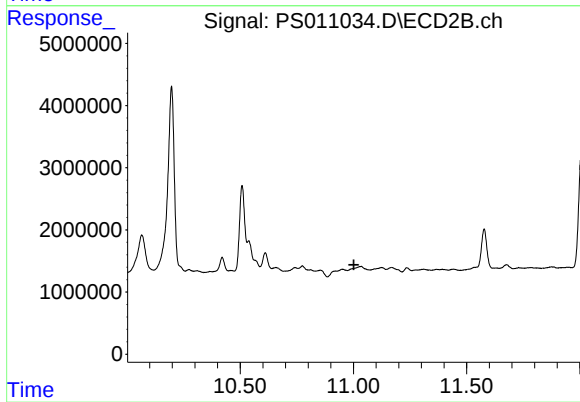

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 11.002 min
Response: 0
Conc: N.D.