

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070120\
 Data File : PS011036.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Jul 2020 18:49
 Operator : DD\AJ
 Sample : L3153-32
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 02 05:04:24 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062420.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 25 02:45:12 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.229	6.920	273.3E6	198.5E6	301.361	358.273
Target Compounds							
1) T	Dalapon	2.994	2.586	42048712	146.4E6	37.553	194.132 #
2) T	3,5-DICHL...	0.000	6.100	0	77153594	N.D.	92.641
3) T	4-Nitroph...	6.996	6.551	6181286	5312190	15.485	16.532
5) T	DICAMBA	7.408	7.055	5246399	6256504	1.439	2.755 #
6) T	MCPD	7.641	0.000	5684457	0	1.993	N.D. #
7) T	MCPA	7.696	7.466	89596936	66952634	22.498	24.258
8) T	DICHLORPROP	8.060	7.741	6593253	8290480	7.519	14.120 #
10) T	Pentachlo...	8.709	0.000	9851762	0	<MDL	N.D. #
12) T	2,4,5-T	9.426	0.000	33063669	0	7.098	N.D. #
15) T	Picloram	10.996	0.000	8343086	0	1.488	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070120\
Data File : PS011036.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Jul 2020 18:49
Operator : DD\AJ
Sample : L3153-32
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 02 05:04:24 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062420.M
Quant Title : 8080.M
QLast Update : Thu Jun 25 02:45:12 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

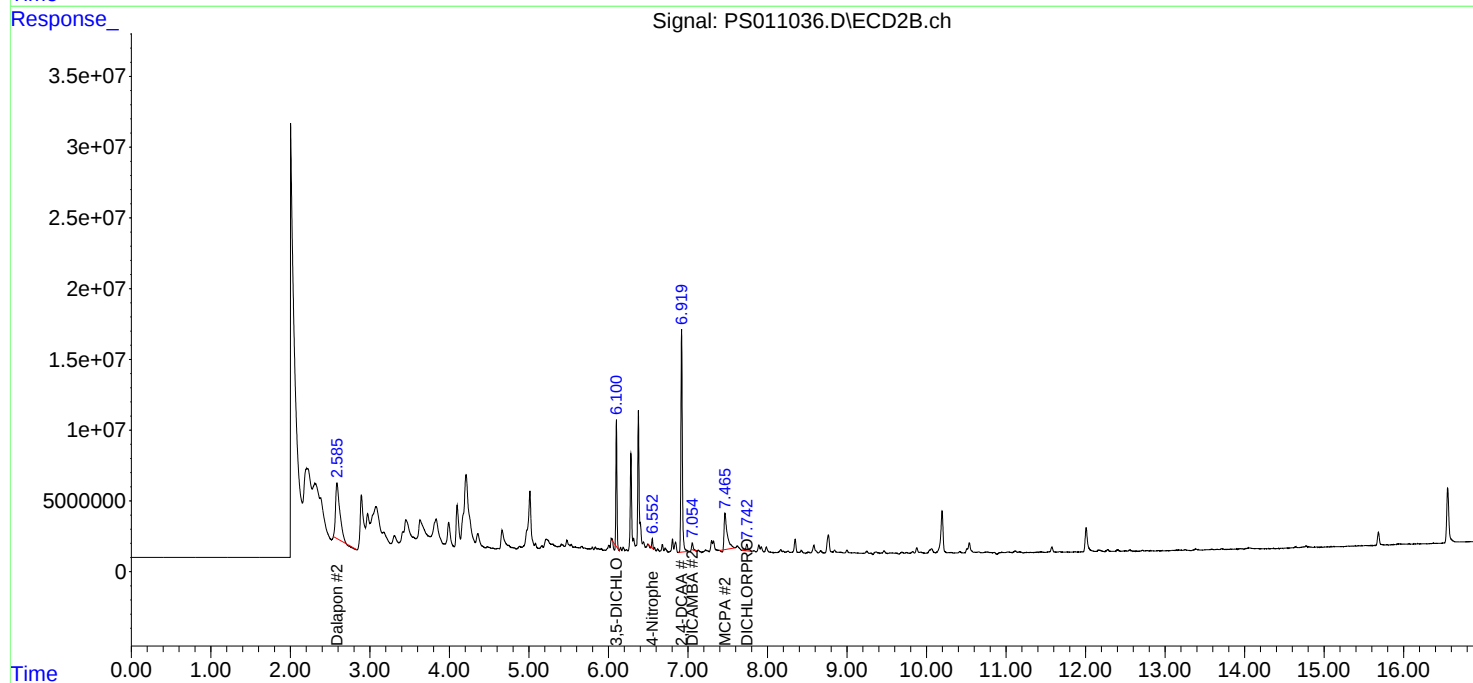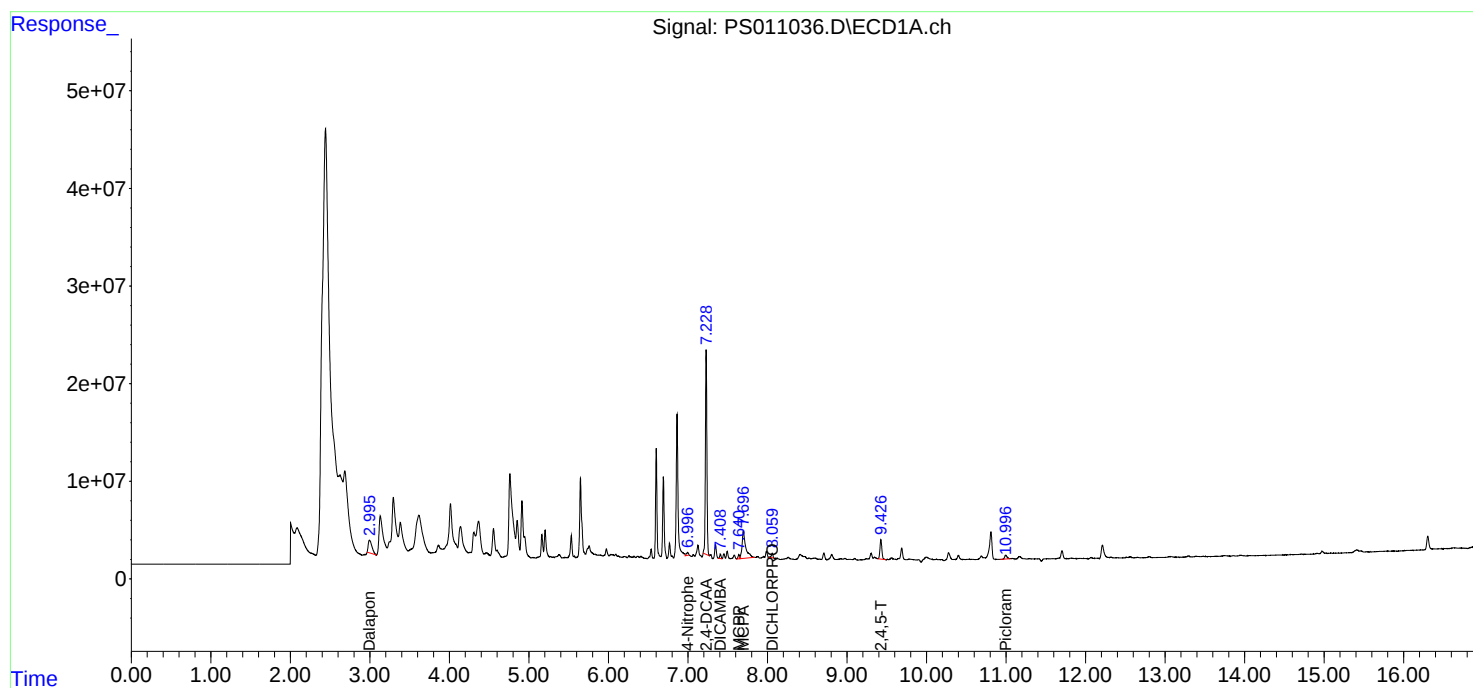


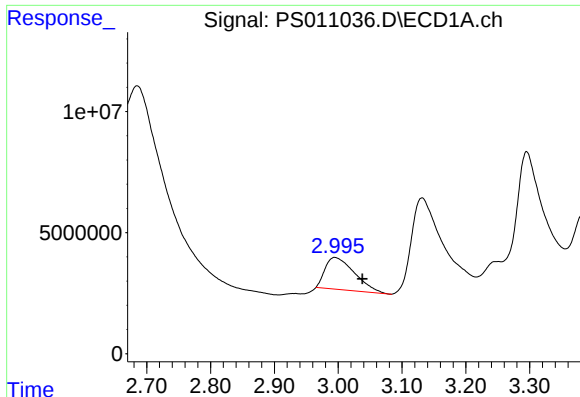

#1 Dalapon


R.T.: 2.994 min
Delta R.T.: -0.044 min
Response: 42048712
Conc: 37.55 ng/ml

Instrument :
ECD_S
ClientSampleId :

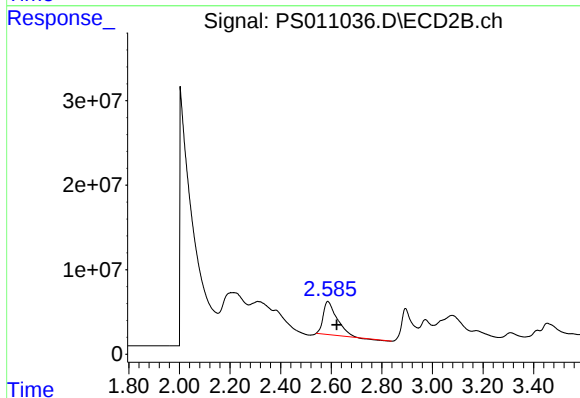


#1 Dalapon

R.T.: 2.586 min
Delta R.T.: -0.036 min
Response: 146445457
Conc: 194.13 ng/ml

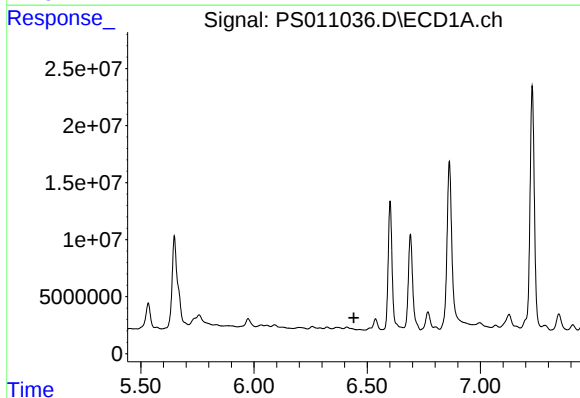


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.441 min
Response: 0
Conc: N.D.

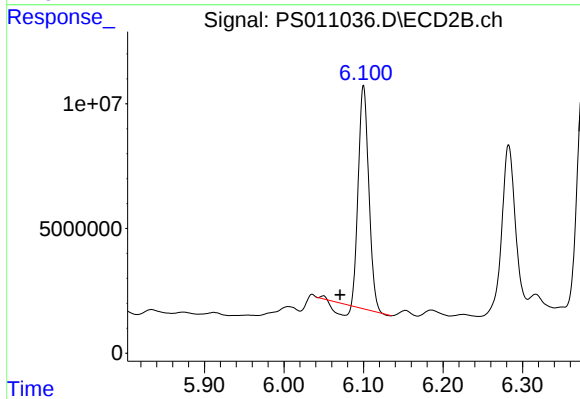

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.100 min
Delta R.T.: 0.030 min
Response: 77153594
Conc: 92.64 ng/ml

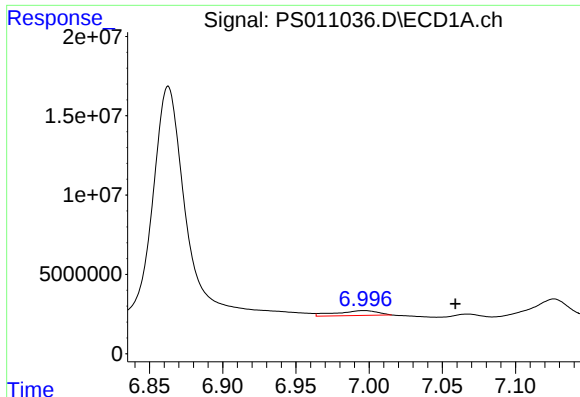

#3 4-Nitrophenol


R.T.: 6.996 min
Delta R.T.: -0.063 min
Response: 6181286
Conc: 15.49 ng/ml

Instrument :
ECD_S
ClientSampleId :

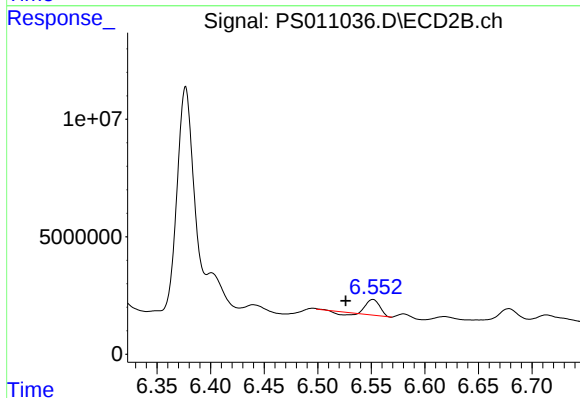


#3 4-Nitrophenol

R.T.: 6.551 min
Delta R.T.: 0.025 min
Response: 5312190
Conc: 16.53 ng/ml

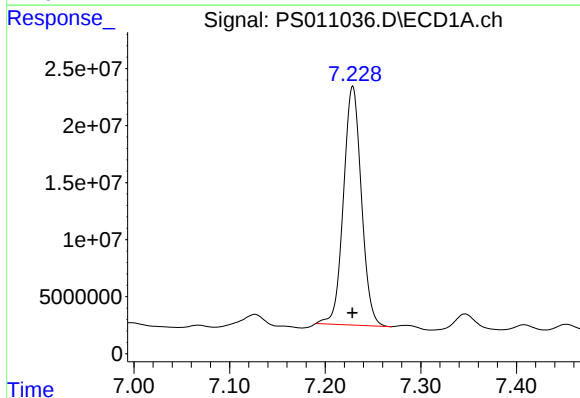


#4 2,4-DCAA

R.T.: 7.229 min
Delta R.T.: 0.000 min
Response: 273279476
Conc: 301.36 ng/ml

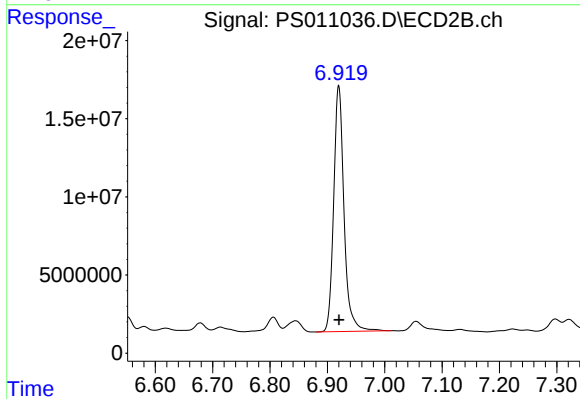

#4 2,4-DCAA


R.T.: 6.920 min
Delta R.T.: 0.000 min
Response: 198510644
Conc: 358.27 ng/ml

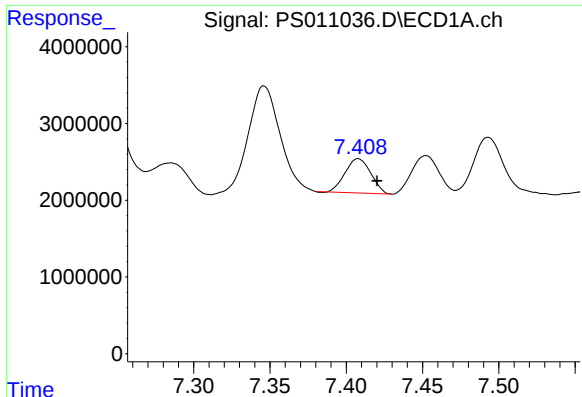

#5 DICAMBA


R.T.: 7.408 min
Delta R.T.: -0.012 min
Response: 5246399
Conc: 1.44 ng/ml

Instrument :
ECD_S
ClientSampleId :

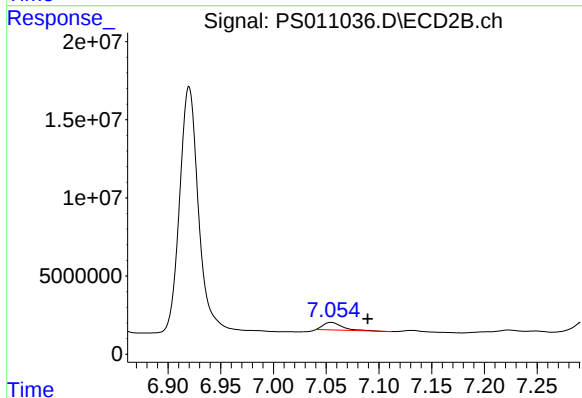


#5 DICAMBA

R.T.: 7.055 min
Delta R.T.: -0.035 min
Response: 6256504
Conc: 2.75 ng/ml

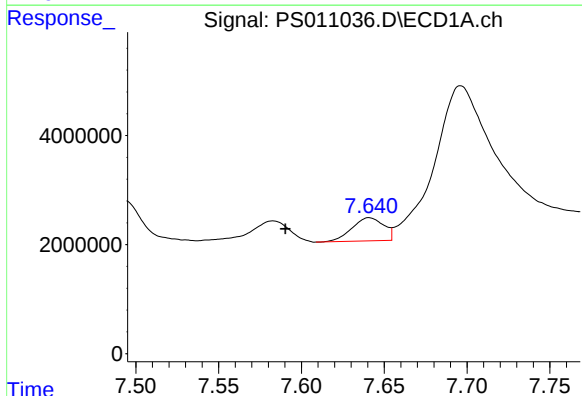


#6 MCP

R.T.: 7.641 min
Delta R.T.: 0.051 min
Response: 5684457
Conc: 1.99 ug/ml

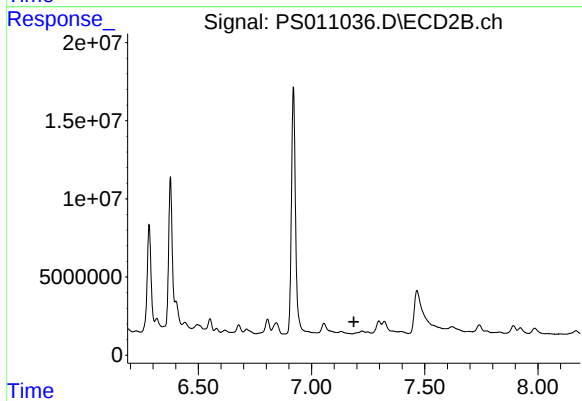

#6 MCP


R.T.: 0.000 min
Exp R.T.: 7.187 min
Response: 0
Conc: N.D.

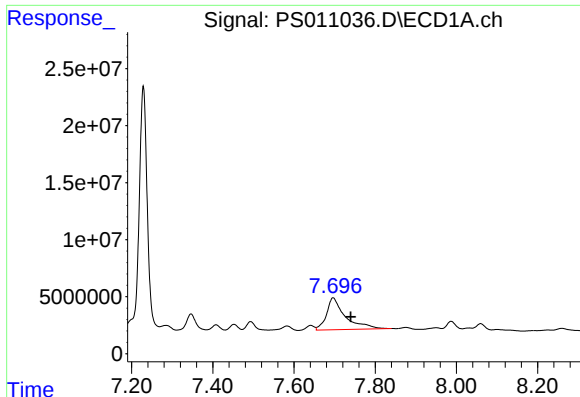

#7 MCPA


R.T.: 7.696 min
Delta R.T.: -0.044 min
Response: 89596936
Conc: 22.50 ug/ml

Instrument :
ECD_S
ClientSampleId :

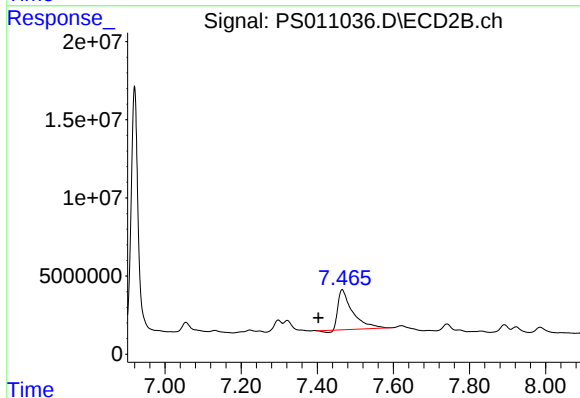


#7 MCPA

R.T.: 7.466 min
Delta R.T.: 0.063 min
Response: 66952634
Conc: 24.26 ug/ml

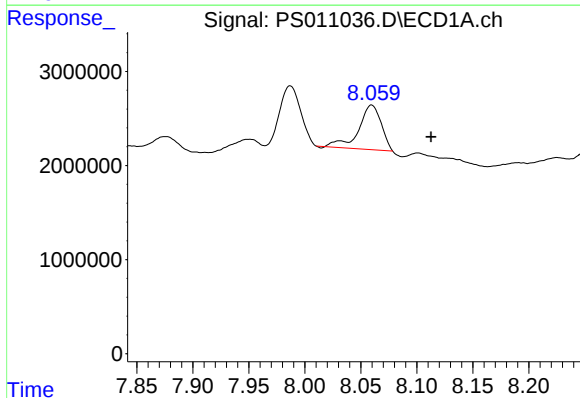


#8 DICHLORPROP

R.T.: 8.060 min
Delta R.T.: -0.053 min
Response: 6593253
Conc: 7.52 ng/ml

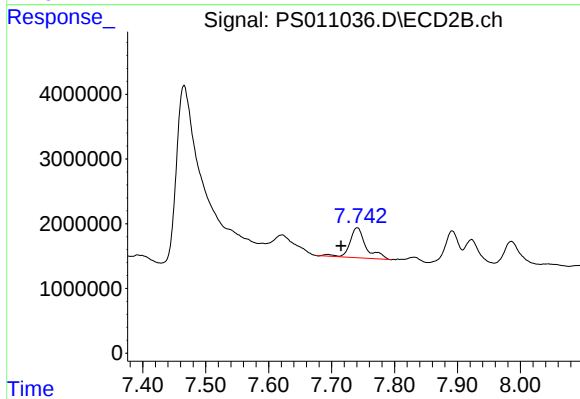

#8 DICHLORPROP


R.T.: 7.741 min
Delta R.T.: 0.025 min
Response: 8290480
Conc: 14.12 ng/ml

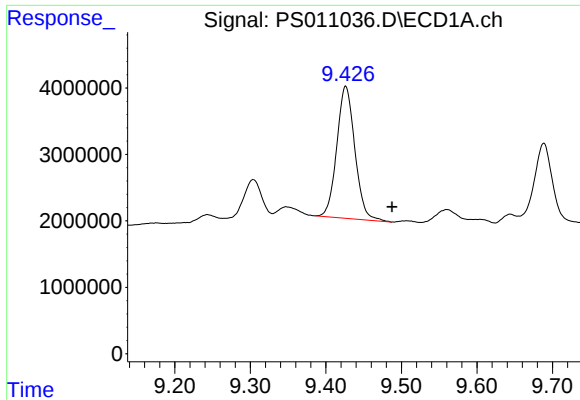

#12 2,4,5-T


R.T.: 9.426 min
Delta R.T.: -0.061 min
Response: 33063669
Conc: 7.10 ng/ml

Instrument :
ECD_S
ClientSampleId :

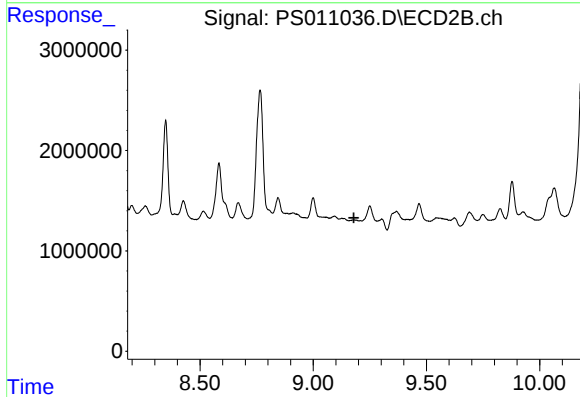


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.179 min
Response: 0
Conc: N.D.

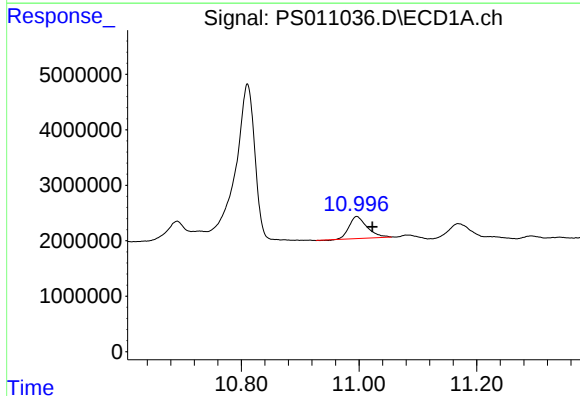

#15 Picloram

R.T.: 10.996 min
Delta R.T.: -0.026 min
Response: 8343086
Conc: 1.49 ng/ml

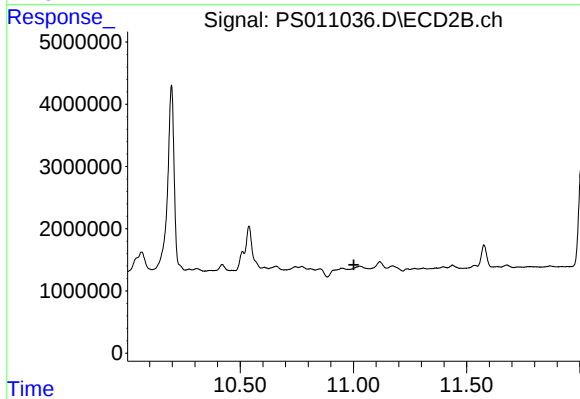

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 11.002 min
Response: 0
Conc: N.D.