

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070120\
 Data File : PS011038.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Jul 2020 19:35
 Operator : DD\AJ
 Sample : L3153-38
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 02 05:04:57 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062420.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 25 02:45:12 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.229	6.920	274.4E6	200.8E6	302.631	362.352
Target Compounds							
1) T	Dalapon	2.996	2.588	42393350	125.6E6	37.861	166.536 #
2) T	3,5-DICHL...	0.000	6.100	0	83198190	N.D.	99.899
3) T	4-Nitroph...	6.996	0.000	6295777	0	15.772	N.D. #
5) T	DICAMBA	7.408	0.000	5788578	0	1.588	N.D. #
6) T	MCPD	7.641	0.000	5912875	0	2.074	N.D. #
7) T	MCPA	7.694	7.464	122.2E6	119.3E6	30.686	43.219 #
10) T	Pentachlo...	8.708	0.000	8949549	0	<MDL	N.D. #
12) T	2,4,5-T	9.426	0.000	46425533	0	9.967	N.D. #
15) T	Picloram	10.997	0.000	8915253	0	1.590	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070120\
Data File : PS011038.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Jul 2020 19:35
Operator : DD\AJ
Sample : L3153-38
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 02 05:04:57 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062420.M
Quant Title : 8080.M
QLast Update : Thu Jun 25 02:45:12 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

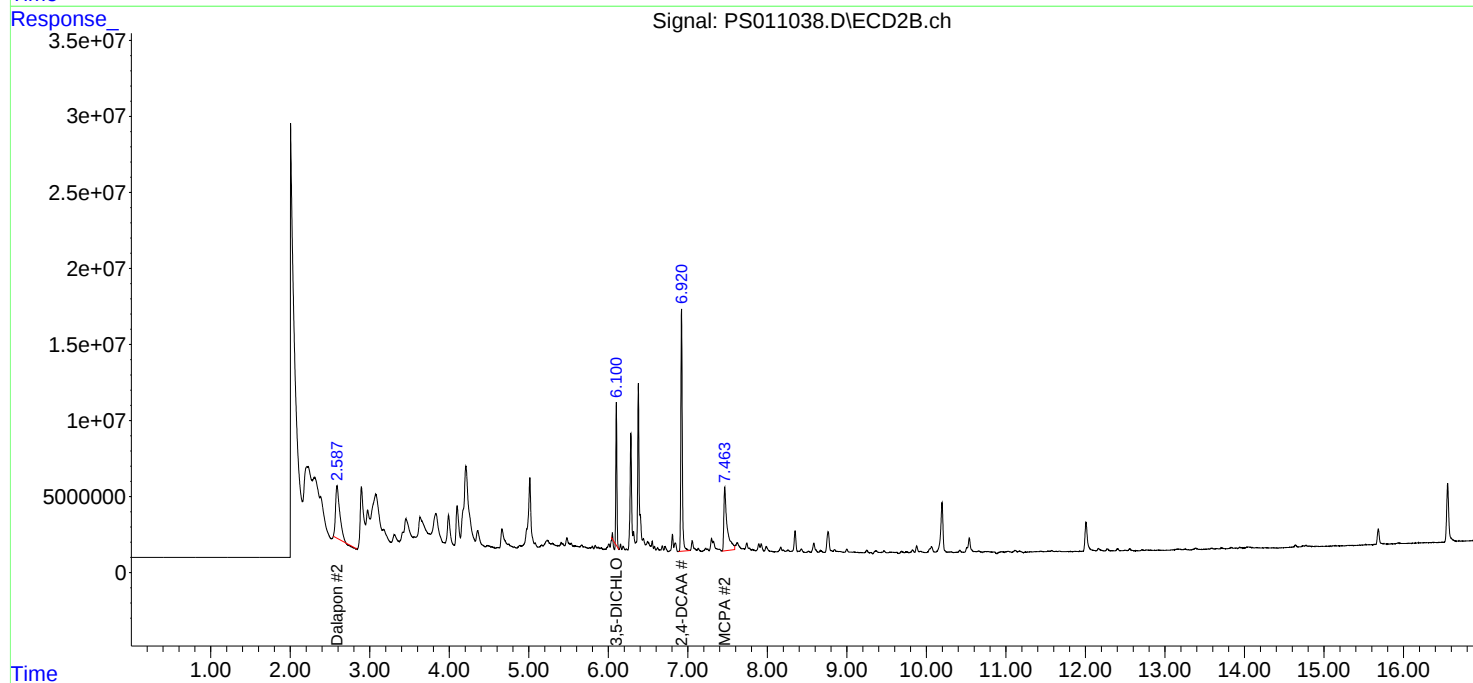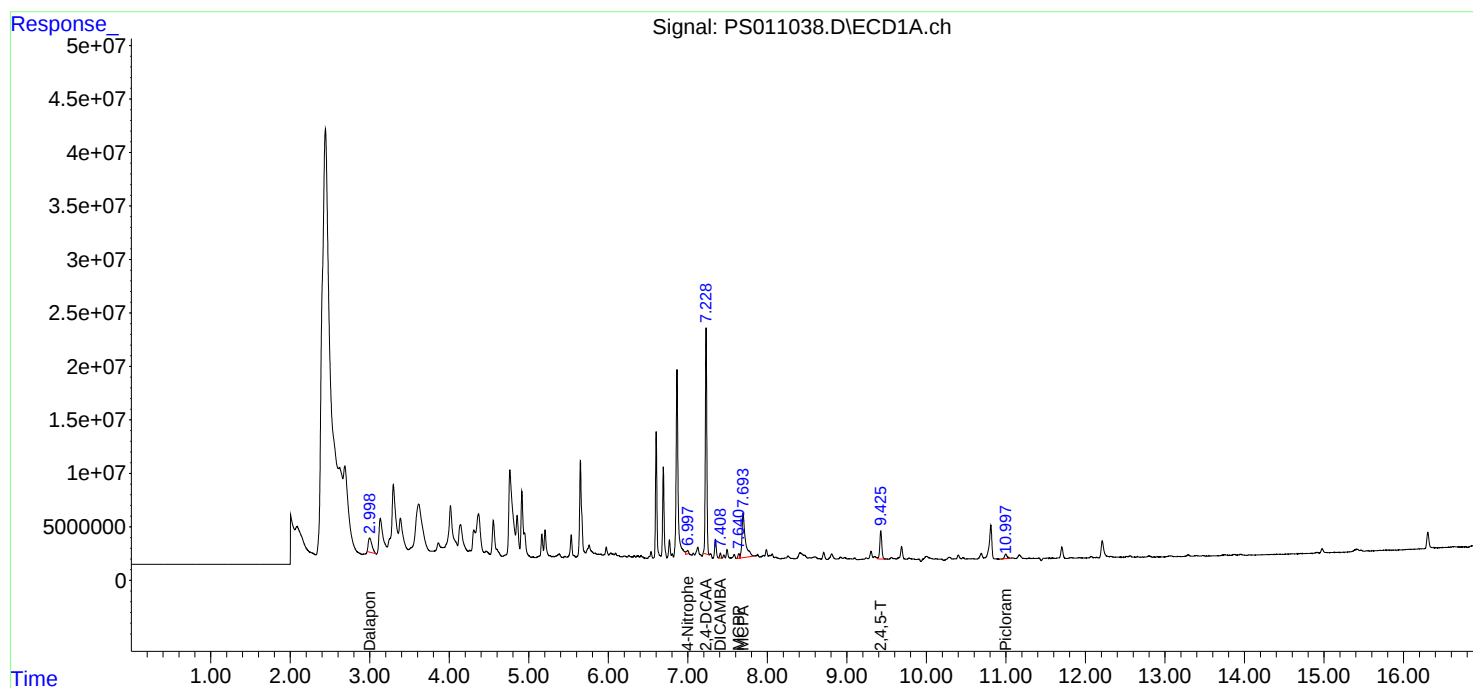


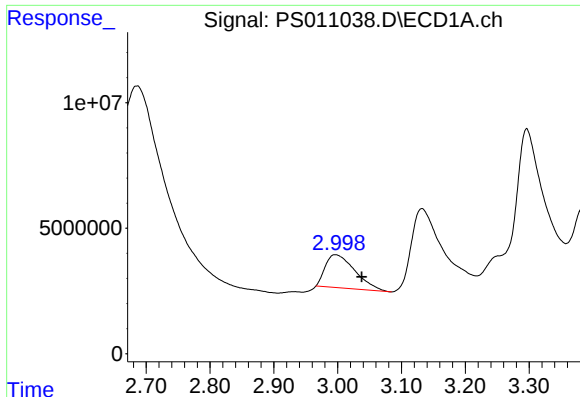

#1 Dalapon


R.T.: 2.996 min
Delta R.T.: -0.042 min
Response: 42393350
Conc: 37.86 ng/ml

Instrument :
ECD_S
ClientSampleId :

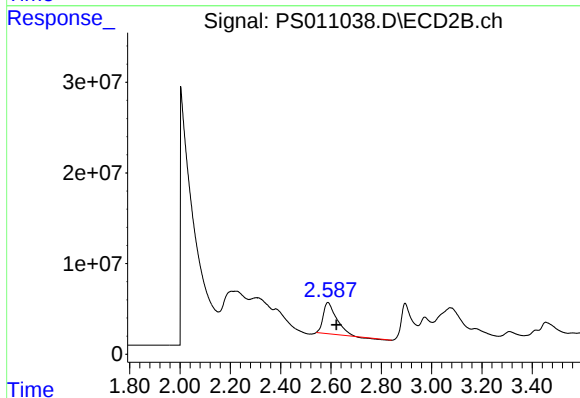


#1 Dalapon

R.T.: 2.588 min
Delta R.T.: -0.034 min
Response: 125627857
Conc: 166.54 ng/ml

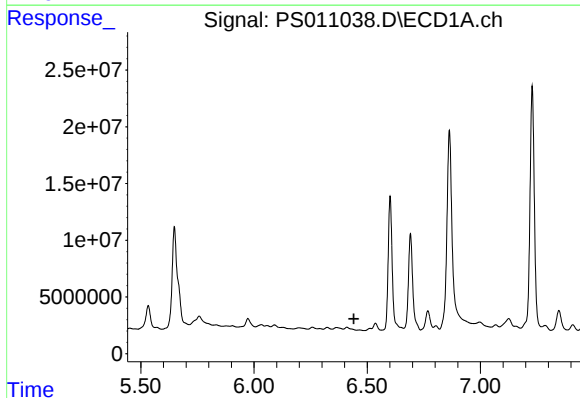


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.441 min
Response: 0
Conc: N.D.

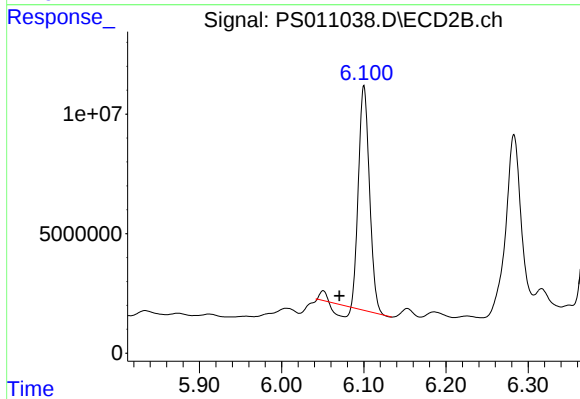

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.100 min
Delta R.T.: 0.030 min
Response: 83198190
Conc: 99.90 ng/ml

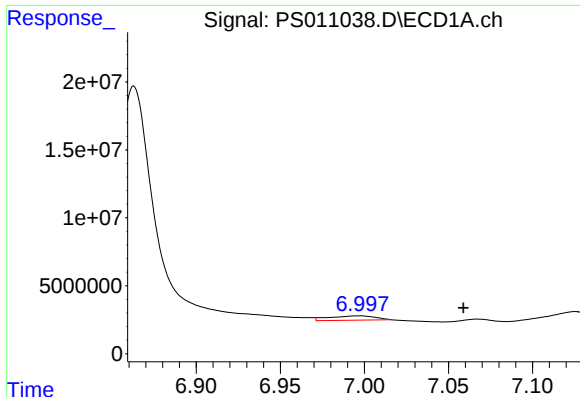

#3 4-Nitrophenol


R.T.: 6.996 min
Delta R.T.: -0.063 min
Response: 6295777
Conc: 15.77 ng/ml

Instrument :
ECD_S
ClientSampleId :

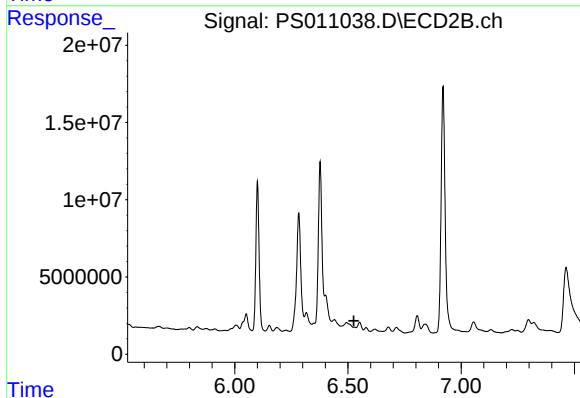


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.526 min
Response: 0
Conc: N.D.

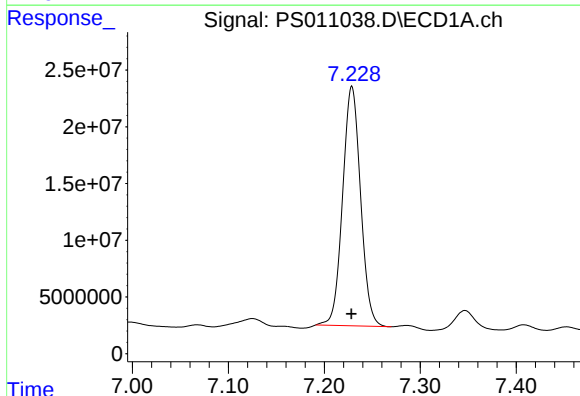


#4 2,4-DCAA

R.T.: 7.229 min
Delta R.T.: 0.000 min
Response: 274431494
Conc: 302.63 ng/ml

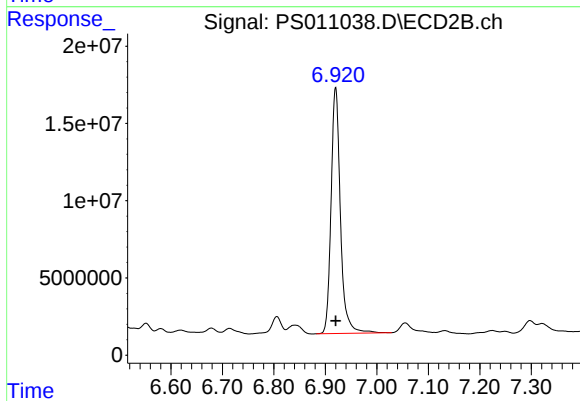

#4 2,4-DCAA


R.T.: 6.920 min
Delta R.T.: 0.000 min
Response: 200770348
Conc: 362.35 ng/ml

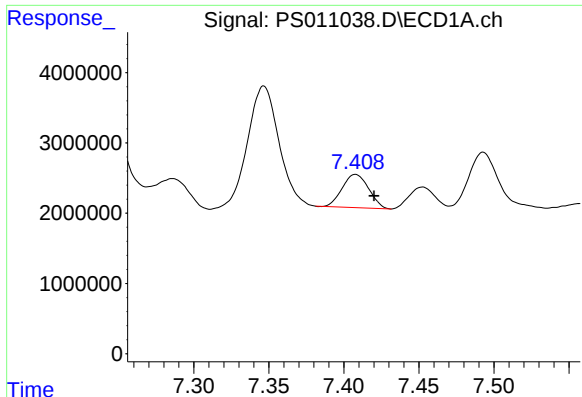

#5 DICAMBA


R.T.: 7.408 min
Delta R.T.: -0.012 min
Response: 5788578
Conc: 1.59 ng/ml

Instrument :
ECD_S
ClientSampleId :

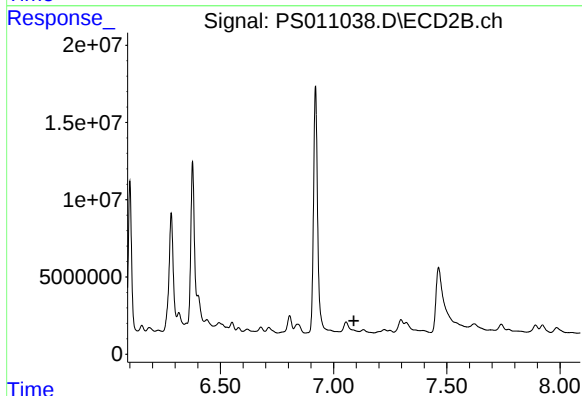


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.089 min
Response: 0
Conc: N.D.

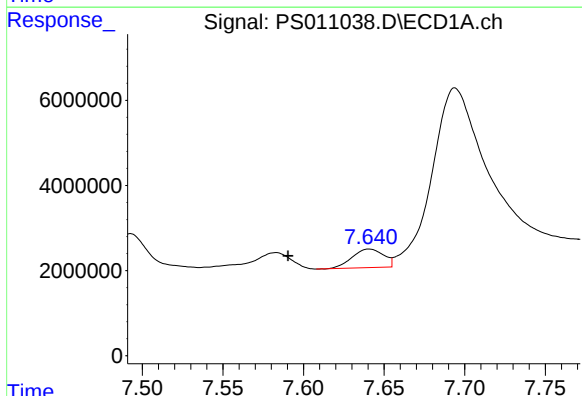


#6 MCP

R.T.: 7.641 min
Delta R.T.: 0.050 min
Response: 5912875
Conc: 2.07 ug/ml

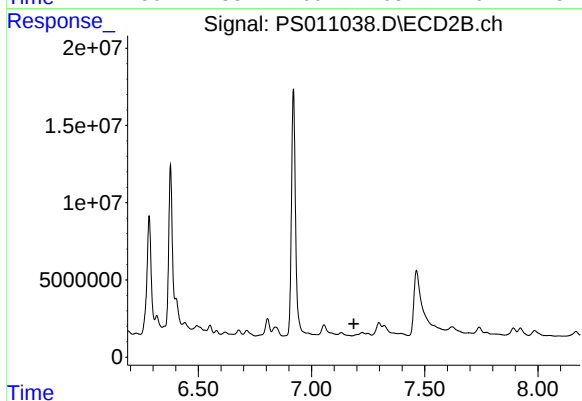

#6 MCP


R.T.: 0.000 min
Exp R.T. : 7.187 min
Response: 0
Conc: N.D.

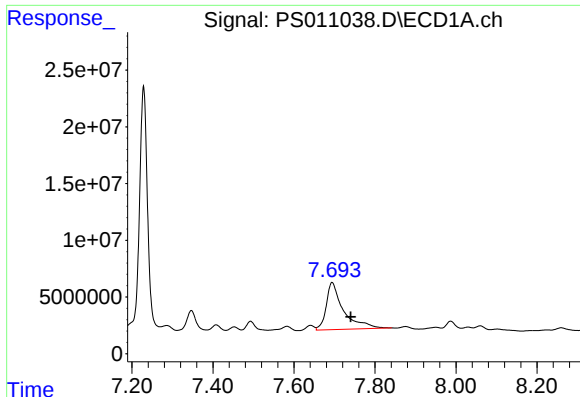

#7 MCPA


R.T.: 7.694 min
Delta R.T.: -0.046 min
Response: 122206984
Conc: 30.69 ug/ml

Instrument :
ECD_S
ClientSampleId :

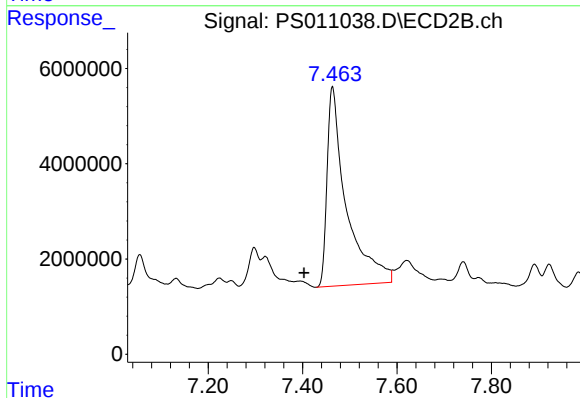


#7 MCPA

R.T.: 7.464 min
Delta R.T.: 0.061 min
Response: 119283990
Conc: 43.22 ug/ml

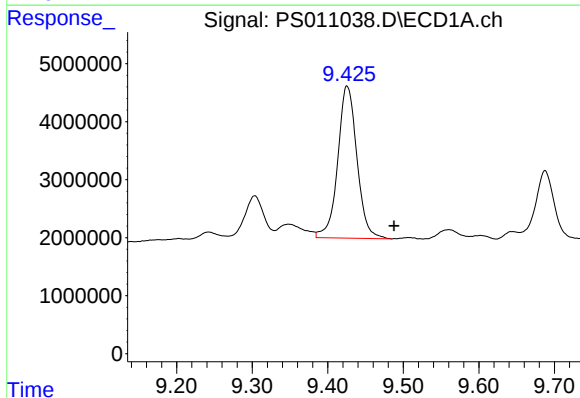


#12 2,4,5-T

R.T.: 9.426 min
Delta R.T.: -0.062 min
Response: 46425533
Conc: 9.97 ng/ml

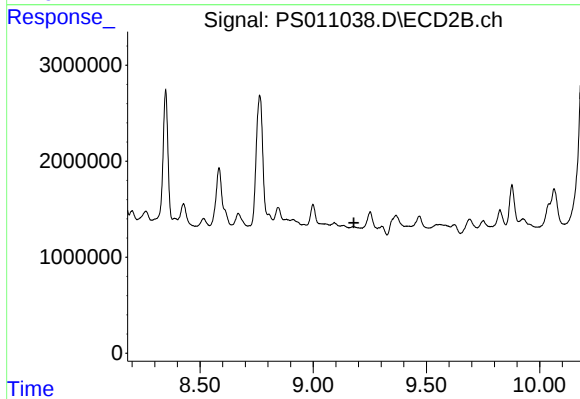

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.179 min
Response: 0
Conc: N.D.

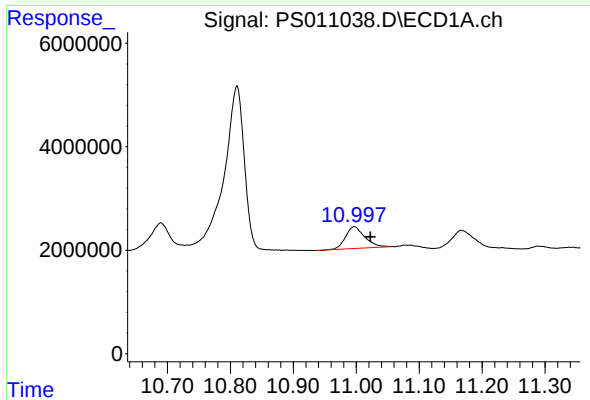

#15 Picloram

R.T.: 10.997 min
Delta R.T.: -0.026 min
Response: 8915253
Conc: 1.59 ng/ml

Instrument :
ECD_S
ClientSampleId :

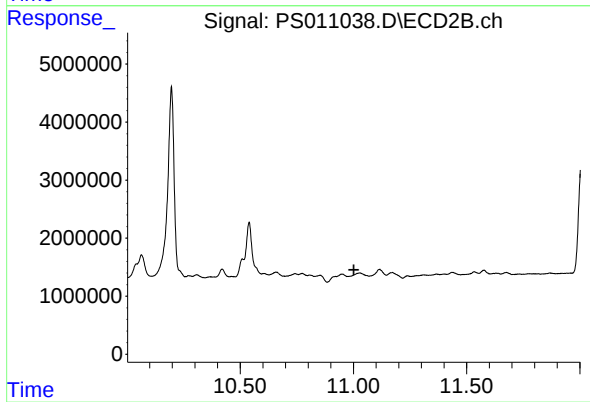

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 11.002 min
Response: 0
Conc: N.D.