

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070120\
 Data File : PS011039.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Jul 2020 19:58
 Operator : DD\AJ
 Sample : PB129894BL
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 02 05:05:14 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062420.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 25 02:45:12 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.228	6.920	439.6E6	294.8E6	484.772	532.144
Target Compounds							
1) T	Dalapon	2.995	2.585	39660068	113.0E6	35.420	149.787 #
2) T	3,5-DICHL...	0.000	6.101	0	14601733	N.D.	17.533
7) T	MCPA	7.776	7.384	45099261	36014754	11.325	13.049
8) T	DICHLORPROP	0.000	7.740	0	5200861	N.D.	8.858
9) T	2,4-D	0.000	7.986	0	7145414	N.D.	9.888
10) T	Pentachlo...	8.708	0.000	15848289	0	1.275	N.D. #
12) T	2,4,5-T	9.509	0.000	6198828	0	1.331	N.D. #
13) T	2,4-DB	0.000	9.626	0	12412676	N.D.	30.202
14) T	DINOSEB	11.168	10.037	55014522	13687201	15.361	6.574 #
15) T	Picloram	10.993	11.034	288.8E6	17551375	51.507	4.189 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070120\
Data File : PS011039.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Jul 2020 19:58
Operator : DD\AJ
Sample : PB129894BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 02 05:05:14 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062420.M
Quant Title : 8080.M
QLast Update : Thu Jun 25 02:45:12 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

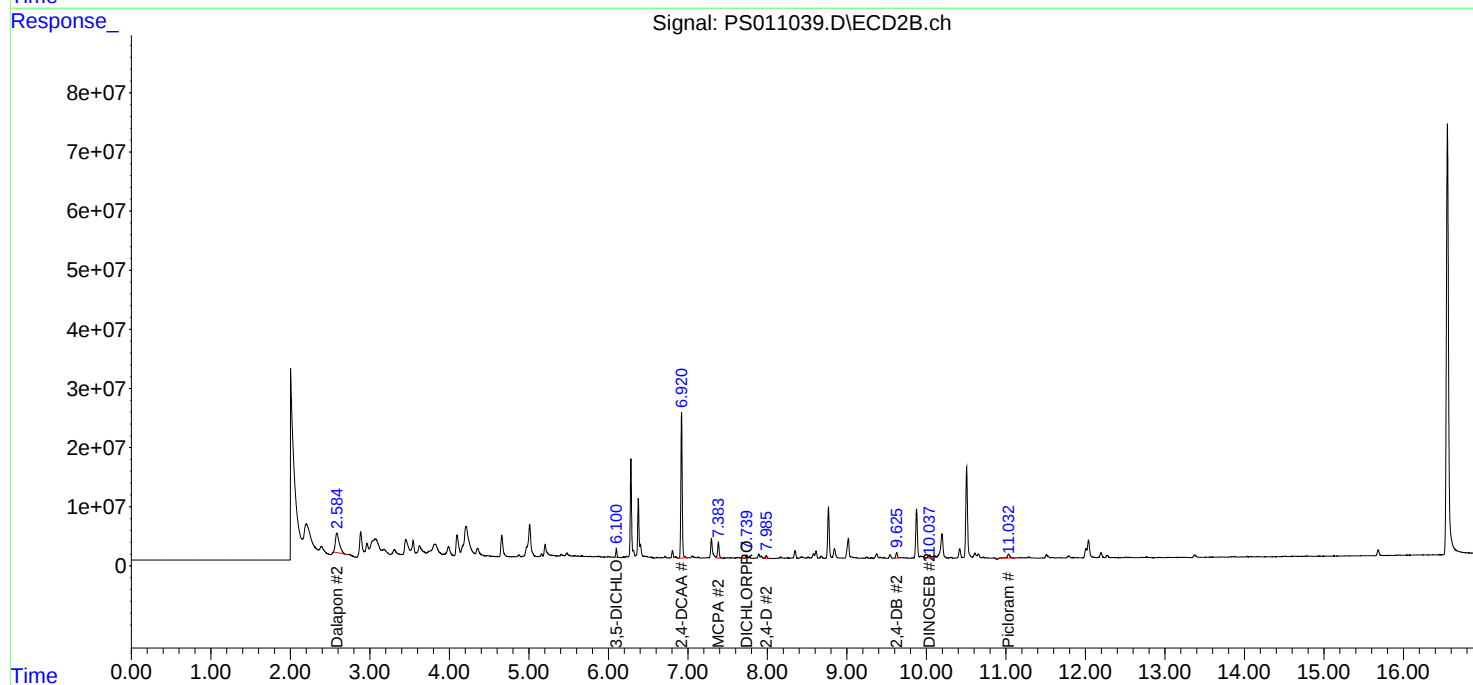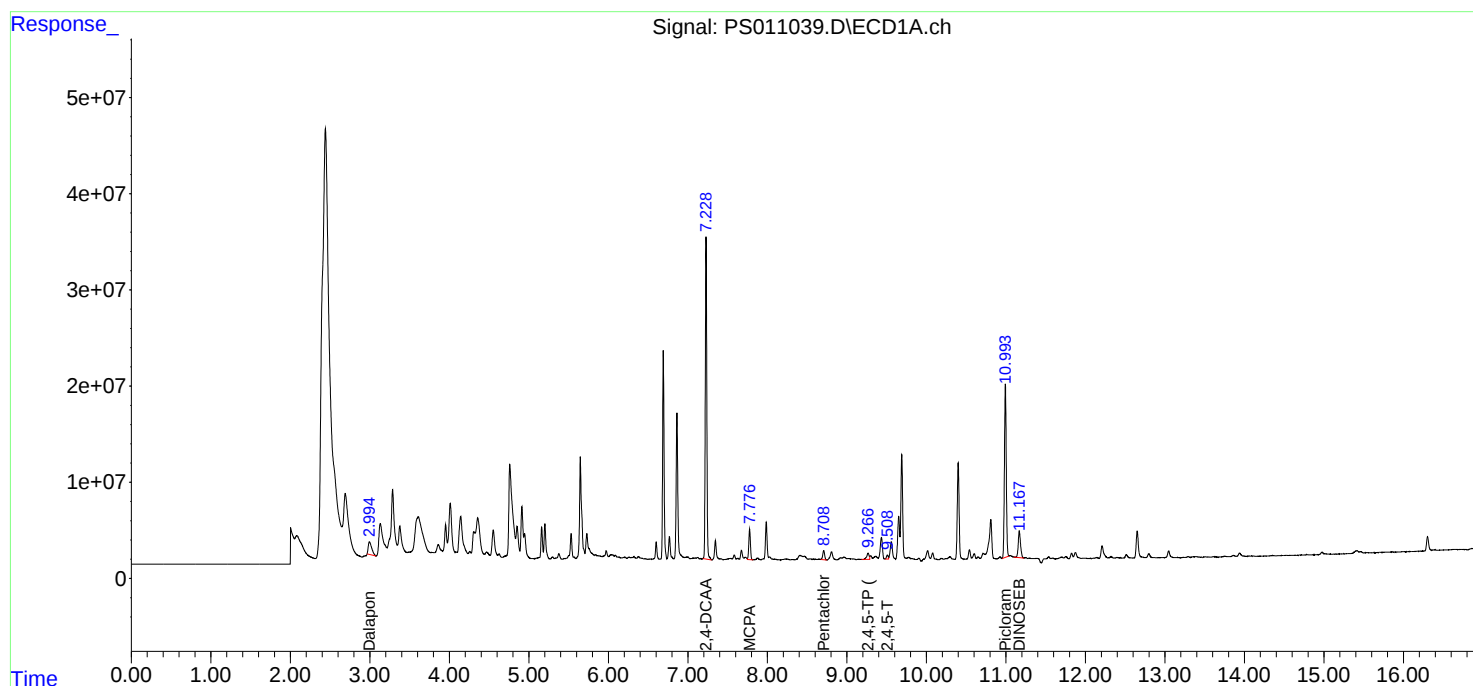


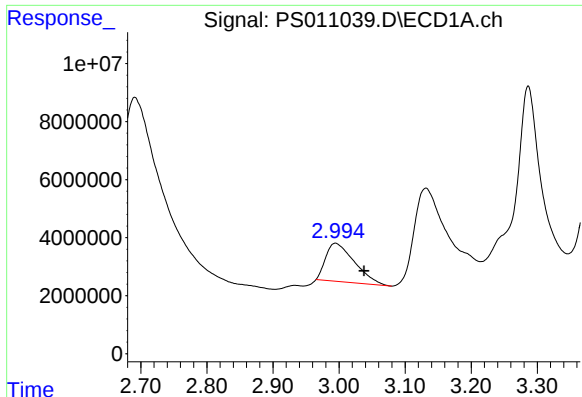

#1 Dalapon


R.T.: 2.995 min
Delta R.T.: -0.043 min
Response: 39660068
Conc: 35.42 ng/ml

Instrument :
ECD_S
ClientSampleId :

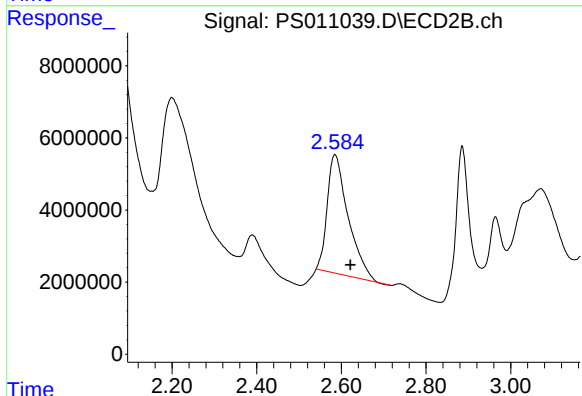


#1 Dalapon

R.T.: 2.585 min
Delta R.T.: -0.037 min
Response: 112993753
Conc: 149.79 ng/ml

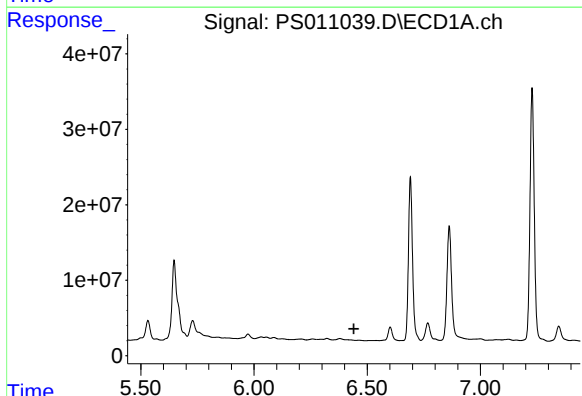


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.441 min
Response: 0
Conc: N.D.

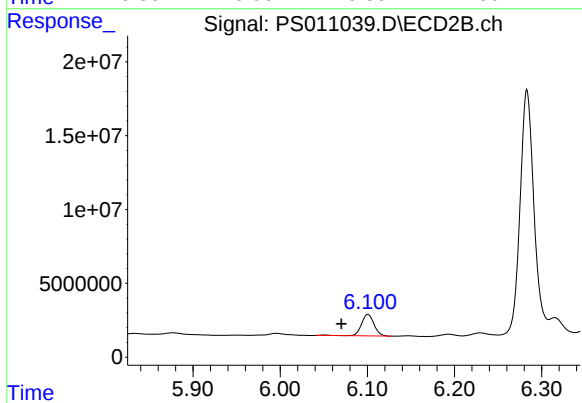

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.101 min
Delta R.T.: 0.030 min
Response: 14601733
Conc: 17.53 ng/ml

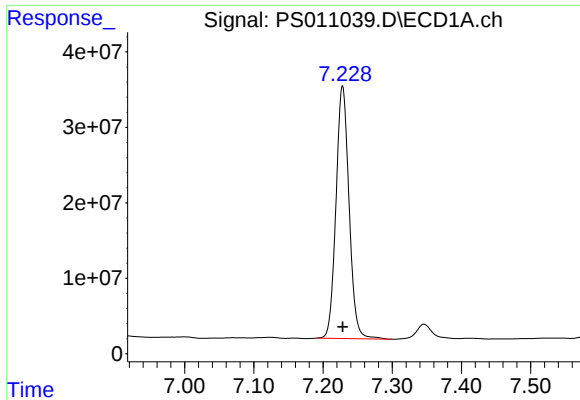

#4 2,4-DCAA


R.T.: 7.228 min
Delta R.T.: 0.000 min
Response: 439600018
Conc: 484.77 ng/ml

Instrument :
ECD_S
ClientSampleId :

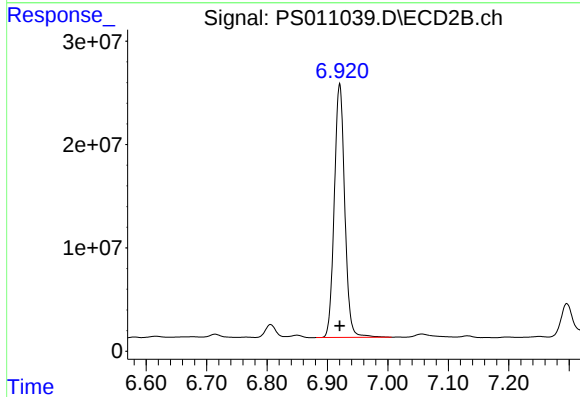


#4 2,4-DCAA

R.T.: 6.920 min
Delta R.T.: 0.000 min
Response: 294848108
Conc: 532.14 ng/ml

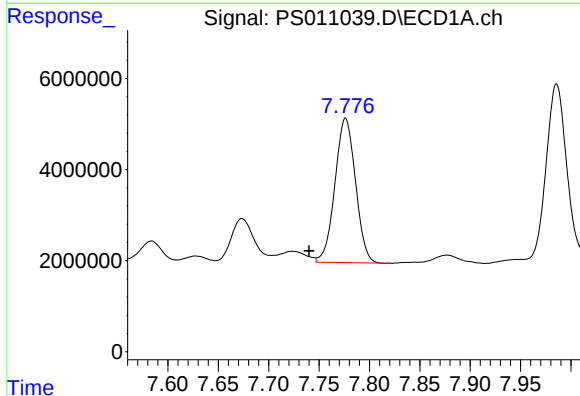


#7 MCPA

R.T.: 7.776 min
Delta R.T.: 0.036 min
Response: 45099261
Conc: 11.32 ug/ml

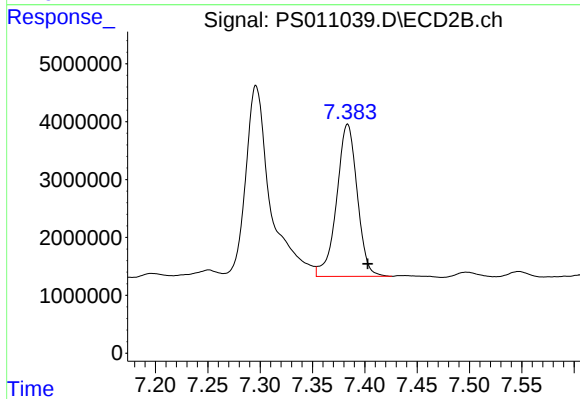

#7 MCPA


R.T.: 7.384 min
Delta R.T.: -0.019 min
Response: 36014754
Conc: 13.05 ug/ml

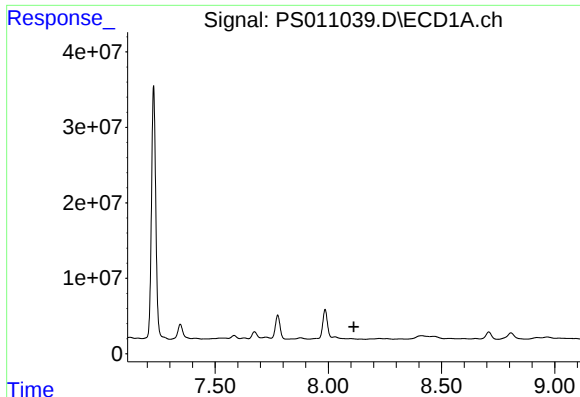

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.113 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

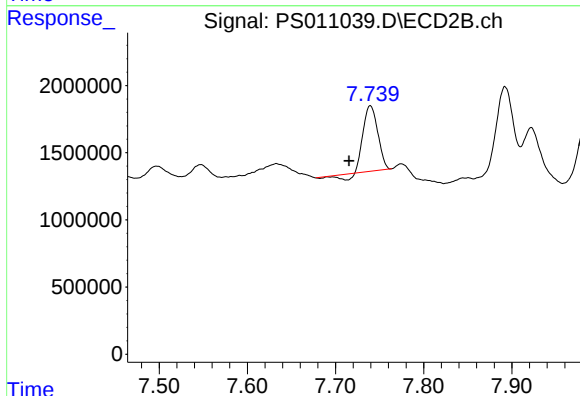


#8 DICHLORPROP

R.T.: 7.740 min
Delta R.T.: 0.024 min
Response: 5200861
Conc: 8.86 ng/ml

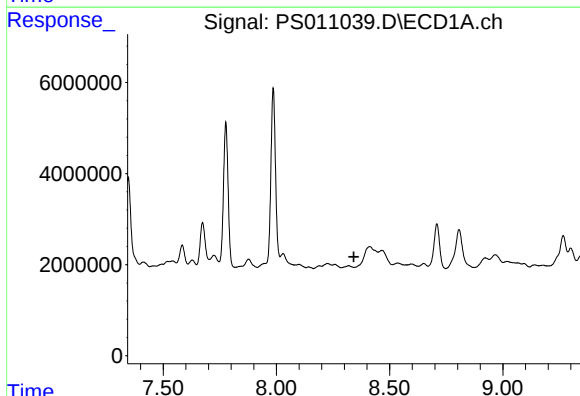


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 8.342 min
Response: 0
Conc: N.D.

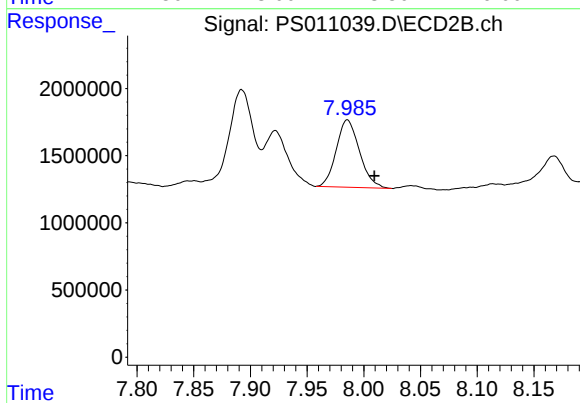

#9 2,4-D


R.T.: 7.986 min
Delta R.T.: -0.024 min
Response: 7145414
Conc: 9.89 ng/ml

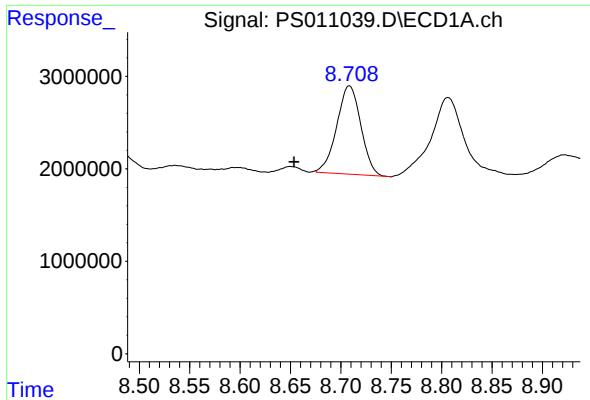

#10 Pentachlorophenol


R.T.: 8.708 min
Delta R.T.: 0.055 min
Response: 15848289
Conc: 1.27 ng/ml

Instrument :
ECD_S
ClientSampleId :

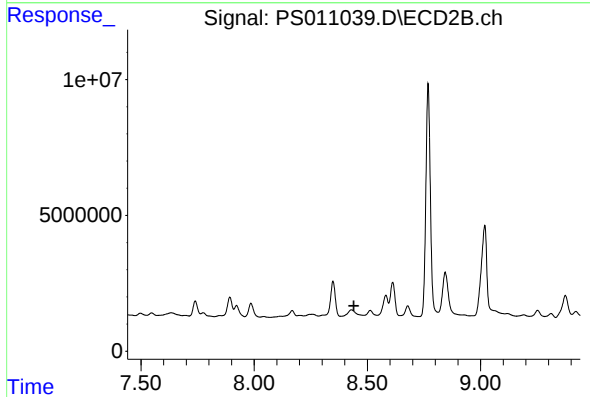


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 8.440 min
Response: 0
Conc: N.D.

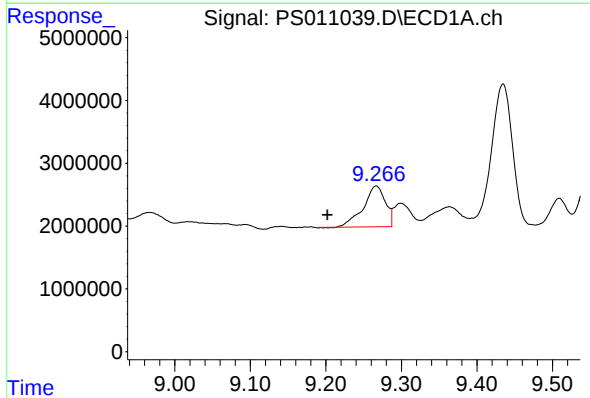


#11 2,4,5-TP (SILVEX)

R.T.: 9.266 min
Delta R.T.: 0.064 min
Response: 13234509
Conc: 2.67 ng/ml

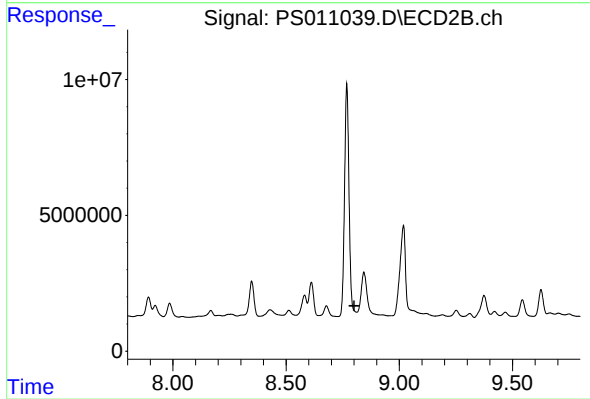

#11 2,4,5-TP (SILVEX)


R.T.: 8.844 min
Delta R.T.: 0.044 min
Response: -123472807
Conc: N.D.

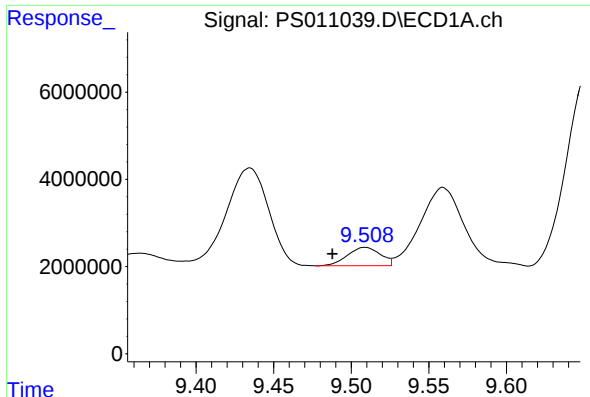

#12 2,4,5-T


R.T.: 9.509 min
Delta R.T.: 0.021 min
Response: 6198828
Conc: 1.33 ng/ml

Instrument :
ECD_S
ClientSampleId :

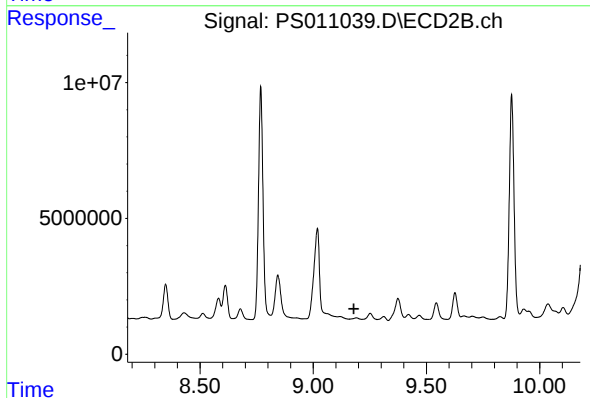


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.179 min
Response: 0
Conc: N.D.

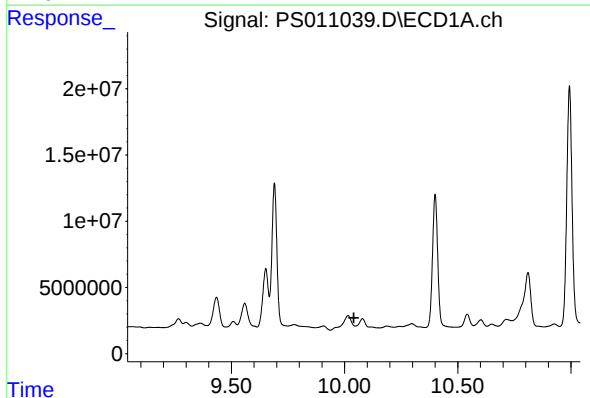


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 10.041 min
Response: 0
Conc: N.D.

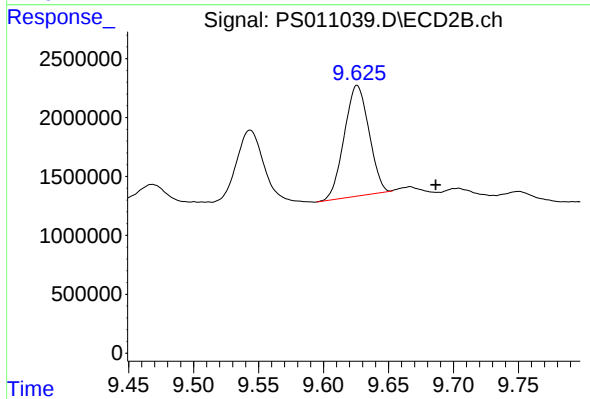

#13 2,4-DB


R.T.: 9.626 min
Delta R.T.: -0.060 min
Response: 12412676
Conc: 30.20 ng/ml

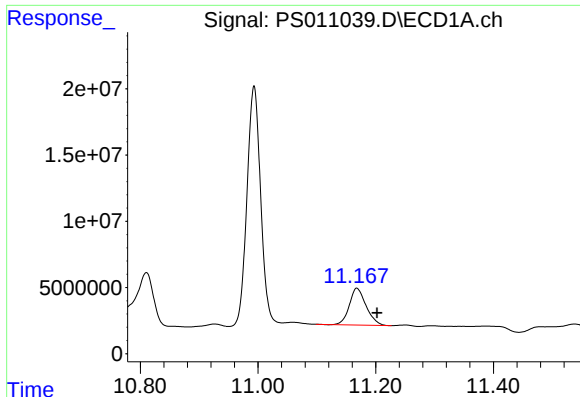

#14 DINOSEB


R.T.: 11.168 min
Delta R.T.: -0.034 min
Response: 55014522
Conc: 15.36 ng/ml

Instrument :
ECD_S
ClientSampleId :

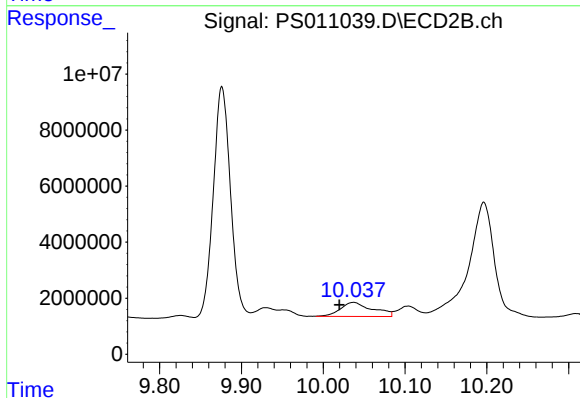


#14 DINOSEB

R.T.: 10.037 min
Delta R.T.: 0.017 min
Response: 13687201
Conc: 6.57 ng/ml

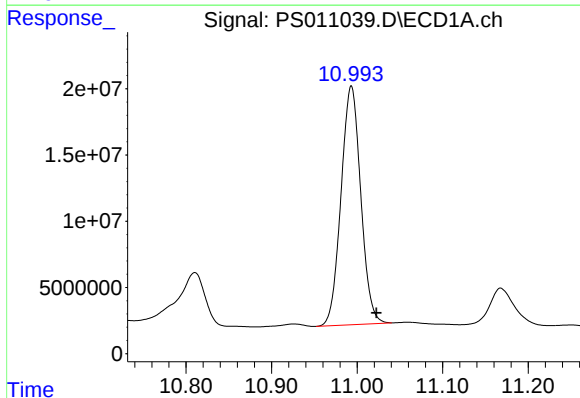

#15 Picloram

R.T.: 10.993 min
Delta R.T.: -0.029 min
Response: 288753449
Conc: 51.51 ng/ml

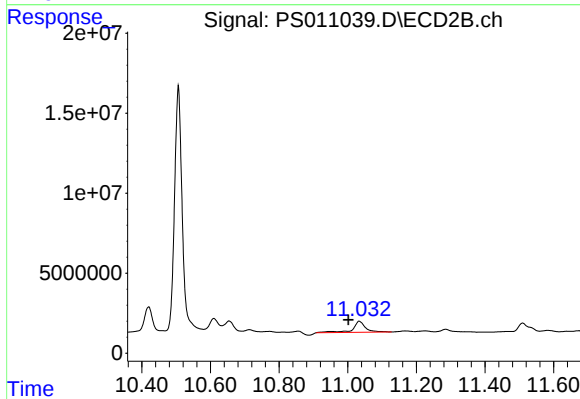

#15 Picloram

R.T.: 11.034 min
Delta R.T.: 0.031 min
Response: 17551375
Conc: 4.19 ng/ml