

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070120\
 Data File : PS011044.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Jul 2020 21:53
 Operator : DD\AJ
 Sample : L3153-01
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 02 05:06:43 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062420.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 25 02:45:12 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.228	6.919	434.5E6	291.6E6	479.131	526.348
Target Compounds							
1) T	Dalapon	2.997	2.585	39150569	109.9E6	34.965	145.737 #
2) T	3,5-DICHL...	0.000	6.100	0	50222053	N.D.	60.303
3) T	4-Nitroph...	7.001	0.000	5130232	0	12.852	N.D. #
7) T	MCPA	7.776	7.383	52586842	45205747	13.205	16.379
8) T	DICHLORPROP	0.000	7.737	0	28585167	N.D.	48.686
10) T	Pentachlo...	8.707	0.000	10650719	0	<MDL	N.D. #
12) T	2,4,5-T	9.507	0.000	8422035	0	1.808	N.D. #
14) T	DINOSEB	11.167	10.035	14123962	18032764	3.944	8.661 #
15) T	Picloram	10.992	11.030	38481508	14603203	6.864	3.486 #
16) T	DCPA	11.525	0.000	7972369	0	1.304	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070120\
Data File : PS011044.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Jul 2020 21:53
Operator : DD\AJ
Sample : L3153-01
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 02 05:06:43 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062420.M
Quant Title : 8080.M
QLast Update : Thu Jun 25 02:45:12 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

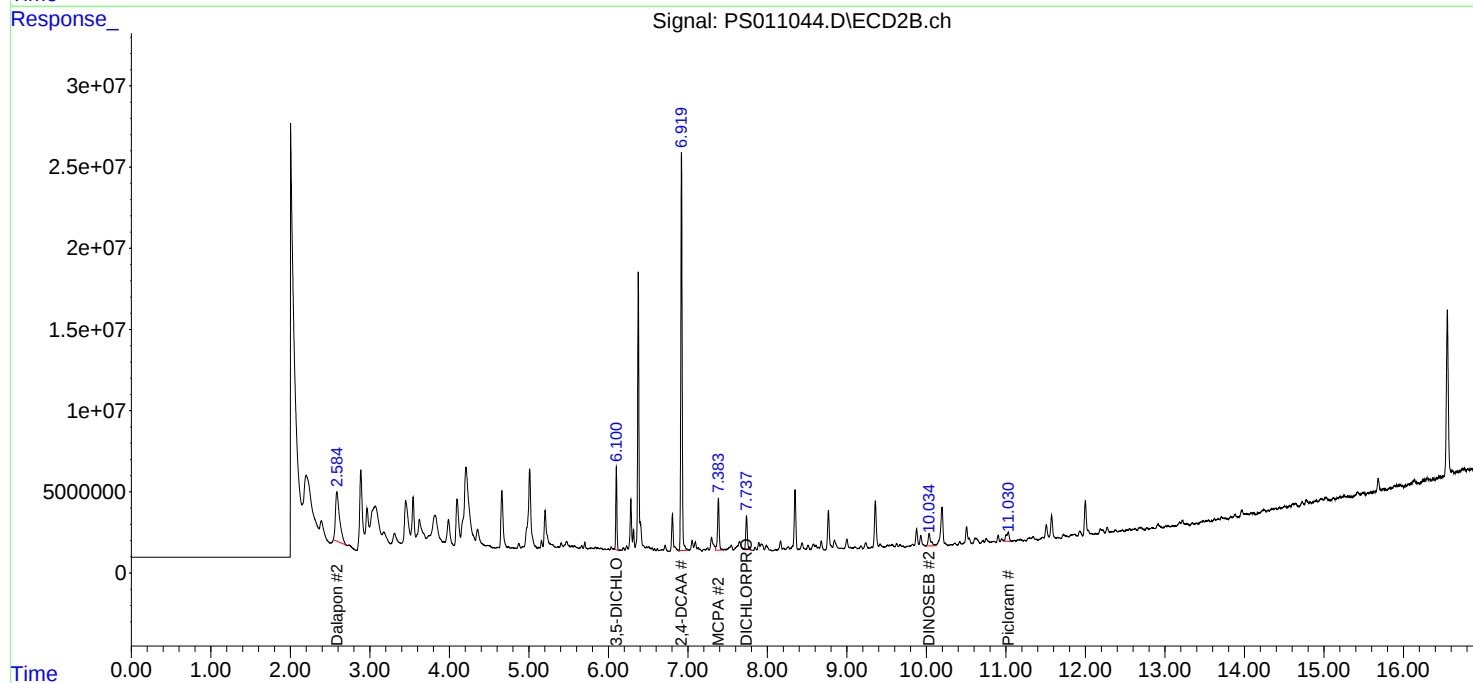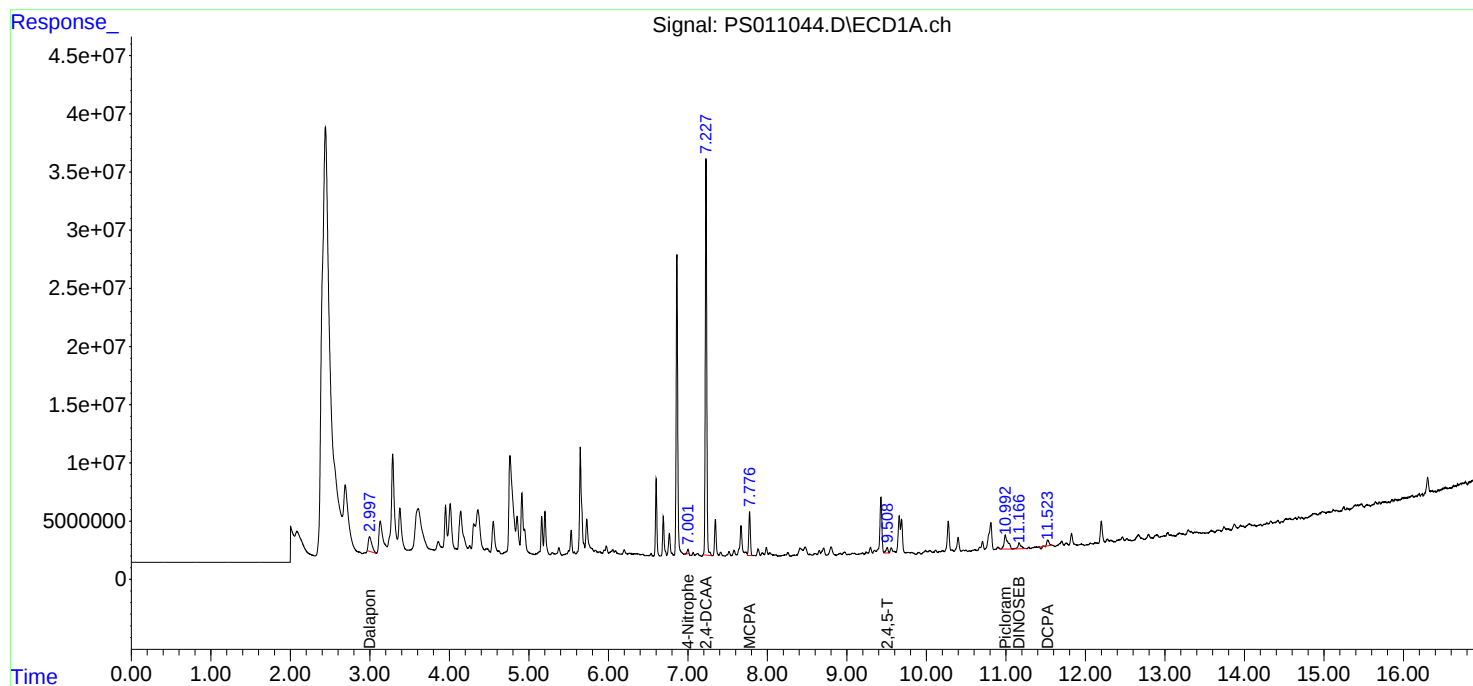


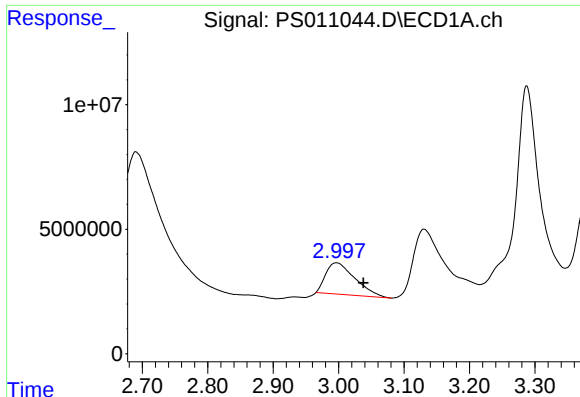

#1 Dalapon


R.T.: 2.997 min
Delta R.T.: -0.041 min
Response: 39150569
Conc: 34.96 ng/ml

Instrument :
ECD_S
ClientSampleId :

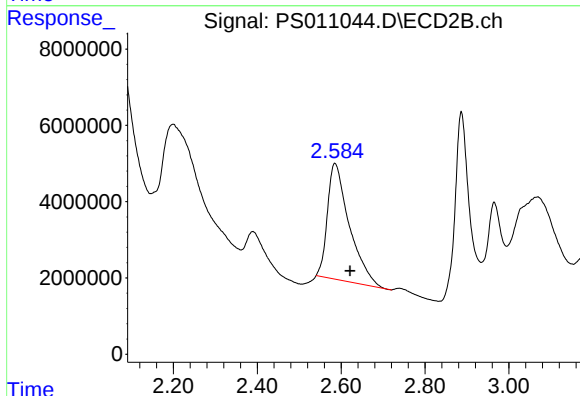


#1 Dalapon

R.T.: 2.585 min
Delta R.T.: -0.037 min
Response: 109938503
Conc: 145.74 ng/ml

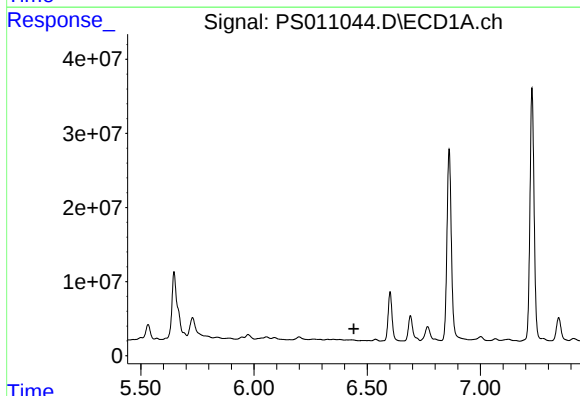


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.441 min
Response: 0
Conc: N.D.

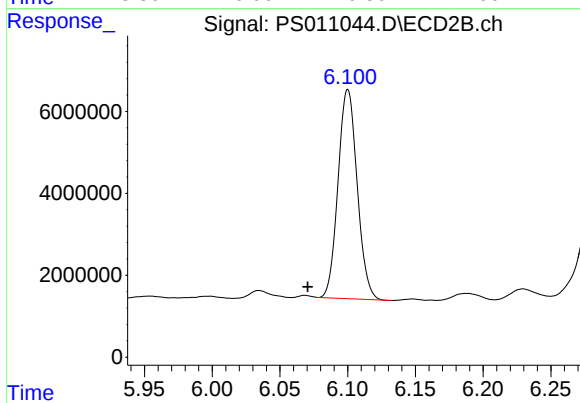

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.100 min
Delta R.T.: 0.030 min
Response: 50222053
Conc: 60.30 ng/ml

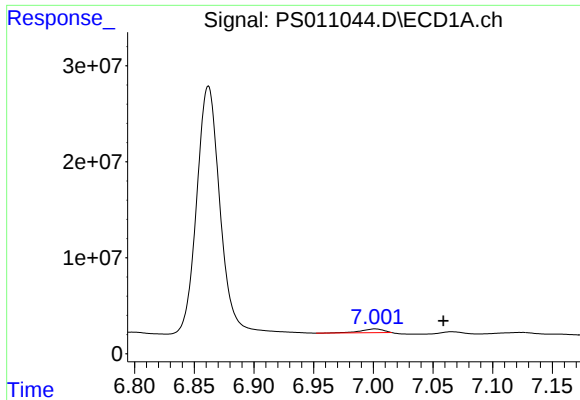

#3 4-Nitrophenol


R.T.: 7.001 min
Delta R.T.: -0.057 min
Response: 5130232
Conc: 12.85 ng/ml

Instrument :
ECD_S
ClientSampleId :

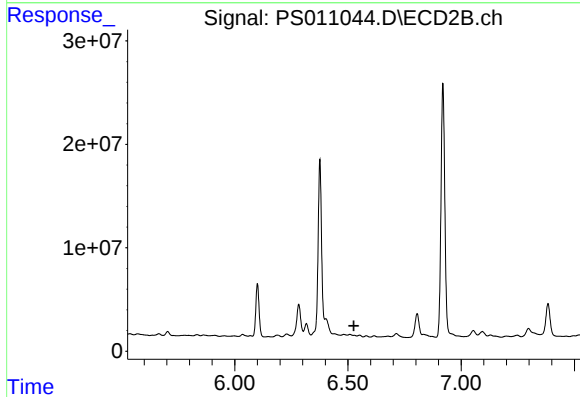


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.526 min
Response: 0
Conc: N.D.

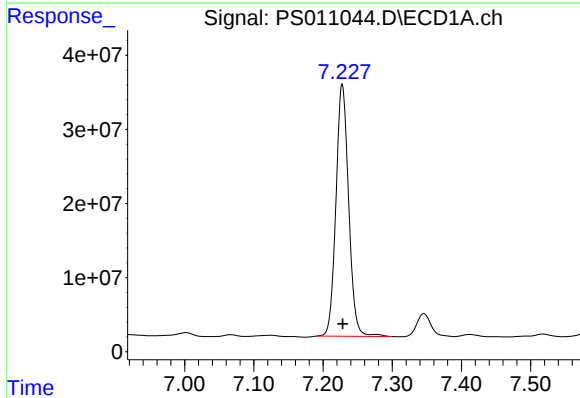


#4 2,4-DCAA

R.T.: 7.228 min
Delta R.T.: 0.000 min
Response: 434484565
Conc: 479.13 ng/ml

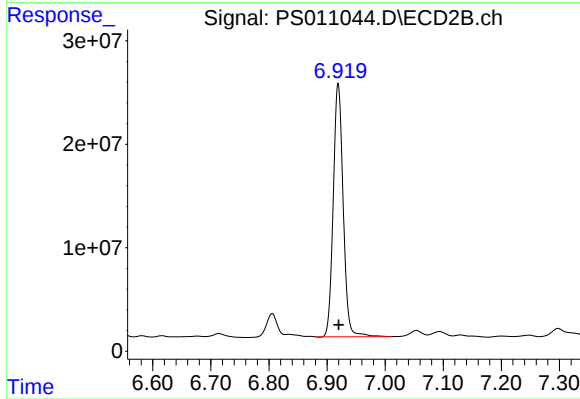

#4 2,4-DCAA


R.T.: 6.919 min
Delta R.T.: -0.001 min
Response: 291636678
Conc: 526.35 ng/ml

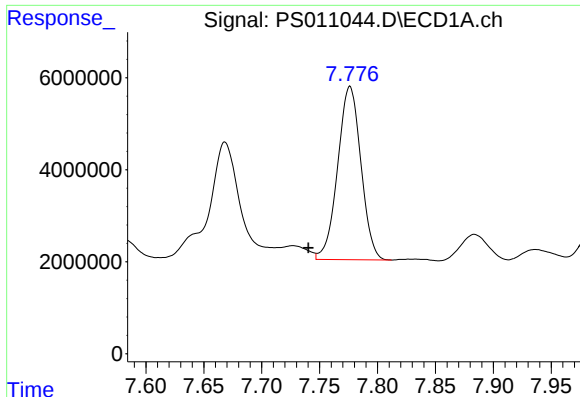

#7 MCPA


R.T.: 7.776 min
Delta R.T.: 0.036 min
Response: 52586842
Conc: 13.20 ug/ml

Instrument :
ECD_S
ClientSampleId :

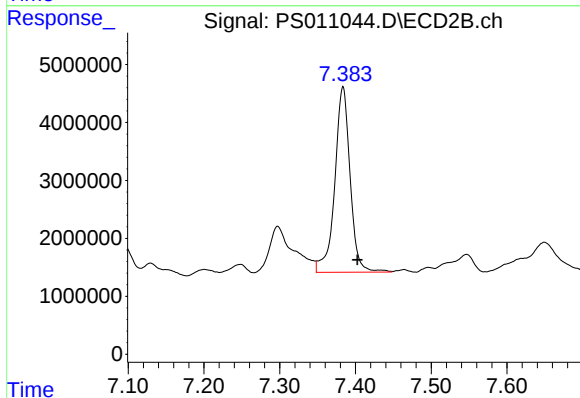


#7 MCPA

R.T.: 7.383 min
Delta R.T.: -0.019 min
Response: 45205747
Conc: 16.38 ug/ml

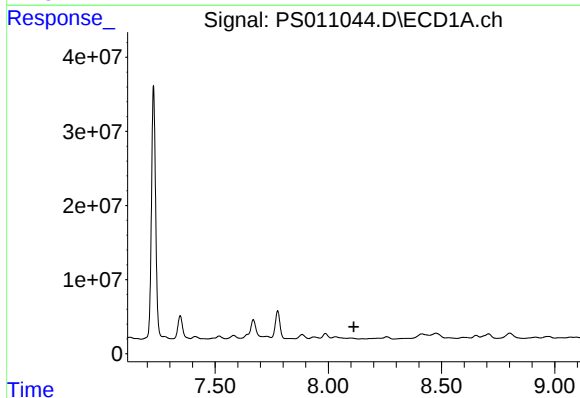


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.113 min
Response: 0
Conc: N.D.

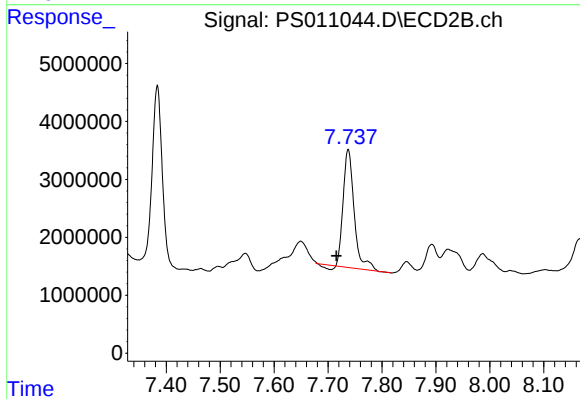

#8 DICHLORPROP


R.T.: 7.737 min
Delta R.T.: 0.022 min
Response: 28585167
Conc: 48.69 ng/ml

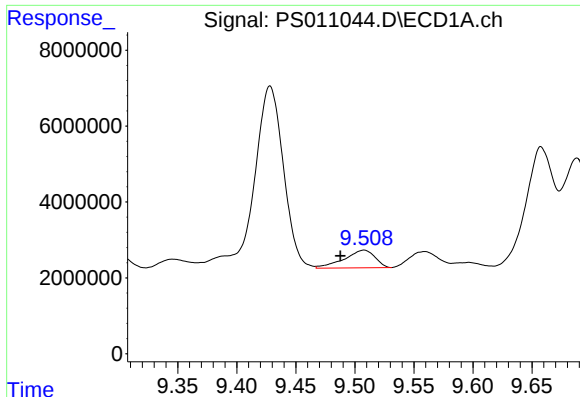

#12 2,4,5-T


R.T.: 9.507 min
Delta R.T.: 0.020 min
Response: 8422035
Conc: 1.81 ng/ml

Instrument :
ECD_S
ClientSampleId :

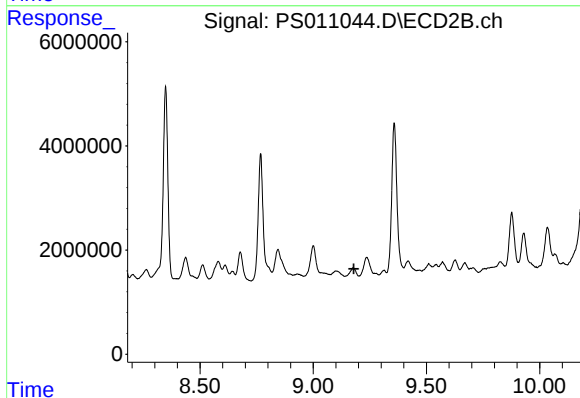


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.179 min
Response: 0
Conc: N.D.

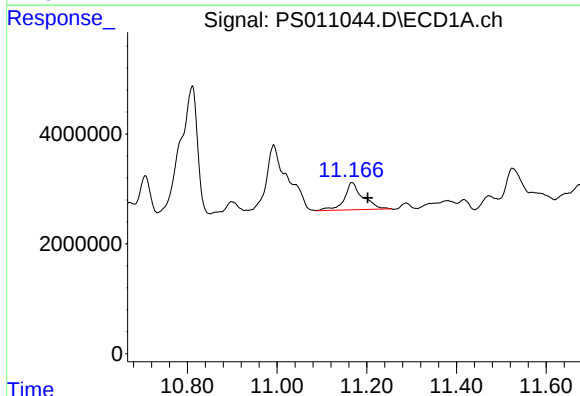


#14 DINOSEB

R.T.: 11.167 min
Delta R.T.: -0.035 min
Response: 14123962
Conc: 3.94 ng/ml

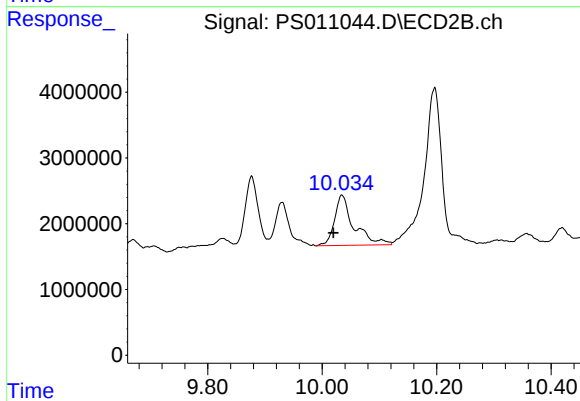

#14 DINOSEB


R.T.: 10.035 min
Delta R.T.: 0.015 min
Response: 18032764
Conc: 8.66 ng/ml

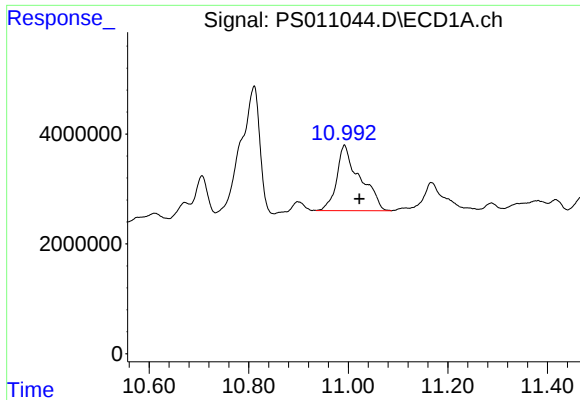

#15 Picloram


R.T.: 10.992 min
Delta R.T.: -0.030 min
Response: 38481508
Conc: 6.86 ng/ml

Instrument :
ECD_S
ClientSampleId :

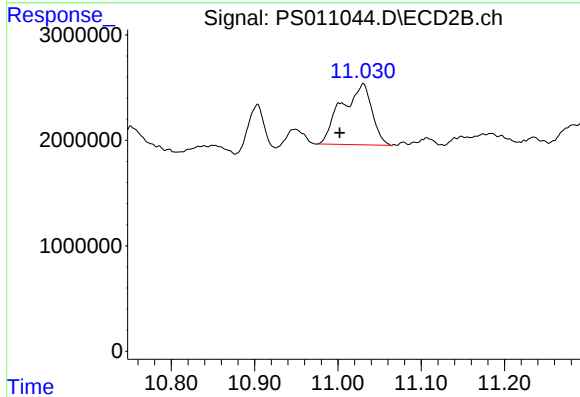


#15 Picloram

R.T.: 11.030 min
Delta R.T.: 0.028 min
Response: 14603203
Conc: 3.49 ng/ml

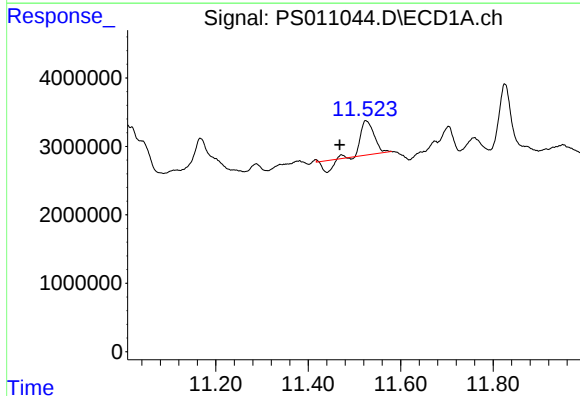

#16 DCPA

R.T.: 11.525 min
Delta R.T.: 0.057 min
Response: 7972369
Conc: 1.30 ng/ml

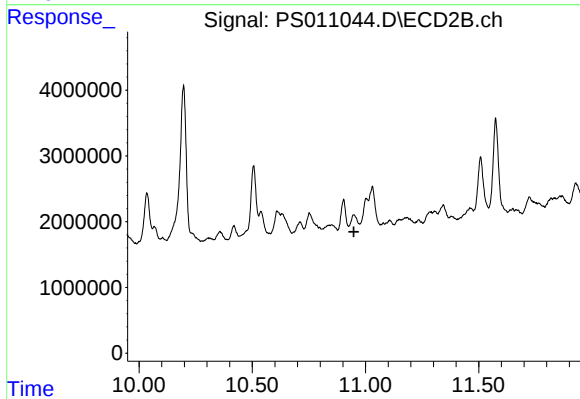

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 10.949 min
Response: 0
Conc: N.D.