

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070120\
 Data File : PS011047.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Jul 2020 23:02
 Operator : DD\AJ
 Sample : PB129913TB
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 02 05:07:36 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062420.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 25 02:45:12 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.228	6.920	397.0E6	285.9E6	437.771	515.985
Target Compounds							
1) T	Dalapon	2.996	2.585	38381354	108.4E6	34.278	143.707 #
2) T	3,5-DICHL...	0.000	6.100	0	88513000	N.D.	106.280
5) T	DICAMBA	7.409	0.000	7612014	0	2.088	N.D. #
6) T	MCP	7.640	0.000	3907785	0	1.370	N.D. #
10) T	Pentachlo...	8.709	0.000	8626430	0	<MDL	N.D. #
12) T	2,4,5-T	9.425	0.000	33664570	0	7.227	N.D. #
14) T	DINOSEB	0.000	10.065	0	18104852	N.D.	8.695
15) T	Picloram	10.998	0.000	16881486	0	3.011	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070120\
Data File : PS011047.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Jul 2020 23:02
Operator : DD\AJ
Sample : PB129913TB
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 02 05:07:36 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062420.M
Quant Title : 8080.M
QLast Update : Thu Jun 25 02:45:12 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

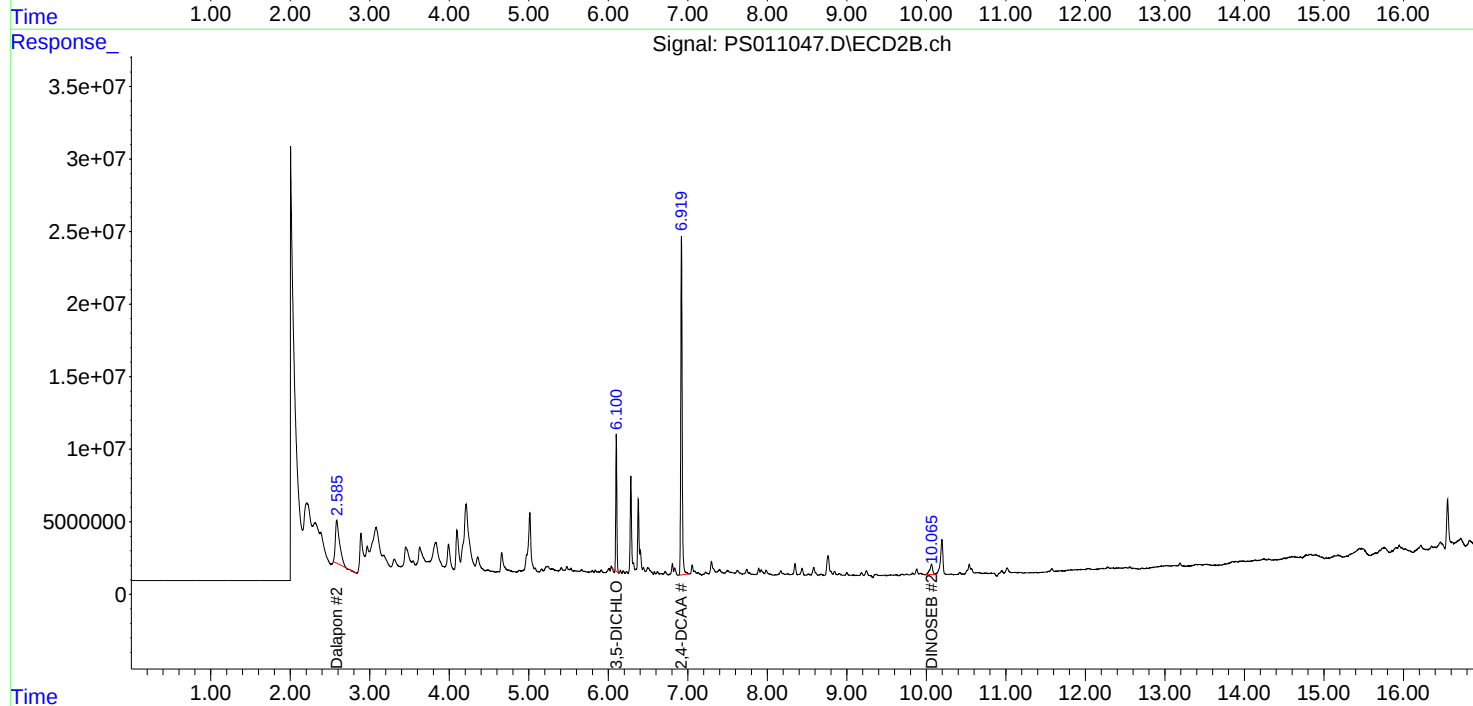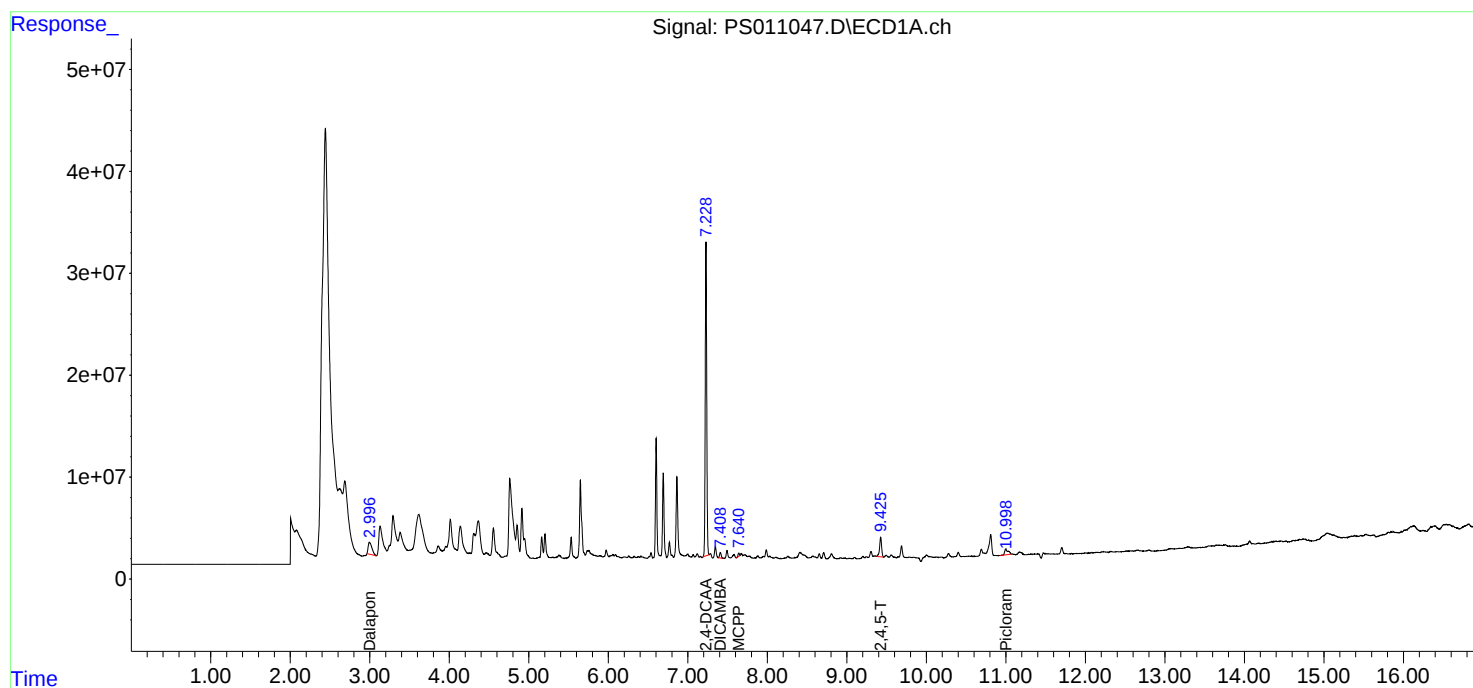


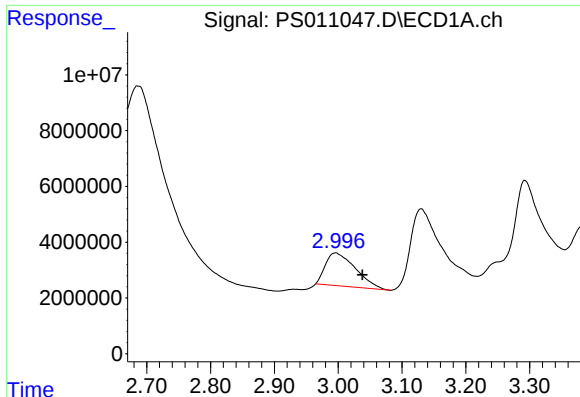

#1 Dalapon


R.T.: 2.996 min
Delta R.T.: -0.042 min
Response: 38381354
Conc: 34.28 ng/ml

Instrument :
ECD_S
ClientSampleId :

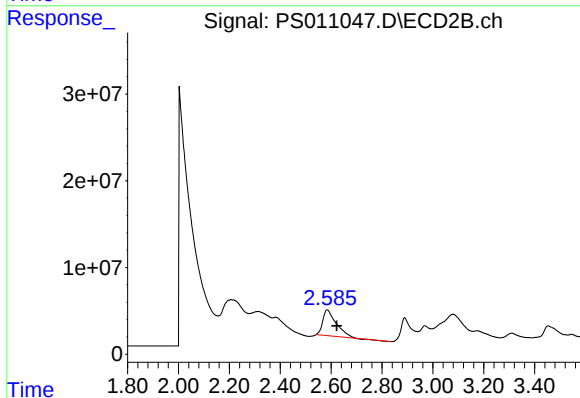


#1 Dalapon

R.T.: 2.585 min
Delta R.T.: -0.037 min
Response: 108406608
Conc: 143.71 ng/ml

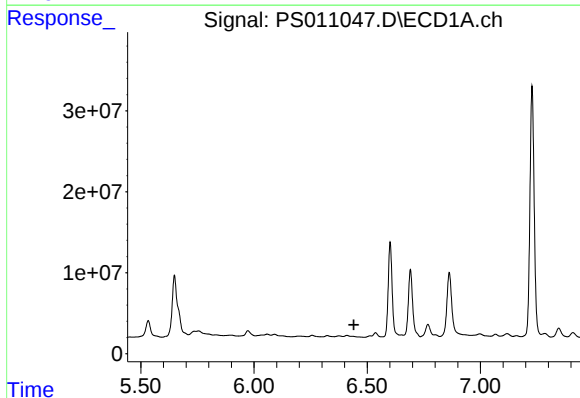


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.441 min
Response: 0
Conc: N.D.

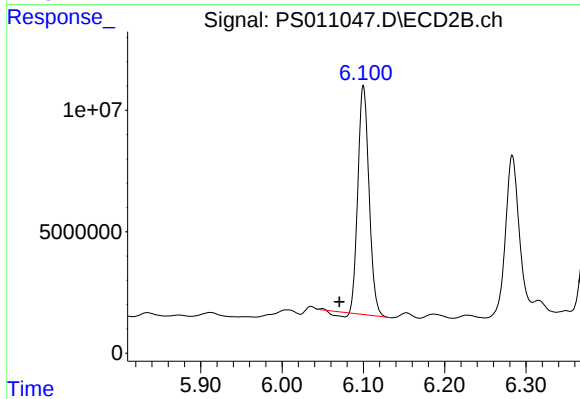

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.100 min
Delta R.T.: 0.030 min
Response: 88513000
Conc: 106.28 ng/ml

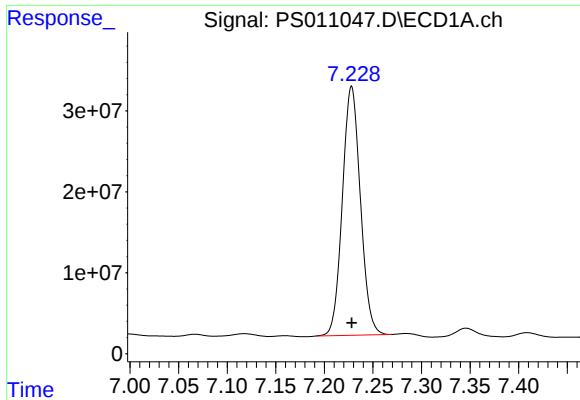

#4 2,4-DCAA


R.T.: 7.228 min
Delta R.T.: 0.000 min
Response: 396978615
Conc: 437.77 ng/ml

Instrument :
ECD_S
ClientSampleId :

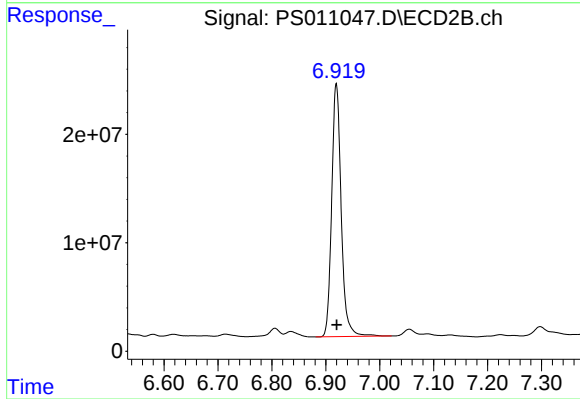


#4 2,4-DCAA

R.T.: 6.920 min
Delta R.T.: 0.000 min
Response: 285894850
Conc: 515.98 ng/ml

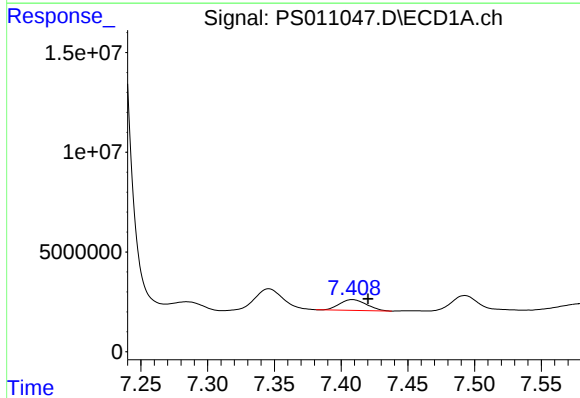


#5 DICAMBA

R.T.: 7.409 min
Delta R.T.: -0.012 min
Response: 7612014
Conc: 2.09 ng/ml

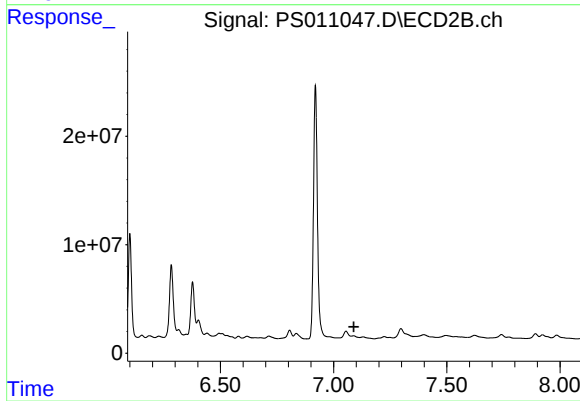

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 7.089 min
Response: 0
Conc: N.D.

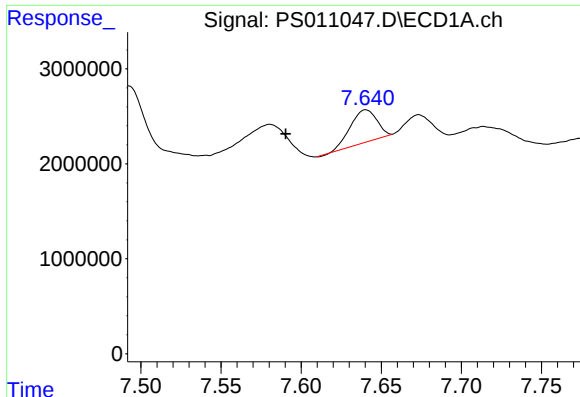

#6 MCP


R.T.: 7.640 min
Delta R.T.: 0.050 min
Response: 3907785
Conc: 1.37 ug/ml

Instrument :
ECD_S
ClientSampleId :

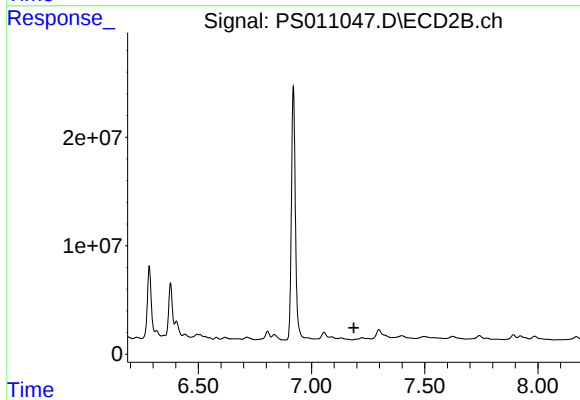


#6 MCP

R.T.: 0.000 min
Exp R.T. : 7.187 min
Response: 0
Conc: N.D.

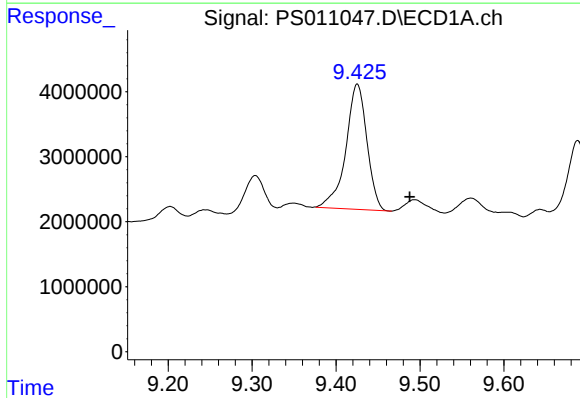


#12 2,4,5-T

R.T.: 9.425 min
Delta R.T.: -0.062 min
Response: 33664570
Conc: 7.23 ng/ml

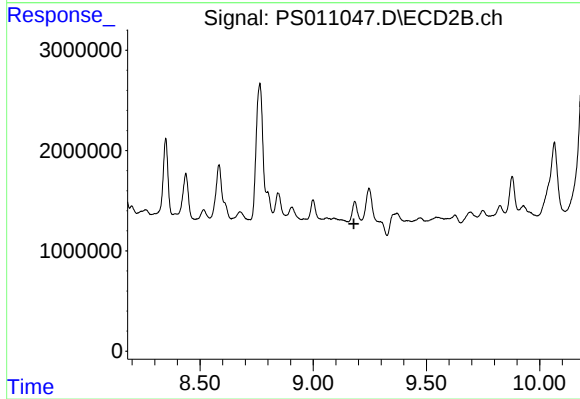

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 9.179 min
Response: 0
Conc: N.D.

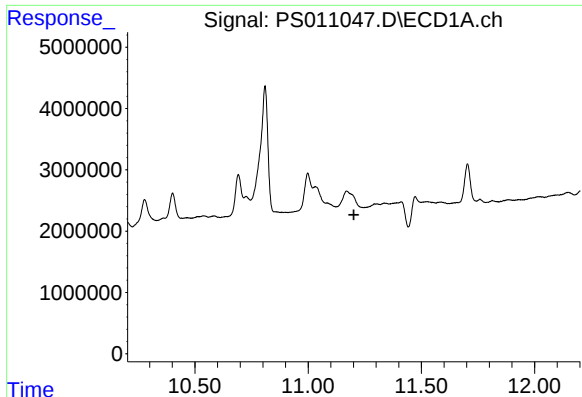

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 11.202 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

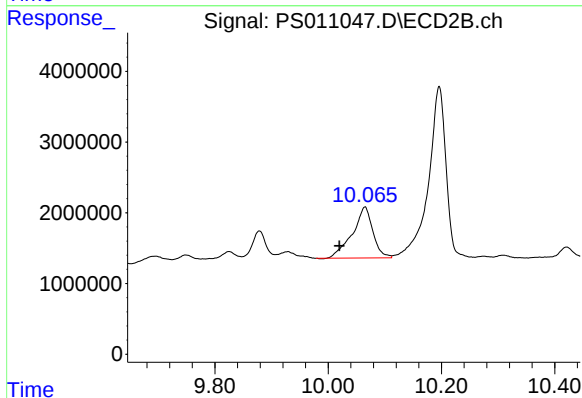


#14 DINOSEB

R.T.: 10.065 min
Delta R.T.: 0.045 min
Response: 18104852
Conc: 8.70 ng/ml

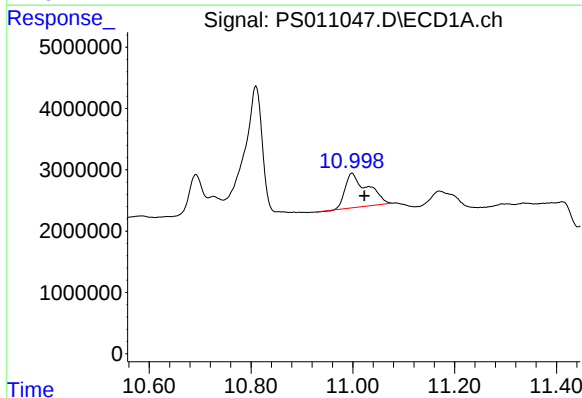

#15 Picloram

R.T.: 10.998 min
Delta R.T.: -0.024 min
Response: 16881486
Conc: 3.01 ng/ml

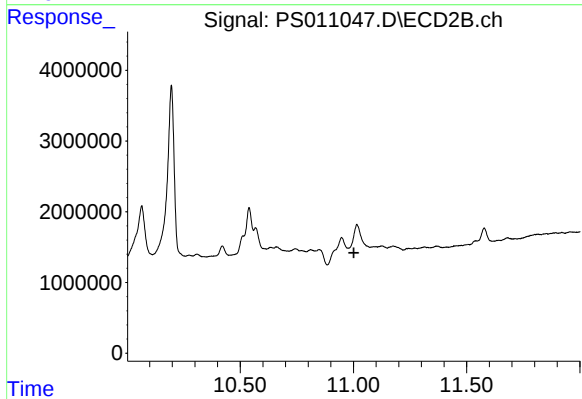

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 11.002 min
Response: 0
Conc: N.D.