

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070120\
 Data File : PS011050.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jul 2020 00:11
 Operator : DD\AJ
 Sample : L2815-20
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 OR-03-062920

Manual Integrations
 APPROVED

Ankita
 7/2/2020 10:08:28 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 02 07:09:38 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062420.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 25 02:45:12 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.228	6.920	294.0E6	203.7E6	324.202m	367.556

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070120\
Data File : PS011050.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jul 2020 00:11
Operator : DD\AJ
Sample : L2815-20
Misc :
ALS Vial : 31 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
OR-03-062920


Manual Integrations
APPROVED

Ankita
7/2/2020 10:08:28 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 02 07:09:38 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062420.M
Quant Title : 8080.M
QLast Update : Thu Jun 25 02:45:12 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

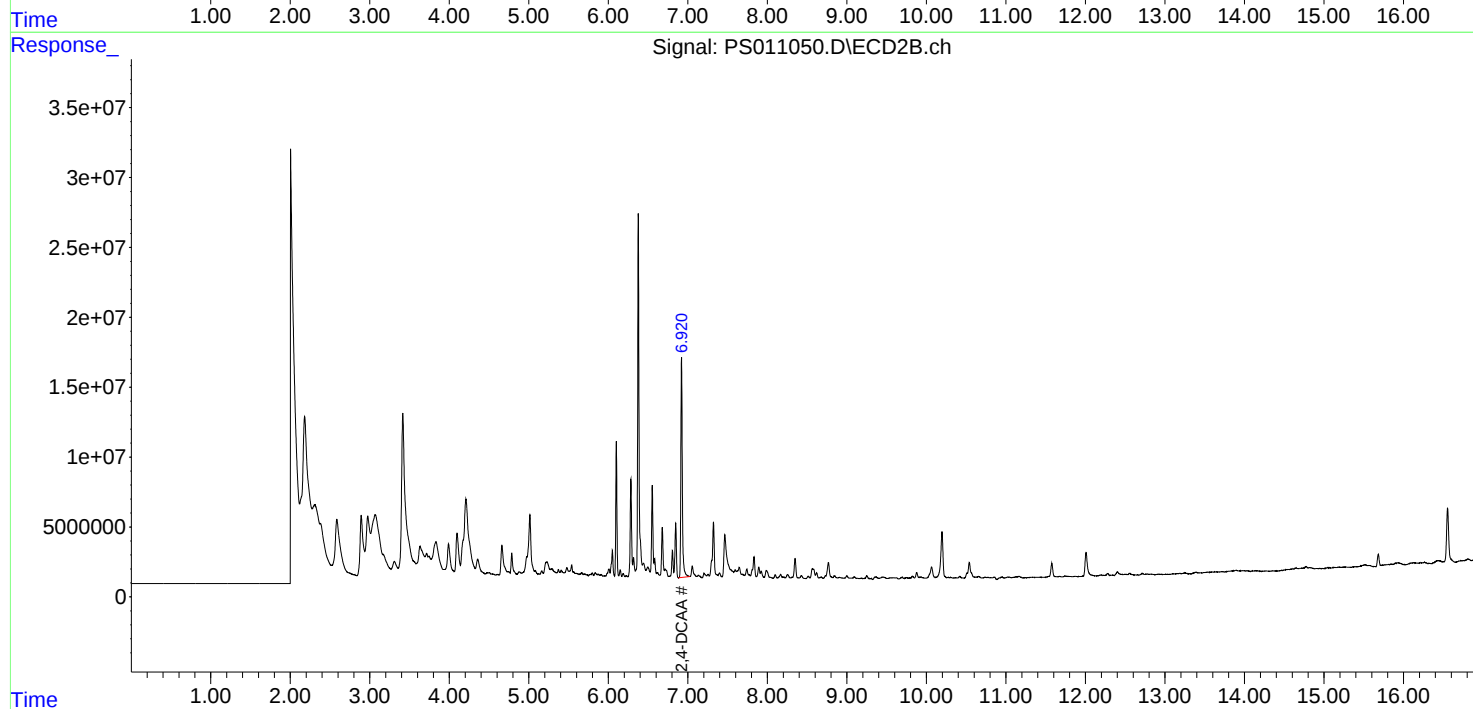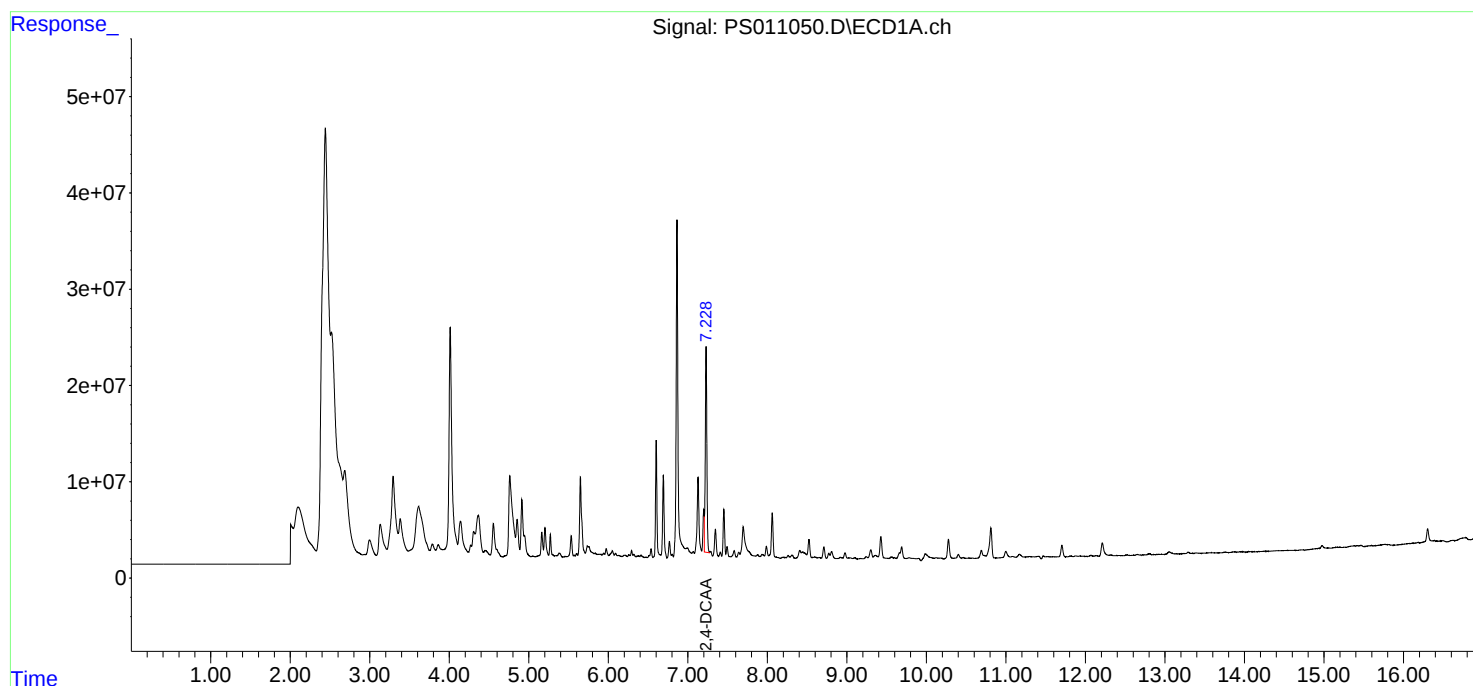

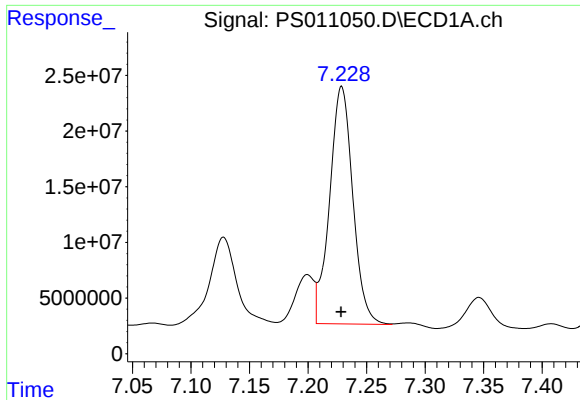


#4 2,4-DCAA

R.T.: 7.228 min
Delta R.T.: 0.000 min
Response: 293992282
Conc: 324.20 ng/ml m

Instrument :
ECD_S
ClientSampleId :
OR-03-062920

Manual Integrations
APPROVED

Ankita
7/2/2020 10:08:28 AM

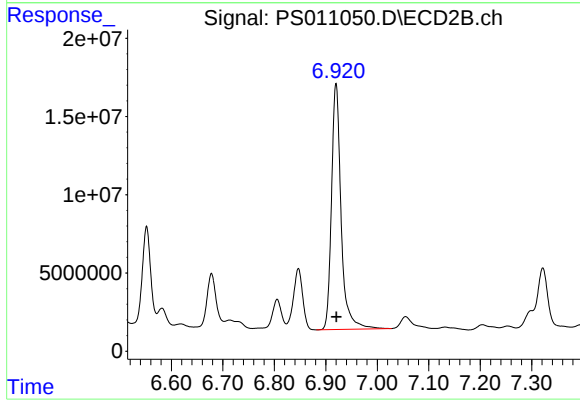

#4 2,4-DCAA

R.T.: 6.920 min
Delta R.T.: 0.000 min
Response: 203654209
Conc: 367.56 ng/ml