

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070218\
 Data File : PS000714.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jul 2018 10:46
 Operator : UA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 02 17:11:34 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061718.M
 Quant Title : 8080.M
 QLast Update : Mon Jun 18 00:27:44 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	0.000	11.204	0	24530	N.D.	0.072 #
Target Compounds							
1) T	Dalapon	0.000	2.561	0	411886	N.D.	0.945 #
2) T	3,5-DICHL...	10.292	9.339	248948	46343	0.461	0.101 #
3) T	4-Nitroph...	0.000	10.335	0	86078	N.D.	0.439 #
5) T	DICAMBA	0.000	11.494	0	119169	N.D.	0.096 #
6) T	MCP	0.000	11.719	0	52496	N.D.	0.055 #
7) T	MCPA	0.000	12.088	0	37460	N.D.	0.027 #
8) T	DICHLORPROP	0.000	12.610	0	174506	N.D.	0.542 #
9) T	2,4-D	0.000	13.123	0	38692	N.D.	0.091 #
12) T	2,4,5-T	15.343	14.847	670352	97533	0.311	0.058 #
15) T	Picloram	17.384	17.099	599478	196582	0.205	0.079 #
16) T	DCPA	17.959	17.099	631153	196582	0.246	0.085 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070218\
Data File : PS000714.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jul 2018 10:46
Operator : UA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 02 17:11:34 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061718.M
Quant Title : 8080.M
QLast Update : Mon Jun 18 00:27:44 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

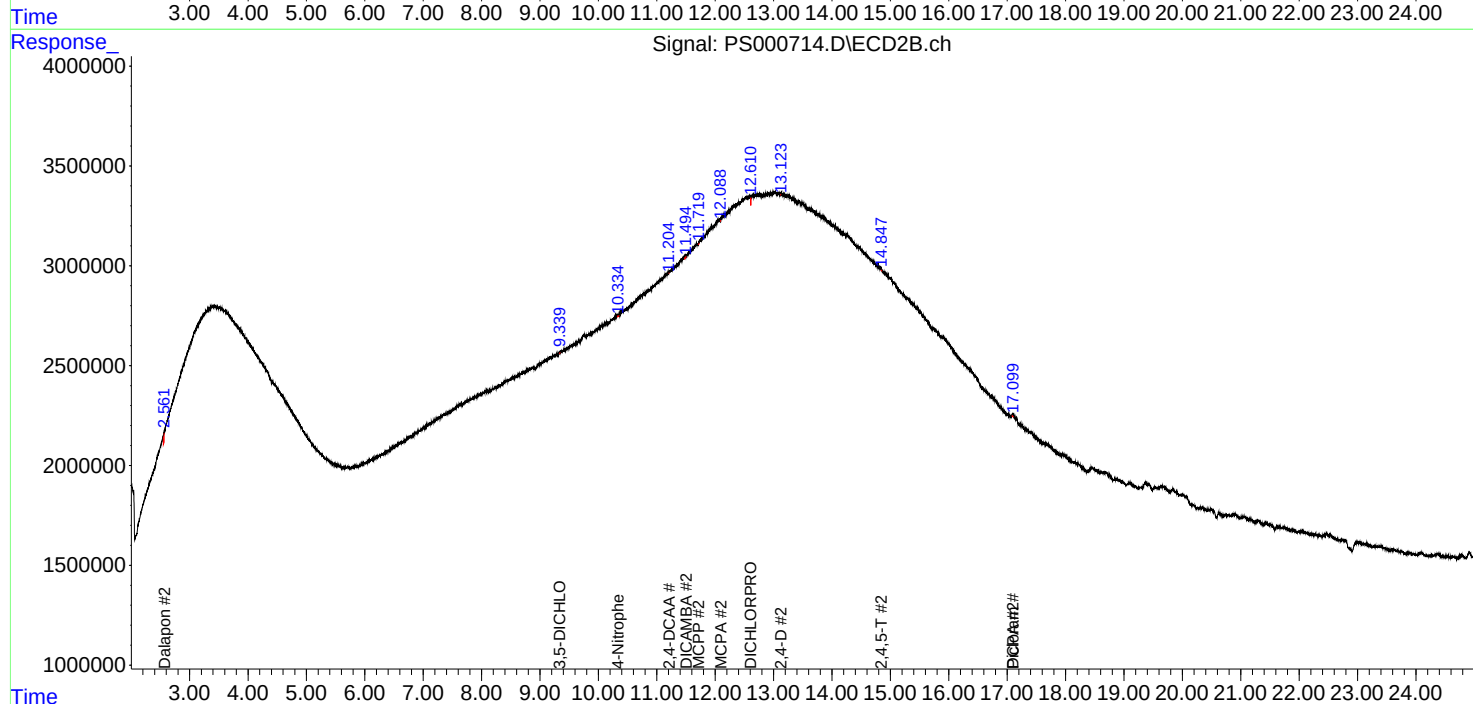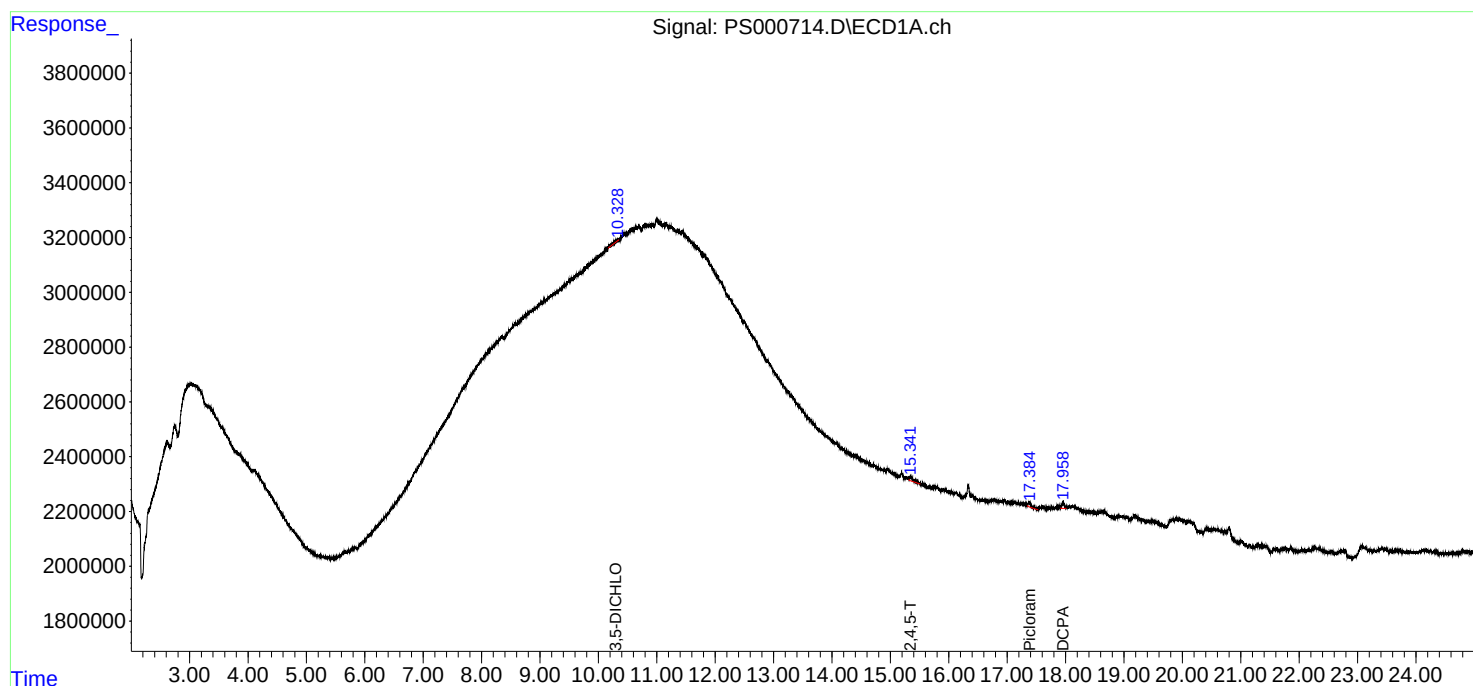


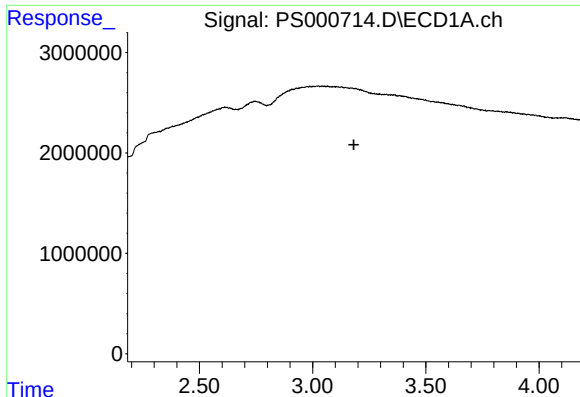

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 3.182 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

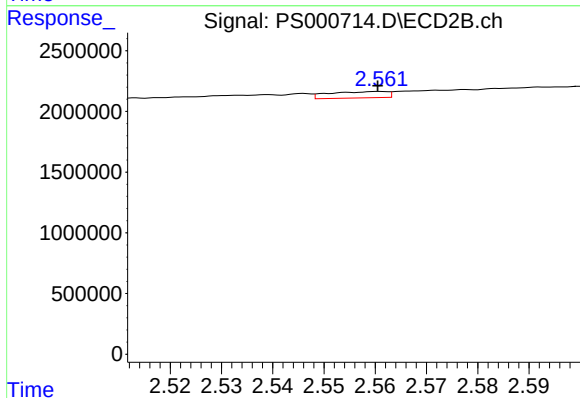


#1 Dalapon

R.T.: 2.561 min
Delta R.T.: 0.000 min
Response: 411886
Conc: 0.94 ng/ml

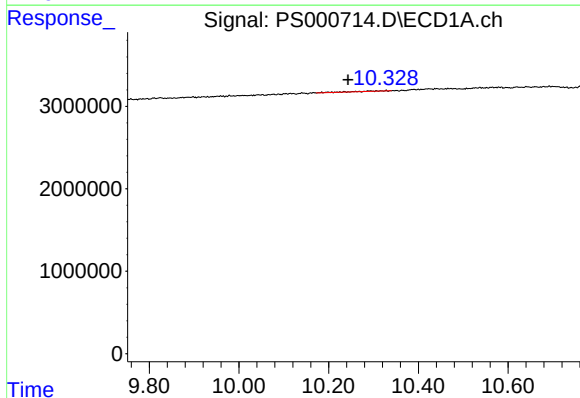


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 10.292 min
Delta R.T.: 0.048 min
Response: 248948
Conc: 0.46 ng/ml

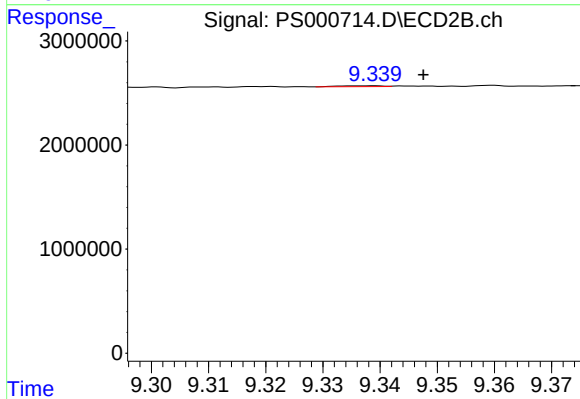

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.339 min
Delta R.T.: -0.009 min
Response: 46343
Conc: 0.10 ng/ml

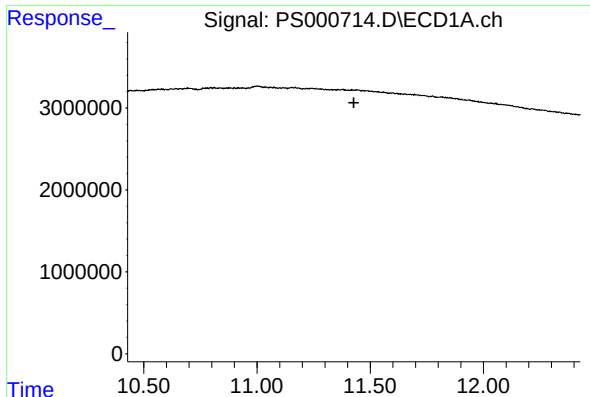

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 11.428 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

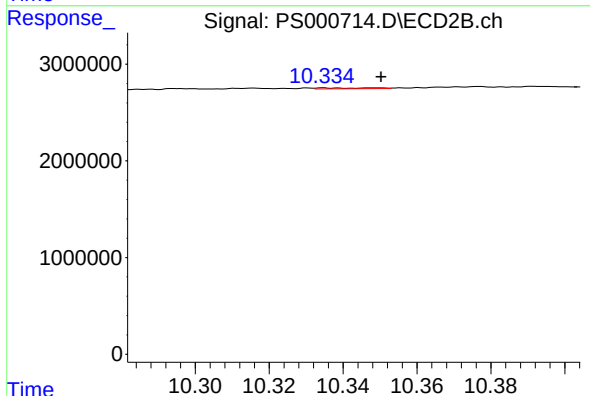


#3 4-Nitrophenol

R.T.: 10.335 min
Delta R.T.: -0.016 min
Response: 86078
Conc: 0.44 ng/ml

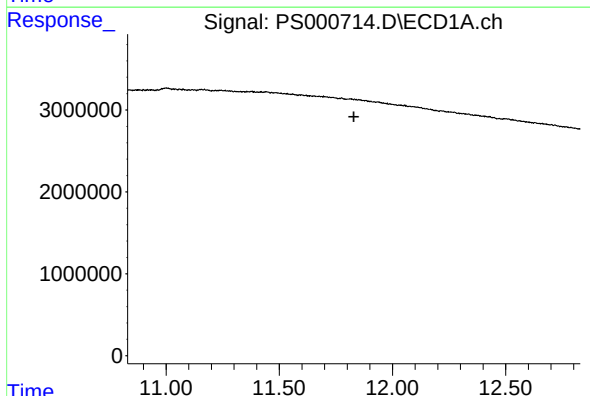


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 11.829 min
Response: 0
Conc: N.D.

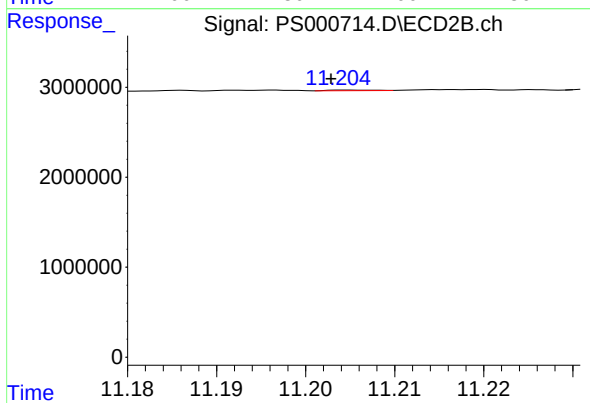

#4 2,4-DCAA


R.T.: 11.204 min
Delta R.T.: 0.002 min
Response: 24530
Conc: 0.07 ng/ml

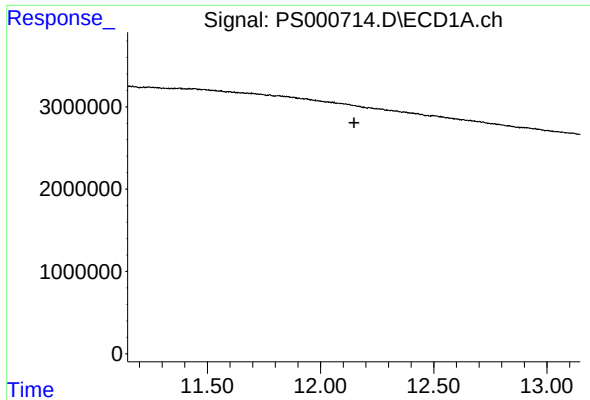

#5 DICAMBA


R.T.: 0.000 min
Exp R.T. : 12.147 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

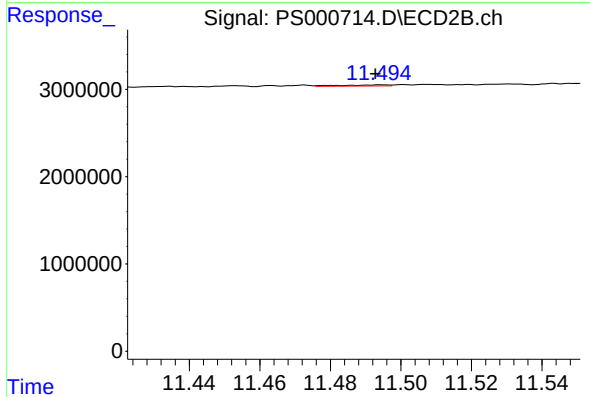


#5 DICAMBA

R.T.: 11.494 min
Delta R.T.: 0.002 min
Response: 119169
Conc: 0.10 ng/ml

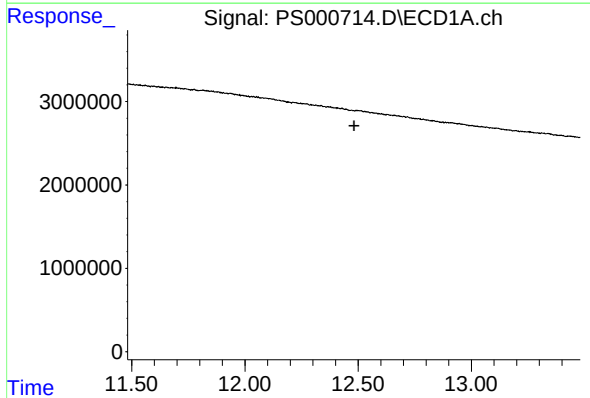


#6 MCP

R.T.: 0.000 min
Exp R.T. : 12.482 min
Response: 0
Conc: N.D.

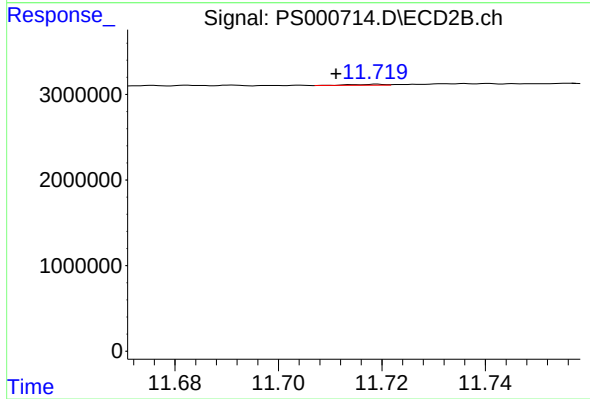

#6 MCP


R.T.: 11.719 min
Delta R.T.: 0.008 min
Response: 52496
Conc: 0.05 ug/ml

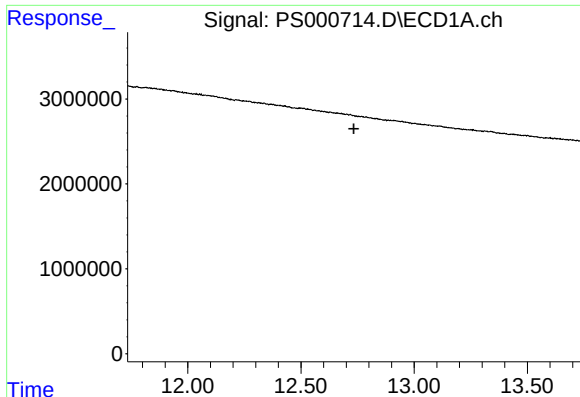

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 12.733 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

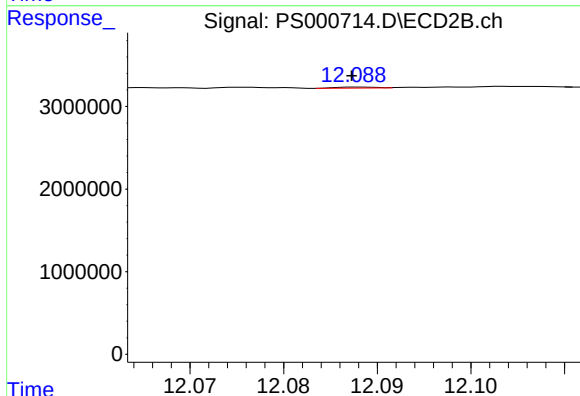


#7 MCPA

R.T.: 12.088 min
Delta R.T.: 0.000 min
Response: 37460
Conc: 0.03 ug/ml

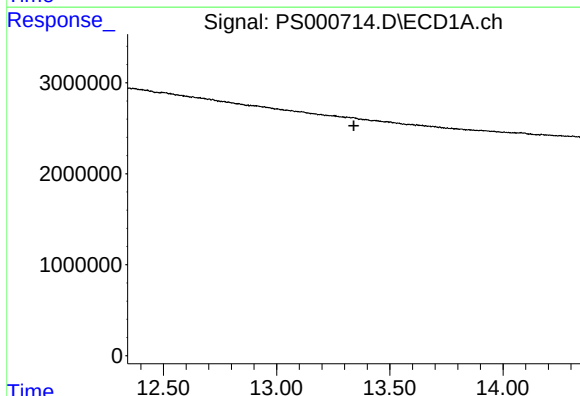


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 13.341 min
Response: 0
Conc: N.D.

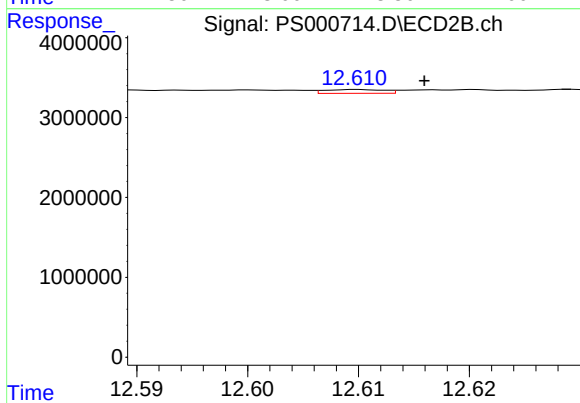

#8 DICHLORPROP


R.T.: 12.610 min
Delta R.T.: -0.006 min
Response: 174506
Conc: 0.54 ng/ml

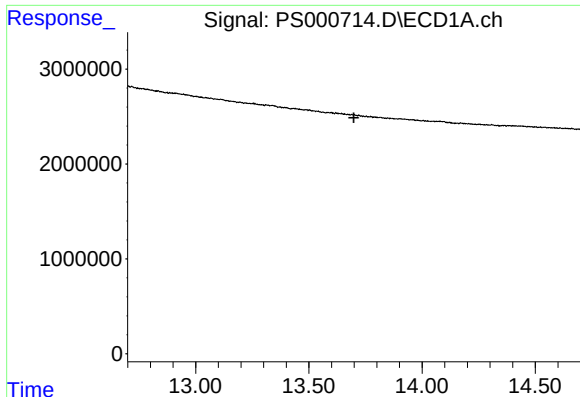

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.699 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

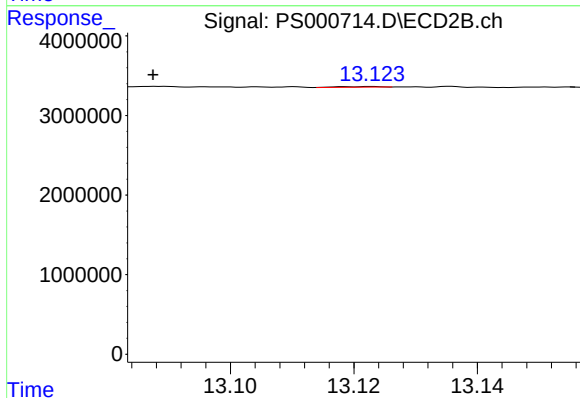


#9 2,4-D

R.T.: 13.123 min
Delta R.T.: 0.036 min
Response: 38692
Conc: 0.09 ng/ml

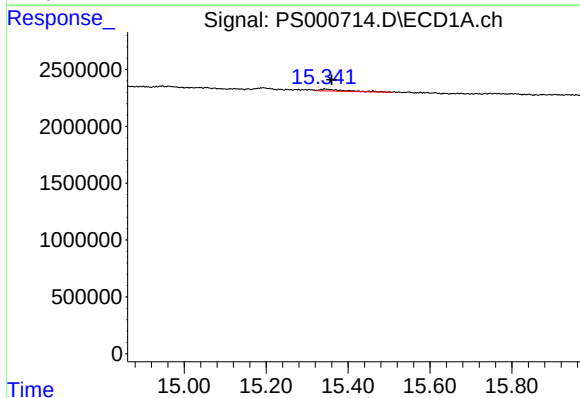


#12 2,4,5-T

R.T.: 15.343 min
Delta R.T.: -0.017 min
Response: 670352
Conc: 0.31 ng/ml

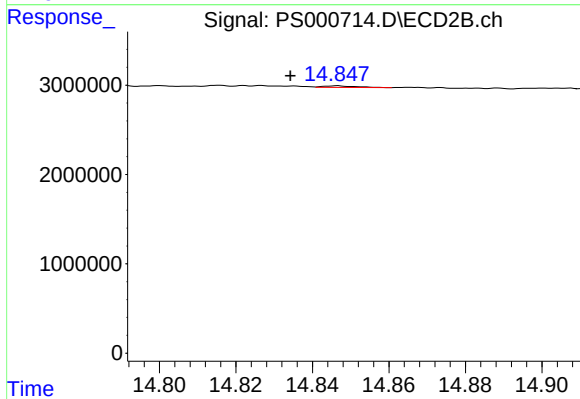

#12 2,4,5-T


R.T.: 14.847 min
Delta R.T.: 0.012 min
Response: 97533
Conc: 0.06 ng/ml

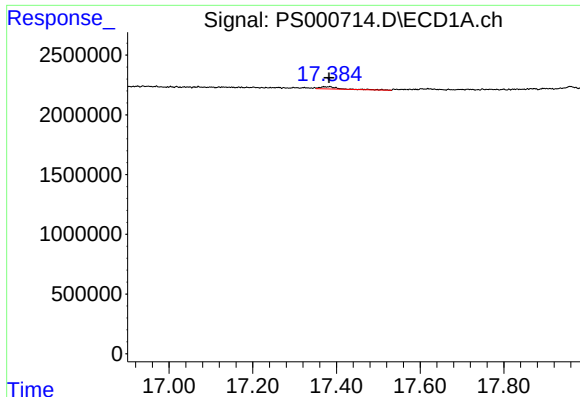

#15 Picloram


R.T.: 17.384 min
Delta R.T.: 0.002 min
Response: 599478
Conc: 0.21 ng/ml

Instrument :
ECD_S
ClientSampleId :

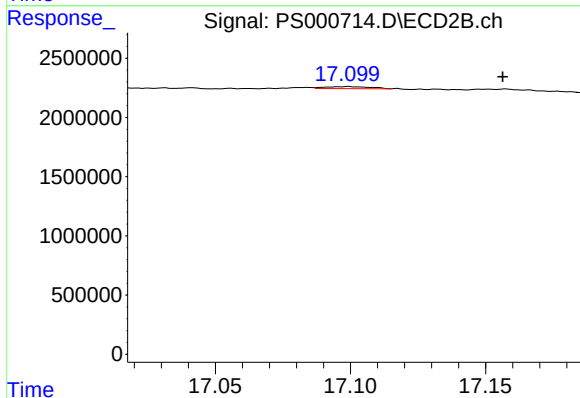


#15 Picloram

R.T.: 17.099 min
Delta R.T.: -0.057 min
Response: 196582
Conc: 0.08 ng/ml

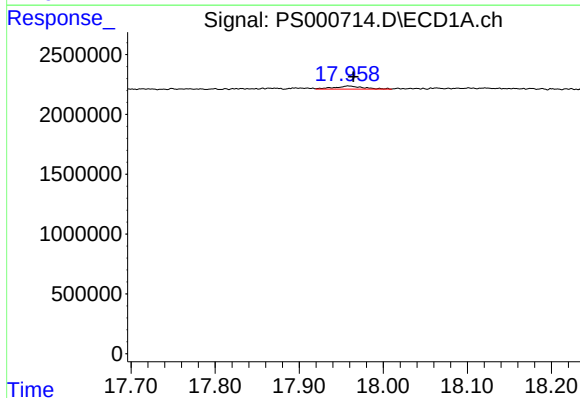

#16 DCPA

R.T.: 17.959 min
Delta R.T.: -0.006 min
Response: 631153
Conc: 0.25 ng/ml

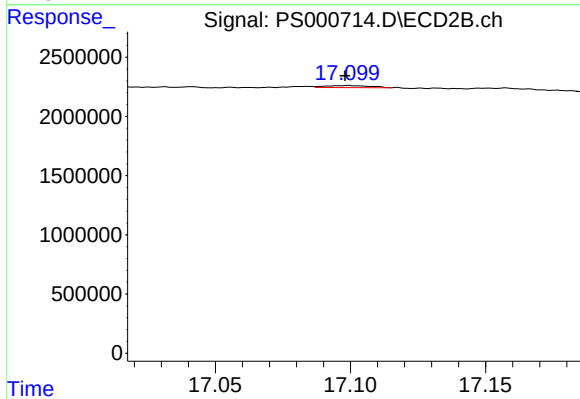

#16 DCPA

R.T.: 17.099 min
Delta R.T.: 0.001 min
Response: 196582
Conc: 0.09 ng/ml