

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070218\
 Data File : PS000725.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jul 2018 18:48
 Operator : UA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 03 01:48:26 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061718.M
 Quant Title : 8080.M
 QLast Update : Mon Jun 18 00:27:44 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.826	11.209	187.7E6	151.3E6	498.424	444.740
Target Compounds							
1) T	Dalapon	0.000	2.563	0	22779	N.D.	0.052 #
3) T	4-Nitroph...	11.449	0.000	641447	0	2.729	N.D. #
6) T	MCP	12.518	0.000	549040	0	0.485	N.D. #
8) T	DICHLORPROP	13.338	0.000	480536	0	1.277	N.D. #
10) T	Pentachlo...	14.095	13.656	380224	70780	0.072	0.015 #
11) T	2,4,5-TP ...	14.957	14.259	754335	126395	0.347	0.065 #
12) T	2,4,5-T	15.365	14.844	2510296	242850	1.166	0.144 #
14) T	DINOSEB	17.607	0.000	627802	0	0.422	N.D. #
15) T	Picloram	17.390	17.170	1283317	785467	0.439	0.315 #
16) T	DCPA	17.954	0.000	186400	0	0.073	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070218\
Data File : PS000725.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jul 2018 18:48
Operator : UA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 03 01:48:26 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061718.M
Quant Title : 8080.M
QLast Update : Mon Jun 18 00:27:44 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

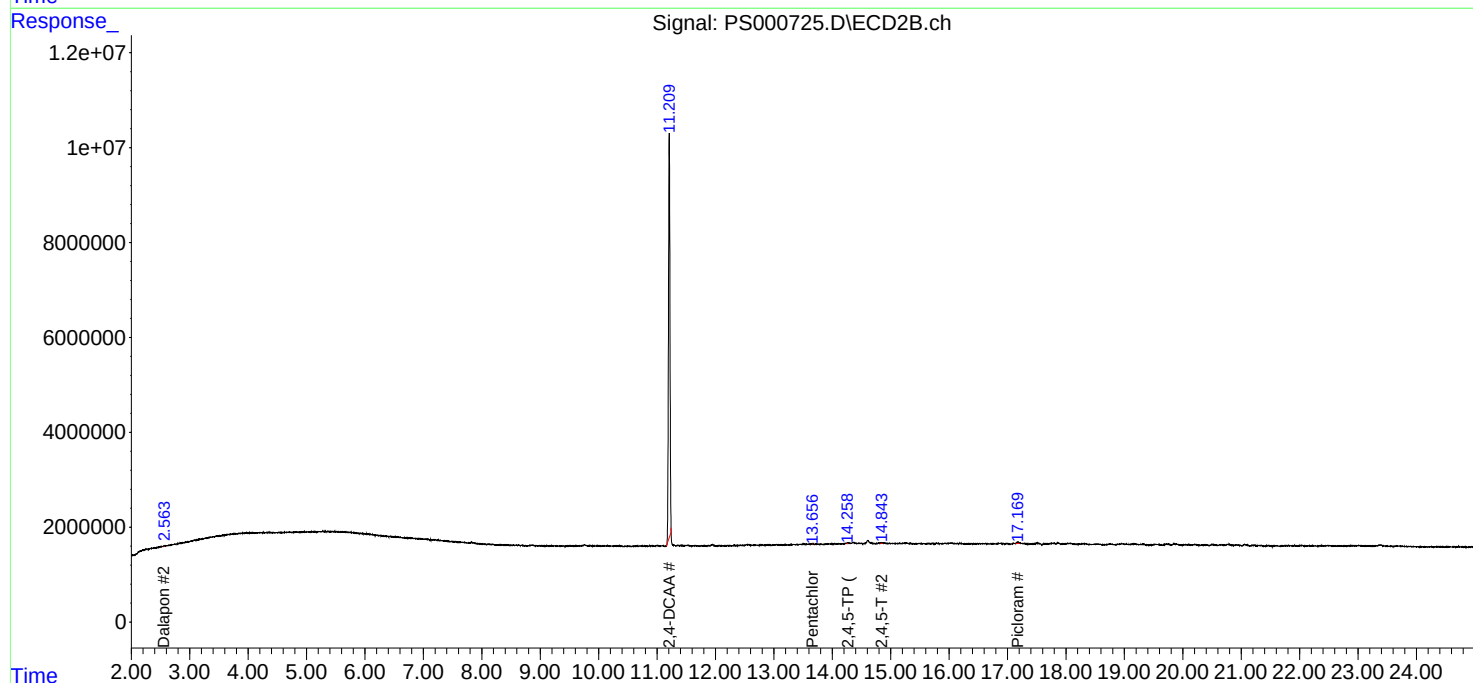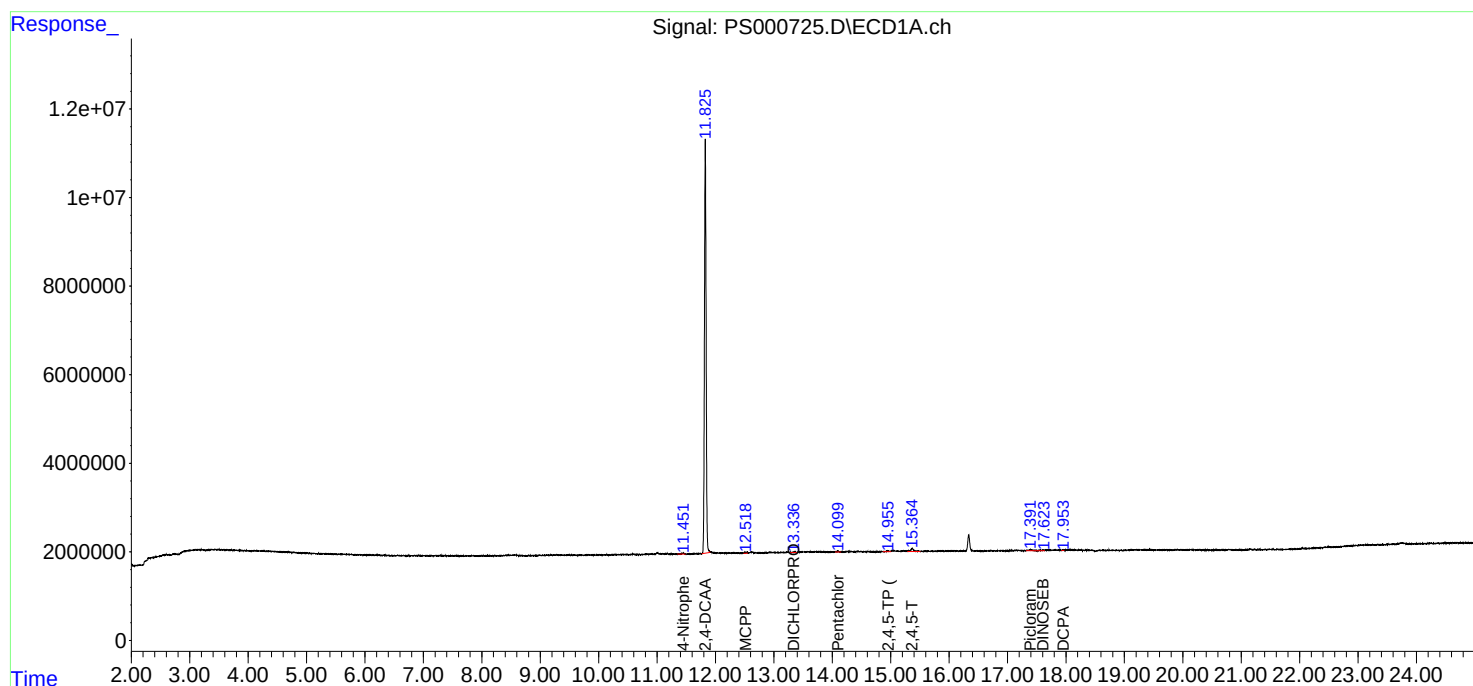


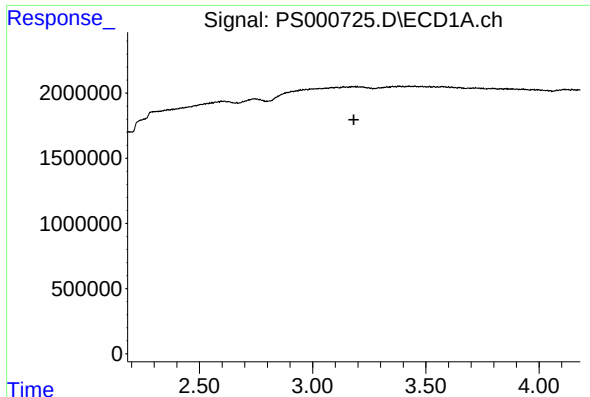

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 3.182 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

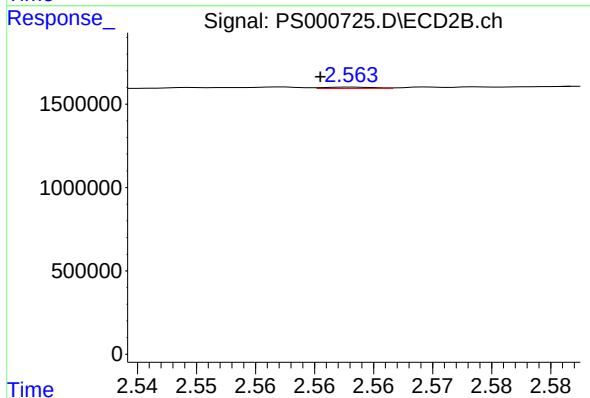


#1 Dalapon

R.T.: 2.563 min
Delta R.T.: 0.003 min
Response: 22779
Conc: 0.05 ng/ml

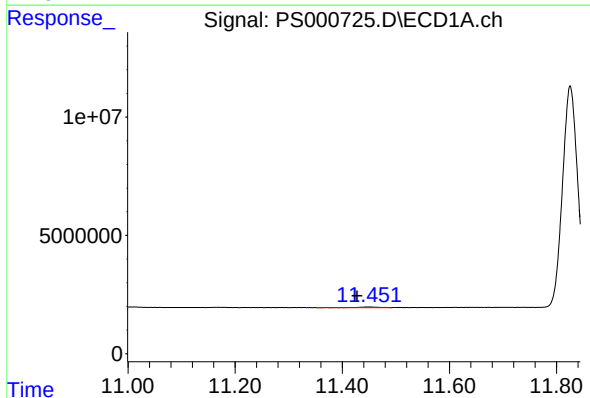


#3 4-Nitrophenol

R.T.: 11.449 min
Delta R.T.: 0.022 min
Response: 641447
Conc: 2.73 ng/ml

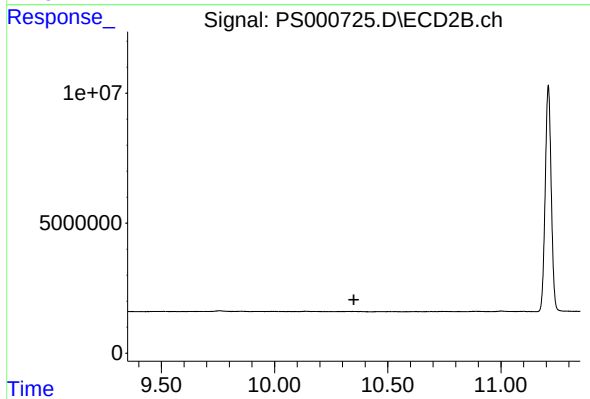

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.350 min
Response: 0
Conc: N.D.

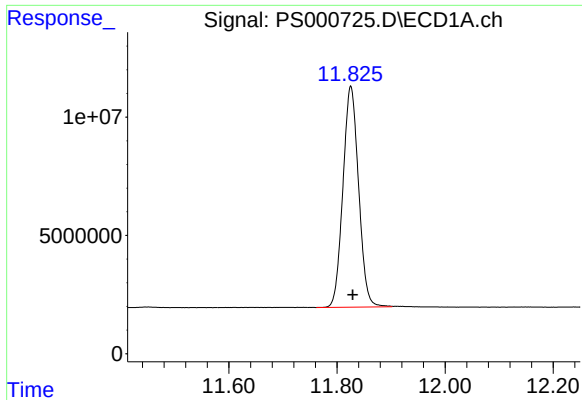

#4 2,4-DCAA


R.T.: 11.826 min
Delta R.T.: -0.004 min
Response: 187733659
Conc: 498.42 ng/ml

Instrument :
ECD_S
ClientSampleId :

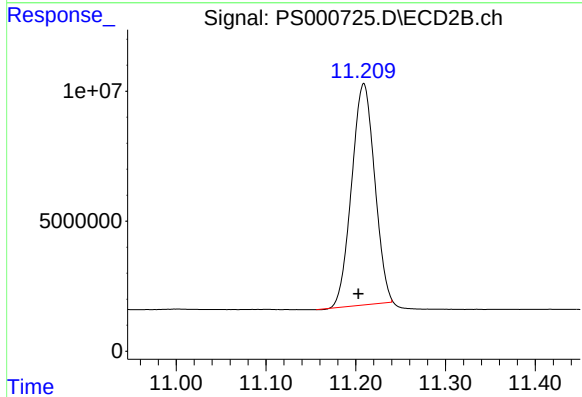


#4 2,4-DCAA

R.T.: 11.209 min
Delta R.T.: 0.006 min
Response: 151348865
Conc: 444.74 ng/ml

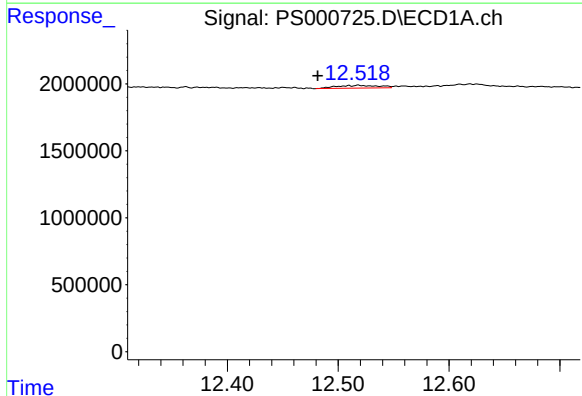


#6 MCP

R.T.: 12.518 min
Delta R.T.: 0.036 min
Response: 549040
Conc: 0.48 ug/ml

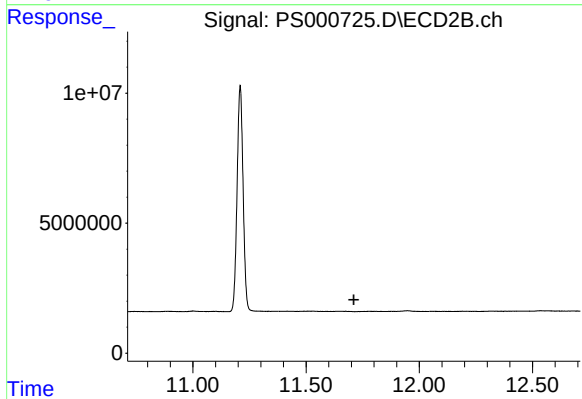

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.711 min
Response: 0
Conc: N.D.

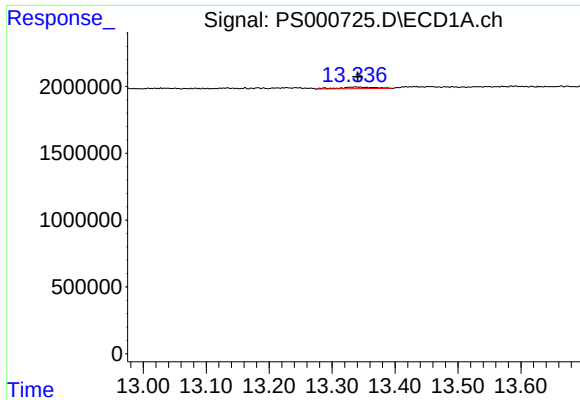

#8 DICHLORPROP


R.T.: 13.338 min
Delta R.T.: -0.002 min
Response: 480536
Conc: 1.28 ng/ml

Instrument :
ECD_S
ClientSampleId :

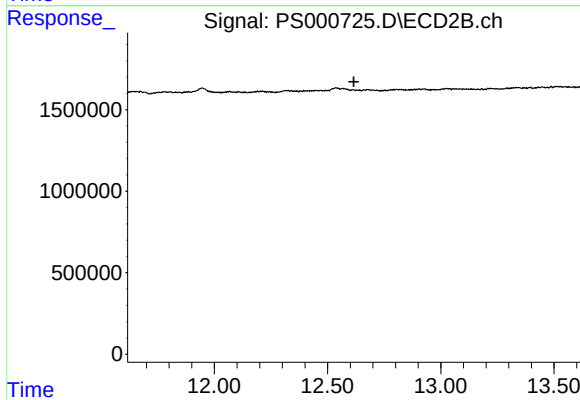


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 12.616 min
Response: 0
Conc: N.D.

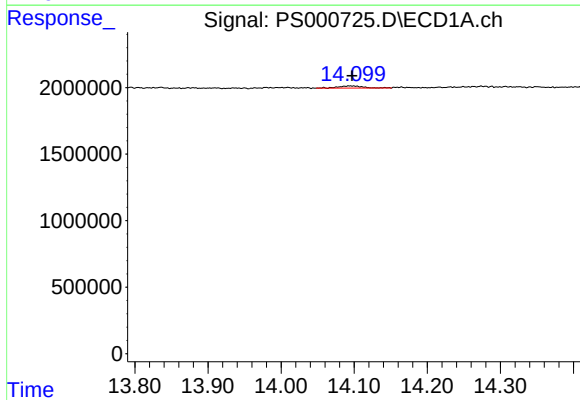


#10 Pentachlorophenol

R.T.: 14.095 min
Delta R.T.: -0.002 min
Response: 380224
Conc: 0.07 ng/ml

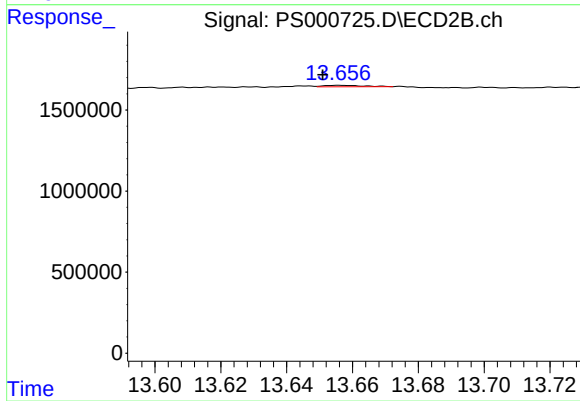

#10 Pentachlorophenol


R.T.: 13.656 min
Delta R.T.: 0.005 min
Response: 70780
Conc: 0.01 ng/ml

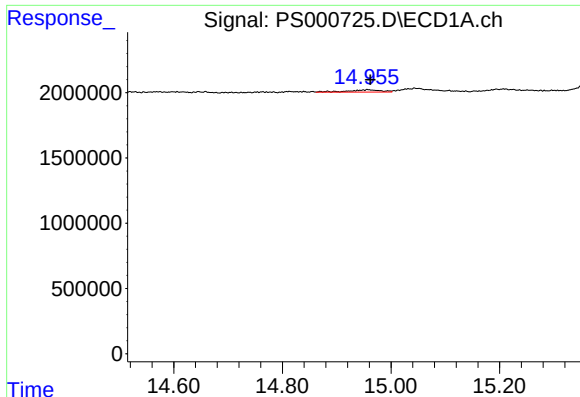

#11 2,4,5-TP (SILVEX)


R.T.: 14.957 min
Delta R.T.: -0.005 min
Response: 754335
Conc: 0.35 ng/ml

Instrument :
ECD_S
ClientSampleId :

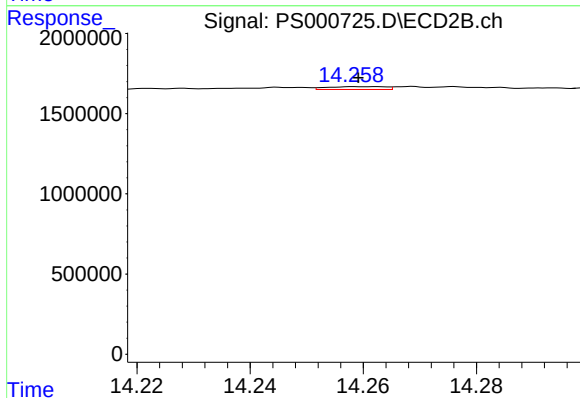


#11 2,4,5-TP (SILVEX)

R.T.: 14.259 min
Delta R.T.: 0.000 min
Response: 126395
Conc: 0.06 ng/ml

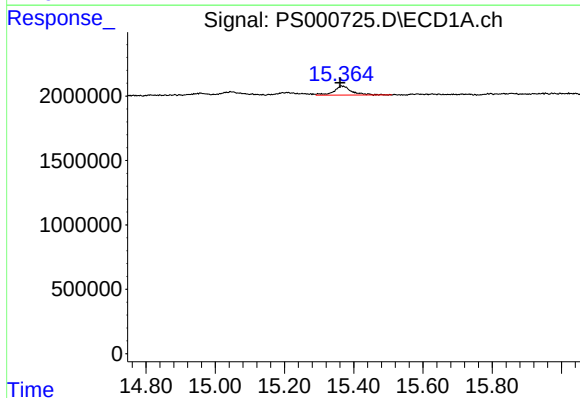


#12 2,4,5-T

R.T.: 15.365 min
Delta R.T.: 0.004 min
Response: 2510296
Conc: 1.17 ng/ml

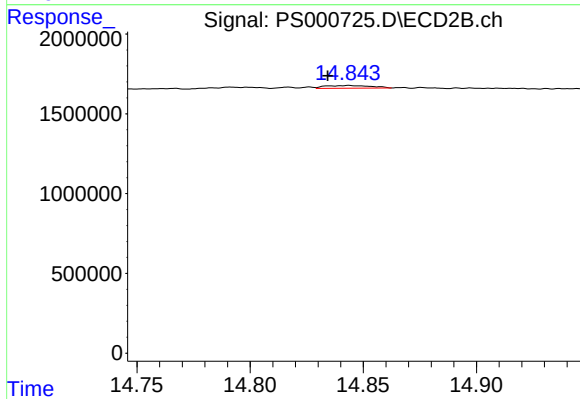

#12 2,4,5-T


R.T.: 14.844 min
Delta R.T.: 0.009 min
Response: 242850
Conc: 0.14 ng/ml

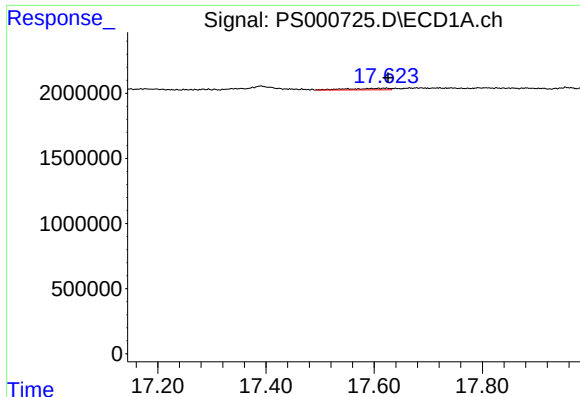

#14 DINoseb


R.T.: 17.607 min
Delta R.T.: -0.018 min
Response: 627802
Conc: 0.42 ng/ml

Instrument :
ECD_S
ClientSampleId :

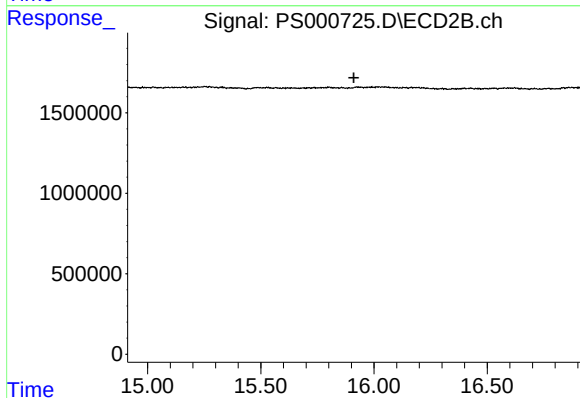


#14 DINoseb

R.T.: 0.000 min
Exp R.T. : 15.911 min
Response: 0
Conc: N.D.

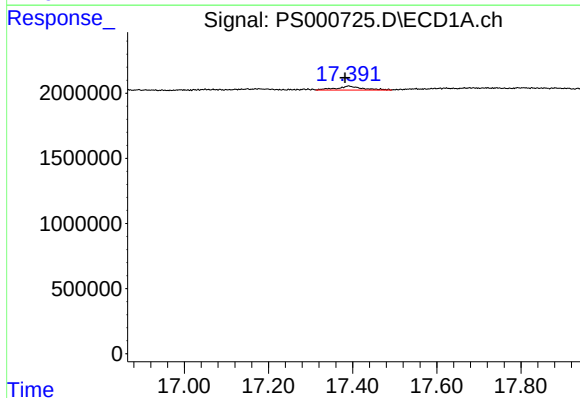


#15 Picloram

R.T.: 17.390 min
Delta R.T.: 0.009 min
Response: 1283317
Conc: 0.44 ng/ml

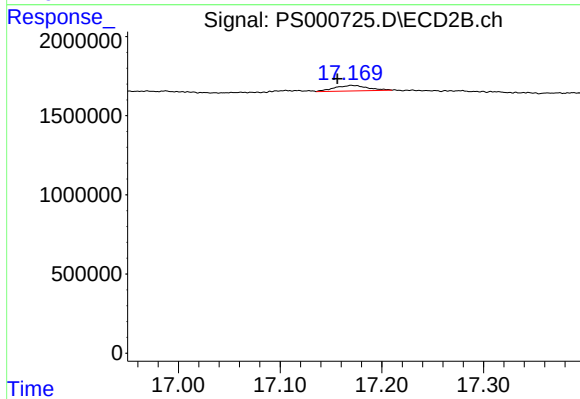

#15 Picloram


R.T.: 17.170 min
Delta R.T.: 0.013 min
Response: 785467
Conc: 0.31 ng/ml

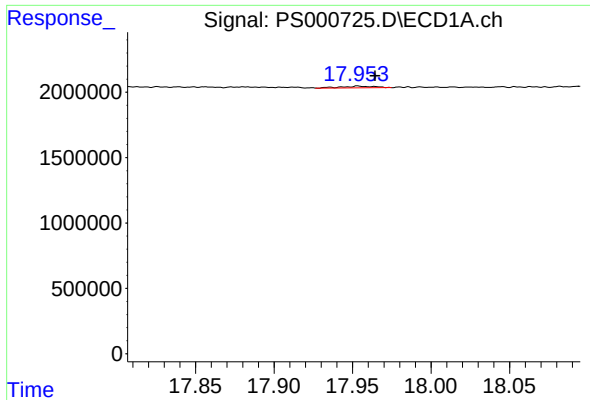

#16 DCPA

R.T.: 17.954 min
Delta R.T.: -0.010 min
Response: 186400
Conc: 0.07 ng/ml

Instrument :
ECD_S
ClientSampleId :

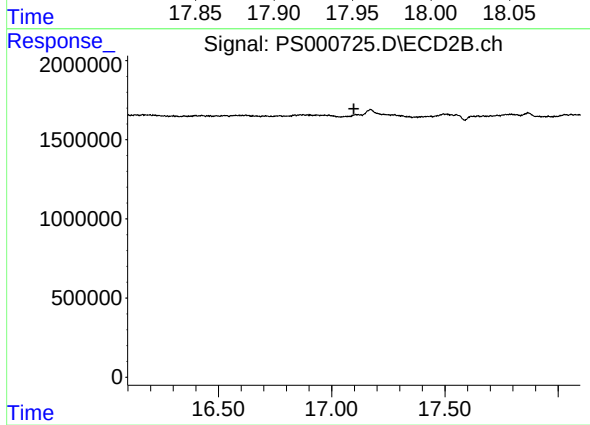

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.098 min
Response: 0
Conc: N.D.