

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070218\
 Data File : PS000735.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jul 2018 23:58
 Operator : UA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 03 01:52:46 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061718.M
 Quant Title : 8080.M
 QLast Update : Mon Jun 18 00:27:44 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.798	11.182	184.3E6	158.7E6	489.402	466.330
Target Compounds							
1) T	Dalapon	0.000	2.519	0	13383	N.D.	0.031 #
3) T	4-Nitroph...	11.423	0.000	455307	0	1.937	N.D. #
6) T	MCP	12.485	0.000	965130	0	0.852	N.D. #
11) T	2,4,5-TP ...	14.929	0.000	247248	0	0.114	N.D. #
12) T	2,4,5-T	15.341	0.000	1061837	0	0.493	N.D. #
15) T	Picloram	17.364	17.146	4060862	15998	1.390	0.006 #
16) T	DCPA	0.000	17.146	0	15998	N.D.	0.007 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070218\
Data File : PS000735.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jul 2018 23:58
Operator : UA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 03 01:52:46 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061718.M
Quant Title : 8080.M
QLast Update : Mon Jun 18 00:27:44 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

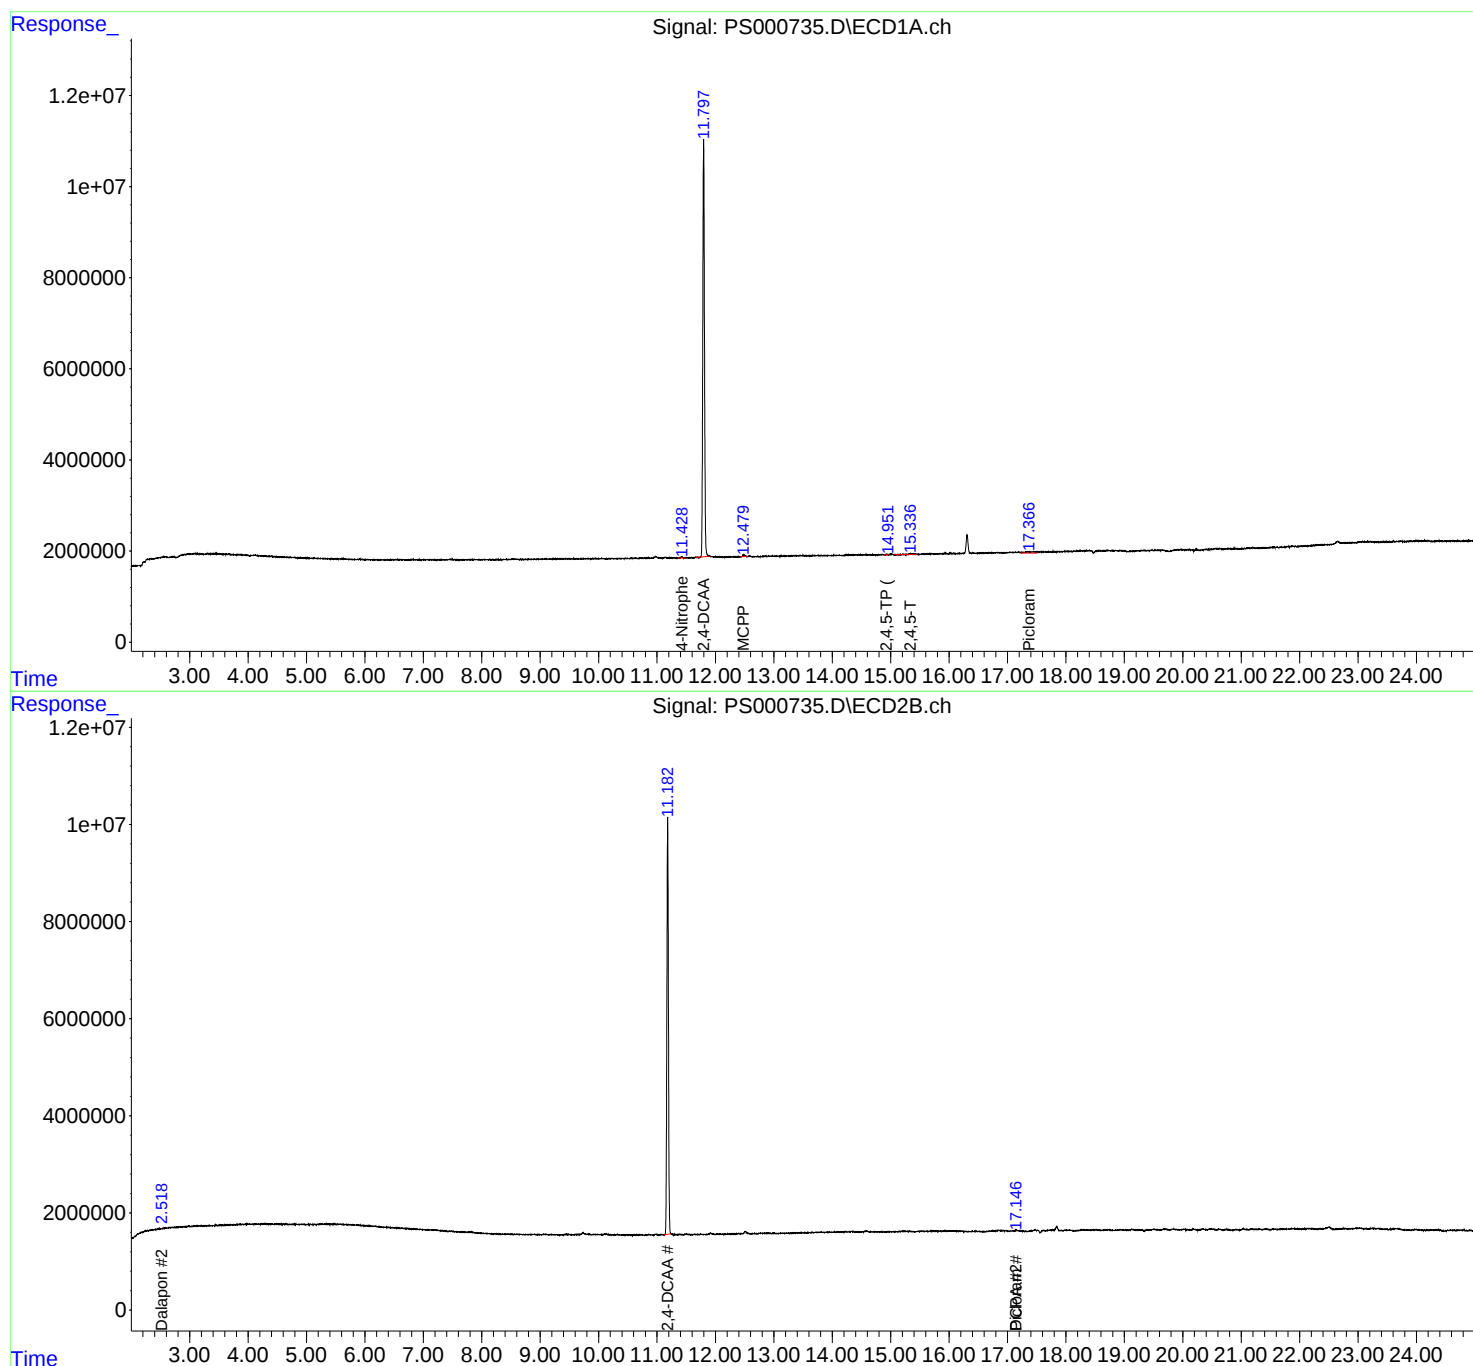


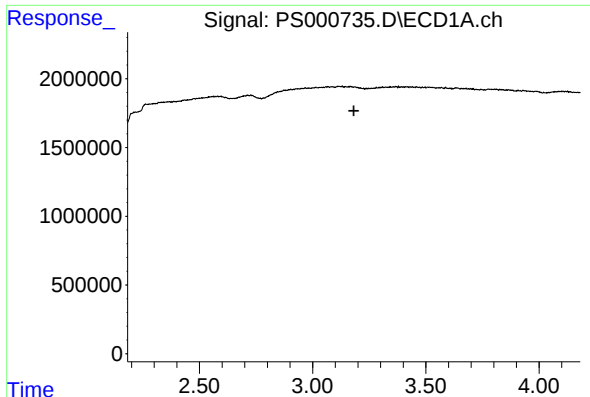

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 3.182 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

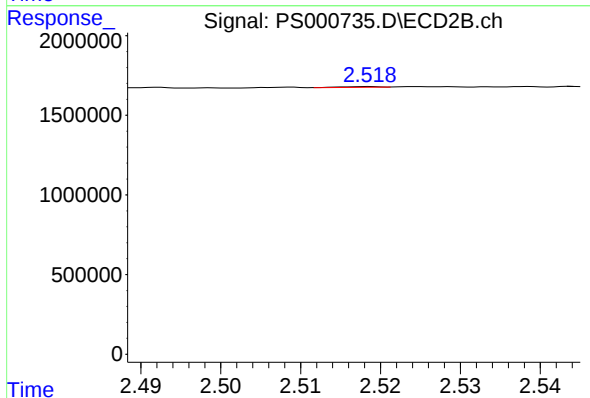


#1 Dalapon

R.T.: 2.519 min
Delta R.T.: -0.042 min
Response: 13383
Conc: 0.03 ng/ml

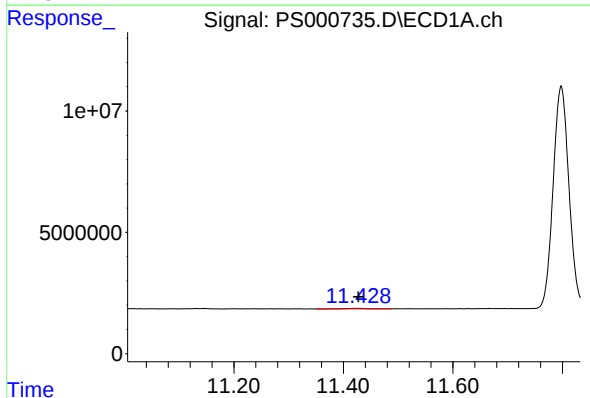


#3 4-Nitrophenol

R.T.: 11.423 min
Delta R.T.: -0.005 min
Response: 455307
Conc: 1.94 ng/ml

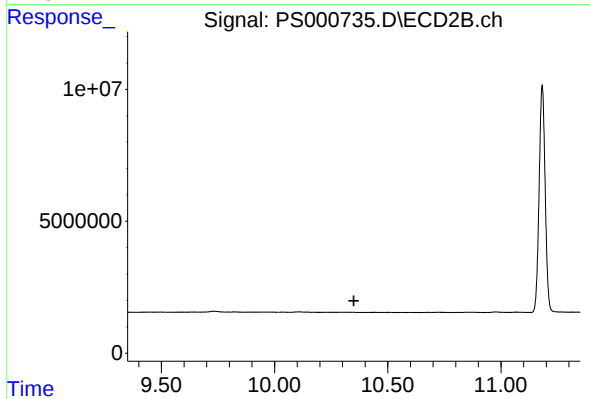

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.350 min
Response: 0
Conc: N.D.

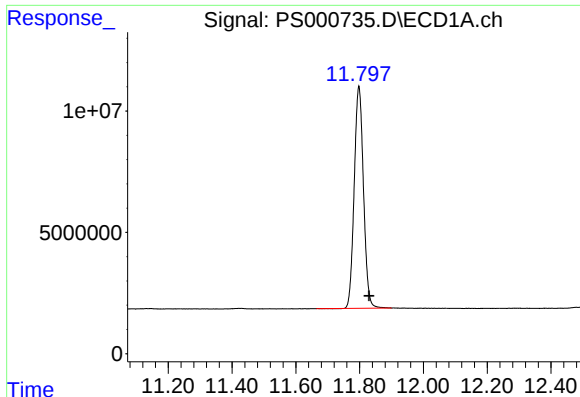

#4 2,4-DCAA


R.T.: 11.798 min
Delta R.T.: -0.032 min
Response: 184335615
Conc: 489.40 ng/ml

Instrument :
ECD_S
ClientSampleId :

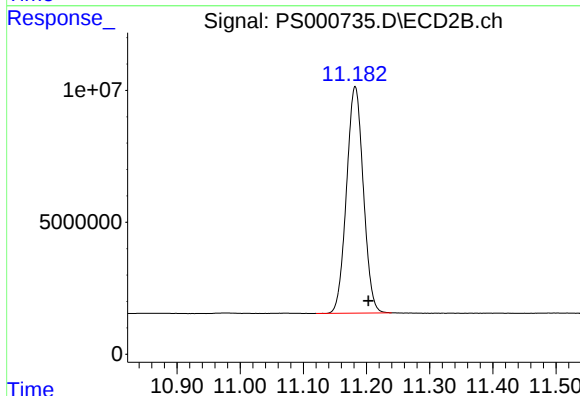


#4 2,4-DCAA

R.T.: 11.182 min
Delta R.T.: -0.021 min
Response: 158696158
Conc: 466.33 ng/ml

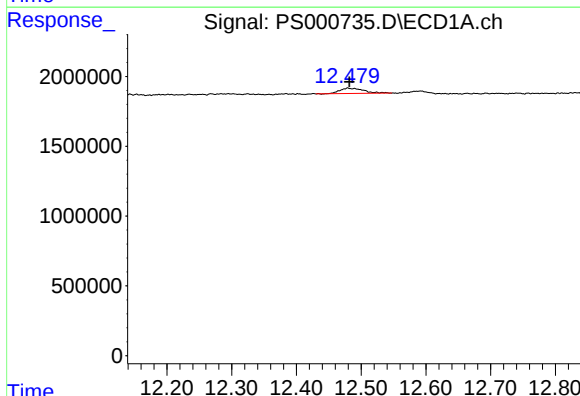


#6 MCP

R.T.: 12.485 min
Delta R.T.: 0.004 min
Response: 965130
Conc: 0.85 ug/ml

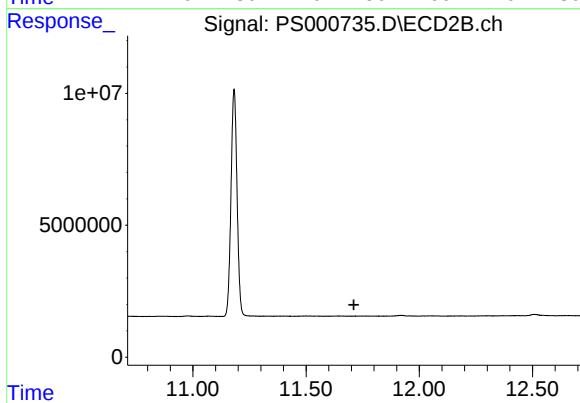

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.711 min
Response: 0
Conc: N.D.

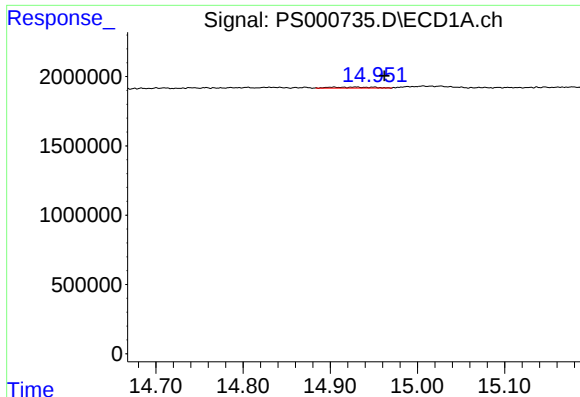

#11 2,4,5-TP (SILVEX)


R.T.: 14.929 min
Delta R.T.: -0.033 min
Response: 247248
Conc: 0.11 ng/ml

Instrument :
ECD_S
ClientSampleId :

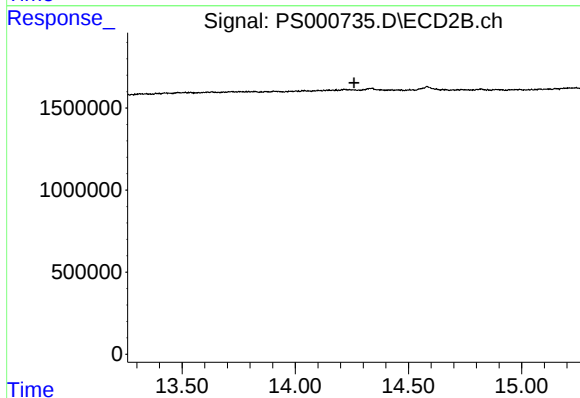


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 14.259 min
Response: 0
Conc: N.D.

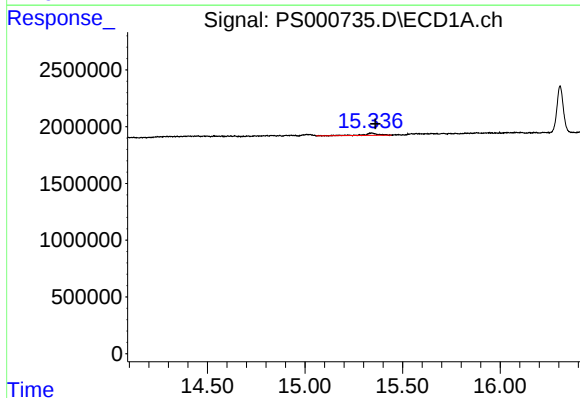


#12 2,4,5-T

R.T.: 15.341 min
Delta R.T.: -0.019 min
Response: 1061837
Conc: 0.49 ng/ml

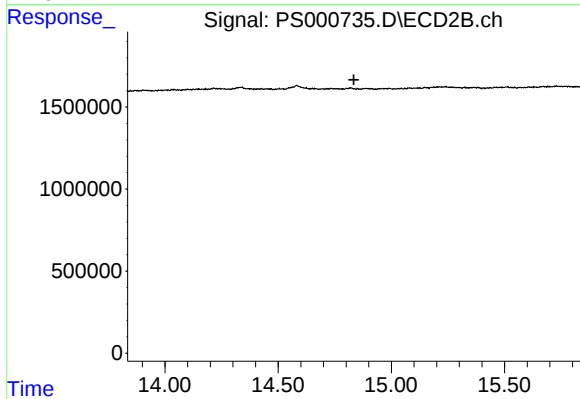

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 14.834 min
Response: 0
Conc: N.D.

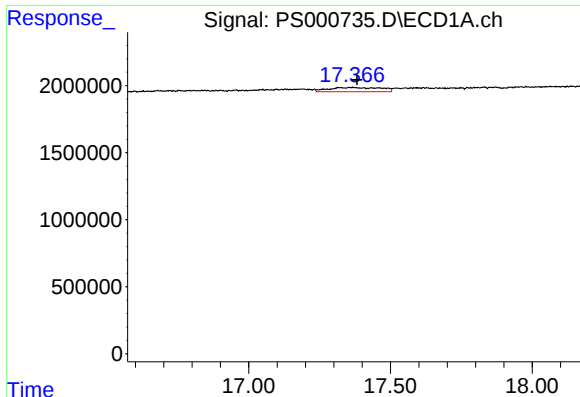

#15 Picloram


R.T.: 17.364 min
Delta R.T.: -0.018 min
Response: 4060862
Conc: 1.39 ng/ml

Instrument :
ECD_S
ClientSampleId :

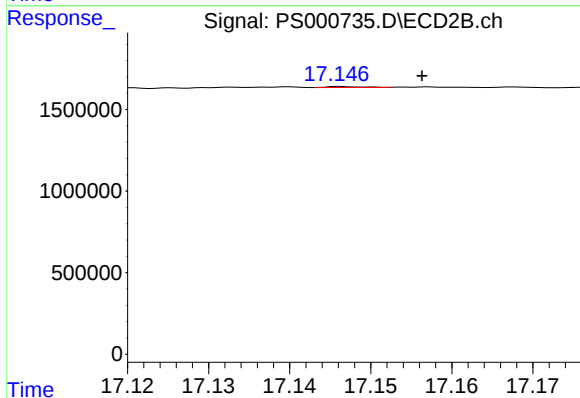


#15 Picloram

R.T.: 17.146 min
Delta R.T.: -0.010 min
Response: 15998
Conc: 0.01 ng/ml

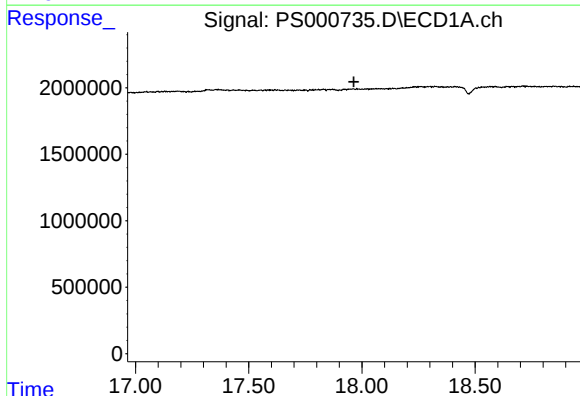

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.964 min
Response: 0
Conc: N.D.

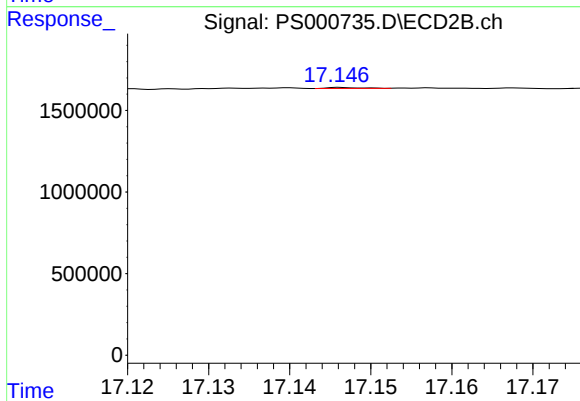

#16 DCPA

R.T.: 17.146 min
Delta R.T.: 0.048 min
Response: 15998
Conc: 0.01 ng/ml