

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070218\
 Data File : PS000747.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jul 2018 06:09
 Operator : UA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 03 06:39:15 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061718.M
 Quant Title : 8080.M
 QLast Update : Mon Jun 18 00:27:44 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.834	11.219	188.6E6	124.0E6	500.716	364.505 #
Target Compounds							
1) T	Dalapon	0.000	2.565	0	40040	N.D.	0.092 #
8) T	DICHLORPROP	0.000	12.555	0	147426	N.D.	0.458 #
10) T	Pentachlo...	0.000	13.650	0	46335	N.D.	0.010 #
11) T	2,4,5-TP ...	0.000	14.270	0	209658	N.D.	0.108 #
12) T	2,4,5-T	0.000	14.846	0	221256	N.D.	0.131 #
15) T	Picloram	0.000	17.177	0	953882	N.D.	0.382 #
16) T	DCPA	0.000	17.111	0	54350	N.D.	0.024 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070218\
Data File : PS000747.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jul 2018 06:09
Operator : UA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 03 06:39:15 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061718.M
Quant Title : 8080.M
QLast Update : Mon Jun 18 00:27:44 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

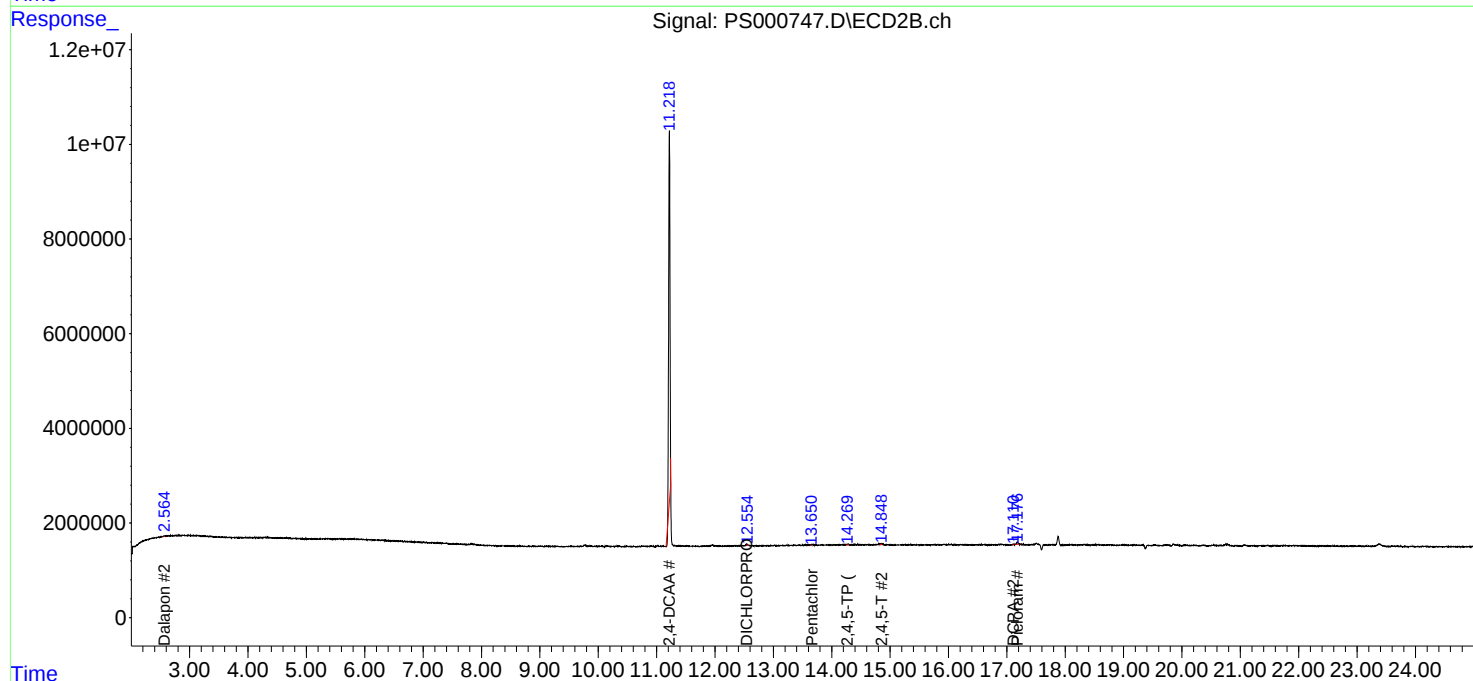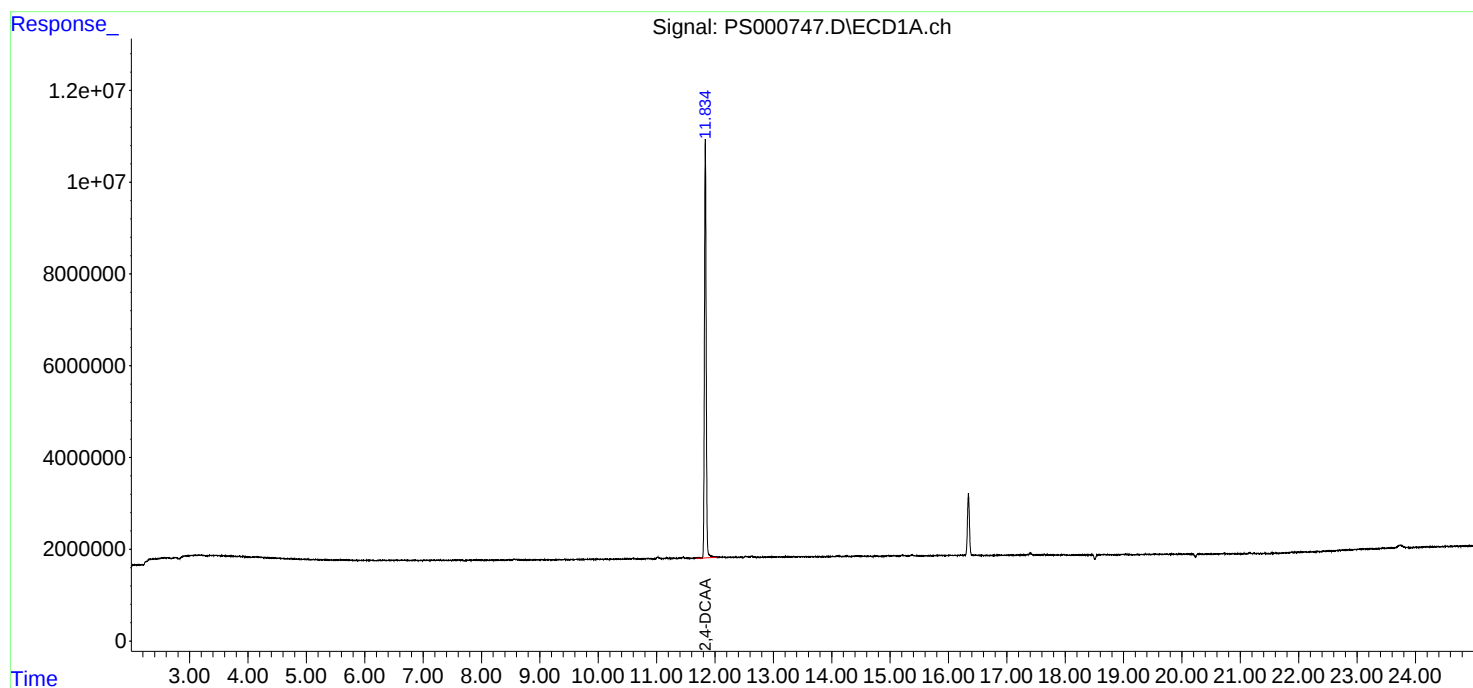


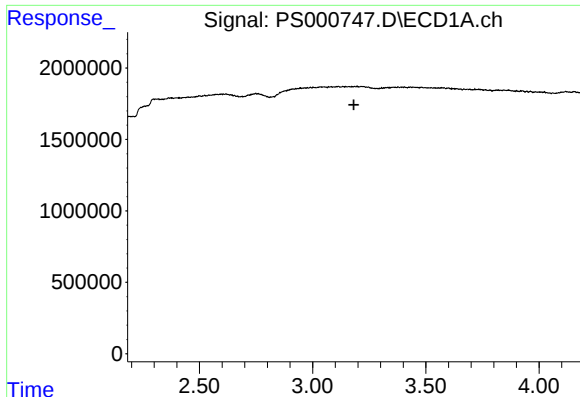

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 3.182 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

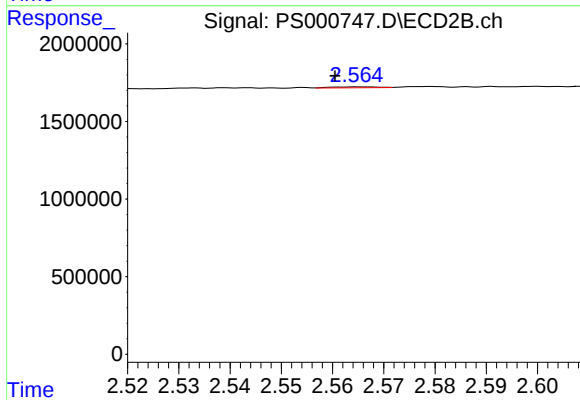


#1 Dalapon

R.T.: 2.565 min
Delta R.T.: 0.004 min
Response: 40040
Conc: 0.09 ng/ml

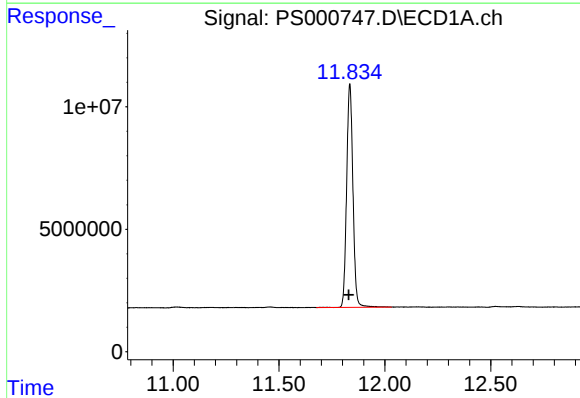


#4 2,4-DCAA

R.T.: 11.834 min
Delta R.T.: 0.005 min
Response: 188597102
Conc: 500.72 ng/ml

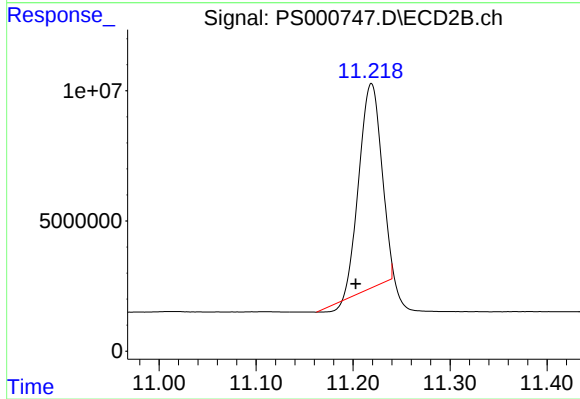

#4 2,4-DCAA


R.T.: 11.219 min
Delta R.T.: 0.016 min
Response: 124044299
Conc: 364.50 ng/ml

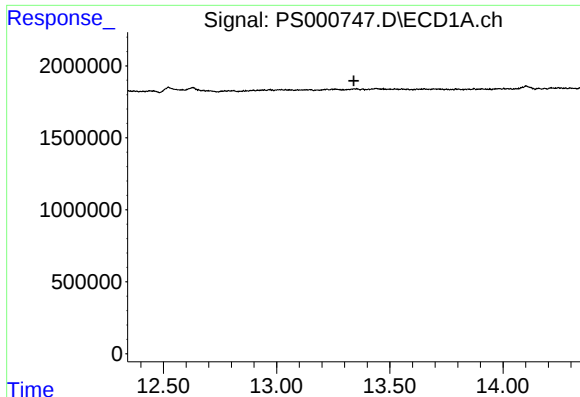

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T. : 13.341 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

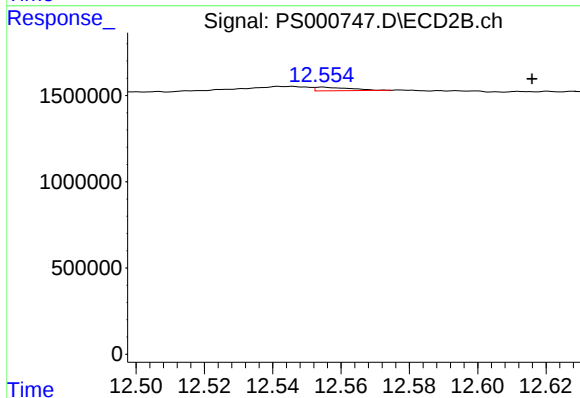


#8 DICHLORPROP

R.T.: 12.555 min
Delta R.T.: -0.061 min
Response: 147426
Conc: 0.46 ng/ml

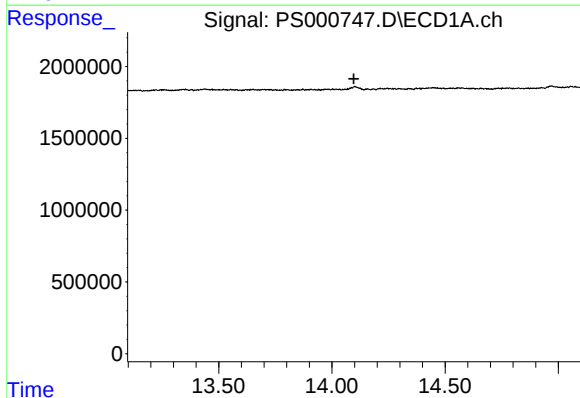


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 14.097 min
Response: 0
Conc: N.D.

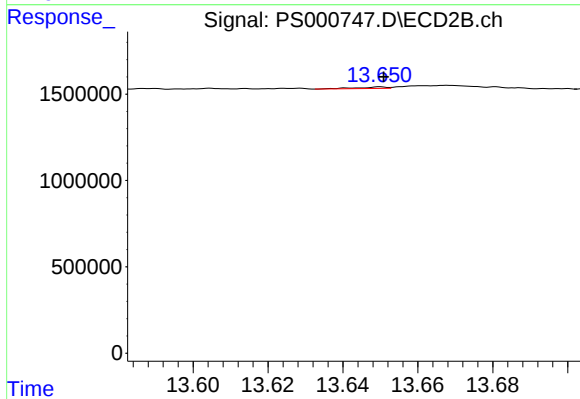

#10 Pentachlorophenol


R.T.: 13.650 min
Delta R.T.: 0.000 min
Response: 46335
Conc: 0.01 ng/ml

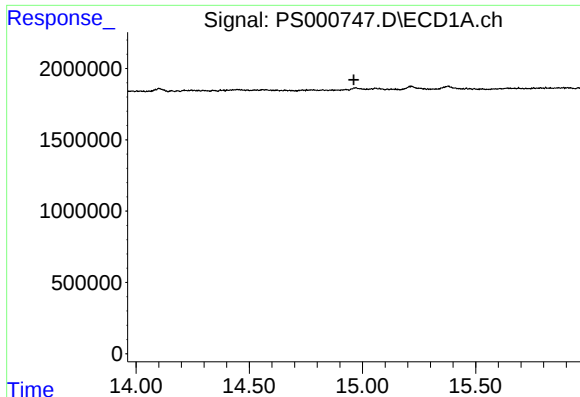

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 14.962 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

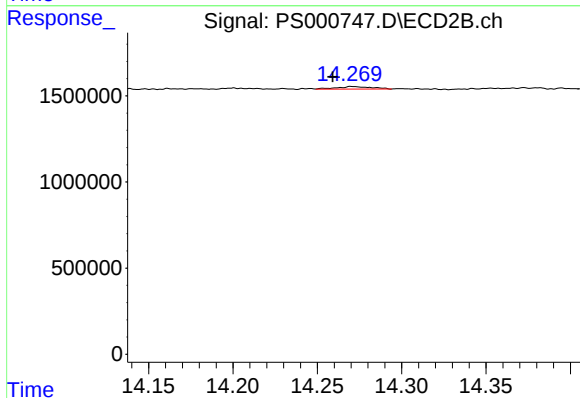


#11 2,4,5-TP (SILVEX)

R.T.: 14.270 min
Delta R.T.: 0.011 min
Response: 209658
Conc: 0.11 ng/ml

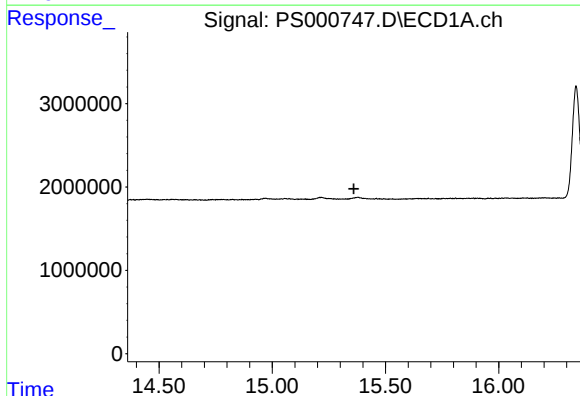


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 15.360 min
Response: 0
Conc: N.D.

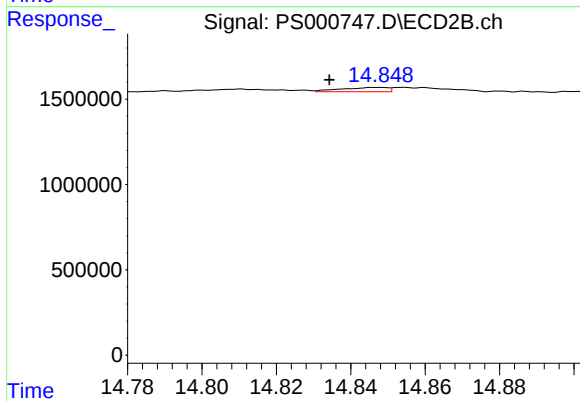

#12 2,4,5-T


R.T.: 14.846 min
Delta R.T.: 0.012 min
Response: 221256
Conc: 0.13 ng/ml

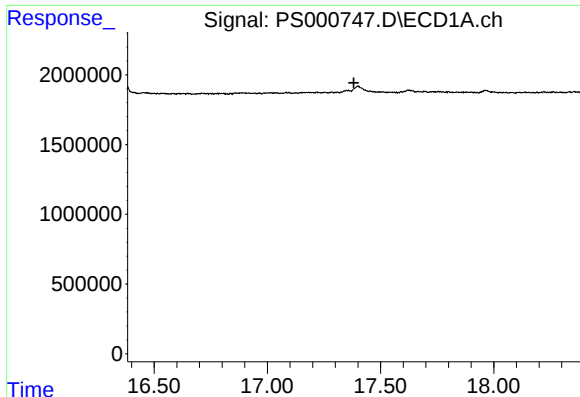

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 17.382 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

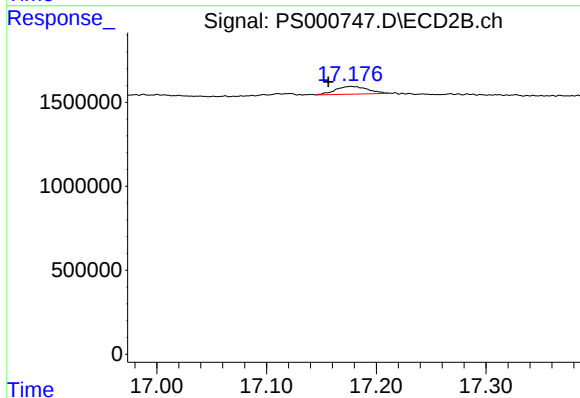


#15 Picloram

R.T.: 17.177 min
Delta R.T.: 0.021 min
Response: 953882
Conc: 0.38 ng/ml

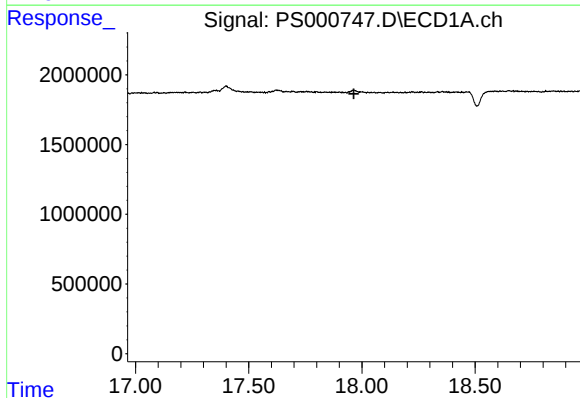

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.964 min
Response: 0
Conc: N.D.

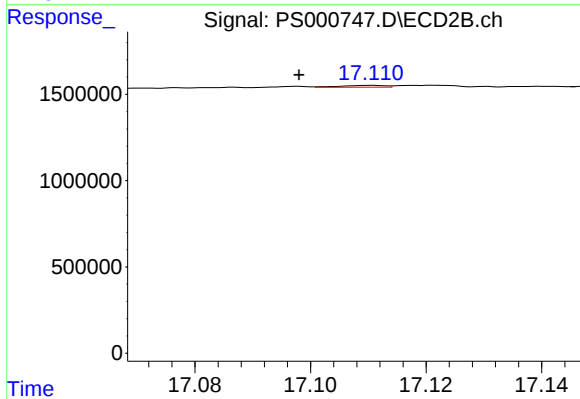

#16 DCPA

R.T.: 17.111 min
Delta R.T.: 0.013 min
Response: 54350
Conc: 0.02 ng/ml